

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN051222\
 Data File : VN072457.D
 Acq On : 12 May 2022 16:56
 Operator : JC\MD
 Sample : N2800-07
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 MW-17

Quant Time: May 13 02:46:33 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N051022W.M
 Quant Title : SW846 8260
 QLast Update : Tue May 10 15:43:28 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	8.086	168	175659	50.000	ug/l	# 0.00
34) 1,4-Difluorobenzene	8.963	114	282615	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.739	117	240638	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.668	152	82276	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.434	65	155681	57.863	ug/l	0.00
Spiked Amount	50.000	Range	61 - 141	Recovery	=	115.720%
35) Dibromofluoromethane	8.022	113	103830	55.222	ug/l	0.00
Spiked Amount	50.000	Range	69 - 133	Recovery	=	110.440%
50) Toluene-d8	10.439	98	353134	49.314	ug/l	0.00
Spiked Amount	50.000	Range	65 - 126	Recovery	=	98.620%
62) 4-Bromofluorobenzene	12.727	95	105917	44.537	ug/l	0.00
Spiked Amount	50.000	Range	58 - 135	Recovery	=	89.080%
Target Compounds						
						Qvalue
30) Chloroform	7.816	83	38412	10.005	ug/l	90


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN051222\
Data File : VN072457.D
Acq On : 12 May 2022 16:56
Operator : JC\MD
Sample : N2800-07
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
MW-17

Quant Time: May 13 02:46:33 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N051022W.M
Quant Title : SW846 8260
QLast Update : Tue May 10 15:43:28 2022
Response via : Initial Calibration




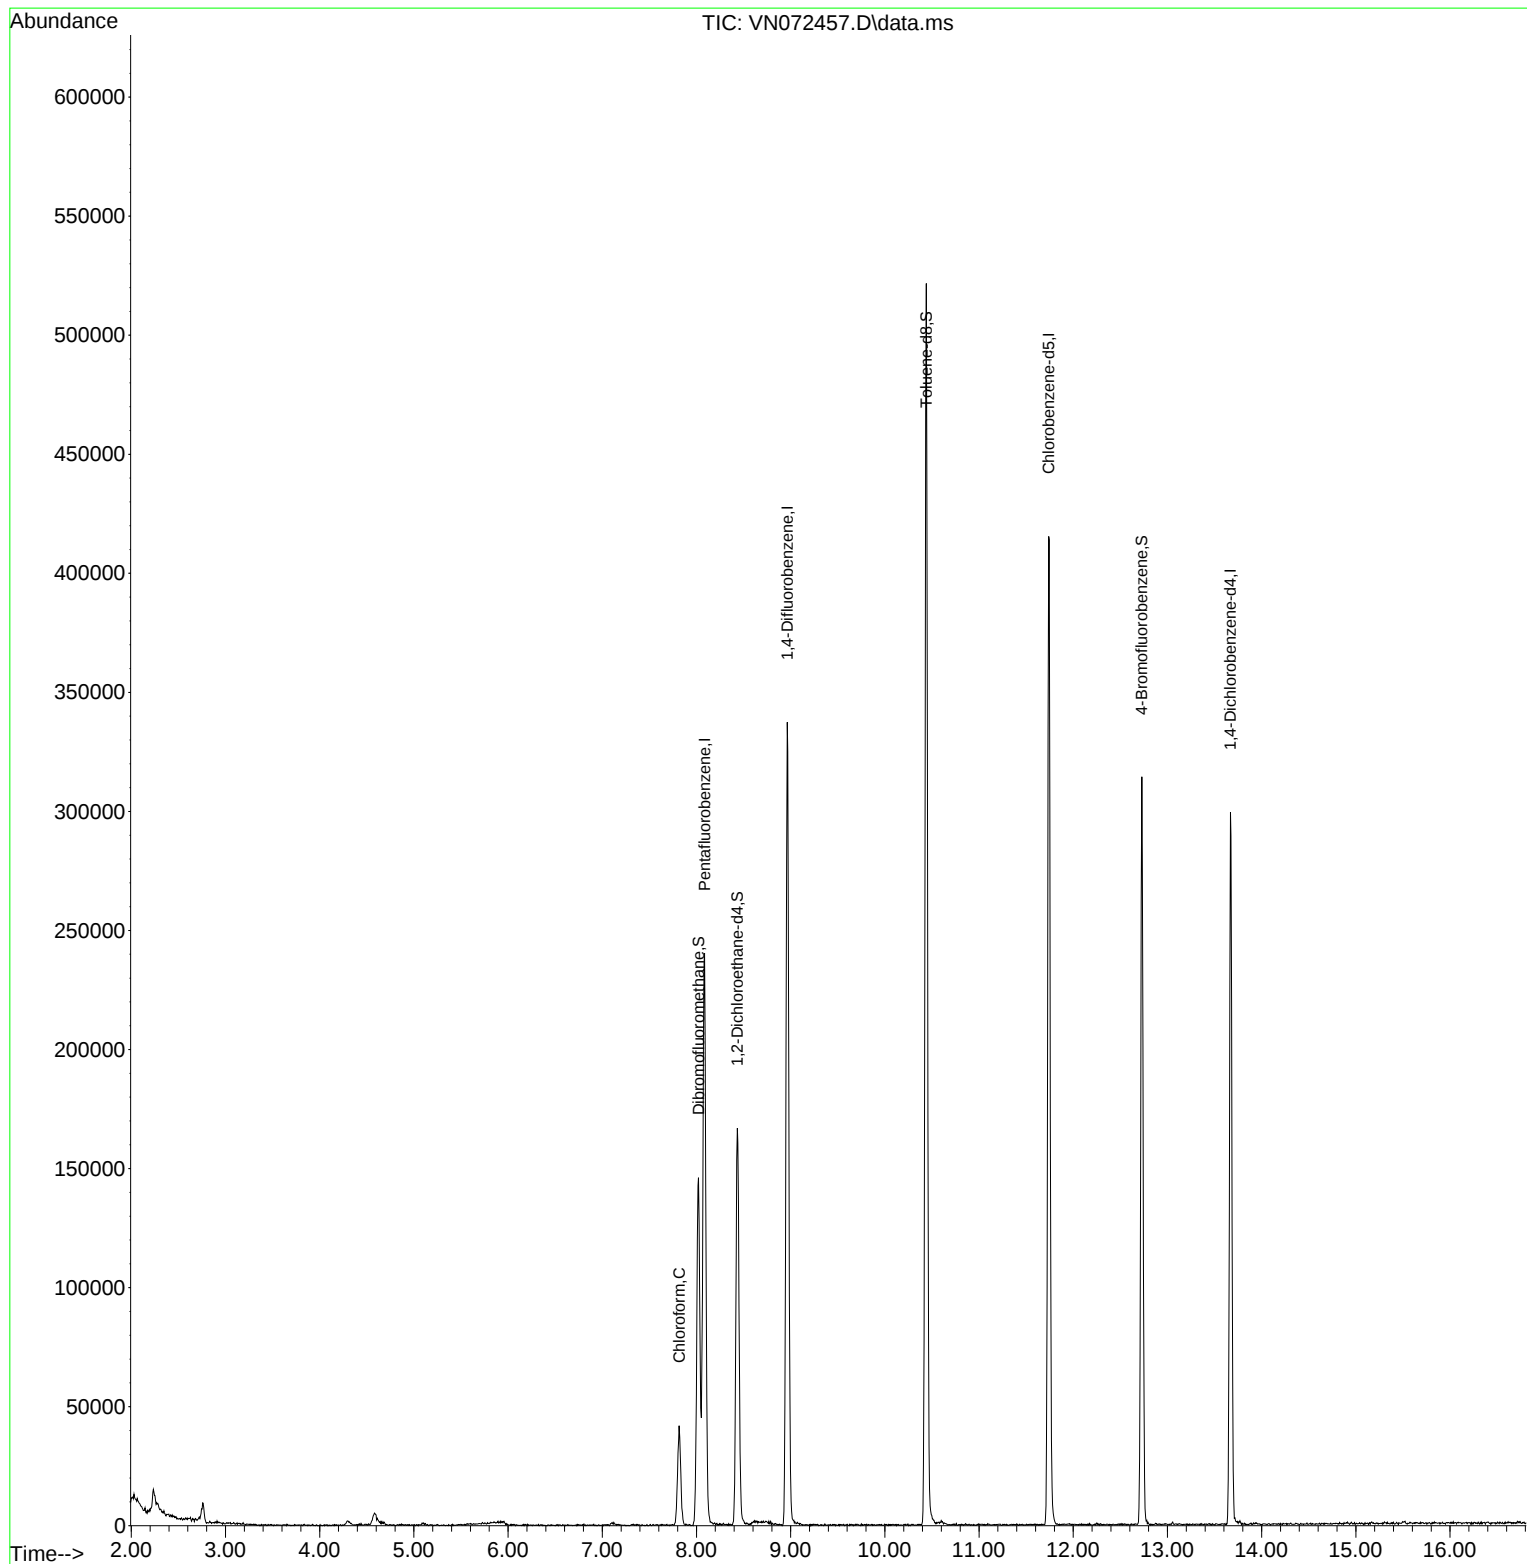


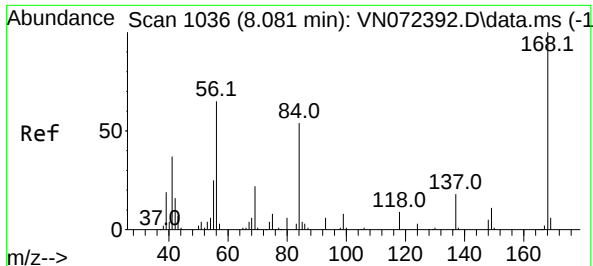

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.086 min Scan# 1036
Delta R.T. 0.005 min
Lab File: VN072457.D
Acq: 12 May 2022 16:56




Instrument :
MSVOA_N
ClientSampleId :
MW-17


Tgt Ion:168 Resp: 175659
Ion Ratio Lower Upper
168 100
99 65.9 42.3 63.5#

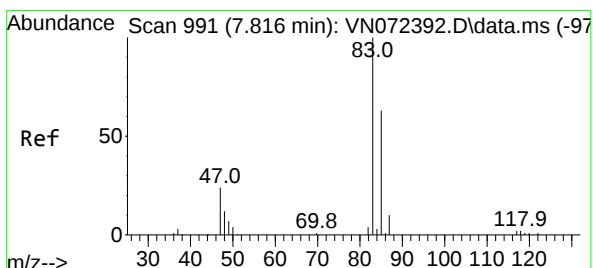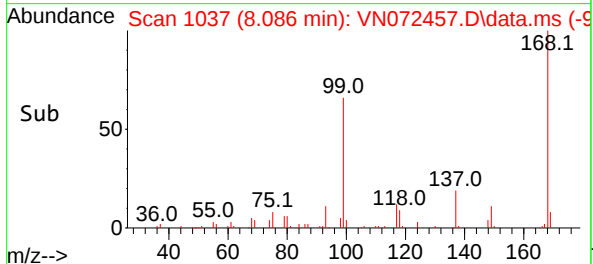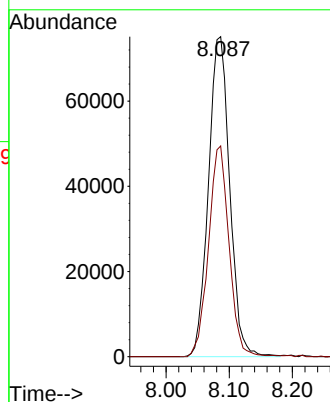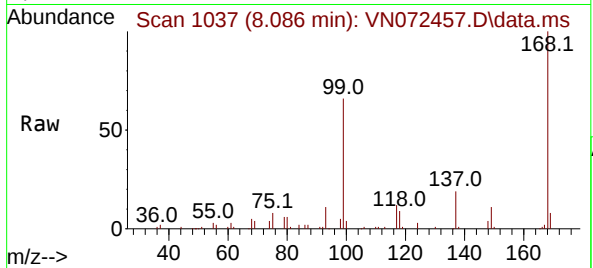

#30
Chloroform
Concen: 10.005 ug/l
RT: 7.816 min Scan# 991
Delta R.T. -0.000 min
Lab File: VN072457.D
Acq: 12 May 2022 16:56

Tgt Ion: 83 Resp: 38412
Ion Ratio Lower Upper
83 100
85 72.4 51.8 77.8

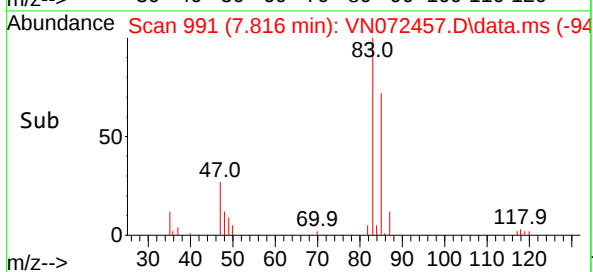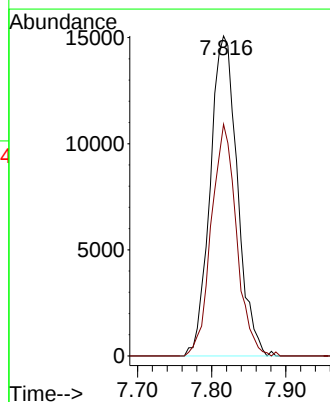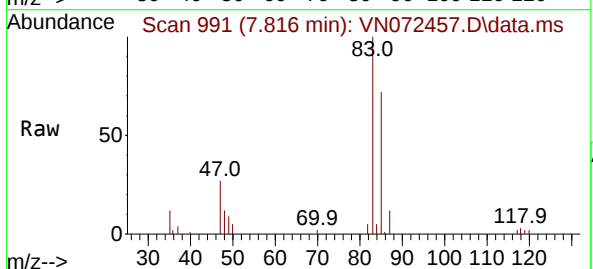

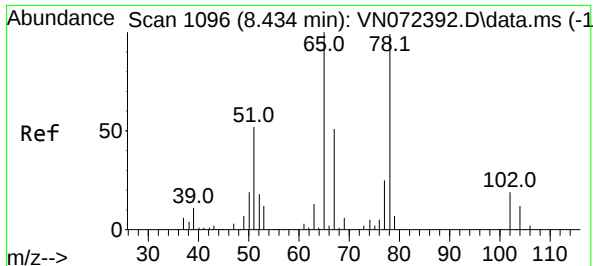

#33

1,2-Dichloroethane-d4

Concen: 57.863 ug/l

RT: 8.434 min Scan# 1096

Delta R.T. -0.000 min

Lab File: VN072457.D

Acq: 12 May 2022 16:56

Instrument :

MSVOA_N

ClientSampleId :





MW-17

Tgt Ion: 65 Resp: 155681

Ion Ratio Lower Upper

65 100

67 49.5 0.0 104.8

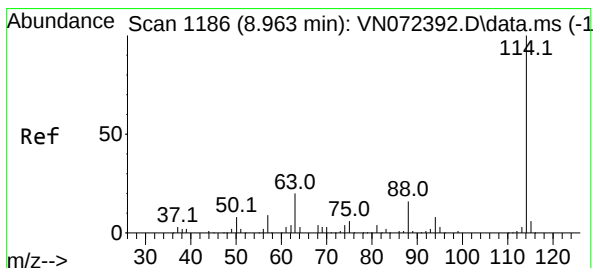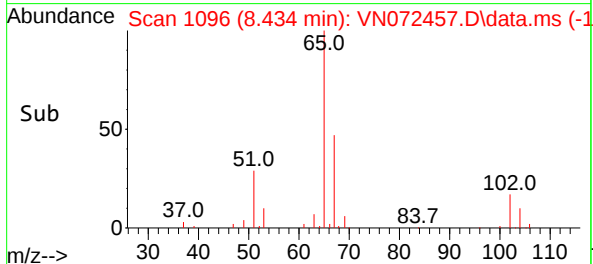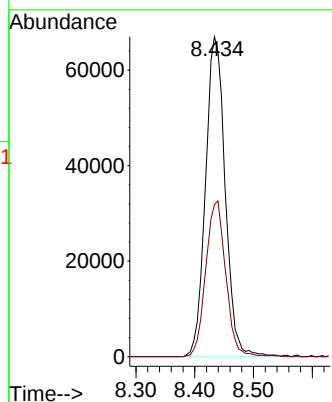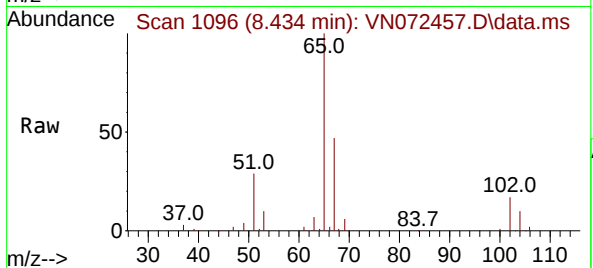

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.963 min Scan# 1186

Delta R.T. -0.000 min

Lab File: VN072457.D

Acq: 12 May 2022 16:56




Tgt Ion: 114 Resp: 282615


Ion Ratio Lower Upper

114 100

63 21.5 0.0 40.0

88 17.0 0.0 32.6

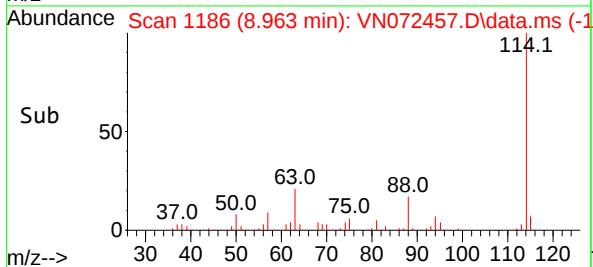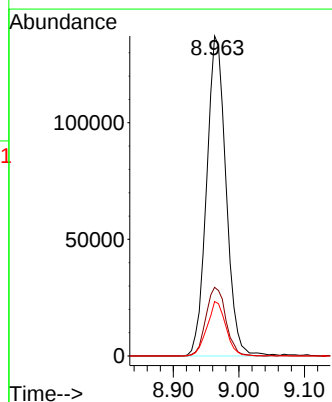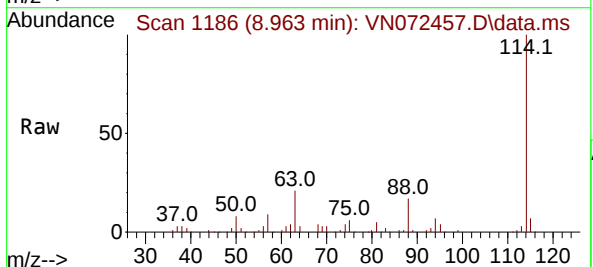

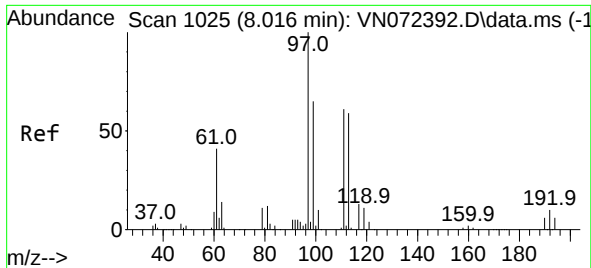

#35

Dibromofluoromethane

Concen: 55.222 ug/l

RT: 8.022 min Scan# 1026

Delta R.T. 0.006 min

Lab File: VN072457.D

Acq: 12 May 2022 16:56

Instrument :

MSVOA_N

ClientSampleId :

MW-17





Tgt Ion:113 Resp: 103830

Ion Ratio Lower Upper

113 100

111 104.0 81.4 122.0

192 20.1 17.0 25.6

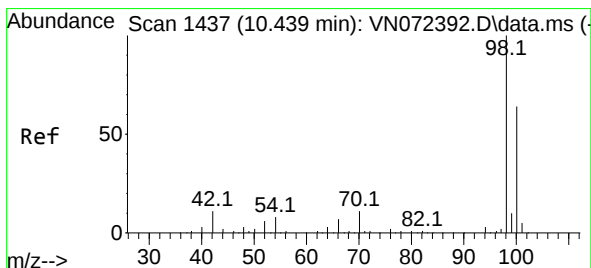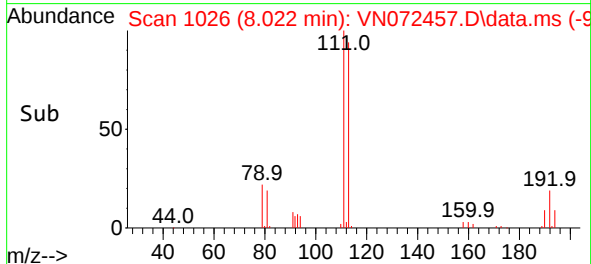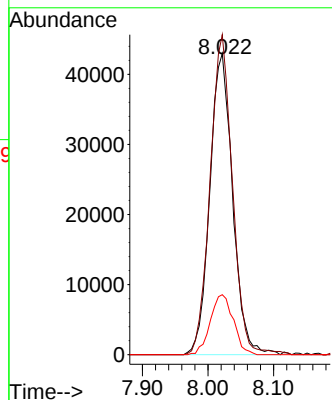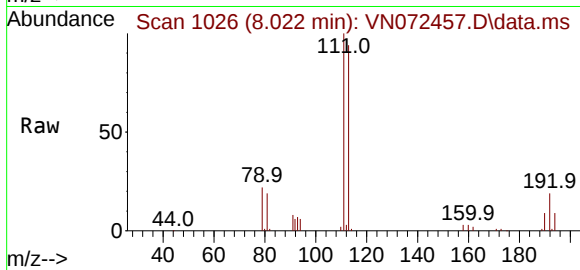

#50

Toluene-d8

Concen: 49.314 ug/l

RT: 10.439 min Scan# 1437

Delta R.T. 0.000 min

Lab File: VN072457.D




Acq: 12 May 2022 16:56


Tgt Ion: 98 Resp: 353134

Ion Ratio Lower Upper

98 100

100 64.7 52.6 78.8


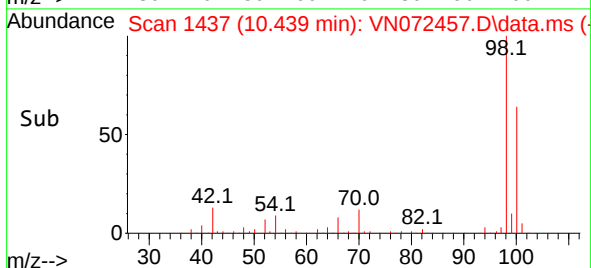
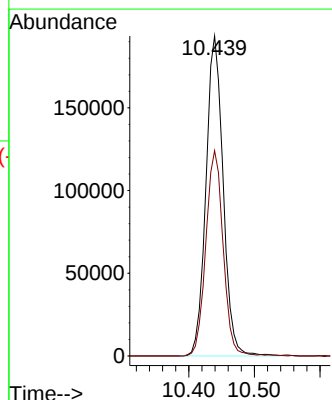
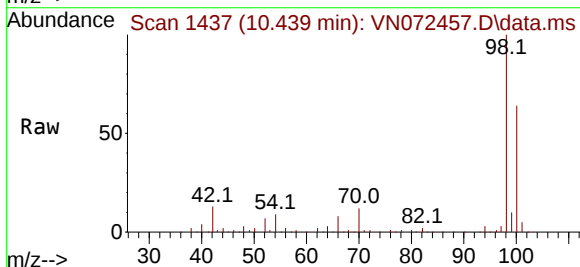


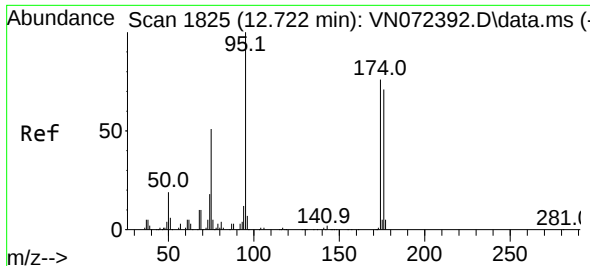

#62
4-Bromofluorobenzene
Concen: 44.537 ug/l
RT: 12.727 min Scan# 1825
Delta R.T. 0.005 min
Lab File: VN072457.D
Acq: 12 May 2022 16:56




Instrument :
MSVOA_N
ClientSampleId :
MW-17


Tgt Ion: 95 Resp: 105917
Ion Ratio Lower Upper
95 100
174 80.1 0.0 167.6
176 76.1 0.0 163.4

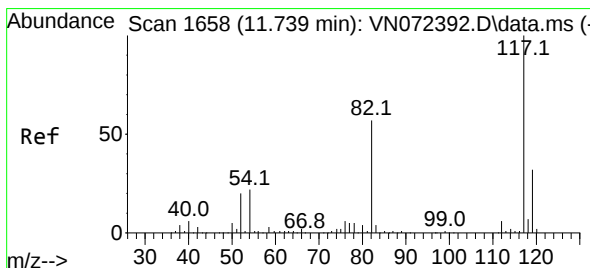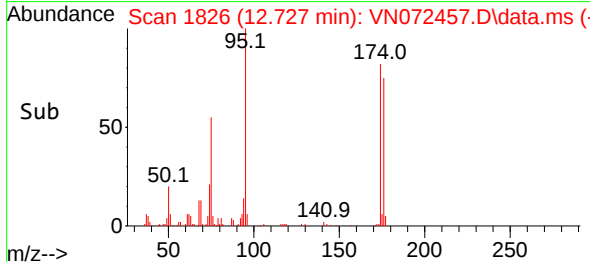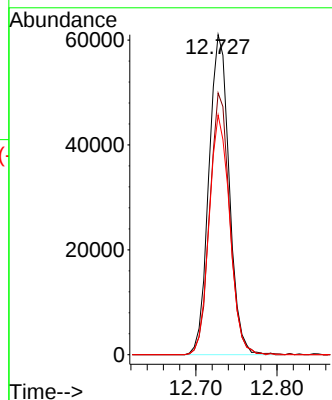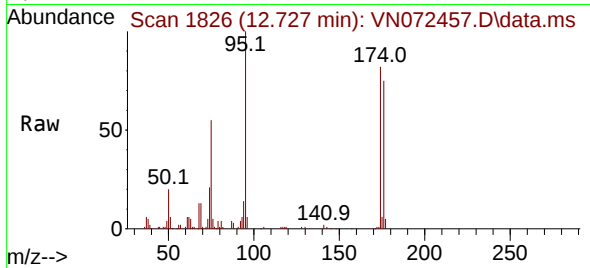

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.739 min Scan# 1658
Delta R.T. 0.000 min
Lab File: VN072457.D
Acq: 12 May 2022 16:56

Tgt Ion: 117 Resp: 240638
Ion Ratio Lower Upper
117 100
82 58.6 44.2 66.2
119 30.0 25.4 38.0

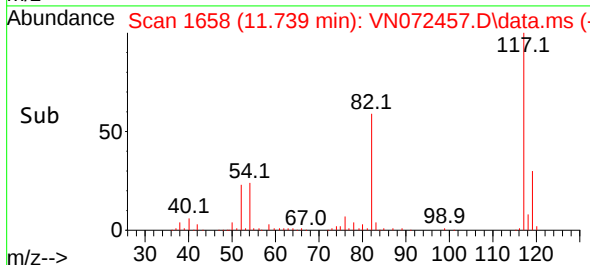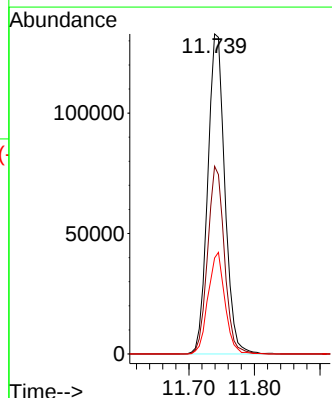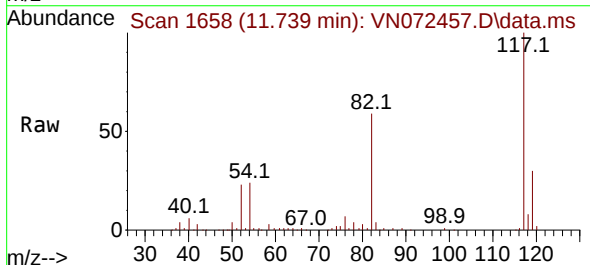

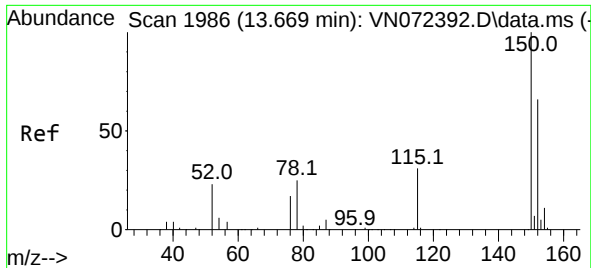

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.668 min Scan# 1986

Delta R.T. -0.001 min

Lab File: VN072457.D


Acq: 12 May 2022 16:56

Instrument :

MSVOA_N

ClientSampleId :

MW-17

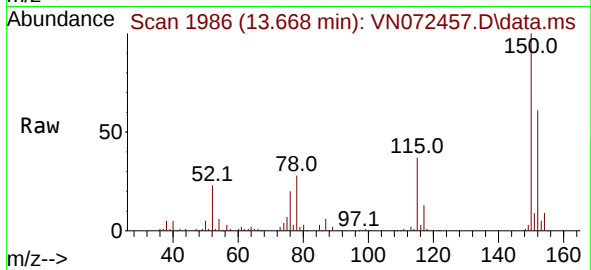

Tgt Ion:152 Resp: 82276

Ion Ratio Lower Upper

152 100

115 60.1 28.9 86.7

150 161.4 0.0 356.2

