
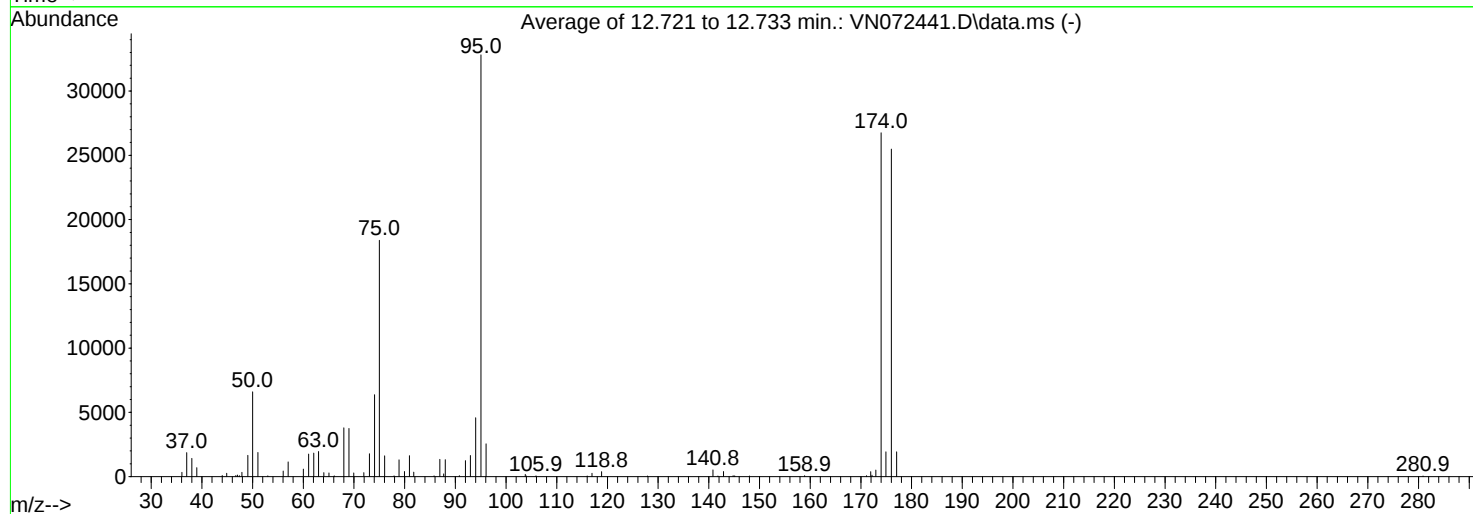


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN051222\
Data File : VN072441.D
Acq On : 12 May 2022 09:49
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N051022W.M
Title : SW846 8260
Last Update : Tue May 10 15:43:28 2022

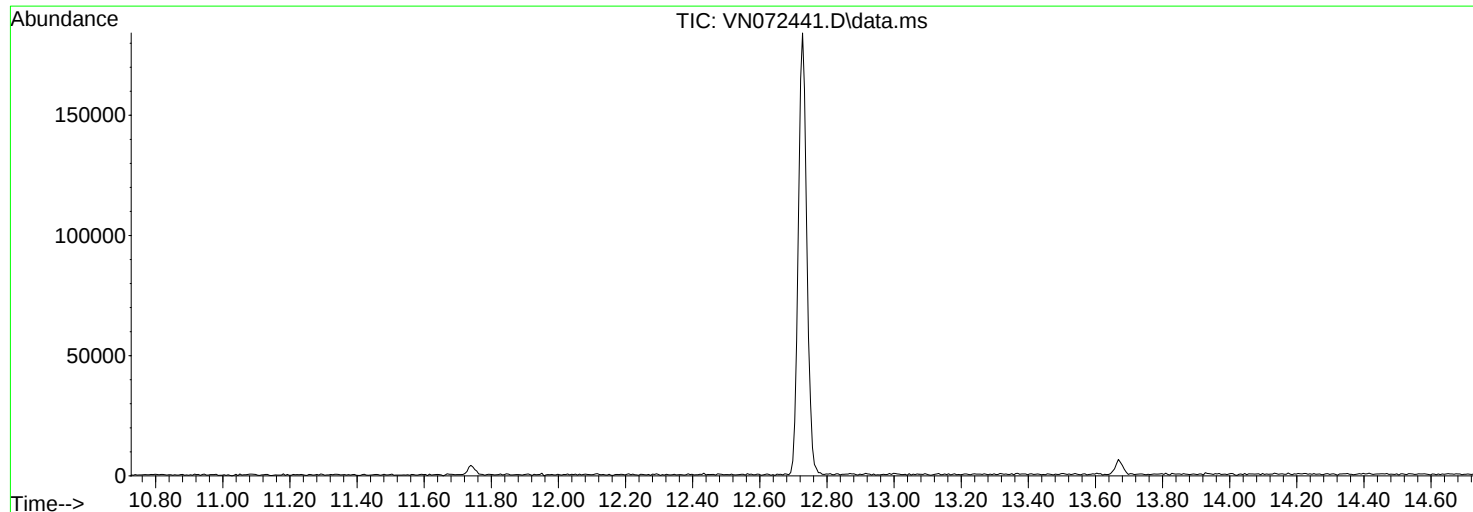

AutoFind: Scans 1825, 1826, 1827; Background Corrected with Scan 1817

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	20.1	6601	PASS
75	95	30	60	56.0	18387	PASS
95	95	100	100	100.0	32816	PASS
96	95	5	9	7.8	2557	PASS
173	174	0.00	2	1.9	508	PASS
174	95	50	100	81.5	26749	PASS
175	174	5	9	7.2	1927	PASS
176	174	95	101	95.3	25480	PASS
177	176	5	9	7.6	1931	PASS