
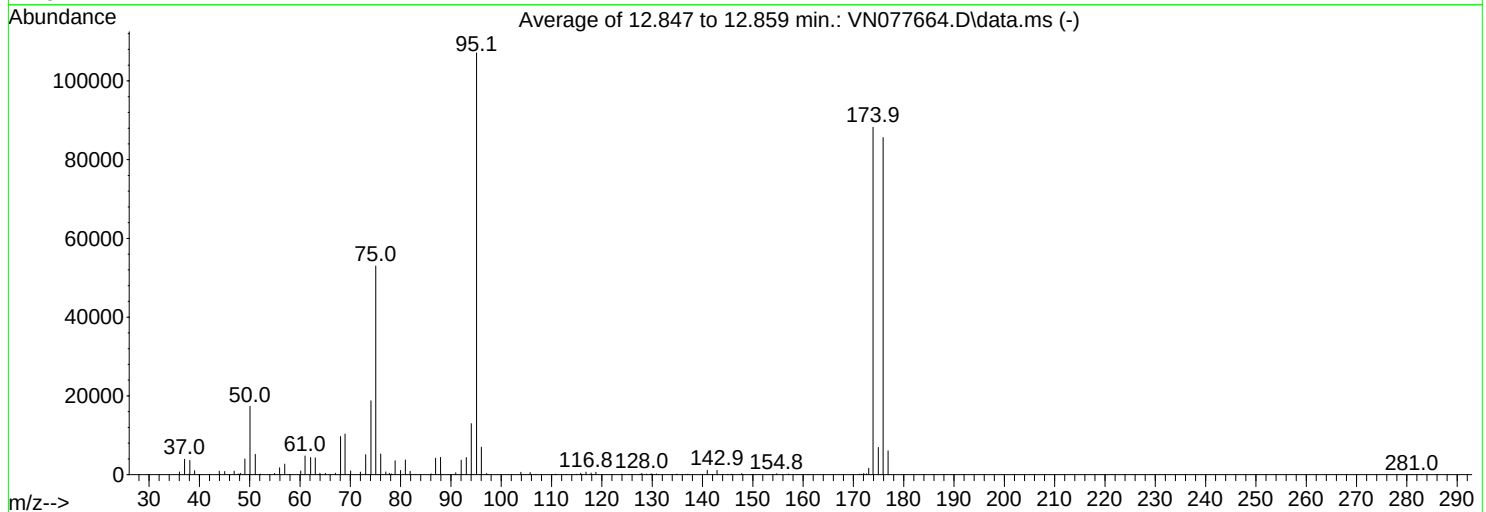


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN051223\
Data File : VN077664.D
Acq On : 12 May 2023 10:28
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT3.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\624N050823W.M
Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
Last Update : Tue May 09 05:58:09 2023

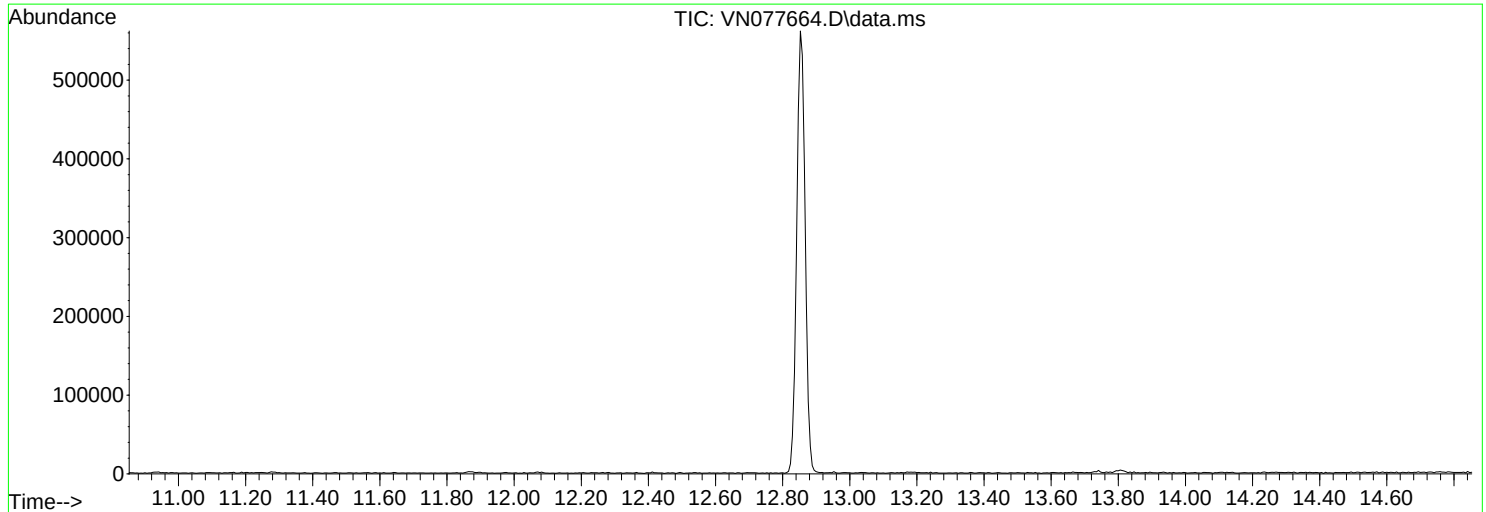

AutoFind: Scans 1852, 1853, 1854; Background Corrected with Scan 1844

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.2	17353	PASS
75	95	30	60	49.5	53005	PASS
95	95	100	100	100.0	107131	PASS
96	95	5	9	6.5	6977	PASS
173	174	0.00	2	1.9	1637	PASS
174	95	50	100	82.4	88227	PASS
175	174	5	9	7.8	6908	PASS
176	174	95	101	97.0	85611	PASS
177	176	5	9	7.1	6040	PASS