
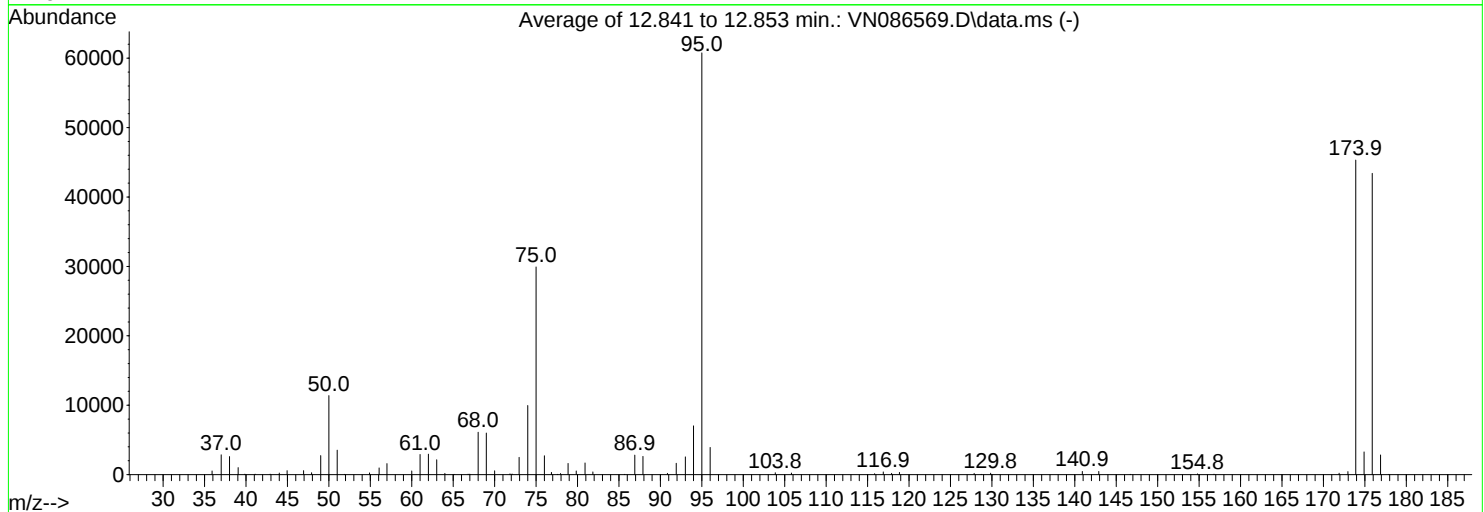


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN051225\
Data File : VN086569.D
Acq On : 12 May 2025 09:43
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N041525W.M
Title : SW846 8260
Last Update : Wed Apr 16 04:19:23 2025

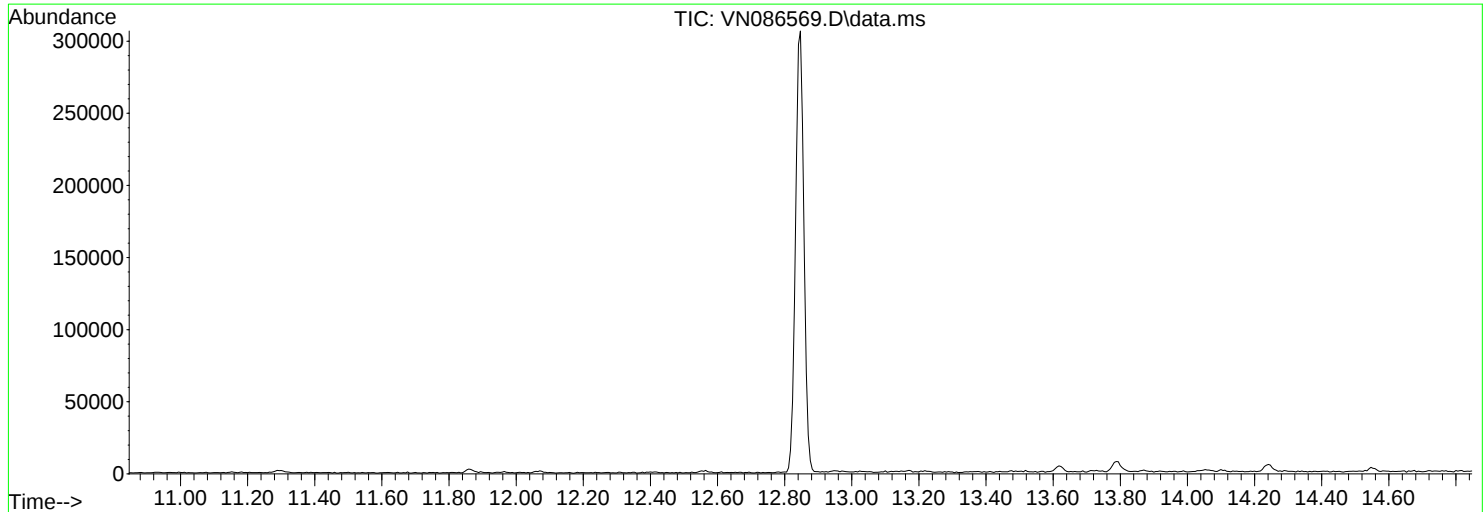

AutoFind: Scans 1851, 1852, 1853; Background Corrected with Scan 1843

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	18.7	11377	PASS
75	95	30	60	49.2	29912	PASS
95	95	100	100	100.0	60765	PASS
96	95	5	9	6.5	3926	PASS
173	174	0.00	2	1.0	440	PASS
174	95	50	100	74.6	45325	PASS
175	174	5	9	7.2	3264	PASS
176	174	95	101	95.8	43411	PASS
177	176	5	9	6.5	2841	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.90	530	49.00	2737	64.00	191	75.00	2991
37.00	2864	50.00	11377	65.10	52	76.00	2721
38.00	2610	51.00	3535	66.80	77	76.85	32
39.05	1027	51.90	55	67.00	66	77.60	5
39.85	71	54.90	262	68.00	6100	77.95	156
41.10	60	56.05	961	69.00	5985	78.85	1620
42.90	80	57.00	1583	70.00	546	79.85	523
44.00	229	60.00	525	71.85	120	80.90	1674
44.95	572	61.00	2917	72.10	102	81.85	388
46.95	587	62.00	2940	72.95	2494	85.70	52
47.90	288	63.00	2152	74.00	9959	86.90	2823

Average of 12.841 to 12.853 min.: VN086569.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
87.90	2629	117.90	184	172.95	440		
90.85	189	118.85	315	173.90	45325		
91.90	1642	127.85	192	174.90	3264		
93.00	2568	128.70	55	175.90	43411		
94.00	7020	129.85	215	176.90	2841		
95.00	60765	140.90	473	177.90	53		
96.00	3926	142.90	472				
103.85	273	146.70	54				
105.80	231	154.80	112				
115.85	140	156.80	72				
116.90	400	171.90	212				

Instrument :

MSVOA_N

ClientSampleId :

BFB