


Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN051319\
 Data File : VN055565.D
 Acq On : 13 May 2019 8:27
 Operator : JC/SP
 Sample : BFB
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N050819W.M
 Title : SW846 8260
 Last Update : Fri May 10 06:48:32 2019

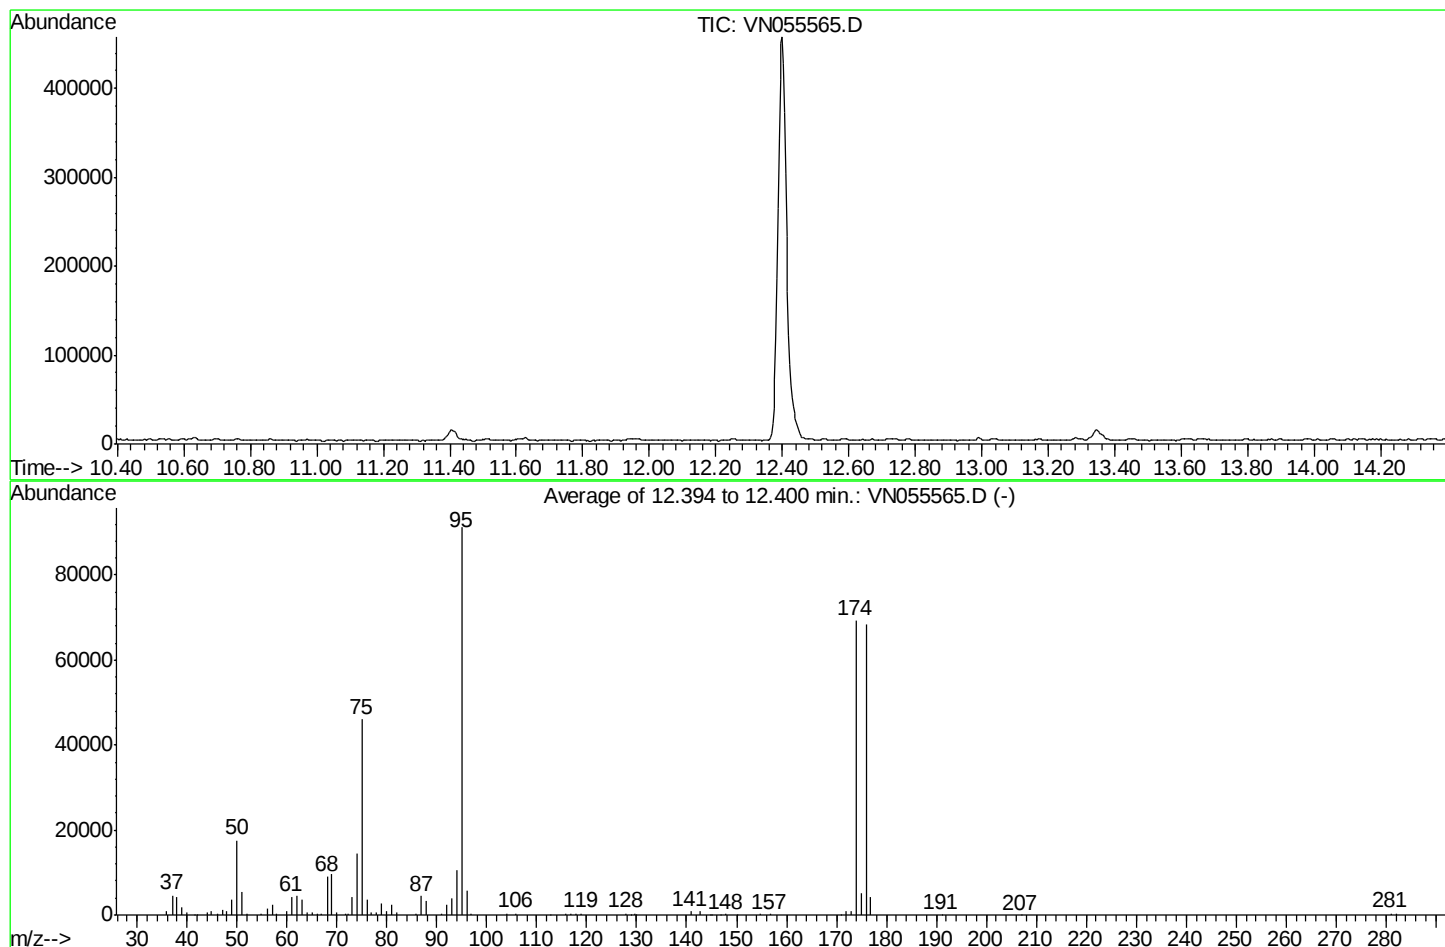

AutoFind: Scans 3303, 3304, 3305; Background Corrected with Scan 3290

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.2	17546	PASS
75	95	30	60	50.5	46064	PASS
95	95	100	100	100.0	91245	PASS
96	95	5	9	6.1	5589	PASS
173	174	0.00	2	1.4	979	PASS
174	95	50	100	75.9	69272	PASS
175	174	5	9	7.5	5211	PASS
176	174	95	101	98.8	68426	PASS
177	176	5	9	6.2	4242	PASS