
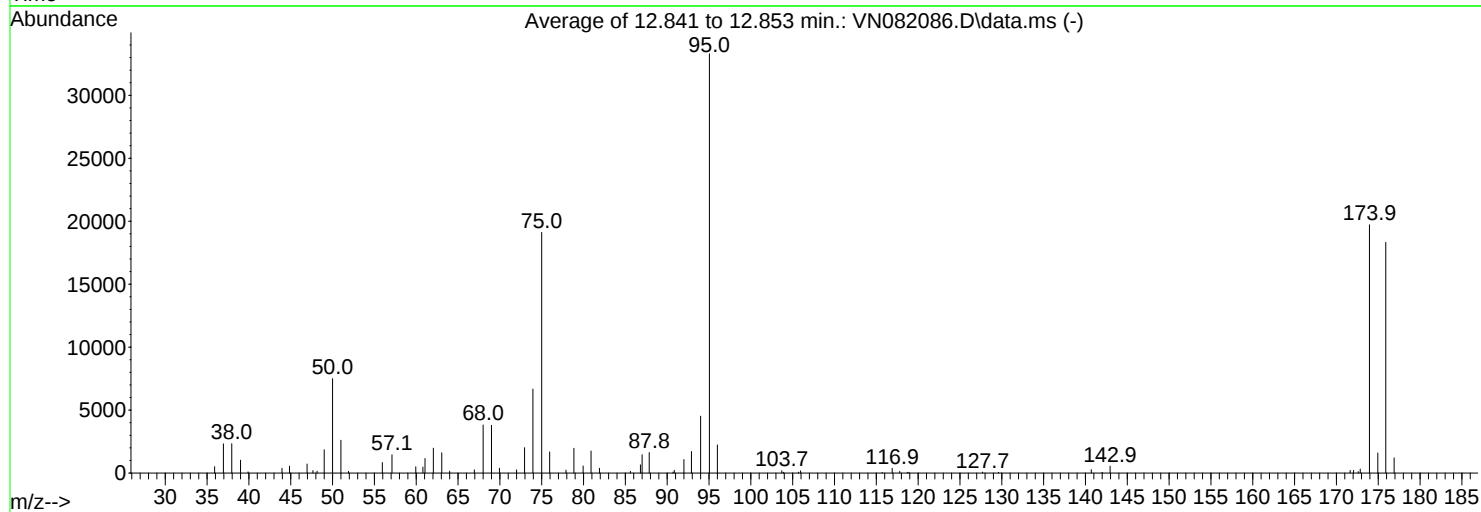


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN051324\
Data File : VN082086.D
Acq On : 13 May 2024 09:50
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT3.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\624N042624W.M
Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
Last Update : Tue May 14 11:29:16 2024

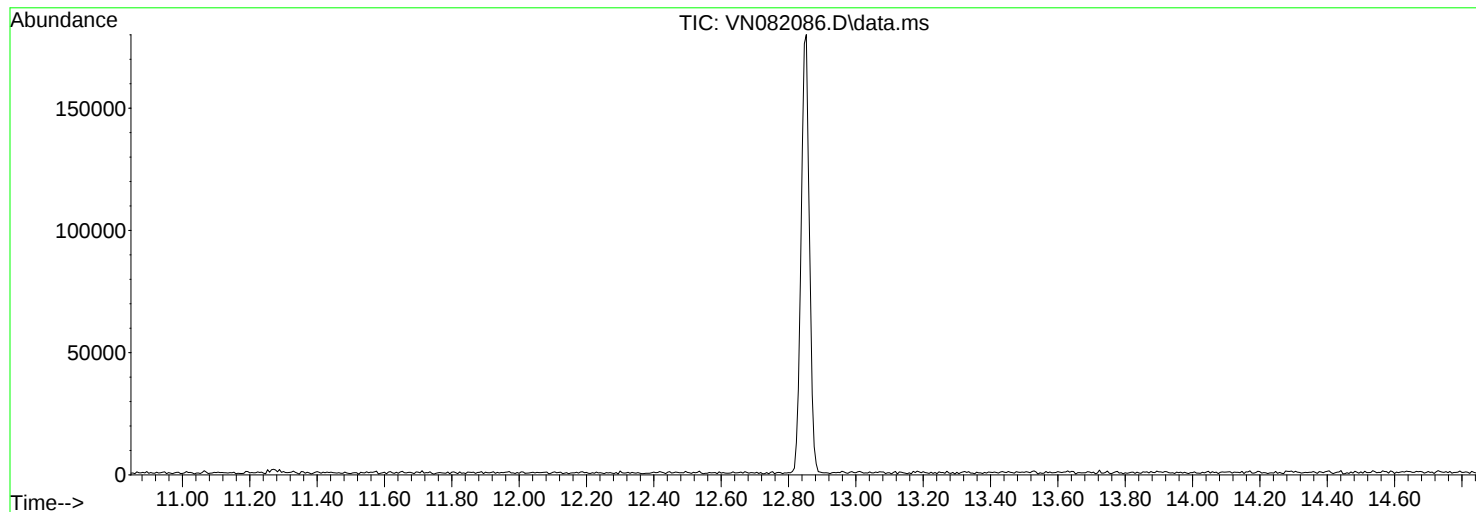

AutoFind: Scans 1851, 1852, 1853; Background Corrected with Scan 1845

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.5	7500	PASS
75	95	30	60	57.4	19114	PASS
95	95	100	100	100.0	33304	PASS
96	95	5	9	6.7	2237	PASS
173	174	0.00	2	1.6	320	PASS
174	95	50	100	59.2	19721	PASS
175	174	5	9	8.1	1597	PASS
176	174	95	101	92.9	18323	FAIL*
177	176	5	9	6.6	1212	PASS