

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN051325\
 Data File : VN086591.D
 Acq On : 13 May 2025 10:57
 Operator : JC\MD
 Sample : VN0513MBL01
 Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_N/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 VN0513MBL01

Quant Time: May 14 01:38:55 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N041525W.M
 Quant Title : SW846 8260
 QLast Update : Wed Apr 16 04:19:23 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	8.224	168	192372	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	9.100	114	365313	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.865	117	352602	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.788	152	151057	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.577	65	123566	44.296	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	=	88.600%
35) Dibromofluoromethane	8.165	113	97618	57.576	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	115.160%
50) Toluene-d8	10.565	98	422779	46.657	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	=	93.320%
62) 4-Bromofluorobenzene	12.847	95	153620	46.480	ug/l	0.00
Spiked Amount	50.000	Range	77 - 121	Recovery	=	92.960%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN051325\
Data File : VN086591.D
Acq On : 13 May 2025 10:57
Operator : JC\MD
Sample : VN0513MBL01
Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_N/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
VN0513MBL01


Quant Time: May 14 01:38:55 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N041525W.M
Quant Title : SW846 8260
QLast Update : Wed Apr 16 04:19:23 2025
Response via : Initial Calibration

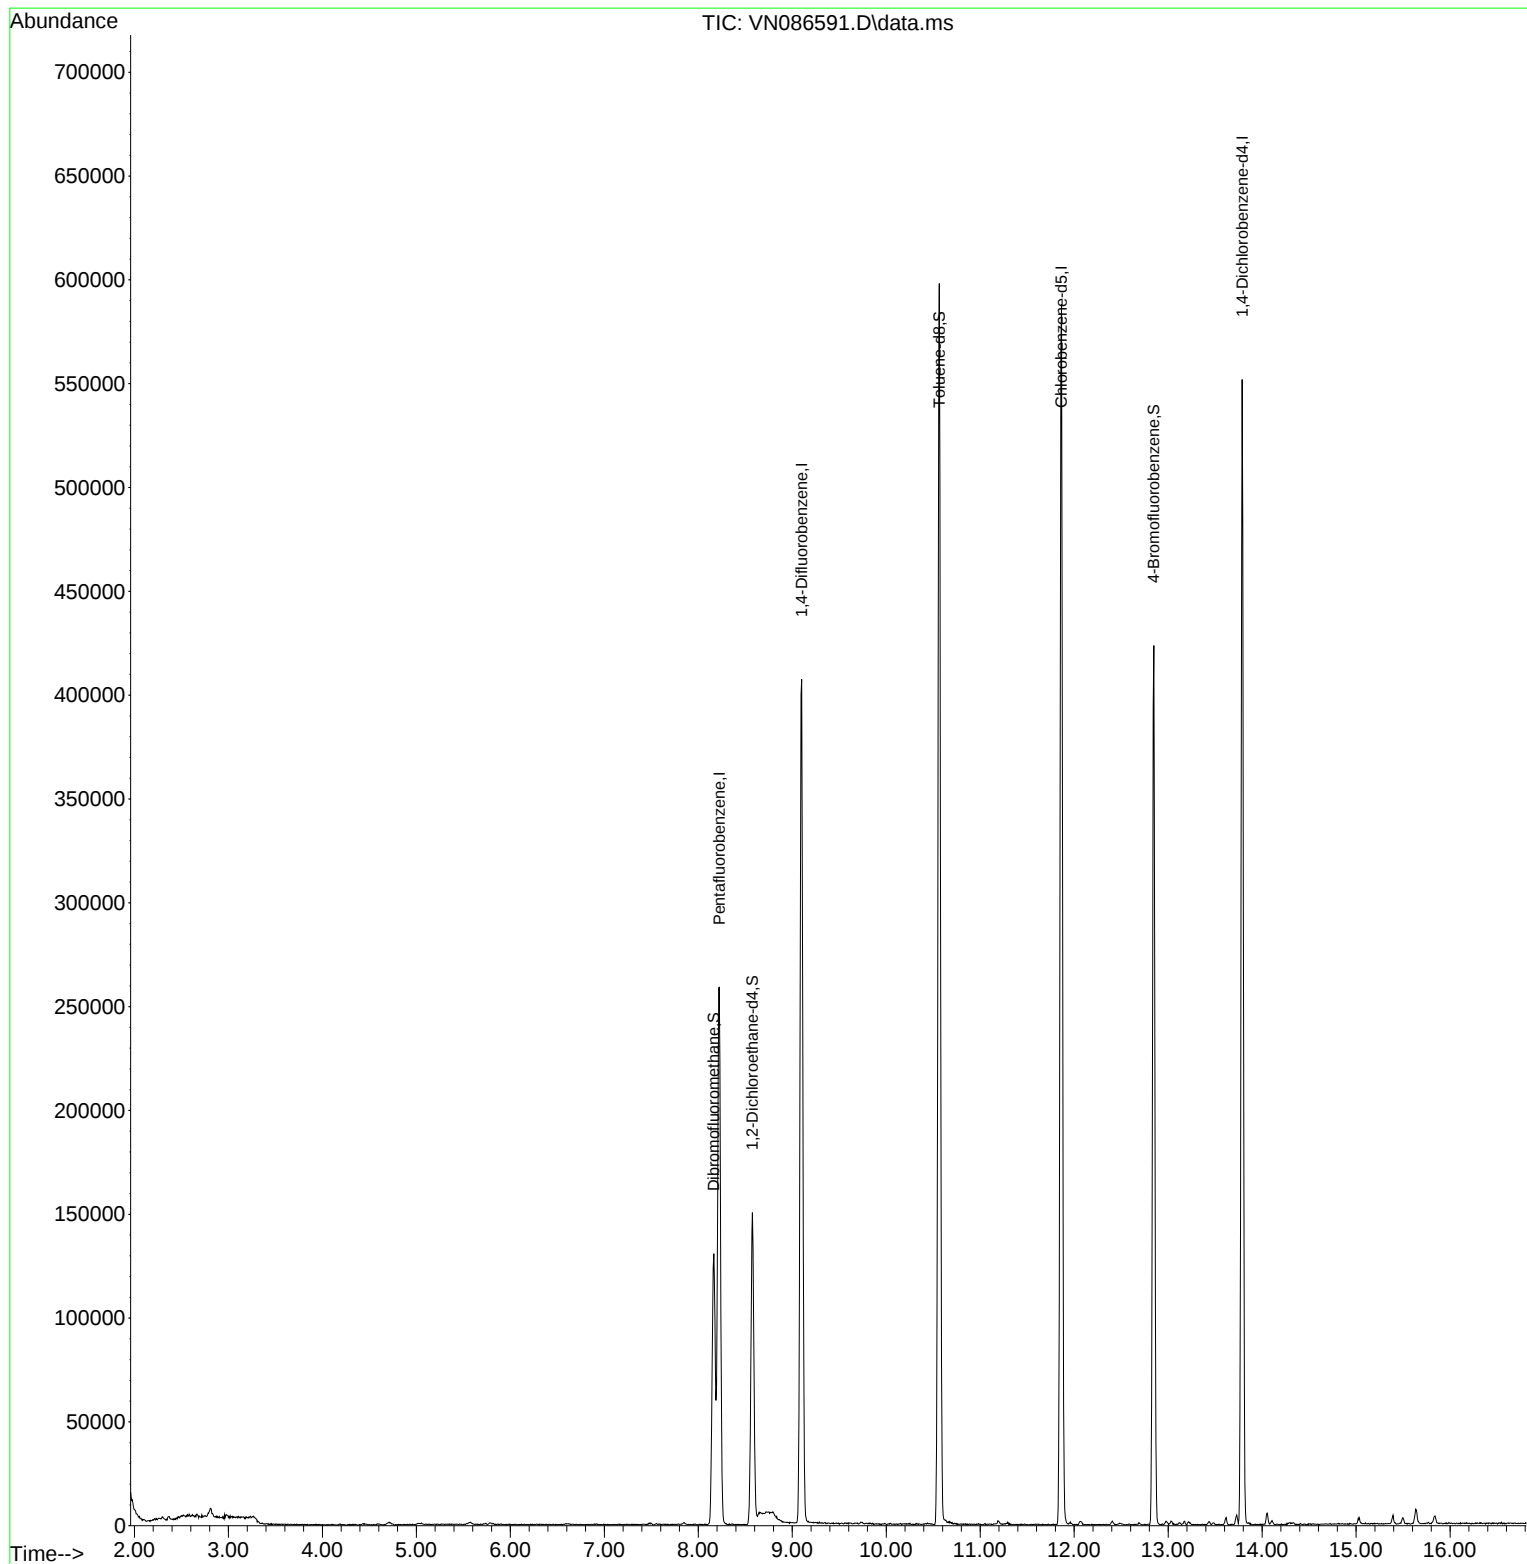



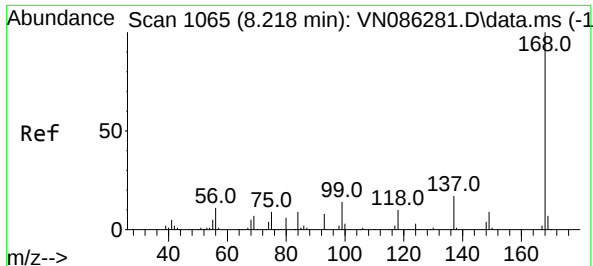


#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.224 min Scan# 1066
Delta R.T. 0.006 min
Lab File: VN086591.D
Acq: 13 May 2025 10:57

Instrument :
MSVOA_N
ClientSampleId :
VN0513MBL01



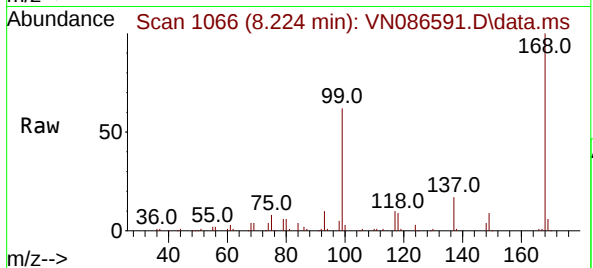



Tgt Ion:168 Resp: 192372
Ion Ratio Lower Upper
168 100
99 61.5 52.5 78.7

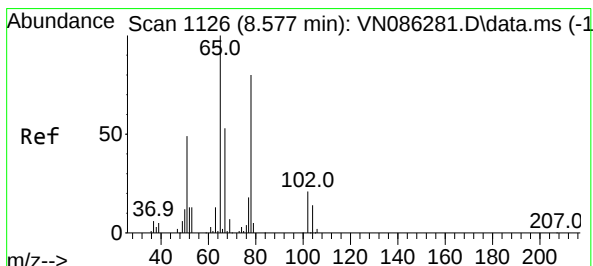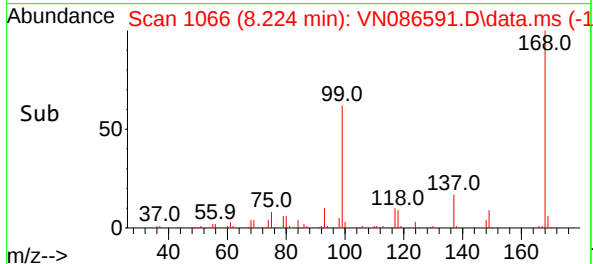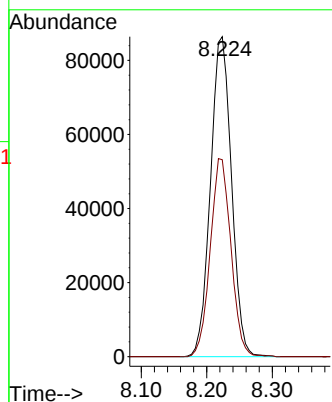

#33
1,2-Dichloroethane-d4
Concen: 44.296 ug/l
RT: 8.577 min Scan# 1126
Delta R.T. -0.000 min
Lab File: VN086591.D
Acq: 13 May 2025 10:57

Tgt Ion: 65 Resp: 123566
Ion Ratio Lower Upper
65 100
67 51.6 0.0 106.0

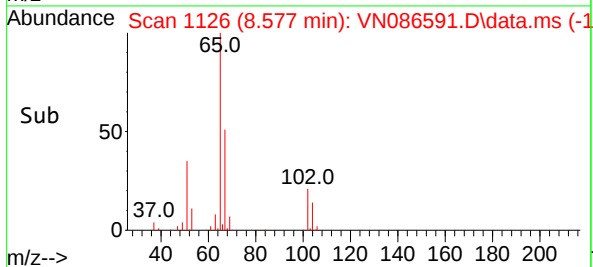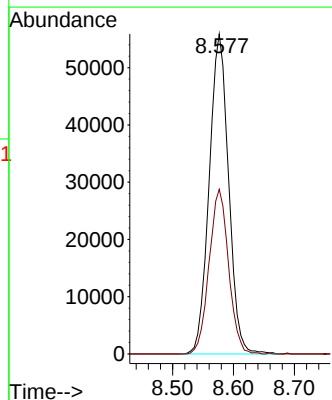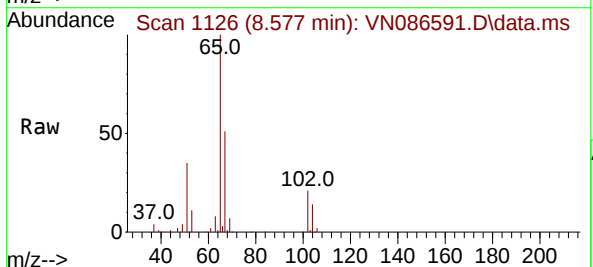

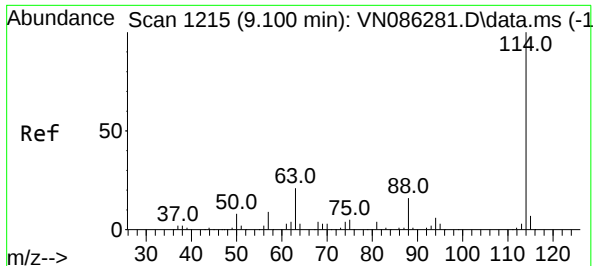

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 9.100 min Scan# 1

Delta R.T. -0.000 min

Lab File: VN086591.D

Acq: 13 May 2025 10:57

Instrument :

MSVOA_N

ClientSampleId :

VN0513MBL01





Tgt Ion:114 Resp: 365313

Ion Ratio Lower Upper

114 100

63 19.9 0.0 42.6

88 16.2 0.0 31.8

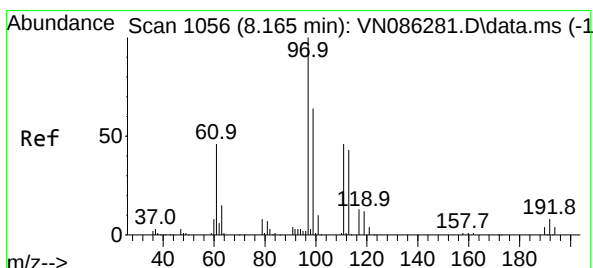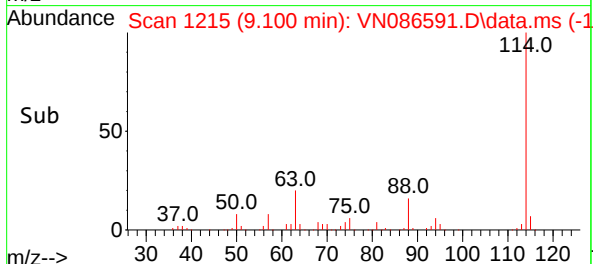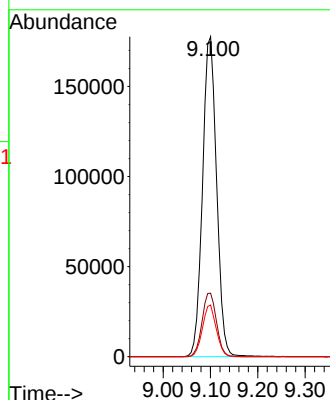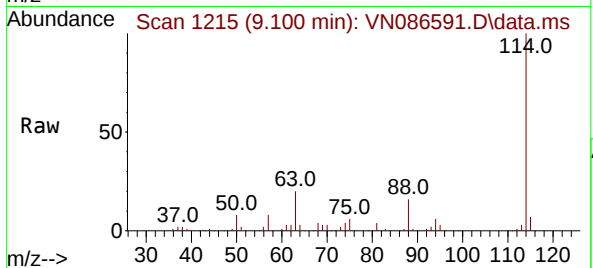

#35

Dibromofluoromethane

Concen: 57.576 ug/l

RT: 8.165 min Scan# 1056

Delta R.T. -0.000 min

Lab File: VN086591.D

Acq: 13 May 2025 10:57




Tgt Ion:113 Resp: 97618


Ion Ratio Lower Upper

113 100

111 103.2 83.4 125.0

192 17.7 13.7 20.5


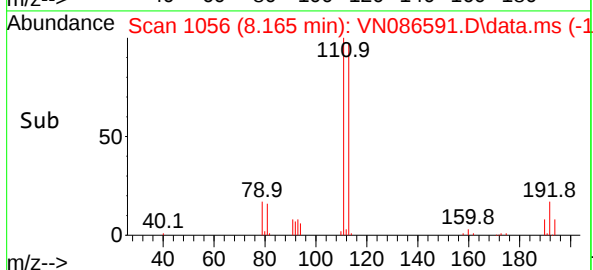
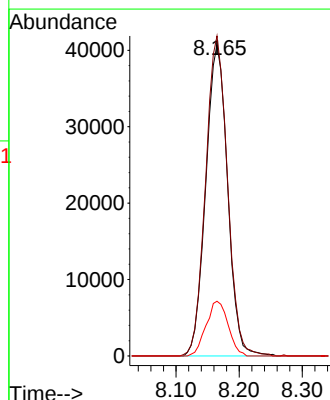
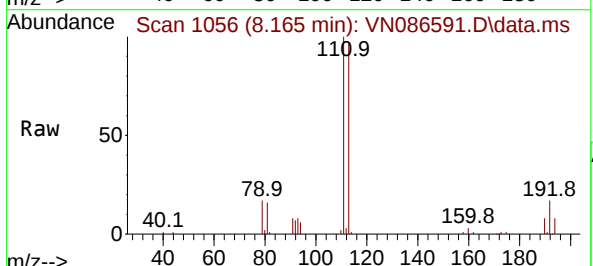


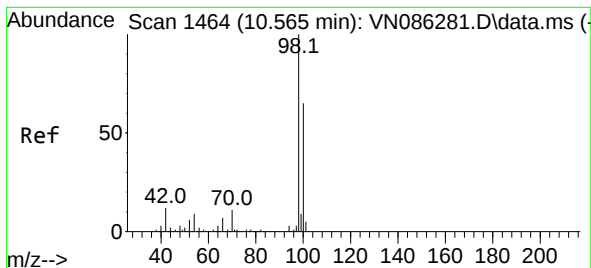

#50
Toluene-d8
Concen: 46.657 ug/l
RT: 10.565 min Scan# 1464
Delta R.T. -0.000 min
Lab File: VN086591.D
Acq: 13 May 2025 10:57




Instrument :
MSVOA_N
ClientSampleId :
VN0513MBL01


Tgt Ion: 98 Resp: 422779
Ion Ratio Lower Upper
98 100
100 65.4 52.5 78.7

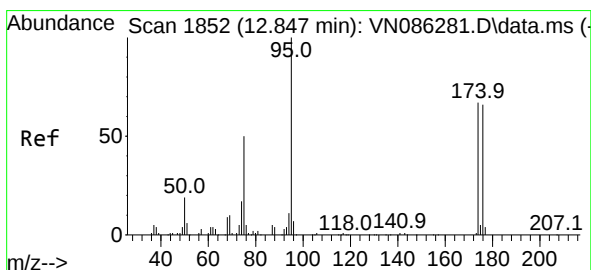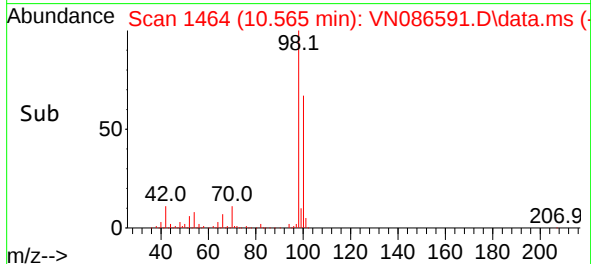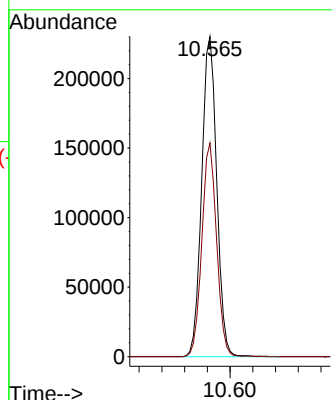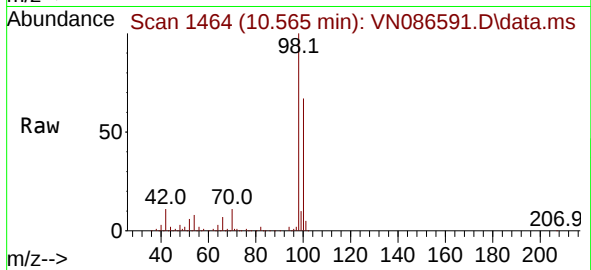

#62
4-Bromofluorobenzene
Concen: 46.480 ug/l
RT: 12.847 min Scan# 1852
Delta R.T. -0.000 min
Lab File: VN086591.D
Acq: 13 May 2025 10:57

Tgt Ion: 95 Resp: 153620
Ion Ratio Lower Upper
95 100
174 73.1 0.0 133.4
176 71.0 0.0 129.2


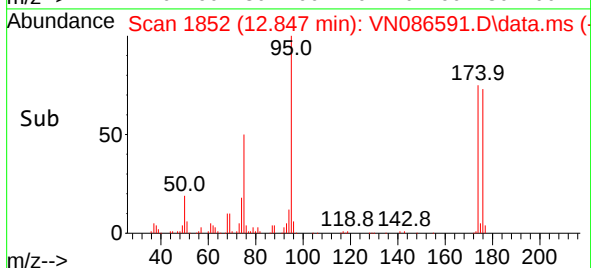
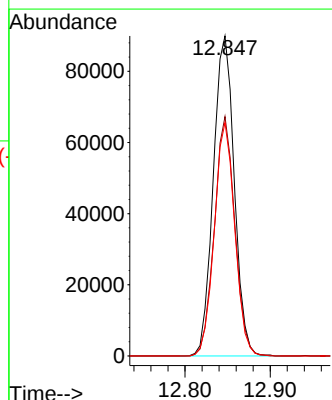
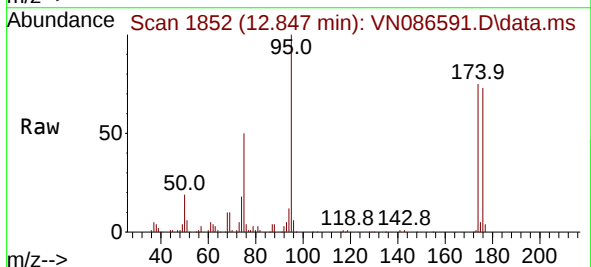


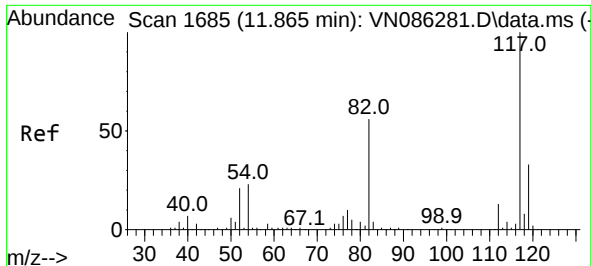

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.865 min Scan# 117
Delta R.T. -0.000 min
Lab File: VN086591.D
Acq: 13 May 2025 10:57

Instrument :
MSVOA_N
ClientSampleId :
VN0513MBL01

Tgt Ion:117 Resp: 352602
Ion Ratio Lower Upper
117 100
82 56.3 44.7 67.1
119 33.0 26.4 39.6

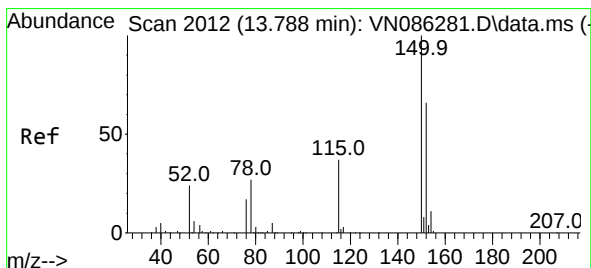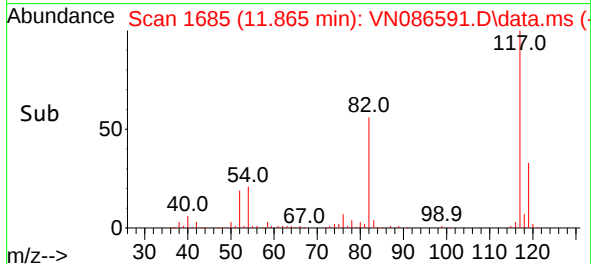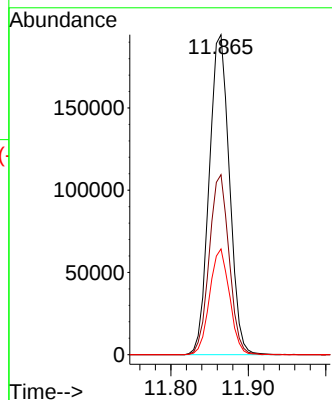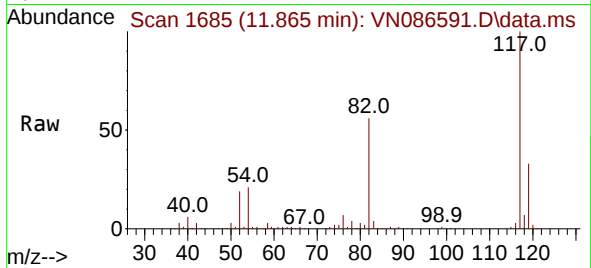

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.788 min Scan# 2012
Delta R.T. -0.000 min
Lab File: VN086591.D
Acq: 13 May 2025 10:57

Tgt Ion:152 Resp: 151057
Ion Ratio Lower Upper
152 100
115 61.0 31.9 95.9
150 157.6 0.0 352.0

