
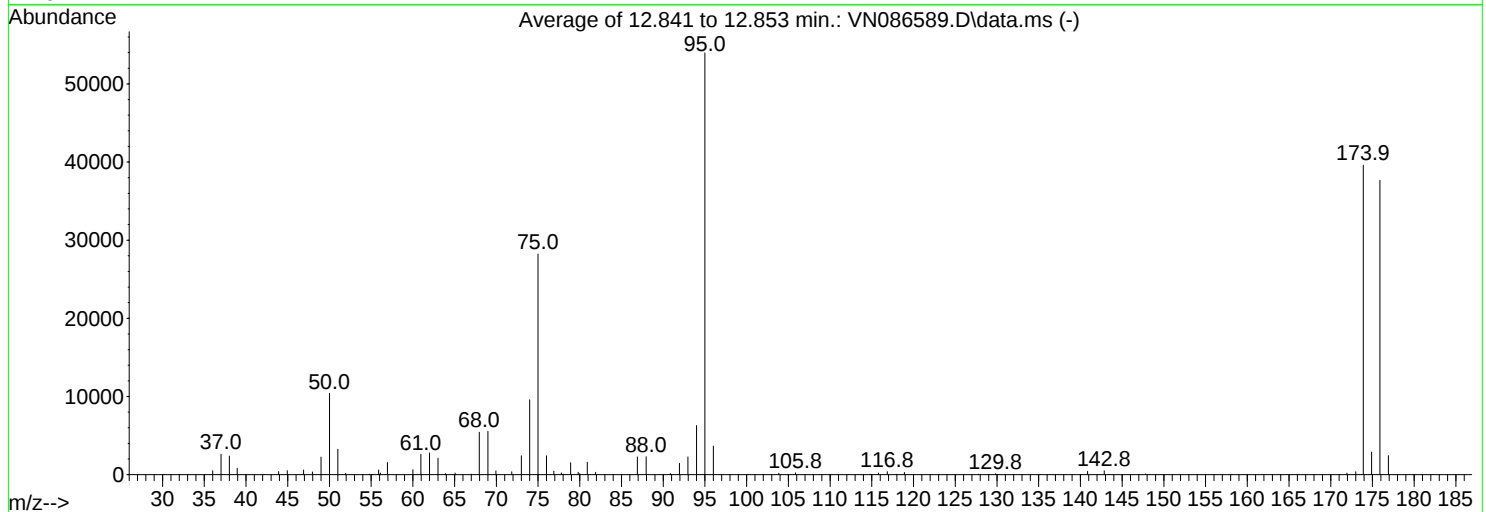


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN051325\
Data File : VN086589.D
Acq On : 13 May 2025 09:47
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N041525W.M
Title : SW846 8260
Last Update : Wed Apr 16 04:19:23 2025

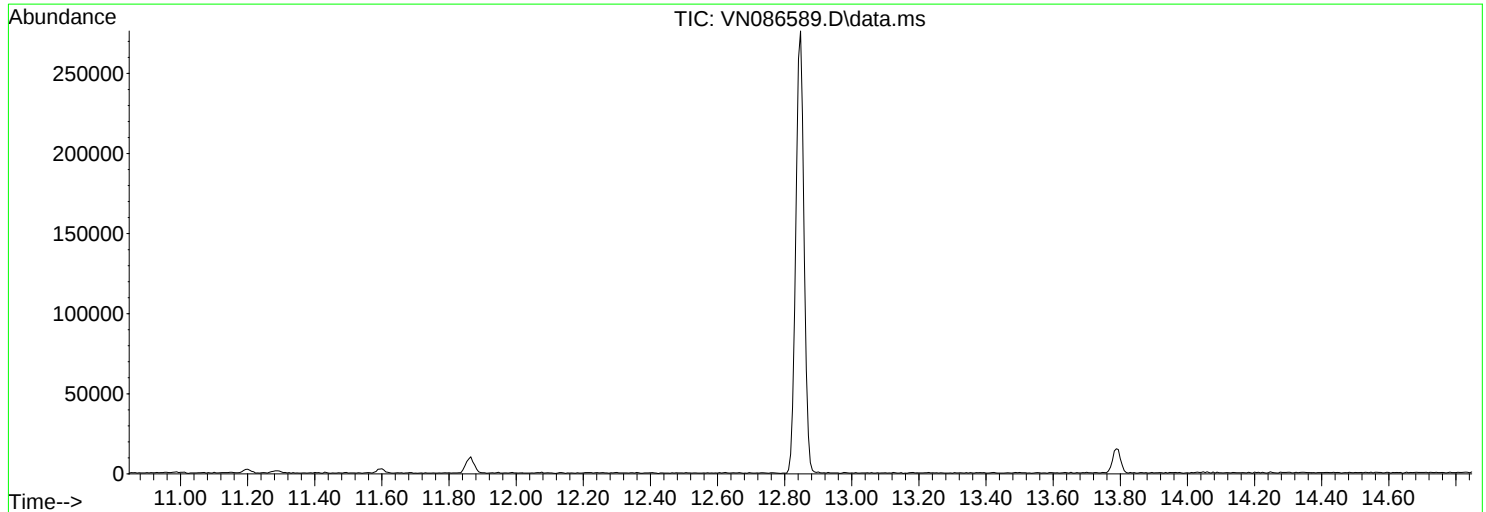

AutoFind: Scans 1851, 1852, 1853; Background Corrected with Scan 1843

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.3	10395	PASS
75	95	30	60	52.3	28224	PASS
95	95	100	100	100.0	53971	PASS
96	95	5	9	6.8	3659	PASS
173	174	0.00	2	0.9	368	PASS
174	95	50	100	73.4	39605	PASS
175	174	5	9	7.3	2894	PASS
176	174	95	101	95.1	37677	PASS
177	176	5	9	6.5	2439	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.00	504	51.95	172	65.05	198	77.80	22
37.00	2615	54.80	66	67.00	62	78.10	50
38.00	2375	55.10	50	67.95	5417	78.90	152
38.95	816	55.90	595	69.00	5555	79.80	31
43.90	395	56.10	205	69.95	484	80.00	152
44.95	511	56.95	1551	71.85	372	80.90	1589
46.90	600	60.00	637	73.00	2417	81.90	315
47.95	354	60.95	2599	74.00	9580	86.90	2273
49.00	2249	62.00	2795	75.00	28224	87.95	2287
50.00	10395	63.00	2108	76.00	2418	90.85	141
51.00	3267	63.90	144	76.90	446	91.95	1463

Average of 12.841 to 12.853 min.: VN086589.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
92.95	2268	127.80	67				
94.00	6290	129.85	116				
95.00	53971	140.85	424				
96.00	3659	142.85	491				
103.85	180	147.80	105				
105.85	217	171.95	196				
114.80	56	173.00	368				
115.80	203	173.90	39605				
116.85	385	174.90	2894				
117.90	61	175.90	37677				
118.90	288	176.90	2439				

Instrument :

MSVOA_N

ClientSampleId :

BFB