



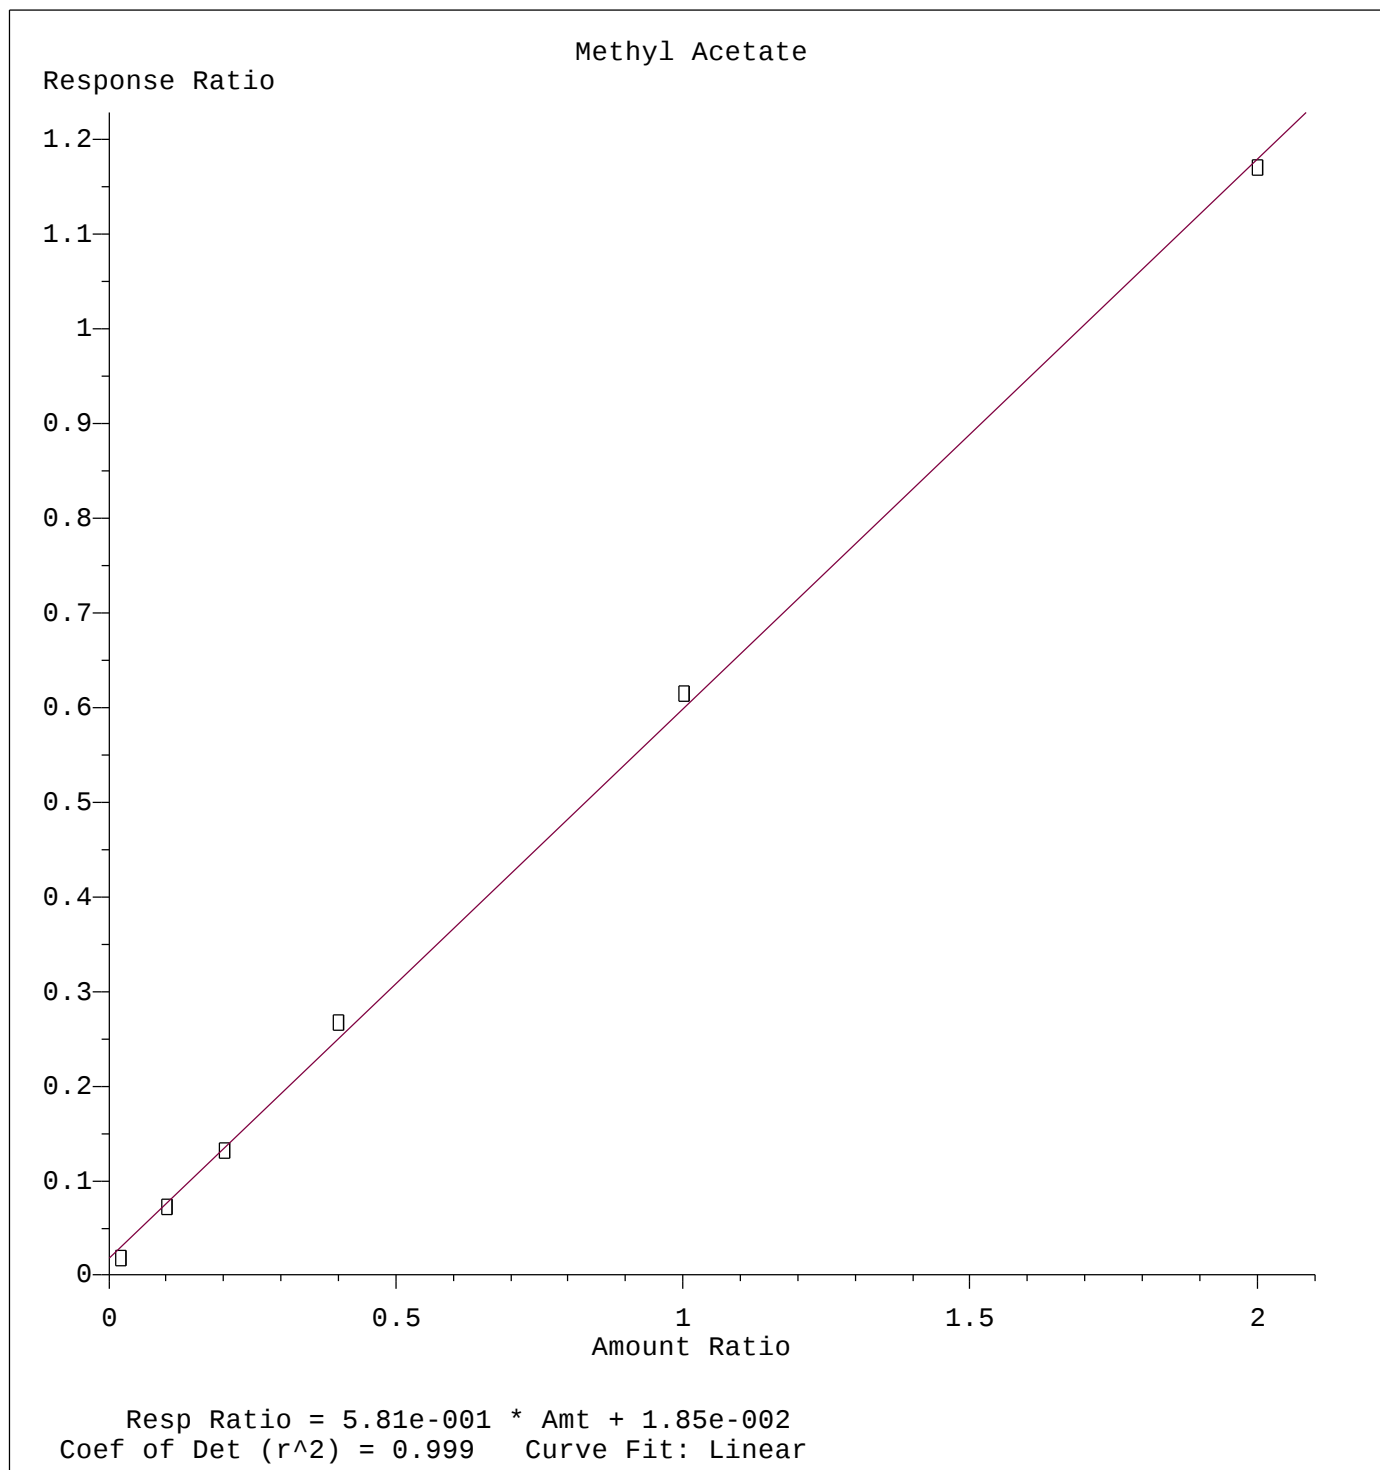

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N051419W.M
Calibration Table Last Updated: Wed May 15 07:28:47 2019

2-Chloroethyl Vinyl ether

Response Ratio

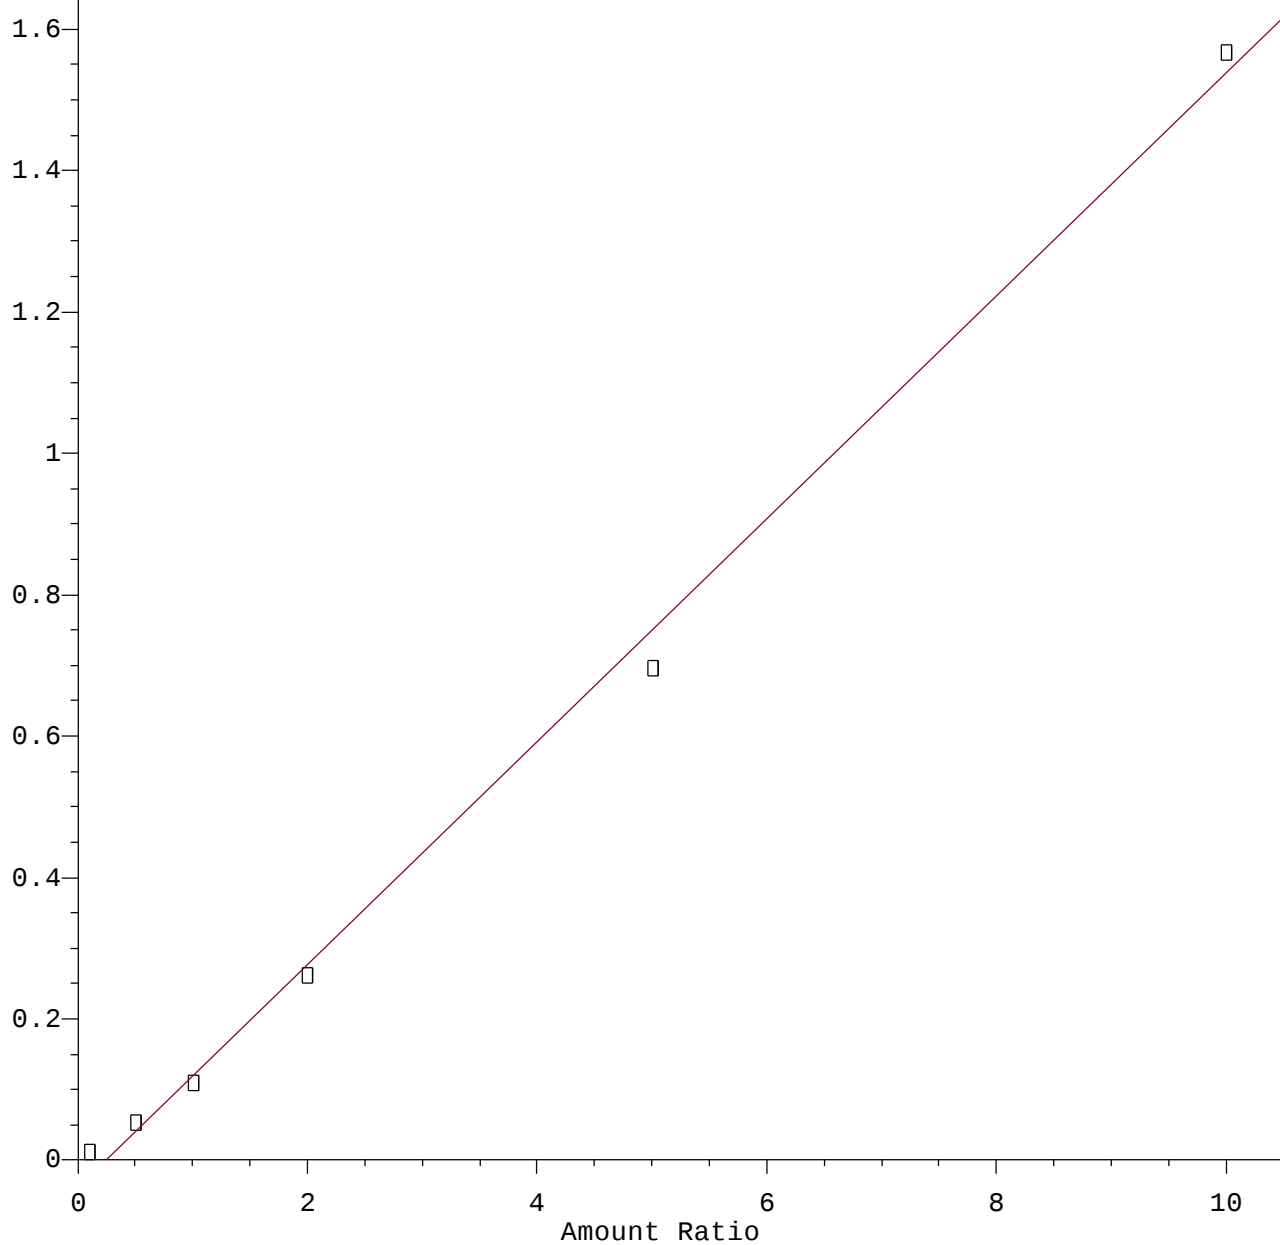


Resp Ratio = $1.58 \times 10^{-1} \times \text{Amt} - 3.96 \times 10^{-2}$
Coef of Det (r^2) = 0.997 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N051419W.M
Calibration Table Last Updated: Wed May 15 07:28:47 2019


1,1,2,2-Tetrachloroethane

Response Ratio

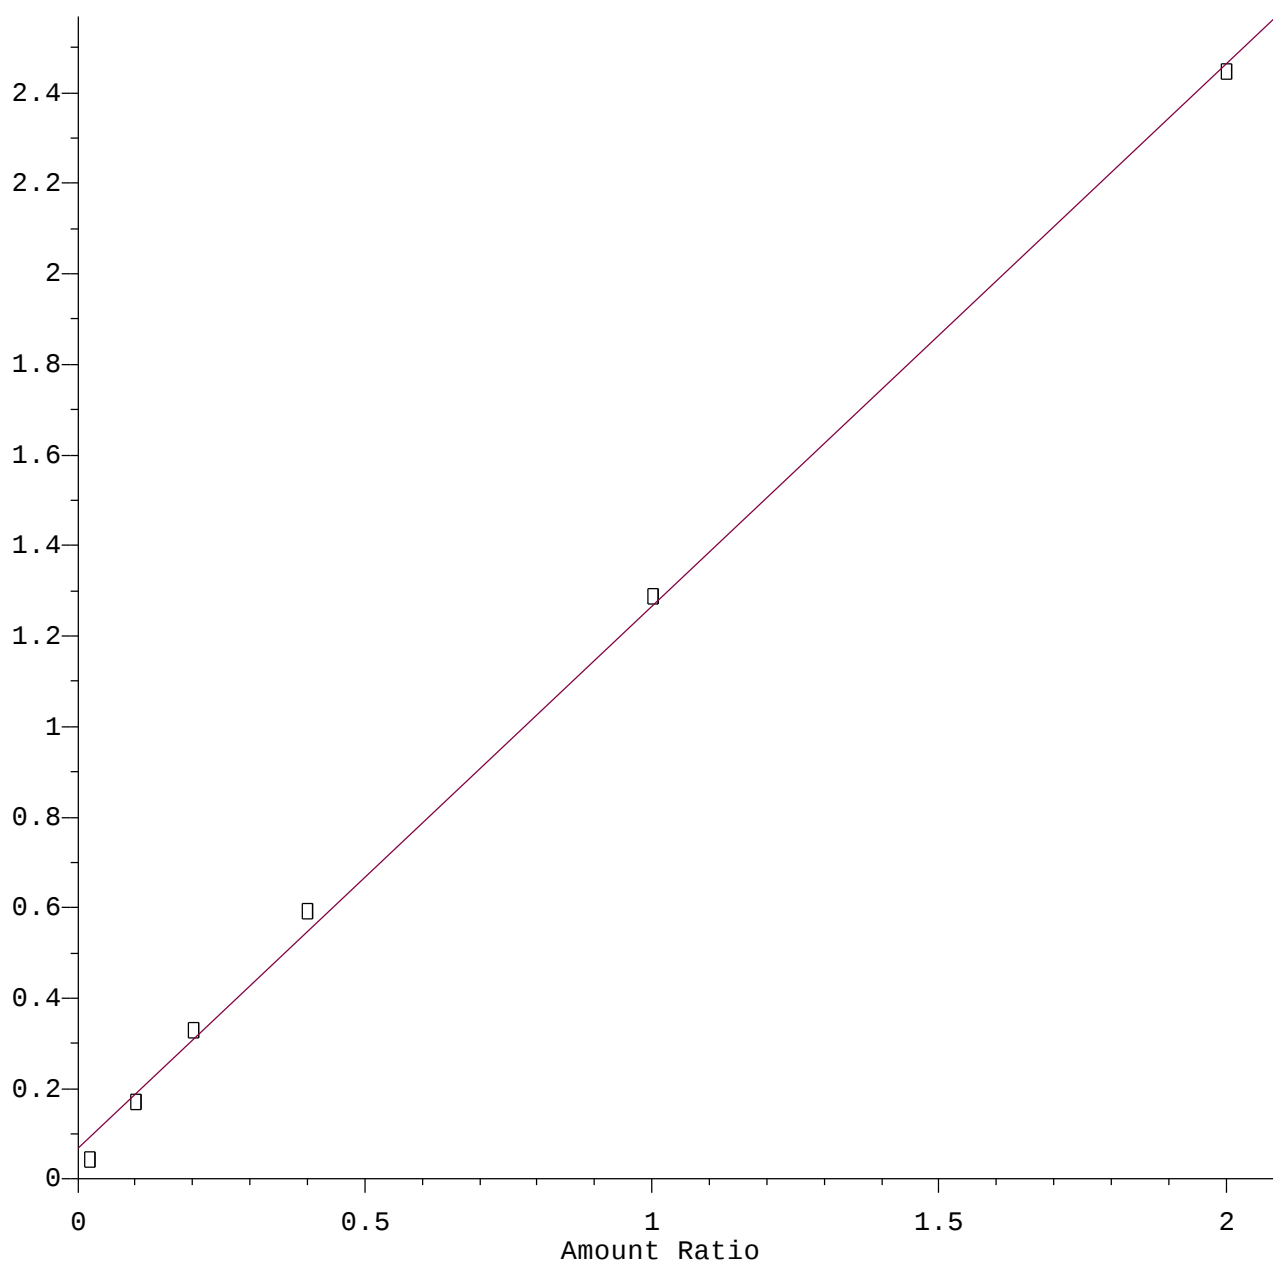


Resp Ratio = 1.20e+000 * Amt + 6.75e-002
Coef of Det (r^2) = 0.999 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N051419W.M
Calibration Table Last Updated: Wed May 15 07:28:47 2019

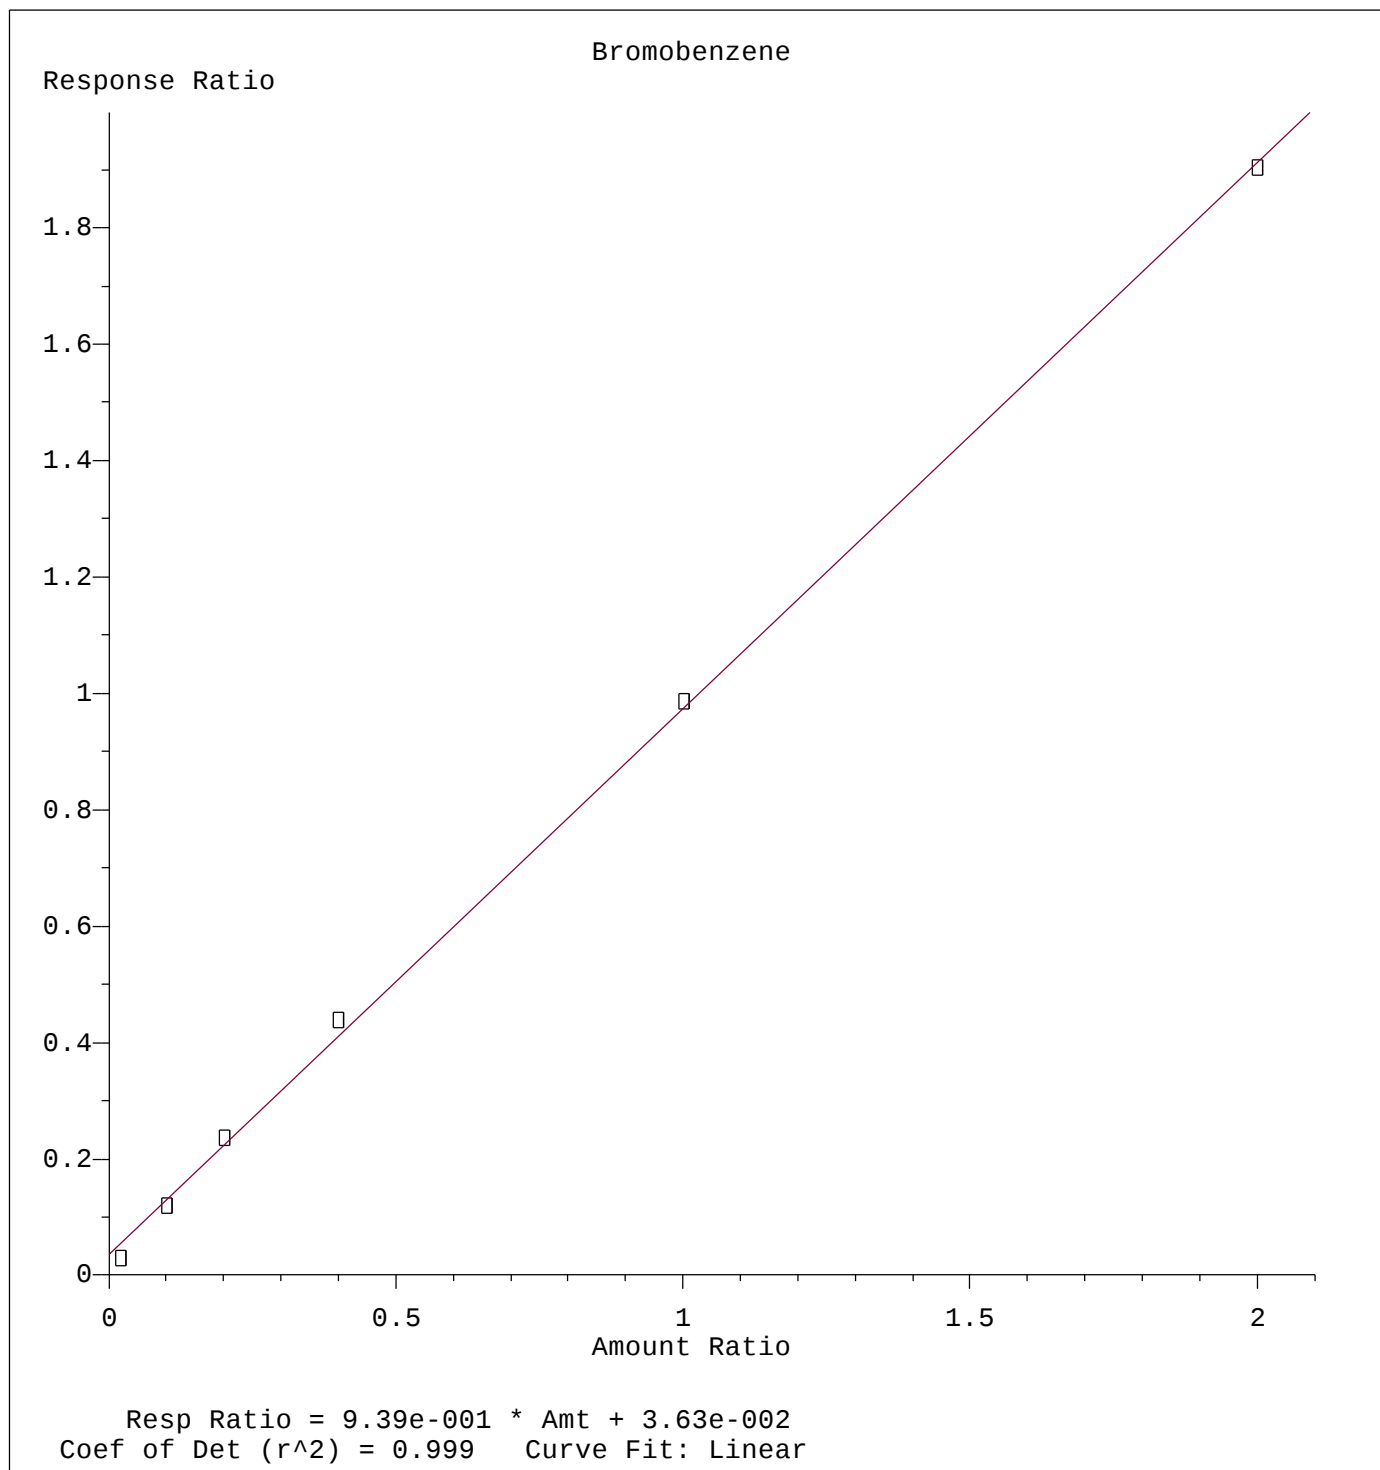


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N051419W.M
Calibration Table Last Updated: Wed May 15 07:28:47 2019

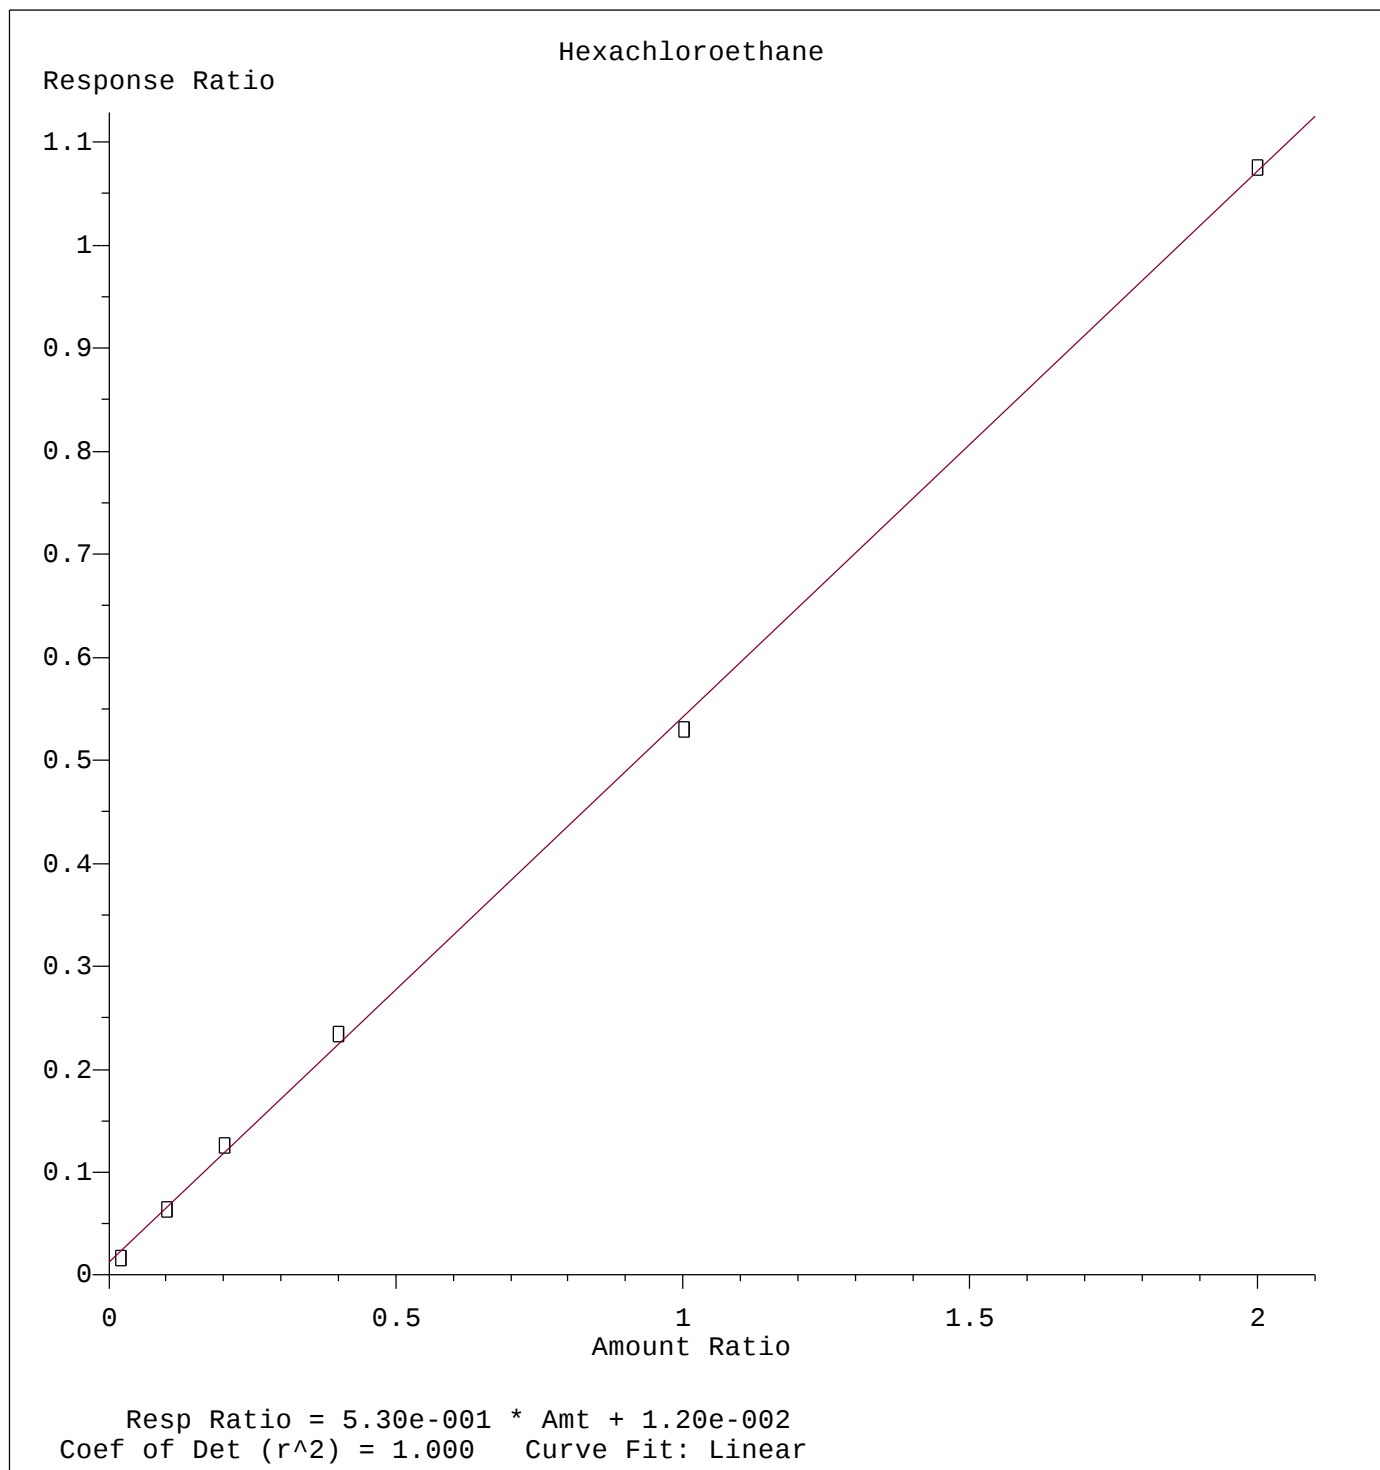

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N051419W.M
Calibration Table Last Updated: Wed May 15 07:28:47 2019


1,2,4-Trichlorobenzene

Response Ratio

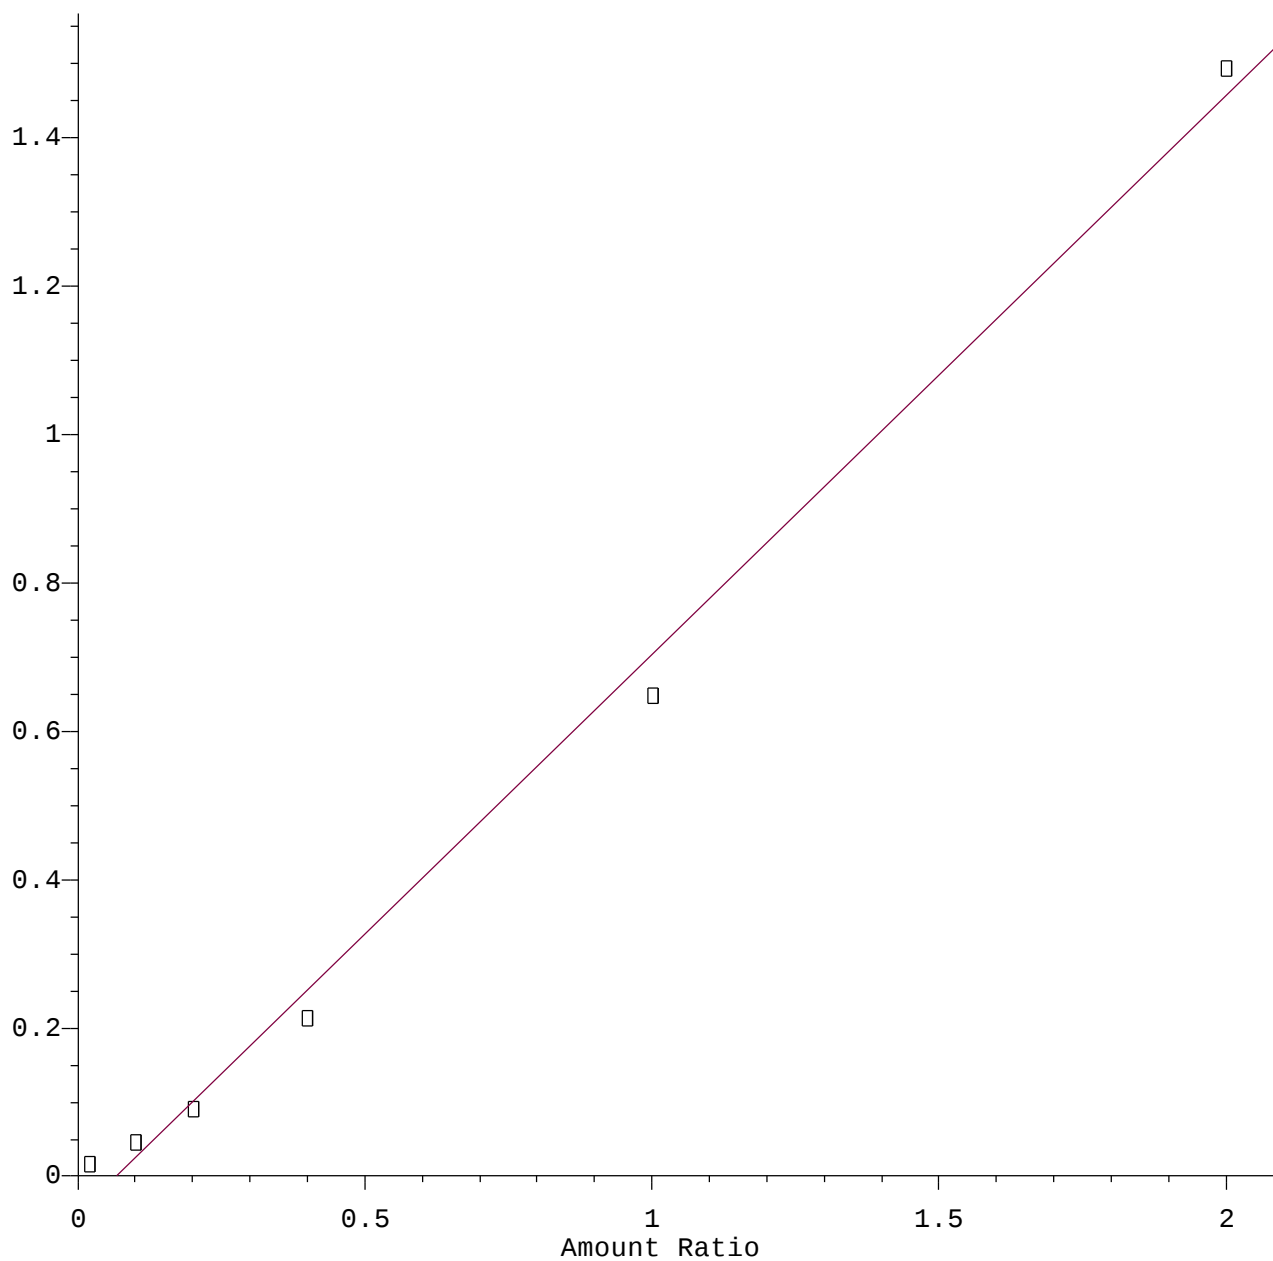


Resp Ratio = $7.54 \times 10^{-1} \times \text{Amt} - 5.05 \times 10^{-2}$
Coef of Det (r^2) = 0.995 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N051419W.M
Calibration Table Last Updated: Wed May 15 07:28:47 2019

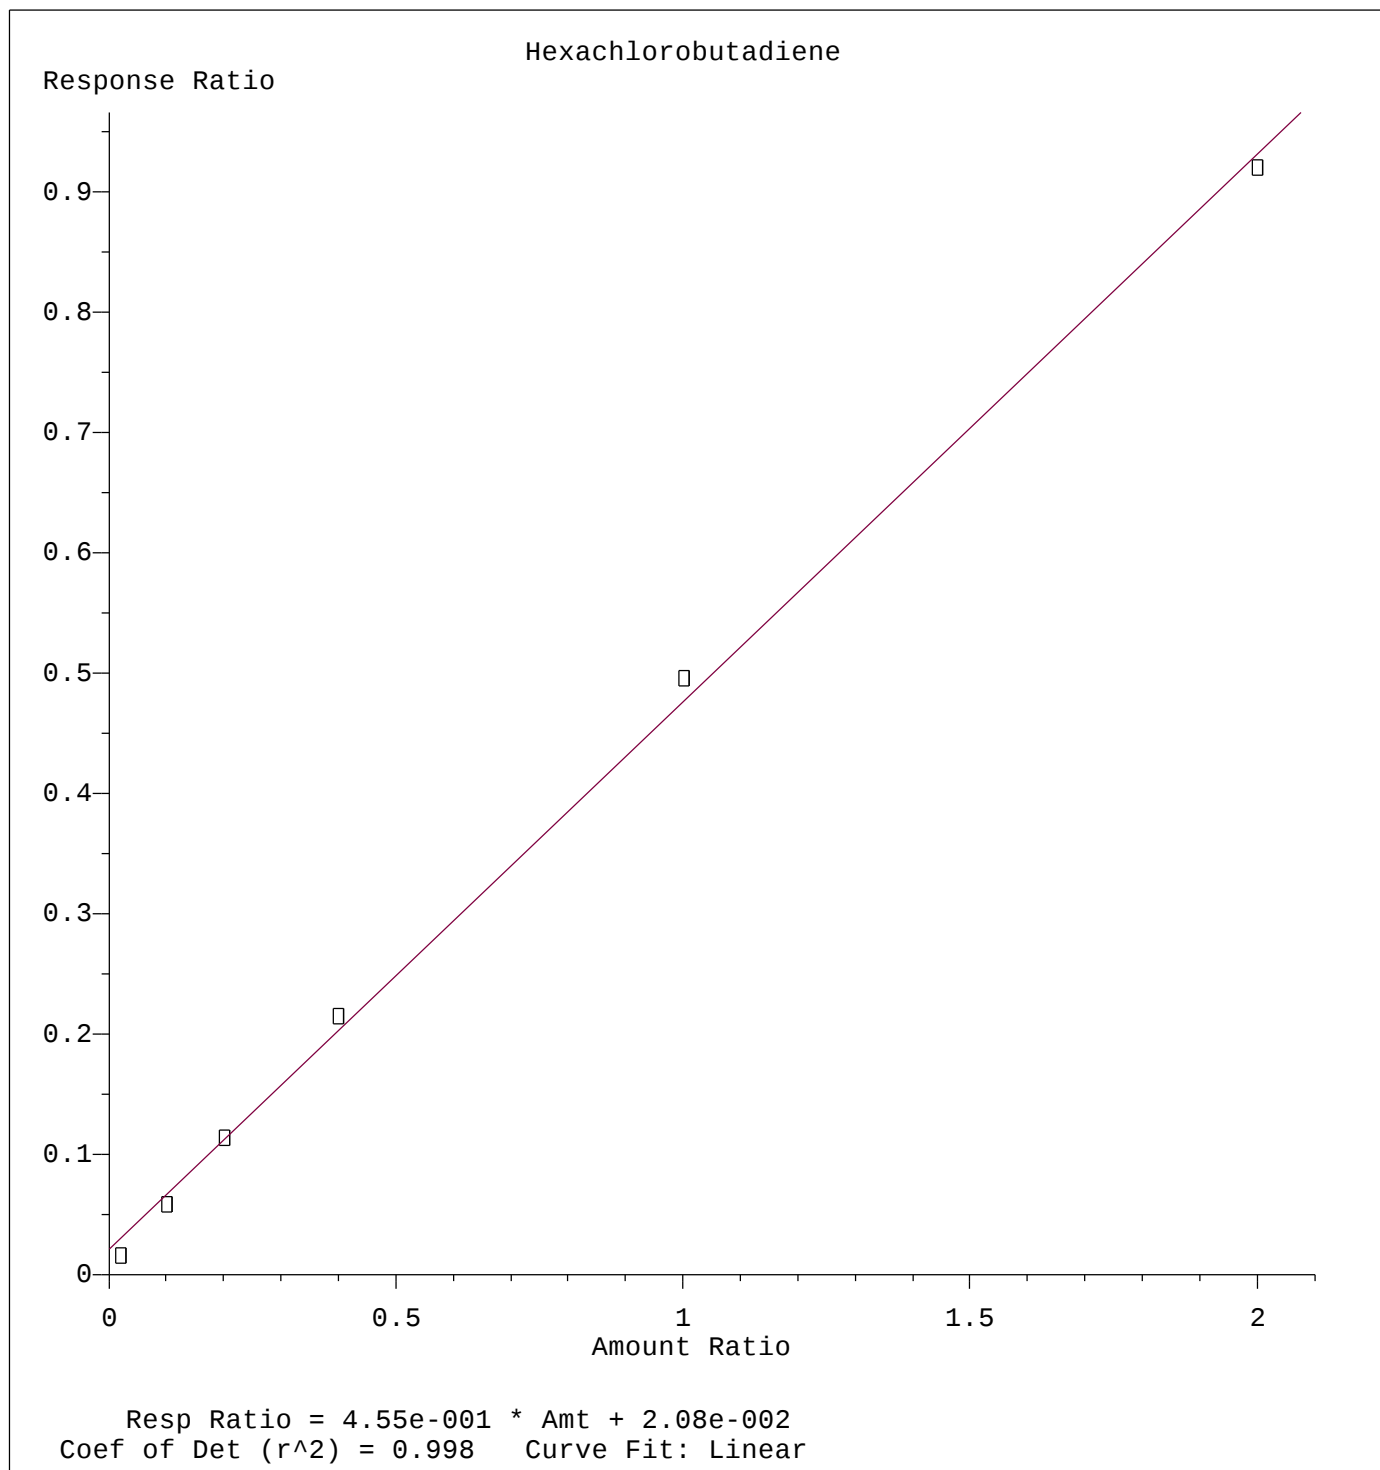


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N051419W.M
Calibration Table Last Updated: Wed May 15 07:28:47 2019

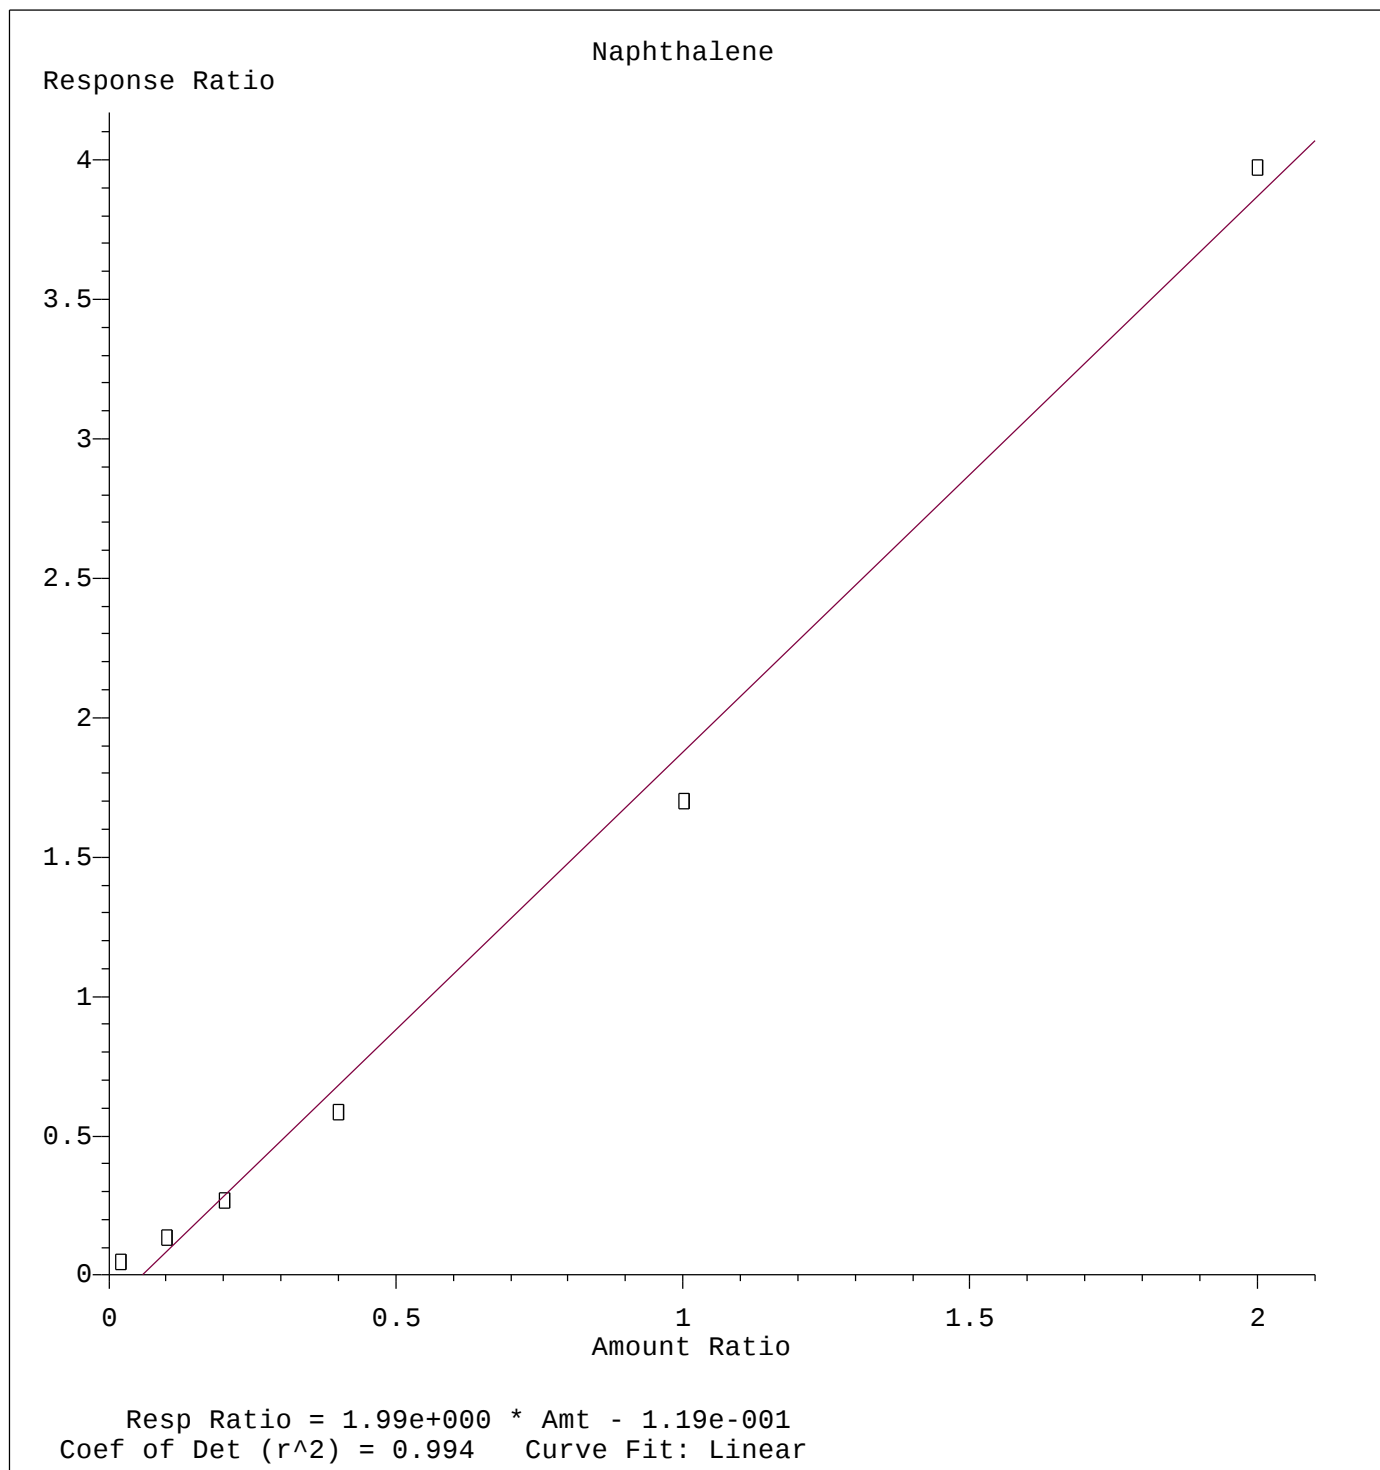

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N051419W.M
Calibration Table Last Updated: Wed May 15 07:28:47 2019

1,2,3-Trichlorobenzene

Response Ratio

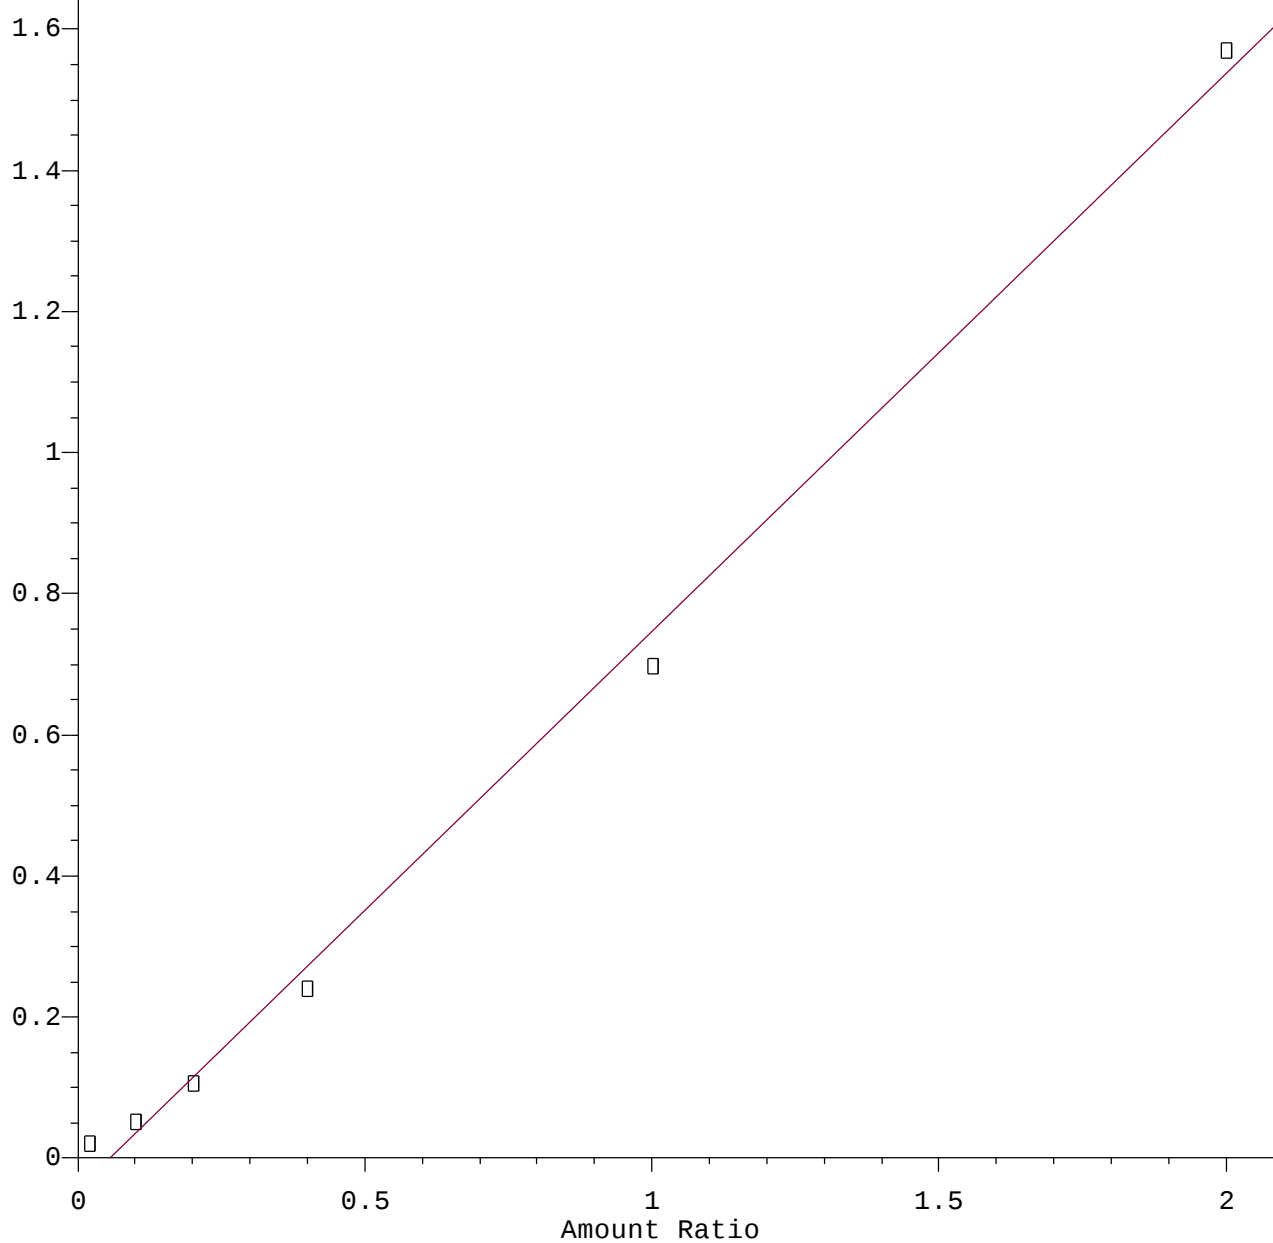

Resp Ratio = $7.90 \times 10^{-1} \times \text{Amt} - 4.36 \times 10^{-2}$
Coef of Det (r^2) = 0.996 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N051419W.M
Calibration Table Last Updated: Wed May 15 07:28:47 2019