


Data Path : Z:\voasrv\HPCHEM1\MSVOA N\Data\VN051420\
 Data File : VN061391.D
 Acq On : 14 May 2020 13:40
 Operator : JC/MD
 Sample : BFB
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT3.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\624N051420W.M
 Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
 Last Update : Thu May 14 16:04:10 2020

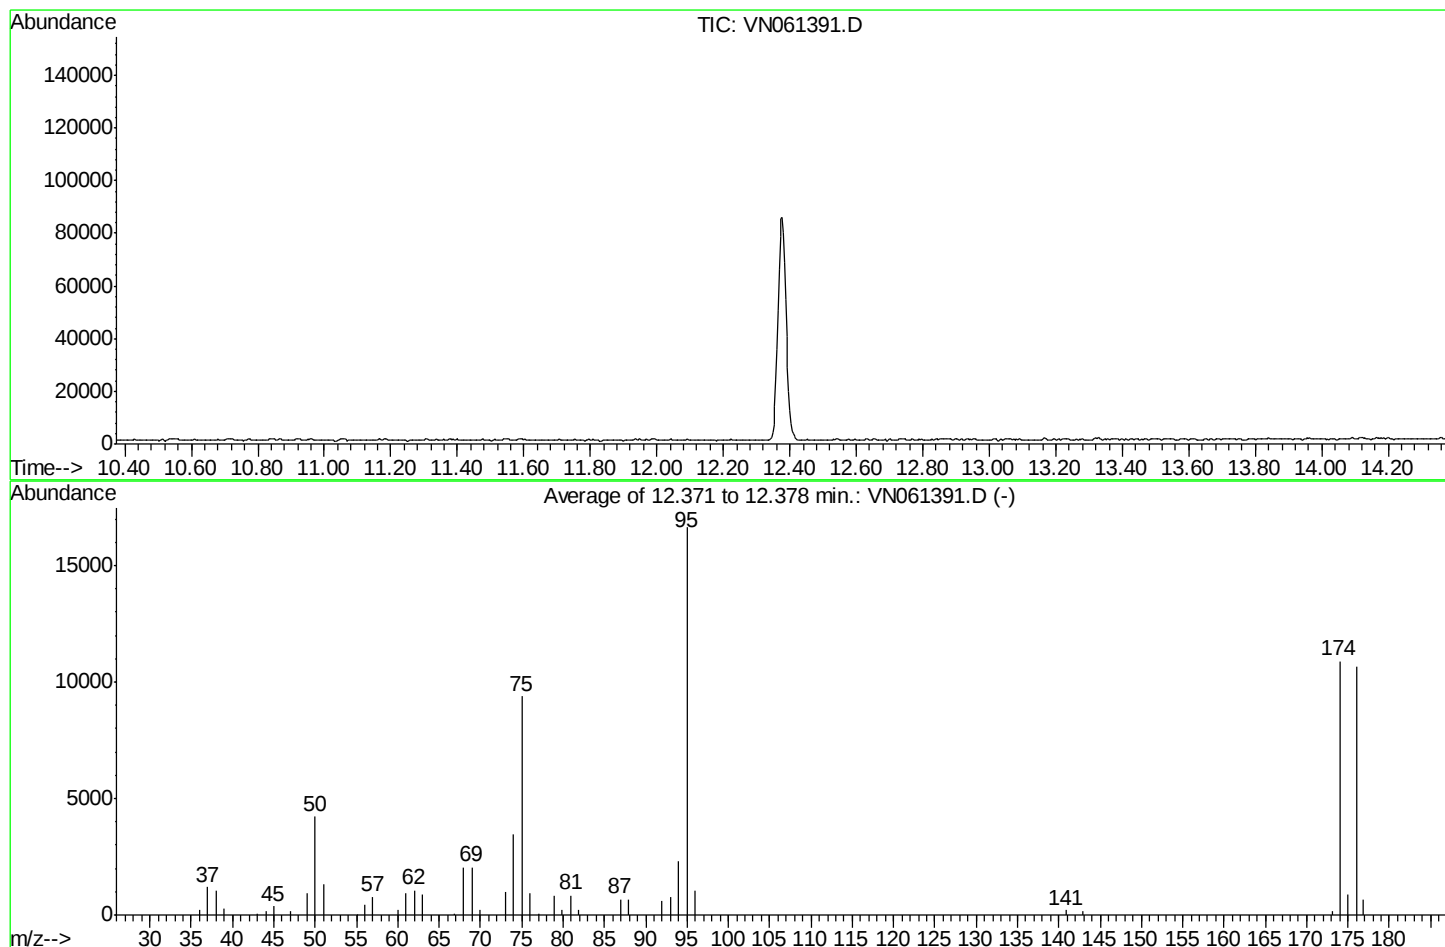

AutoFind: Scans 3296, 3297, 3298; Background Corrected with Scan 3285

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	25.4	4228	PASS
75	95	30	60	56.4	9387	PASS
95	95	100	100	100.0	16640	PASS
96	95	5	9	6.3	1049	PASS
173	174	0.00	2	1.8	193	PASS
174	95	50	100	65.5	10904	PASS
175	174	5	9	8.2	893	PASS
176	174	95	101	97.9	10676	PASS
177	176	5	9	6.4	686	PASS