
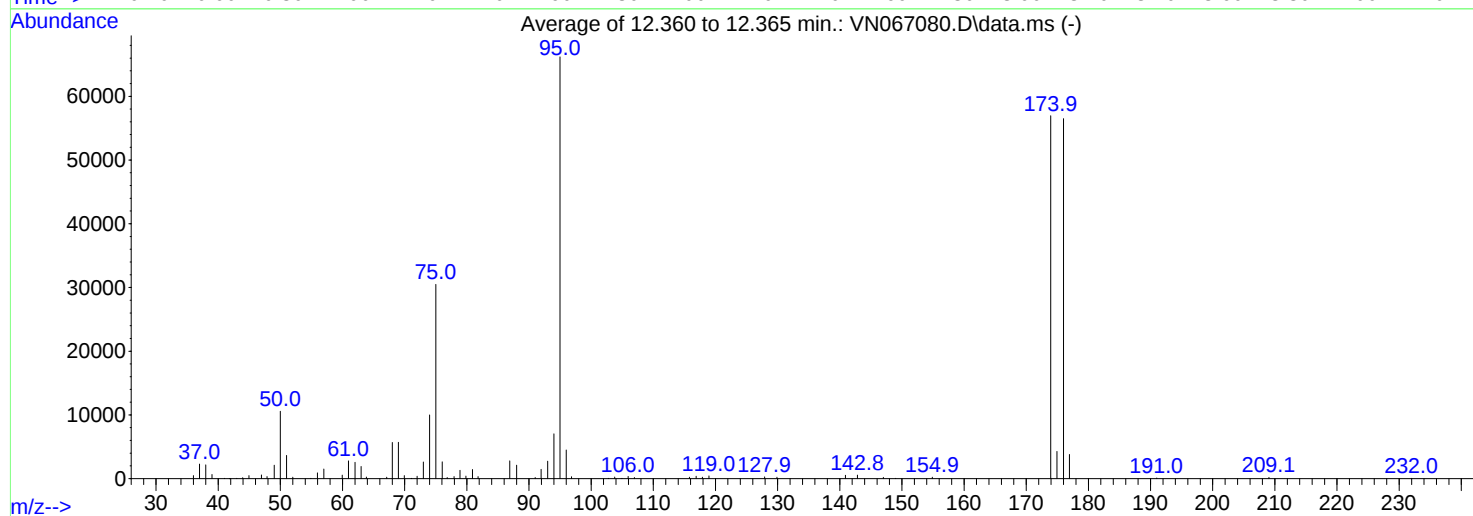


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN051421\
 Data File : VN067080.D
 Acq On : 14 May 2021 17:14
 Operator : JC/MD
 Sample : BFB
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N051421W.M
 Title : SW846 8260
 Last Update : Mon May 17 16:06:46 2021

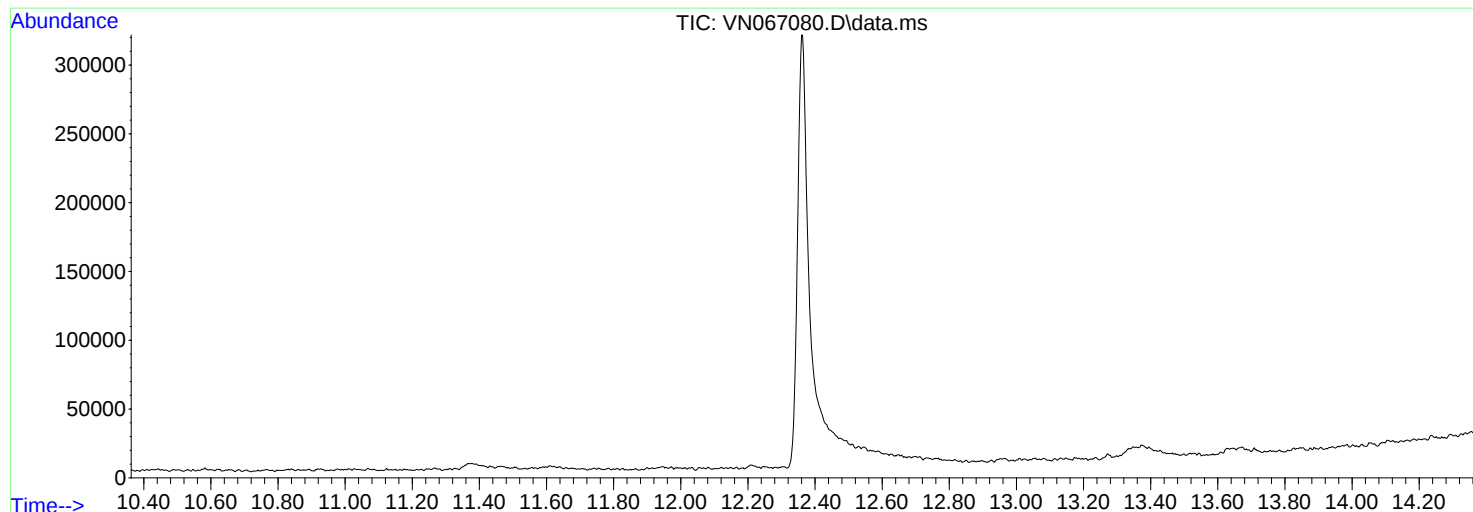

AutoFind: Scans 3960, 3961, 3962; Background Corrected with Scan 3942

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.0	10560	PASS
75	95	30	60	46.1	30493	PASS
95	95	100	100	100.0	66195	PASS
96	95	5	9	6.8	4497	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	86.0	56960	PASS
175	174	5	9	7.5	4279	PASS
176	174	95	101	99.2	56496	PASS
177	176	5	9	6.7	3803	PASS