


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN051425\
Data File : VN086615.D
Acq On : 14 May 2025 09:01
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N041525W.M
Title : SW846 8260
Last Update : Wed Apr 16 04:19:23 2025

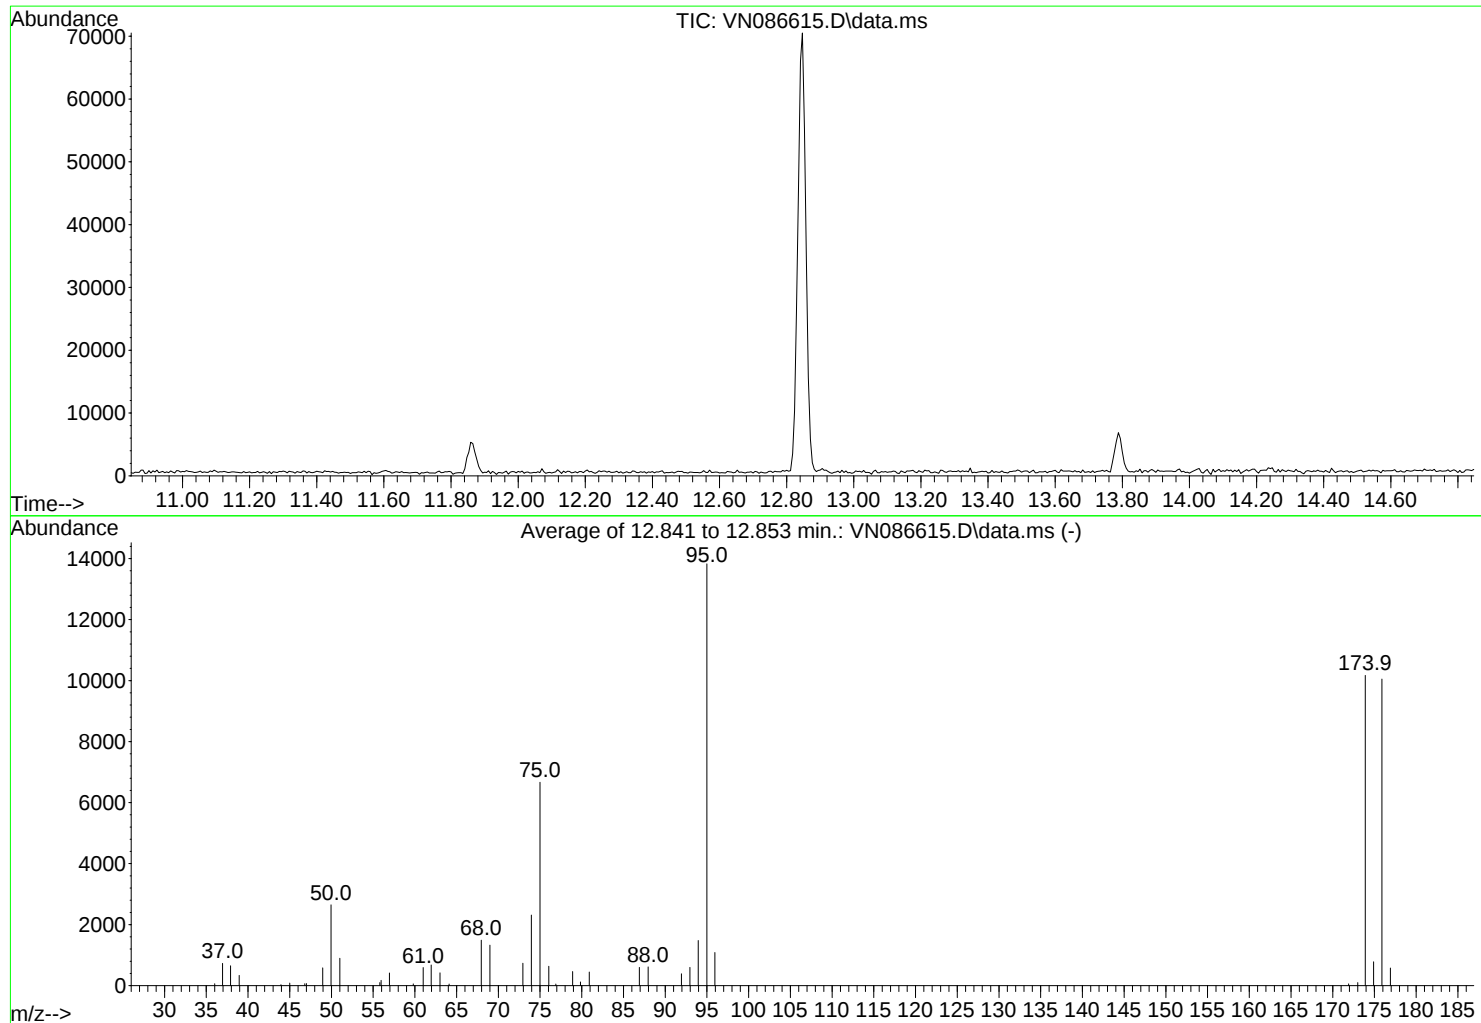

AutoFind: Scans 1851, 1852, 1853; Background Corrected with Scan 1843

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.2	2651	PASS
75	95	30	60	48.2	6666	PASS
95	95	100	100	100.0	13829	PASS
96	95	5	9	7.9	1087	PASS
173	174	0.00	2	1.0	101	PASS
174	95	50	100	73.6	10174	PASS
175	174	5	9	7.7	784	PASS
176	174	95	101	98.8	10050	PASS
177	176	5	9	5.8	578	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.00	61	55.80	99	73.95	2311	93.95	1481
36.95	730	55.95	172	75.00	6666	95.00	1382
37.90	652	56.95	412	76.05	635	95.95	1081
38.95	336	59.80	58	76.90	50	171.90	51
43.95	34	61.00	593	78.90	464	173.00	101
45.00	84	61.95	679	79.85	119	173.90	10174
46.80	65	63.00	419	80.90	446	174.90	784
47.00	68	64.10	51	86.90	600	175.90	10050
48.95	582	67.95	1488	87.95	615	176.90	578
49.95	2651	69.00	1328	91.95	386		
51.00	896	72.95	733	92.95	599		

Instrument :

MSVOA_N

ClientSampleId :

BFB