


Data Path : Z:\VOASRV\HPCHEM1\MSVOA_N\DATA\VN051520\
 Data File : VN061409.D
 Acq On : 15 May 2020 14:01
 Operator : JC/MD
 Sample : BFB
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT3.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\624N051420W.M
 Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
 Last Update : Thu May 14 16:04:10 2020

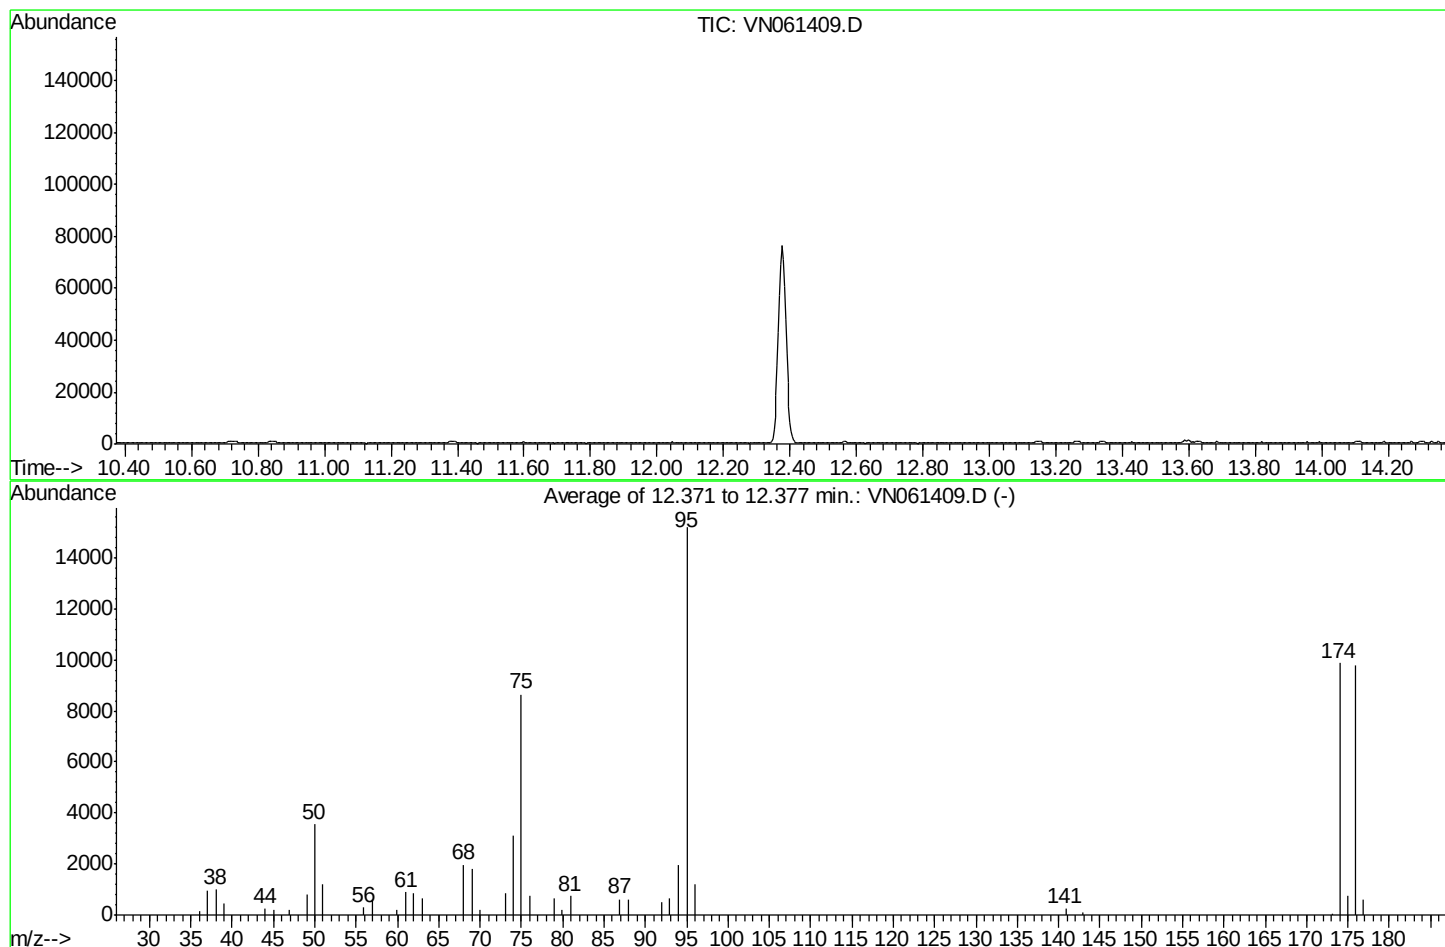

AutoFind: Scans 3296, 3297, 3298; Background Corrected with Scan 3286

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	23.3	3544	PASS
75	95	30	60	56.9	8643	PASS
95	95	100	100	100.0	15194	PASS
96	95	5	9	8.0	1209	PASS
173	174	0.00	2	0.6	60	PASS
174	95	50	100	65.0	9879	PASS
175	174	5	9	7.6	747	PASS
176	174	95	101	98.9	9769	PASS
177	176	5	9	6.2	609	PASS