
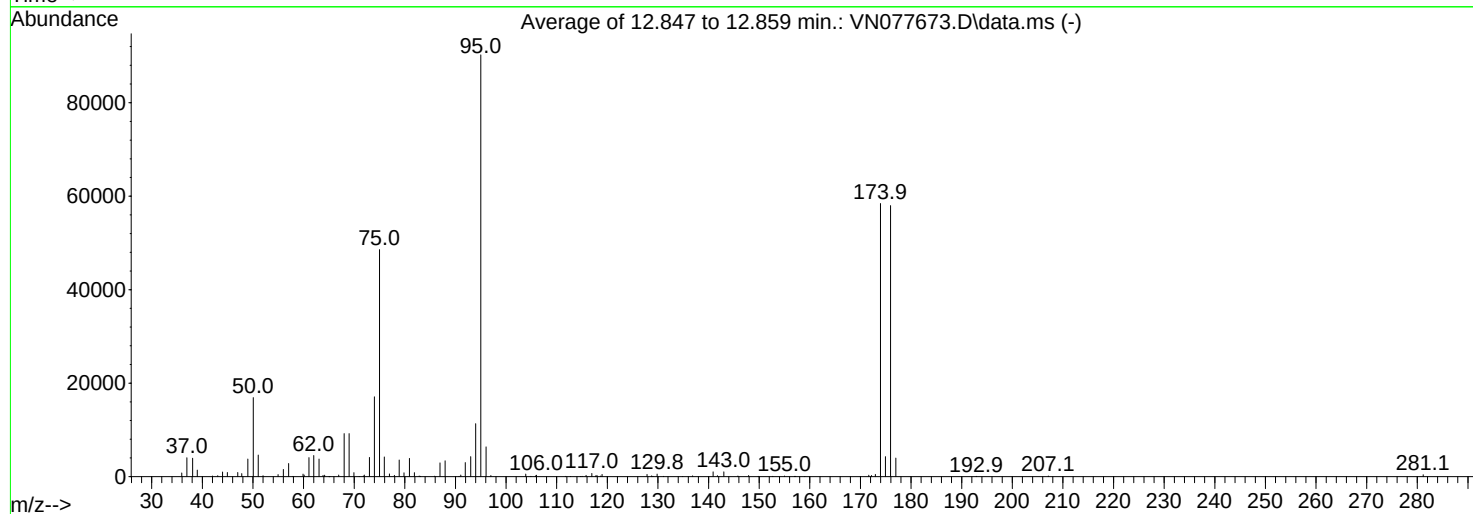


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN051523\
Data File : VN077673.D
Acq On : 15 May 2023 16:36
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N051523W.M
Title : SW846 8260
Last Update : Tue May 16 04:07:42 2023

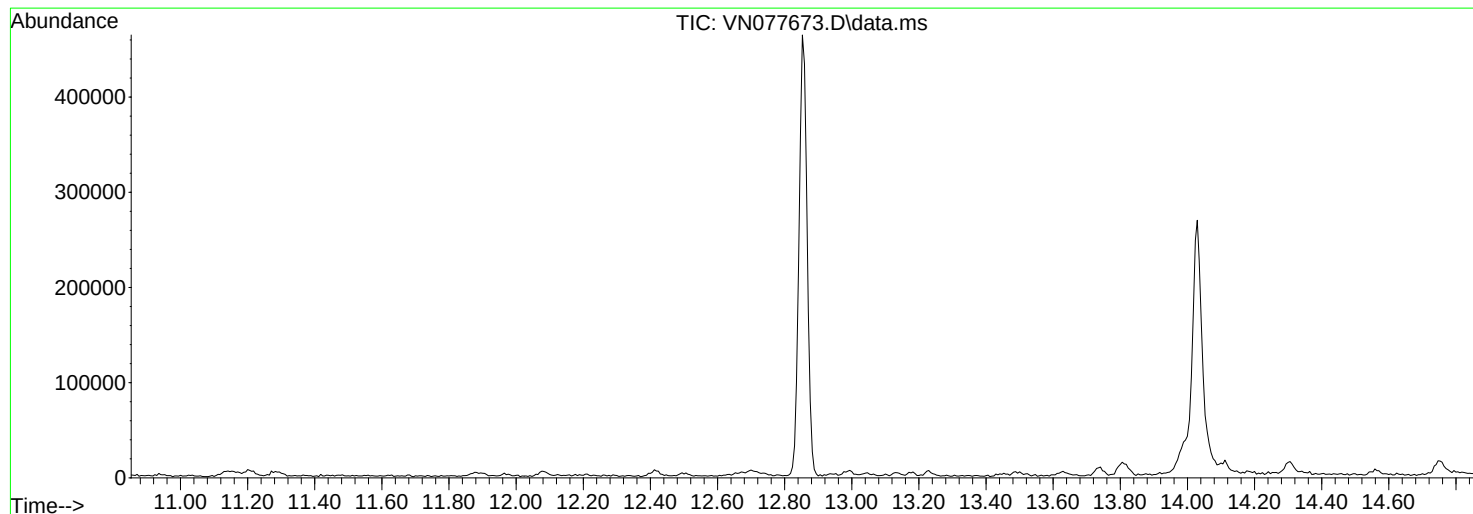

AutoFind: Scans 1852, 1853, 1854; Background Corrected with Scan 1844

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.8	16926	PASS
75	95	30	60	53.8	48579	PASS
95	95	100	100	100.0	90243	PASS
96	95	5	9	7.1	6370	PASS
173	174	0.00	2	0.8	464	PASS
174	95	50	100	64.8	58443	PASS
175	174	5	9	7.3	4280	PASS
176	174	95	101	99.2	57987	PASS
177	176	5	9	6.8	3960	PASS

Average of 12.847 to 12.859 min.: VN077673.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.95	788	50.05	16926	63.05	3779	73.00	4094
36.95	4032	51.05	4610	63.85	295	74.00	1706
38.10	3955	52.00	193	64.15	299	75.00	4857
39.00	1393	54.95	456	65.00	1	75.95	422
42.00	128	56.00	1538	66.95	357	76.95	602
43.05	210	57.05	2801	68.00	9217	77.95	270
44.00	982	57.90	66	69.00	9210	78.90	3559
44.95	902	59.90	548	69.95	874	79.85	810
47.00	908	60.10	344	71.00	53	80.90	3917
47.80	637	61.05	4076	71.80	126	81.90	853
49.00	3754	62.00	4511	72.00	330	82.85	152

Average of 12.847 to 12.859 min.: VN077673.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
83.10	62	97.00	232	117.70	158	140.90	1033
85.90	89	103.90	535	117.95	268	141.75	213
86.95	2954	104.90	63	118.70	140	143.00	1045
87.95	3376	105.80	173	118.95	469	145.80	149
90.70	70	106.00	297	127.85	497	147.90	237
91.05	343	111.80	76	128.75	182	149.80	60
91.95	3018	112.70	51	129.00	86	152.70	76
93.00	4284	114.70	50	129.85	533	155.00	127
94.00	11335	115.00	59	131.10	64	157.00	68
95.00	90243	115.80	275	134.90	52	157.20	77
96.05	6370	116.95	694	136.85	185	159.00	51

Average of 12.847 to 12.859 min.: VN077673.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
171.65	326						
172.20	226						
172.95	464						
173.95	58443						
174.95	4280						
175.95	57987						
177.00	3960						
192.90	60						
207.10	141						
281.15	401						