


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN051524\
Data File : VN082126.D
Acq On : 15 May 2024 11:53
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N051524W.M
Title : SW846 8260
Last Update : Thu May 16 05:21:06 2024

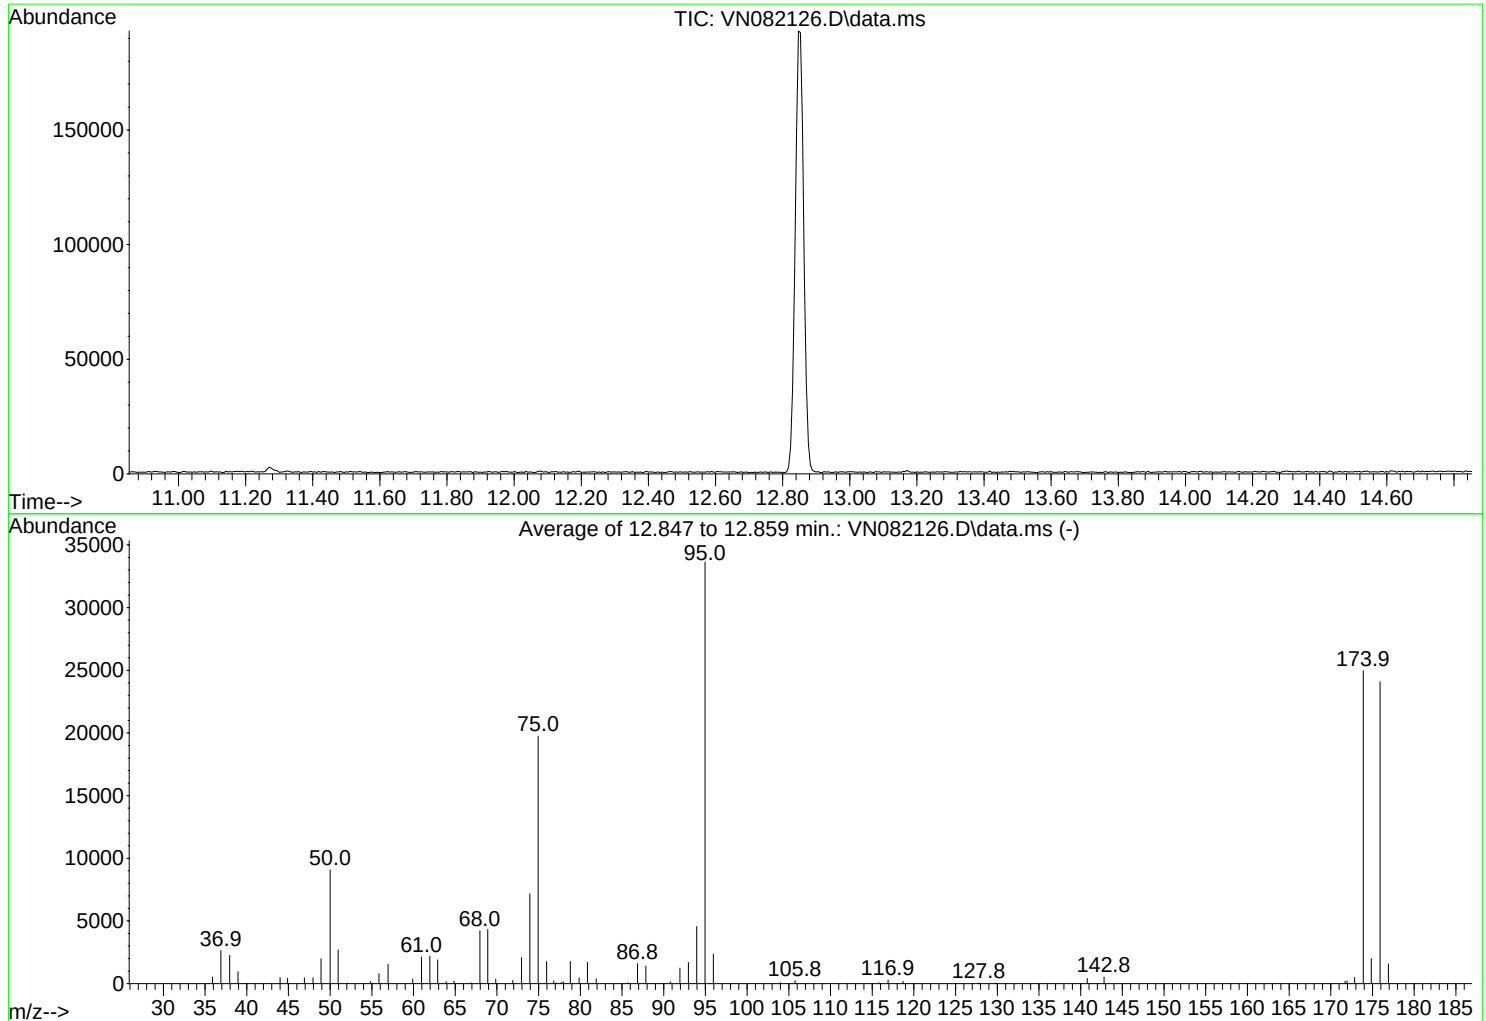

AutoFind: Scans 1852, 1853, 1854; Background Corrected with Scan 1844

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	27.0	9074	PASS
75	95	30	60	58.7	19752	PASS
95	95	100	100	100.0	33653	PASS
96	95	5	9	7.0	2367	PASS
173	174	0.00	2	2.0	491	PASS
174	95	50	100	74.2	24973	PASS
175	174	5	9	8.0	2008	PASS
176	174	95	101	96.5	24088	PASS
177	176	5	9	6.5	1572	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.90	539	50.95	2701	66.90	68	77.70	84
36.90	2647	52.10	54	67.95	4230	77.95	16
37.95	2257	54.85	163	68.90	4317	78.80	175
38.95	940	55.85	797	69.85	353	79.85	46
39.85	26	56.95	1542	71.90	245	80.85	1701
44.00	481	59.90	363	72.95	2065	81.90	391
44.90	421	60.95	2119	73.95	7163	85.70	83
46.90	466	61.95	2195	74.95	19752	86.85	1610
47.95	475	62.90	1894	75.95	1766	87.85	1402
48.90	1997	63.90	160	76.80	230	90.80	150
50.00	9074	64.85	222	77.10	64	91.95	1235

Average of 12.847 to 12.859 min.: VN082126.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
92.95	1687	140.80	406				
93.95	4564	142.80	533				
94.95	33653	171.70	191				
95.95	2367	171.95	221				
104.00	83	172.85	491				
105.75	248	173.90	24973				
115.80	74	174.85	2008				
116.90	296	175.90	24088				
118.70	188	176.90	1572				
127.80	60						
129.80	55						

Instrument :

MSVOA_N

ClientSampleId :

BFB