
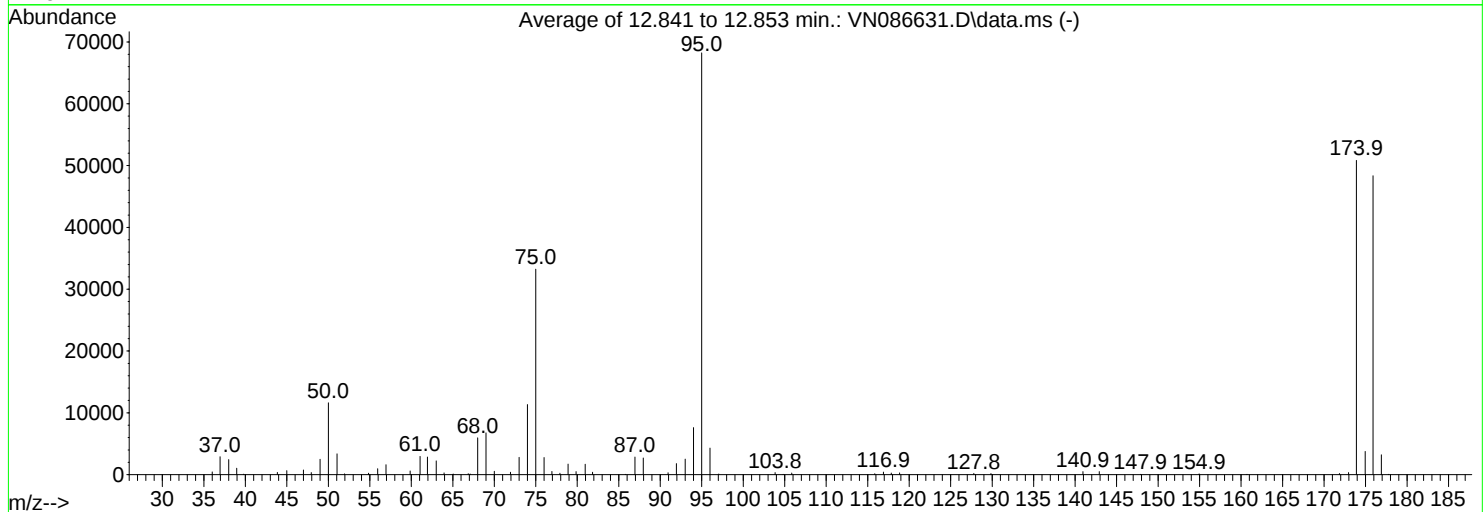


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN051525\
Data File : VN086631.D
Acq On : 15 May 2025 08:57
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N041525W.M
Title : SW846 8260
Last Update : Wed Apr 16 04:19:23 2025

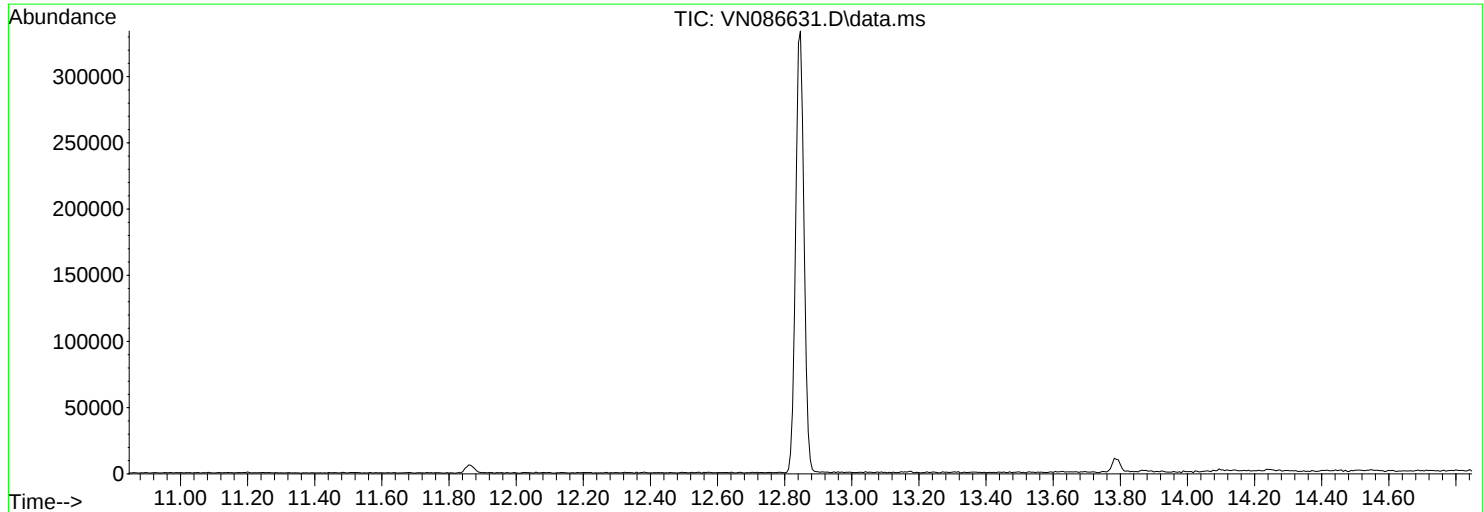

AutoFind: Scans 1851, 1852, 1853; Background Corrected with Scan 1841

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.0	11615	PASS
75	95	30	60	48.7	33232	PASS
95	95	100	100	100.0	68240	PASS
96	95	5	9	6.3	4290	PASS
173	174	0.00	2	0.7	333	PASS
174	95	50	100	74.5	50853	PASS
175	174	5	9	7.4	3748	PASS
176	174	95	101	95.1	48371	PASS
177	176	5	9	6.7	3217	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.00	455	51.05	3375	66.85	157	77.90	22
36.95	2908	51.95	125	67.10	101	78.90	172
38.00	2445	54.85	231	68.00	5954	79.85	49
38.95	1047	55.95	959	69.00	6767	80.95	169
39.80	85	56.95	1618	70.00	554	81.85	388
43.85	361	59.85	584	71.95	402	85.80	63
45.00	651	61.05	2957	73.00	2800	86.95	2839
47.00	755	61.95	2850	74.00	11333	87.95	2696
47.95	345	63.00	2238	75.00	33232	90.95	320
49.00	2496	63.95	280	76.00	2761	91.95	1780
50.00	11615	65.05	119	76.95	520	93.00	2507

Average of 12.841 to 12.853 min.: VN086631.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
94.00	7623	127.80	205	175.90	48371		
95.00	68240	129.85	192	176.90	3217		
96.00	4290	140.95	495	177.80	59		
97.05	118	142.90	489				
103.85	328	147.90	64				
104.80	51	154.95	122				
105.85	255	160.70	51				
115.85	146	171.85	184				
116.90	406	172.95	333				
117.85	254	173.90	50853				
118.85	296	174.95	3748				

Instrument :

MSVOA_N

ClientSampleId :

BFB