


Data Path : Z:\voasrv\HPCHEM1\MSVOA N\Data\VN051620\
 Data File : VN061417.D
 Acq On : 15 May 2020 19:38
 Operator : JC/MD
 Sample : BFB
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N051620W.M
 Title : SW846 8260
 Last Update : Sat May 16 03:04:07 2020

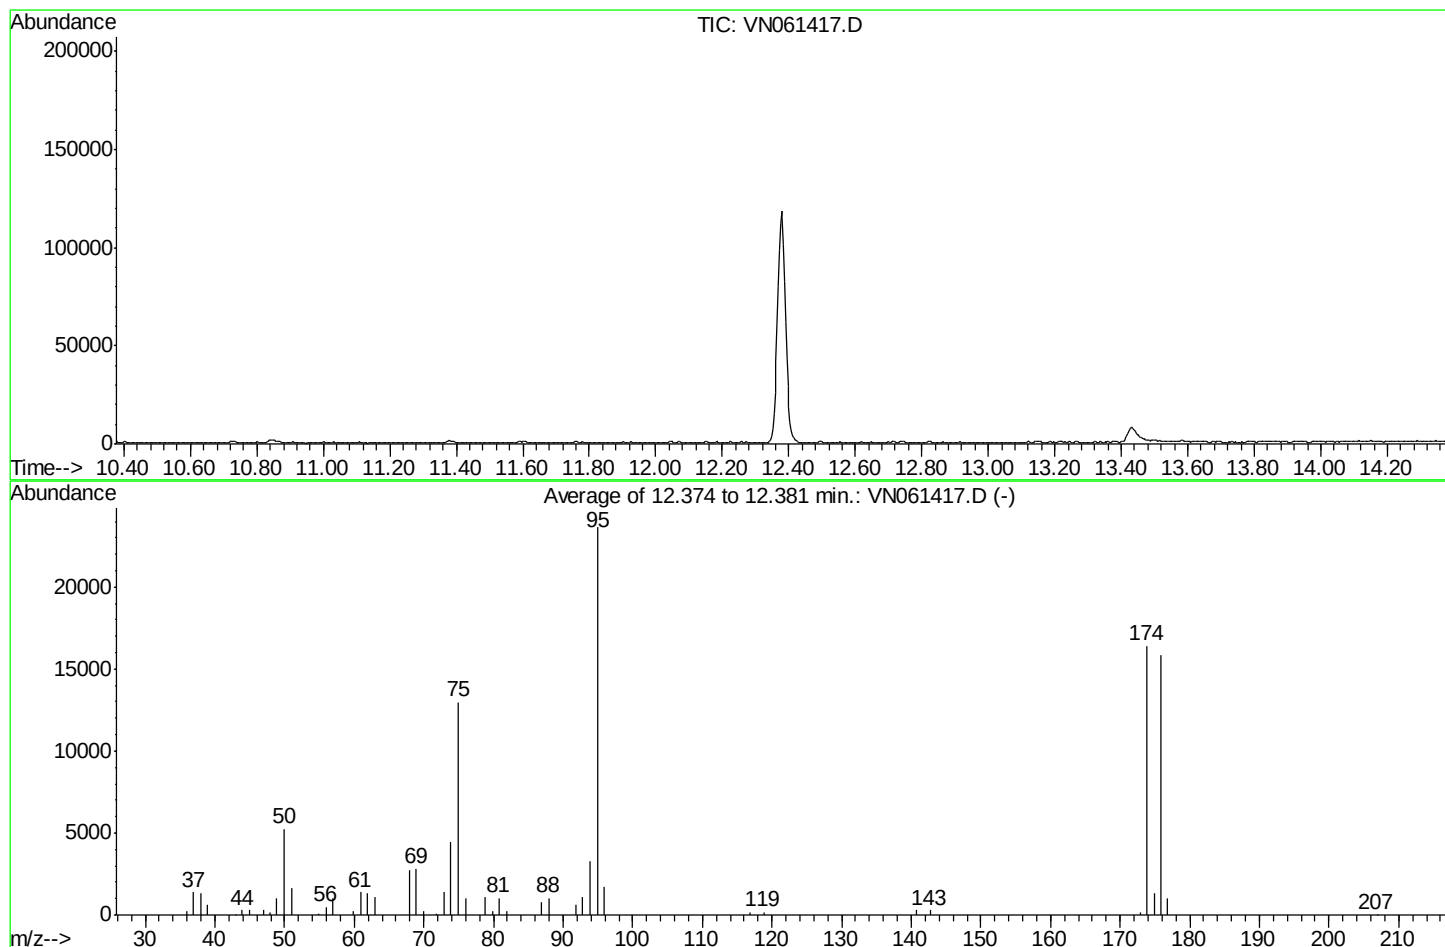

AutoFind: Scans 3297, 3298, 3299; Background Corrected with Scan 3284

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.3	5270	PASS
75	95	30	60	54.9	12976	PASS
95	95	100	100	100.0	23640	PASS
96	95	5	9	7.1	1682	PASS
173	174	0.00	2	0.8	133	PASS
174	95	50	100	69.5	16428	PASS
175	174	5	9	8.2	1354	PASS
176	174	95	101	96.5	15847	PASS
177	176	5	9	6.5	1025	PASS