


Data Path : Z:\voasrv\HPCHEM1\MSVOA\_N\Data\VN051622\  
 Data File : VN072502.D  
 Acq On : 16 May 2022 15:17  
 Operator : JC\MD  
 Sample : BFB  
 Misc : 5.0mL/MSVOA\_N/WATER  
 ALS Vial : 9 Sample Multiplier: 1

Instrument :  
 MSVOA\_N  
 ClientSampleId :  
 BFB

Integration File: RTEINT3.P

Method : Z:\voasrv\HPCHEM1\MSVOA\_N\methods\624N051622W.M  
 Title : METHOD 624 VOLATILE ORGANIC ANALYSIS  
 Last Update : Tue May 17 06:34:50 2022

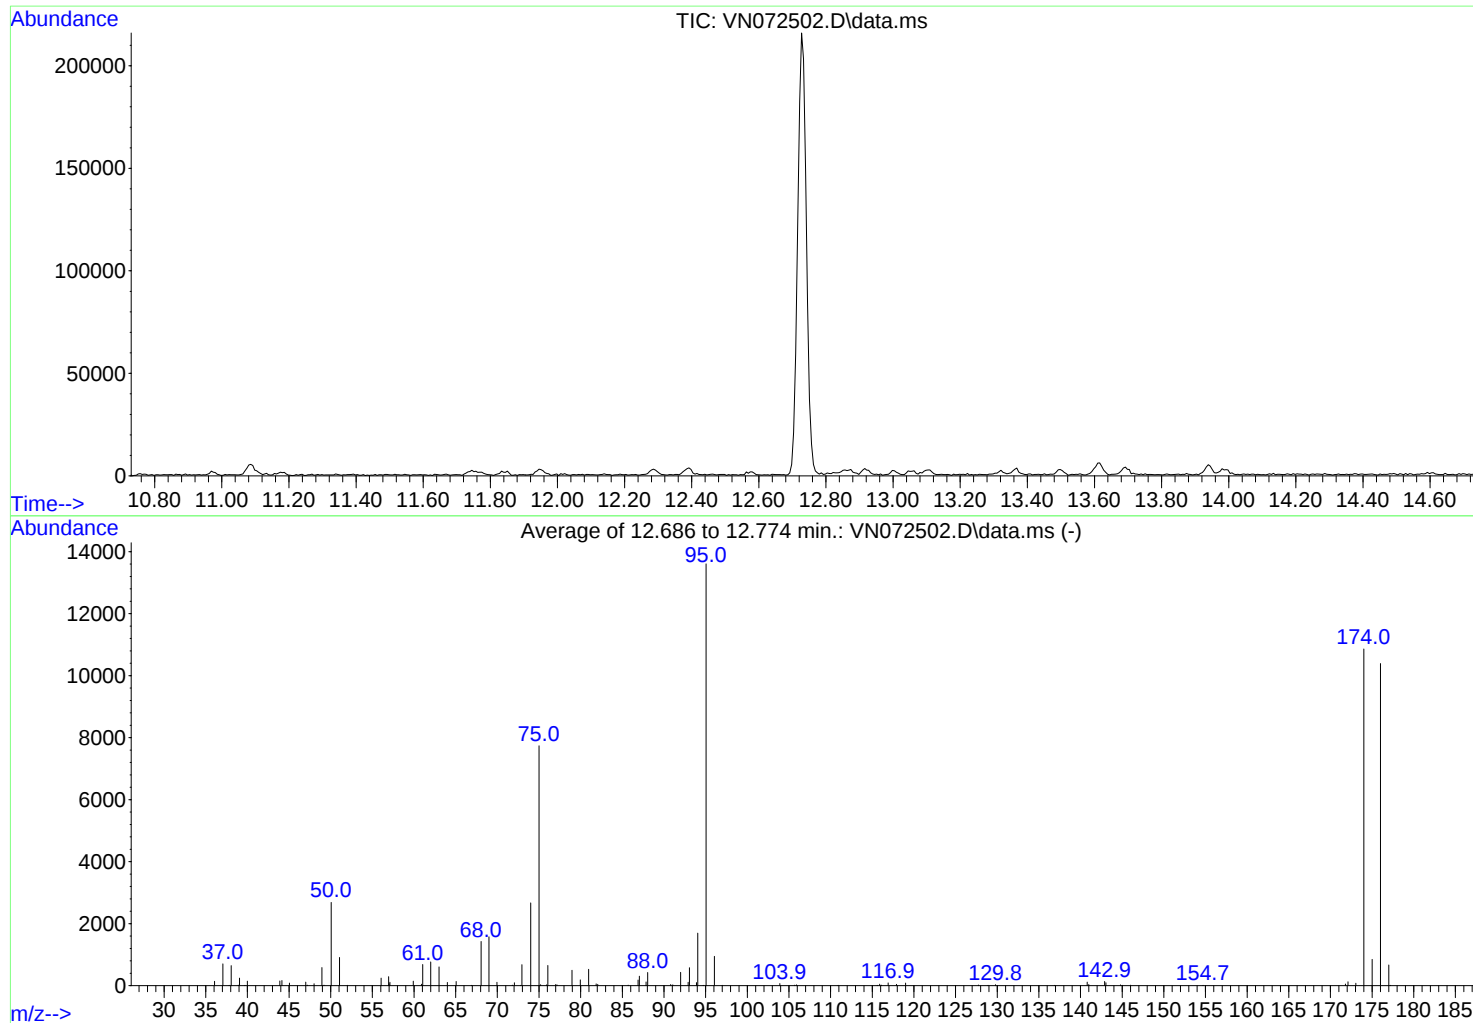

AutoFind: Averaged scan 1819 to 1834; Bkg corrected with scan 1818

| Target<br>Mass | Rel. to<br>Mass | Lower<br>Limit% | Upper<br>Limit% | Rel.<br>Abn% | Raw<br>Abn | Result<br>Pass/Fail |
|----------------|-----------------|-----------------|-----------------|--------------|------------|---------------------|
| 50             | 95              | 15              | 40              | 19.7         | 2684       | PASS                |
| 75             | 95              | 30              | 60              | 56.9         | 7738       | PASS                |
| 95             | 95              | 100             | 100             | 100.0        | 13607      | PASS                |
| 96             | 95              | 5               | 9               | 6.9          | 944        | PASS                |
| 173            | 174             | 0.00            | 2               | 0.7          | 78         | PASS                |
| 174            | 95              | 50              | 100             | 79.8         | 10858      | PASS                |
| 175            | 174             | 5               | 9               | 7.8          | 846        | PASS                |
| 176            | 174             | 95              | 101             | 95.7         | 10391      | PASS                |
| 177            | 176             | 5               | 9               | 6.4          | 665        | PASS                |