
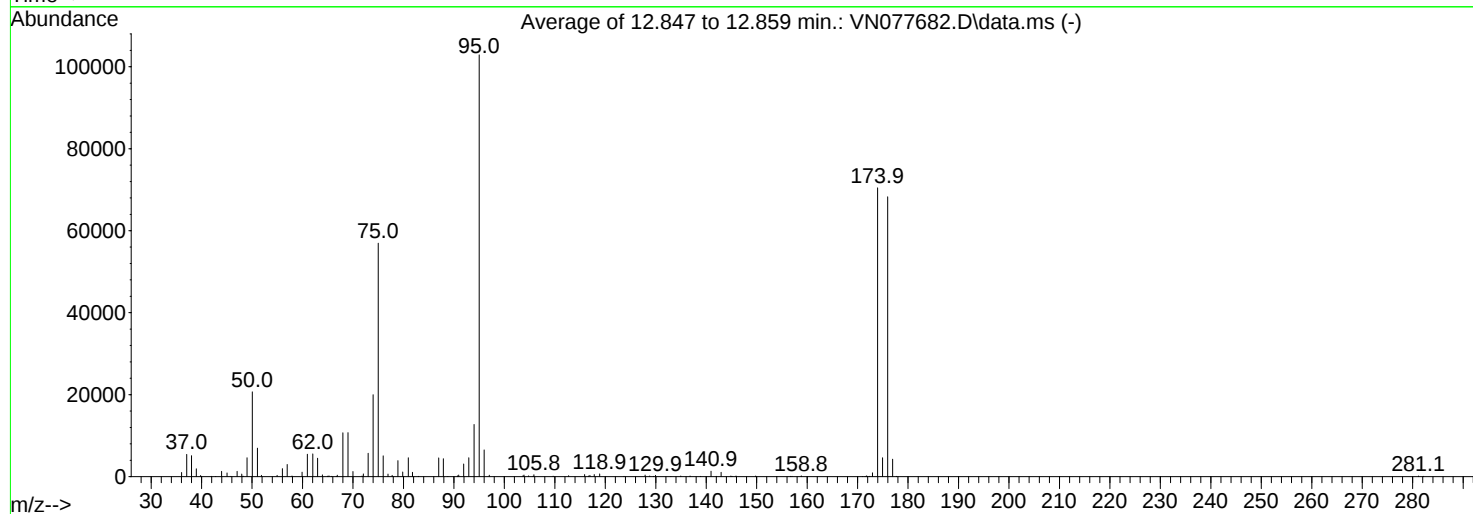


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN051623\
Data File : VN077682.D
Acq On : 16 May 2023 10:36
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N051523W.M
Title : SW846 8260
Last Update : Tue May 16 04:07:42 2023

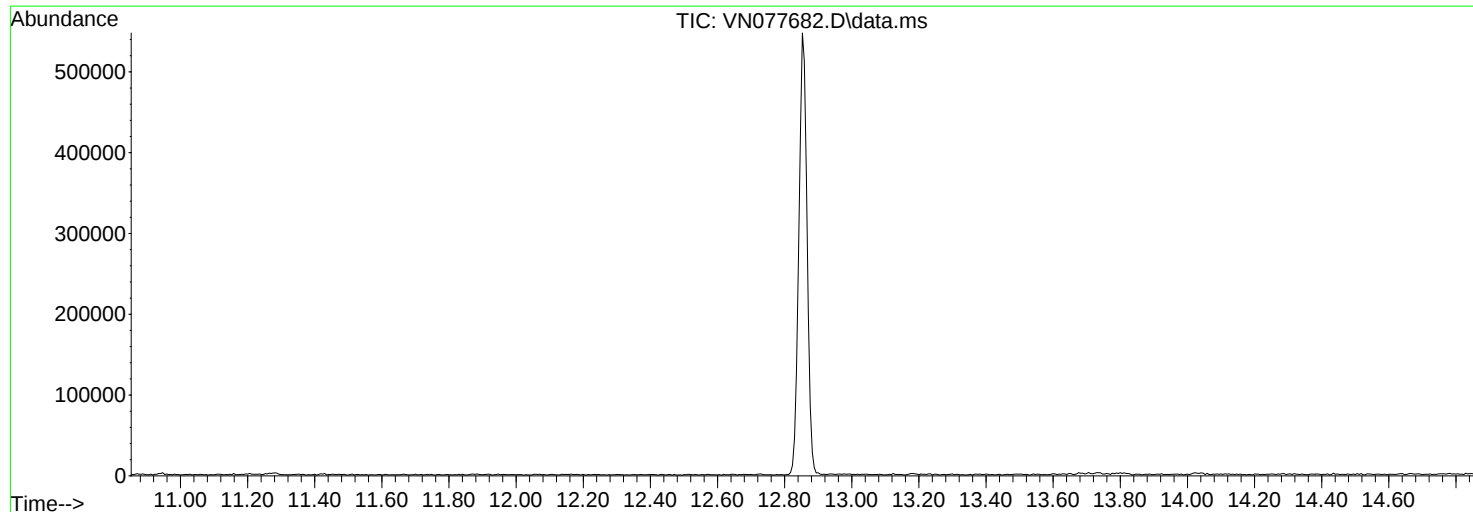

AutoFind: Scans 1852, 1853, 1854; Background Corrected with Scan 1844

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.1	20701	PASS
75	95	30	60	55.4	56963	PASS
95	95	100	100	100.0	102907	PASS
96	95	5	9	6.3	6530	PASS
173	174	0.00	2	1.3	950	PASS
174	95	50	100	68.5	70451	PASS
175	174	5	9	6.5	4614	PASS
176	174	95	101	96.9	68264	PASS
177	176	5	9	6.2	4249	PASS

Average of 12.847 to 12.859 min.: VN077682.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.05	1031	47.95	610	60.95	5453	70.00	125
37.05	5431	48.20	125	62.05	5533	71.80	16
38.00	5135	49.00	4594	63.00	4508	72.05	66
38.95	1912	50.05	20701	63.95	451	73.00	570
39.80	260	51.05	6968	65.00	110	74.00	19987
41.90	77	51.85	303	65.25	209	75.00	56963
42.80	55	54.95	312	65.70	70	76.00	5060
43.95	1281	56.00	1954	66.70	56	76.95	628
45.05	889	56.95	2986	66.90	358	77.75	331
45.80	70	57.90	142	68.00	10686	78.90	3913
47.05	1290	59.90	1076	69.00	10729	79.85	1122

Average of 12.847 to 12.859 min.: VN077682.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
80.95	4601	95.00	102907	116.70	151	136.80	141
81.80	1059	96.00	6530	116.95	304	138.90	79
83.00	74	97.00	358	117.80	509	140.95	1316
87.00	4569	103.70	222	118.90	660	142.00	88
87.90	4356	103.90	410	123.70	90	142.95	1049
88.80	56	104.80	184	127.90	402	144.90	176
90.70	185	105.70	125	128.80	178	145.10	79
90.95	407	105.85	491	129.60	87	145.90	176
91.95	3104	109.65	120	129.95	301	149.80	154
92.95	4626	112.75	245	133.00	52	154.00	52
94.00	12709	115.90	521	134.95	156	156.70	80

Average of 12.847 to 12.859 min.: VN077682.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
157.00	89	176.95	4249				
158.85	209	177.70	71				
171.00	58	281.15	150				
171.50	55	282.10	61				
171.75	189						
172.00	66						
172.30	78						
172.95	950						
173.95	70451						
174.95	4614						
175.95	68264						

Instrument :

MSVOA_N

ClientSampleId :

BFB