
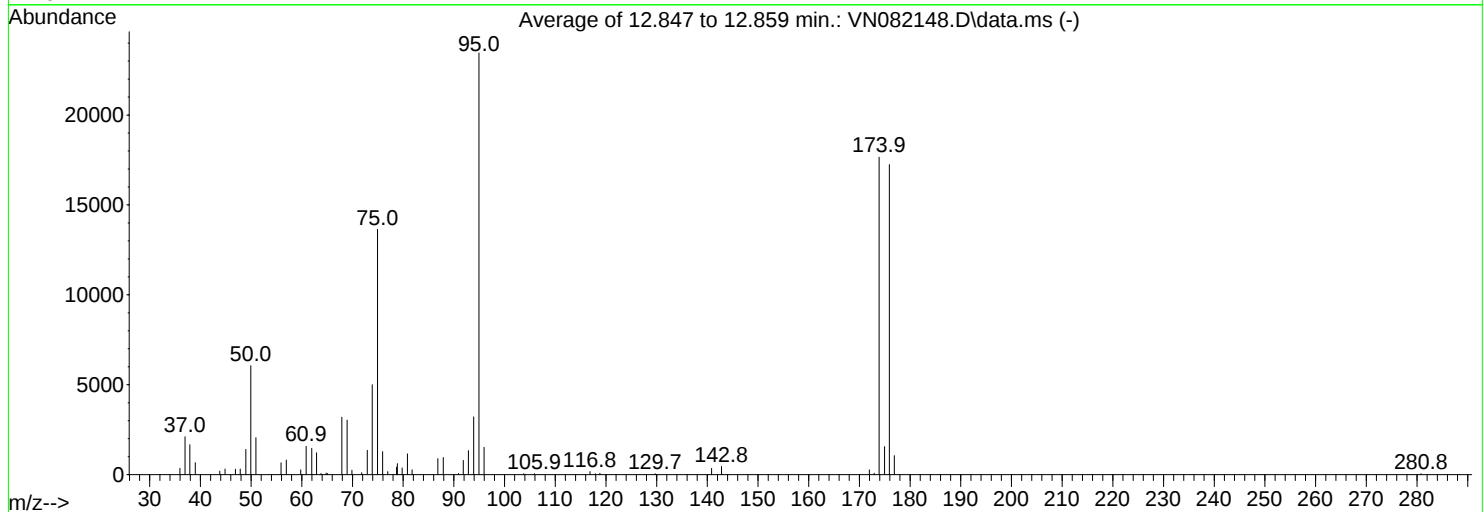


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN051624\
Data File : VN082148.D
Acq On : 16 May 2024 09:16
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N051524W.M
Title : SW846 8260
Last Update : Thu May 16 05:21:06 2024

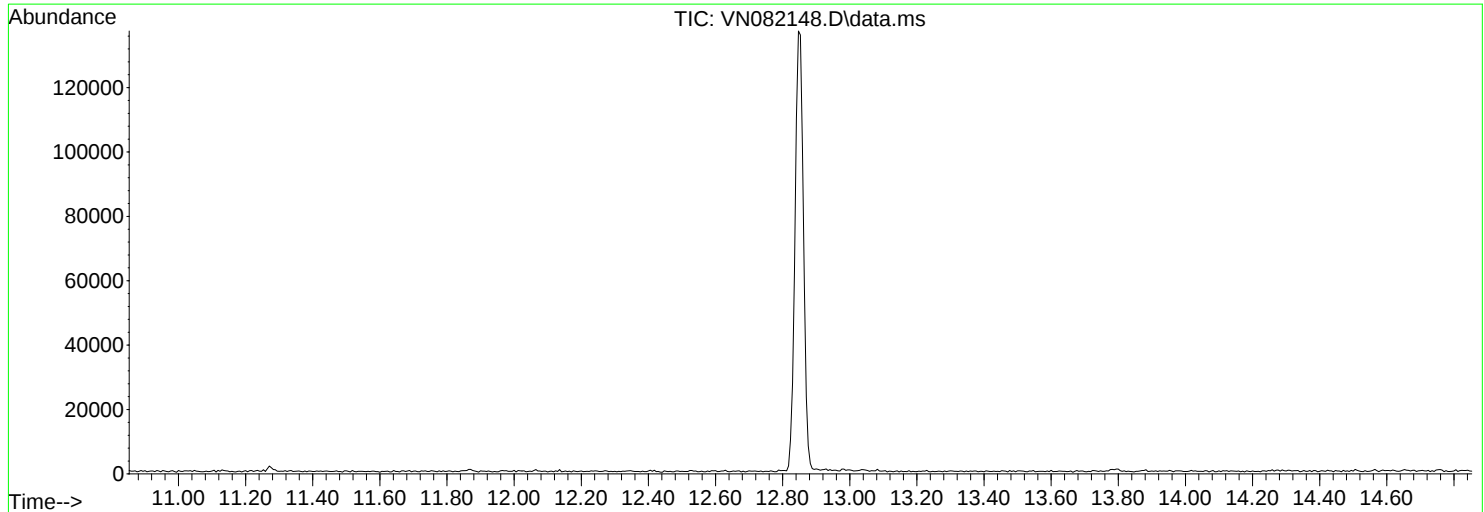

AutoFind: Scans 1852, 1853, 1854; Background Corrected with Scan 1844

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	25.8	6058	PASS
75	95	30	60	58.1	13639	PASS
95	95	100	100	100.0	23459	PASS
96	95	5	9	6.5	1526	PASS
173	174	0.00	2	0.4	77	PASS
174	95	50	100	75.2	17652	PASS
175	174	5	9	8.8	1562	PASS
176	174	95	101	97.7	17243	PASS
177	176	5	9	6.1	1057	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.95	355	55.90	661	69.90	246	81.75	261
36.95	2106	56.95	812	71.80	103	86.85	88
37.90	1664	59.80	268	72.90	1352	87.90	95
39.00	672	60.85	1578	73.90	5003	90.90	6
43.80	197	61.95	1457	74.95	13639	91.85	792
44.85	312	62.90	1218	75.95	1278	92.85	1331
46.90	304	63.80	64	76.95	170	93.90	3209
47.85	310	64.80	88	78.70	421	94.95	23459
48.95	1409	65.10	59	78.85	618	95.95	1526
49.95	6058	67.90	3192	79.80	371	103.80	51
50.95	2054	68.95	3032	80.85	1156	105.90	51

Average of 12.847 to 12.859 min.: VN082148.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
116.85	170	176.90	1057				
117.90	54	280.80	55				
118.80	82						
129.70	51						
140.85	345						
142.80	451						
171.95	271						
172.90	77						
173.90	17652						
174.95	1562						
175.90	17243						

Instrument :

MSVOA_N

ClientSampleId :

BFB