

Data File : VN055647.D
Acq On : 18 May 2019 6:54
Operator : JC/SP
Sample : K2896-09
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 55 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
TP-20

Quant Time: May 20 02:17:52 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N051719W.M
Quant Title : SW846 8260
QLast Update : Fri May 17 23:54:12 2019
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.67	168	399098	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.59	114	563556	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.41	117	472492	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.34	152	195499	50.00	ug/l	0.00

System Monitoring Compounds

33) 1,2-Dichloroethane-d4	8.03	65	182636	41.75	ug/l	0.00
Spiked Amount	50.000		Recovery	=	83.50%	
35) Dibromofluoromethane	7.59	113	172256	48.12	ug/l	0.00
Spiked Amount	50.000		Recovery	=	96.24%	
50) Toluene-d8	10.09	98	649016	47.95	ug/l	0.00
Spiked Amount	50.000		Recovery	=	95.90%	
62) 4-Bromofluorobenzene	12.40	95	211881	45.33	ug/l	0.00
Spiked Amount	50.000		Recovery	=	90.66%	

Target Compounds


						Qvalue
11) Tert butyl alcohol	4.76	59	165	0.202	ug/l #	74
16) Acetone	3.83	43	2971	1.664	ug/l #	87
17) Carbon Disulfide	4.06	76	2028	0.200	ug/l #	75
29) Tetrahydrofuran	7.23	42	723	0.437	ug/l #	35
31) Cyclohexane	7.66	56	6384	0.984	ug/l #	1
36) 1,1-Dichloropropene	7.66	75	23275	4.632	ug/l #	49
38) Carbon Tetrachloride	7.67	117	33372	6.216	ug/l #	15
39) Methylcyclohexane	9.08	83	1341	0.221	ug/l	88
52) Toluene	10.16	92	5964	0.643	ug/l	97
55) 1,1,2-Trichloroethane	10.53	97	885	0.232	ug/l #	15
68) m/p-Xylenes	11.62	106	2218	0.345	ug/l	100
69) o-Xylene	11.95	106	1613	0.257	ug/l	80
71) Bromoform	12.40	173	1298	0.398	ug/l #	1
73) Isopropylbenzene	12.25	105	3436	Below Cal		93
75) 1,1,2,2-Tetrachloroethane	12.56	83	60	Below Cal	#	26
76) 1,2,3-Trichloropropane	12.40	75	96658	24.230	ug/l #	100
79) 2-Chlorotoluene	12.66	91	225	Below Cal	#	39
80) 1,3,5-Trimethylbenzene	12.73	105	1253	Below Cal		96
81) trans-1,4-Dichloro-2-buten	12.40	75	96658	62.285	ug/l #	17
83) tert-Butylbenzene	12.99	119	2367	Below Cal		93
84) 1,2,4-Trimethylbenzene	13.04	105	3840	Below Cal		100
85) sec-Butylbenzene	13.17	105	3987	Below Cal	#	75
86) p-Isopropyltoluene	13.44	119	4490	Below Cal		95
90) Hexachloroethane	13.89	117	1376	Below Cal	#	3
92) 1,2-Dibromo-3-Chloropropan	13.99	75	297	0.335	ug/l #	1
95) Naphthalene	15.13	128	2916	2.041	ug/l #	93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : VN055647.D
Acq On : 18 May 2019 6:54
Operator : JC/SP
Sample : K2896-09
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 55 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
TP-20

Quant Time: May 20 02:17:52 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N051719W.M
Quant Title : SW846 8260
QLast Update : Fri May 17 23:54:12 2019
Response via : Initial Calibration

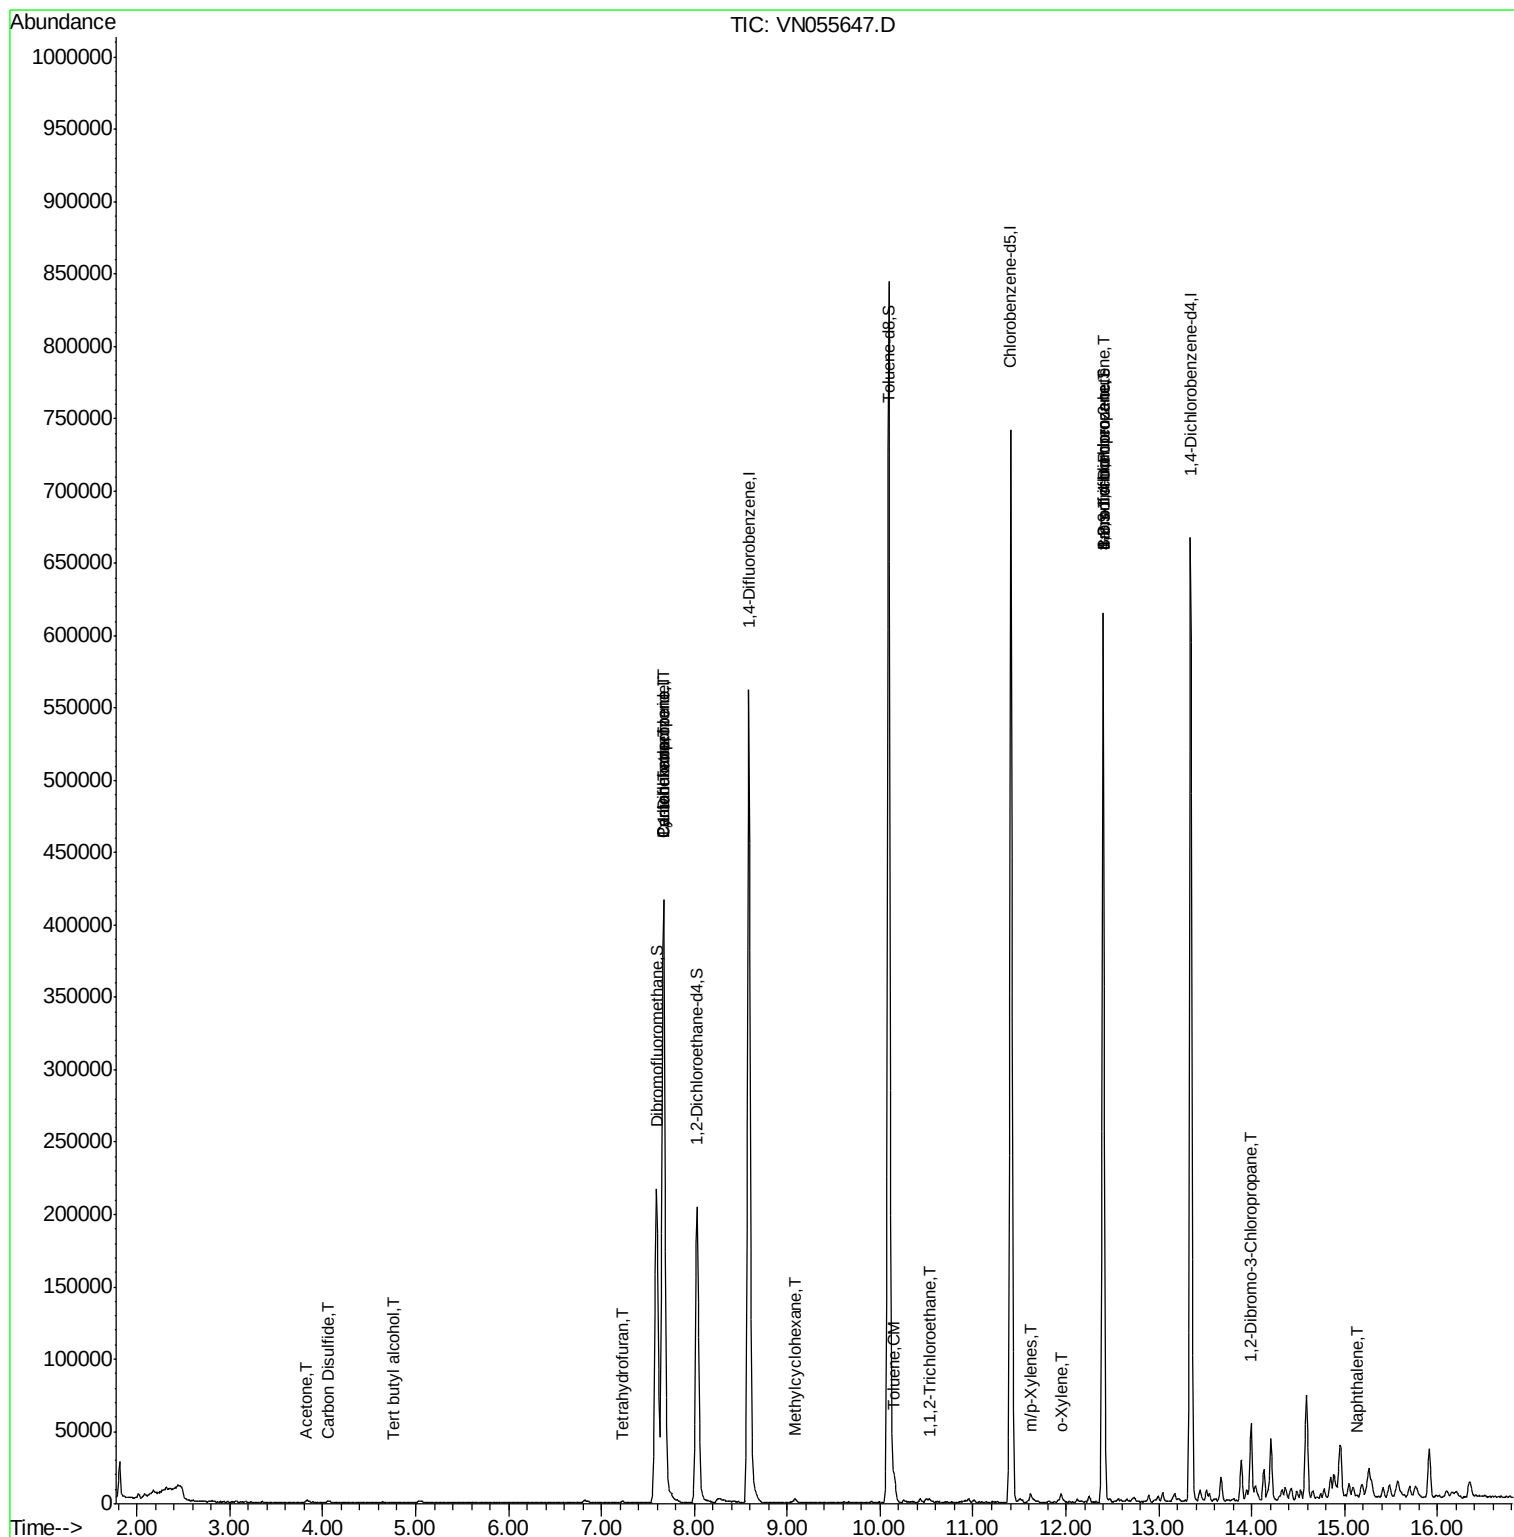

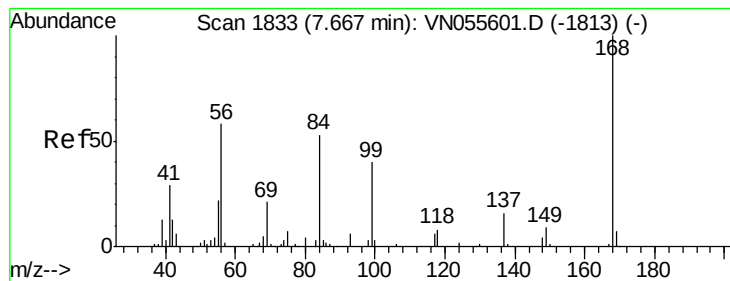

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.67 min Scan# 1833

Delta R.T. -0.00 min

Lab File: VN055647.D

Acq: 18 May 2019 6:54

Instrument :

MSVOA_N

ClientSampled :


TP-20

Tgt Ion: 168 Resp: 399098

Ion Ratio Lower Upper

168 100

99 48.5 40.2 60.2



Abundance Ion 167.90 (167.60 to 168.60): VN055647.D (-1740) (-)

Ion 98.90 (98.60 to 99.60): VN055647.D (-1740) (-)

7.67



150000

100000

50000

0

Time--> 7.50 7.60 7.70 7.80 7.90

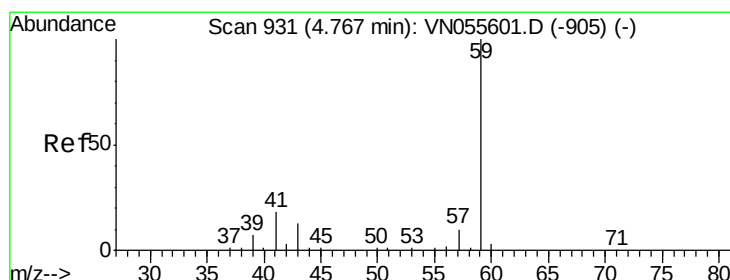

#11

Tert butyl alcohol

Concen: 0.202 ug/l

RT: 4.76 min Scan# 930

Delta R.T. -0.00 min

Lab File: VN055647.D


Acq: 18 May 2019 6:54

Tgt Ion: 59 Resp: 165

Ion Ratio Lower Upper

59 100

57 0.0 7.8 11.6#



Abundance Ion 59.00 (58.70 to 59.70): VN055647.D (-838) (-)

Ion 57.00 (56.70 to 57.70): VN055647.D (-838) (-)

4.76

250

200


150


100

50

0

Time--> 4.75 4.76 4.77



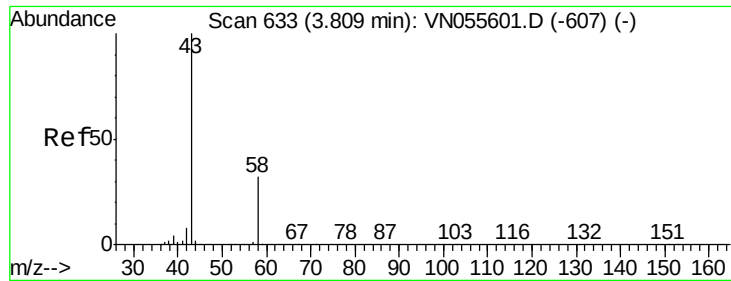

#16

Acetone

Concen: 1.664 ug/l

RT: 3.83 min Scan# 639

Delta R.T. 0.02 min

Lab File: VN055647.D

Acq: 18 May 2019 6:54

Instrument :

MSVOA_N

ClientSampled :


TP-20

Tgt Ion: 43 Resp: 2971

Ion Ratio Lower Upper




43 100

58 25.4 26.0 39.0#

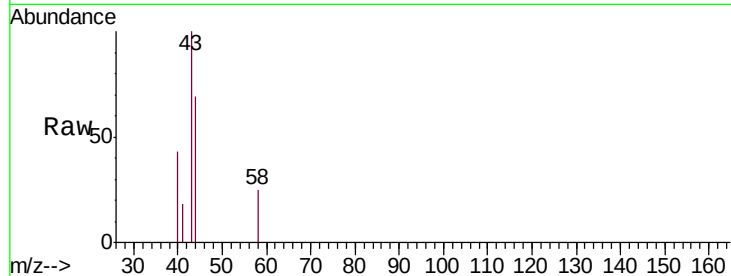

Abundance Ion 43.00 (42.70 to 43.70): VN0

Ion 58.00 (57.70 to 58.70): VN0

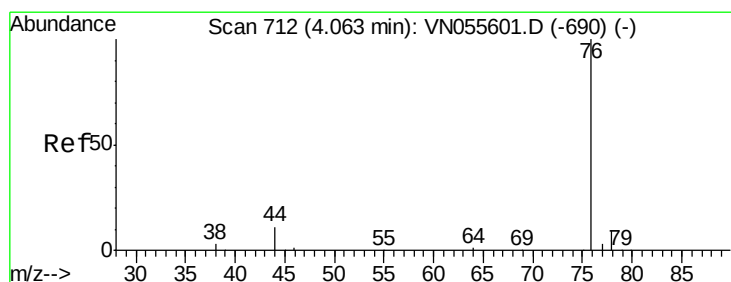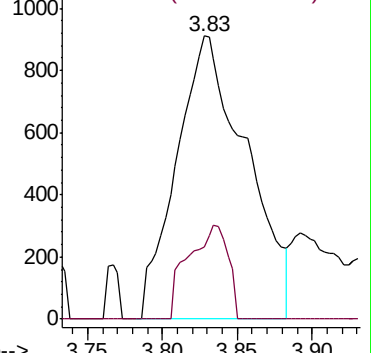

#17

Carbon Disulfide

Concen: 0.200 ug/l

RT: 4.06 min Scan# 712

Delta R.T. -0.00 min

Lab File: VN055647.D


Acq: 18 May 2019 6:54

Tgt Ion: 76 Resp: 2028

Ion Ratio Lower Upper



76 100


78 0.0 7.3 10.9#



Abundance Ion 75.90 (75.60 to 76.60): VN0

Ion 77.90 (77.60 to 78.60): VN0

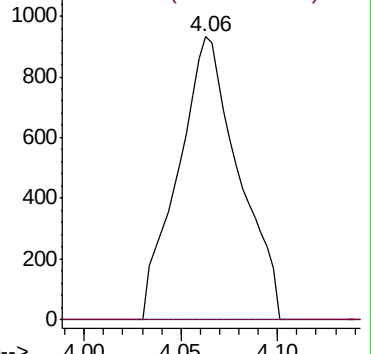

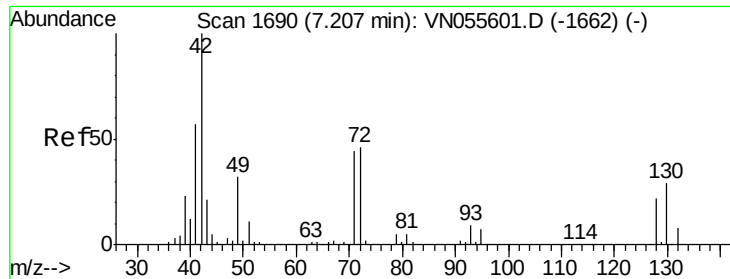

#29

Tetrahydrofuran

Concen: 0.437 ug/l

RT: 7.23 min Scan# 1696

Delta R.T. 0.02 min

Lab File: VN055647.D

Acq: 18 May 2019 6:54

Instrument :

MSVOA_N

ClientSampleId :

TP-20


Tgt Ion: 42 Resp: 723

Ion Ratio Lower Upper

42 100

72 0.0 36.5 54.7#




71 4.6 34.9 52.3#



Abundance Ion 42.00 (41.70 to 42.70): VN0

Ion 72.00 (71.70 to 72.70): VN0

Ion 71.00 (70.70 to 71.70): VN0

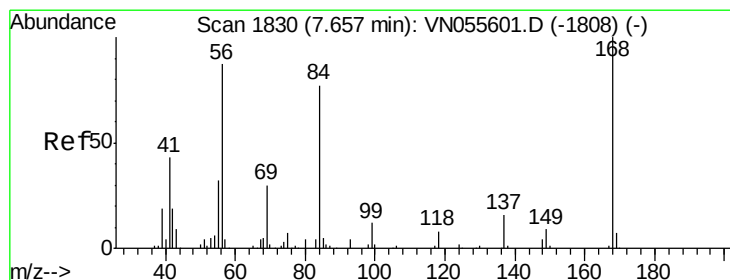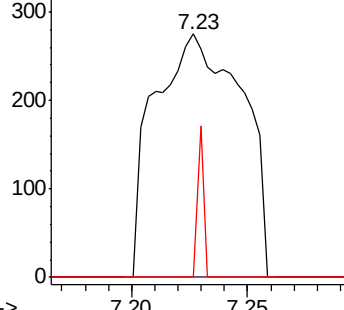

#31

Cyclohexane

Concen: 0.984 ug/l

RT: 7.66 min Scan# 1832

Delta R.T. 0.01 min

Lab File: VN055647.D

Acq: 18 May 2019 6:54


Tgt Ion: 56 Resp: 6384

Ion Ratio Lower Upper

56 100

69 192.7 27.2 40.8#



84 149.6 71.3 106.9#




Abundance Ion 56.00 (55.70 to 56.70): VN0

Ion 69.00 (68.70 to 69.70): VN0

Ion 84.00 (83.70 to 84.70): VN0



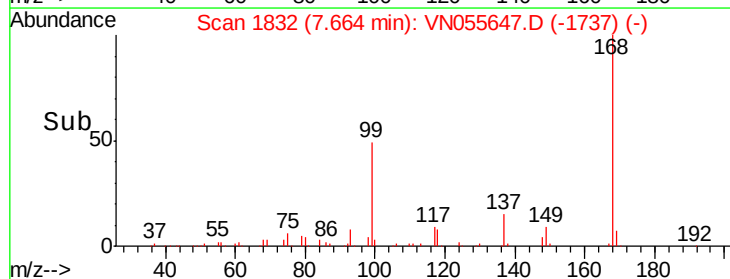
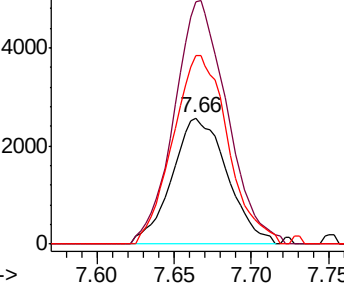


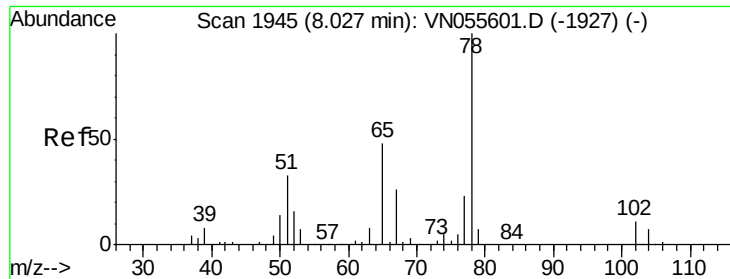

#33
 1,2-Dichloroethane-d4
 Concen: 41.746 ug/l
 RT: 8.03 min Scan# 1946
 Delta R.T. 0.00 min
 Lab File: VN055647.D
 Acq: 18 May 2019 6:54




Instrument :
 MSVOA_N
 ClientSampled :
 TP-20


Tgt Ion: 65 Resp: 182636
 Ion Ratio Lower Upper
 65 100
 67 54.5 0.0 108.6

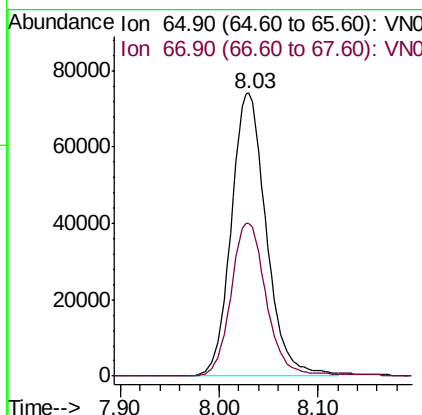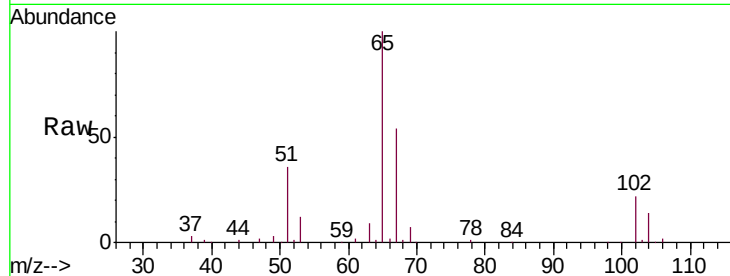

#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 8.59 min Scan# 2119
 Delta R.T. -0.00 min
 Lab File: VN055647.D
 Acq: 18 May 2019 6:54

Tgt Ion: 114 Resp: 563556
 Ion Ratio Lower Upper
 114 100
 63 18.3 0.0 38.2
 88 15.2 0.0 31.0


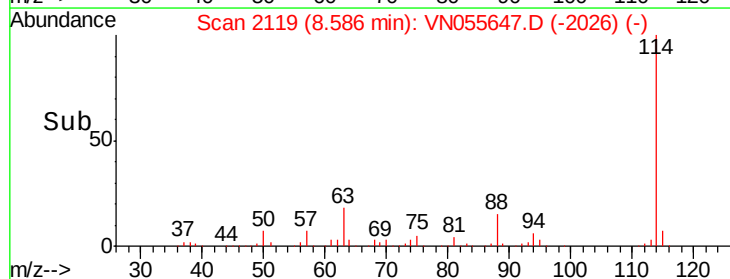
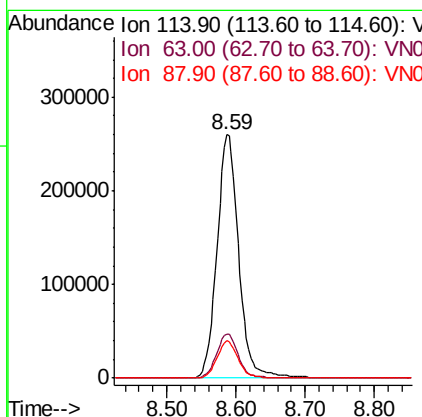





#35
 Dibromofluoromethane
 Concen: 48.117 ug/l
 RT: 7.59 min Scan# 1810
 Delta R.T. -0.00 min
 Lab File: VN055647.D
 Acq: 18 May 2019 6:54




Instrument :
 MSVOA_N
 ClientSampleId :
 TP-20


Tgt Ion	Ratio	Lower	Upper
113	100		
111	102.3	82.5	123.7
192	24.1	18.7	28.1

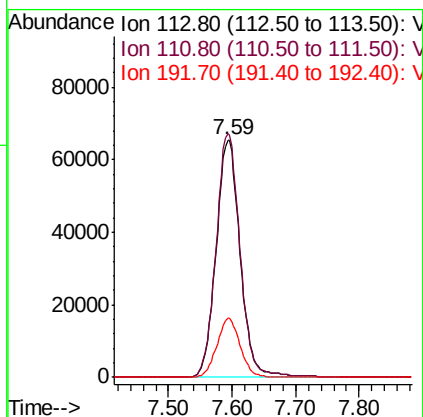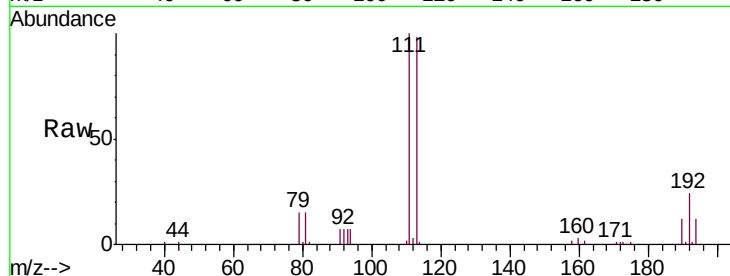

#36
 1,1-Dichloropropene
 Concen: 4.632 ug/l
 RT: 7.66 min Scan# 1832
 Delta R.T. -0.13 min
 Lab File: VN055647.D
 Acq: 18 May 2019 6:54

Tgt Ion	Ratio	Lower	Upper
75	100		
110	9.1	18.6	55.6#
77	0.0	24.9	37.3#



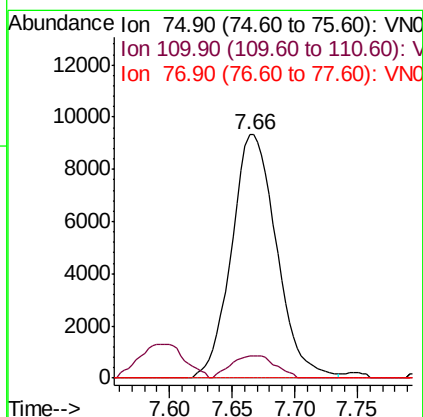





#38
Carbon Tetrachloride
Concen: 6.216 ug/l
RT: 7.67 min Scan# 1833
Delta R.T. -0.11 min
Lab File: VN055647.D
Acq: 18 May 2019 6:54




Instrument :
MSVOA_N
ClientSampled :
TP-20


Tgt Ion: 117 Resp: 33372
Ion Ratio Lower Upper
117 100
119 4.2 77.8 116.8#
121 0.0 24.6 37.0#

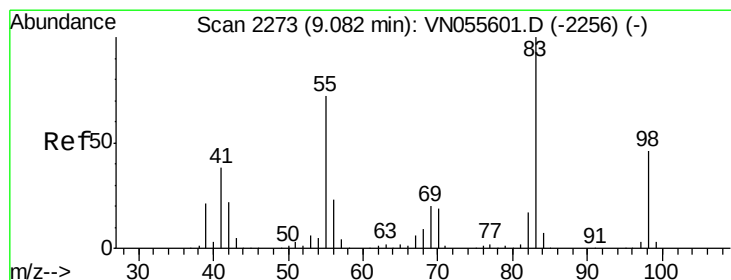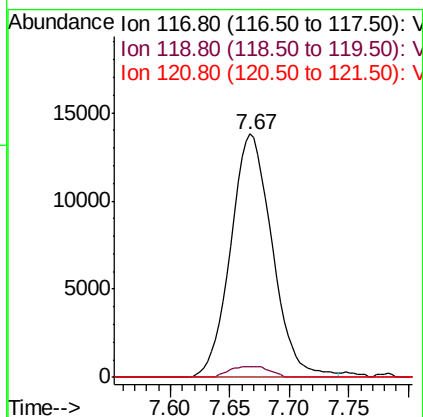

#39
Methylcyclohexane
Concen: 0.221 ug/l
RT: 9.08 min Scan# 2273
Delta R.T. -0.00 min
Lab File: VN055647.D
Acq: 18 May 2019 6:54

Tgt Ion: 83 Resp: 1341
Ion Ratio Lower Upper
83 100
55 59.6 57.8 86.6
98 50.2 36.7 55.1



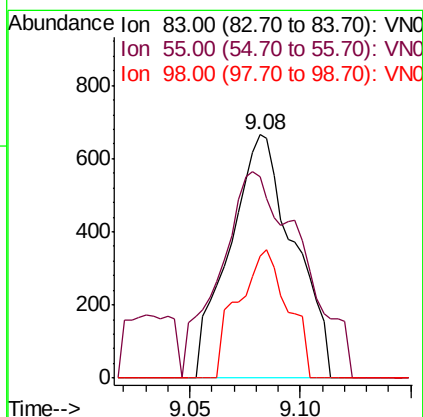
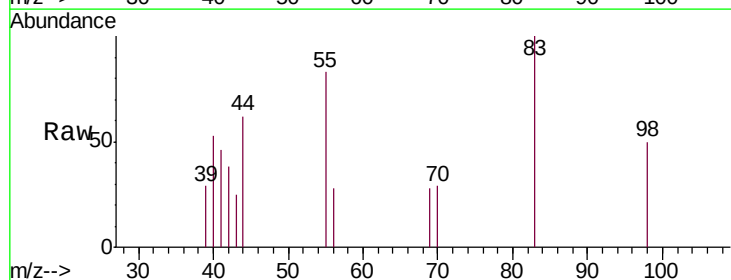




#50
Toluene-d8
Concen: 47.946 ug/l
RT: 10.09 min Scan# 2587
Delta R.T. -0.00 min
Lab File: VN055647.D
Acq: 18 May 2019 6:54




Instrument :
MSVOA_N
ClientSampled :
TP-20


Tgt Ion: 98 Resp: 649016
Ion Ratio Lower Upper
98 100
100 64.6 51.9 77.9

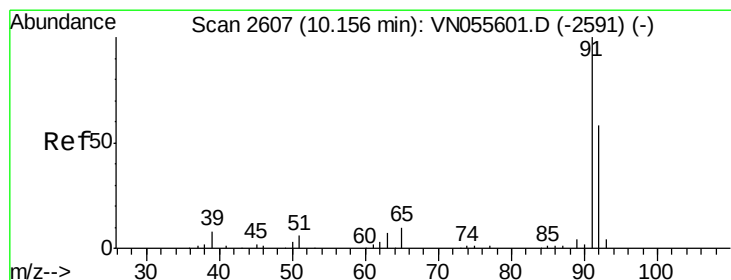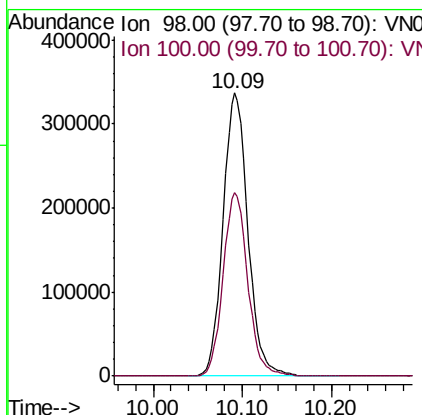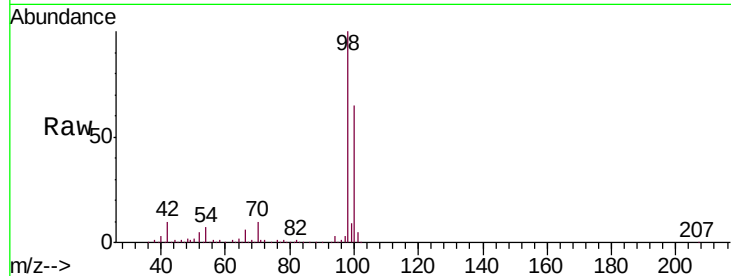

#52
Toluene
Concen: 0.643 ug/l
RT: 10.16 min Scan# 2607
Delta R.T. -0.00 min
Lab File: VN055647.D
Acq: 18 May 2019 6:54

Tgt Ion: 92 Resp: 5964
Ion Ratio Lower Upper
92 100
91 178.0 138.9 208.3

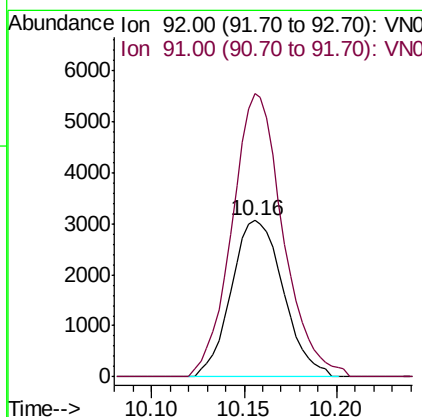







#55
 1,1,2-Trichloroethane
 Concen: 0.232 ug/l
 RT: 10.53 min Scan# 2724
 Delta R.T. -0.03 min
 Lab File: VN055647.D
 Acq: 18 May 2019 6:54

Instrument :
 MSVOA_N
 ClientSampled :
 TP-20

Tgt Ion: 97 Resp: 885
 Ion Ratio Lower Upper
 97 100
 83 0.0 68.4 102.6#
 85 0.0 44.8 67.2#
 99 0.0 49.9 74.9#

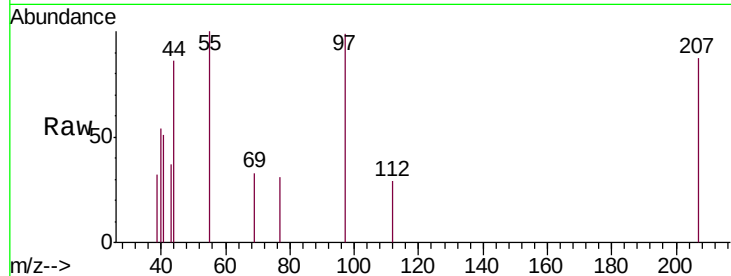


Abundance Ion 96.90 (96.60 to 97.60): VNO
 Ion 82.90 (82.60 to 83.60): VNO
 Ion 84.90 (84.60 to 85.60): VNO
 Ion 98.90 (98.60 to 99.60): VNO

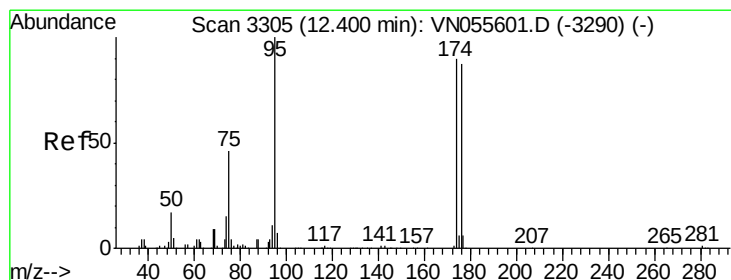
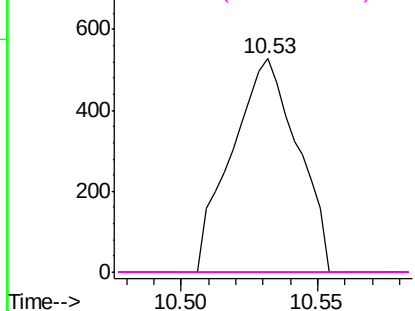



#62
 4-Bromofluorobenzene
 Concen: 45.329 ug/l
 RT: 12.40 min Scan# 3305
 Delta R.T. -0.00 min
 Lab File: VN055647.D
 Acq: 18 May 2019 6:54

Tgt Ion: 95 Resp: 211881
 Ion Ratio Lower Upper
 95 100
 174 92.7 0.0 180.6
 176 90.6 0.0 177.4



Abundance Ion 94.90 (94.60 to 95.60): VNO
 Ion 173.80 (173.50 to 174.50): VNO
 Ion 175.80 (175.50 to 176.50): VNO

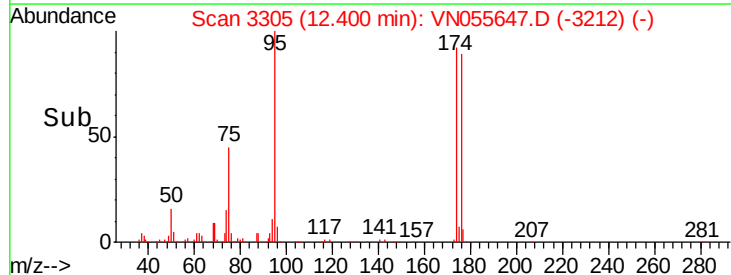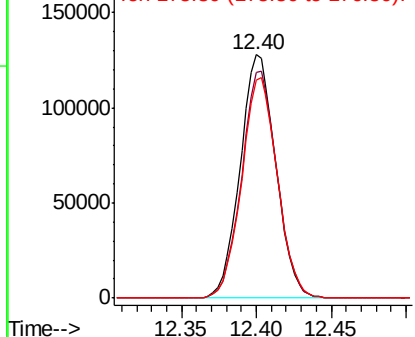







#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.41 min Scan# 2996
Delta R.T. -0.00 min
Lab File: VN055647.D
Acq: 18 May 2019 6:54

Instrument :
MSVOA_N
ClientSampled :
TP-20

Tgt Ion:117 Resp: 472492
Ion Ratio Lower Upper
117 100
82 51.2 42.3 63.5
119 32.4 25.4 38.2

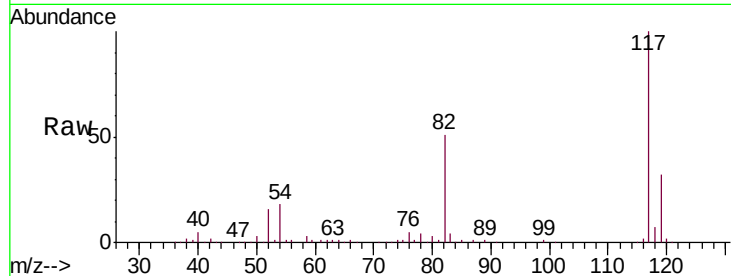


Abundance Ion 116.90 (116.60 to 117.60): V
Ion 82.00 (81.70 to 82.70): VN
Ion 118.90 (118.60 to 119.60): V


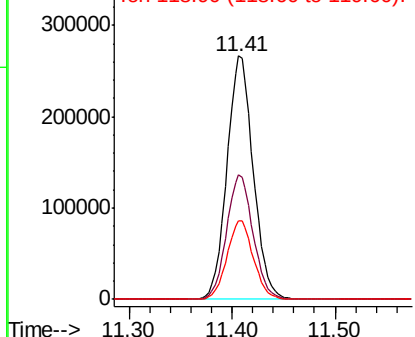



#68
m/p-Xylenes
Concen: 0.345 ug/l
RT: 11.62 min Scan# 3063
Delta R.T. -0.00 min
Lab File: VN055647.D
Acq: 18 May 2019 6:54

Tgt Ion:106 Resp: 2218
Ion Ratio Lower Upper
106 100
91 201.0 160.5 240.7



Abundance Ion 106.00 (105.70 to 106.70): V
Ion 91.00 (90.70 to 91.70): VN

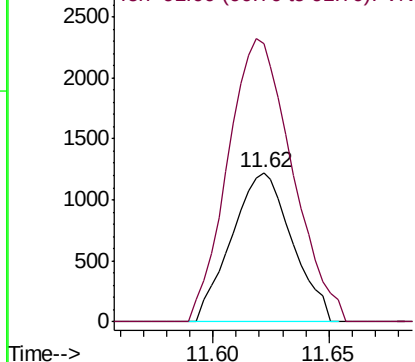


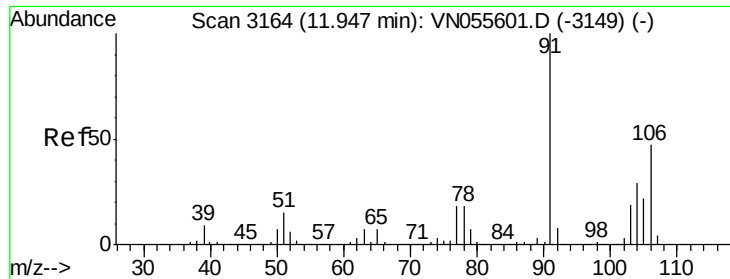




#69
o-Xylene
Concen: 0.257 ug/l
RT: 11.95 min Scan# 3164
Delta R.T. -0.00 min
Lab File: VN055647.D
Acq: 18 May 2019 6:54

Instrument :
MSVOA_N
ClientSampled :
TP-20

Tgt Ion:106 Resp: 1613
Ion Ratio Lower Upper
106 100
91 244.8 106.7 320.2

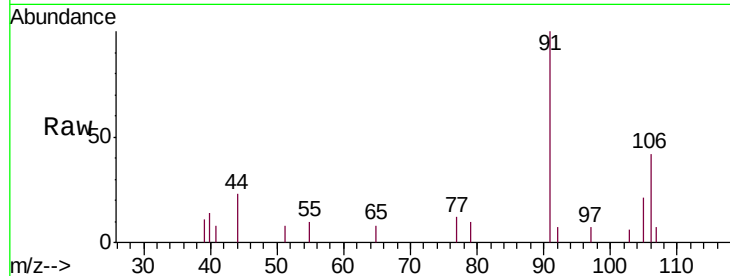


Abundance Ion 106.00 (105.70 to 106.70): V
Ion 91.00 (90.70 to 91.70): VN


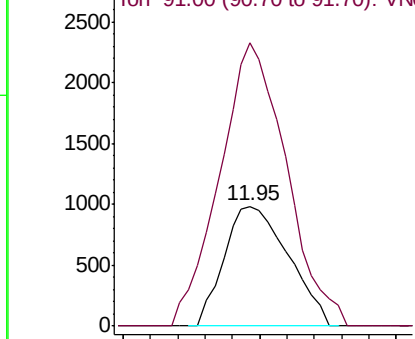



#71
Bromoform
Concen: 0.398 ug/l
RT: 12.40 min Scan# 3305
Delta R.T. 0.27 min
Lab File: VN055647.D
Acq: 18 May 2019 6:54

Tgt Ion:173 Resp: 1298
Ion Ratio Lower Upper
173 100
175 971.4 24.3 72.9#
254 0.0 0.1 0.1#



Abundance Ion 172.70 (172.40 to 173.40): V
Ion 174.70 (174.40 to 175.40): V
Ion 254.40 (254.10 to 255.10): V

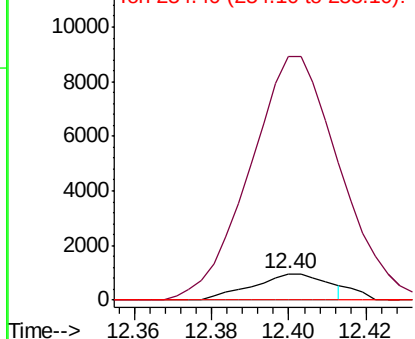




#72




1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.34 min Scan# 3598
Delta R.T. -0.00 min
Lab File: VN055647.D
Acq: 18 May 2019 6:54

Instrument :
MSVOA_N
ClientSampled :
TP-20

Tgt Ion:152 Resp: 195499
Ion Ratio Lower Upper
152 100
115 55.3 28.1 84.2
150 155.8 0.0 348.0

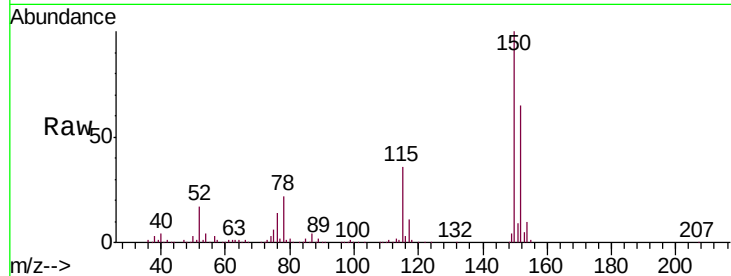


Abundance Ion 151.90 (151.60 to 152.60): V
Ion 114.90 (114.60 to 115.60): V
Ion 149.90 (149.60 to 150.60): V

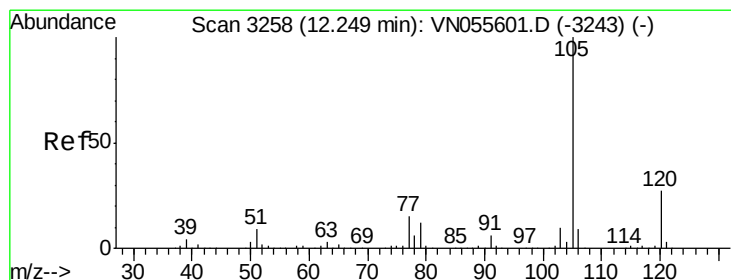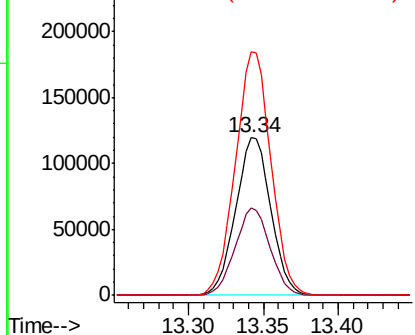



#73


Isopropylbenzene
Concen: Below Cal
RT: 12.25 min Scan# 3258
Delta R.T. 0.00 min
Lab File: VN055647.D
Acq: 18 May 2019 6:54

Tgt Ion:105 Resp: 3436
Ion Ratio Lower Upper
105 100
120 23.1 13.4 40.2



Abundance Ion 105.00 (104.70 to 105.70): V
Ion 120.00 (119.70 to 120.70): V

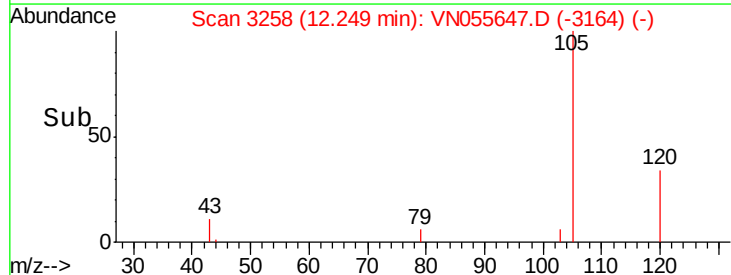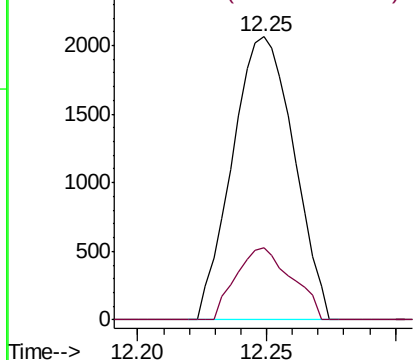

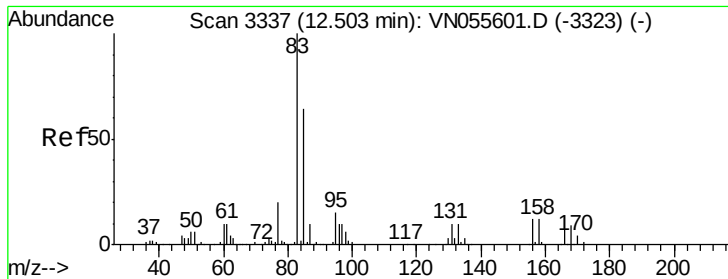

#75

1,1,2,2-Tetrachloroethane

Concen: Below Cal

RT: 12.56 min Scan# 3356

Delta R.T. 0.06 min

Lab File: VN055647.D

Acq: 18 May 2019 6:54

Instrument :


MSVOA_N

ClientSampled :

TP-20

Tgt Ion: 83 Resp: 60




Ion	Ratio	Lower	Upper
83	100		
131	0.0	5.3	16.1#
85	0.0	32.0	96.2#

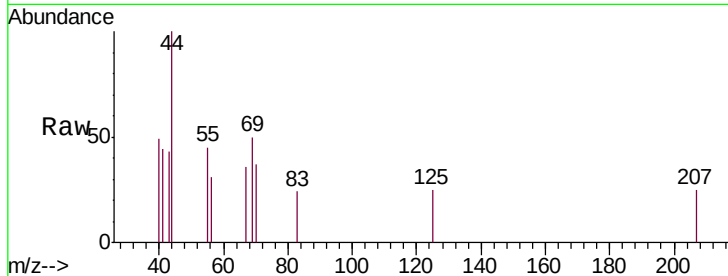

Abundance Ion 82.90 (82.60 to 83.60): VN0

Ion 130.80 (130.50 to 131.50): VN0

Ion 84.90 (84.60 to 85.60): VN0

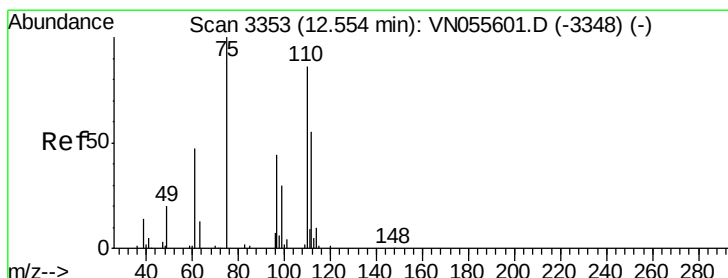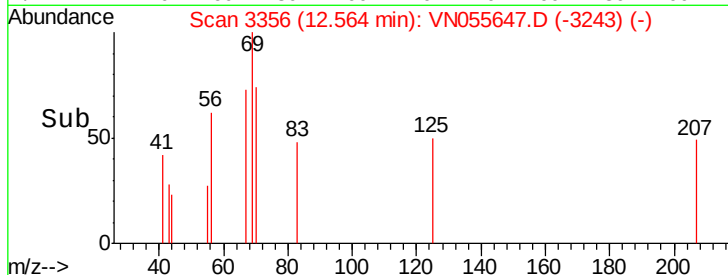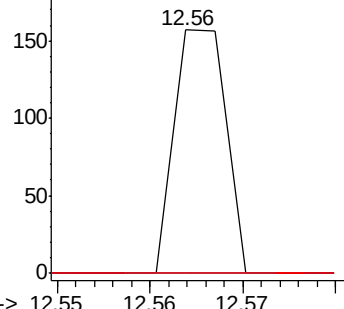

#76

1,2,3-Trichloropropane

Concen: 24.230 ug/l

RT: 12.40 min Scan# 3305


Delta R.T. -0.15 min

Lab File: VN055647.D

Acq: 18 May 2019 6:54



Tgt Ion: 75 Resp: 96658


Ion	Ratio	Lower	Upper
75	100		
77	1.2	0.0	0.0#

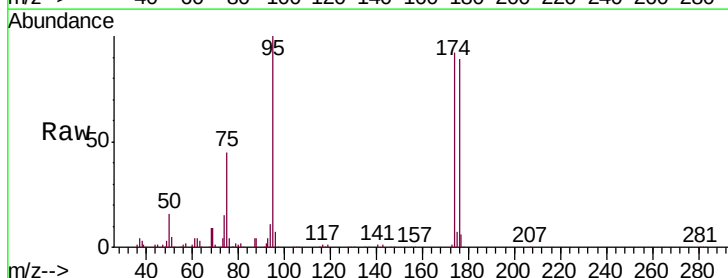

Abundance Ion 74.90 (74.60 to 75.60): VN0

Ion 77.00 (76.70 to 77.70): VN0



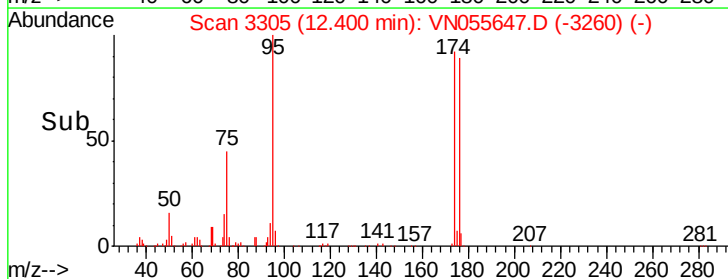
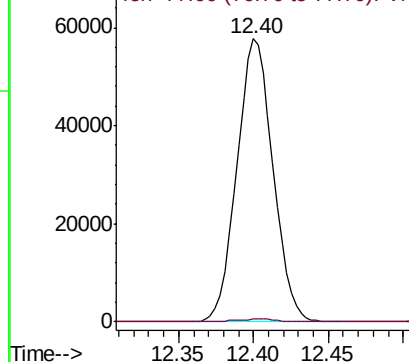


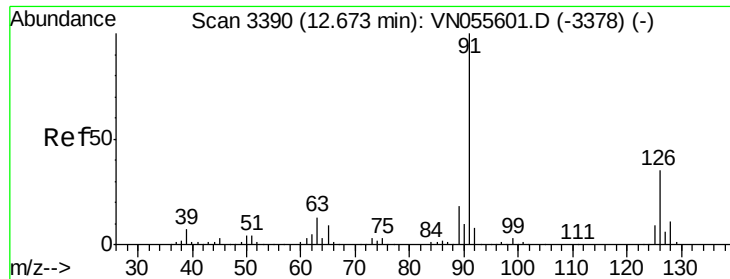

#79
 2-Chlorotoluene
 Concen: Below Cal
 RT: 12.66 min Scan# 3386
 Delta R.T. -0.01 min
 Lab File: VN055647.D
 Acq: 18 May 2019 6:54




Instrument :
 MSVOA_N
 ClientSampled :
 TP-20


Tgt Ion: 91 Resp: 225
 Ion Ratio Lower Upper
 91 100
 126 0.0 17.8 53.4#

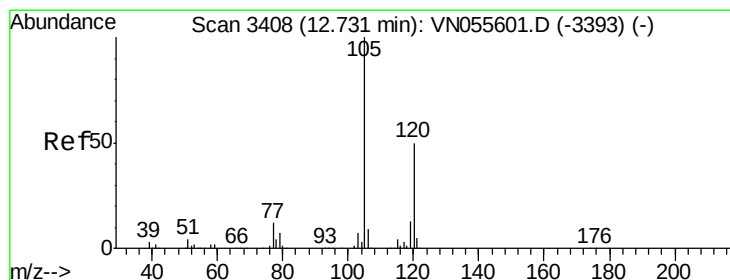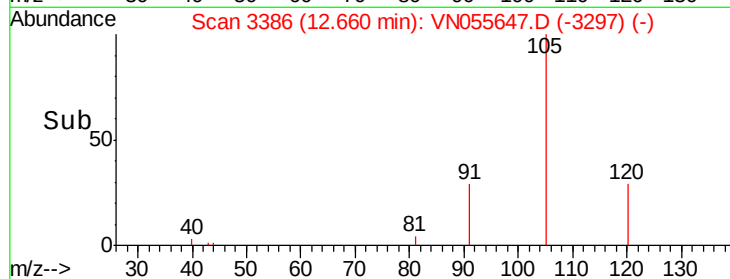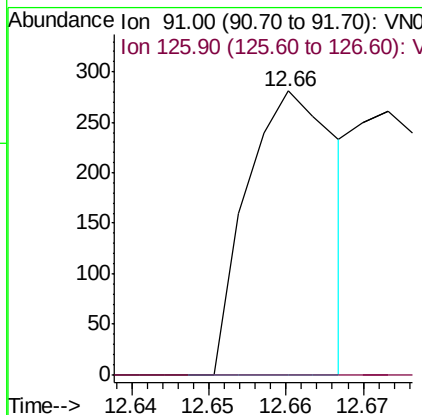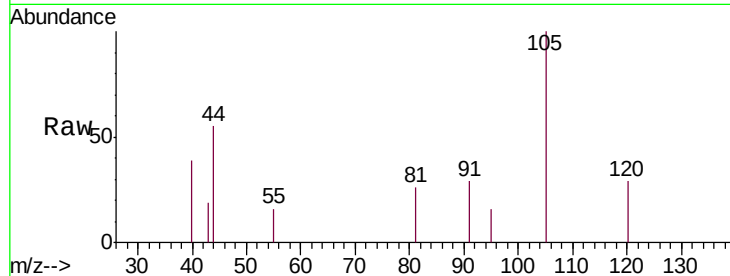

#80
 1,3,5-Trimethylbenzene
 Concen: Below Cal
 RT: 12.73 min Scan# 3409
 Delta R.T. 0.00 min
 Lab File: VN055647.D
 Acq: 18 May 2019 6:54

Tgt Ion: 105 Resp: 1253
 Ion Ratio Lower Upper
 105 100
 120 46.6 24.6 74.0


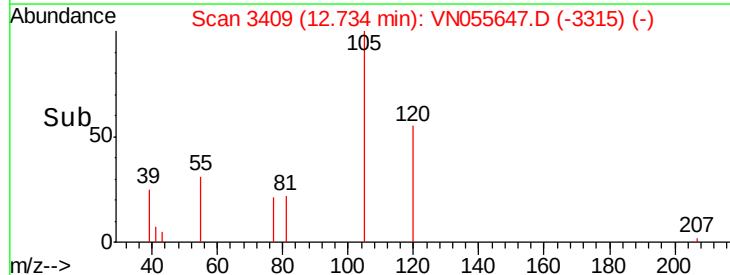
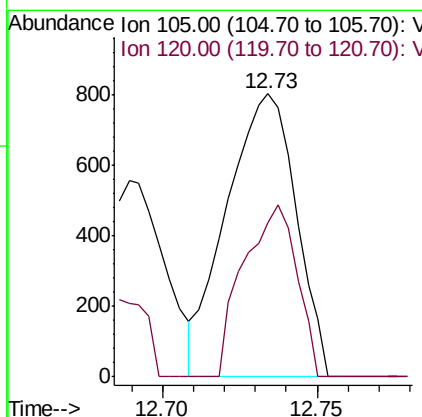





#81
 trans-1,4-Dichloro-2-butene
 Concen: 62.285 ug/l
 RT: 12.40 min Scan# 3305
 Delta R.T. 0.10 min
 Lab File: VN055647.D
 Acq: 18 May 2019 6:54




Instrument :
 MSVOA_N
 ClientSampled :
 TP-20


Tgt Ion: 75 Resp: 96658
 Ion Ratio Lower Upper
 75 100
 53 0.0 65.1 97.7#
 89 0.0 36.4 54.6#

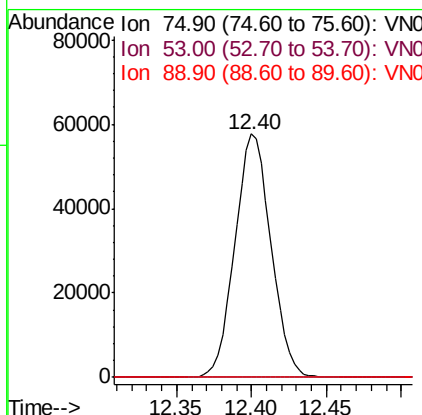

#83
 tert-Butylbenzene
 Concen: Below Cal
 RT: 12.99 min Scan# 3489
 Delta R.T. 0.00 min
 Lab File: VN055647.D
 Acq: 18 May 2019 6:54

Tgt Ion: 119 Resp: 2367
 Ion Ratio Lower Upper
 119 100
 91 70.2 31.3 93.8
 134 25.9 13.2 39.6



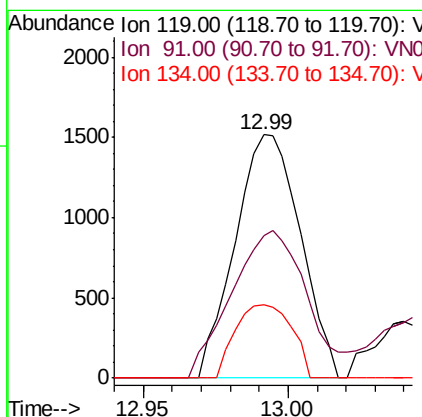





#84
 1,2,4-Trimethylbenzene
 Concen: Below Cal
 RT: 13.04 min Scan# 3504
 Delta R.T. 0.00 min
 Lab File: VN055647.D
 Acq: 18 May 2019 6:54




Instrument :
 MSVOA_N
 ClientSampled :
 TP-20


Tgt Ion:105 Resp: 3840
 Ion Ratio Lower Upper
 105 100
 120 46.4 23.1 69.2

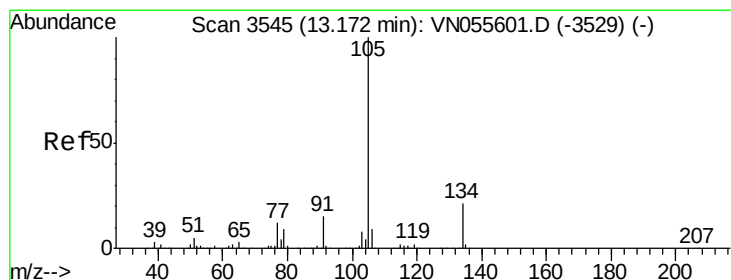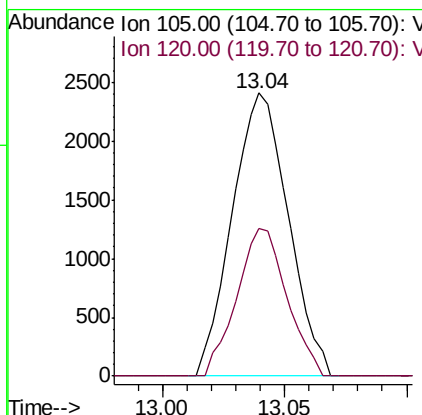

#85
 sec-Butylbenzene
 Concen: Below Cal
 RT: 13.17 min Scan# 3545
 Delta R.T. 0.00 min
 Lab File: VN055647.D
 Acq: 18 May 2019 6:54

Tgt Ion:105 Resp: 3987
 Ion Ratio Lower Upper
 105 100
 134 32.4 10.3 30.9#



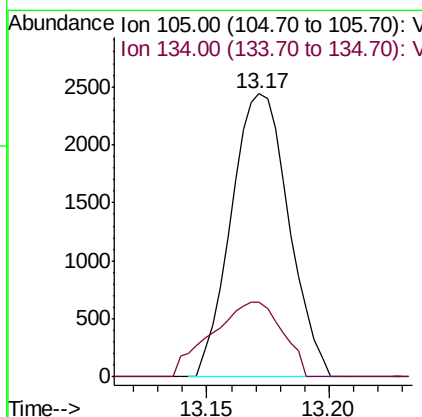





#86
p-Isopropyltoluene
Concen: Below Cal
RT: 13.44 min Scan# 3629
Delta R.T. 0.15 min
Lab File: VN055647.D
Acq: 18 May 2019 6:54




Instrument :
MSVOA_N
ClientSampled :
TP-20


Tgt Ion:119 Resp: 4490
Ion Ratio Lower Upper
119 100
134 29.4 13.4 40.2
91 24.3 11.0 33.0

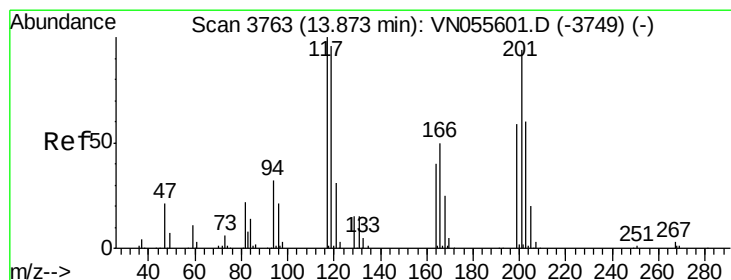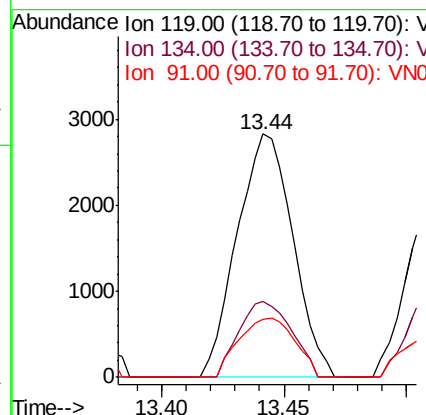

#90
Hexachloroethane
Concen: Below Cal
RT: 13.89 min Scan# 3768
Delta R.T. 0.02 min
Lab File: VN055647.D
Acq: 18 May 2019 6:54

Tgt Ion:117 Resp: 1376
Ion Ratio Lower Upper
117 100
201 0.0 47.1 141.3#



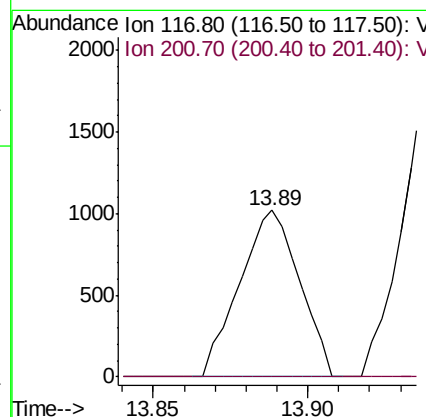
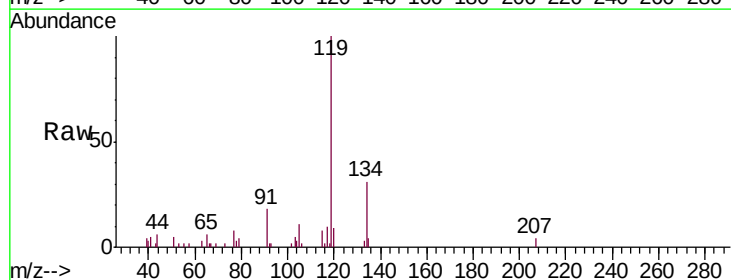




#92
 1,2-Dibromo-3-Chloropropane
 Concen: 0.335 ug/l
 RT: 13.99 min Scan# 3800
 Delta R.T. -0.28 min
 Lab File: VN055647.D
 Acq: 18 May 2019 6:54

Instrument :
 MSVOA_N
 ClientSampleId :
 TP-20

Tgt Ion: 75 Resp: 297
 Ion Ratio Lower Upper
 75 100
 155 0.0 48.4 145.0#
 157 0.0 62.3 186.8#

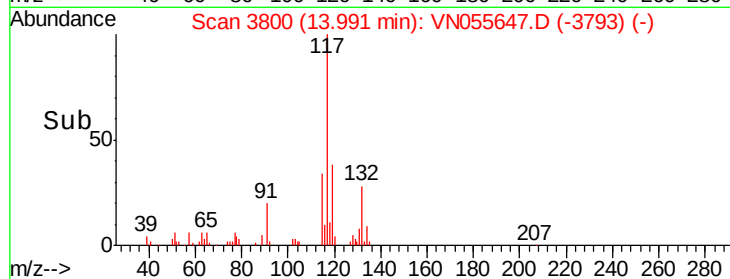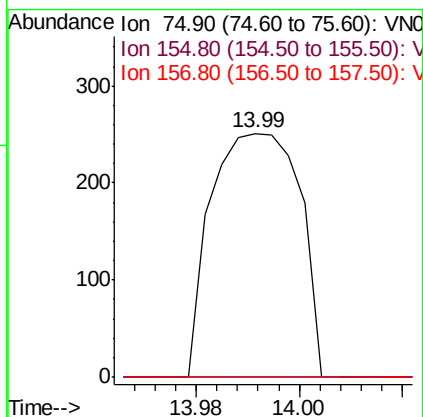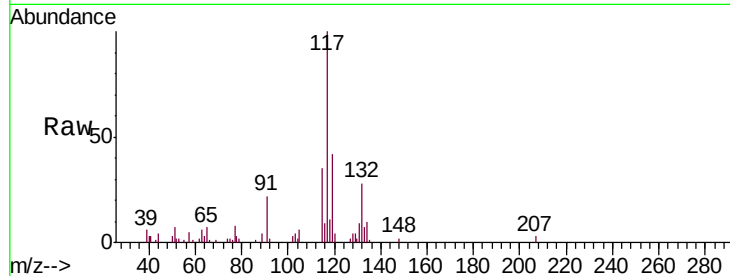

#95
 Naphthalene
 Concen: 2.041 ug/l
 RT: 15.13 min Scan# 4154
 Delta R.T. 0.00 min
 Lab File: VN055647.D
 Acq: 18 May 2019 6:54

Tgt Ion: 128 Resp: 2916
 Ion Ratio Lower Upper
 128 100
 127 9.7 10.2 15.4#
 129 8.8 8.6 12.8

