



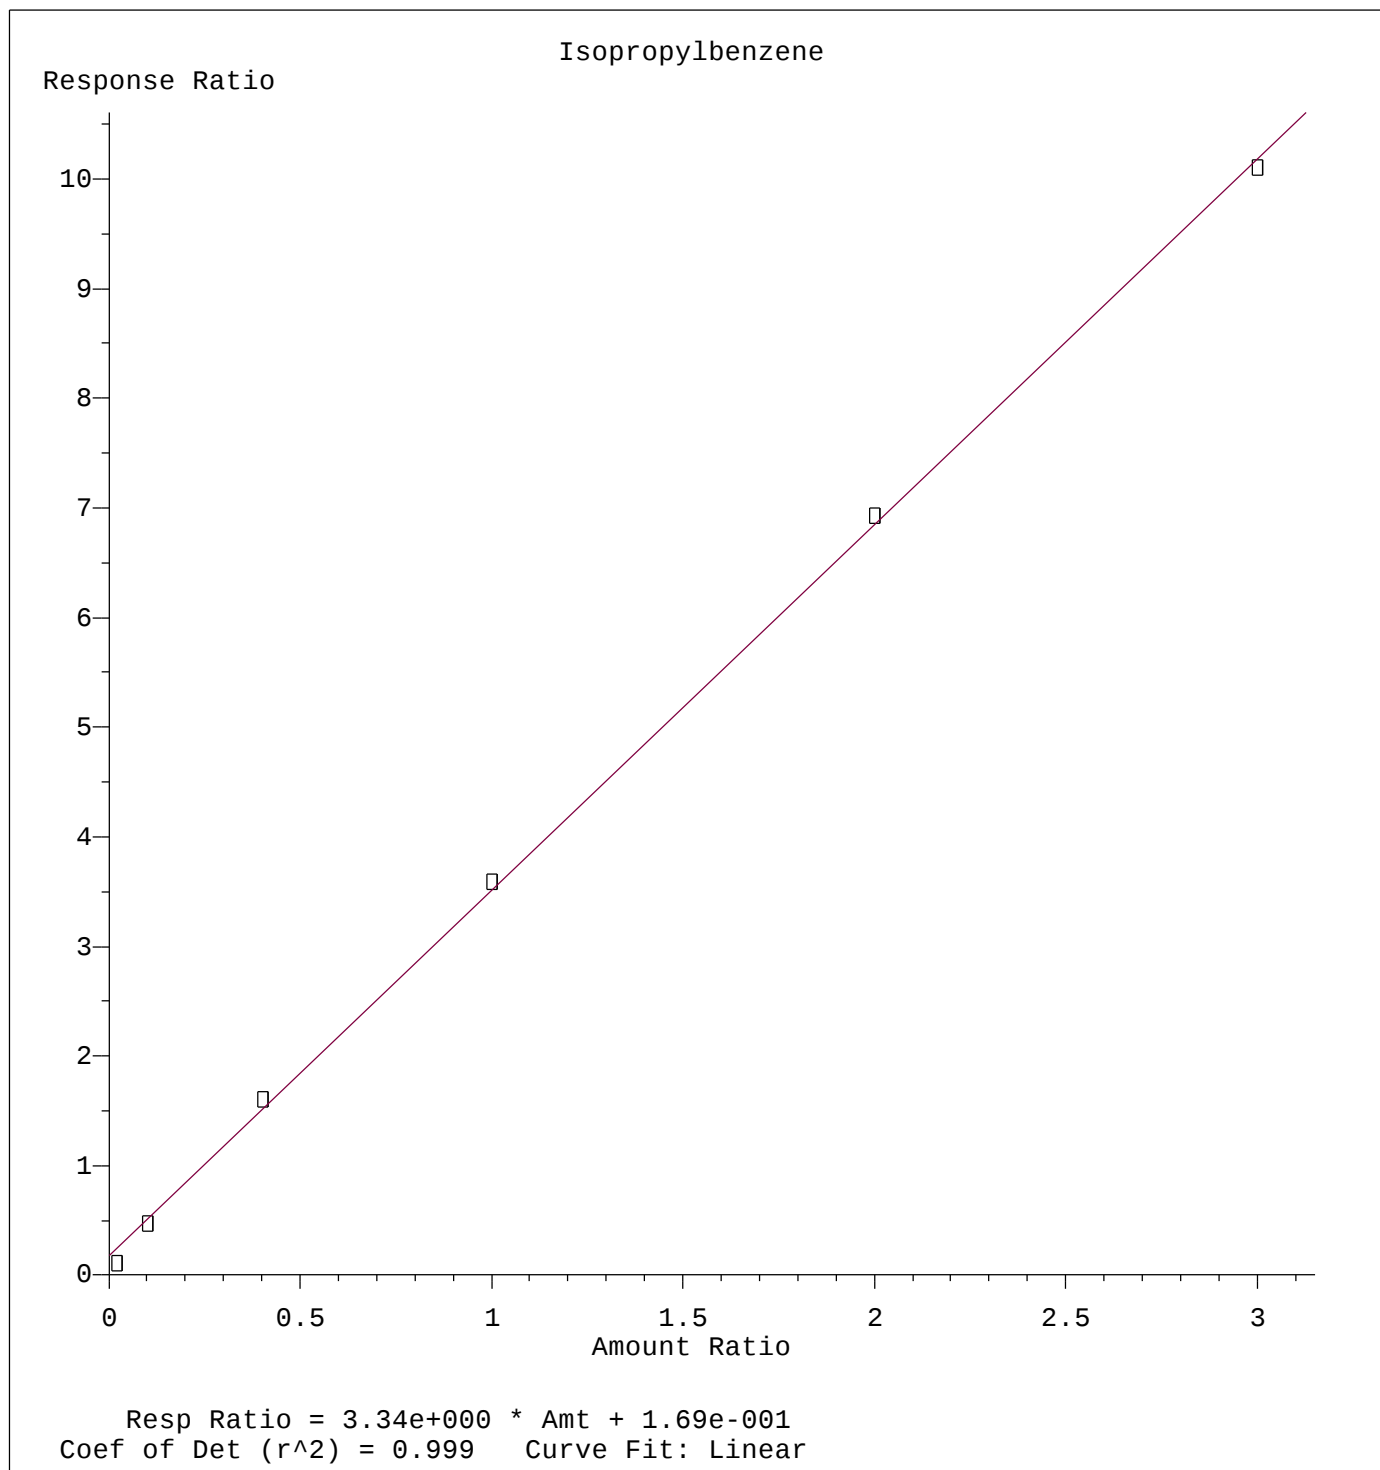

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N051719W.M
Calibration Table Last Updated: Fri May 17 23:54:12 2019

1,1,2,2-Tetrachloroethane

Response Ratio

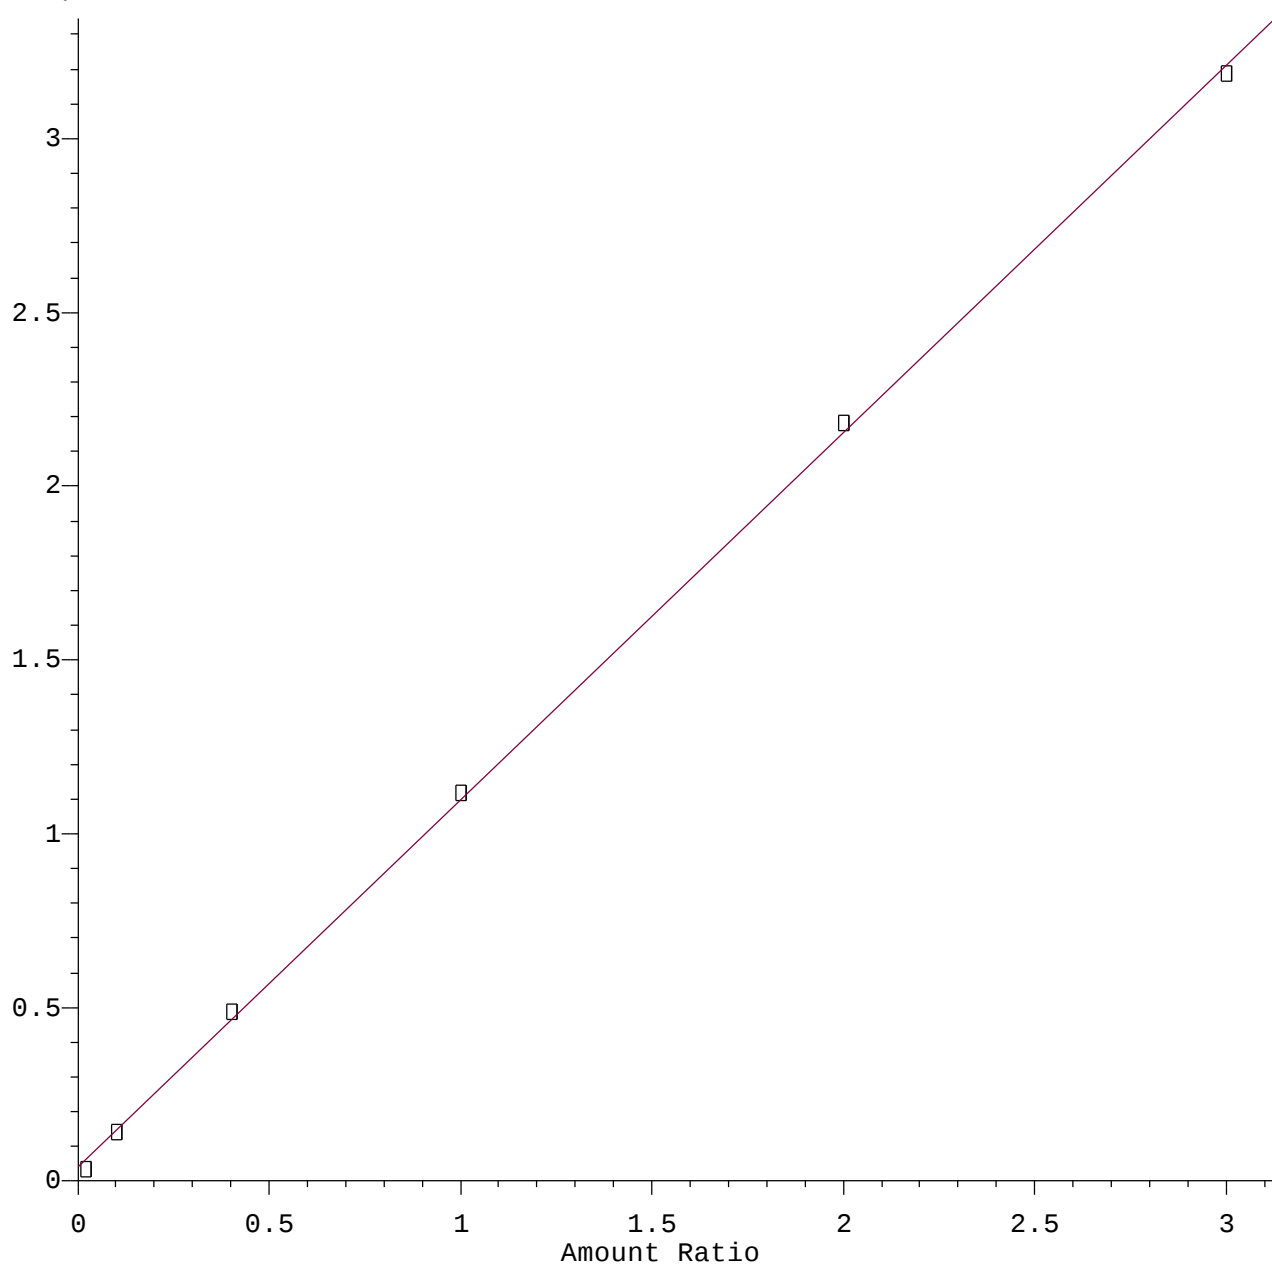


Resp Ratio = 1.06e+000 * Amt + 4.24e-002
Coef of Det (r^2) = 1.000 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N051719W.M
Calibration Table Last Updated: Fri May 17 23:54:12 2019

2-Chlorotoluene

Response Ratio

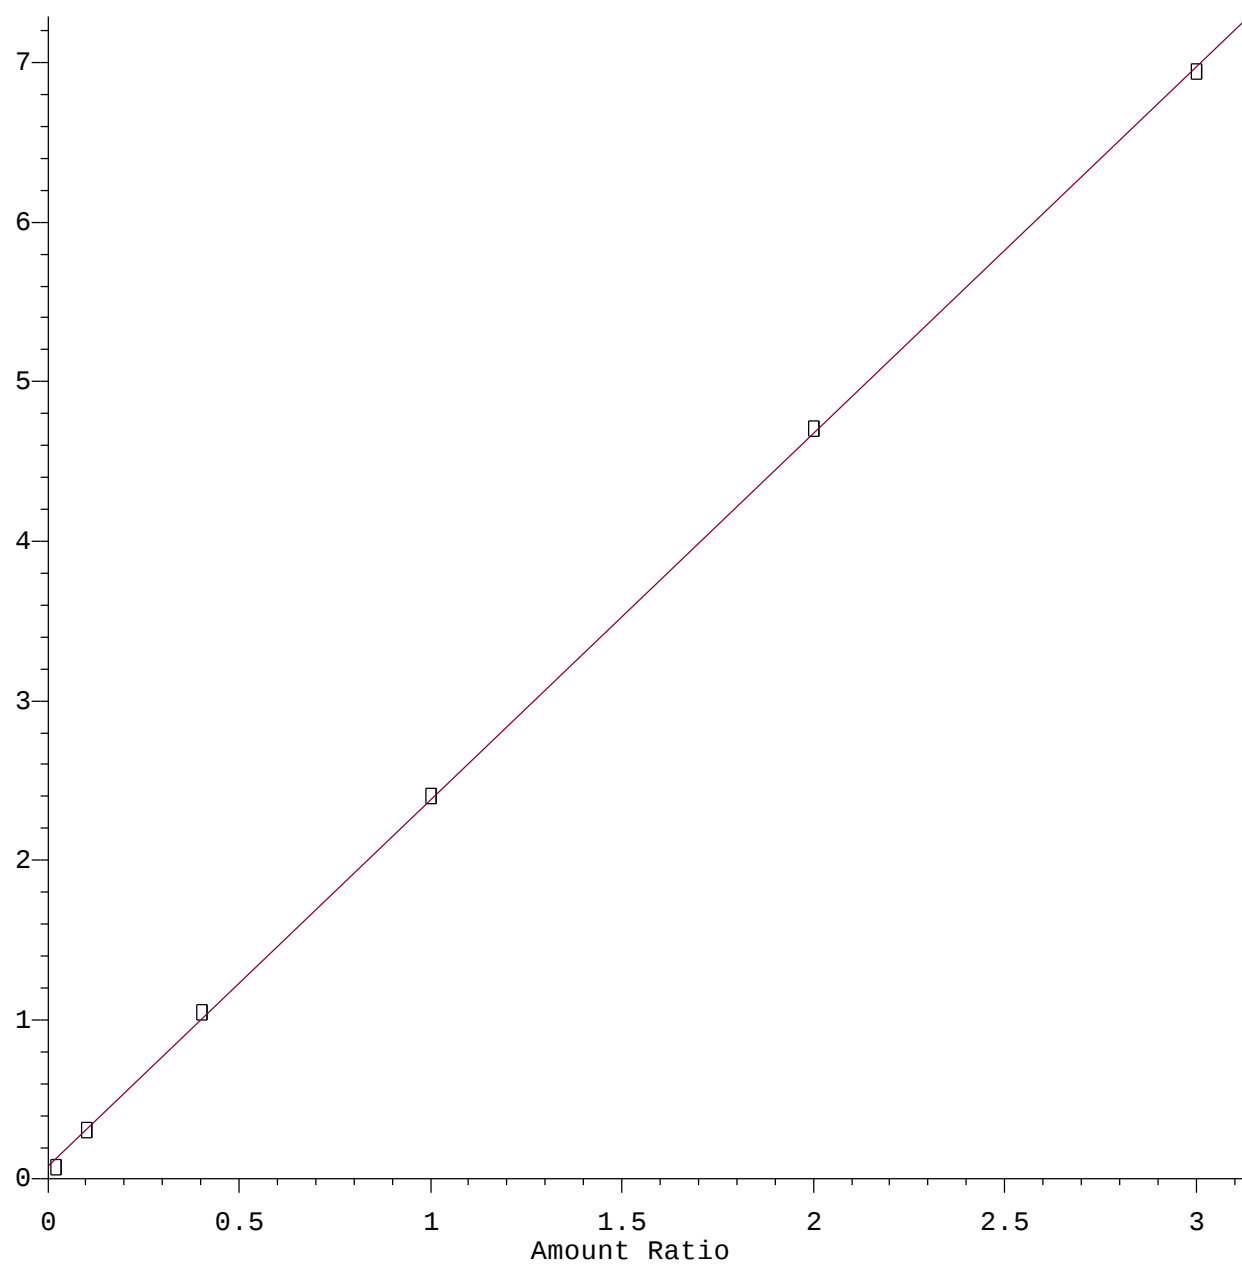


Resp Ratio = 2.30e+000 * Amt + 7.99e-002
Coef of Det (r^2) = 1.000 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N051719W.M
Calibration Table Last Updated: Fri May 17 23:54:12 2019

1,3,5-Trimethylbenzene

Response Ratio

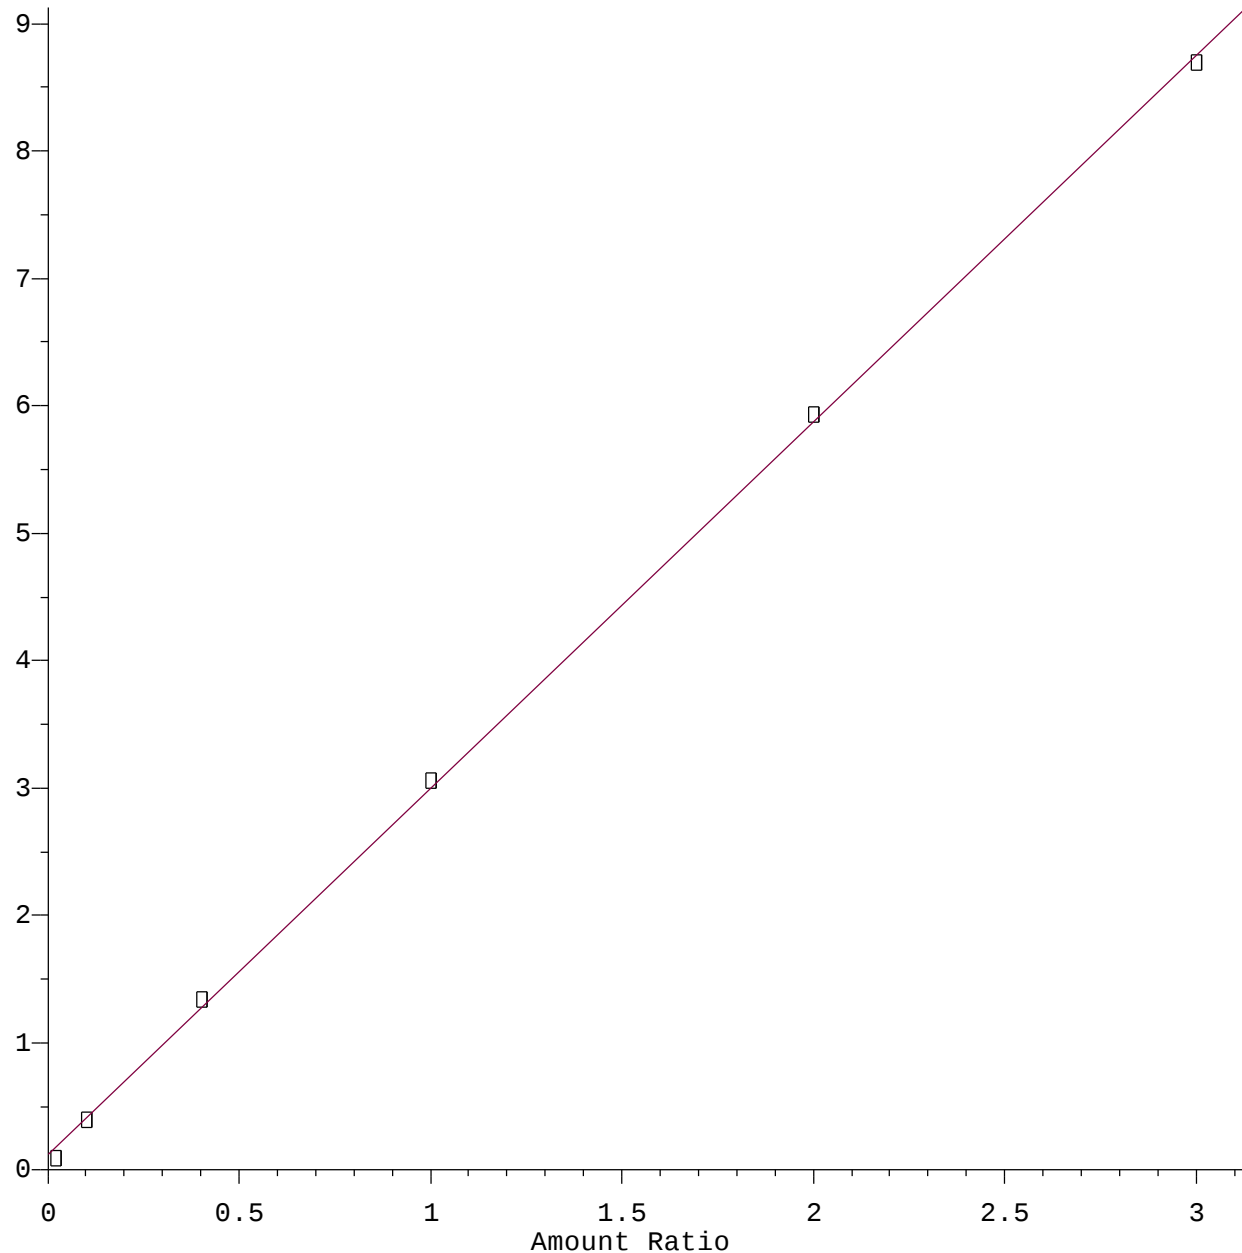


Resp Ratio = 2.88e+000 * Amt + 1.22e-001
Coef of Det (r^2) = 1.000 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N051719W.M
Calibration Table Last Updated: Fri May 17 23:54:12 2019

tert-Butylbenzene

Response Ratio

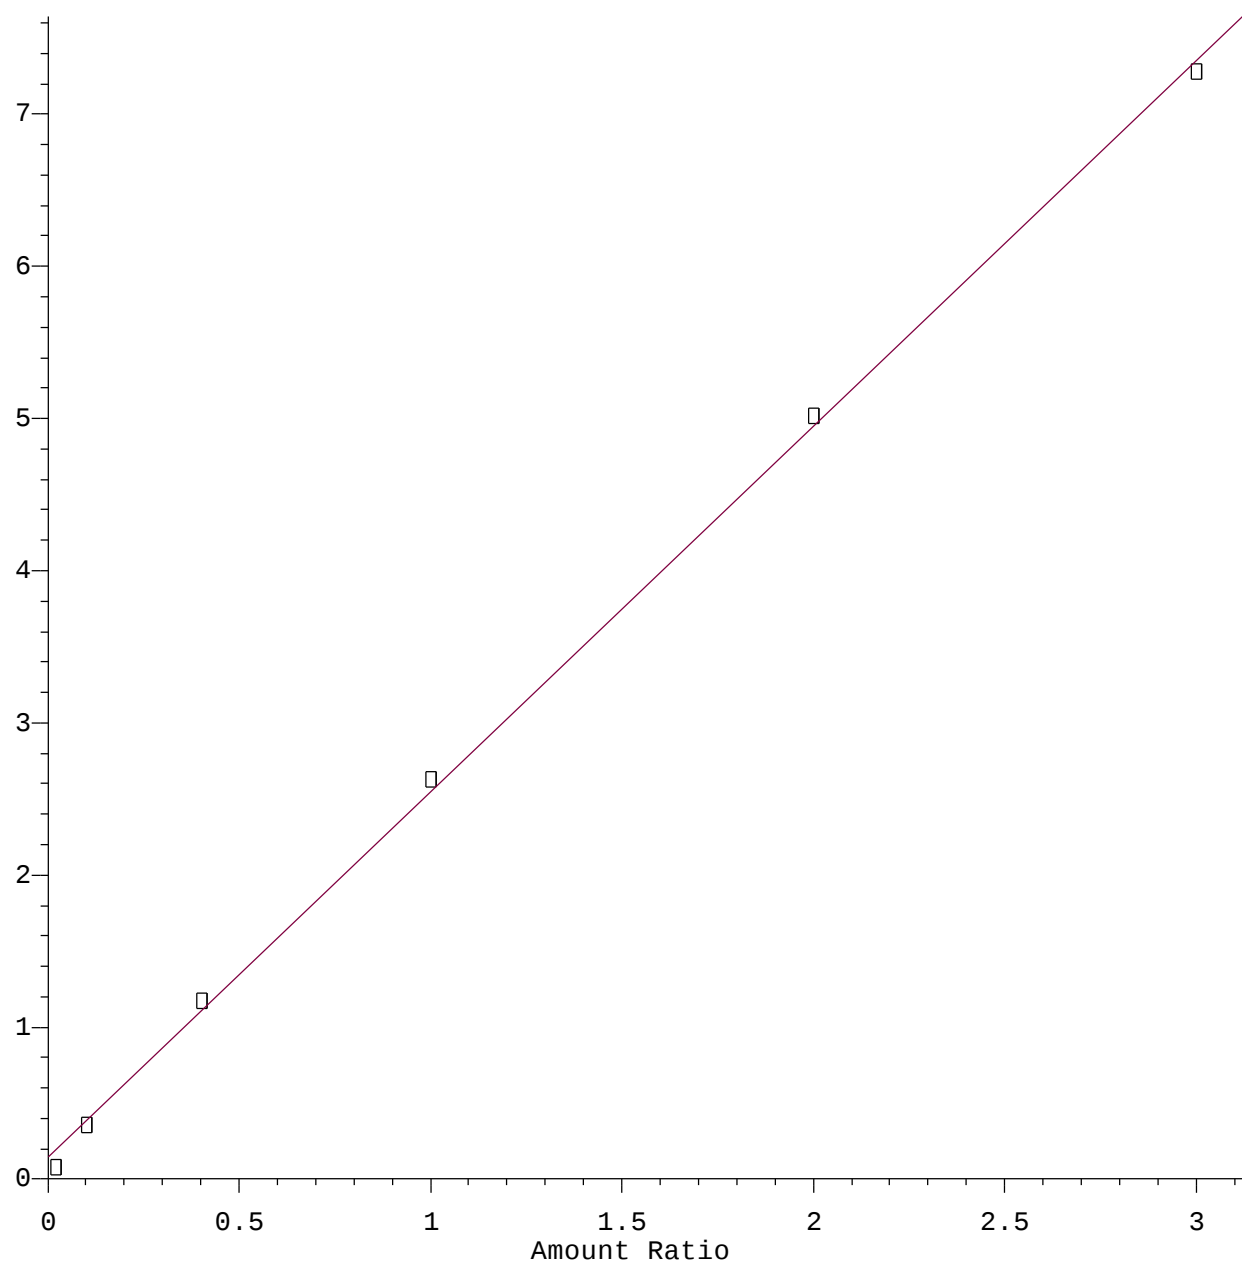


Resp Ratio = 2.40e+000 * Amt + 1.40e-001
Coef of Det (r^2) = 0.999 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N051719W.M
Calibration Table Last Updated: Fri May 17 23:54:12 2019

1,2,4-Trimethylbenzene

Response Ratio

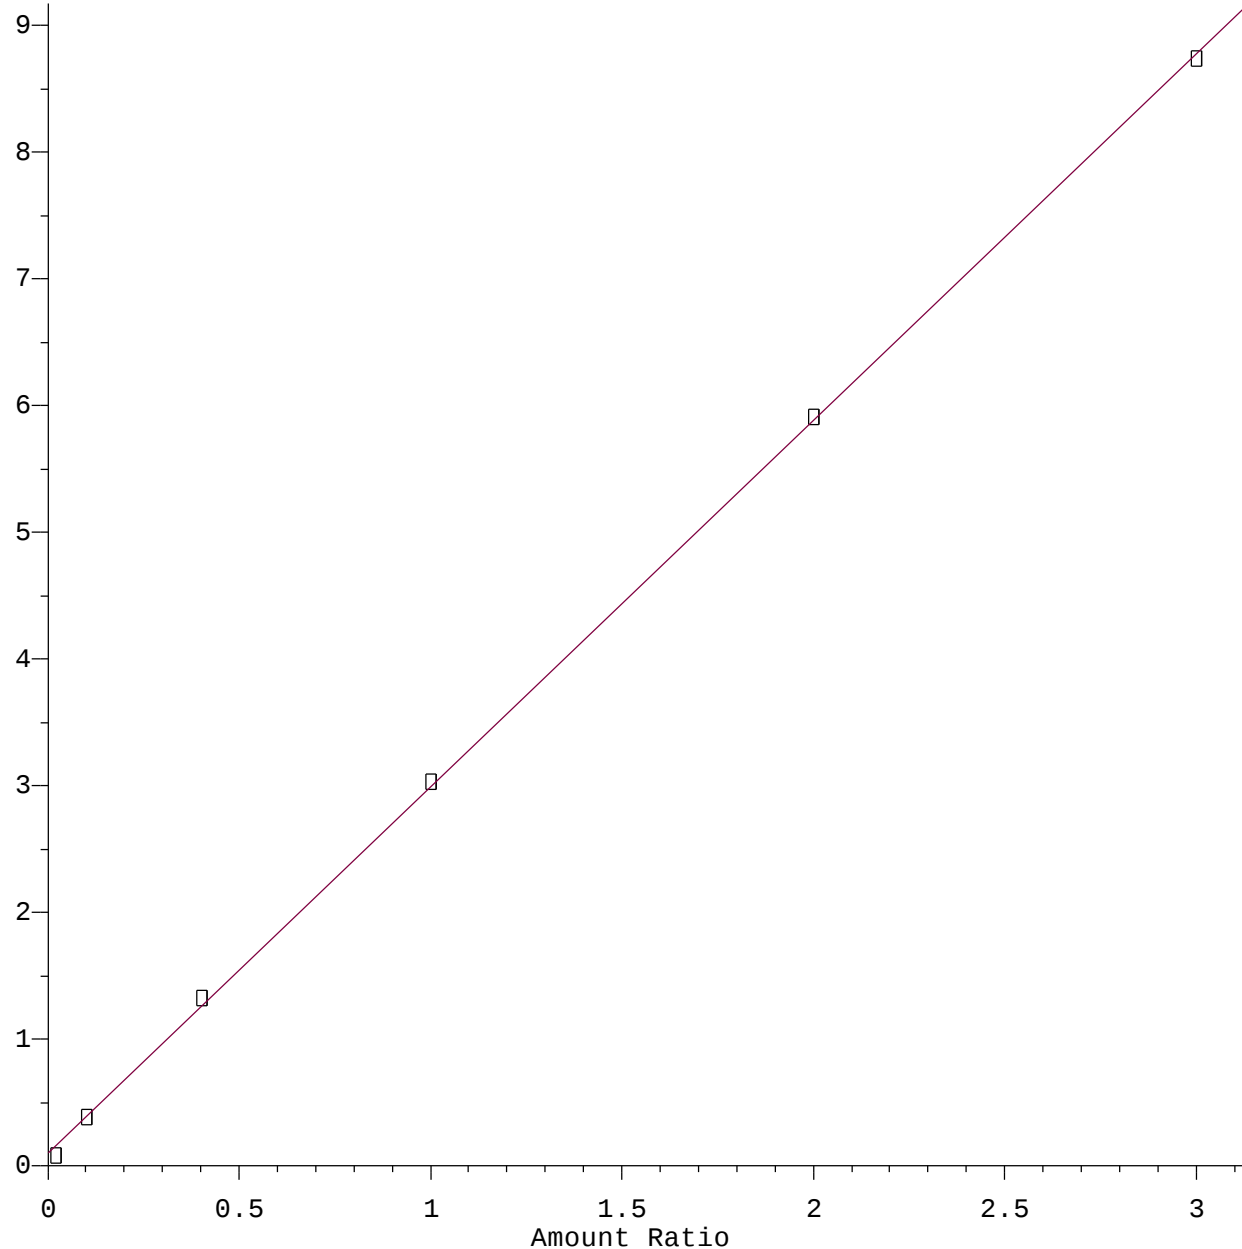


Resp Ratio = 2.89e+000 * Amt + 1.04e-001
Coef of Det (r^2) = 1.000 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N051719W.M
Calibration Table Last Updated: Fri May 17 23:54:12 2019

sec-Butylbenzene

Response Ratio

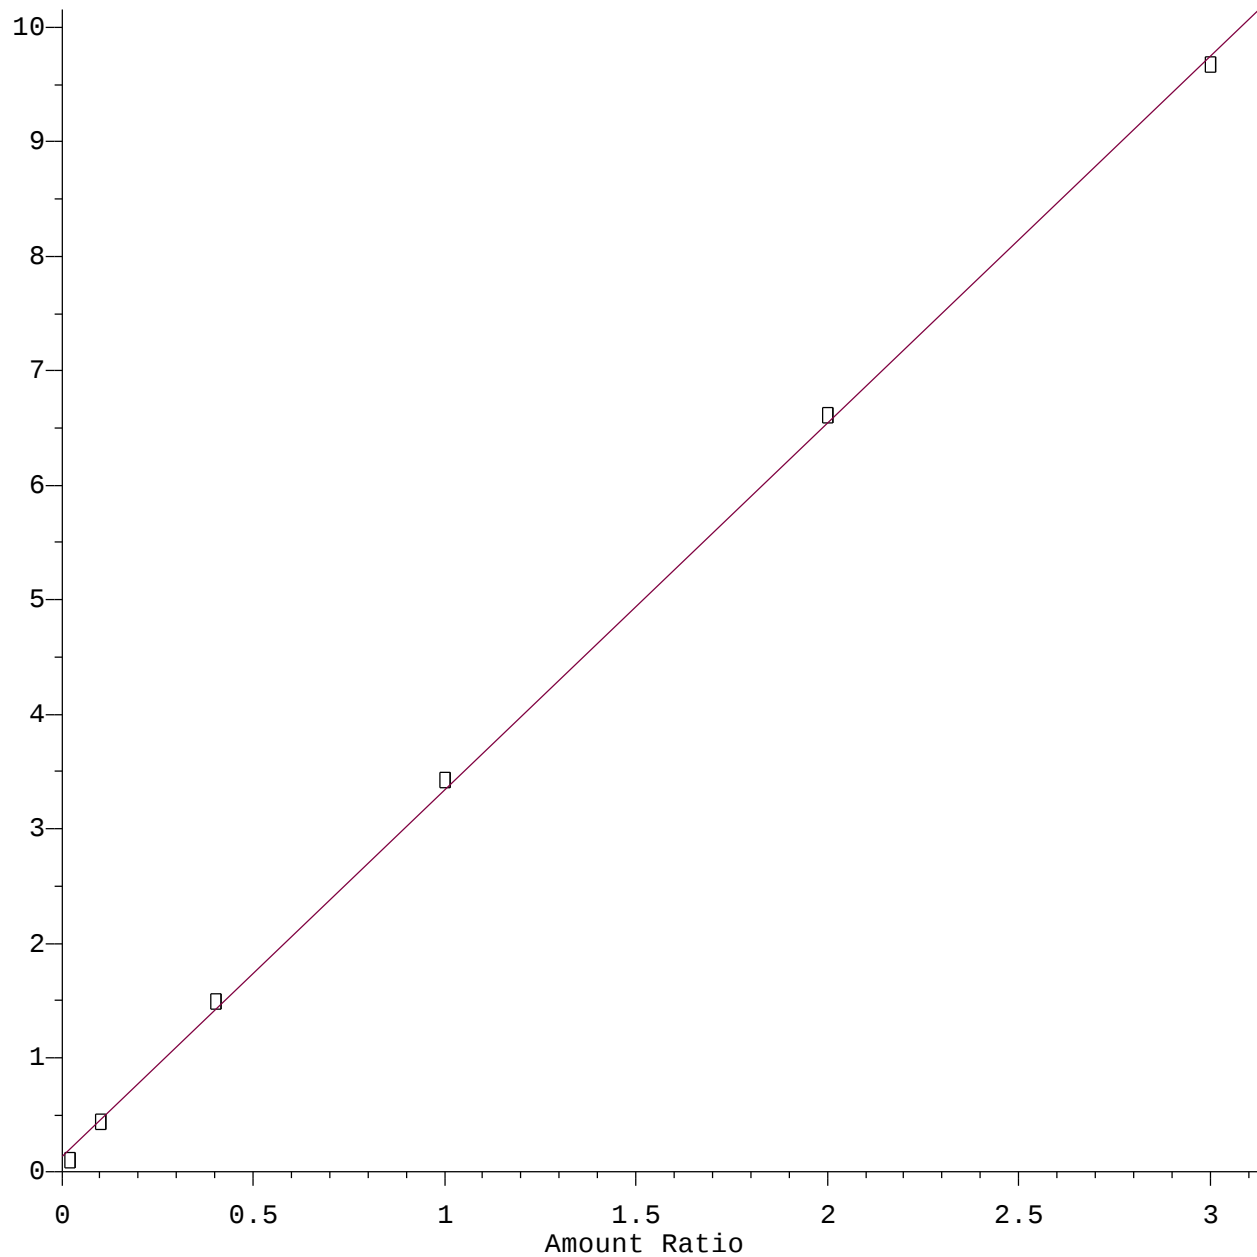


Resp Ratio = 3.20e+000 * Amt + 1.43e-001
Coef of Det (r^2) = 1.000 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N051719W.M
Calibration Table Last Updated: Fri May 17 23:54:12 2019


p-Isopropyltoluene

Response Ratio

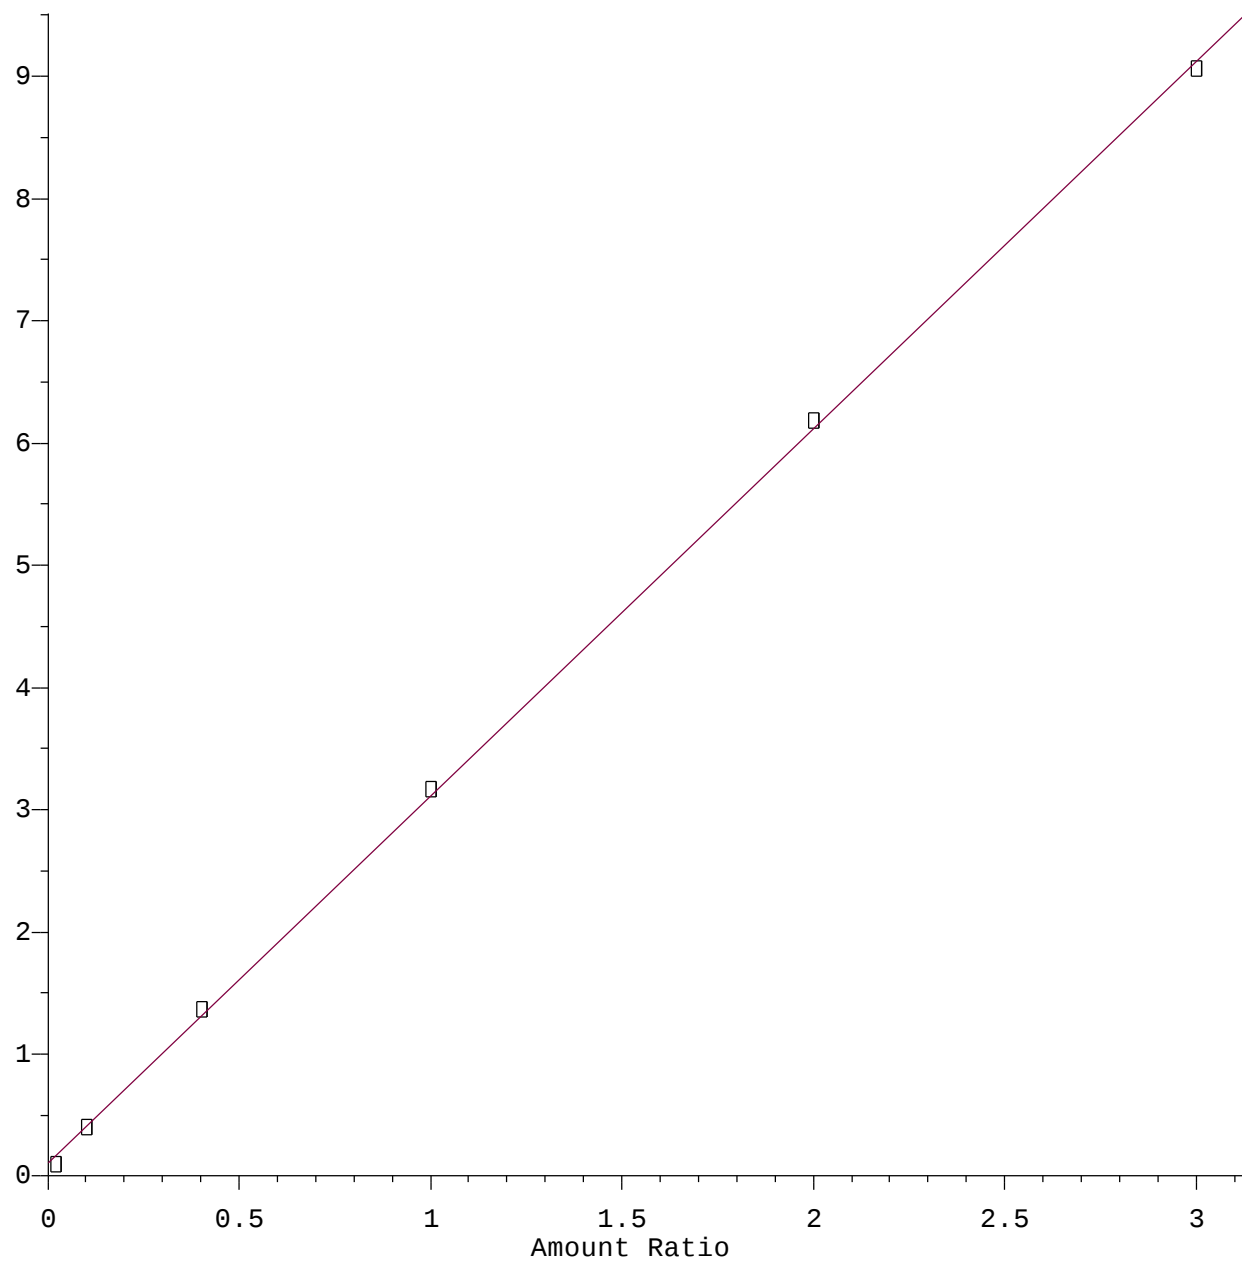


Resp Ratio = 3.00e+000 * Amt + 1.09e-001
Coef of Det (r^2) = 1.000 Curve Fit: Linear


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N051719W.M
Calibration Table Last Updated: Fri May 17 23:54:12 2019

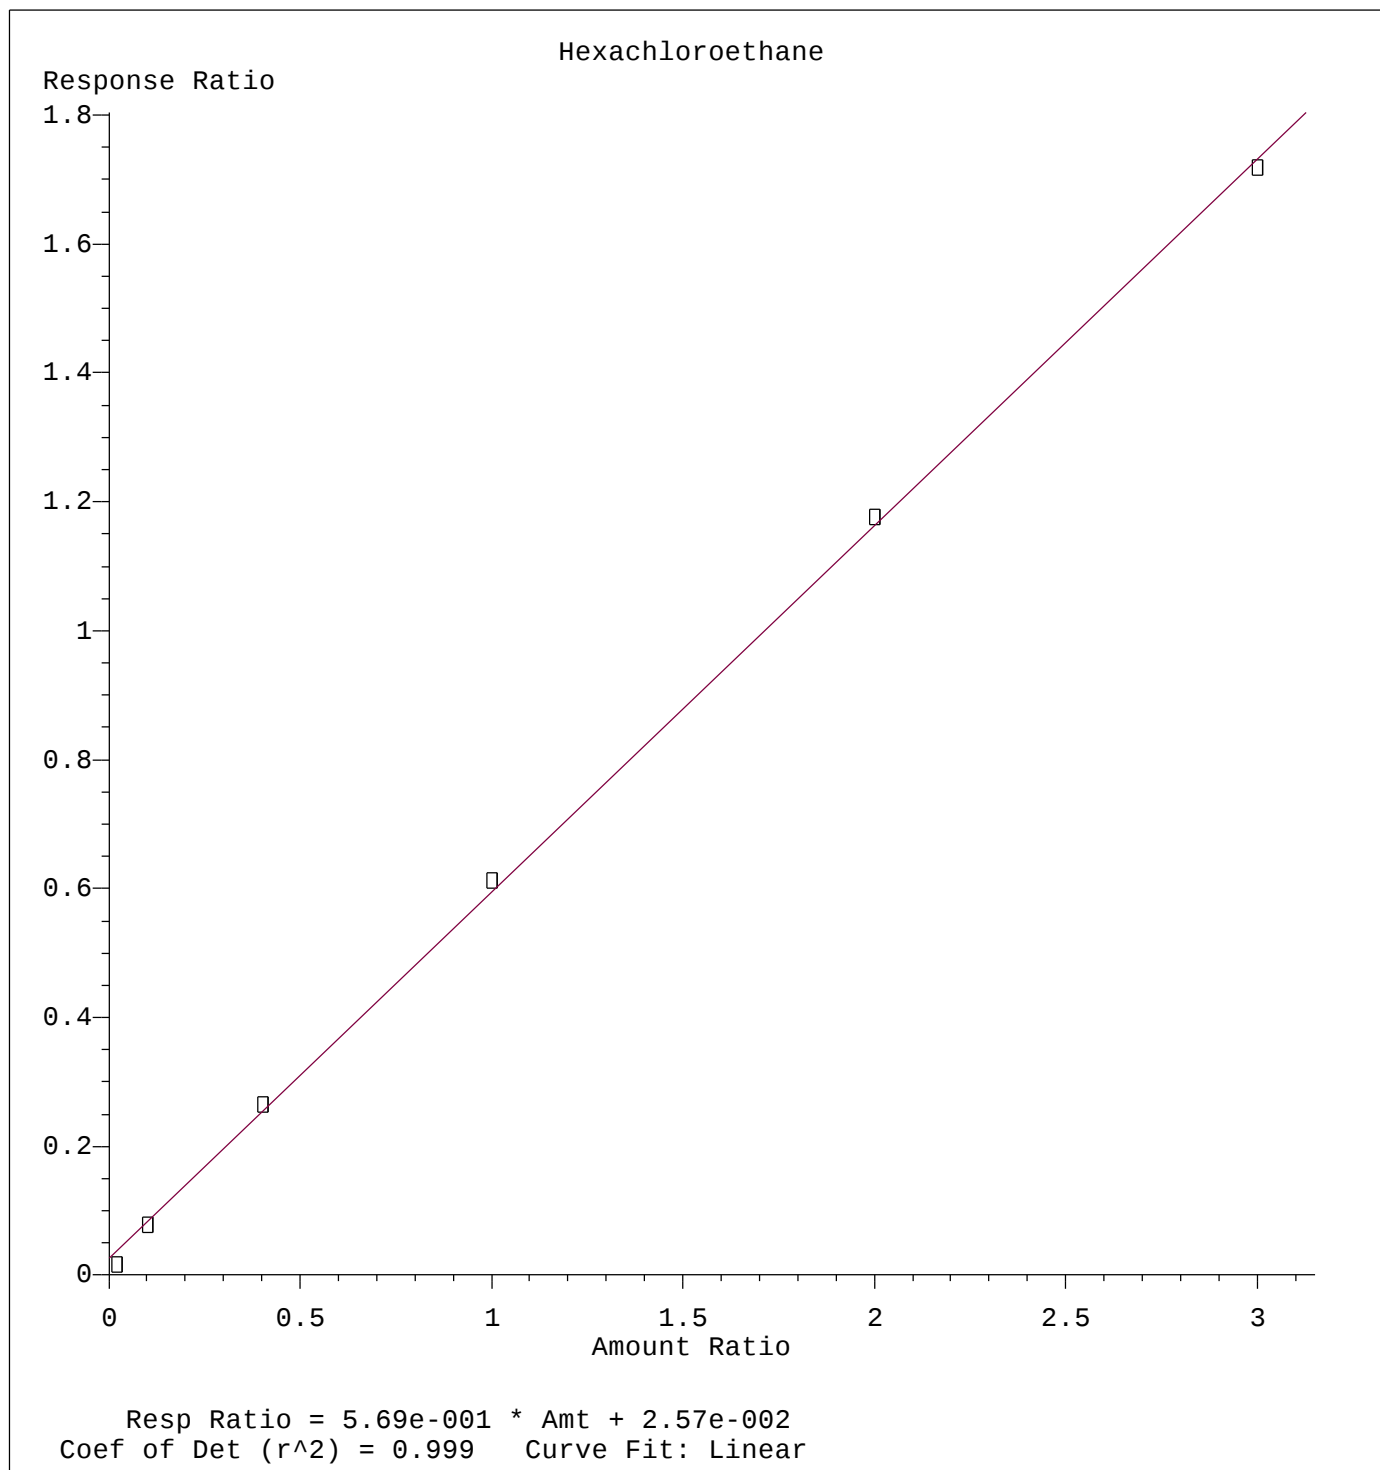

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N051719W.M
Calibration Table Last Updated: Fri May 17 23:54:12 2019

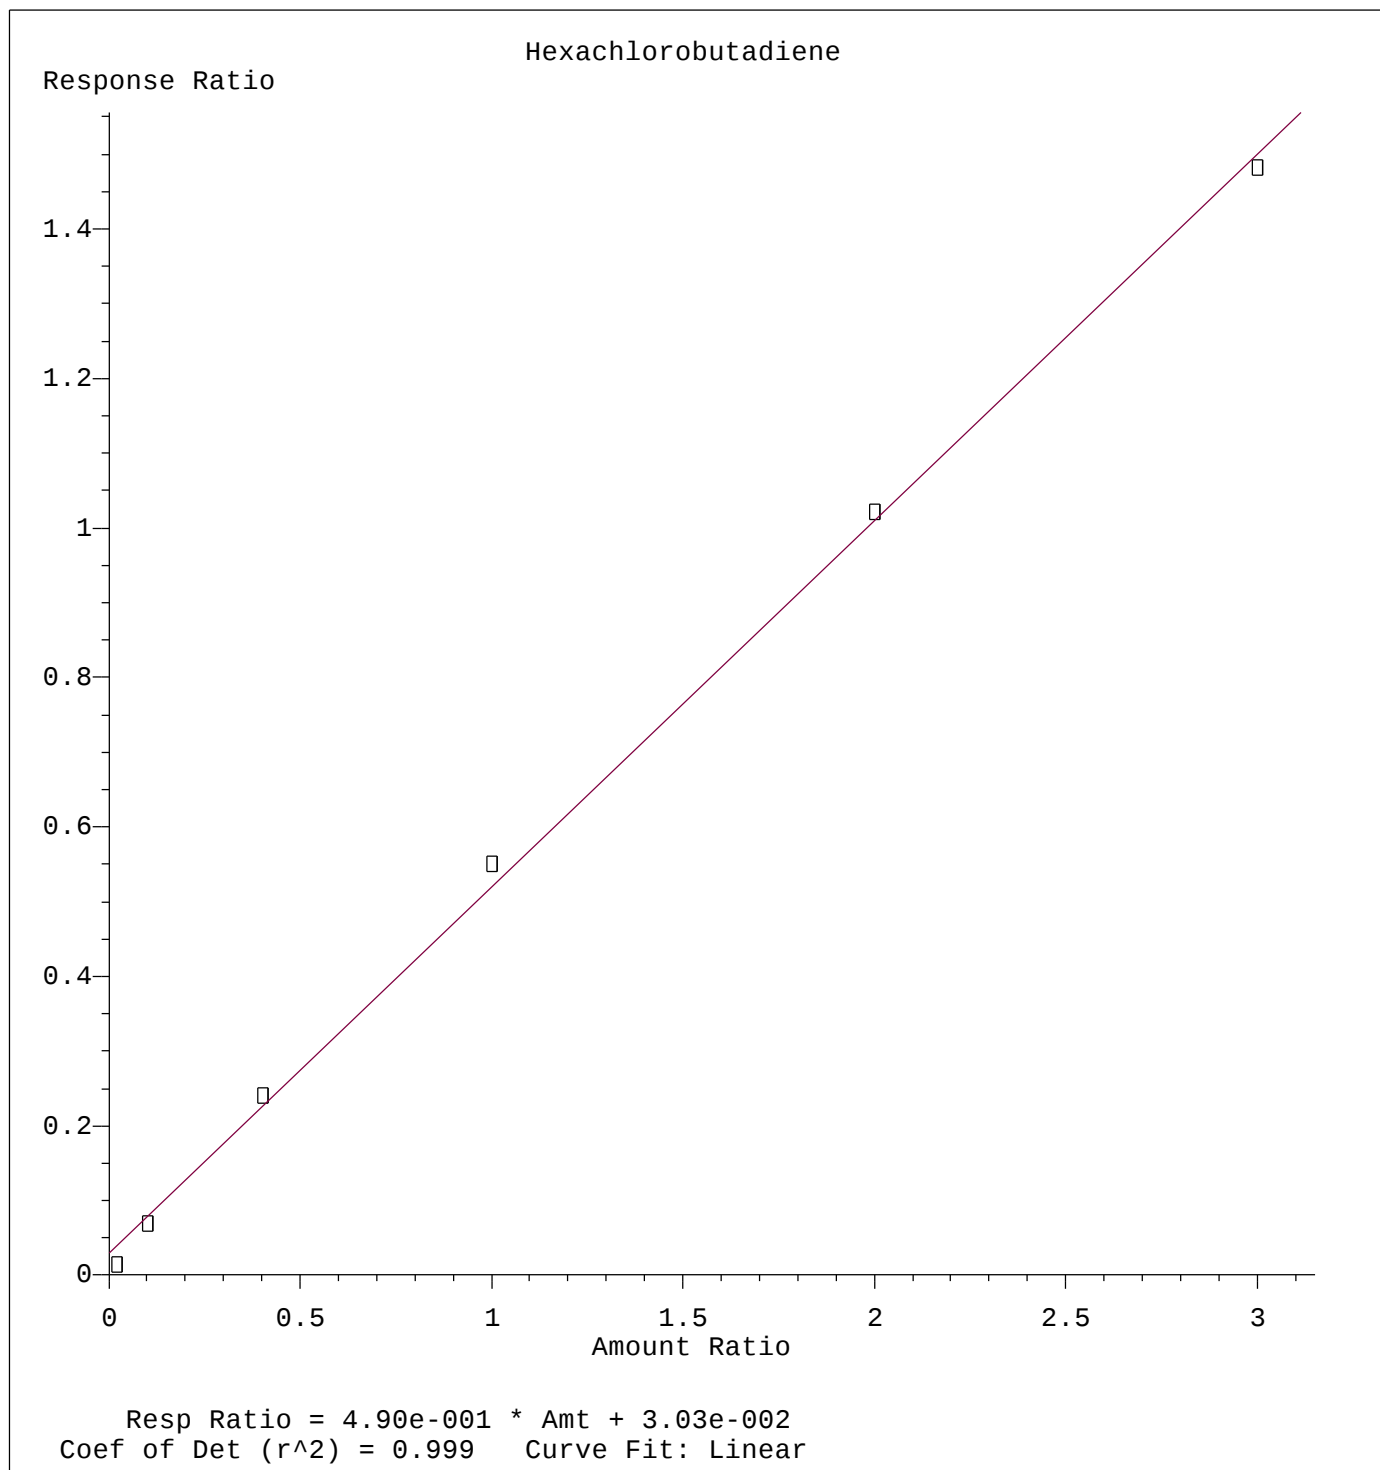


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N051719W.M
Calibration Table Last Updated: Fri May 17 23:54:12 2019

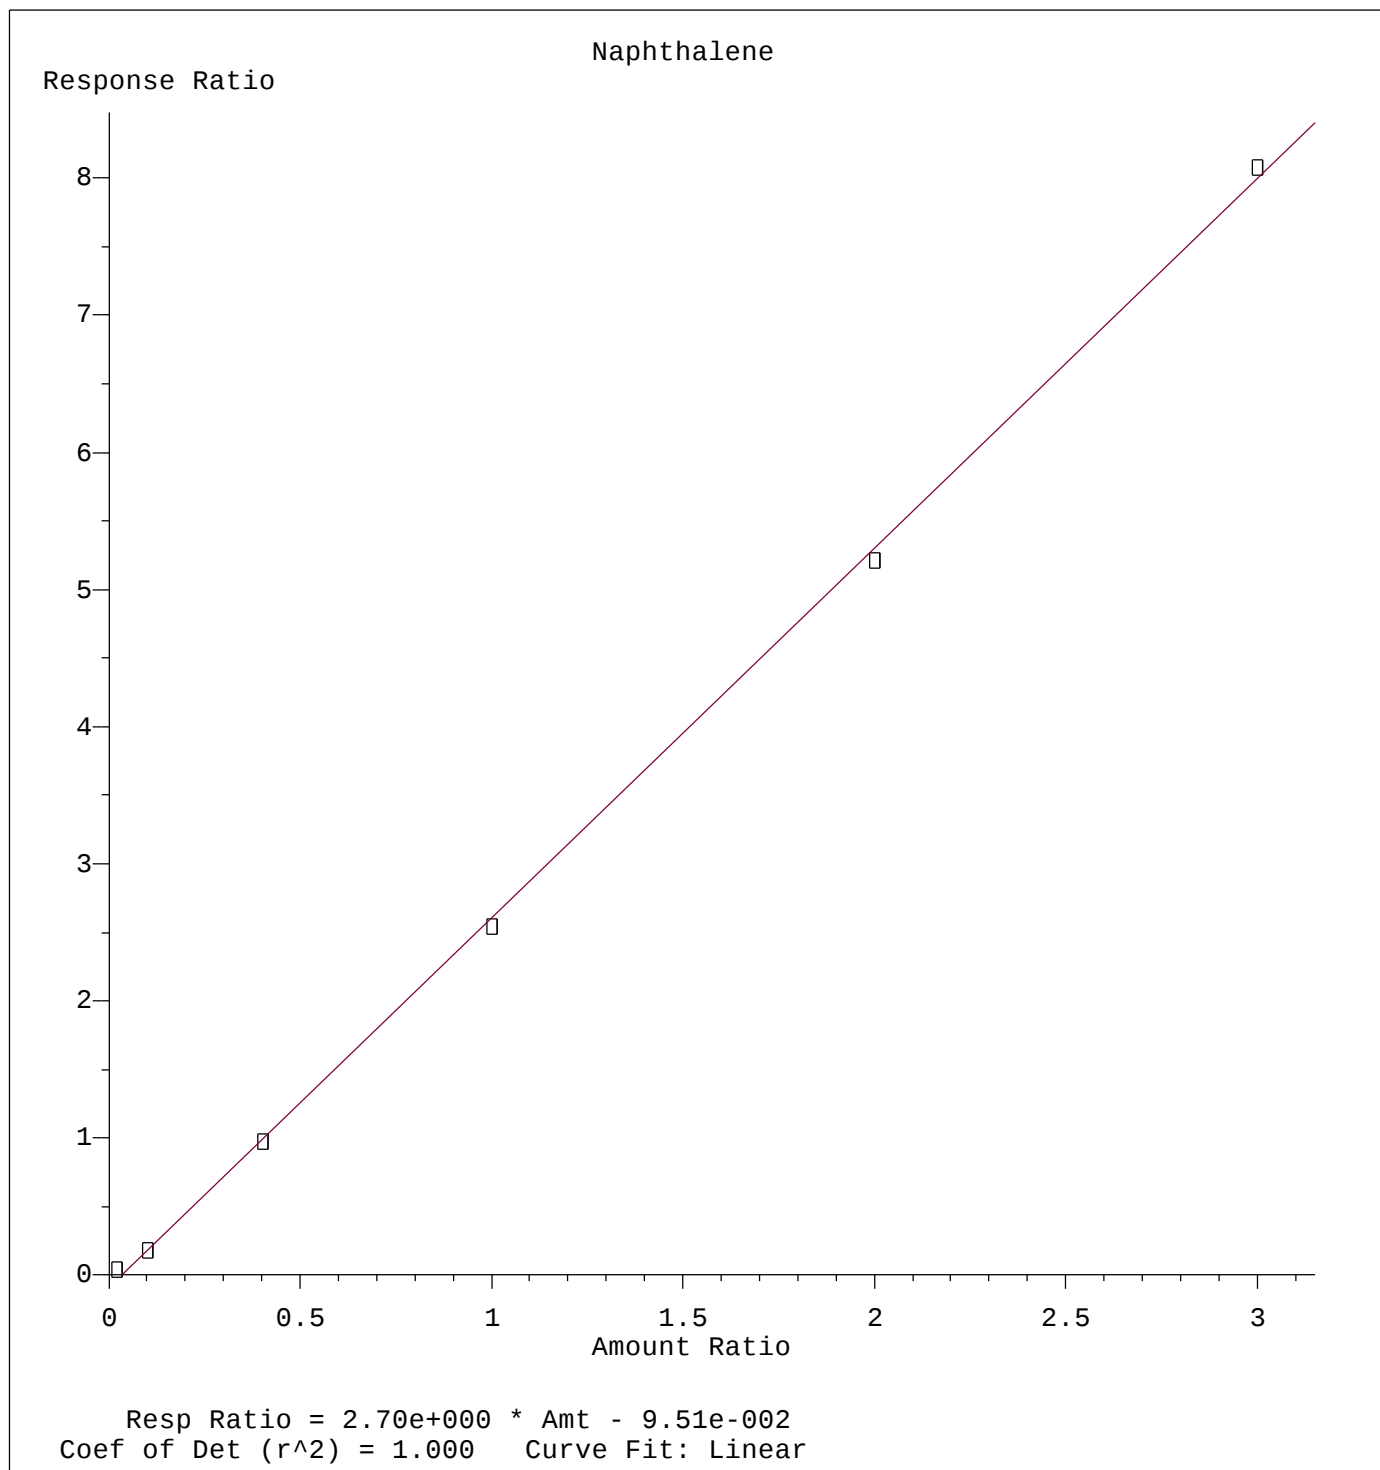

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N051719W.M
Calibration Table Last Updated: Fri May 17 23:54:12 2019

Acrolein

Response Ratio

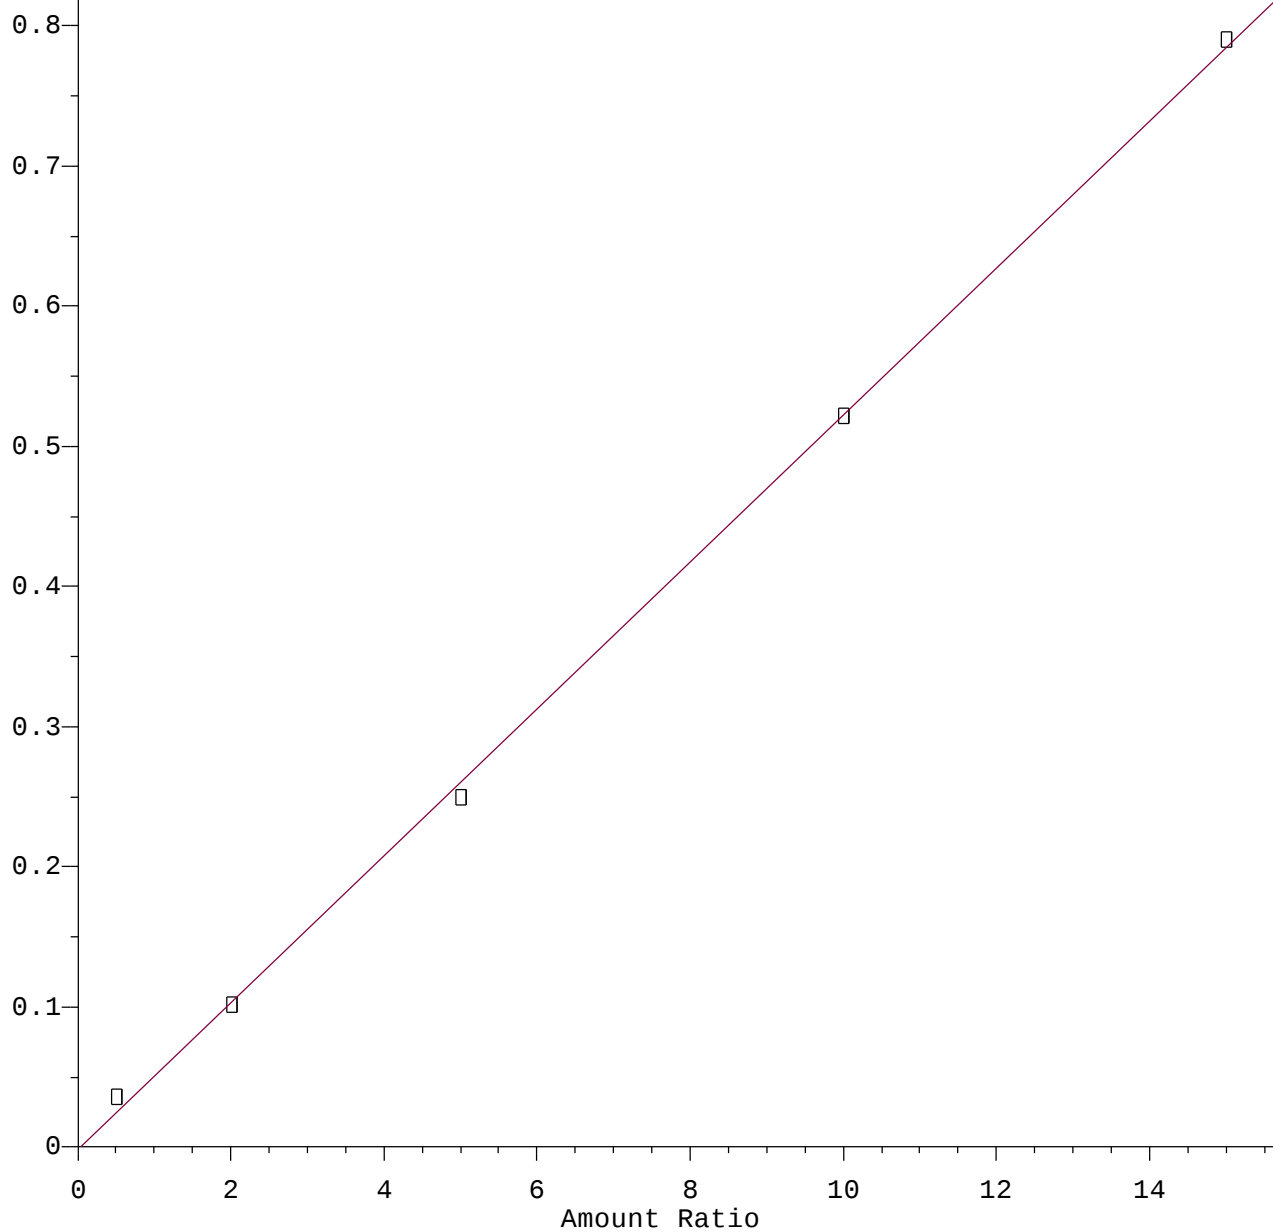

Resp Ratio = 5.24e-002 * Amt - 1.43e-003
Coef of Det (r^2) = 0.999 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N051719W.M
Calibration Table Last Updated: Fri May 17 23:54:12 2019