

Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN051719\
 Data File : VN055630.D
 Acq On : 17 May 2019 23:03
 Operator : JC/SP
 Sample : K2902-02
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 FM-EA-3MW01-051519

Quant Time: May 20 09:41:49 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N051719W.M
 Quant Title : SW846 8260
 QLast Update : Fri May 17 23:54:12 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.67	168	400097	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.59	114	563218	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.41	117	463924	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.35	152	184569	50.00	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.03	65	186591	42.54	ug/l	0.00
Spiked Amount	50.000		Recovery	=	85.08%	
35) Dibromofluoromethane	7.59	113	171654	47.98	ug/l	0.00
Spiked Amount	50.000		Recovery	=	95.96%	
50) Toluene-d8	10.09	98	647920	47.89	ug/l	0.00
Spiked Amount	50.000		Recovery	=	95.78%	
62) 4-Bromofluorobenzene	12.40	95	203483	43.56	ug/l	0.00
Spiked Amount	50.000		Recovery	=	87.12%	


Target Compounds	Qvalue
------------------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA N\DATA\VN051719\
Data File : VN055630.D
Acq On : 17 May 2019 23:03
Operator : JC/SP
Sample : K2902-02
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 35 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
FM-EA-3MW01-051519

Quant Time: May 20 09:41:49 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_N\METHODS\82N051719W.M
Quant Title : SW846 8260
QLast Update : Fri May 17 23:54:12 2019
Response via : Initial Calibration

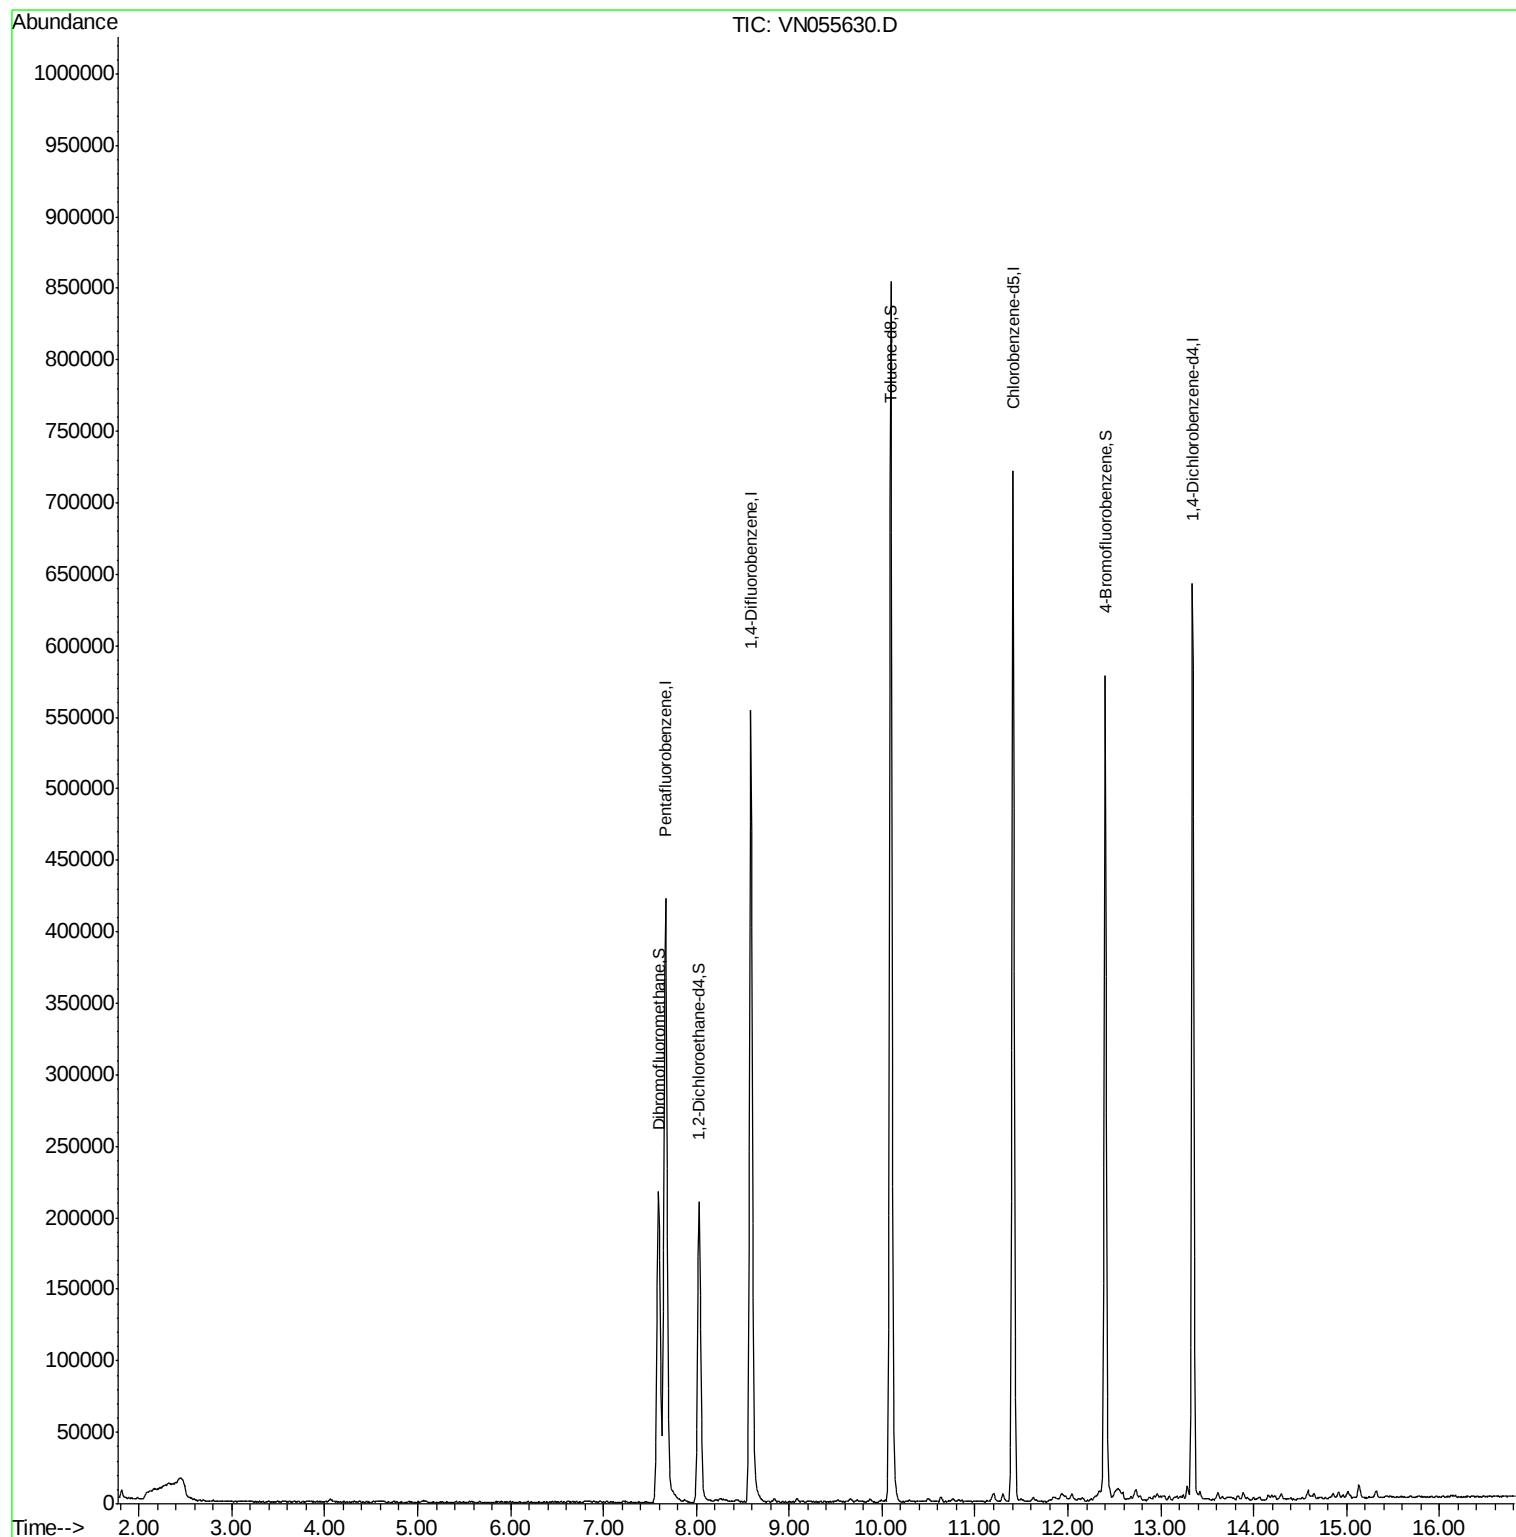



#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.67 min Scan# 1834

Delta R.T. 0.00 min

Lab File: VN055630.D

Acq: 17 May 2019 23:03

Instrument :

MSVOA_N

ClientSampleId :


FM-EA-3MW01-051519

Tot Ion:168 Resp: 400097

Ion Ratio Lower Upper




168 100

99 48.3 40.2 60.2

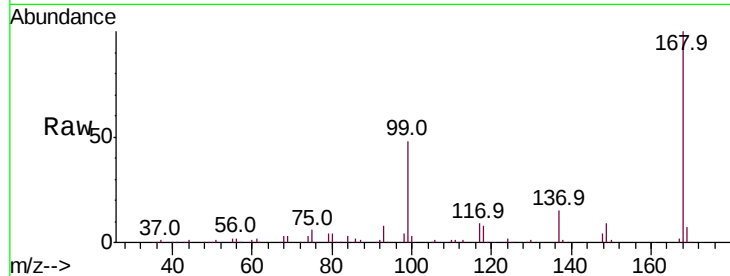

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VN0

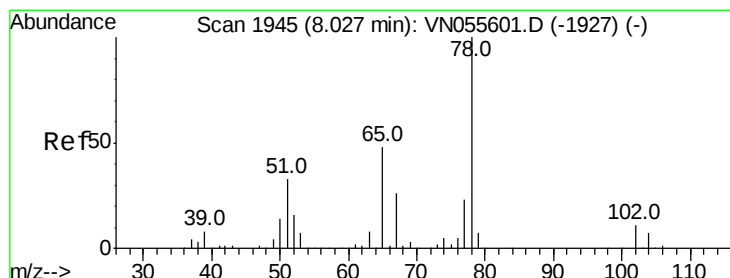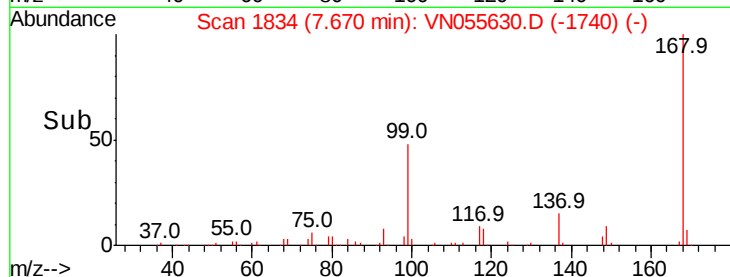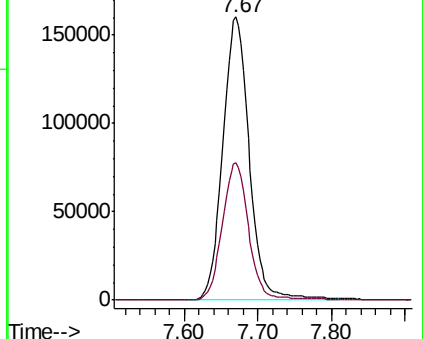

#33

1,2-Dichloroethane-d4

Concen: 42.544 ug/l

RT: 8.03 min Scan# 1946

Delta R.T. 0.00 min

Lab File: VN055630.D


Acq: 17 May 2019 23:03

Tgt Ion: 65 Resp: 186591

Ion Ratio Lower Upper



65 100


67 53.0 0.0 108.6

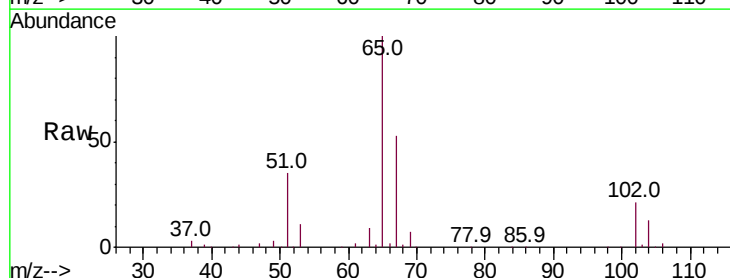

Abundance Ion 64.90 (64.60 to 65.60): VN0

Ion 66.90 (66.60 to 67.60): VN0

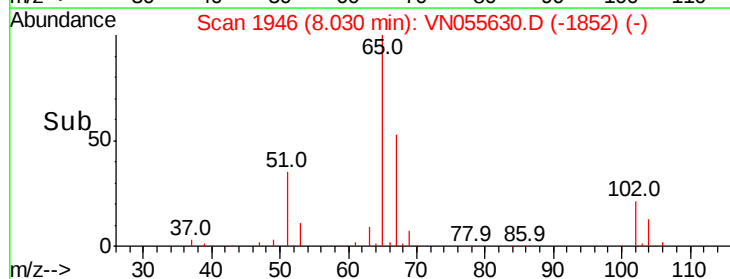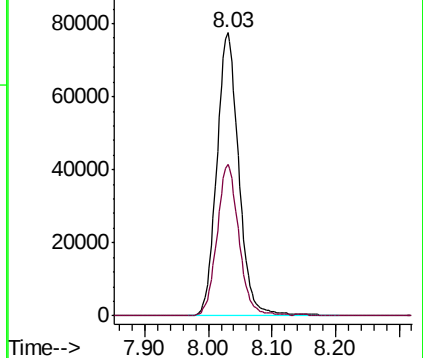

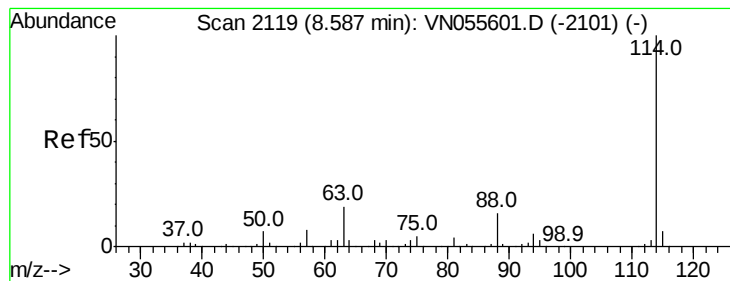

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.59 min Scan# 2119

Delta R.T. -0.00 min

Lab File: VN055630.D

Acq: 17 May 2019 23:03

Instrument :

MSVOA_N

ClientSampleId :

FM-EA-3MW01-051519


Tot Ion:114 Resp: 563218

Ion Ratio Lower Upper

114 100

63 18.5 0.0 38.2




88 15.9 0.0 31.0

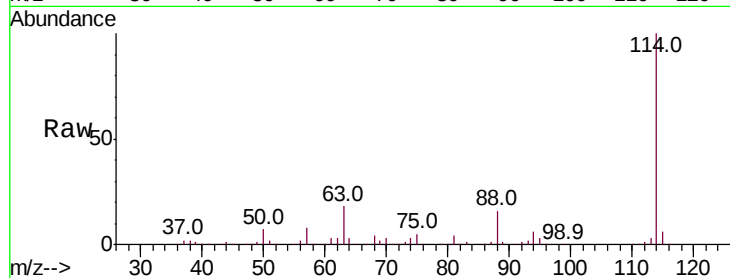

Abundance Ion 113.90 (113.60 to 114.60): V

Ion 63.00 (62.70 to 63.70): VN

Ion 87.90 (87.60 to 88.60): VN

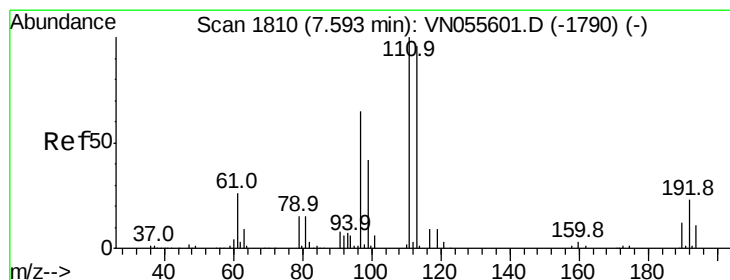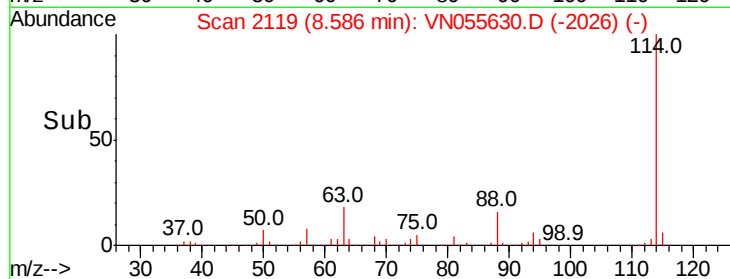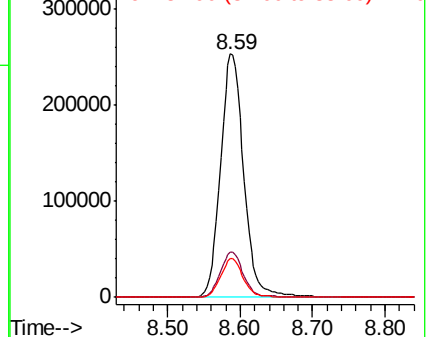

#35

Dibromofluoromethane

Concen: 47.977 ug/l

RT: 7.59 min Scan# 1810

Delta R.T. -0.00 min

Lab File: VN055630.D

Acq: 17 May 2019 23:03


Tgt Ion:113 Resp: 171654

Ion Ratio Lower Upper

113 100

111 102.1 82.5 123.7



192 23.5 18.7 28.1

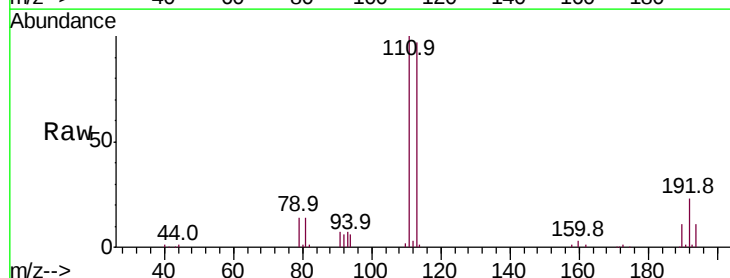


Abundance Ion 112.80 (112.50 to 113.50): V

Ion 110.80 (110.50 to 111.50): V

Ion 191.70 (191.40 to 192.40): V

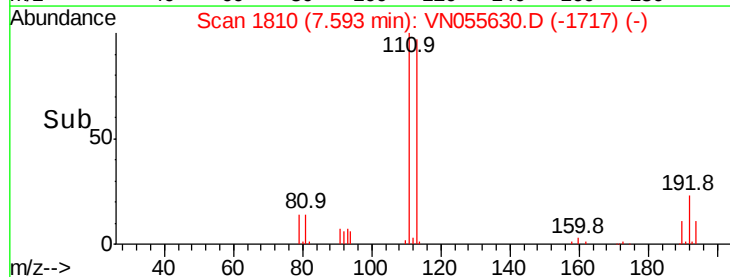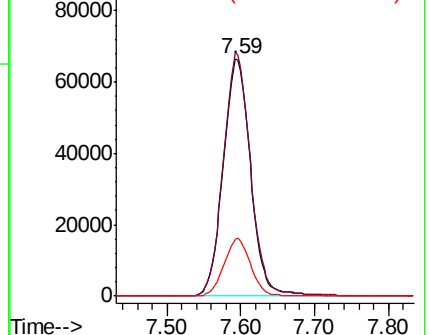

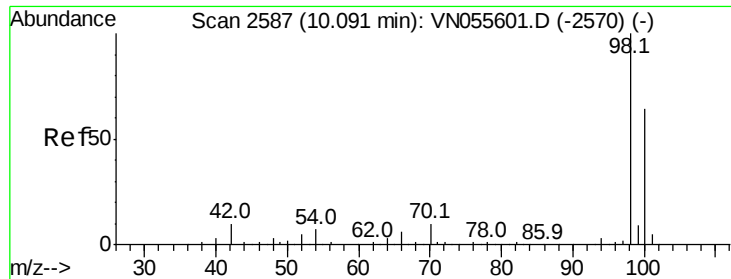

#50

Toluene-d8

Concen: 47.894 ug/l

RT: 10.09 min Scan# 2587

Delta R.T. -0.00 min

Lab File: VN055630.D

Acq: 17 May 2019 23:03

Instrument :

MSVOA_N

ClientSampleId :


FM-EA-3MW01-051519

Tot Ion: 98 Resp: 647920

Ion Ratio Lower Upper

98 100

100 64.8 51.9 77.9

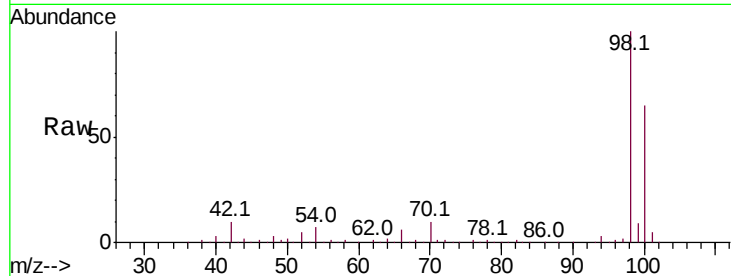

Abundance Ion 98.00 (97.70 to 98.70): VN055630.D (-2494) (-)

Ion 100.00 (99.70 to 100.70): VN055630.D (-2494) (-)

10.09



300000

200000

100000

0

Time-->

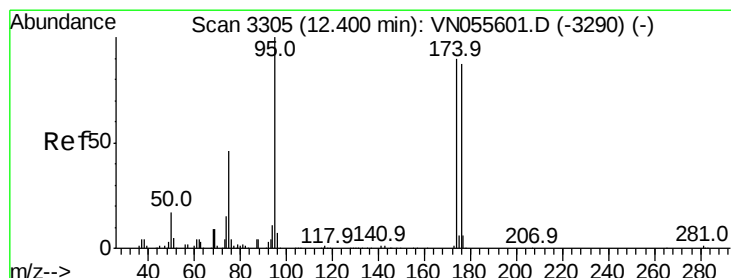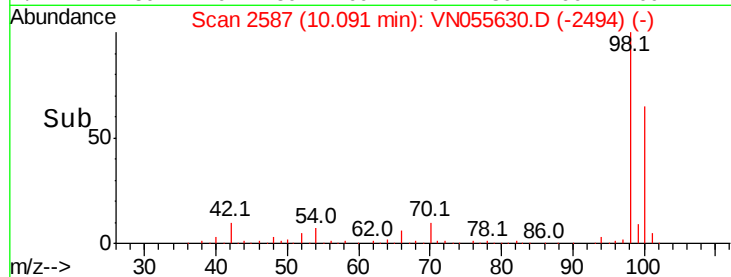

#62

4-Bromofluorobenzene

Concen: 43.559 ug/l

RT: 12.40 min Scan# 3306

Delta R.T. 0.00 min

Lab File: VN055630.D

Acq: 17 May 2019 23:03


Tgt Ion: 95 Resp: 203483

Ion Ratio Lower Upper

95 100

174 92.7 0.0 180.6

176 89.6 0.0 177.4

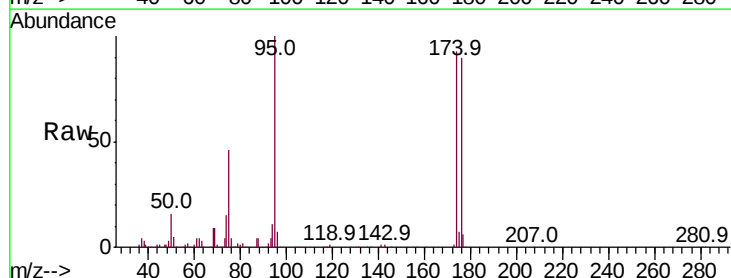

Abundance Ion 94.90 (94.60 to 95.60): VN055630.D (-3212) (-)

Ion 173.80 (173.50 to 174.50): VN055630.D (-3212) (-)

Ion 175.80 (175.50 to 176.50): VN055630.D (-3212) (-)

12.40


150000


100000

50000

0

Time-->

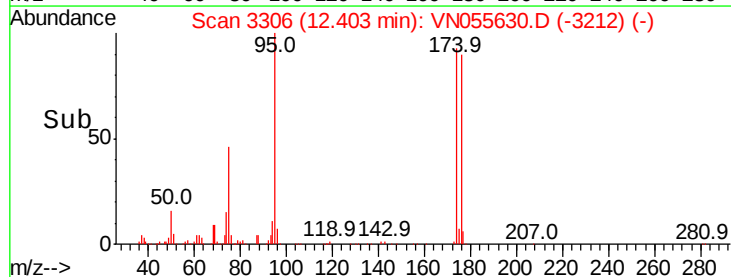


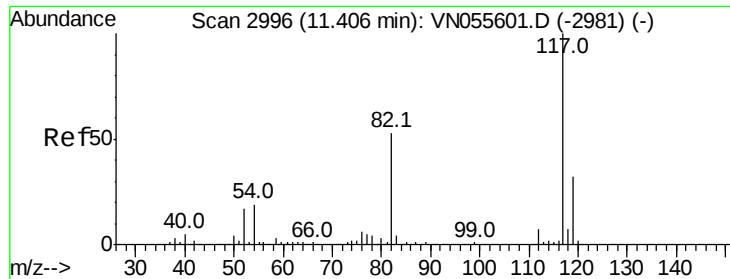




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.41 min Scan# 2997
Delta R.T. 0.00 min
Lab File: VN055630.D
Acq: 17 May 2019 23:03

Instrument :
MSVOA_N
ClientSampleId :
FM-EA-3MW01-051519

Tot Ion:117 Resp: 463924
Ion Ratio Lower Upper
117 100
82 51.6 42.3 63.5
119 32.1 25.4 38.2

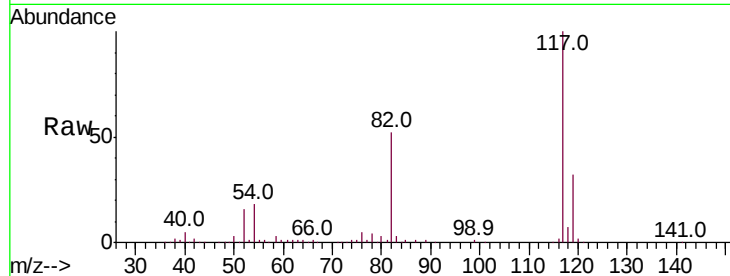


Abundance Ion 116.90 (116.60 to 117.60): V
Ion 82.00 (81.70 to 82.70): V
Ion 118.90 (118.60 to 119.60): V

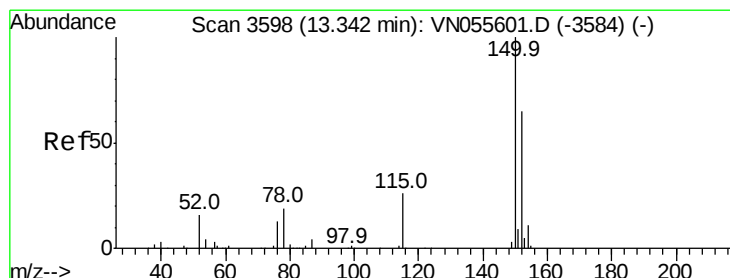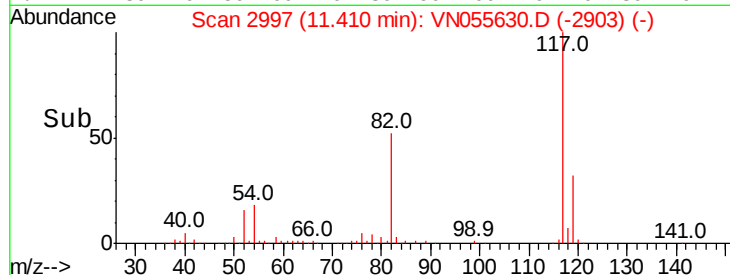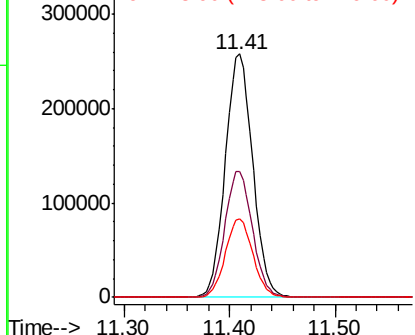

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.35 min Scan# 3599
Delta R.T. 0.00 min
Lab File: VN055630.D
Acq: 17 May 2019 23:03

Tgt Ion:152 Resp: 184569
Ion Ratio Lower Upper
152 100
115 56.0 28.1 84.2
150 157.3 0.0 348.0

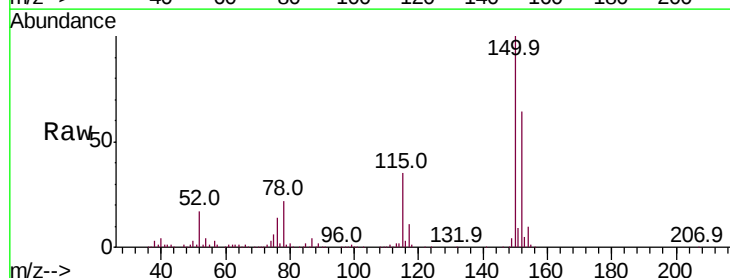

Abundance Ion 151.90 (151.60 to 152.60): V
Ion 114.90 (114.60 to 115.60): V
Ion 149.90 (149.60 to 150.60): V

