

Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN051719\
 Data File : VN055652.D
 Acq On : 18 May 2019 8:51
 Operator : JC/SP
 Sample : K2896-04
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 60 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 TP-18-S

Quant Time: May 20 03:39:25 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N051719W.M
 Quant Title : SW846 8260
 QLast Update : Fri May 17 23:54:12 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.67	168	431991	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.59	114	615468	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.41	117	536217	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.34	152	238388	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.03	65	200815	42.41	ug/l	0.00
Spiked Amount 50.000			Recovery	=	84.82%	
35) Dibromofluoromethane	7.59	113	188359	48.18	ug/l	0.00
Spiked Amount 50.000			Recovery	=	96.36%	
50) Toluene-d8	10.09	98	715635	48.41	ug/l	0.00
Spiked Amount 50.000			Recovery	=	96.82%	
62) 4-Bromofluorobenzene	12.40	95	245792	48.15	ug/l	0.00
Spiked Amount 50.000			Recovery	=	96.30%	
Target Compounds						
16) Acetone	3.82	43	12744	6.594	ug/l	99
20) Methylene Chloride	4.55	84	4762	1.080	ug/l	98
43) Isopropyl Acetate	8.17	43	18871	2.191	ug/l #	82
95) Naphthalene	15.13	128	26732	3.845	ug/l	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA N\DATA\VN051719\
Data File : VN055652.D
Acq On : 18 May 2019 8:51
Operator : JC/SP
Sample : K2896-04
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 60 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
TP-18-S

Quant Time: May 20 03:39:25 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_N\METHODS\82N051719W.M
Quant Title : SW846 8260
QLast Update : Fri May 17 23:54:12 2019
Response via : Initial Calibration

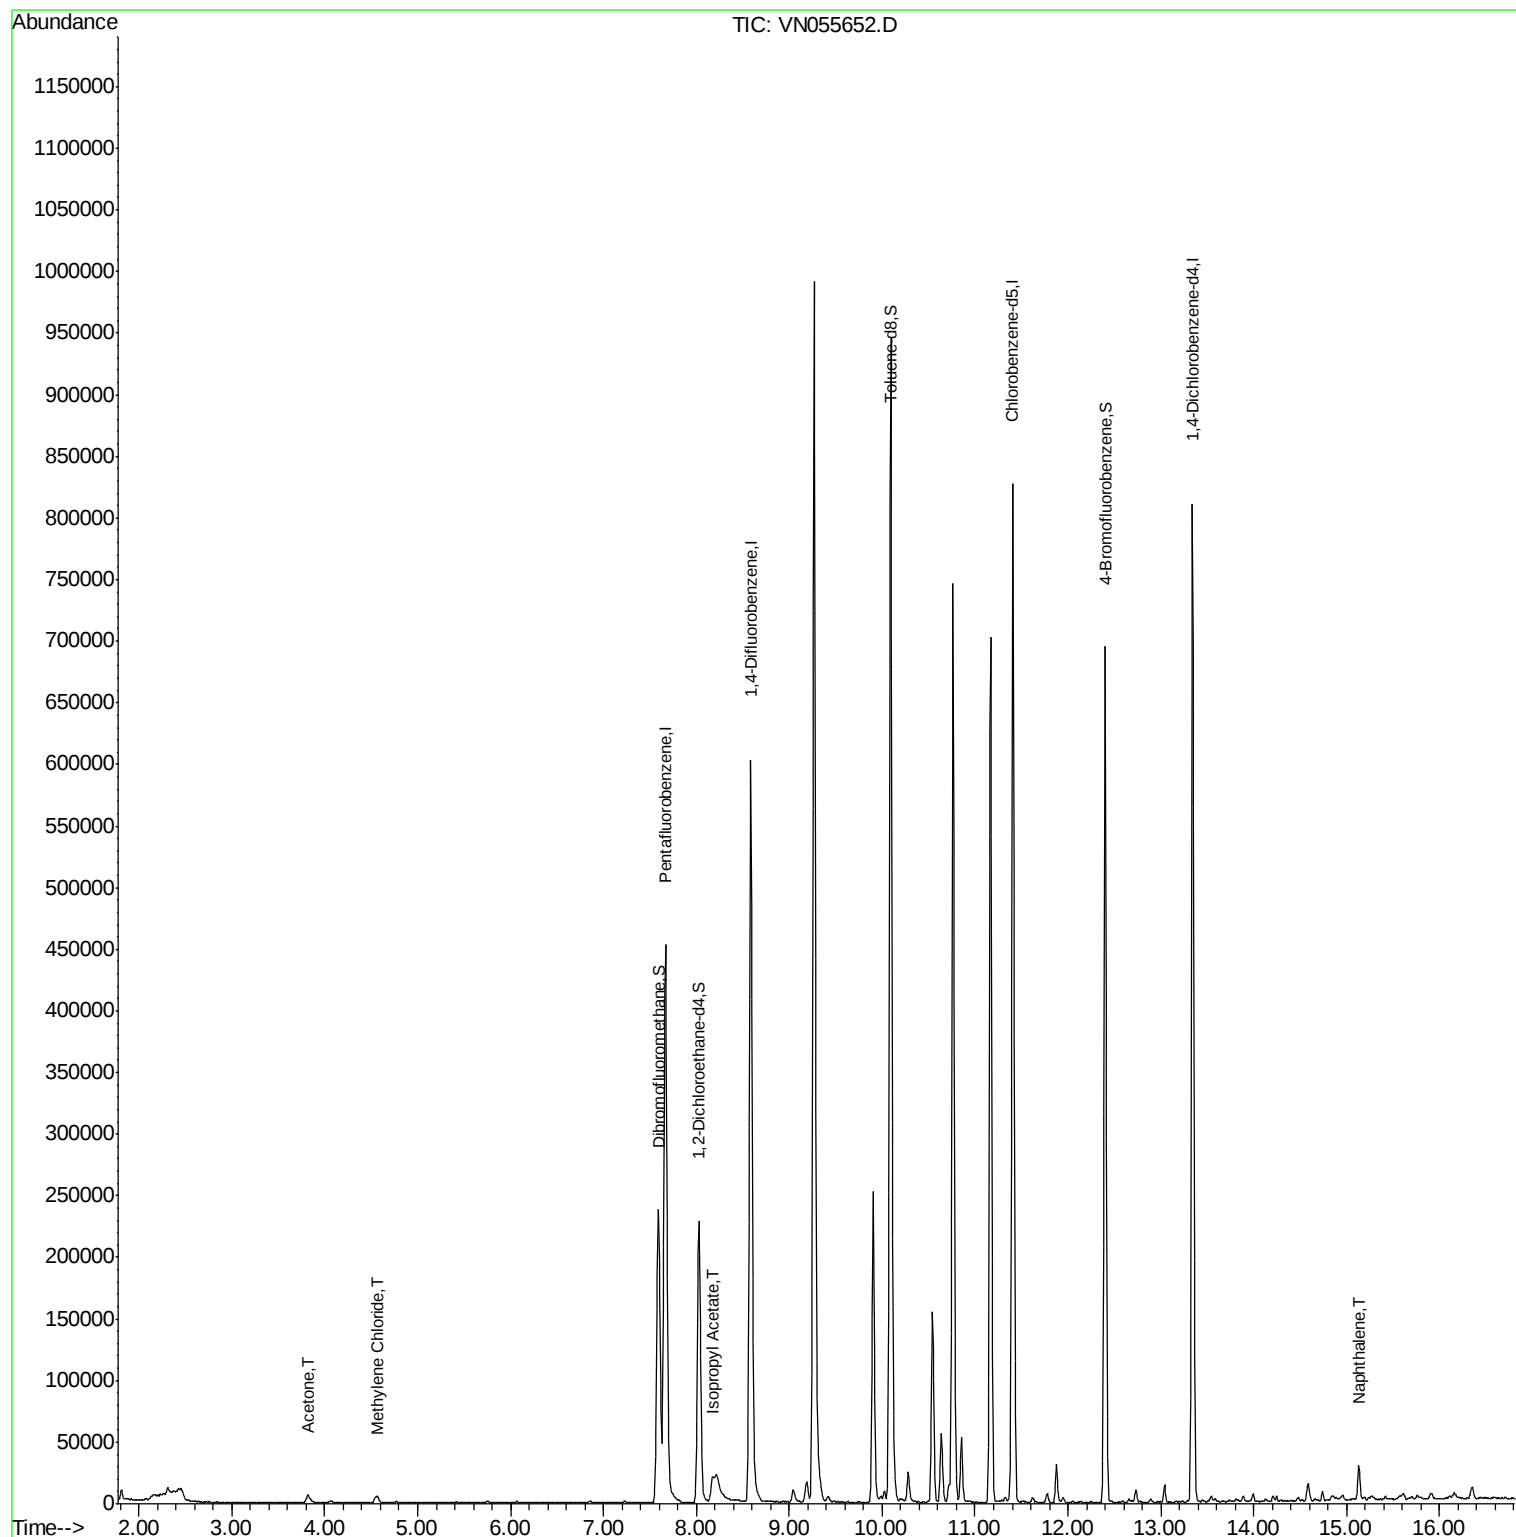



#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.67 min Scan# 1833

Delta R.T. -0.00 min

Lab File: VN055652.D

Acq: 18 May 2019 8:51

Instrument :

MSVOA_N

ClientSampled :


TP-18-S

Tot Ion:168 Resp: 431991

Ion Ratio Lower Upper

168 100

99 48.2 40.2 60.2



Abundance Ion 167.90 (167.60 to 168.60): VN055601.D (-1813) (-)

Ion 98.90 (98.60 to 99.60): VN055601.D (-1813) (-)

7.67



150000

100000

50000

0

Time--> 7.50 7.60 7.70 7.80 7.90



#16

Acetone

Concen: 6.594 ug/l

RT: 3.82 min Scan# 636

Delta R.T. 0.01 min

Lab File: VN055652.D


Acq: 18 May 2019 8:51

Tgt Ion: 43 Resp: 12744

Ion Ratio Lower Upper

43 100

58 31.8 26.0 39.0



Abundance Ion 43.00 (42.70 to 43.70): VN055601.D (-607) (-)

Ion 58.00 (57.70 to 58.70): VN055601.D (-607) (-)

3.82

4000


3000


2000

1000

0

Time--> 3.70 3.80 3.90



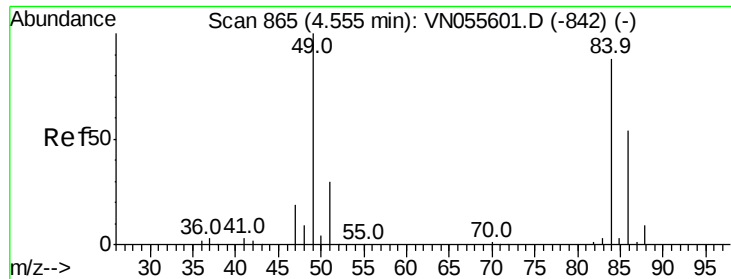

#20

Methvlene Chloride

Concen: 1.080 ug/l

RT: 4.55 min Scan# 865

Delta R.T. -0.00 min

Lab File: VN055652.D

Acq: 18 May 2019 8:51

Instrument :

MSVOA_N

ClientSampled :

TP-18-S

Tot Ion: 84 Resp: 4762


Ion Ratio Lower Upper

84 100

49 112.1 91.0 136.4

51 32.2 27.5 41.3

86 59.7 49.4 74.0



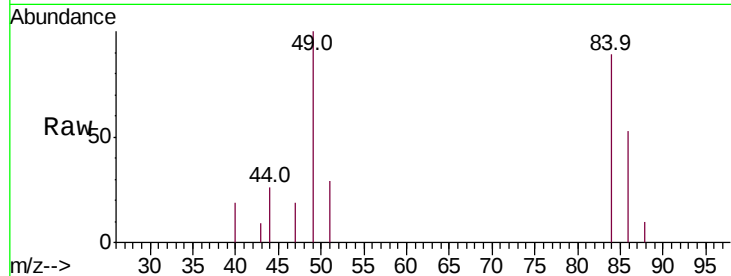


Abundance Ion 83.90 (83.60 to 84.60): VNO

Ion 48.90 (48.60 to 49.60): VNO

Ion 50.90 (50.60 to 51.60): VNO

Ion 85.90 (85.60 to 86.60): VNO

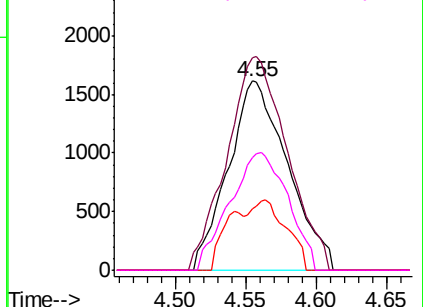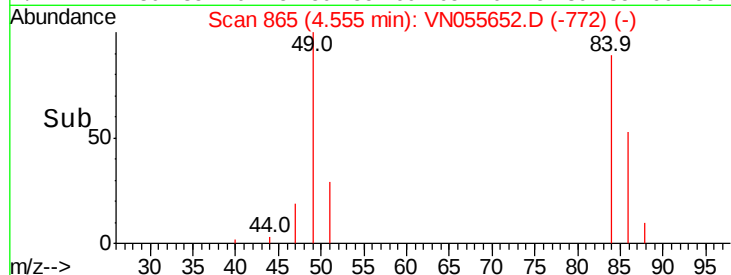

#33

1,2-Dichloroethane-d4

Concen: 42.406 ug/l

RT: 8.03 min Scan# 1945

Delta R.T. -0.00 min

Lab File: VN055652.D


Acq: 18 May 2019 8:51

Tgt Ion: 65 Resp: 200815

Ion Ratio Lower Upper



65 100


67 54.7 0.0 108.6



Abundance Ion 64.90 (64.60 to 65.60): VNO

Ion 66.90 (66.60 to 67.60): VNO

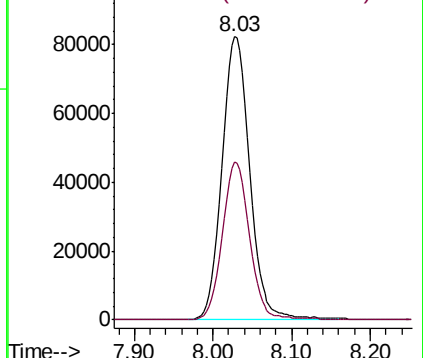


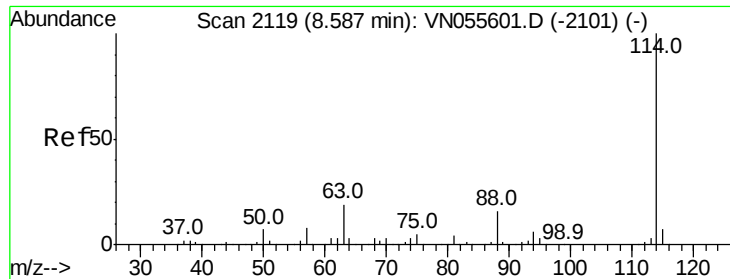




#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 8.59 min Scan# 2119
 Delta R.T. -0.00 min
 Lab File: VN055652.D
 Acq: 18 May 2019 8:51

Instrument :
 MSVOA_N
 ClientSampleId :
 TP-18-S

Tot Ion	Ratio	Lower	Upper
114	100		
63	18.6	0.0	38.2
88	15.4	0.0	31.0

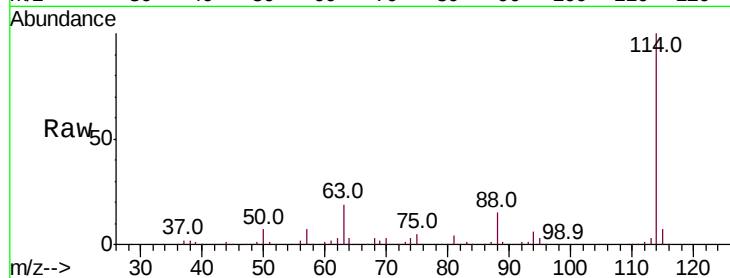


Abundance Ion 113.90 (113.60 to 114.60): V
 Ion 63.00 (62.70 to 63.70): VN
 Ion 87.90 (87.60 to 88.60): VN

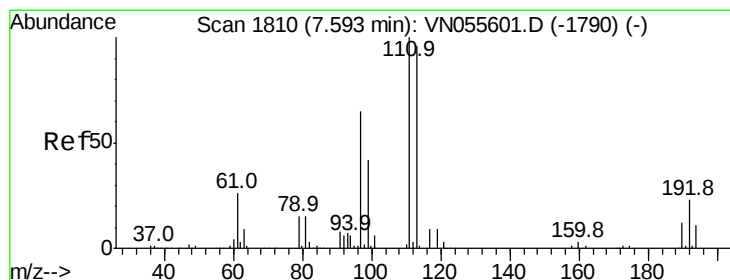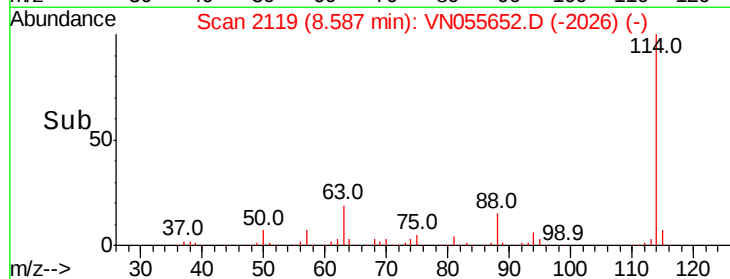
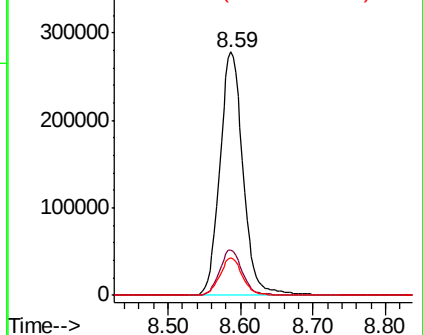



#35
 Dibromofluoromethane
 Concen: 48.177 ug/l
 RT: 7.59 min Scan# 1810
 Delta R.T. -0.00 min
 Lab File: VN055652.D
 Acq: 18 May 2019 8:51

Tgt Ion	Ratio	Lower	Upper
113	100		
111	102.3	82.5	123.7
192	24.0	18.7	28.1

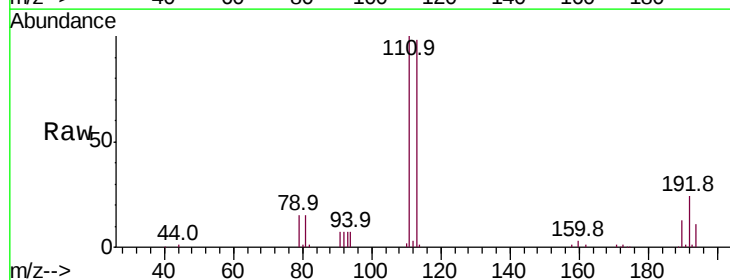

Abundance Ion 112.80 (112.50 to 113.50): V
 Ion 110.80 (110.50 to 111.50): V
 Ion 191.70 (191.40 to 192.40): V

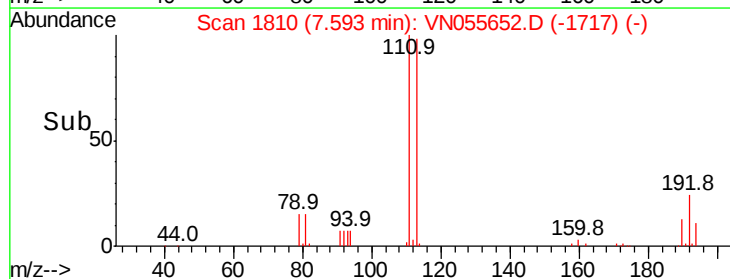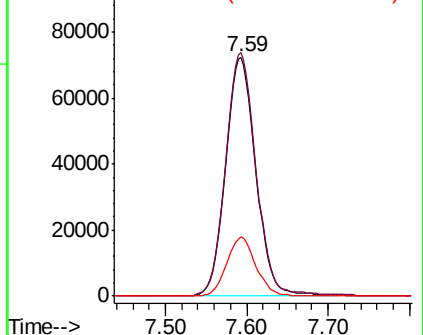



#43

Isopropyl Acetate

Concen: 2.191 ug/l

RT: 8.17 min Scan# 1991

Delta R.T. 0.01 min

Lab File: VN055652.D

Acq: 18 May 2019 8:51

Instrument :

MSVOA_N

ClientSampleId :

TP-18-S


Tot Ion: 43 Resp: 18871

Ion Ratio Lower Upper

43 100

61 16.3 22.1 33.1#




87 9.8 11.8 17.6#

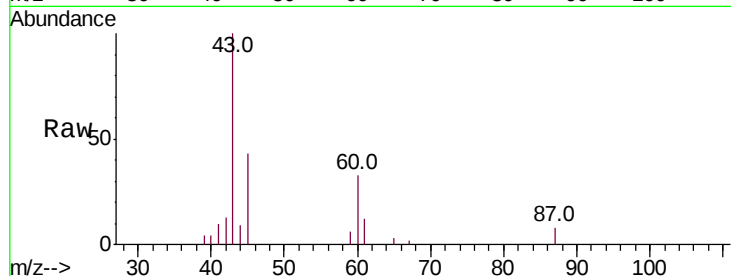

Abundance Ion 43.00 (42.70 to 43.70): VN0

Ion 61.00 (60.70 to 61.70): VN0

Ion 87.00 (86.70 to 87.70): VN0

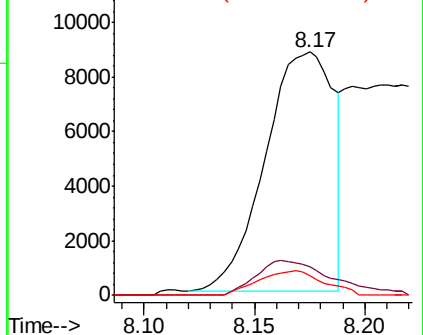

#50

Toluene-d8

Concen: 48.409 ug/l

RT: 10.09 min Scan# 2587

Delta R.T. -0.00 min

Lab File: VN055652.D


Acq: 18 May 2019 8:51

Tgt Ion: 98 Resp: 715635

Ion Ratio Lower Upper



98 100


100 64.6 51.9 77.9



Abundance Ion 98.00 (97.70 to 98.70): VN0

Ion 100.00 (99.70 to 100.70): VN0

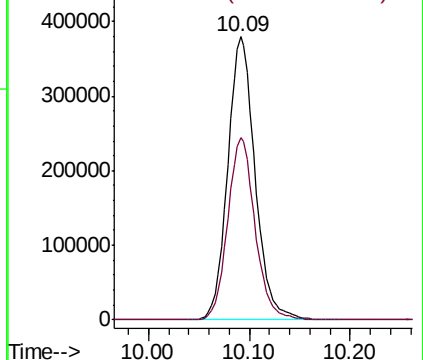



#62

4-Bromofluorobenzene

Concen: 48.149 ug/l

RT: 12.40 min Scan# 3305

Delta R.T. -0.00 min

Lab File: VN055652.D

Acq: 18 May 2019 8:51

Instrument :

MSVOA_N

ClientSampleId :

TP-18-S


Tot Ion: 95 Resp: 245792

Ion Ratio Lower Upper

95 100

174 93.5 0.0 180.6




176 90.6 0.0 177.4

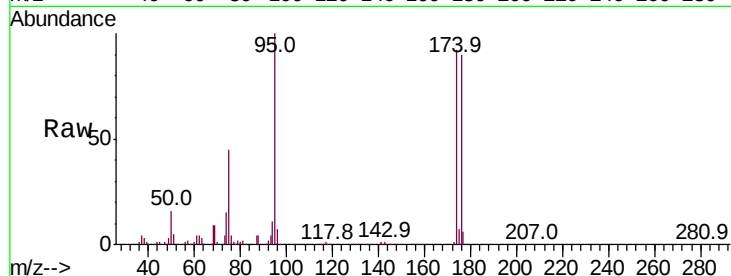

Abundance Ion 94.90 (94.60 to 95.60): VN055601.D (-3290) (-)

200000 Ion 173.80 (173.50 to 174.50): VN055601.D (-3290) (-)

150000 Ion 175.80 (175.50 to 176.50): VN055601.D (-3290) (-)

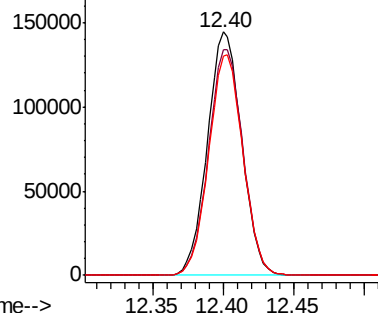

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 11.41 min Scan# 2996

Delta R.T. -0.00 min

Lab File: VN055652.D

Acq: 18 May 2019 8:51


Tgt Ion: 117 Resp: 536217

Ion Ratio Lower Upper

117 100

82 51.1 42.3 63.5



119 32.2 25.4 38.2




Abundance Ion 116.90 (116.60 to 117.60): VN055601.D (-2981) (-)

400000 Ion 82.00 (81.70 to 82.70): VN055601.D (-2981) (-)

300000 Ion 118.90 (118.60 to 119.60): VN055601.D (-2981) (-)

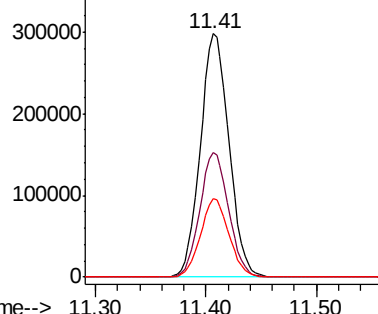

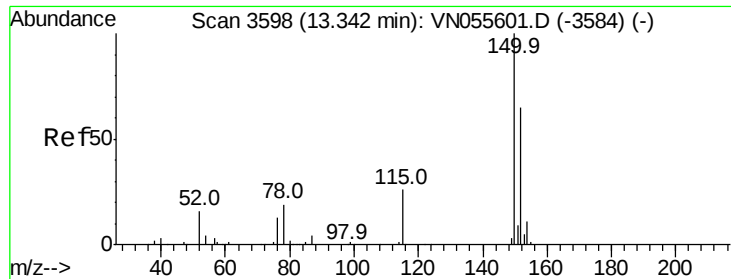

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.34 min Scan# 3598

Delta R.T. -0.00 min

Lab File: VN055652.D

Acq: 18 May 2019 8:51

Instrument :

MSVOA_N

ClientSampleId :

TP-18-S


Tot Ion:152 Resp: 238388

Ion Ratio Lower Upper

152 100

115 55.3 28.1 84.2




150 155.2 0.0 348.0

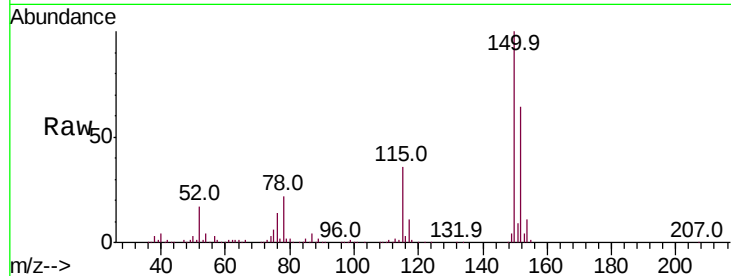

Abundance Ion 151.90 (151.60 to 152.60): V

Ion 114.90 (114.60 to 115.60): V

Ion 149.90 (149.60 to 150.60): V

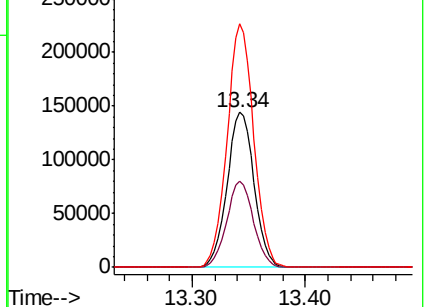

#95

Naphthalene

Concen: 3.845 ug/l

RT: 15.13 min Scan# 4155

Delta R.T. 0.00 min

Lab File: VN055652.D

Acq: 18 May 2019 8:51


Tgt Ion:128 Resp: 26732

Ion Ratio Lower Upper

128 100

127 13.2 10.2 15.4

129 10.6 8.6 12.8



Abundance Ion 128.00 (127.70 to 128.70): V

Ion 127.00 (126.70 to 127.70): V

Ion 129.00 (128.70 to 129.70): V

