


Data Path : Z:\voasrv\HPCHEM1\MSVOA N\Data\VN051719\
Data File : VN055597.D
Acq On : 17 May 2019 8:33
Operator : JC/SP
Sample : BFB
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N051719W.M
Title : SW846 8260
Last Update : Fri May 17 23:54:12 2019

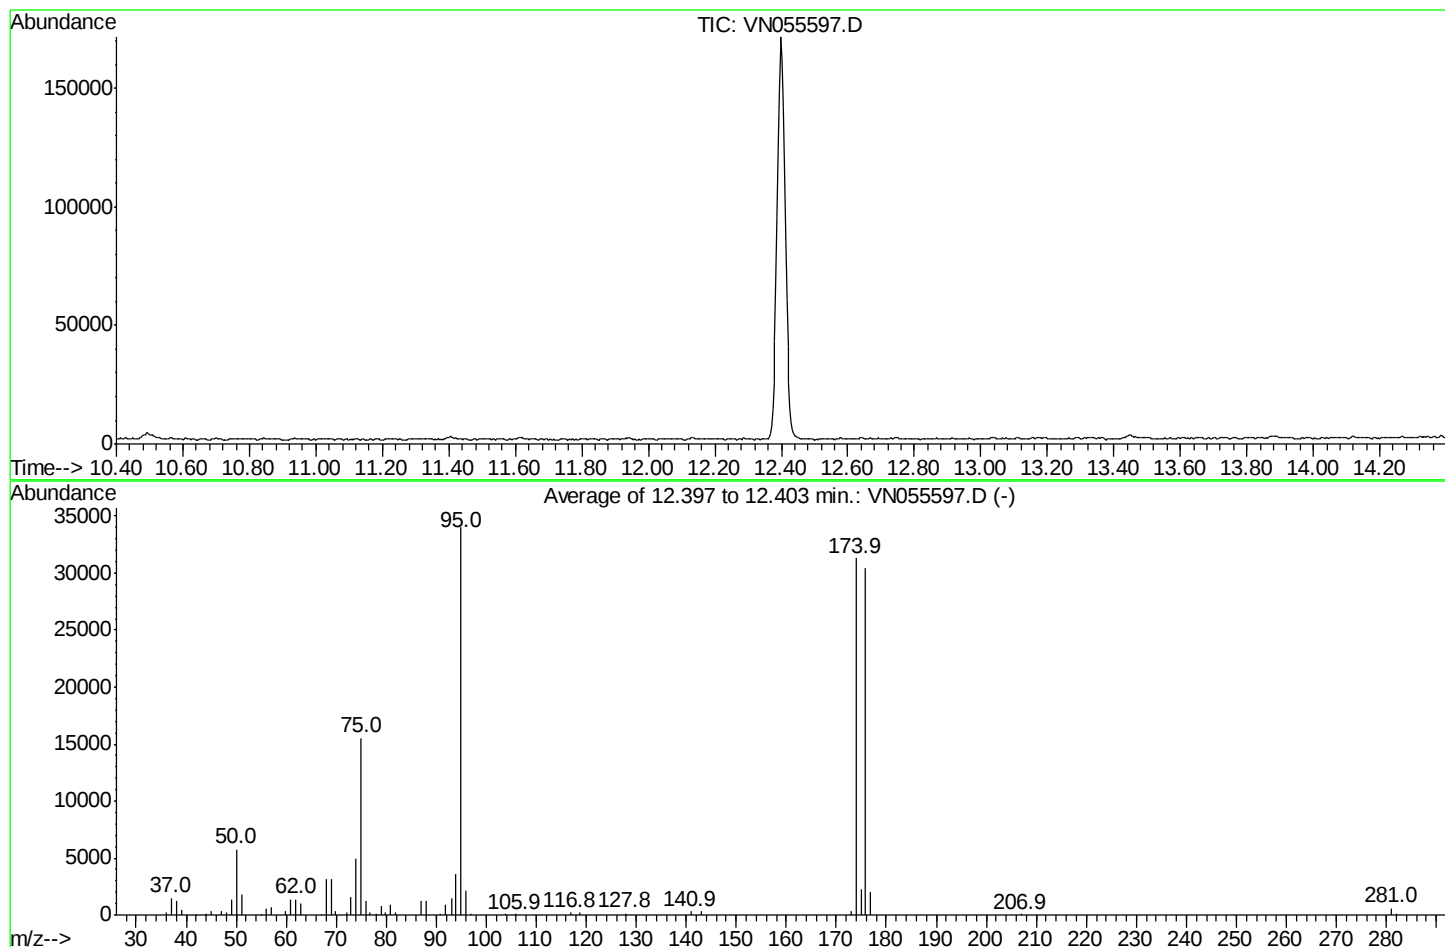

AutoFind: Scans 3304, 3305, 3306; Background Corrected with Scan 3290

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.0	5776	PASS
75	95	30	60	45.7	15545	PASS
95	95	100	100	100.0	34024	PASS
96	95	5	9	6.4	2183	PASS
173	174	0.00	2	1.1	343	PASS
174	95	50	100	92.0	31309	PASS
175	174	5	9	7.1	2208	PASS
176	174	95	101	97.2	30442	PASS
177	176	5	9	6.8	2058	PASS