


Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN051719\
 Data File : VN055605.D
 Acq On : 17 May 2019 12:32
 Operator : JC/SP
 Sample : BFB
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N051719W.M
 Title : SW846 8260
 Last Update : Fri May 17 23:54:12 2019

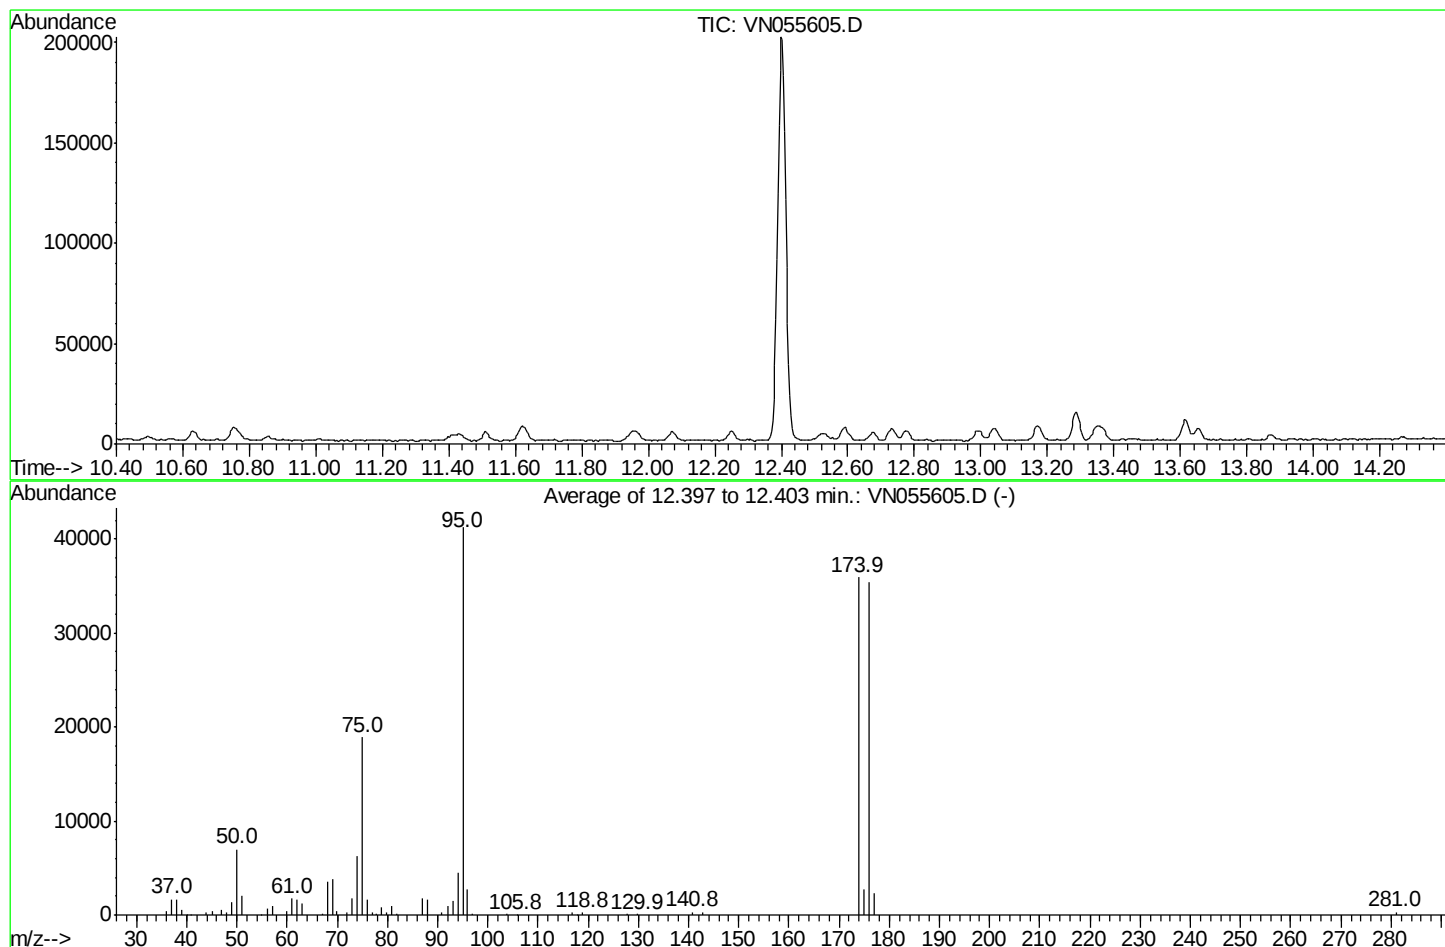

AutoFind: Scans 3304, 3305, 3306; Background Corrected with Scan 3291

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.8	6947	PASS
75	95	30	60	45.8	18901	PASS
95	95	100	100	100.0	41232	PASS
96	95	5	9	6.8	2793	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	87.1	35912	PASS
175	174	5	9	7.6	2738	PASS
176	174	95	101	98.5	35386	PASS
177	176	5	9	6.6	2340	PASS