


Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN051719\
Data File : VN055634.D
Acq On : 18 May 2019 1:01
Operator : JC/SP
Sample : BFB
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N051719W.M
Title : SW846 8260
Last Update : Fri May 17 23:54:12 2019

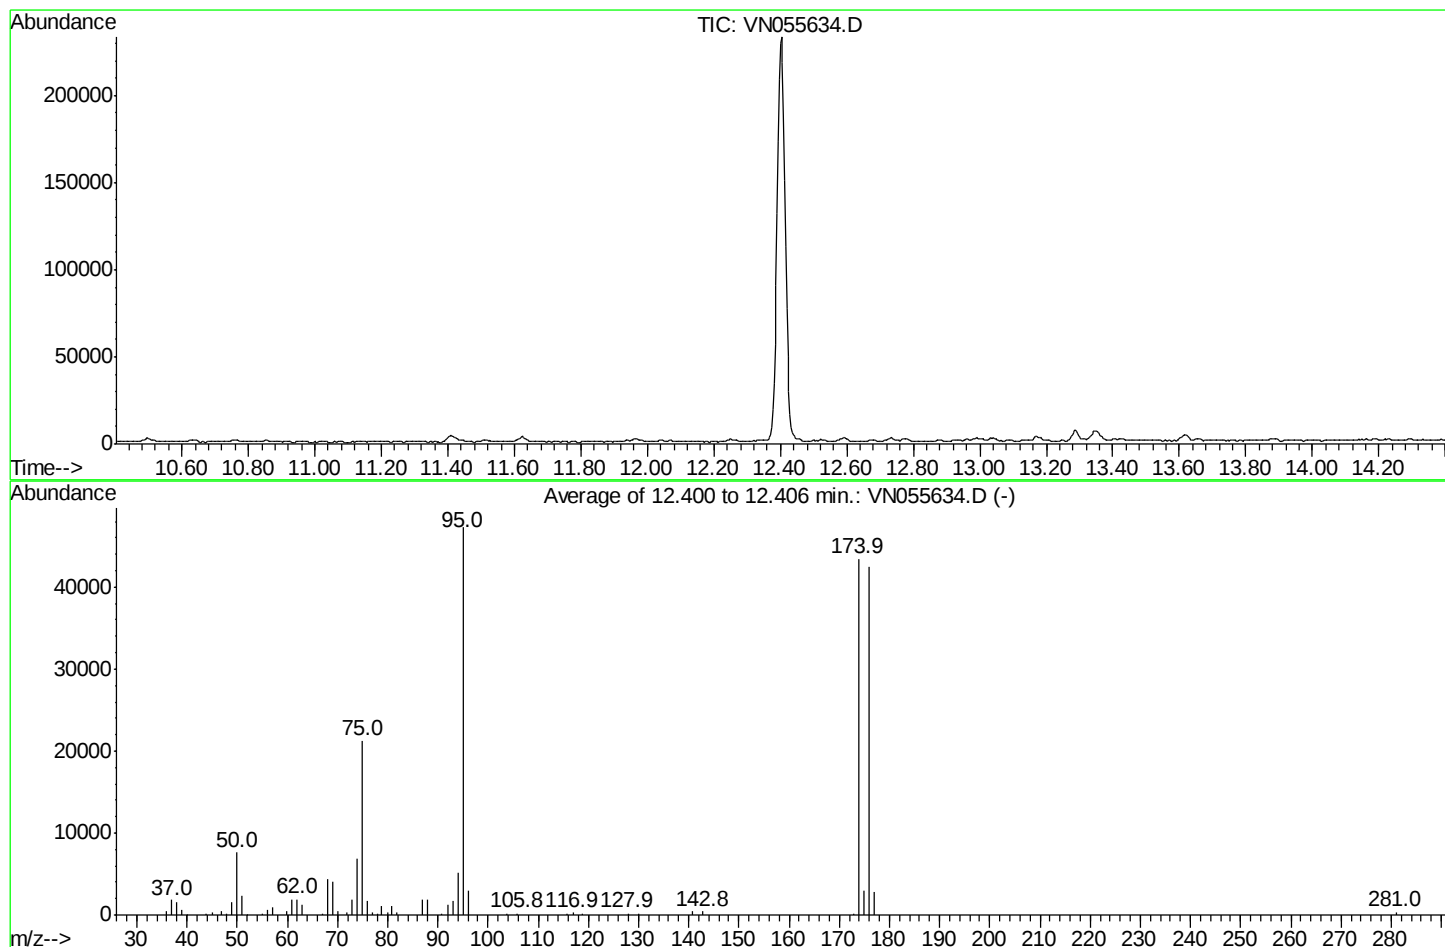

AutoFind: Scans 3305, 3306, 3307; Background Corrected with Scan 3291

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.1	7603	PASS
75	95	30	60	45.0	21301	PASS
95	95	100	100	100.0	47290	PASS
96	95	5	9	6.3	2985	PASS
173	174	0.00	2	0.5	233	PASS
174	95	50	100	92.0	43490	PASS
175	174	5	9	7.0	3033	PASS
176	174	95	101	97.8	42528	PASS
177	176	5	9	6.6	2796	PASS