
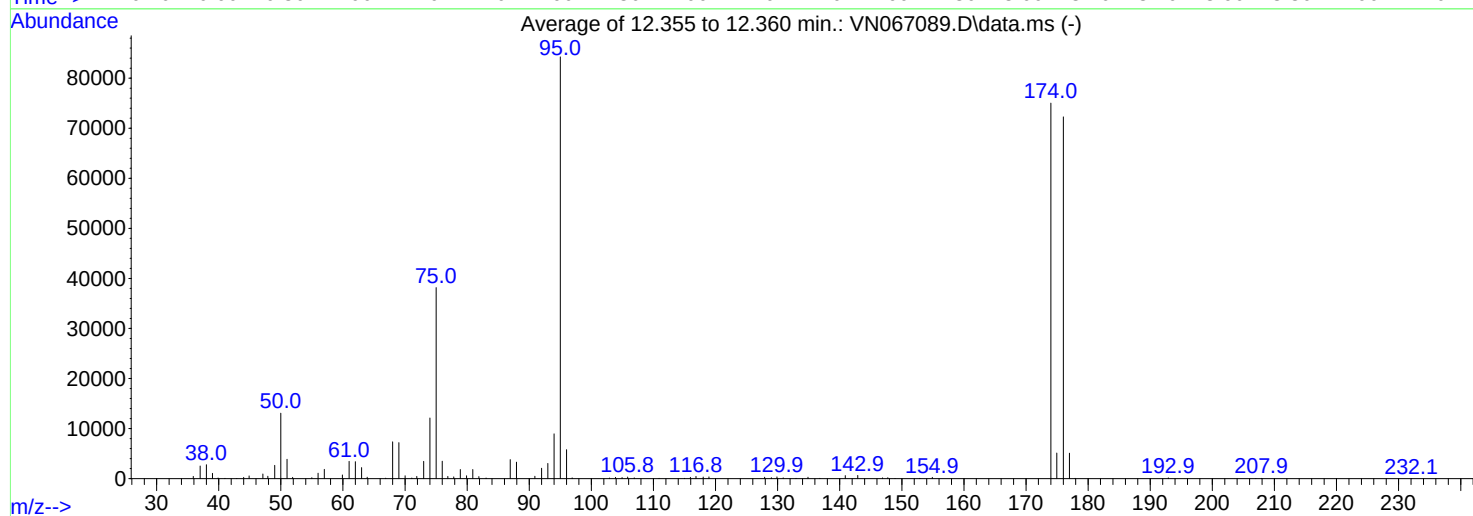


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN051721\
 Data File : VN067089.D
 Acq On : 17 May 2021 9:23
 Operator : JC/MD
 Sample : BFB
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N051421W.M
 Title : SW846 8260
 Last Update : Tue May 18 04:00:15 2021

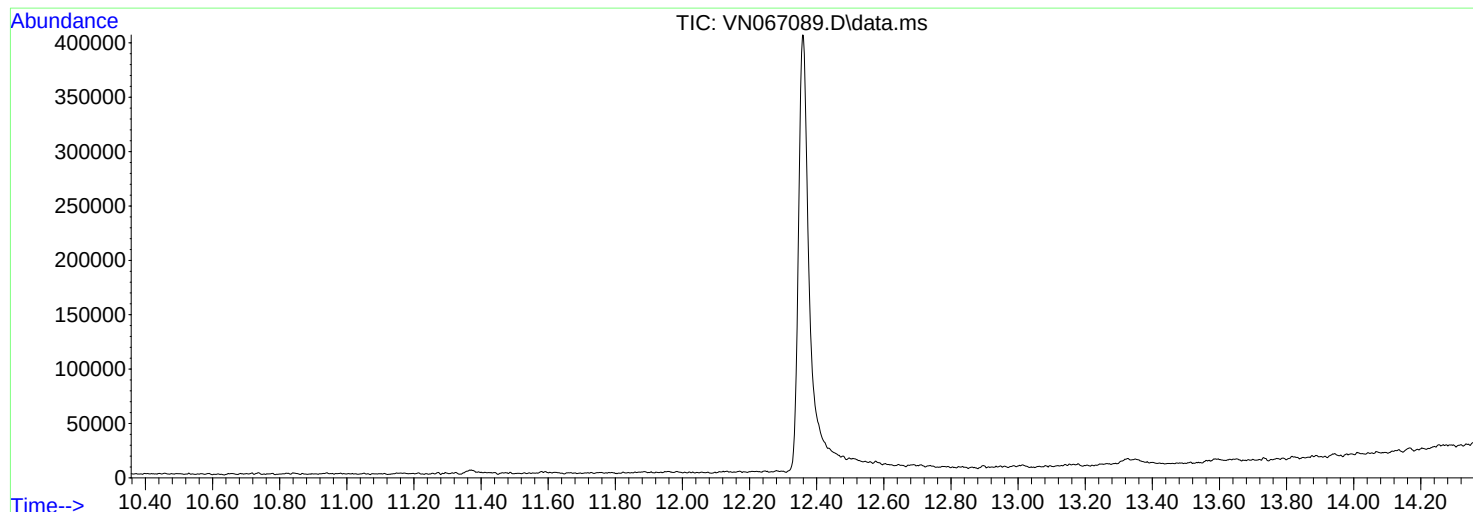

AutoFind: Scans 3958, 3959, 3960; Background Corrected with Scan 3941

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.5	13090	PASS
75	95	30	60	45.3	38181	PASS
95	95	100	100	100.0	84264	PASS
96	95	5	9	6.9	5783	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	89.0	75011	PASS
175	174	5	9	6.8	5101	PASS
176	174	95	101	96.4	72285	PASS
177	176	5	9	7.0	5080	PASS