

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN051722\
 Data File : VN072528.D
 Acq On : 17 May 2022 14:00
 Operator : JC\MD
 Sample : VN0517WBL01
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 VN0517WBL01

Quant Time: May 18 07:24:34 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\624N051622W.M
 Quant Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
 QLast Update : Tue May 17 06:34:50 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Bromochloromethane	7.651	128	25323	30.000	ug/l	0.00
28) 1,4-Difluorobenzene	8.963	114	130855	30.000	ug/l	0.00
57) Chlorobenzene-d5	11.739	117	110230	30.000	ug/l	0.00

System Monitoring Compounds						
27) 1,2-Dichloroethane-d4	8.434	65	82170	28.837	ug/l	0.00
Spiked Amount	30.000	Range	91 - 110	Recovery	=	96.133%
60) 4-Bromofluorobenzene	12.727	95	47922	22.266	ug/l	0.00
Spiked Amount	30.000	Range	63 - 112	Recovery	=	74.233%
63) Toluene-d8	10.439	98	185684	30.859	ug/l	0.00
Spiked Amount	30.000	Range	91 - 112	Recovery	=	102.867%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN051722\
Data File : VN072528.D
Acq On : 17 May 2022 14:00
Operator : JC\MD
Sample : VN0517WBL01
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
VN0517WBL01


Quant Time: May 18 07:24:34 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\624N051622W.M
Quant Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
QLast Update : Tue May 17 06:34:50 2022
Response via : Initial Calibration

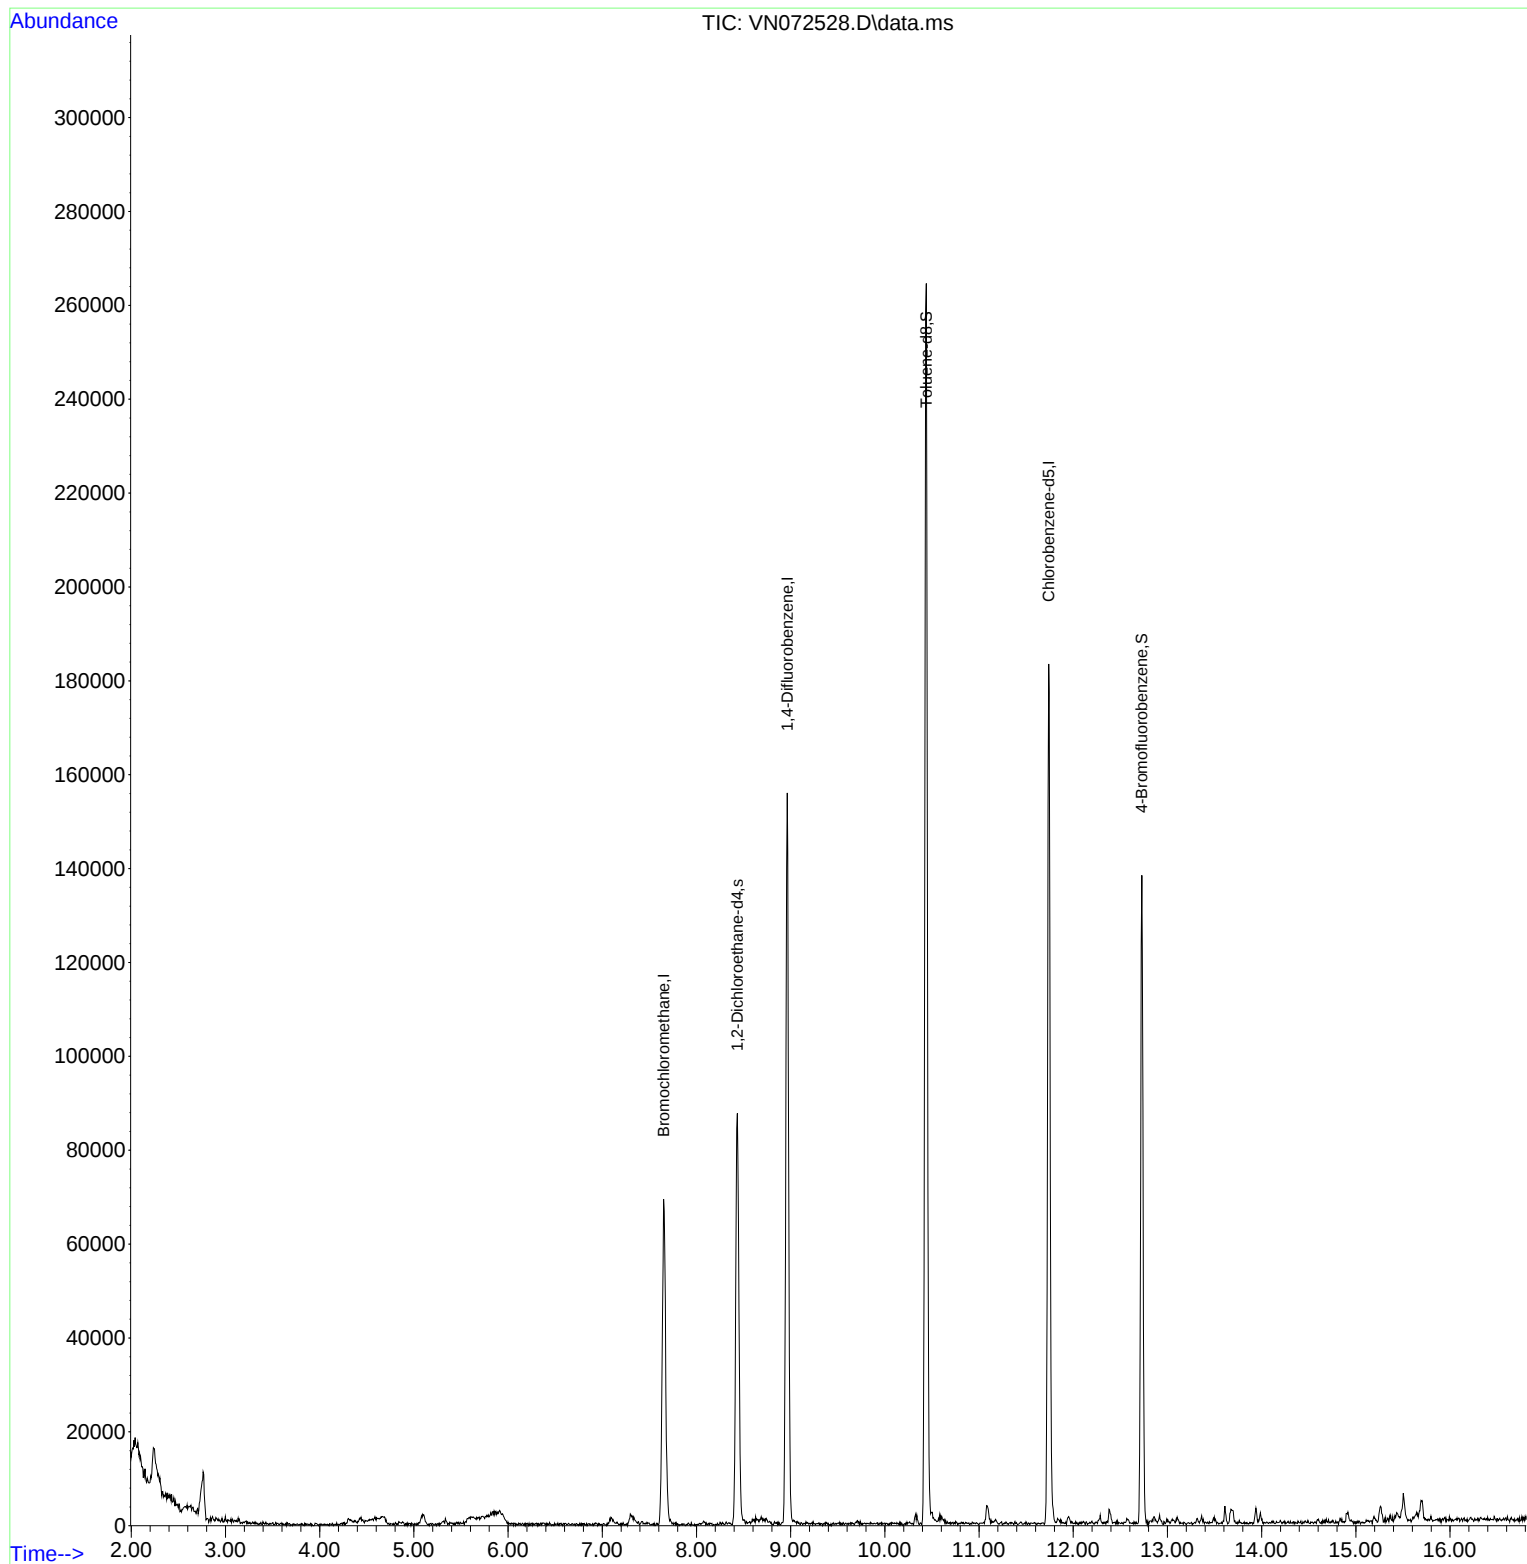



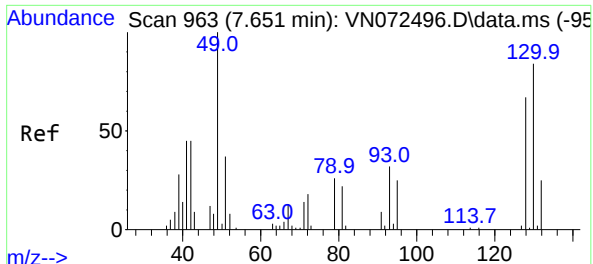


#1
Bromochloromethane
Concen: 30.000 ug/l
RT: 7.651 min Scan# 90
Delta R.T. 0.000 min
Lab File: VN072528.D
Acq: 17 May 2022 14:00

Instrument :
MSVOA_N
ClientSampleId :
VN0517WBL01



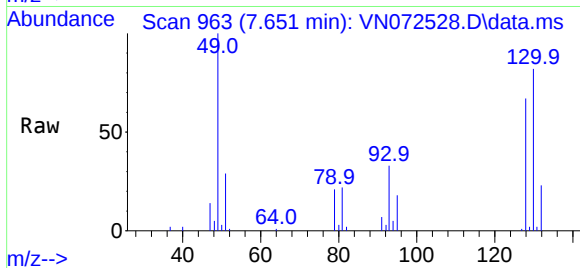



Tgt Ion:128 Resp: 25323
Ion Ratio Lower Upper
128 100
49 151.4 0.0 392.3
130 126.3 0.0 320.2

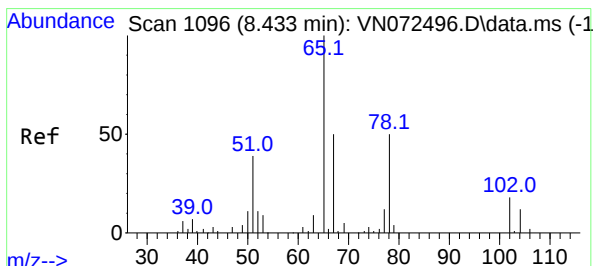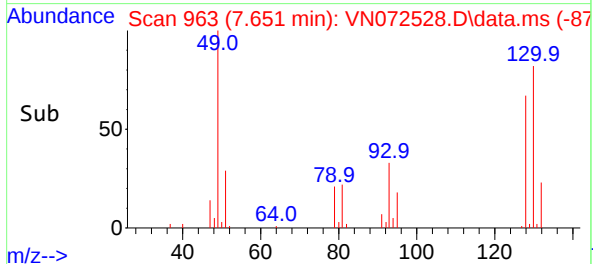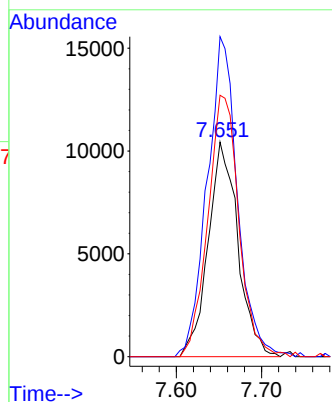

#27
1,2-Dichloroethane-d4
Concen: 28.837 ug/l
RT: 8.434 min Scan# 1096
Delta R.T. 0.000 min
Lab File: VN072528.D
Acq: 17 May 2022 14:00

Tgt Ion: 65 Resp: 82170
Ion Ratio Lower Upper
65 100
67 49.0 40.2 60.2


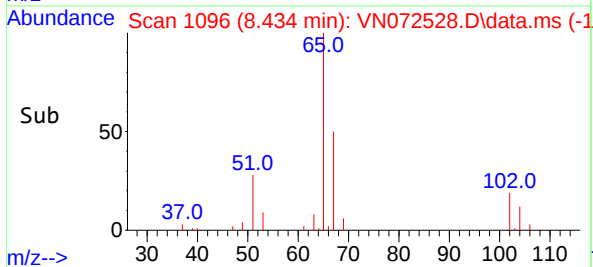
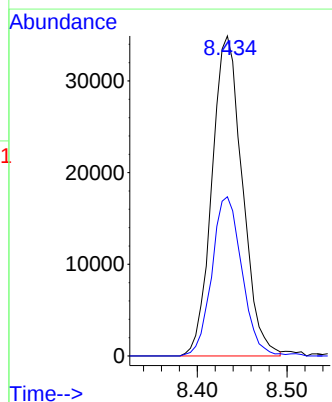
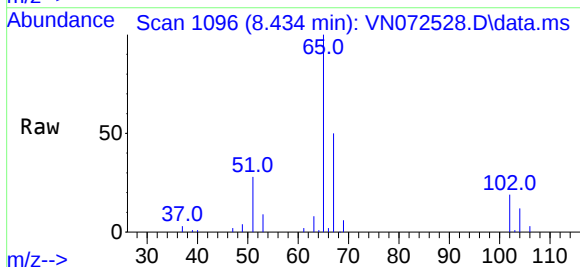


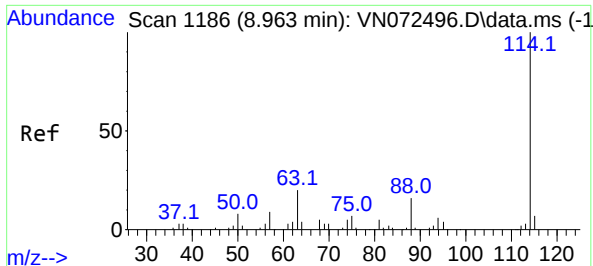

#28
1,4-Difluorobenzene
Concen: 30.000 ug/l
RT: 8.963 min Scan# 1186
Delta R.T. 0.000 min
Lab File: VN072528.D
Acq: 17 May 2022 14:00




Instrument :
MSVOA_N
ClientSampleId :
VN0517WBL01


Tgt Ion:114 Resp: 130855
Ion Ratio Lower Upper
114 100
63 21.2 15.8 23.6
88 15.6 11.6 17.4

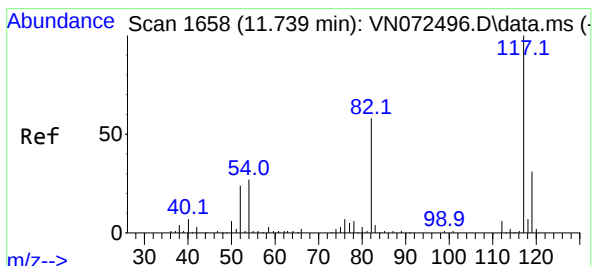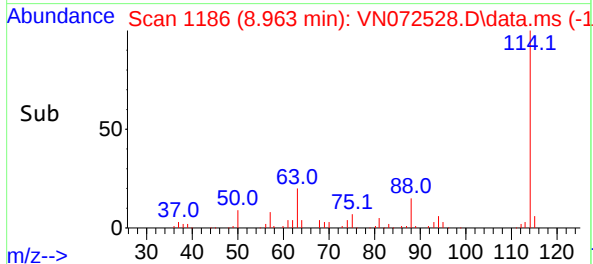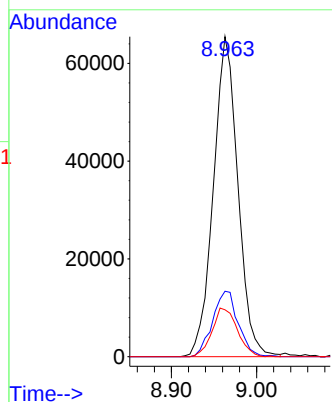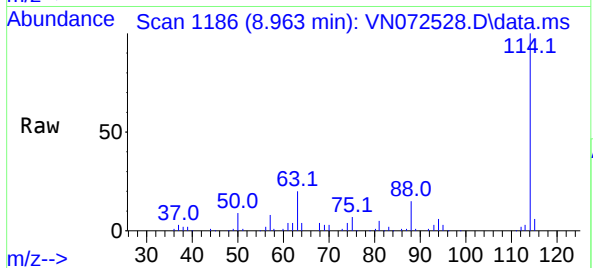

#57
Chlorobenzene-d5
Concen: 30.000 ug/l
RT: 11.739 min Scan# 1658
Delta R.T. 0.000 min
Lab File: VN072528.D
Acq: 17 May 2022 14:00

Tgt Ion:117 Resp: 110230
Ion Ratio Lower Upper
117 100
82 56.3 43.6 65.4
119 32.3 25.8 38.6


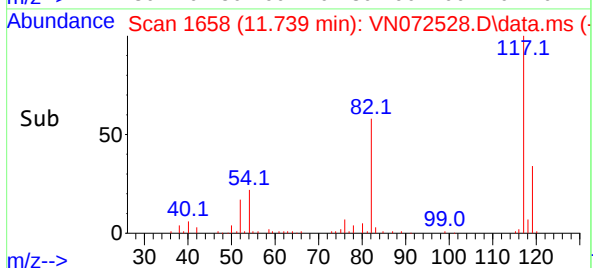
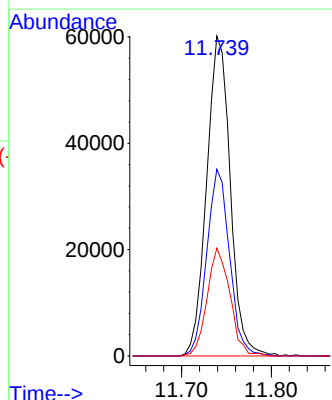
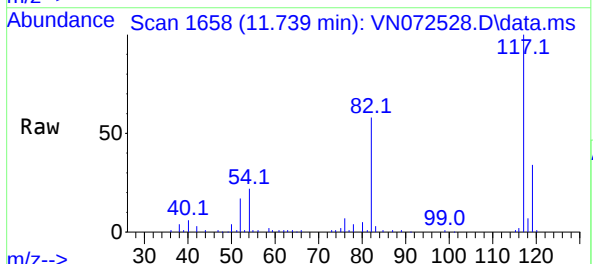


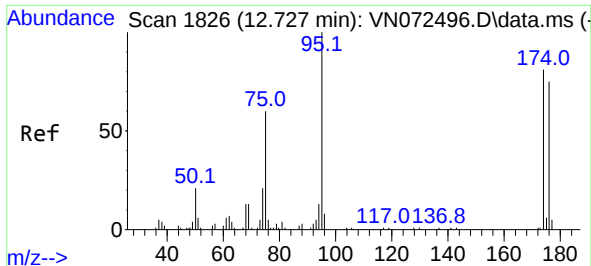

#60
4-Bromofluorobenzene
Concen: 22.266 ug/l
RT: 12.727 min Scan# 11
Delta R.T. 0.000 min
Lab File: VN072528.D
Acq: 17 May 2022 14:00

Instrument :
MSVOA_N
ClientSampleId :
VN0517WBL01

Tgt Ion: 95 Resp: 47922
Ion Ratio Lower Upper
95 100
174 80.6 62.9 94.3
176 74.8 61.0 91.4

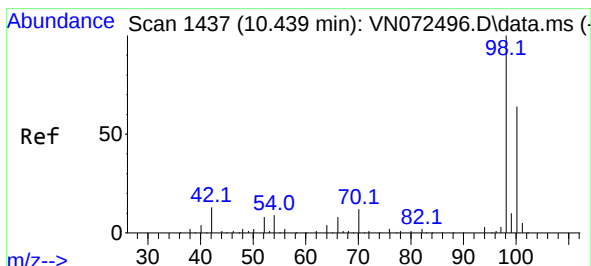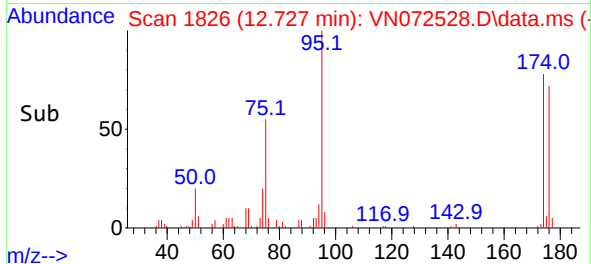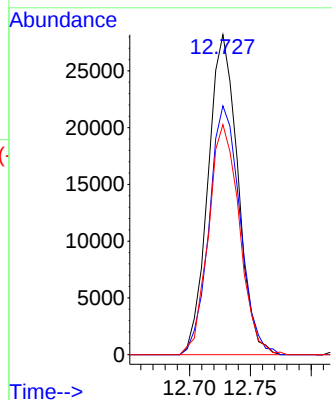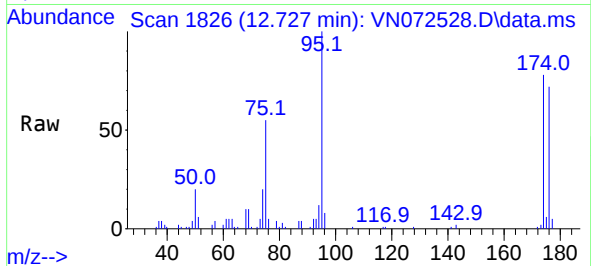

#63
Toluene-d8
Concen: 30.859 ug/l
RT: 10.439 min Scan# 1437
Delta R.T. 0.000 min
Lab File: VN072528.D
Acq: 17 May 2022 14:00

Tgt Ion: 98 Resp: 185684
Ion Ratio Lower Upper
98 100
100 64.8 50.6 76.0

