
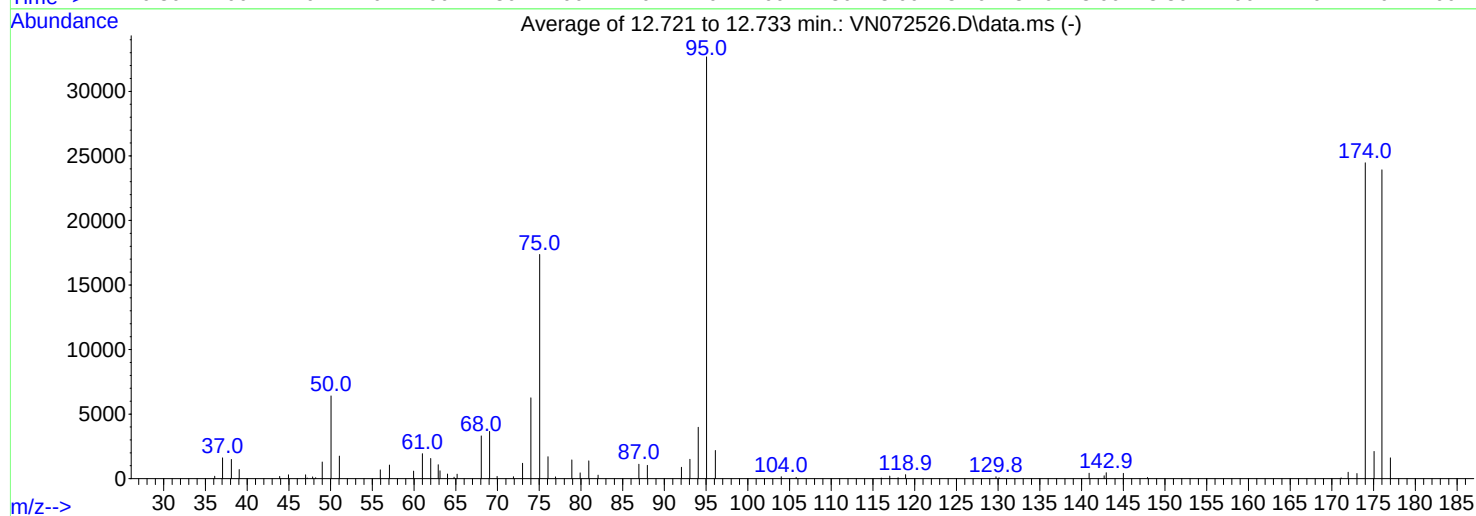


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN051722\
 Data File : VN072526.D
 Acq On : 17 May 2022 11:07
 Operator : JC\MD
 Sample : BFB
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT3.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\624N051622W.M
 Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
 Last Update : Tue May 17 06:34:50 2022

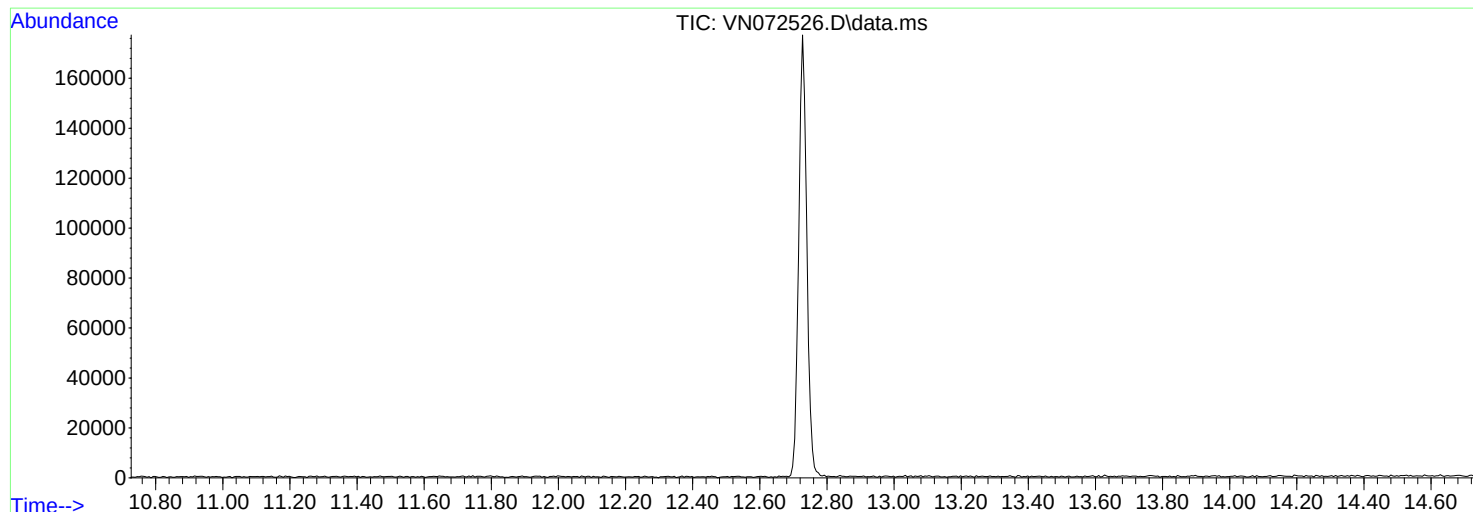

AutoFind: Scans 1825, 1826, 1827; Background Corrected with Scan 1818

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.6	6413	PASS
75	95	30	60	53.2	17371	PASS
95	95	100	100	100.0	32675	PASS
96	95	5	9	6.7	2180	PASS
173	174	0.00	2	1.6	398	PASS
174	95	50	100	74.9	24469	PASS
175	174	5	9	8.6	2107	PASS
176	174	95	101	97.8	23925	PASS
177	176	5	9	6.8	1615	PASS