



Acrolein

Response Ratio

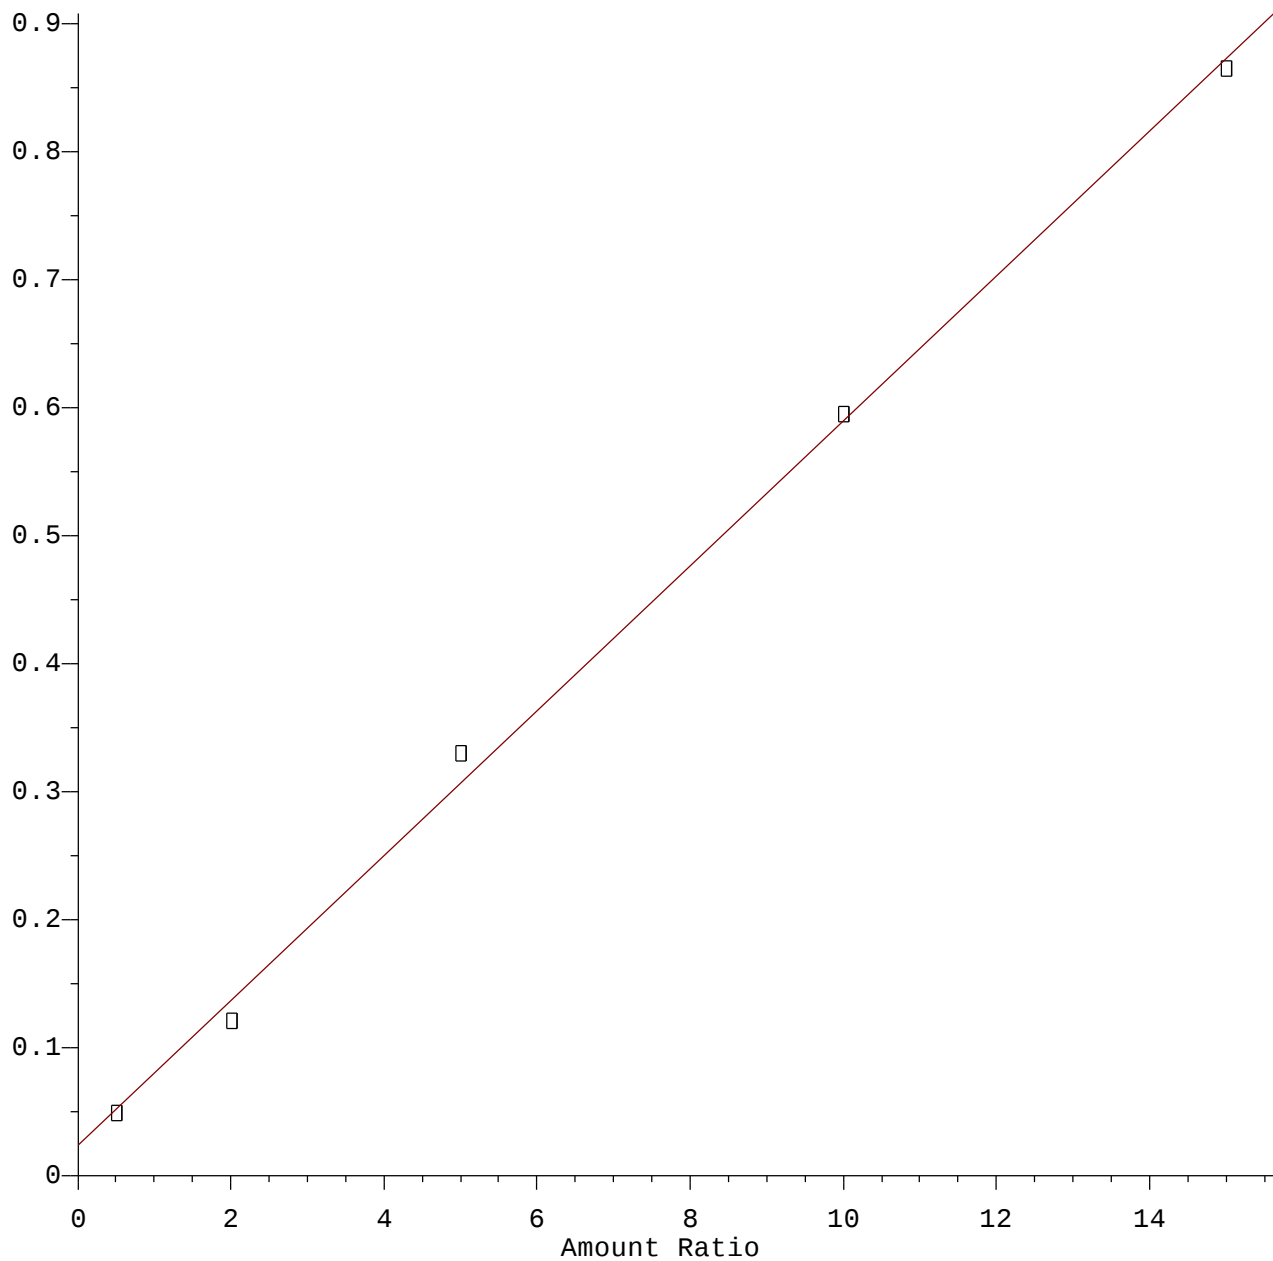


Resp Ratio = $5.66 \times 10^{-2} \times \text{Amt} + 2.36 \times 10^{-2}$
Coef of Det (r^2) = 0.998 Curve Fit: Linear


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N051820W.M
Calibration Table Last Updated: Mon May 18 13:09:55 2020

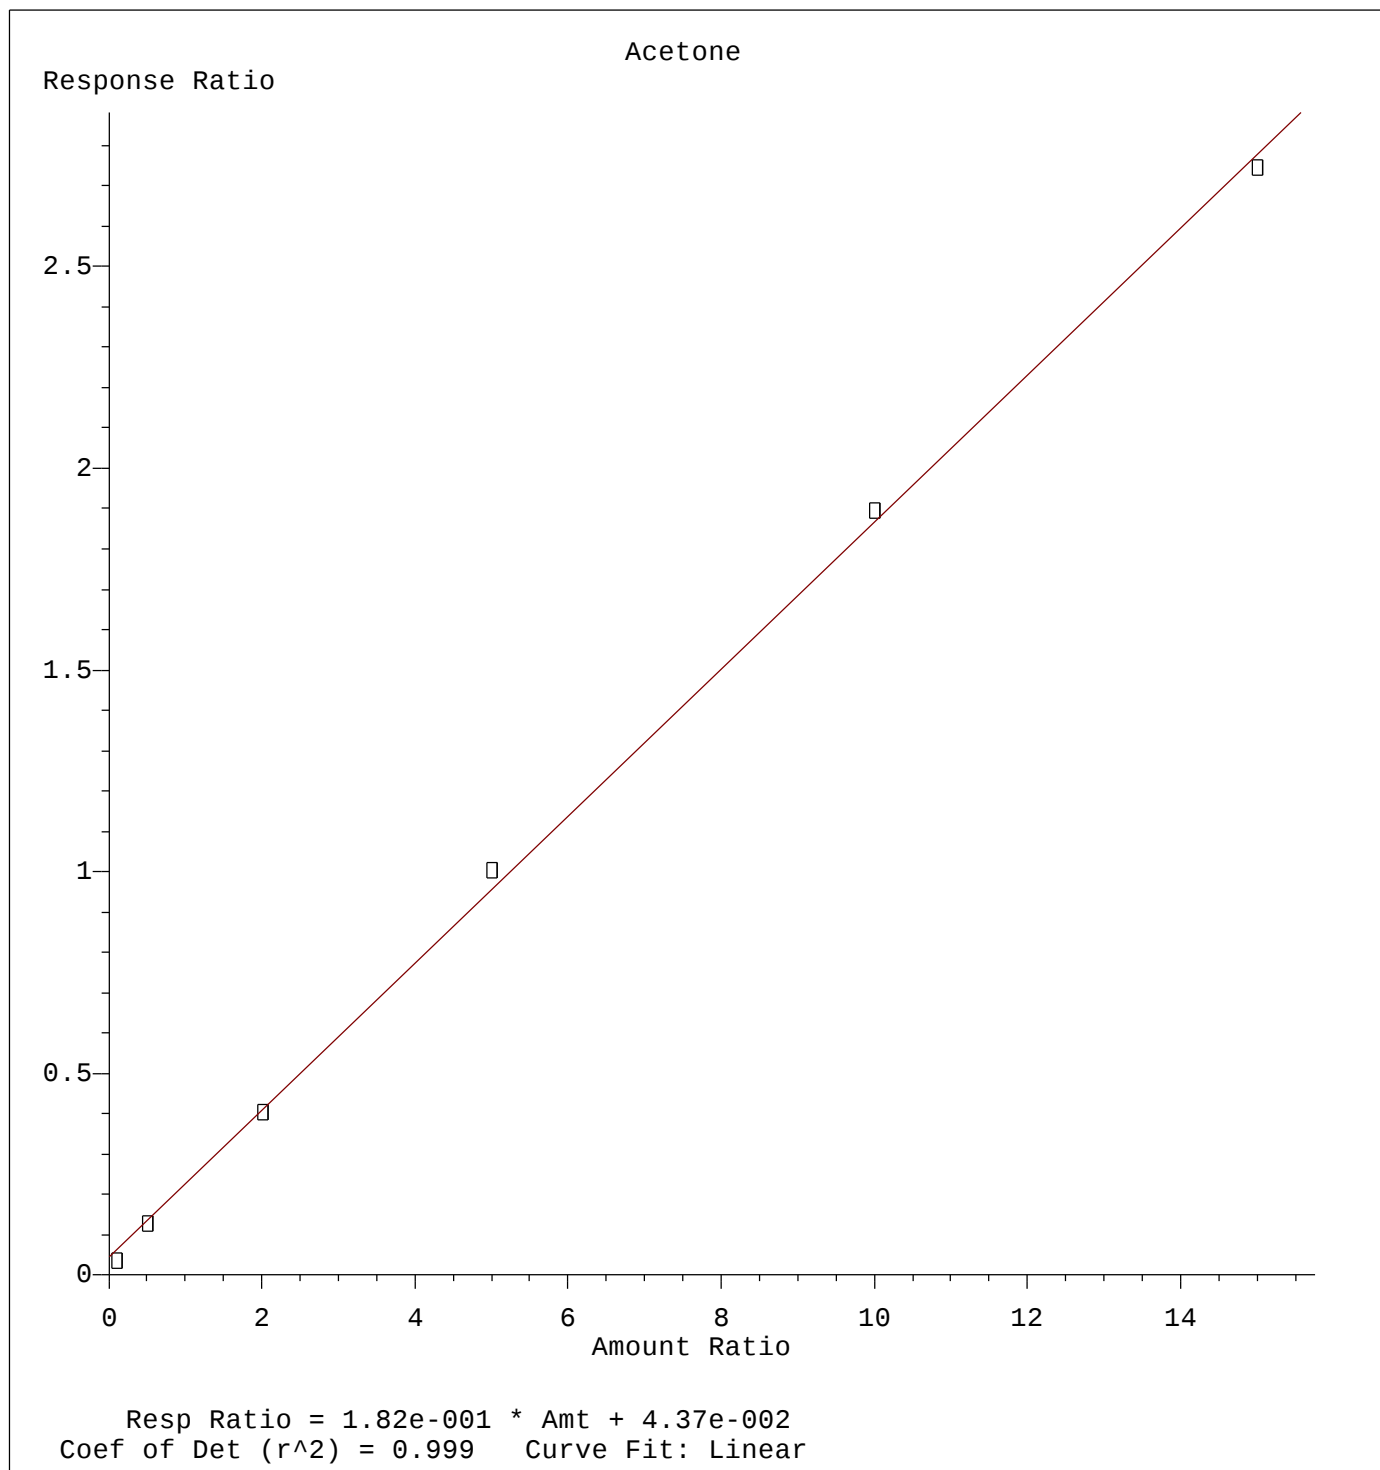


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N051820W.M
Calibration Table Last Updated: Mon May 18 13:09:55 2020

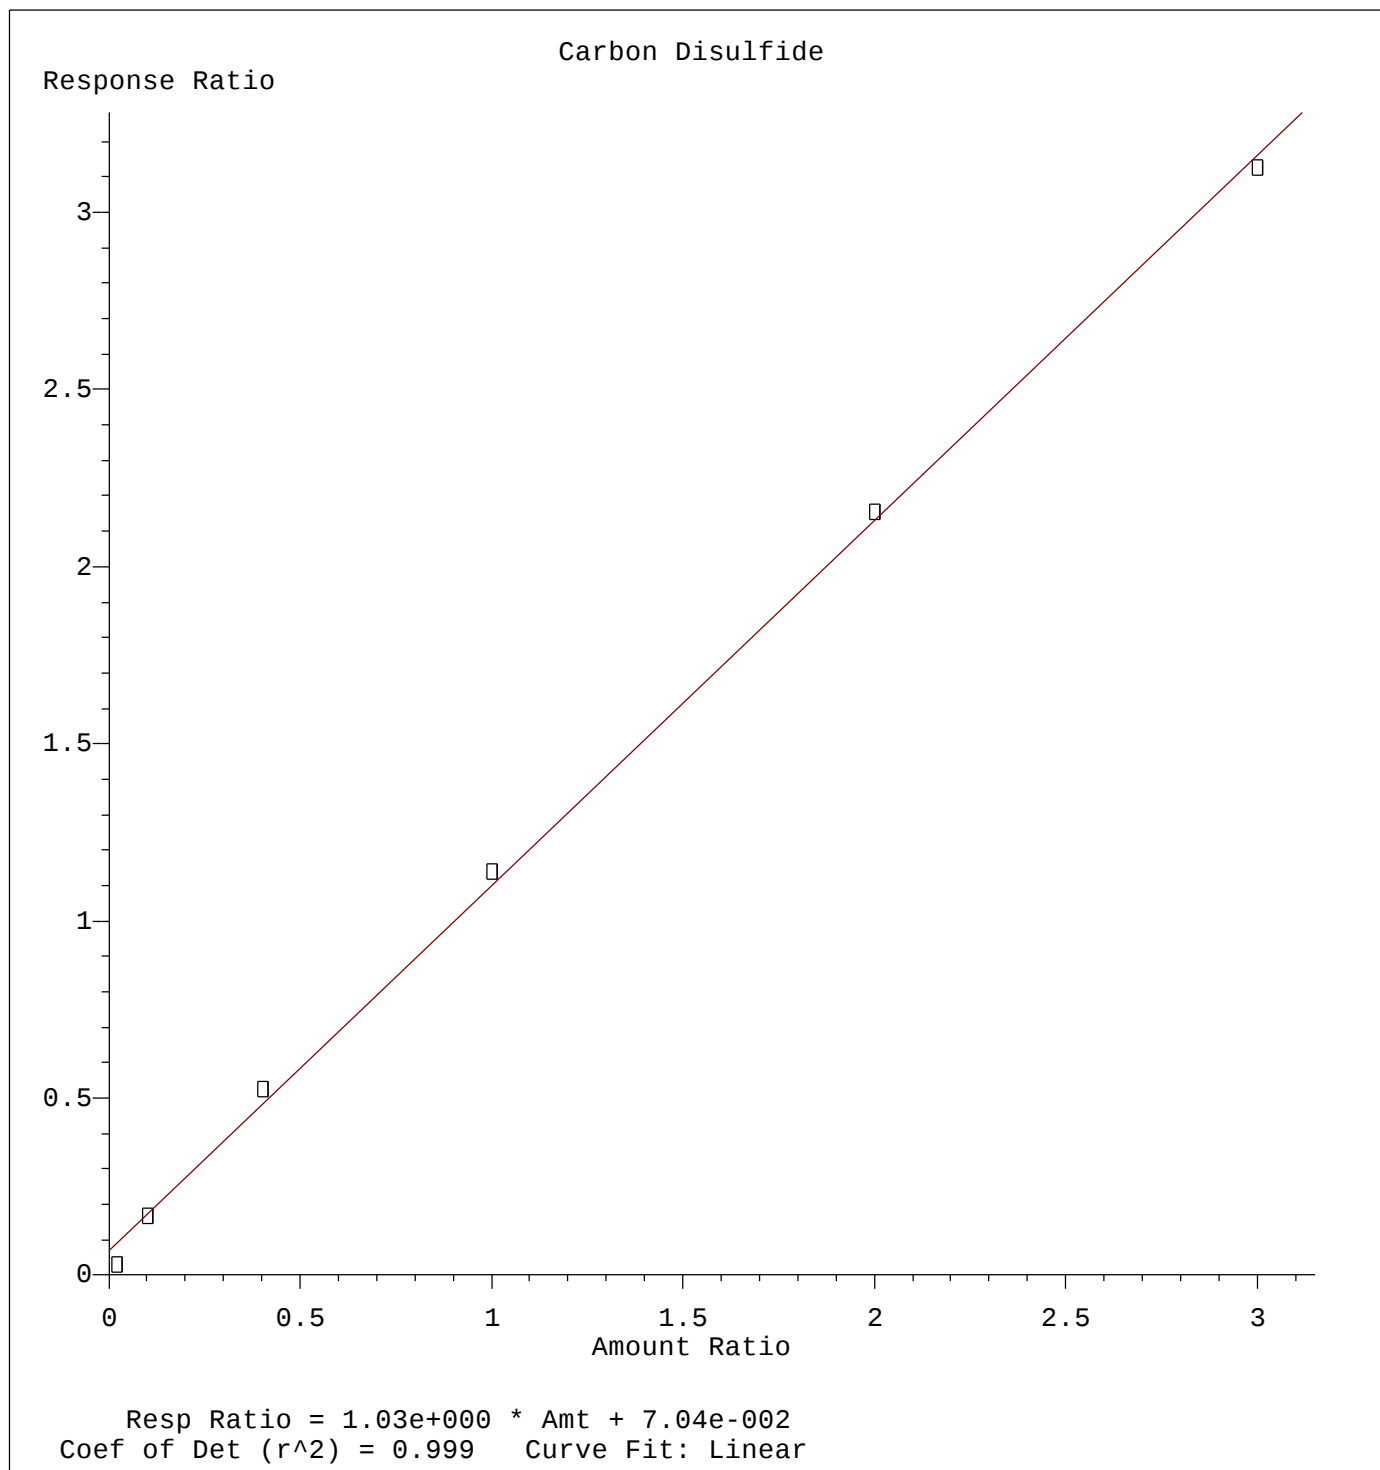


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N051820W.M
Calibration Table Last Updated: Mon May 18 13:09:55 2020

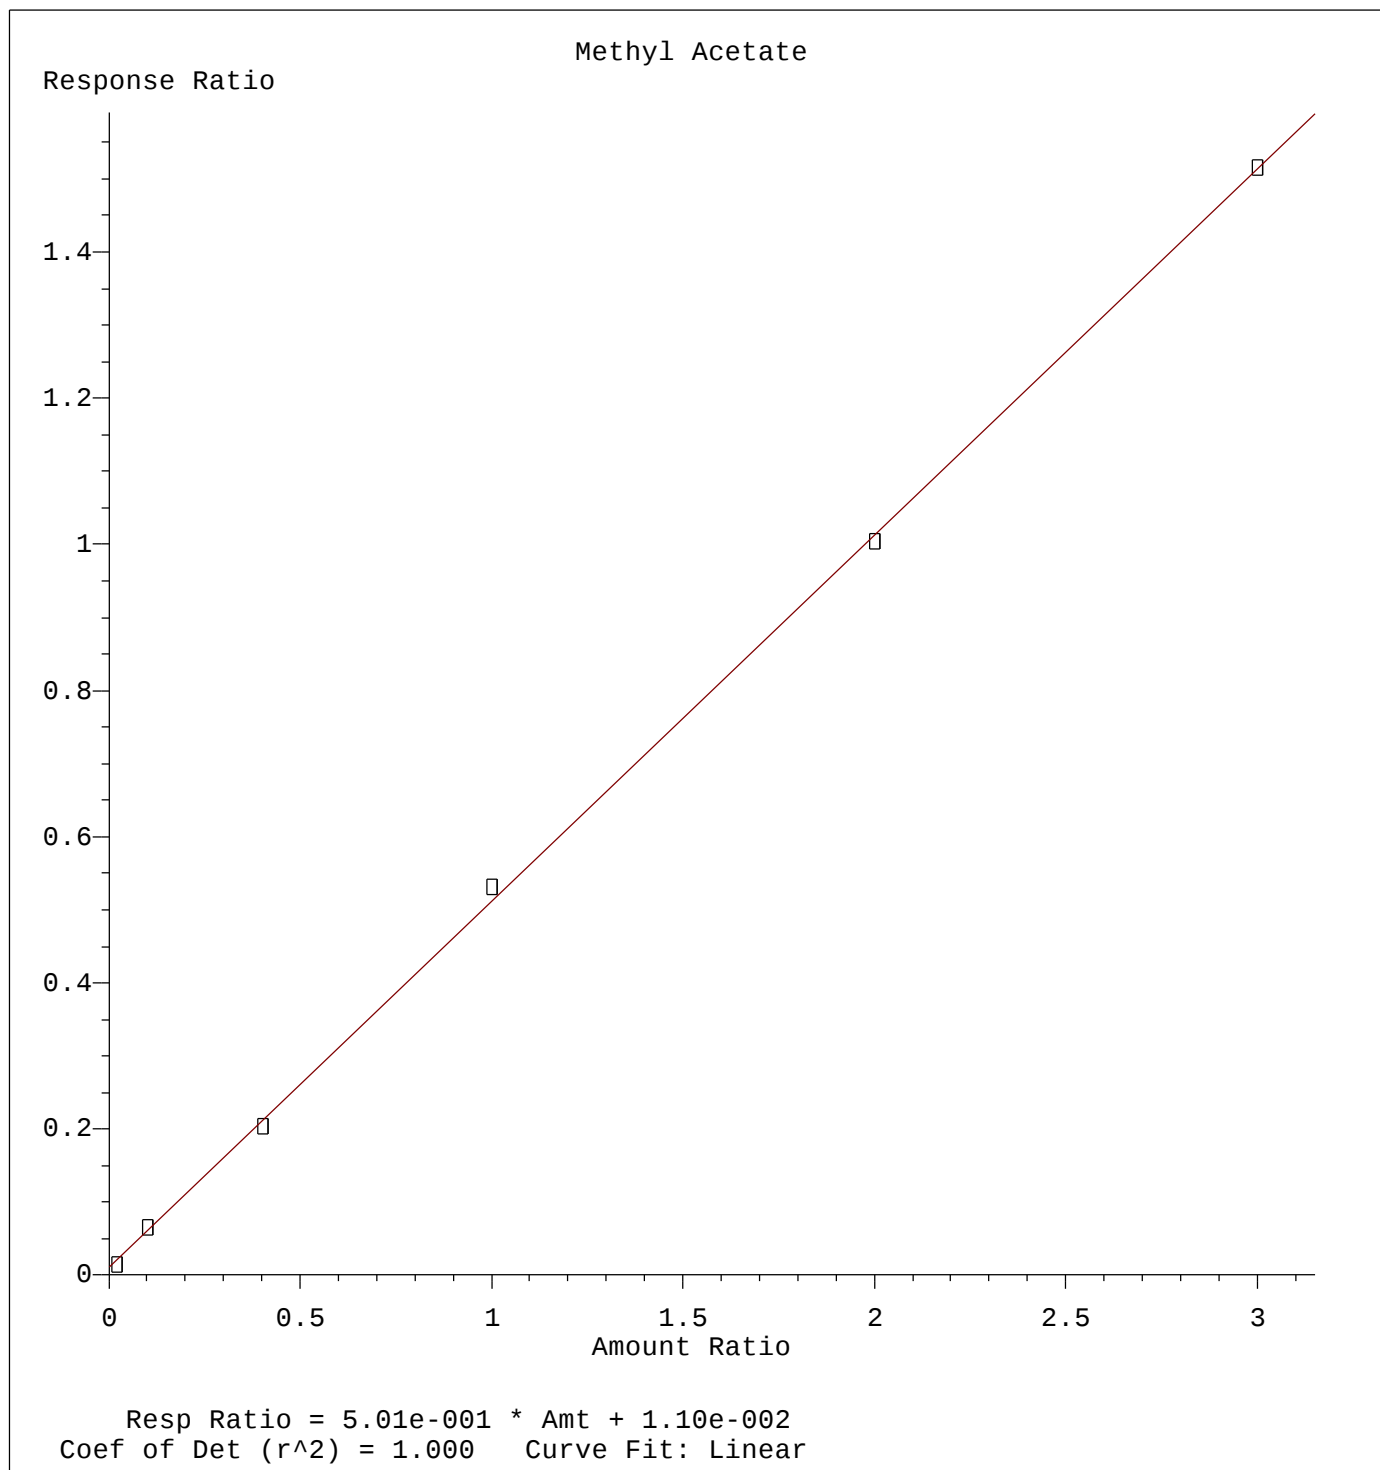


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N051820W.M
Calibration Table Last Updated: Mon May 18 13:09:55 2020

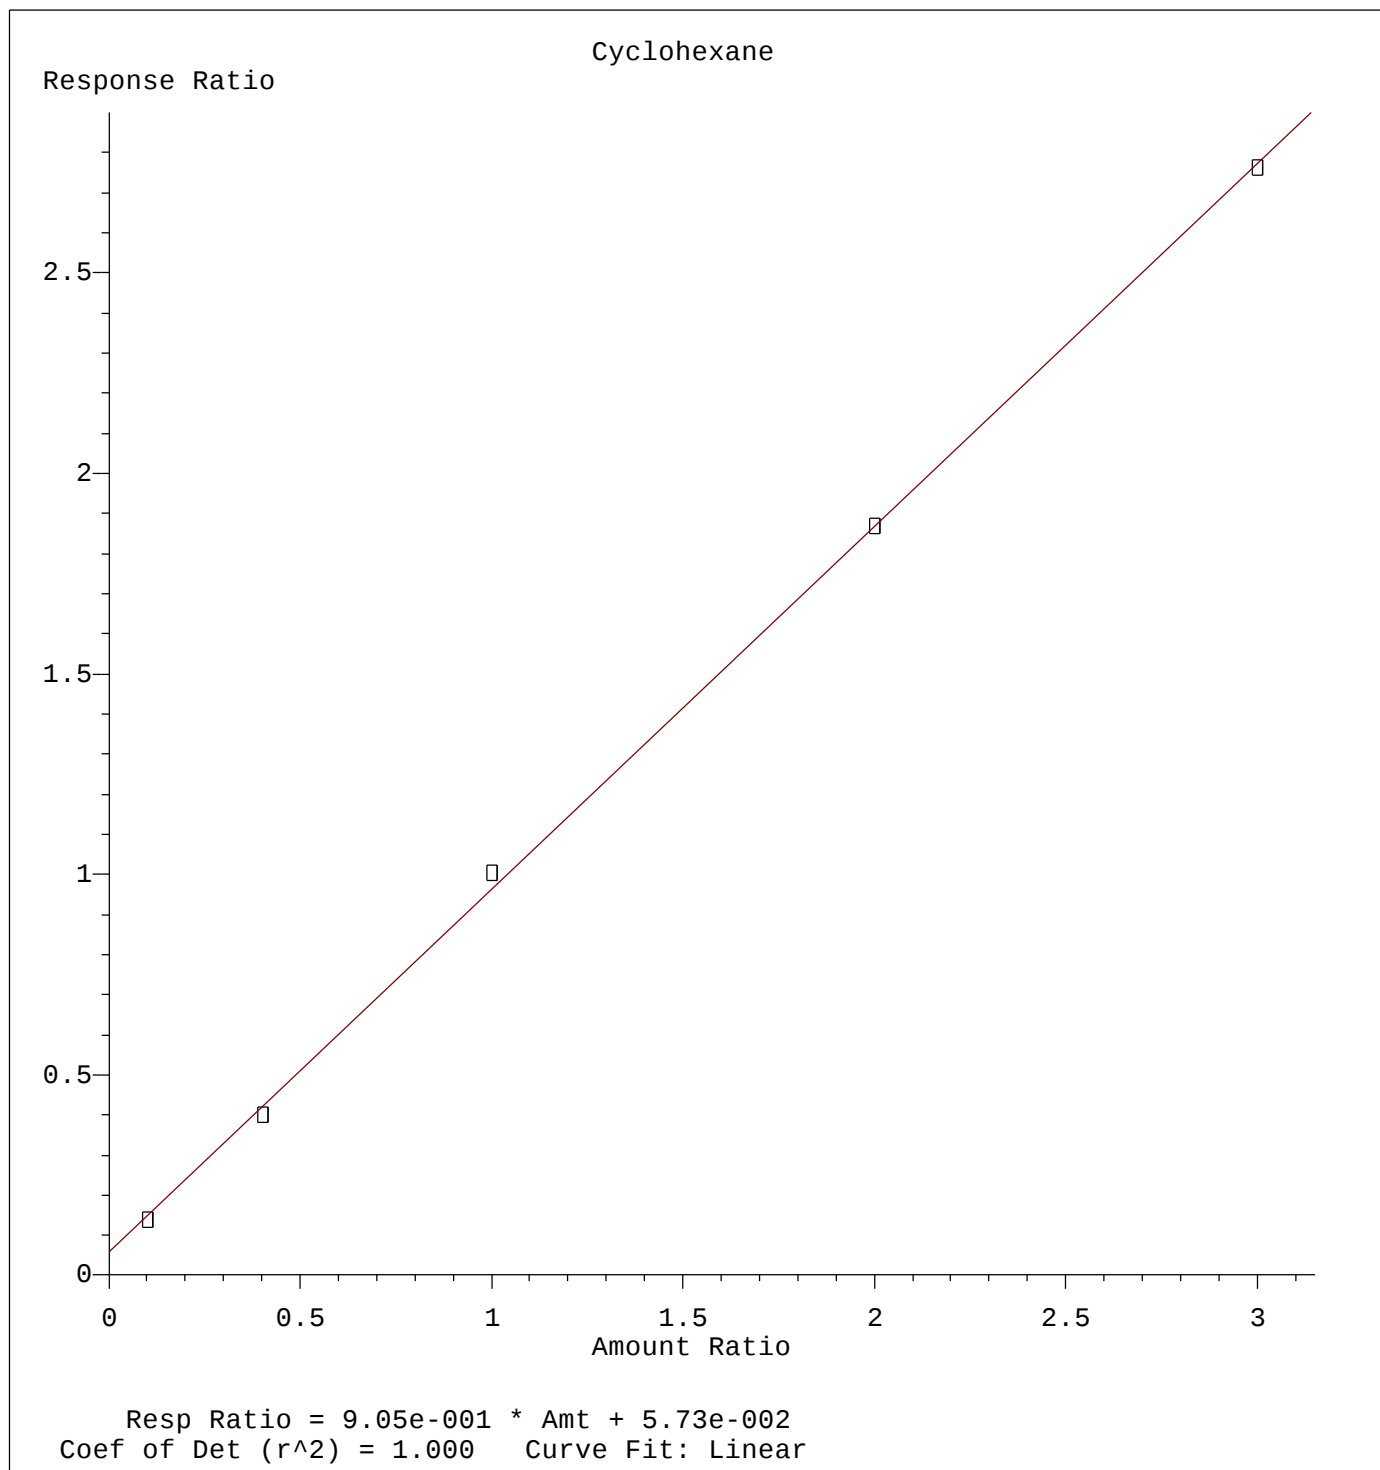

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N051820W.M
Calibration Table Last Updated: Mon May 18 13:09:55 2020

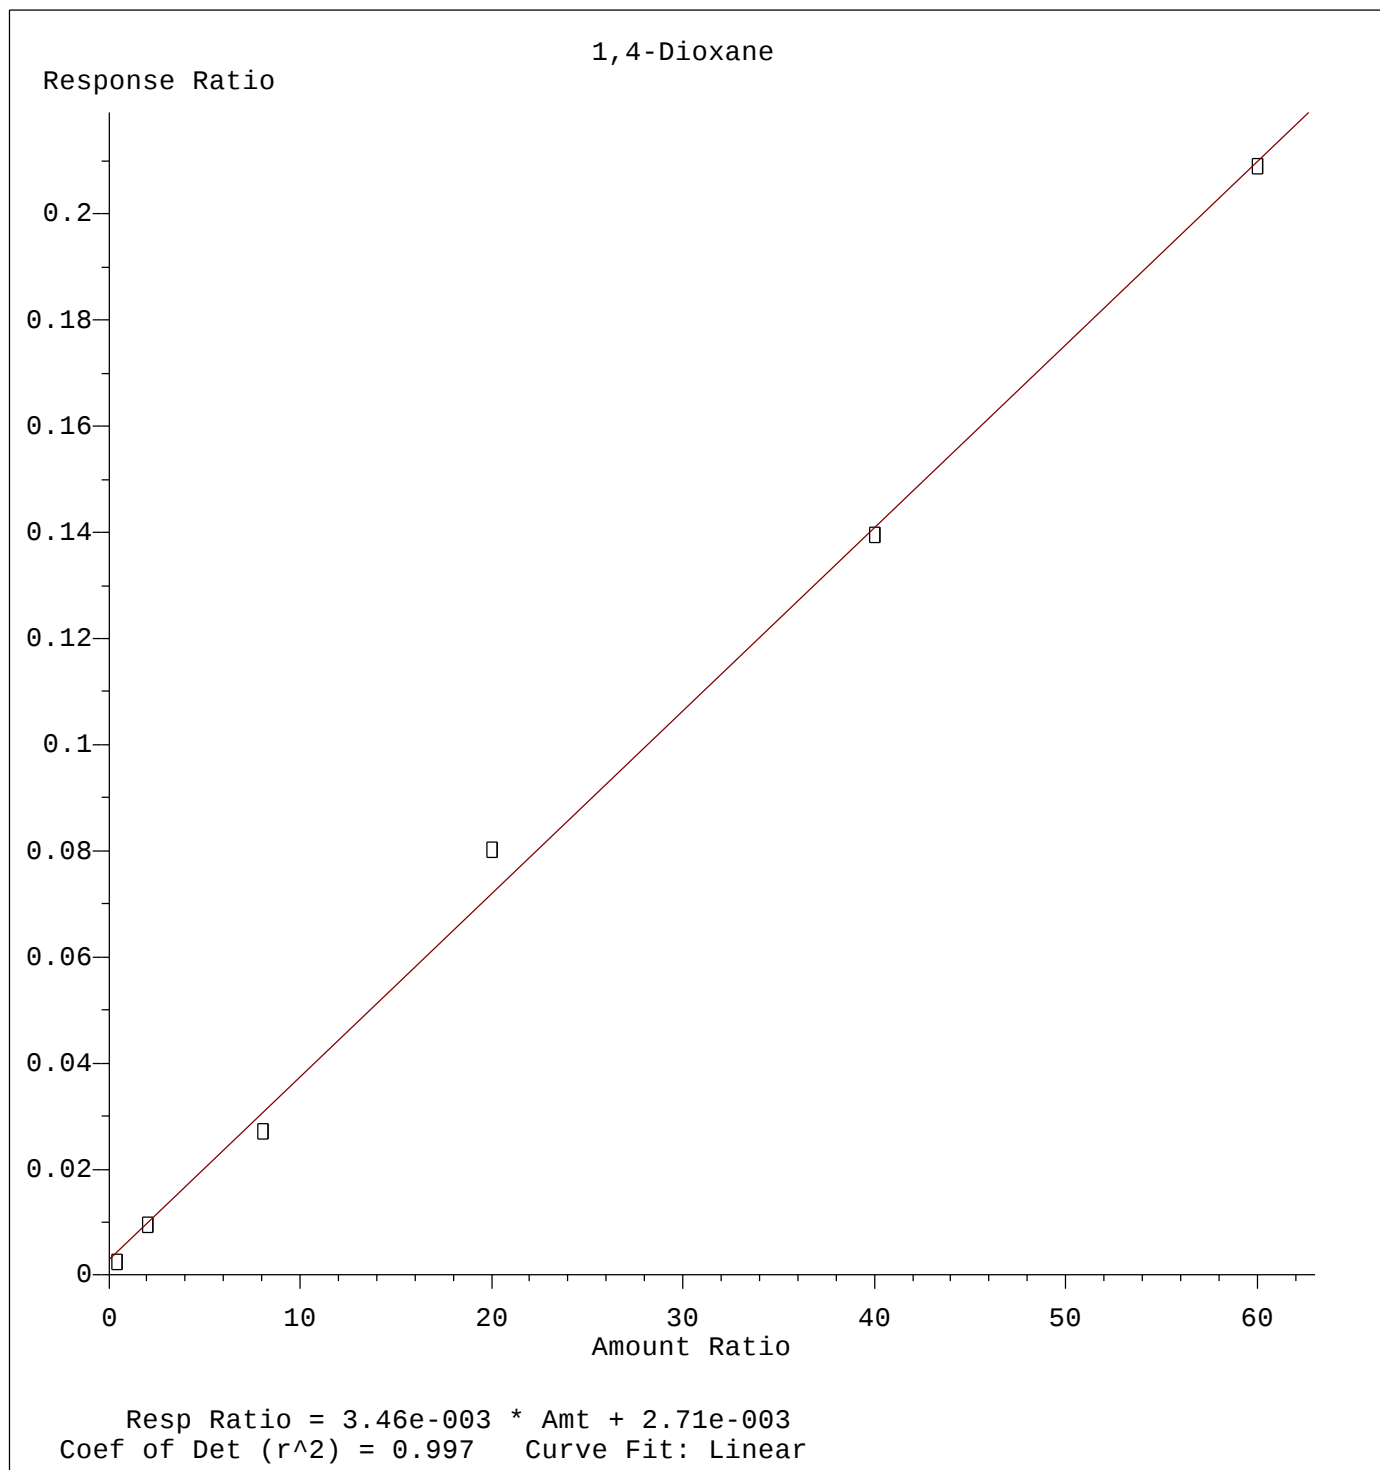


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N051820W.M
Calibration Table Last Updated: Mon May 18 13:09:55 2020

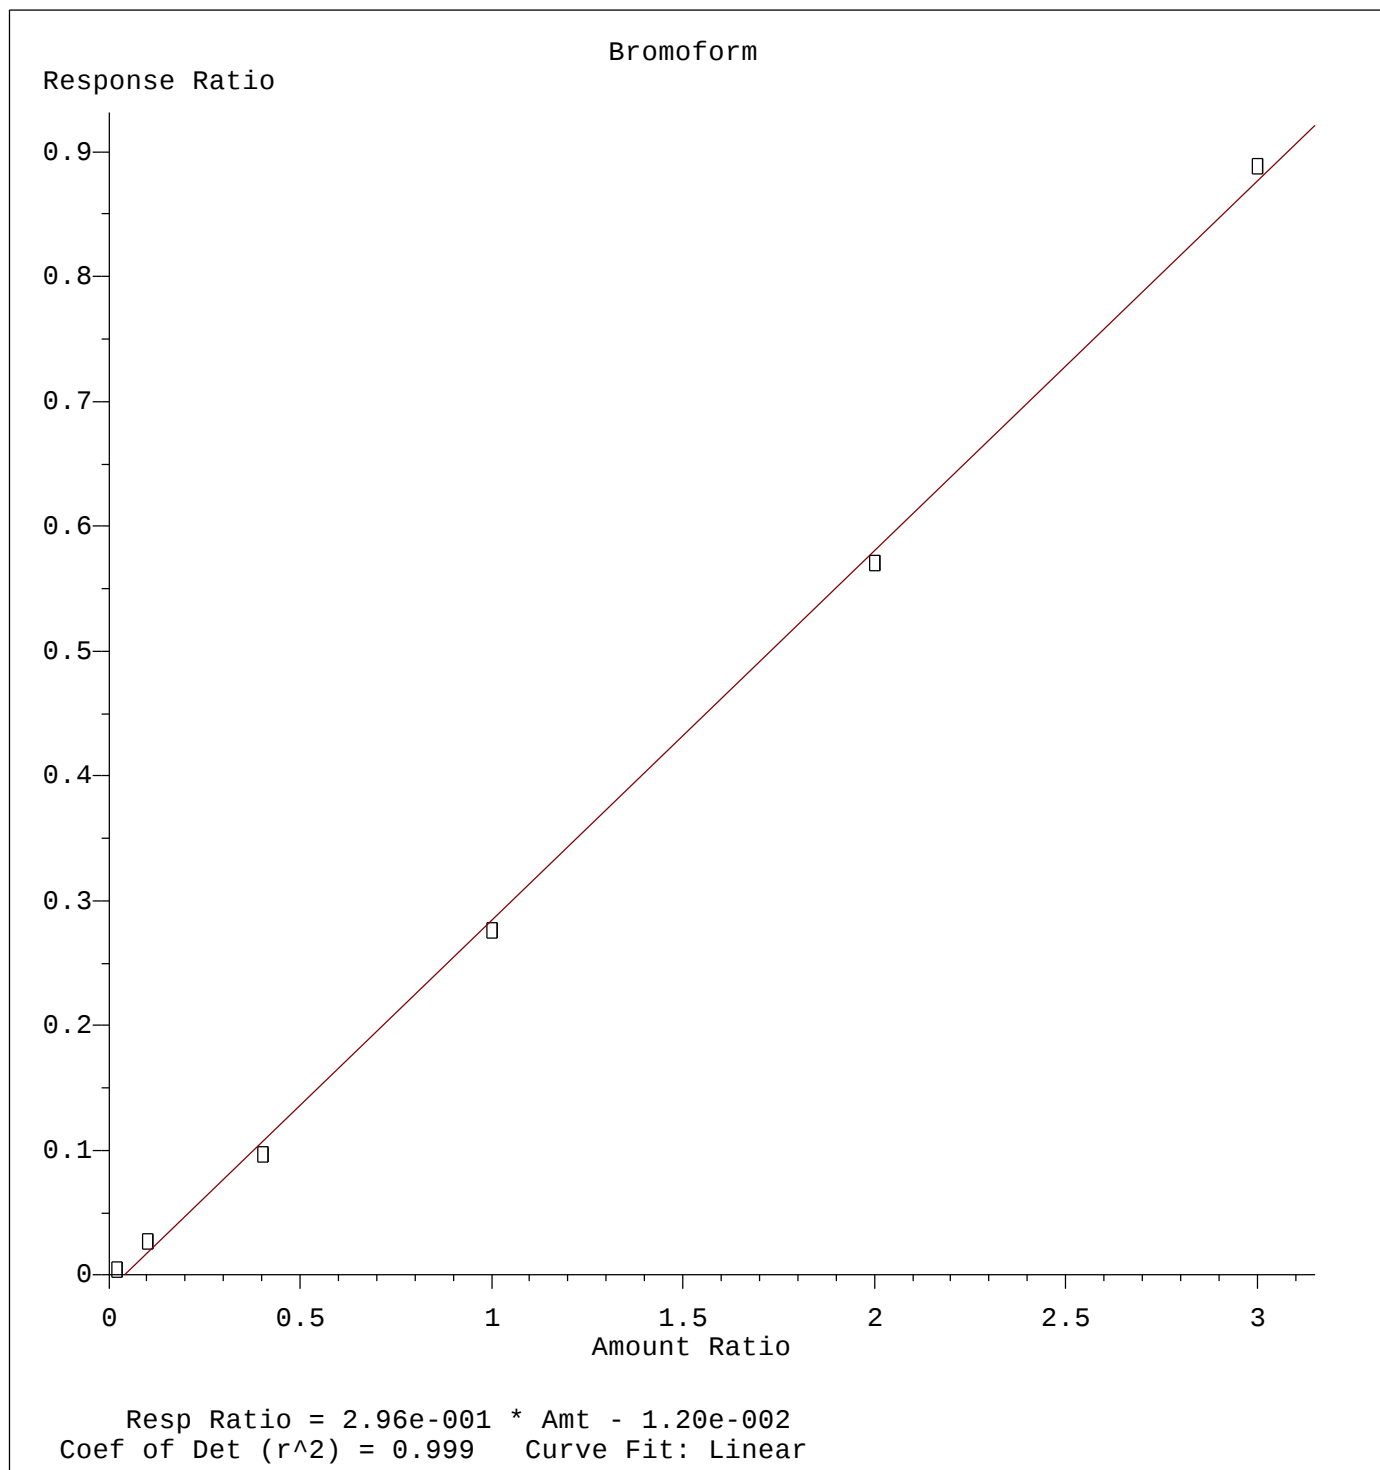

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N051820W.M
Calibration Table Last Updated: Mon May 18 13:09:55 2020

Bromomethane

Response Ratio

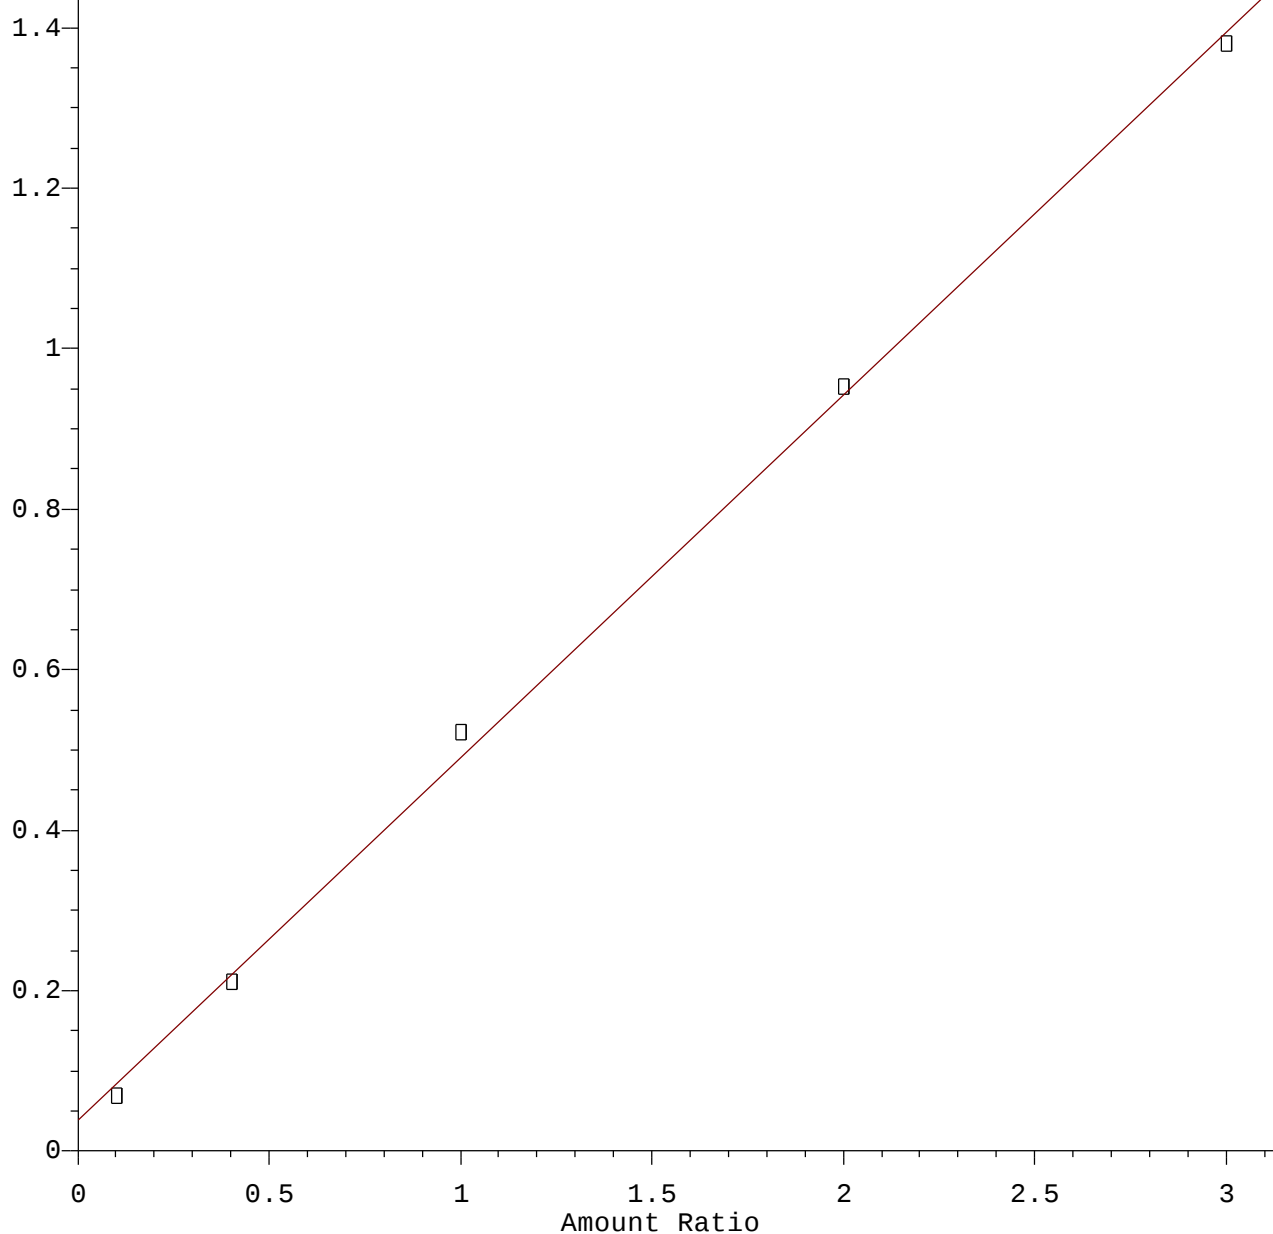

Resp Ratio = $4.52 \times 10^{-1} \times \text{Amt} + 3.92 \times 10^{-2}$
Coef of Det (r^2) = 0.999 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N051820W.M
Calibration Table Last Updated: Mon May 18 13:09:55 2020