


Data Path : Z:\voasrv\HPCHEM1\MSVOA N\Data\VN051820\
Data File : VN061450.D
Acq On : 18 May 2020 23:40
Operator : JC/MD
Sample : BFB
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N051820W.M
Title : SW846 8260
Last Update : Mon May 18 13:09:55 2020

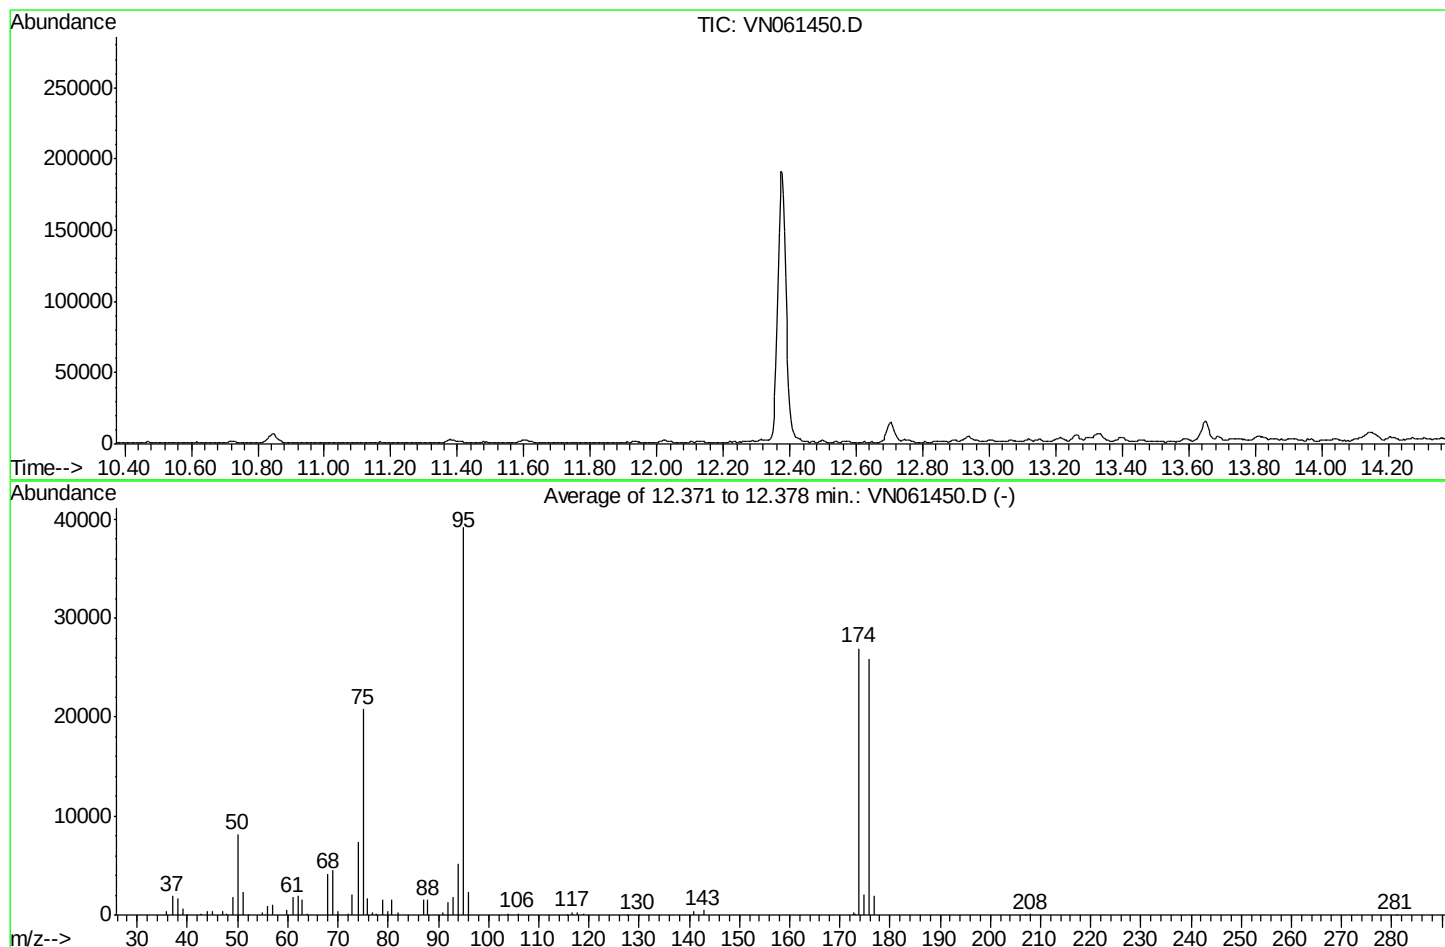

AutoFind: Scans 3296, 3297, 3298; Background Corrected with Scan 3284

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.7	8123	PASS
75	95	30	60	53.1	20810	PASS
95	95	100	100	100.0	39168	PASS
96	95	5	9	5.9	2300	PASS
173	174	0.00	2	0.8	221	PASS
174	95	50	100	68.7	26912	PASS
175	174	5	9	7.9	2113	PASS
176	174	95	101	96.3	25904	PASS
177	176	5	9	7.3	1886	PASS