

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN051821\
 Data File : VN067129.D
 Acq On : 18 May 2021 16:03
 Operator : JC/MD
 Sample : M2387-08
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :

Quant Time: May 19 02:50:18 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N051421W.M
 Quant Title : SW846 8260
 QLast Update : Tue May 18 04:00:15 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.597	168	649247	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.525	114	901528	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.360	117	767296	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.301	152	325210	50.00	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	7.959	65	317258	45.23	ug/l	0.00
Spiked Amount	50.000	Range	61 - 141	Recovery	=	90.46%
35) Dibromofluoromethane	7.519	113	292658	49.44	ug/l	0.00
Spiked Amount	50.000	Range	69 - 133	Recovery	=	98.88%
50) Toluene-d8	10.037	98	1109949	49.47	ug/l	0.00
Spiked Amount	50.000	Range	65 - 126	Recovery	=	98.94%
62) 4-Bromofluorobenzene	12.357	95	332267	44.21	ug/l	0.00
Spiked Amount	50.000	Range	58 - 135	Recovery	=	88.42%


Target Compounds						Qvalue
3) Chloromethane	2.059	50	2163	0.30	ug/l #	86
11) Tert butyl alcohol	4.724	59	51297	43.87	ug/l #	77
13) Acrolein	3.569	56	2724	Below Cal	#	51
16) Acetone	3.772	43	45398	20.83	ug/l	98
18) Methyl Acetate	4.274	43	13358	2.06	ug/l #	74
20) Methylene Chloride	4.488	84	3473	0.56	ug/l	96
22) Diisopropyl ether	5.872	45	14029	0.81	ug/l #	1
25) 2-Butanone	6.760	43	48838	14.37	ug/l	98
31) Cyclohexane	7.594	56	10579	1.09	ug/l #	1
36) 1,1-Dichloropropene	7.597	75	36832	4.48	ug/l #	49
37) Ethyl Acetate	6.760	43	48838	6.72	ug/l #	65
38) Carbon Tetrachloride	7.600	117	52942	6.05	ug/l #	15
39) Methylcyclohexane	9.029	83	2295	0.24	ug/l	95
40) Benzene	7.975	78	77330	3.10	ug/l	99
41) Methacrylonitrile	7.122	41	1379	0.47	ug/l #	33
43) Isopropyl Acetate	8.203	43	10136	0.84	ug/l #	65
48) Methyl methacrylate	9.077	41	10306	3.65	ug/l #	32
49) 1,4-Dioxane	9.152	88	2001	23.33	ug/l #	27
51) 4-Methyl-2-Pentanone	9.941	43	1957	5.67	ug/l #	55
52) Toluene	10.102	92	72303	4.48	ug/l	99
56) Ethyl methacrylate	10.357	69	230	1.96	ug/l #	79
59) 2-Hexanone	10.467	43	120	21.94	ug/l	78
67) Ethyl Benzene	11.470	91	11568	0.40	ug/l	98
68) m/p-Xylenes	11.574	106	25625	2.30	ug/l	89
69) o-Xylene	11.907	106	10269	0.92	ug/l	96
71) Bromoform	12.363	173	619	1.86	ug/l #	1
76) 1,2,3-Trichloropropane	12.357	75	154726	22.55	ug/l #	100
80) 1,3,5-Trimethylbenzene	12.693	105	8545	0.38	ug/l	90
81) trans-1,4-Dichloro-2-b...	12.357	75	154726	67.65	ug/l #	15
82) 4-Chlorotoluene	12.682	91	922	1.23	ug/l #	39
84) 1,2,4-Trimethylbenzene	13.001	105	23164	1.11	ug/l	100
95) Naphthalene	15.098	128	18453	4.50	ug/l #	87


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN051821\
Data File : VN067129.D
Acq On : 18 May 2021 16:03
Operator : JC/MD
Sample : M2387-08
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :

Quant Time: May 19 02:50:18 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N051421W.M
Quant Title : SW846 8260
QLast Update : Tue May 18 04:00:15 2021
Response via : Initial Calibration




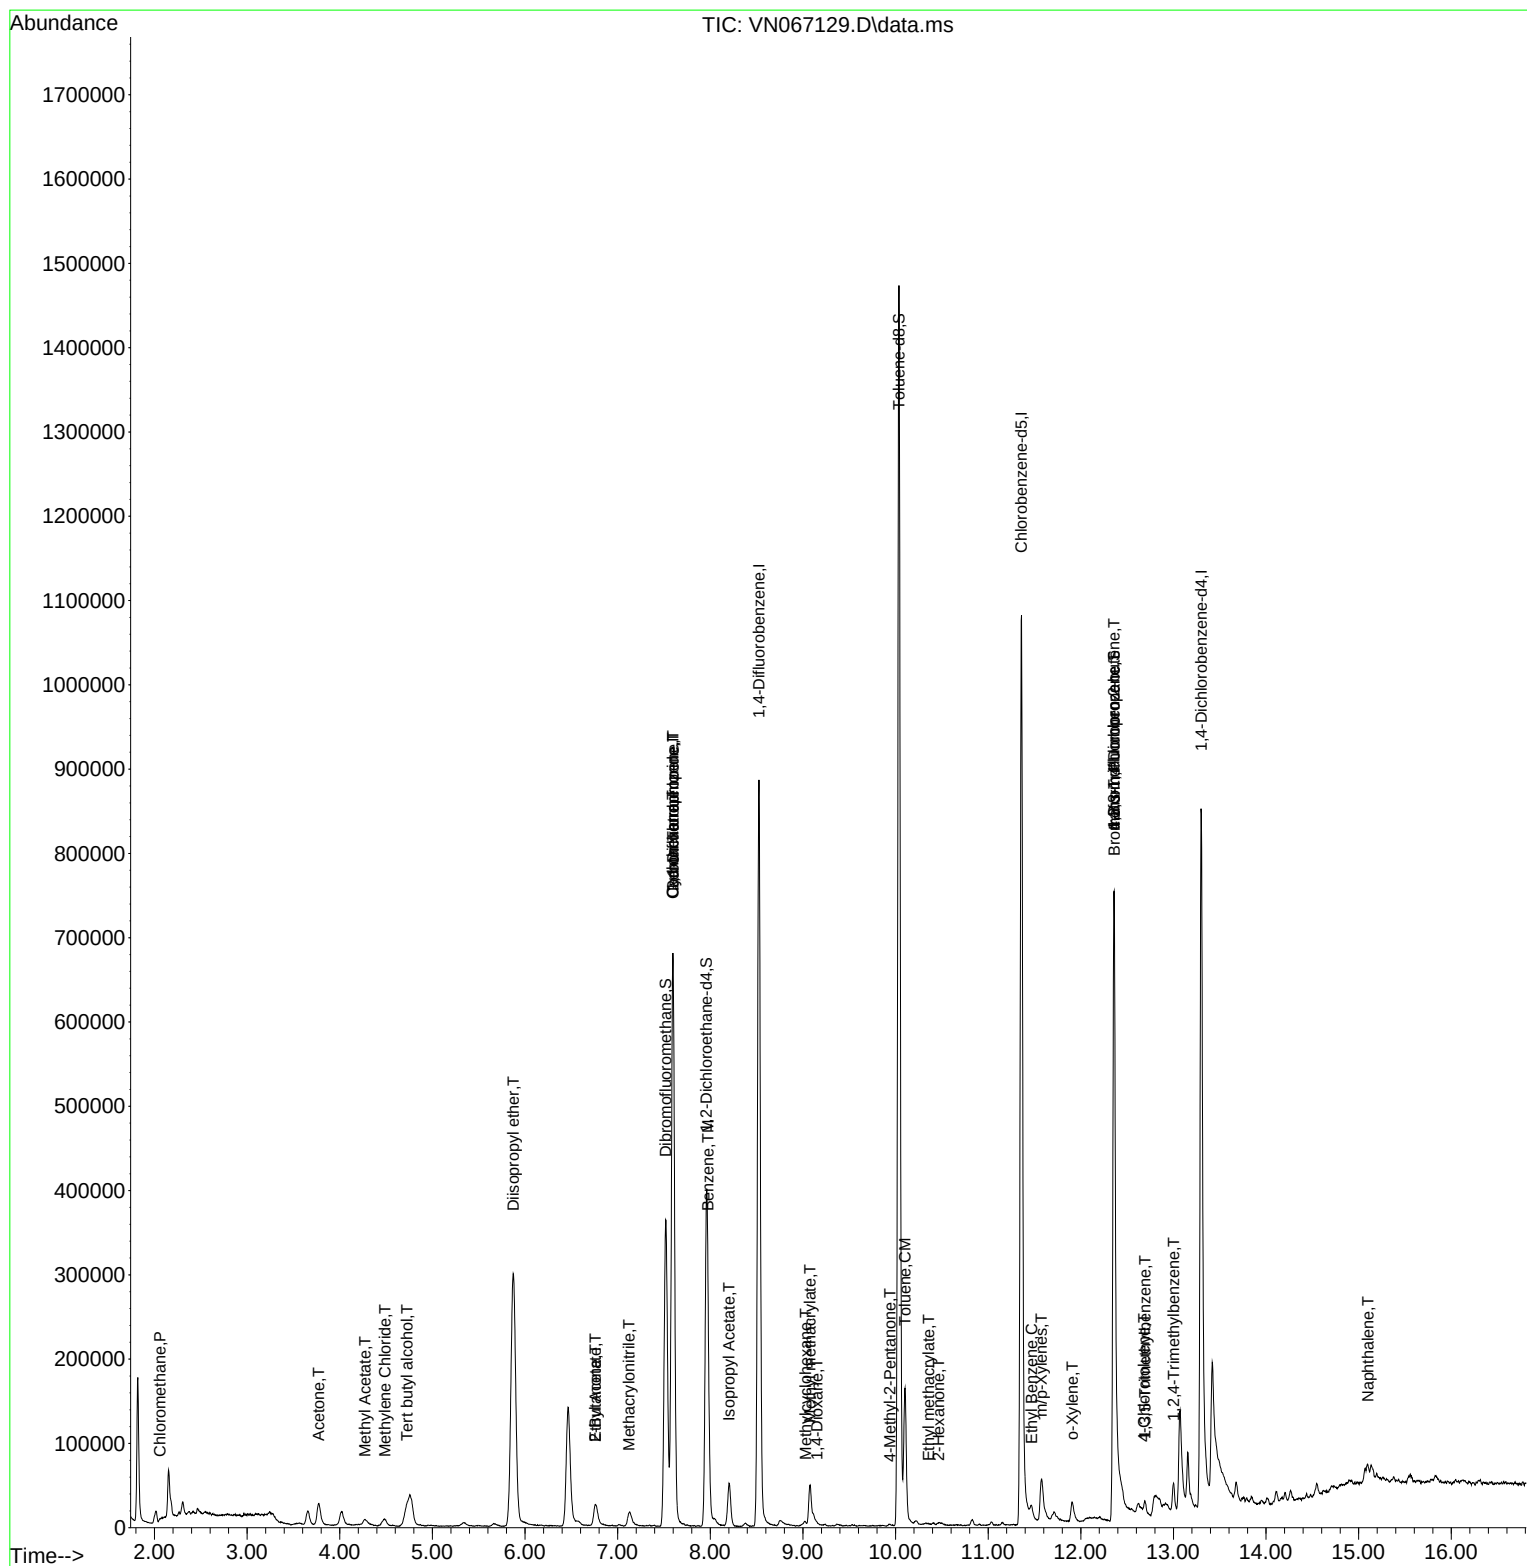




#1
Pentafluorobenzene
Concen: 50.00 ug/l
RT: 7.597 min Scan# 2184
Delta R.T. -0.000 min
Lab File: VN067129.D
Acq: 18 May 2021 16:03




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion:168 Resp: 649247
Ion Ratio Lower Upper
168 100
99 46.1 38.5 57.7

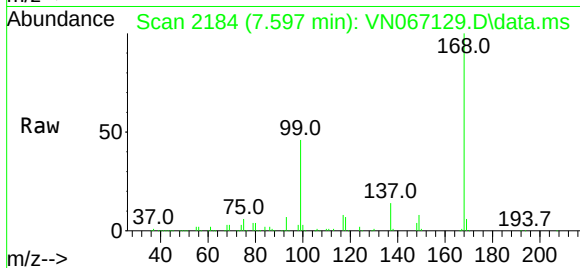

#3
Chloromethane
Concen: 0.30 ug/l
RT: 2.059 min Scan# 119
Delta R.T. 0.006 min
Lab File: VN067129.D
Acq: 18 May 2021 16:03

Tgt Ion: 50 Resp: 2163
Ion Ratio Lower Upper
50 100
52 41.3 26.5 39.7#


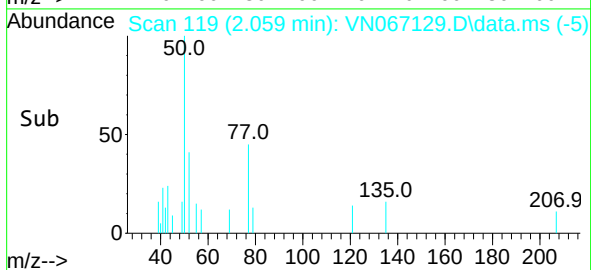

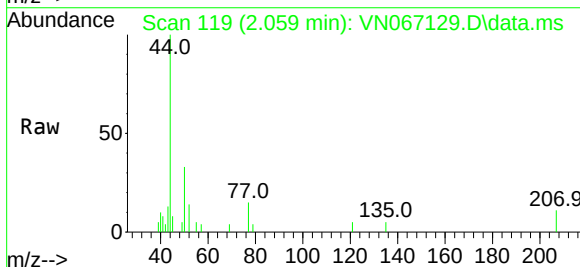




#11
Tert butyl alcohol
Concen: 43.87 ug/l
RT: 4.724 min Scan# 1113
Delta R.T. 0.010 min
Lab File: VN067129.D
Acq: 18 May 2021 16:03




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion: 59 Resp: 51297
Ion Ratio Lower Upper
59 100
57 12.0 3.5 5.3#

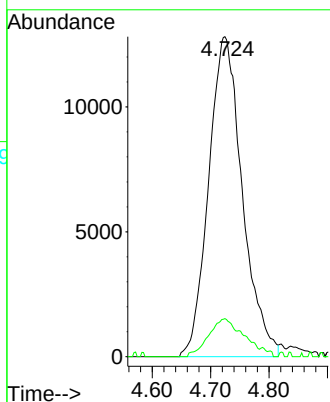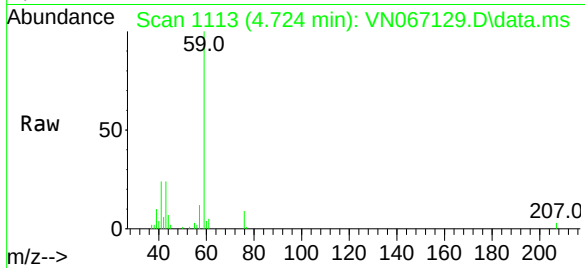

#16
Acetone
Concen: 20.83 ug/l
RT: 3.772 min Scan# 758
Delta R.T. 0.008 min
Lab File: VN067129.D
Acq: 18 May 2021 16:03


Tgt Ion: 43 Resp: 45398
Ion Ratio Lower Upper
43 100
58 32.8 27.2 40.8

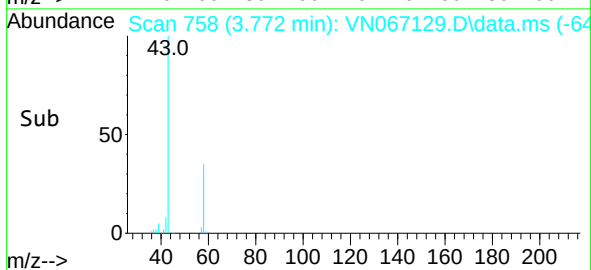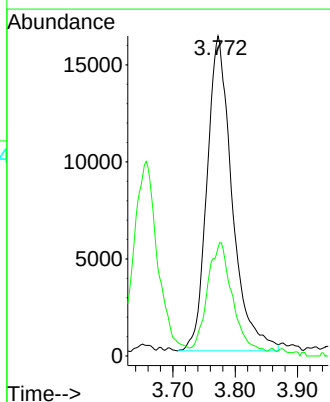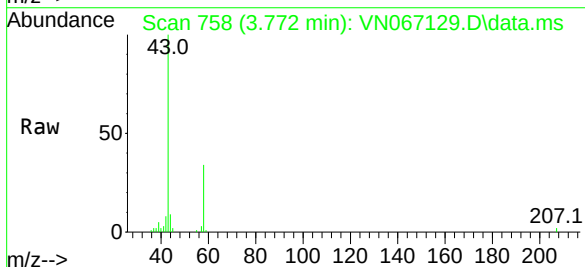






#18
Methyl Acetate
Concen: 2.06 ug/l
RT: 4.274 min Scan# 945
Delta R.T. 0.011 min
Lab File: VN067129.D
Acq: 18 May 2021 16:03

Instrument :
MSVOA_N
ClientSampled :







Tgt Ion: 43 Resp: 13358
Ion Ratio Lower Upper
43 100
74 13.4 21.4 32.2#



#20
Methylene Chloride
Concen: 0.56 ug/l
RT: 4.488 min Scan# 1025
Delta R.T. 0.005 min
Lab File: VN067129.D
Acq: 18 May 2021 16:03

Tgt Ion: 84 Resp: 3473
Ion Ratio Lower Upper
84 100
49 104.3 88.3 132.5
51 30.6 26.7 40.1
86 64.8 51.1 76.7





#22

Diisopropyl ether

Concen: 0.81 ug/l





RT: 5.872 min Scan# 1541

Delta R.T. 0.000 min

Lab File: VN067129.D

Acq: 18 May 2021 16:03

Tgt Ion:	45	Resp:	14029
Ion	Ratio	Lower	Upper
45	100		
43	9.2	55.6	83.4#
87	0.0	26.5	39.7#
59	208.3	10.0	15.0#

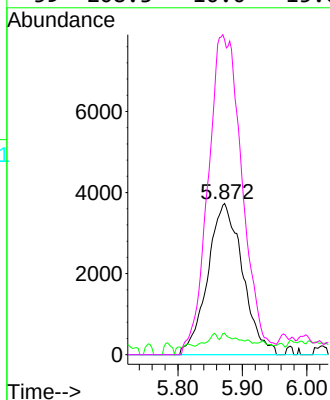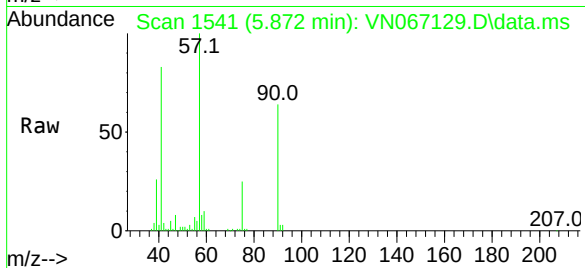

#25

2-Butanone

Concen: 14.37 ug/l




RT: 6.760 min Scan# 1872


Delta R.T. 0.008 min

Lab File: VN067129.D

Acq: 18 May 2021 16:03


Tgt Ion:	43	Resp:	48838
Ion	Ratio	Lower	Upper
43	100		
72	29.5	24.4	36.6

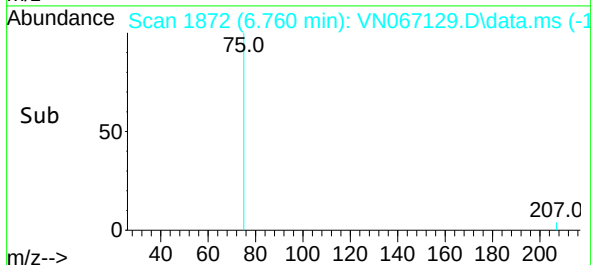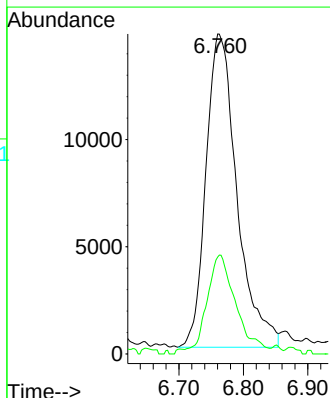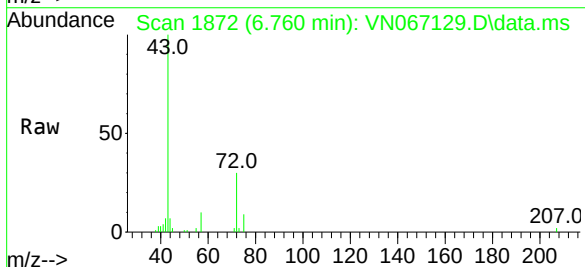






#31
Cyclohexane
Concen: 1.09 ug/l
RT: 7.594 min Scan# 2183
Delta R.T. 0.011 min
Lab File: VN067129.D
Acq: 18 May 2021 16:03

Instrument :
MSVOA_N
ClientSampleId :







Tgt Ion: 56 Resp: 10579
Ion Ratio Lower Upper
56 100
69 182.1 28.0 42.0#
84 133.2 74.2 111.2#



#33
1,2-Dichloroethane-d4
Concen: 45.23 ug/l
RT: 7.959 min Scan# 2319
Delta R.T. -0.000 min
Lab File: VN067129.D
Acq: 18 May 2021 16:03

Tgt Ion: 65 Resp: 317258
Ion Ratio Lower Upper
65 100
67 53.6 0.0 110.4


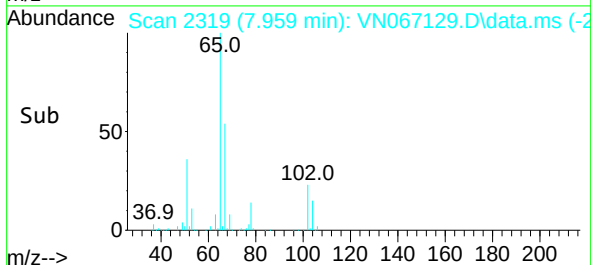






#34
1,4-Difluorobenzene
Concen: 50.00 ug/l
RT: 8.525 min Scan# 2530
Delta R.T. -0.000 min
Lab File: VN067129.D
Acq: 18 May 2021 16:03




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion	Ratio	Lower	Upper
114	100		
63	17.5	0.0	35.8
88	15.2	0.0	30.4

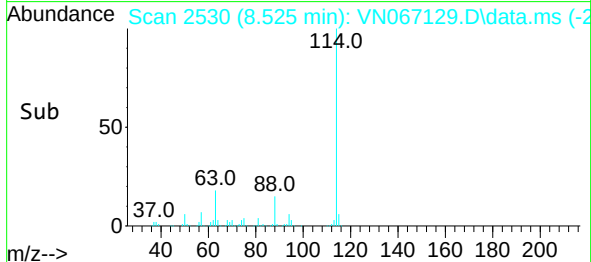

#35
Dibromofluoromethane
Concen: 49.44 ug/l
RT: 7.519 min Scan# 2155
Delta R.T. -0.003 min
Lab File: VN067129.D
Acq: 18 May 2021 16:03

Tgt Ion	Ratio	Lower	Upper
113	100		
111	102.7	82.6	124.0
192	24.0	18.2	27.4


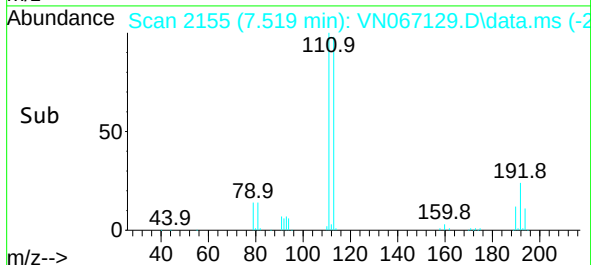






#36
1,1-Dichloropropene
Concen: 4.48 ug/l
RT: 7.597 min Scan# 2184
Delta R.T. -0.126 min
Lab File: VN067129.D
Acq: 18 May 2021 16:03




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion: 75 Resp: 36832
Ion Ratio Lower Upper
75 100
110 10.2 19.1 57.3#
77 0.0 24.8 37.2#



#37
Ethyl Acetate
Concen: 6.72 ug/l
RT: 6.760 min Scan# 1872
Delta R.T. -0.089 min
Lab File: VN067129.D
Acq: 18 May 2021 16:03


Tgt Ion: 43 Resp: 48838
Ion Ratio Lower Upper
43 100
61 0.0 13.0 19.4#
70 0.0 9.2 13.8#

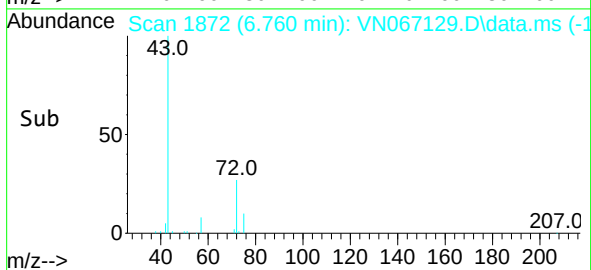






#38
Carbon Tetrachloride
Concen: 6.05 ug/l
RT: 7.600 min Scan# 2185
Delta R.T. -0.107 min
Lab File: VN067129.D
Acq: 18 May 2021 16:03


Instrument :
MSVOA_N
ClientSampleId :





Tgt Ion:117 Resp: 52942
Ion Ratio Lower Upper
117 100
119 4.8 78.2 117.2#
121 0.0 24.7 37.1#




#39
Methylcyclohexane
Concen: 0.24 ug/l
RT: 9.029 min Scan# 2718
Delta R.T. 0.008 min
Lab File: VN067129.D
Acq: 18 May 2021 16:03



Tgt Ion: 83 Resp: 2295
Ion Ratio Lower Upper
83 100
55 74.3 56.2 84.2
98 48.8 36.8 55.2




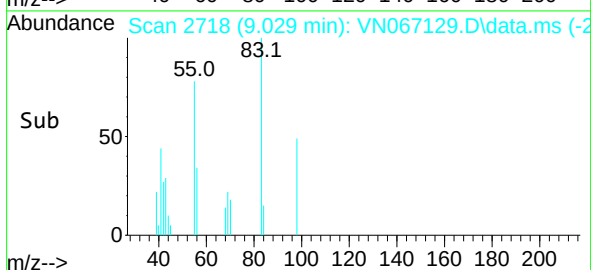




#40
Benzene
Concen: 3.10 ug/l
RT: 7.975 min Scan# 2325
Delta R.T. -0.000 min
Lab File: VN067129.D
Acq: 18 May 2021 16:03




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion: 78 Resp: 77330
Ion Ratio Lower Upper
78 100
77 23.3 18.4 27.6



#41
Methacrylonitrile
Concen: 0.47 ug/l
RT: 7.122 min Scan# 2007
Delta R.T. 0.029 min
Lab File: VN067129.D
Acq: 18 May 2021 16:03


Tgt Ion: 41 Resp: 1379
Ion Ratio Lower Upper
41 100
39 55.5 45.3 67.9
67 0.0 85.1 127.7#
52 0.0 30.1 45.1#

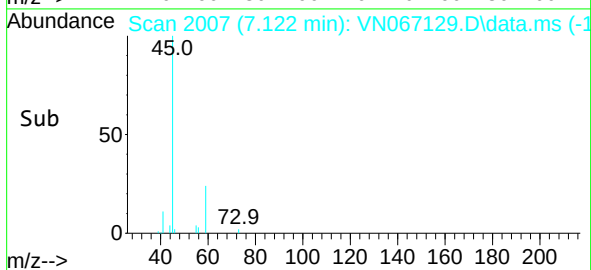






#43
Isopropyl Acetate
Concen: 0.84 ug/l
RT: 8.203 min Scan# 2410
Delta R.T. 0.105 min
Lab File: VN067129.D
Acq: 18 May 2021 16:03

Instrument :
MSVOA_N
ClientSampleId :







Tgt Ion: 43 Resp: 10136
Ion Ratio Lower Upper
43 100
61 11.2 23.4 35.0#
87 0.0 12.2 18.2#



#48
Methyl methacrylate
Concen: 3.65 ug/l
RT: 9.077 min Scan# 2736
Delta R.T. -0.065 min
Lab File: VN067129.D
Acq: 18 May 2021 16:03

Tgt Ion: 41 Resp: 10306
Ion Ratio Lower Upper
41 100
69 0.8 80.5 120.7#
39 47.6 41.4 62.0









#49
1,4-Dioxane
Concen: 23.33 ug/l
RT: 9.152 min Scan# 2764
Delta R.T. 0.008 min
Lab File: VN067129.D
Acq: 18 May 2021 16:03




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion: 88 Resp: 2001
Ion Ratio Lower Upper
88 100
43 0.0 21.8 32.8#
58 0.0 50.8 76.2#



#50
Toluene-d8
Concen: 49.47 ug/l
RT: 10.037 min Scan# 3094
Delta R.T. 0.000 min
Lab File: VN067129.D
Acq: 18 May 2021 16:03

Tgt Ion: 98 Resp: 1109949
Ion Ratio Lower Upper
98 100
100 65.0 51.8 77.8


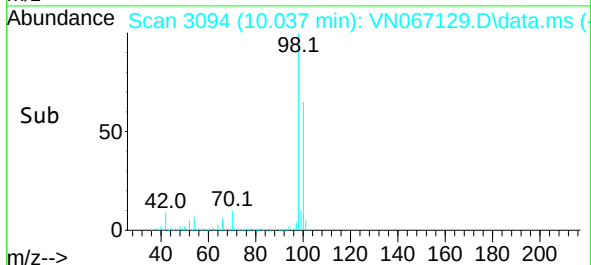

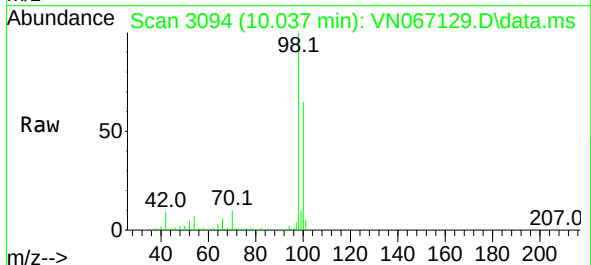




#51
4-Methyl-2-Pentanone
Concen: 5.67 ug/l
RT: 9.941 min Scan# 3058
Delta R.T. 0.013 min
Lab File: VN067129.D
Acq: 18 May 2021 16:03




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion: 43 Resp: 1957
Ion Ratio Lower Upper
43 100
58 14.6 34.5 51.7#

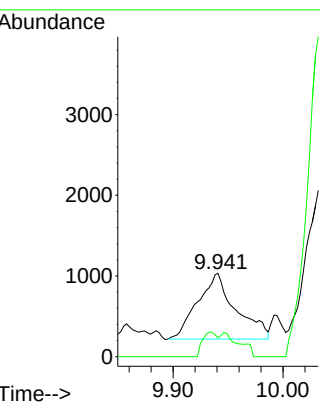

#52
Toluene
Concen: 4.48 ug/l
RT: 10.102 min Scan# 3118
Delta R.T. -0.000 min
Lab File: VN067129.D
Acq: 18 May 2021 16:03

Tgt Ion: 92 Resp: 72303
Ion Ratio Lower Upper
92 100
91 174.3 138.7 208.1


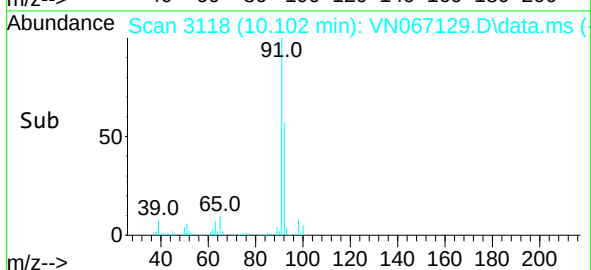
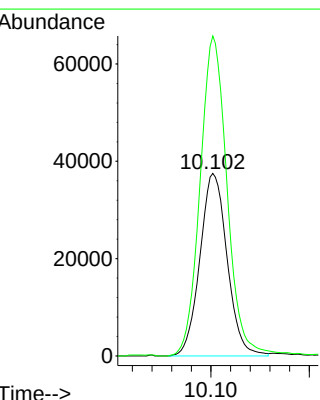





#56
Ethyl methacrylate
Concen: 1.96 ug/l
RT: 10.357 min Scan# 3213
Delta R.T. -0.021 min
Lab File: VN067129.D
Acq: 18 May 2021 16:03




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion: 69 Resp: 230
Ion Ratio Lower Upper
69 100
41 53.9 45.5 68.3
39 0.0 22.9 34.3#



#59
2-Hexanone
Concen: 21.94 ug/l
RT: 10.467 min Scan# 3254
Delta R.T. -0.236 min
Lab File: VN067129.D
Acq: 18 May 2021 16:03


Tgt Ion: 43 Resp: 120
Ion Ratio Lower Upper
43 100
58 43.3 29.8 89.5

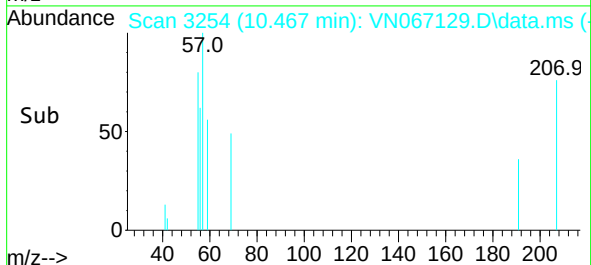



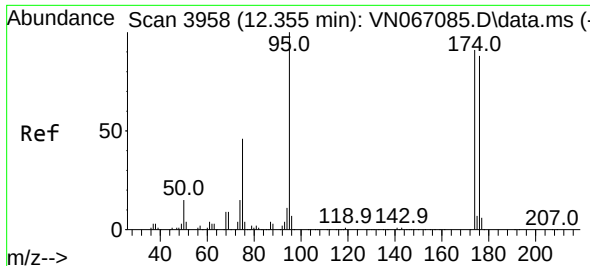


#62
4-Bromofluorobenzene
Concen: 44.21 ug/l
RT: 12.357 min Scan# 3959
Delta R.T. 0.002 min
Lab File: VN067129.D
Acq: 18 May 2021 16:03


Instrument :
MSVOA_N
ClientSampleId :

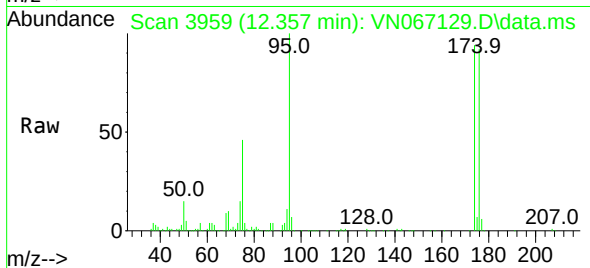



Tgt Ion: 95 Resp: 332267
Ion Ratio Lower Upper
95 100
174 96.6 0.0 182.8
176 94.6 0.0 176.6

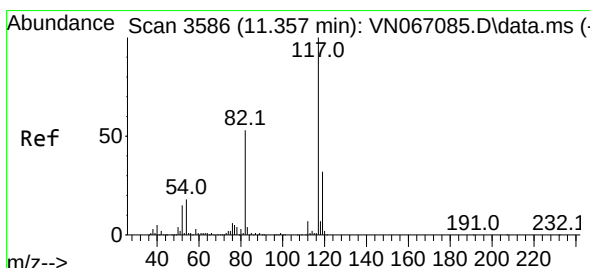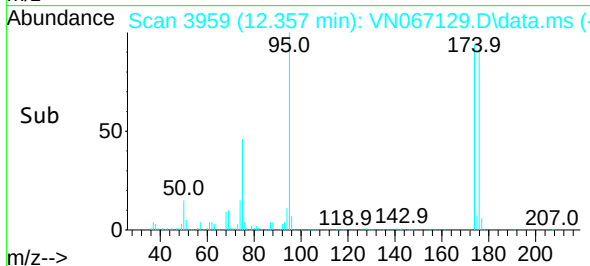


#63
Chlorobenzene-d5
Concen: 50.00 ug/l
RT: 11.360 min Scan# 3587
Delta R.T. 0.003 min
Lab File: VN067129.D
Acq: 18 May 2021 16:03

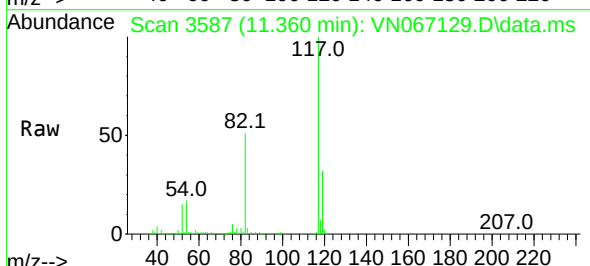

Tgt Ion: 117 Resp: 767296
Ion Ratio Lower Upper
117 100
82 50.8 42.2 63.2
119 31.9 25.8 38.6




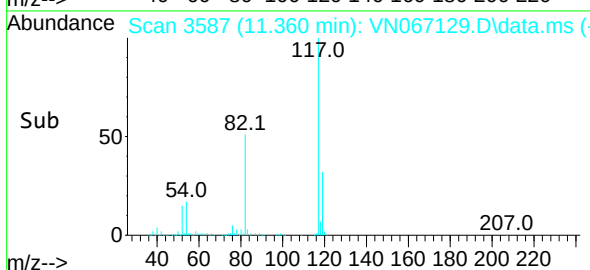




#67
Ethyl Benzene
Concen: 0.40 ug/l
RT: 11.470 min Scan# 3628
Delta R.T. 0.008 min
Lab File: VN067129.D
Acq: 18 May 2021 16:03




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion: 91 Resp: 11568
Ion Ratio Lower Upper
91 100
106 33.7 26.2 39.2



#68
m/p-Xylenes
Concen: 2.30 ug/l
RT: 11.574 min Scan# 3667
Delta R.T. 0.000 min
Lab File: VN067129.D
Acq: 18 May 2021 16:03

Tgt Ion: 106 Resp: 25625
Ion Ratio Lower Upper
106 100
91 177.0 155.2 232.8


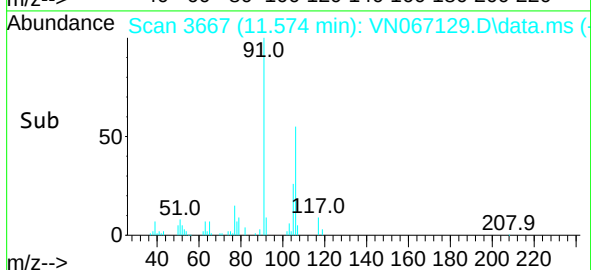




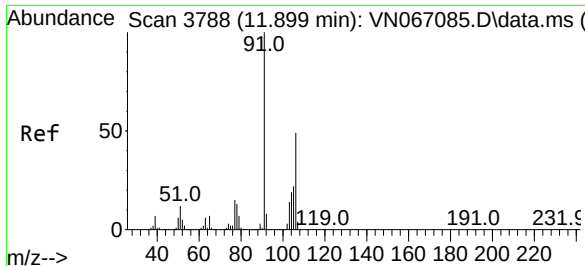

#69
o-Xylene
Concen: 0.92 ug/l
RT: 11.907 min Scan# 3791
Delta R.T. 0.008 min
Lab File: VN067129.D
Acq: 18 May 2021 16:03




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion:106 Resp: 10269
Ion Ratio Lower Upper
106 100
91 198.5 102.3 306.8

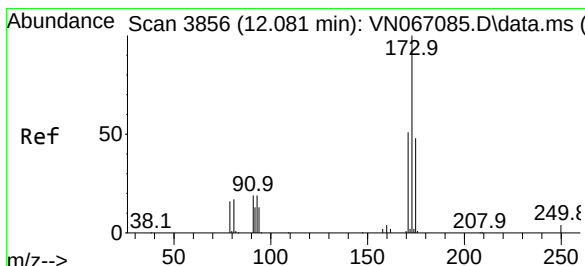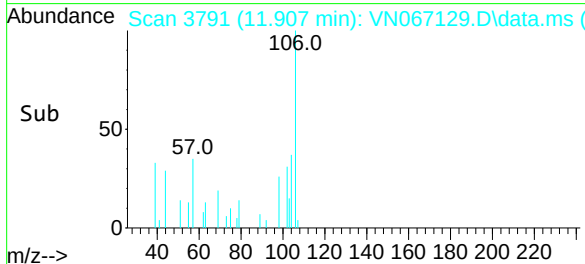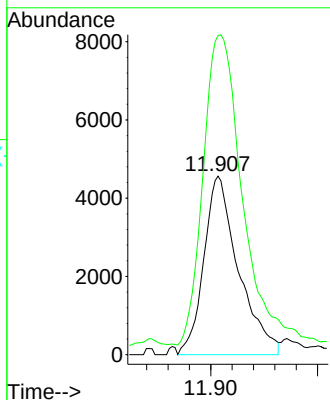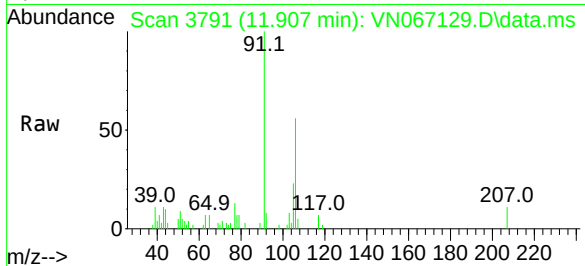

#71
Bromoform
Concen: 1.86 ug/l
RT: 12.363 min Scan# 3961
Delta R.T. 0.282 min
Lab File: VN067129.D
Acq: 18 May 2021 16:03

Tgt Ion:173 Resp: 619
Ion Ratio Lower Upper
173 100
175 2627.1 24.3 73.0#
254 0.0 0.0 0.0

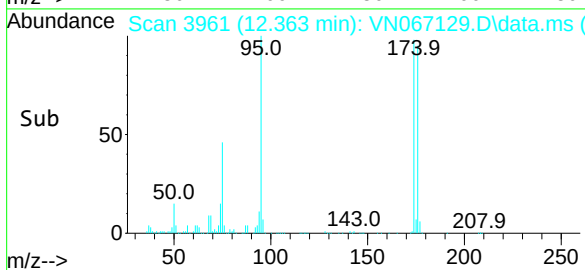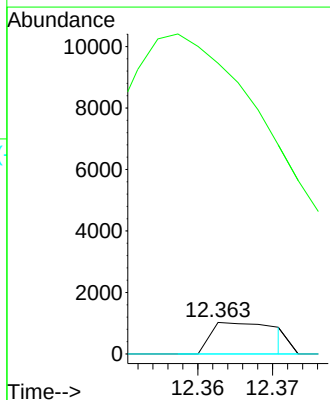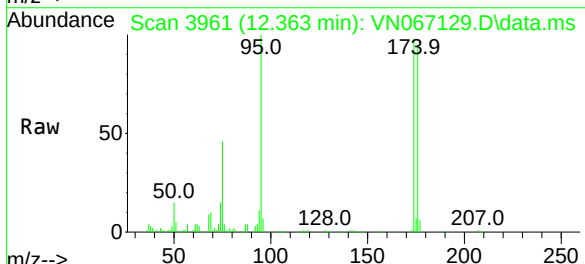



#72

1,4-Dichlorobenzene-d4

Concen: 50.00 ug/l

RT: 13.301 min Scan# 4311

Delta R.T. 0.002 min

Lab File: VN067129.D

Acq: 18 May 2021 16:03





Tgt Ion:152 Resp: 325210

Ion Ratio Lower Upper

152 100

115 52.6 27.0 80.8

150 159.8 0.0 350.2

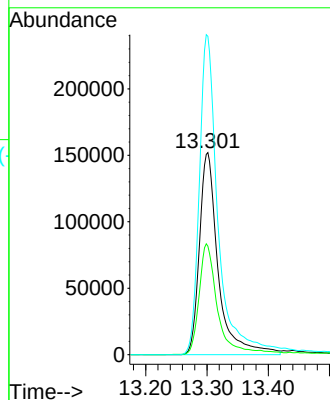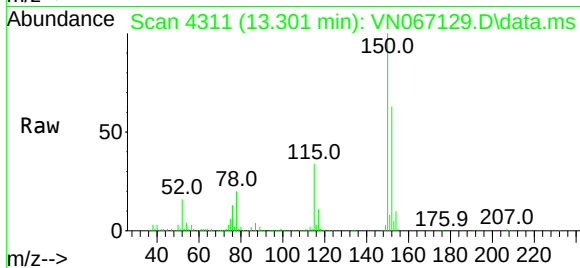

#76

1,2,3-Trichloropropane

Concen: 22.55 ug/l

RT: 12.357 min Scan# 3959

Delta R.T. -0.151 min

Lab File: VN067129.D




Acq: 18 May 2021 16:03


Tgt Ion: 75 Resp: 154726

Ion Ratio Lower Upper

75 100

77 0.9 0.0 0.0#

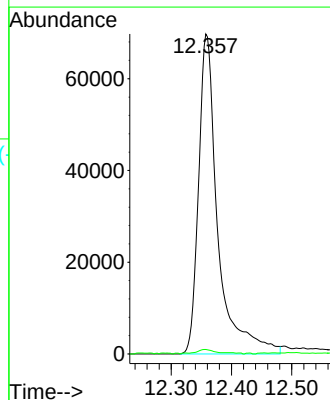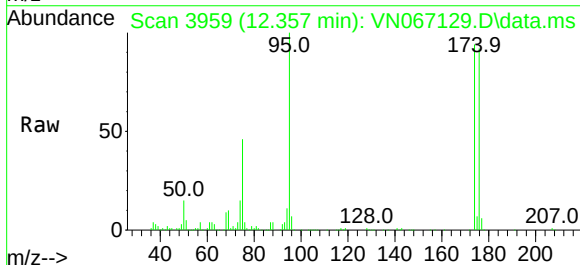



#80

1,3,5-Trimethylbenzene

Concen: 0.38 ug/l

RT: 12.693 min Scan# 4084

Delta R.T. 0.006 min

Lab File: VN067129.D





Acq: 18 May 2021 16:03

Tgt Ion:105 Resp: 8545

Ion Ratio Lower Upper

105 100

120 56.6 25.0 75.0

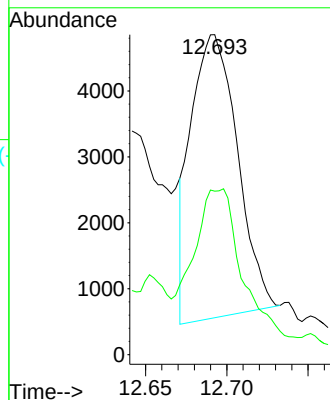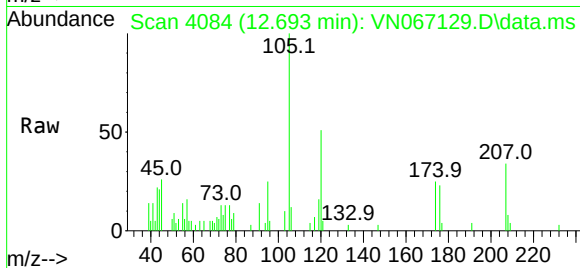

#81

trans-1,4-Dichloro-2-butene

Concen: 67.65 ug/l

RT: 12.357 min Scan# 3959

Delta R.T. 0.102 min

Lab File: VN067129.D

Acq: 18 May 2021 16:03




Tgt Ion: 75 Resp: 154726


Ion Ratio Lower Upper

75 100

53 0.1 66.3 99.5#

89 0.0 39.5 59.3#


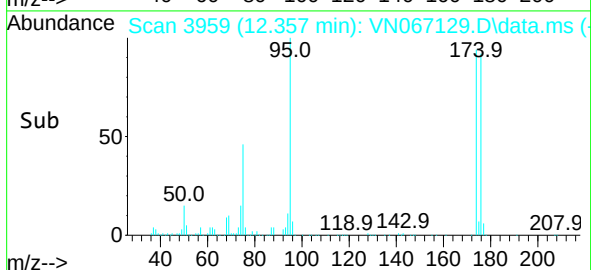
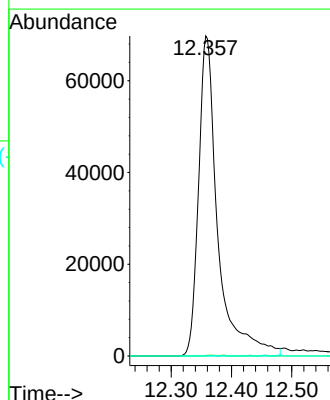
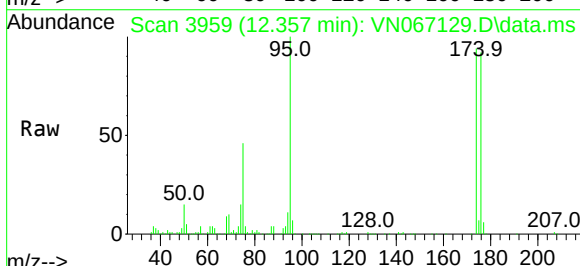




#82
4-Chlorotoluene
Concen: 1.23 ug/l
RT: 12.682 min Scan# 4080
Delta R.T. -0.045 min
Lab File: VN067129.D
Acq: 18 May 2021 16:03




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion: 91 Resp: 922
Ion Ratio Lower Upper
91 100
126 0.0 17.7 53.1#

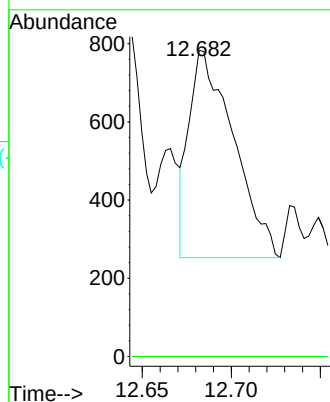

#84
1,2,4-Trimethylbenzene
Concen: 1.11 ug/l
RT: 13.001 min Scan# 4199
Delta R.T. 0.008 min
Lab File: VN067129.D
Acq: 18 May 2021 16:03

Tgt Ion: 105 Resp: 23164
Ion Ratio Lower Upper
105 100
120 47.3 23.8 71.2

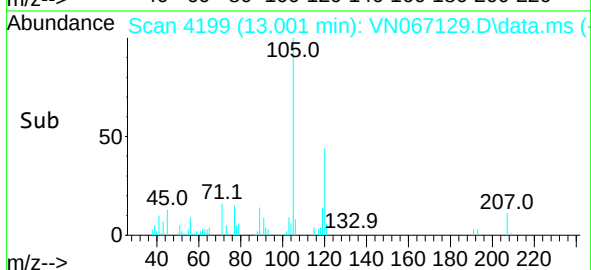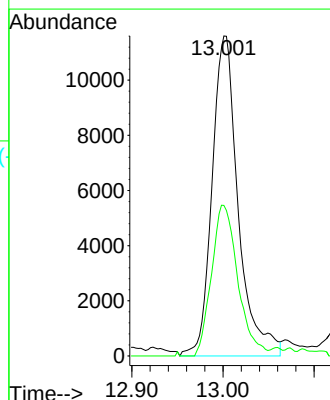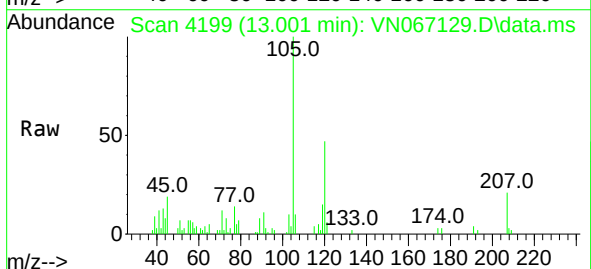

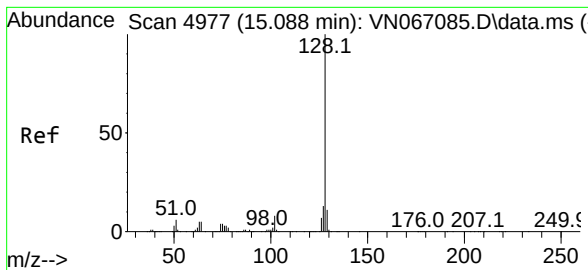

#95
Naphthalene
Concen: 4.50 ug/l
RT: 15.098 min Scan# 4981
Delta R.T. 0.010 min
Lab File: VN067129.D
Acq: 18 May 2021 16:03

Instrument :
MSVOA_N
ClientSampleId :

Tgt Ion	Ratio	Lower	Upper
128	100		
127	14.1	10.2	15.2
129	1.4	8.6	13.0

