


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN051821\
 Data File : VN067117.D
 Acq On : 18 May 2021 10:33
 Operator : JC/MD
 Sample : BFB
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N051421W.M
 Title : SW846 8260
 Last Update : Tue May 18 04:00:15 2021

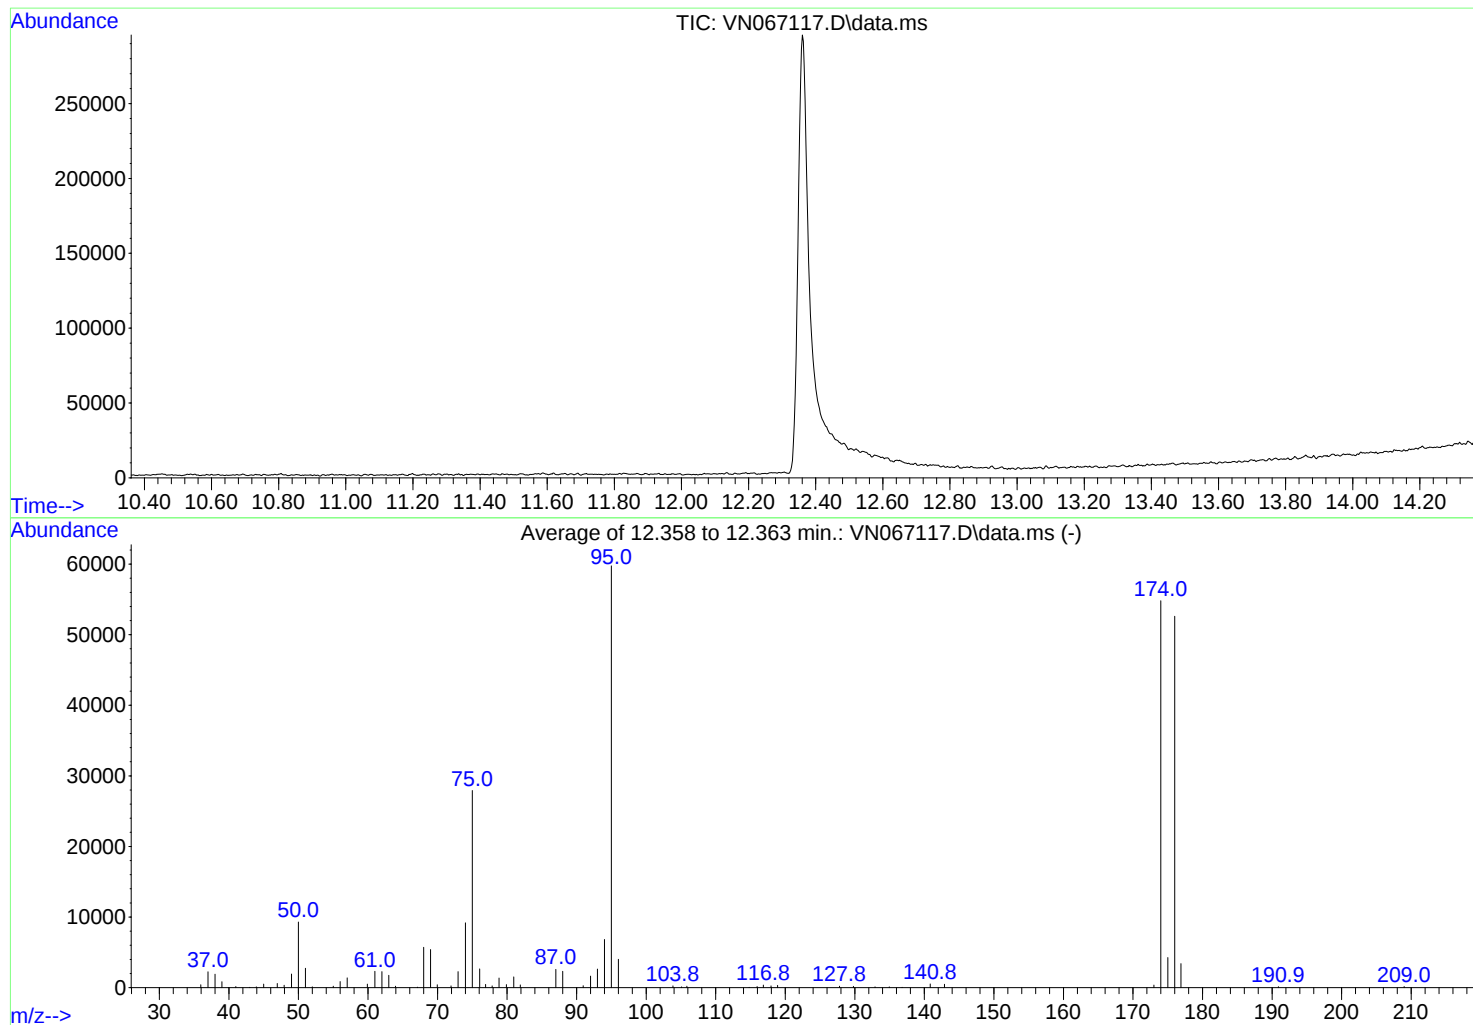

AutoFind: Scans 3959, 3960, 3961; Background Corrected with Scan 3943

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.5	9288	PASS
75	95	30	60	46.7	27920	PASS
95	95	100	100	100.0	59757	PASS
96	95	5	9	6.7	4014	PASS
173	174	0.00	2	0.7	363	PASS
174	95	50	100	91.7	54811	PASS
175	174	5	9	7.8	4268	PASS
176	174	95	101	96.0	52616	PASS
177	176	5	9	6.5	3412	PASS