


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN051822\
Data File : VN072534.D
Acq On : 18 May 2022 09:48
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N051822W.M
Title : SW846 8260
Last Update : Thu May 19 02:22:47 2022

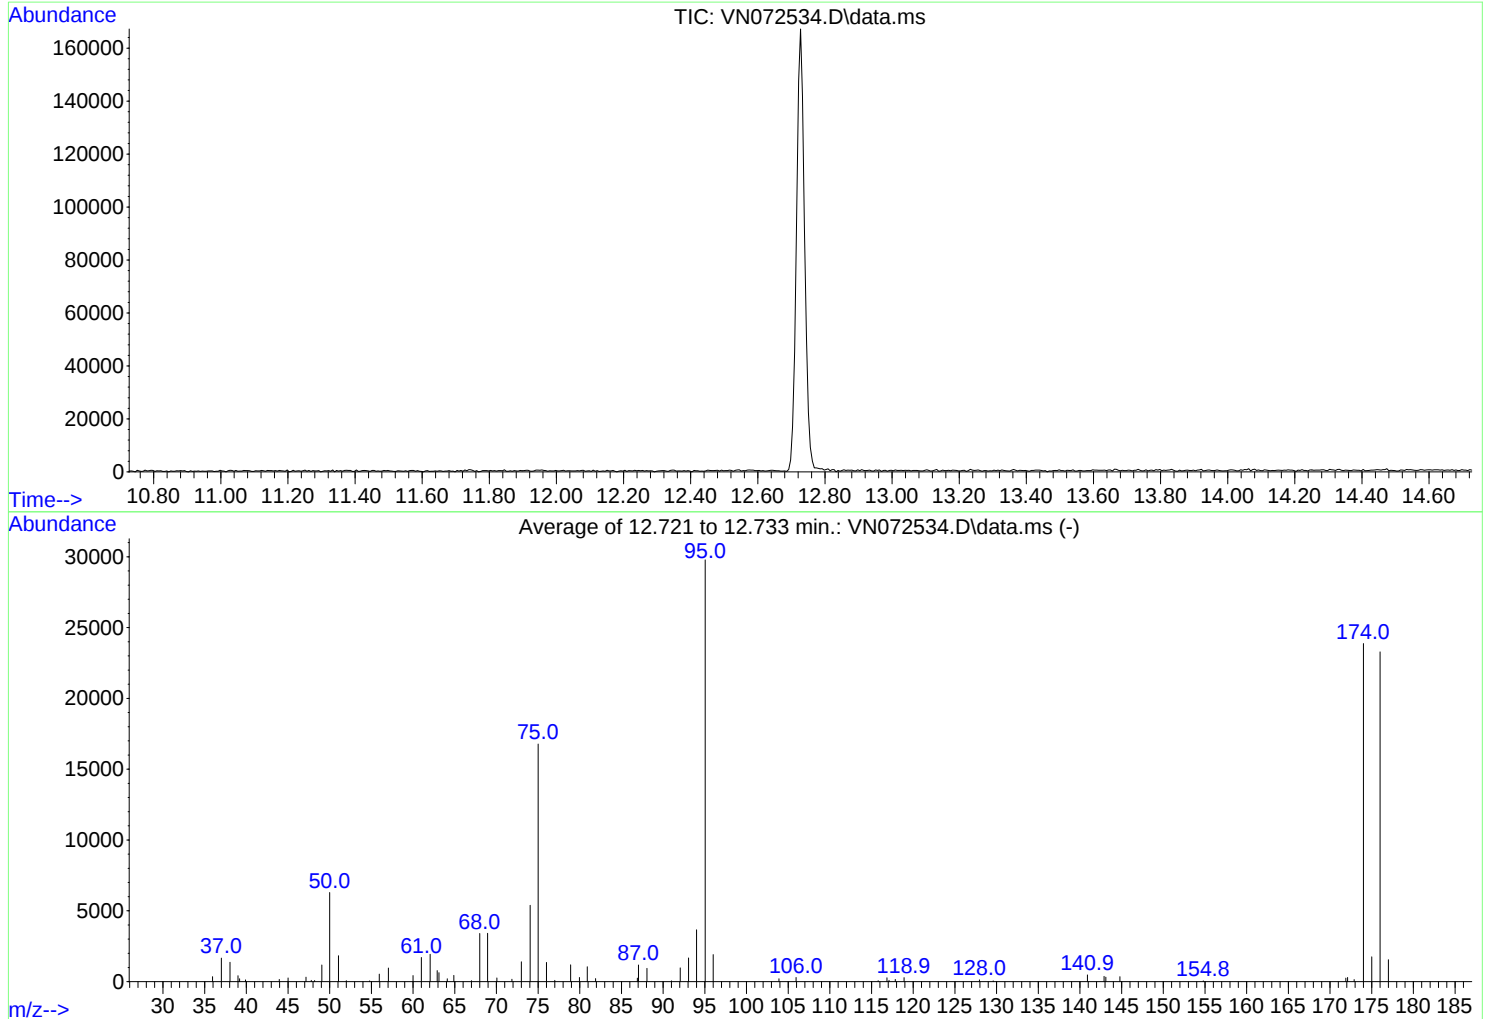

AutoFind: Scans 1825, 1826, 1827; Background Corrected with Scan 1817

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	21.1	6289	PASS
75	95	30	60	56.3	16782	PASS
95	95	100	100	100.0	29784	PASS
96	95	5	9	6.4	1915	PASS
173	174	0.00	2	0.6	151	PASS
174	95	50	100	80.1	23869	PASS
175	174	5	9	7.4	1757	PASS
176	174	95	101	97.6	23285	PASS
177	176	5	9	6.7	1553	PASS