
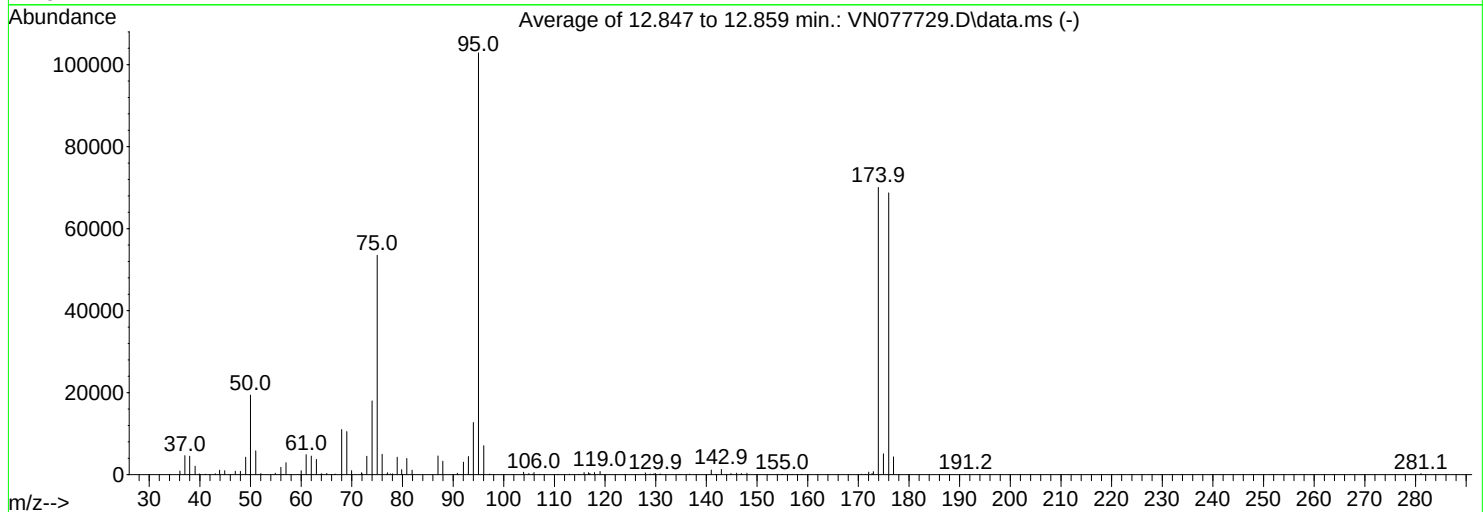


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN051823\
Data File : VN077729.D
Acq On : 18 May 2023 09:24
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N051523W.M
Title : SW846 8260
Last Update : Tue May 16 04:07:42 2023

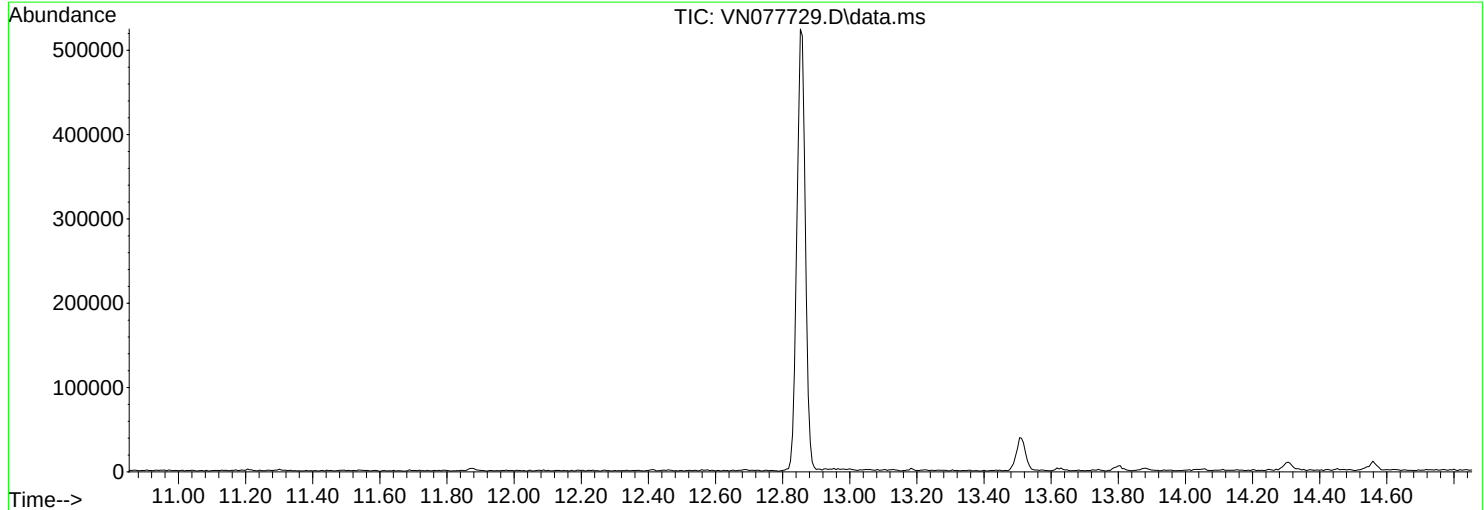

AutoFind: Scans 1852, 1853, 1854; Background Corrected with Scan 1843

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	18.9	19400	PASS
75	95	30	60	52.0	53512	PASS
95	95	100	100	100.0	102885	PASS
96	95	5	9	6.9	7080	PASS
173	174	0.00	2	1.1	741	PASS
174	95	50	100	68.1	70067	PASS
175	174	5	9	7.2	5076	PASS
176	174	95	101	98.1	68725	PASS
177	176	5	9	6.3	4327	PASS

Average of 12.847 to 12.859 min.: VN077729.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.05	916	48.00	838	62.00	4544	72.95	4491
37.05	4653	49.05	4260	63.00	3694	74.00	1798
38.00	4488	50.00	19400	63.80	73	75.00	5351
39.05	2053	51.05	5811	64.05	223	76.00	4941
39.90	192	52.05	288	65.05	310	76.80	107
41.10	109	54.90	353	66.70	164	77.05	489
43.05	221	56.00	1805	68.00	11001	77.60	209
43.90	1104	57.00	2919	69.00	10498	78.05	201
44.90	985	57.90	56	69.95	996	78.95	4243
46.00	73	60.00	995	71.90	462	79.85	1192
47.00	838	61.00	4877	72.10	151	80.85	3959

Average of 12.847 to 12.859 min.: VN077729.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
81.90	1107	103.90	595	117.90	503	140.95	1130
87.00	4564	104.95	268	119.00	789	141.80	58
87.95	3290	105.70	128	123.90	59	142.00	75
90.85	342	105.95	500	127.95	437	142.95	1291
91.10	89	107.00	73	128.90	166	144.00	61
92.05	3033	110.70	61	129.65	251	144.85	278
93.00	4409	112.95	109	129.95	257	145.95	355
94.00	12724	114.80	63	130.90	207	146.90	287
95.00	102885	115.85	492	134.60	62	148.00	364
96.05	7080	116.75	491	135.00	90	154.80	53
97.20	175	117.00	277	136.70	101	155.00	91

Average of 12.847 to 12.859 min.: VN077729.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
156.90	70	178.10	57				
158.80	87	191.20	80				
170.70	111	281.10	291				
171.40	65						
172.05	612						
172.70	265						
172.95	741						
173.95	70067						
174.95	5076						
176.00	68725						
176.95	4327						

Instrument :

MSVOA_N

ClientSampleId :

BFB