


Data Path : Z:\voasrv\HPCHEM1\MSVOA N\Data\VN051920\
Data File : VN061474.D
Acq On : 19 May 2020 10:58
Operator : JC/MD
Sample : BFB
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N051820W.M
Title : SW846 8260
Last Update : Mon May 18 13:09:55 2020

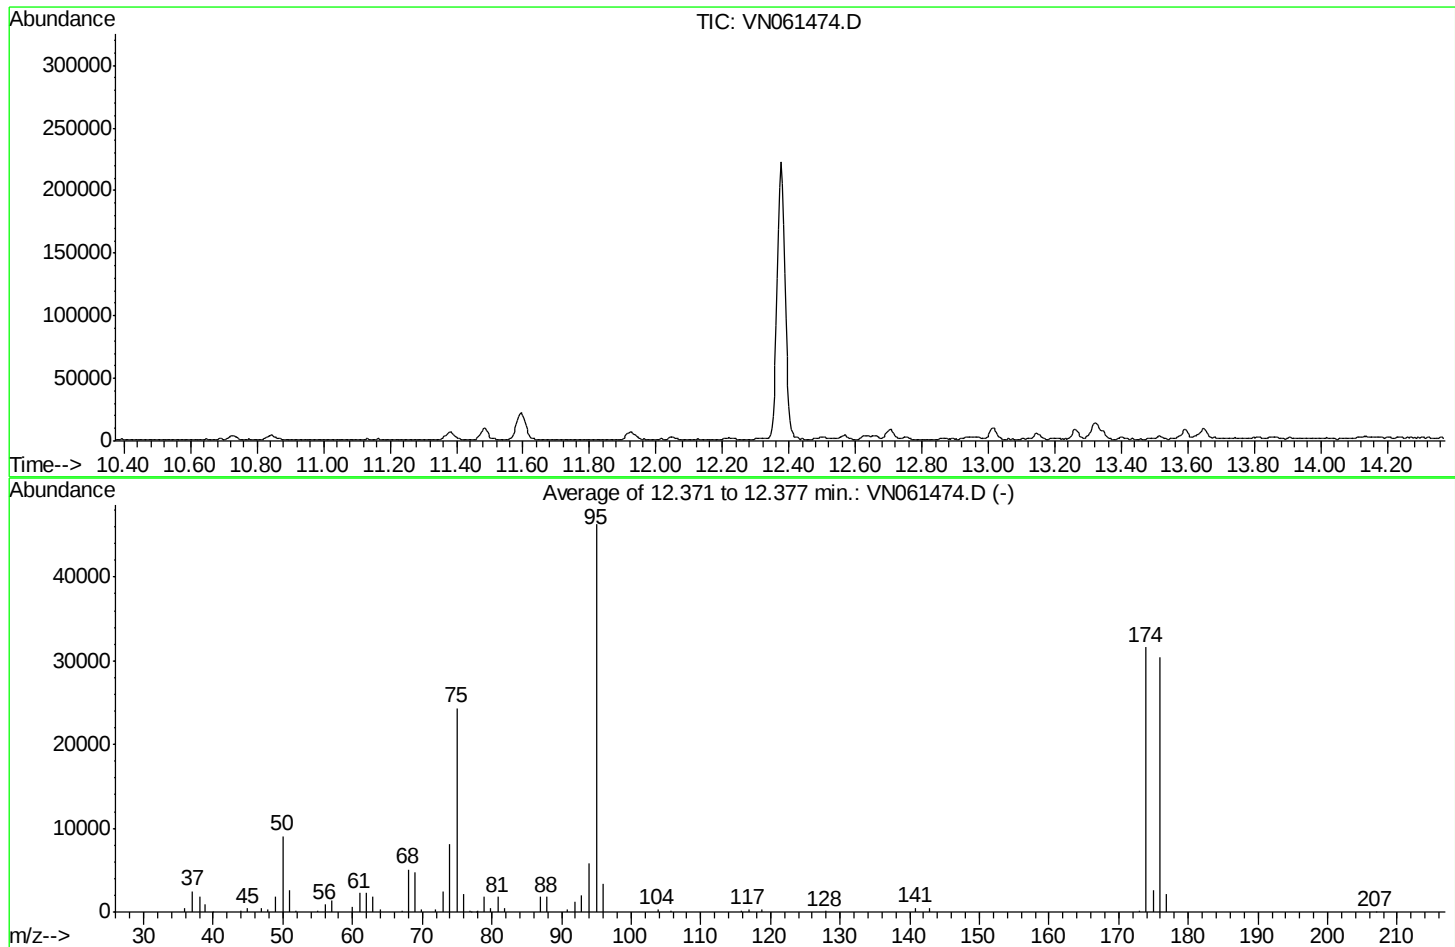

AutoFind: Scans 3296, 3297, 3298; Background Corrected with Scan 3283

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.6	9093	PASS
75	95	30	60	52.5	24325	PASS
95	95	100	100	100.0	46298	PASS
96	95	5	9	7.3	3381	PASS
173	174	0.00	2	0.4	116	PASS
174	95	50	100	68.3	31621	PASS
175	174	5	9	8.3	2639	PASS
176	174	95	101	96.2	30432	PASS
177	176	5	9	7.0	2136	PASS