

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN051921\
 Data File : VN067147.D
 Acq On : 19 May 2021 13:32
 Operator : JC/MD
 Sample : M2392-07
 Misc : 5.04g/10mL/100uL/5.00mL/MSVOA_N/MEOH
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :

Quant Time: May 20 01:54:41 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N051421W.M
 Quant Title : SW846 8260
 QLast Update : Tue May 18 04:00:15 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.589	168	571012	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.519	114	782649	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.360	117	630703	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.301	152	304812	50.00	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	7.954	65	272697	44.21	ug/l	0.00
Spiked Amount	50.000	Range	61 - 141	Recovery	=	88.42%
35) Dibromofluoromethane	7.514	113	258718	50.34	ug/l	0.00
Spiked Amount	50.000	Range	69 - 133	Recovery	=	100.68%
50) Toluene-d8	10.035	98	966040	49.60	ug/l	0.00
Spiked Amount	50.000	Range	65 - 126	Recovery	=	99.20%
62) 4-Bromofluorobenzene	12.360	95	289319	44.34	ug/l	0.00
Spiked Amount	50.000	Range	58 - 135	Recovery	=	88.68%


Target Compounds						Qvalue
3) Chloromethane	2.045	50	1824	0.29	ug/l	99
11) Tert butyl alcohol	4.652	59	7195	7.00	ug/l #	91
13) Acrolein	3.555	56	784	Below Cal	#	75
17) Carbon Disulfide	3.944	76	2939	0.20	ug/l #	74
18) Methyl Acetate	4.271	43	2213	0.39	ug/l #	74
20) Methylene Chloride	4.462	84	1656	0.34	ug/l #	82
31) Cyclohexane	7.586	56	10335	1.22	ug/l #	1
36) 1,1-Dichloropropene	7.589	75	32768	4.59	ug/l #	45
38) Carbon Tetrachloride	7.589	117	46937	6.18	ug/l #	15
39) Methylcyclohexane	9.016	83	19030	2.28	ug/l	98
48) Methyl methacrylate	9.142	41	398	2.02	ug/l #	9
51) 4-Methyl-2-Pentanone	9.965	43	3152	5.89	ug/l #	74
55) 1,1,2-Trichloroethane	10.475	97	7747	1.39	ug/l #	20
56) Ethyl methacrylate	10.375	69	1495	2.11	ug/l #	1
59) 2-Hexanone	10.668	43	16102	25.54	ug/l #	25
71) Bromoform	12.097	173	53	1.77	ug/l #	28
74) N-amyl acetate	11.998	43	24027	5.67	ug/l #	58
75) 1,1,2,2-Tetrachloroethane	12.510	83	11499	1.49	ug/l #	58
76) 1,2,3-Trichloropropane	12.360	75	134334	20.88	ug/l #	100
81) trans-1,4-Dichloro-2-b...	12.360	75	134334	62.98	ug/l #	15
82) 4-Chlorotoluene	12.752	91	613	1.22	ug/l #	1
85) sec-Butylbenzene	13.127	105	7008	0.29	ug/l	96
86) p-Isopropyltoluene	13.248	119	7254	0.35	ug/l	88
87) 1,3-Dichlorobenzene	13.248	146	2434	0.24	ug/l #	74
88) 1,4-Dichlorobenzene	13.320	146	4179	0.39	ug/l #	1
89) n-Butylbenzene	13.580	91	5866	0.37	ug/l #	69
90) Hexachloroethane	13.854	117	2362	0.62	ug/l #	4
92) 1,2-Dibromo-3-Chloropr...	14.251	75	675	0.59	ug/l #	25
93) 1,2,4-Trichlorobenzene	14.873	180	6921	1.28	ug/l #	1
94) Hexachlorobutadiene	14.967	225	2088	0.56	ug/l	94
95) Naphthalene	15.090	128	33513	5.67	ug/l #	72
96) 1,2,3-Trichlorobenzene	15.267	180	3710	0.74	ug/l #	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN051921\
Data File : VN067147.D
Acq On : 19 May 2021 13:32
Operator : JC/MD
Sample : M2392-07
Misc : 5.04g/10mL/100uL/5.00mL/MSVOA_N/MEOH
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :

Quant Time: May 20 01:54:41 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N051421W.M
Quant Title : SW846 8260
QLast Update : Tue May 18 04:00:15 2021
Response via : Initial Calibration




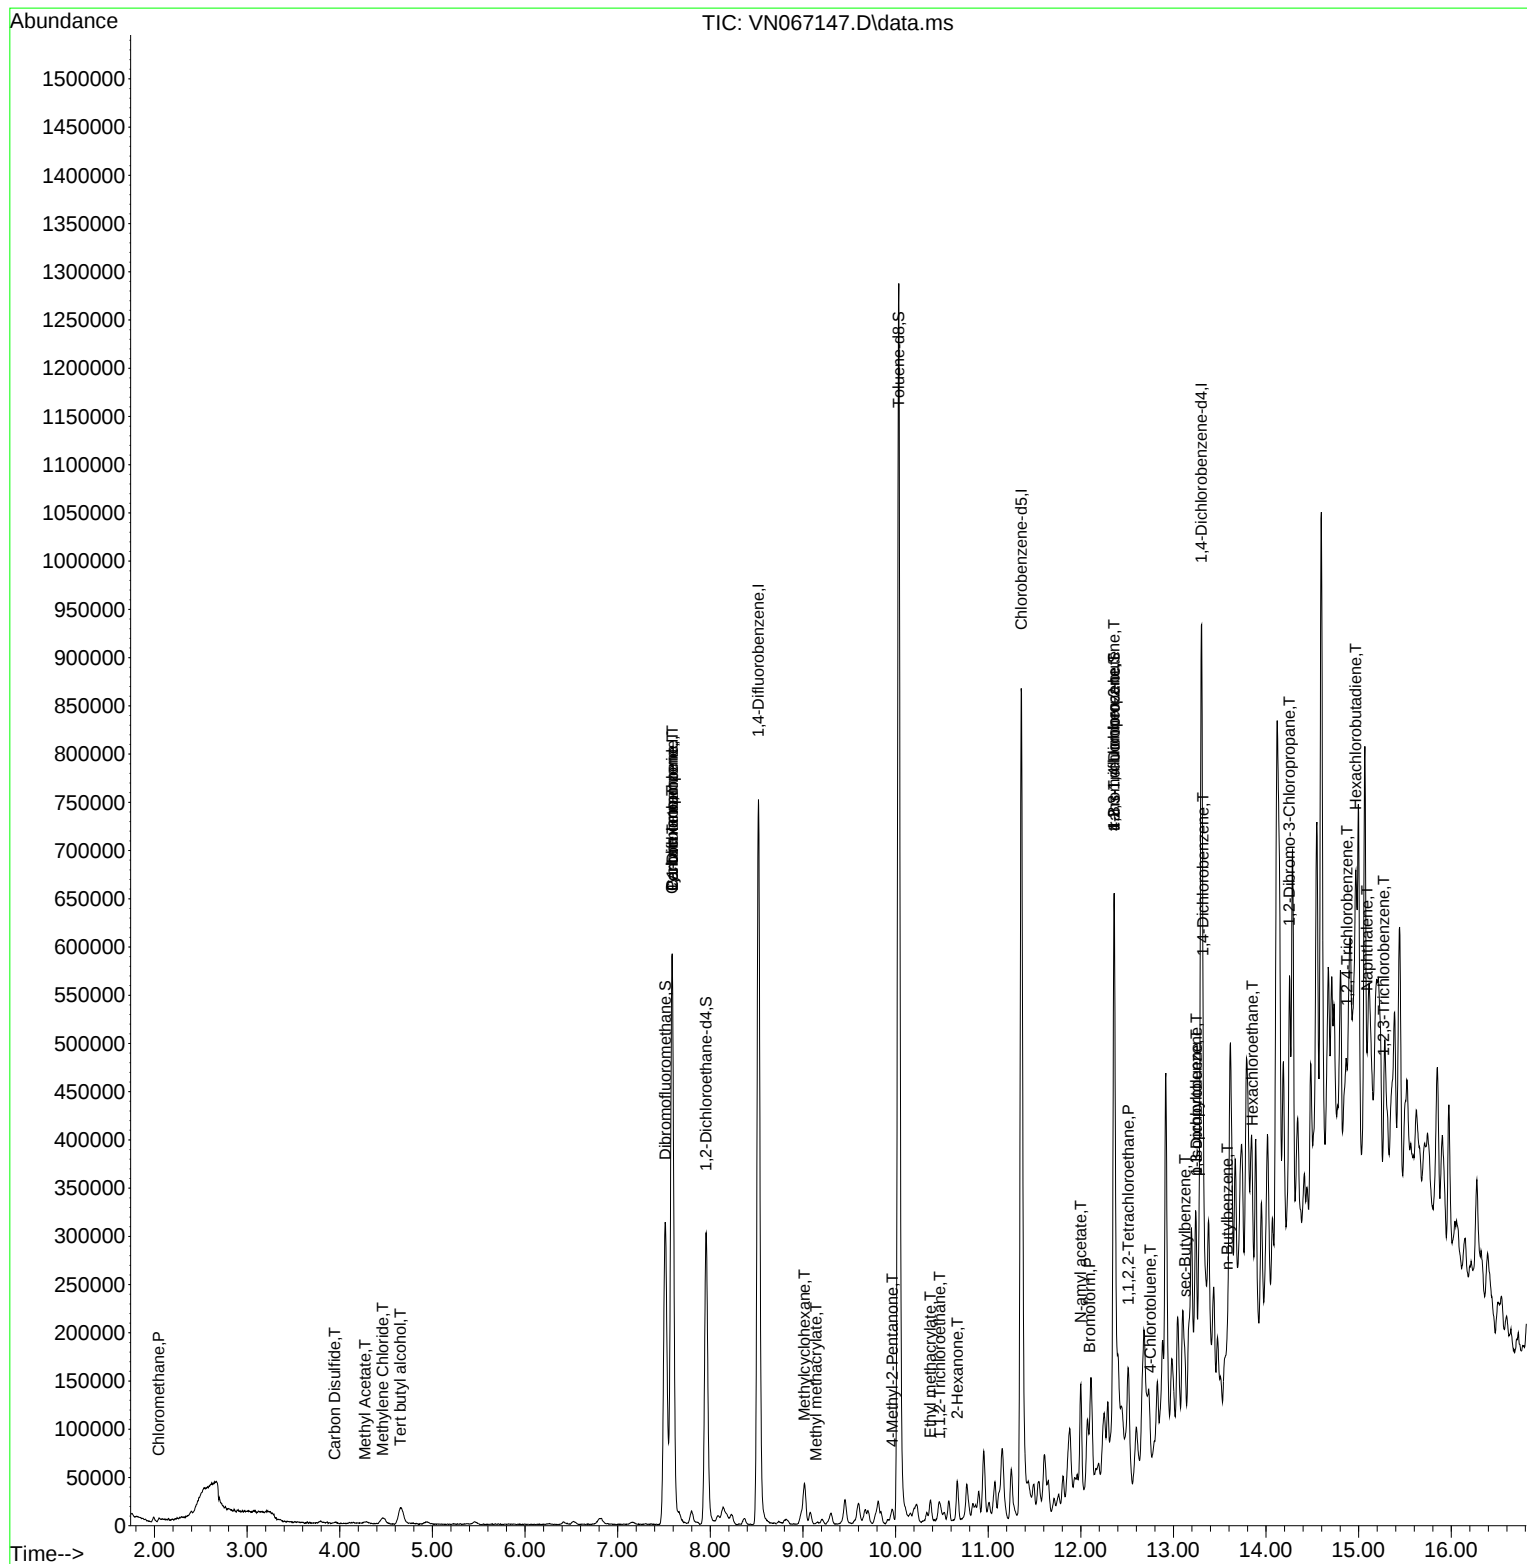




#1
Pentafluorobenzene
Concen: 50.00 ug/l
RT: 7.589 min Scan# 2181
Delta R.T. -0.008 min
Lab File: VN067147.D
Acq: 19 May 2021 13:32




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion:168 Resp: 571012
Ion Ratio Lower Upper
168 100
99 46.2 38.5 57.7

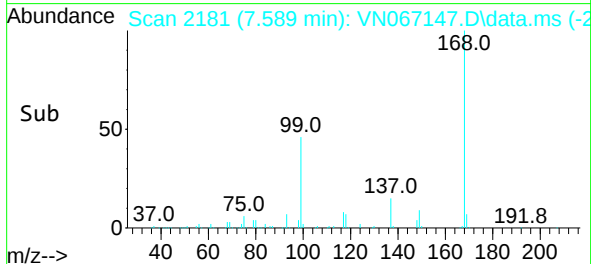

#3
Chloromethane
Concen: 0.29 ug/l
RT: 2.045 min Scan# 114
Delta R.T. -0.008 min
Lab File: VN067147.D
Acq: 19 May 2021 13:32


Tgt Ion: 50 Resp: 1824
Ion Ratio Lower Upper
50 100
52 33.9 26.5 39.7

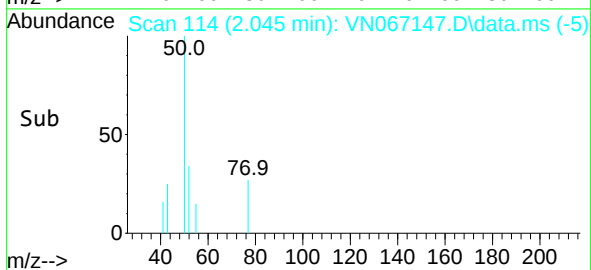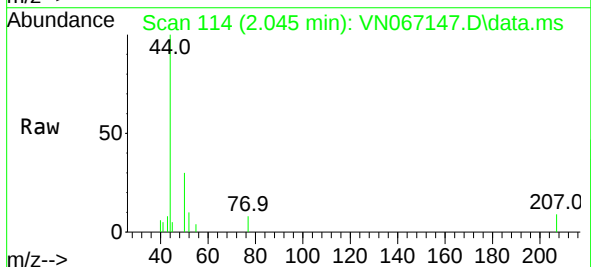






#11
Tert butyl alcohol
Concen: 7.00 ug/l
RT: 4.652 min Scan# 1086
Delta R.T. -0.062 min
Lab File: VN067147.D
Acq: 19 May 2021 13:32


Instrument :
MSVOA_N
ClientSampled :





Tgt Ion: 59 Resp: 7195
Ion Ratio Lower Upper
59 100
57 1.4 3.5 5.3#

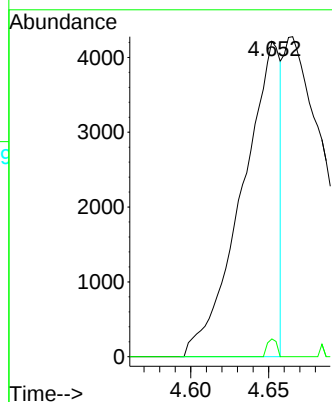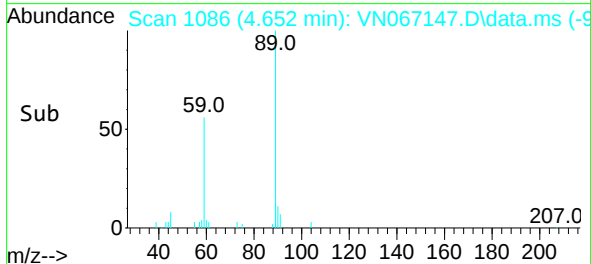


#13
Acrolein
Concen: Below Cal
RT: 3.555 min Scan# 677
Delta R.T. -0.008 min
Lab File: VN067147.D
Acq: 19 May 2021 13:32

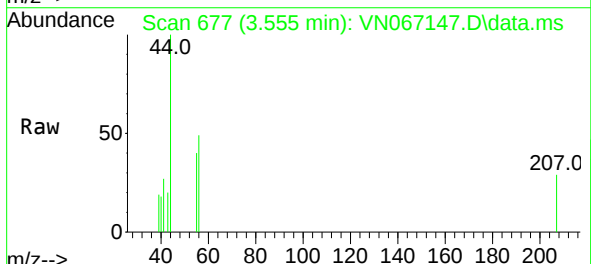

Tgt Ion: 56 Resp: 784
Ion Ratio Lower Upper
56 100
55 46.9 53.8 80.6#







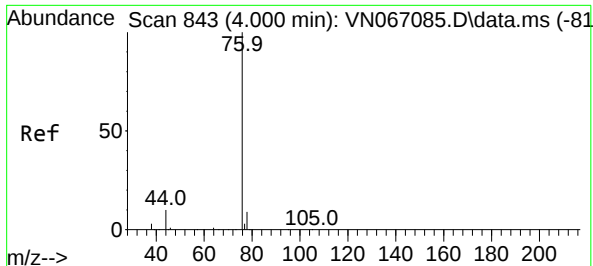

#17
Carbon Disulfide
Concen: 0.20 ug/l
RT: 3.944 min Scan# 822
Delta R.T. -0.056 min
Lab File: VN067147.D
Acq: 19 May 2021 13:32




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 76 Resp: 2939
Ion Ratio Lower Upper
76 100
78 0.0 7.5 11.3#

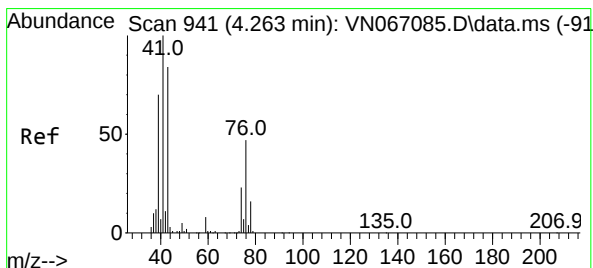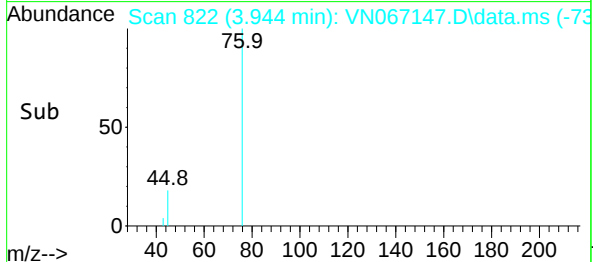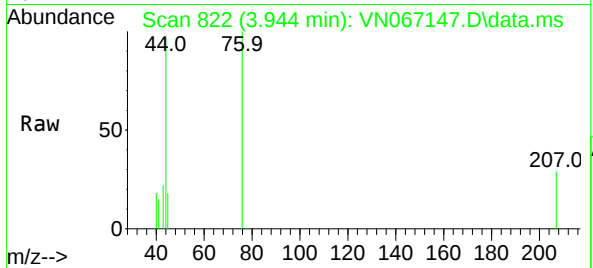

#18
Methyl Acetate
Concen: 0.39 ug/l
RT: 4.271 min Scan# 944
Delta R.T. 0.008 min
Lab File: VN067147.D
Acq: 19 May 2021 13:32


Tgt Ion: 43 Resp: 2213
Ion Ratio Lower Upper
43 100
74 13.3 21.4 32.2#

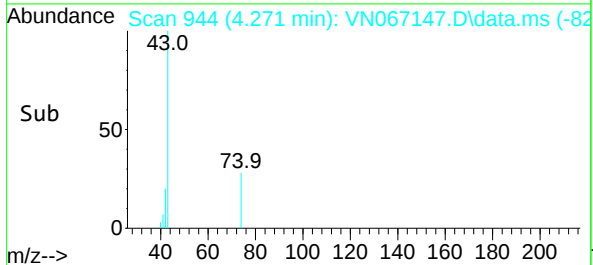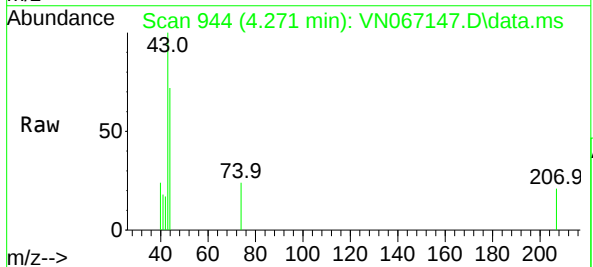






#20
Methylene Chloride
Concen: 0.34 ug/l
RT: 4.462 min Scan# 1015
Delta R.T. -0.021 min
Lab File: VN067147.D
Acq: 19 May 2021 13:32

Instrument :
MSVOA_N
ClientSampleId :







Tgt Ion: 84 Resp: 1656
Ion Ratio Lower Upper
84 100
49 92.0 88.3 132.5
51 52.6 26.7 40.1#
86 72.5 51.1 76.7

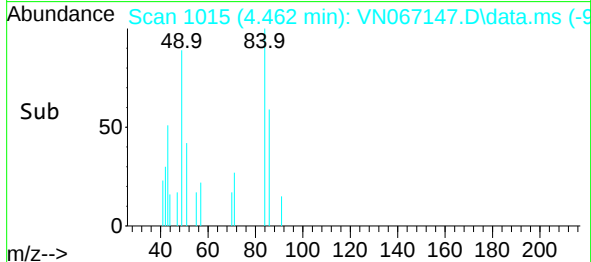

#31
Cyclohexane
Concen: 1.22 ug/l
RT: 7.586 min Scan# 2180
Delta R.T. 0.003 min
Lab File: VN067147.D
Acq: 19 May 2021 13:32

Tgt Ion: 56 Resp: 10335
Ion Ratio Lower Upper
56 100
69 172.2 28.0 42.0#
84 149.0 74.2 111.2#

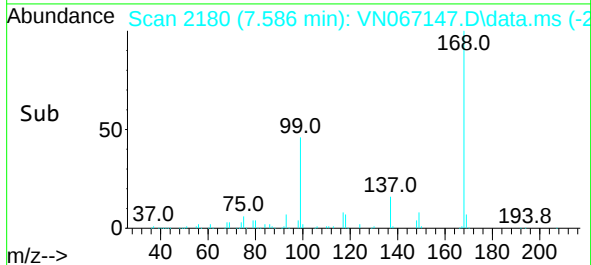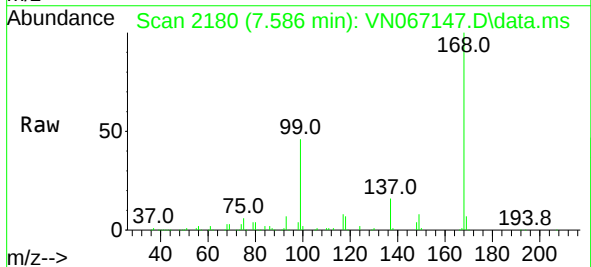



#33

1,2-Dichloroethane-d4

Concen: 44.21 ug/l

RT: 7.954 min Scan# 2317

Delta R.T. -0.005 min

Lab File: VN067147.D





Acq: 19 May 2021 13:32

Tgt Ion: 65 Resp: 272697

Ion Ratio Lower Upper

65 100

67 54.3 0.0 110.4

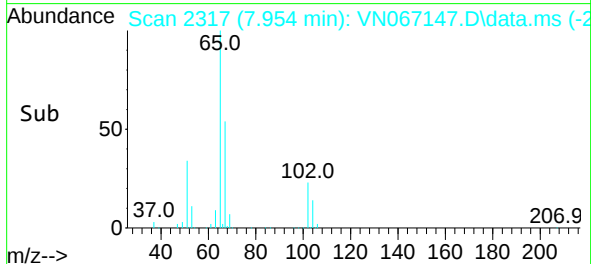

#34

1,4-Difluorobenzene

Concen: 50.00 ug/l

RT: 8.519 min Scan# 2528

Delta R.T. -0.006 min

Lab File: VN067147.D

Acq: 19 May 2021 13:32




Tgt Ion: 114 Resp: 782649


Ion Ratio Lower Upper

114 100

63 17.9 0.0 35.8


88 15.1 0.0 30.4

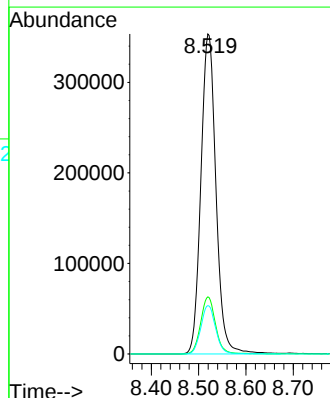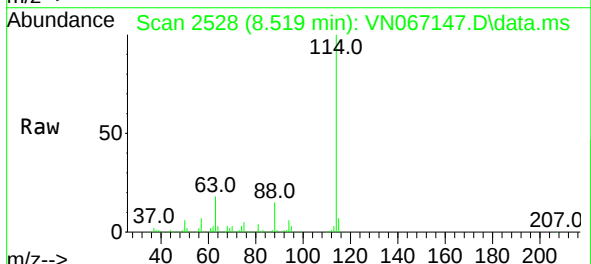






#35
Dibromofluoromethane
Concen: 50.34 ug/l
RT: 7.514 min Scan# 2153
Delta R.T. -0.008 min
Lab File: VN067147.D
Acq: 19 May 2021 13:32


Instrument :
MSVOA_N
ClientSampleId :





Tgt Ion:113 Resp: 258718
Ion Ratio Lower Upper
113 100
111 101.4 82.6 124.0
192 23.7 18.2 27.4

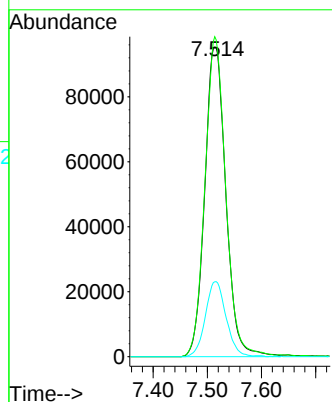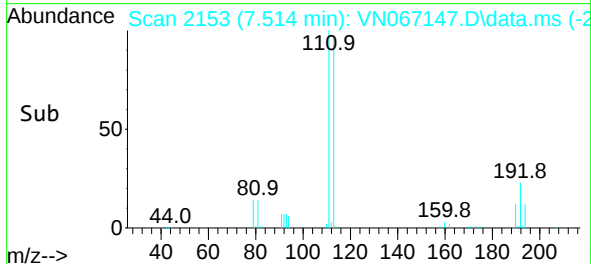


#36
1,1-Dichloropropene
Concen: 4.59 ug/l
RT: 7.589 min Scan# 2181
Delta R.T. -0.134 min
Lab File: VN067147.D
Acq: 19 May 2021 13:32




Tgt Ion: 75 Resp: 32768
Ion Ratio Lower Upper
75 100
110 5.3 19.1 57.3#
77 0.0 24.8 37.2#

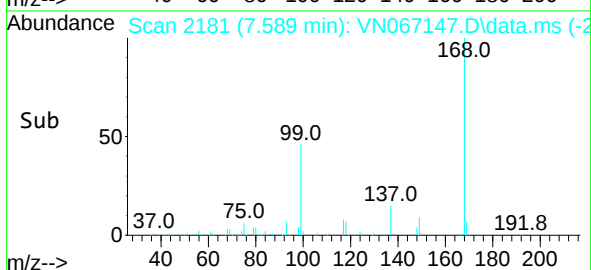






#38
Carbon Tetrachloride
Concen: 6.18 ug/l
RT: 7.589 min Scan# 2181
Delta R.T. -0.118 min
Lab File: VN067147.D
Acq: 19 May 2021 13:32

Instrument :
MSVOA_N
ClientSampleId :







Tgt Ion: 117 Resp: 46937
Ion Ratio Lower Upper
117 100
119 5.1 78.2 117.2#
121 0.0 24.7 37.1#

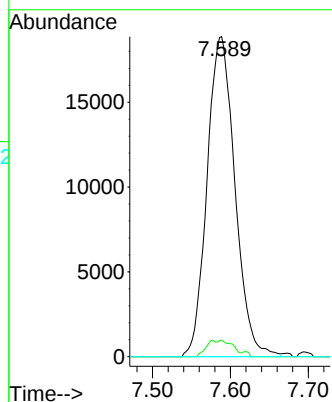

#39
Methylcyclohexane
Concen: 2.28 ug/l
RT: 9.016 min Scan# 2713
Delta R.T. -0.005 min
Lab File: VN067147.D
Acq: 19 May 2021 13:32


Tgt Ion: 83 Resp: 19030
Ion Ratio Lower Upper
83 100
55 72.3 56.2 84.2
98 46.4 36.8 55.2

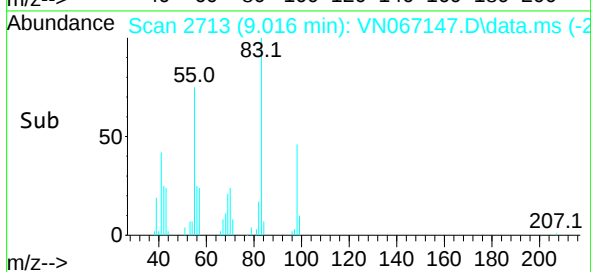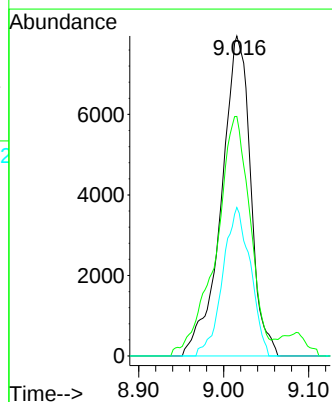






#48
Methyl methacrylate
Concen: 2.02 ug/l
RT: 9.142 min Scan# 2760
Delta R.T. -0.000 min
Lab File: VN067147.D
Acq: 19 May 2021 13:32

Instrument :
MSVOA_N
ClientSampleId :



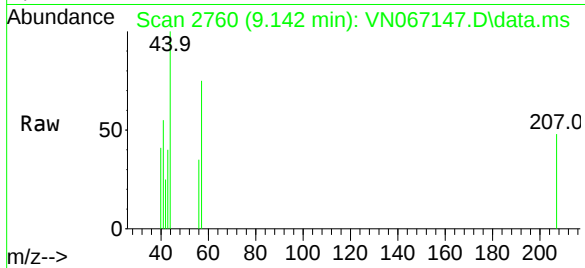



Tgt Ion: 41 Resp: 398
Ion Ratio Lower Upper
41 100
69 0.0 80.5 120.7#
39 0.0 41.4 62.0#

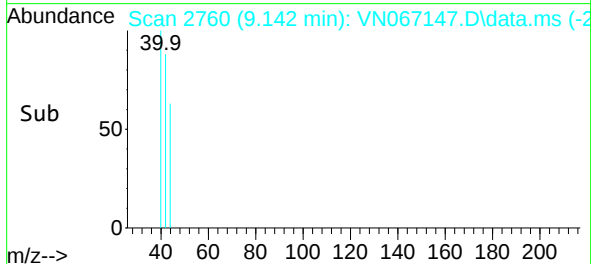

#50
Toluene-d8
Concen: 49.60 ug/l
RT: 10.035 min Scan# 3093
Delta R.T. -0.002 min
Lab File: VN067147.D
Acq: 19 May 2021 13:32

Tgt Ion: 98 Resp: 966040
Ion Ratio Lower Upper
98 100
100 64.4 51.8 77.8


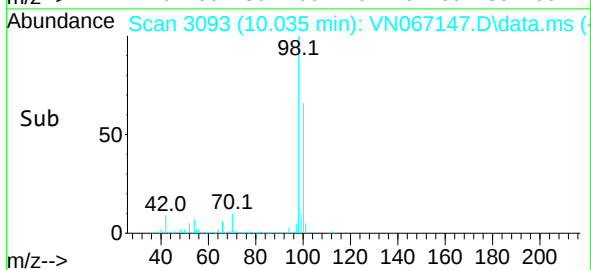

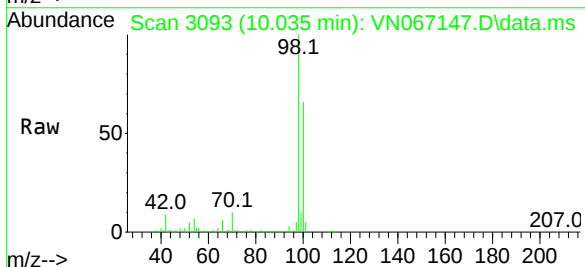




#51
4-Methyl-2-Pentanone
Concen: 5.89 ug/l
RT: 9.965 min Scan# 3067
Delta R.T. 0.037 min
Lab File: VN067147.D
Acq: 19 May 2021 13:32




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion: 43 Resp: 3152
Ion Ratio Lower Upper
43 100
58 26.5 34.5 51.7#

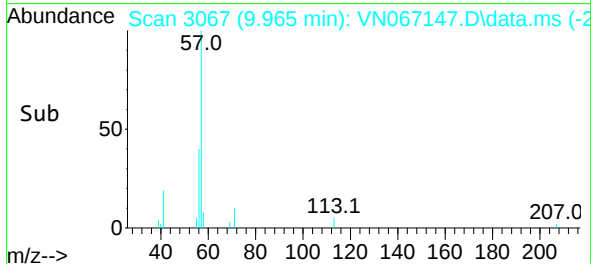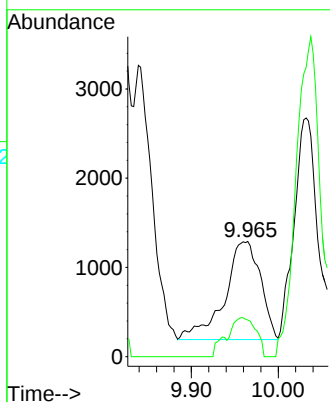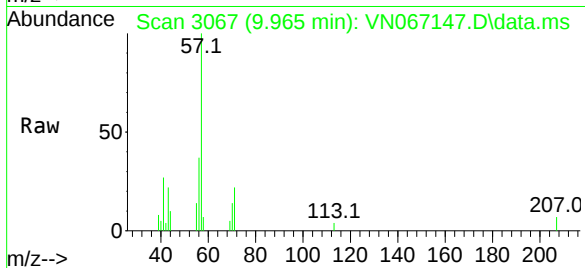

#55
1,1,2-Trichloroethane
Concen: 1.39 ug/l
RT: 10.475 min Scan# 3257
Delta R.T. -0.035 min
Lab File: VN067147.D
Acq: 19 May 2021 13:32

Tgt Ion: 97 Resp: 7747
Ion Ratio Lower Upper
97 100
83 9.1 67.3 100.9#
85 0.4 44.2 66.4#
99 0.0 49.8 74.8#


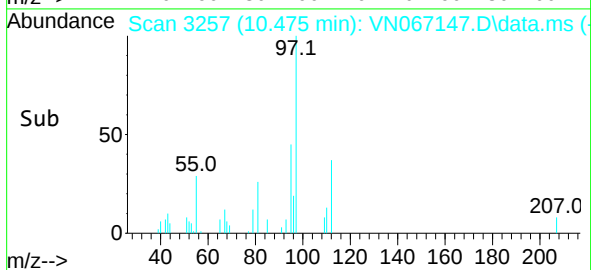

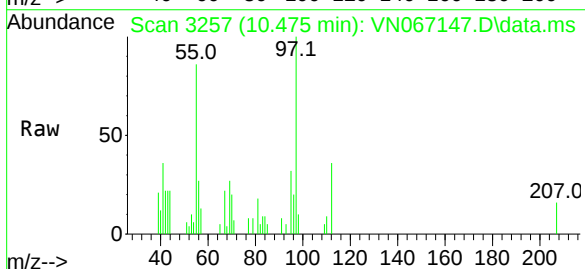


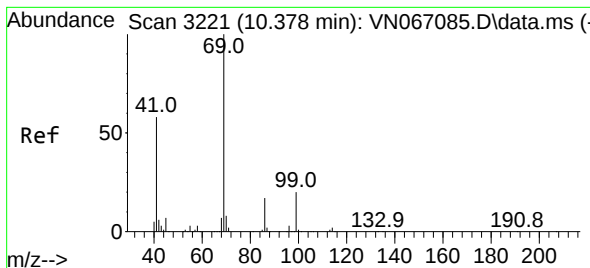

#56
Ethyl methacrylate
Concen: 2.11 ug/l
RT: 10.375 min Scan# 3220
Delta R.T. -0.003 min
Lab File: VN067147.D
Acq: 19 May 2021 13:32




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 69 Resp: 1495
Ion Ratio Lower Upper
69 100
41 197.1 45.5 68.3#
39 88.3 22.9 34.3#

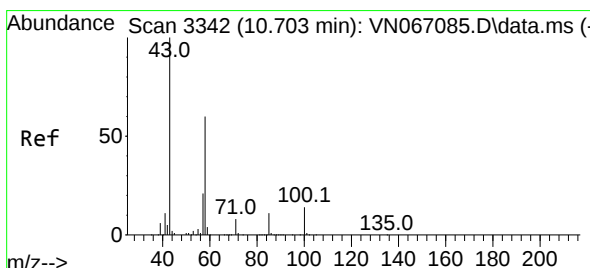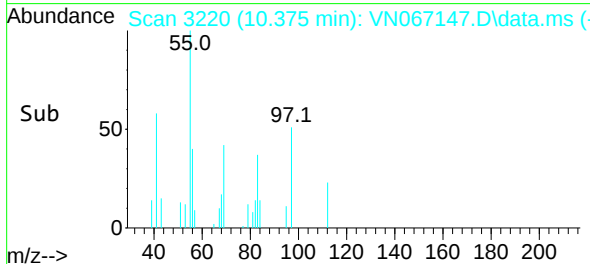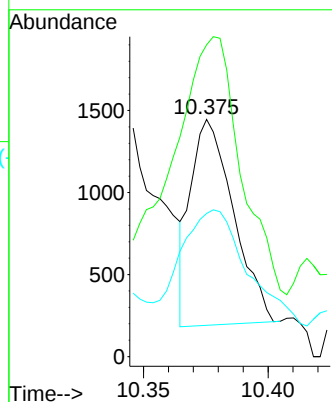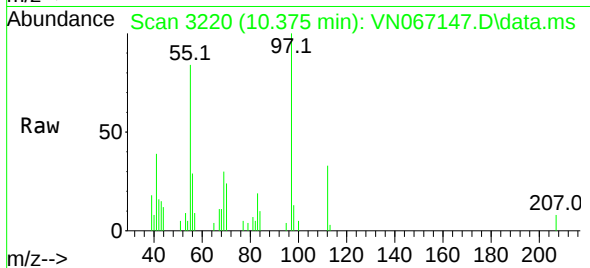

#59
2-Hexanone
Concen: 25.54 ug/l
RT: 10.668 min Scan# 3329
Delta R.T. -0.035 min
Lab File: VN067147.D
Acq: 19 May 2021 13:32

Tgt Ion: 43 Resp: 16102
Ion Ratio Lower Upper
43 100
58 3.5 29.8 89.5#


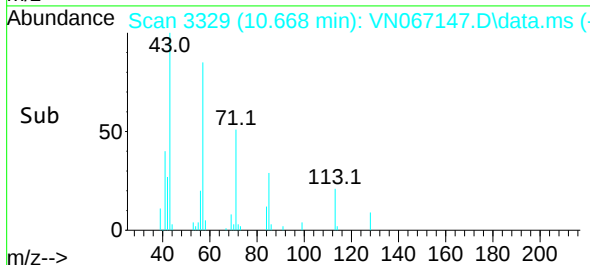

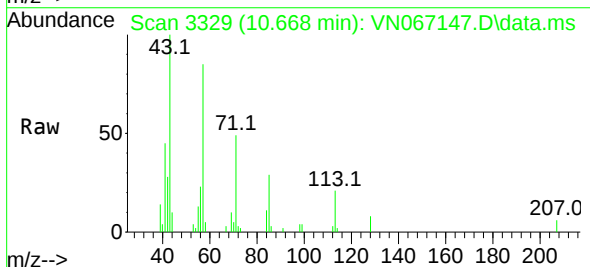




#62
4-Bromofluorobenzene
Concen: 44.34 ug/l
RT: 12.360 min Scan# 3960
Delta R.T. 0.005 min
Lab File: VN067147.D
Acq: 19 May 2021 13:32




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 95 Resp: 289319
Ion Ratio Lower Upper
95 100
174 97.5 0.0 182.8
176 96.5 0.0 176.6

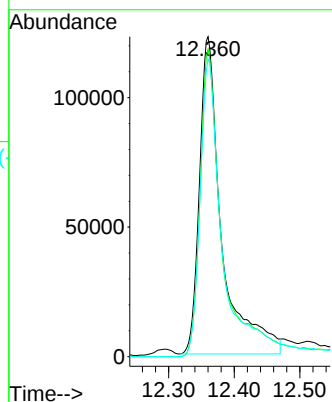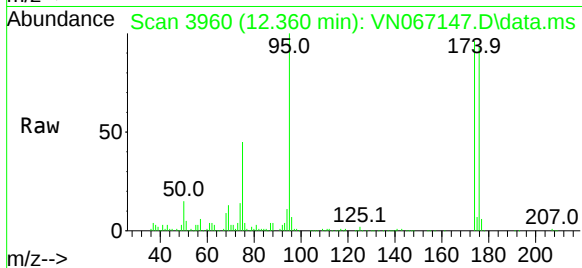

#63
Chlorobenzene-d5
Concen: 50.00 ug/l
RT: 11.360 min Scan# 3587
Delta R.T. 0.003 min
Lab File: VN067147.D
Acq: 19 May 2021 13:32

Tgt Ion: 117 Resp: 630703
Ion Ratio Lower Upper
117 100
82 50.6 42.2 63.2
119 32.0 25.8 38.6


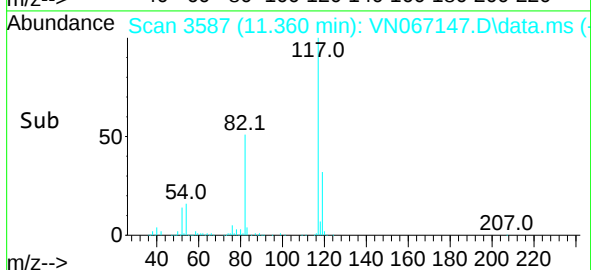

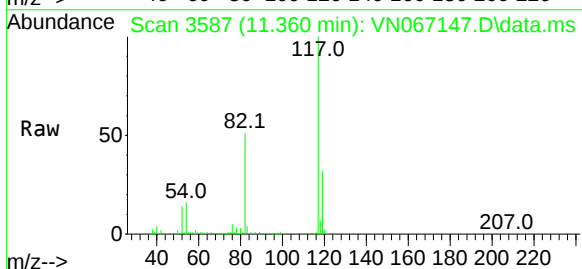


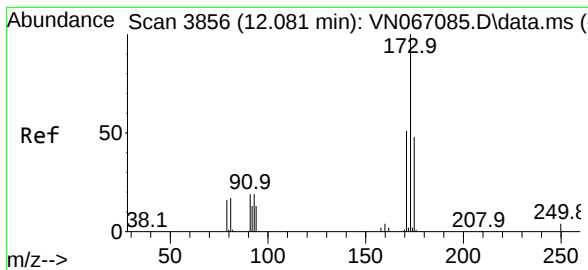

#71
Bromoform
Concen: 1.77 ug/l
RT: 12.097 min Scan# 3862
Delta R.T. 0.016 min
Lab File: VN067147.D
Acq: 19 May 2021 13:32




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion:173 Resp: 53
Ion Ratio Lower Upper
173 100
175 0.0 24.3 73.0#
254 0.0 0.0 0.0

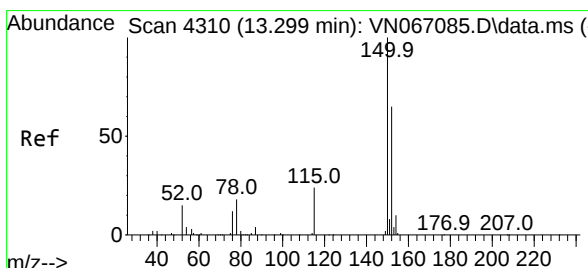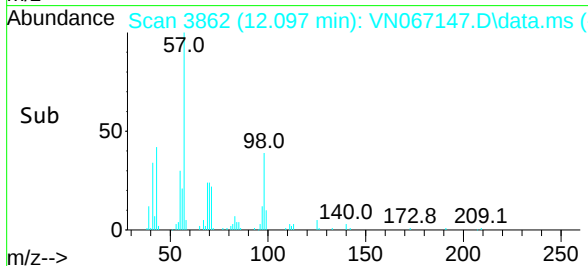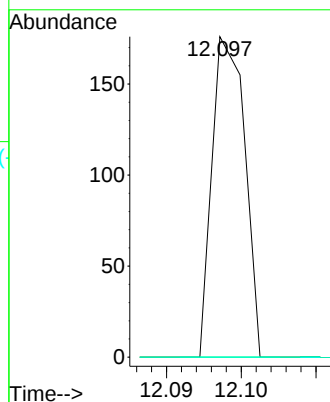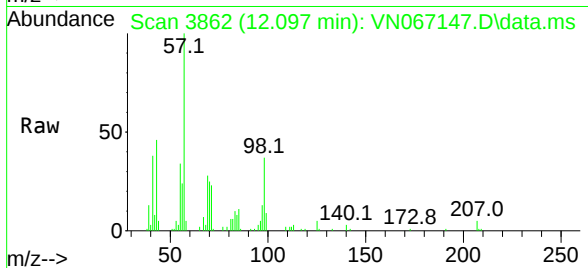

#72
1,4-Dichlorobenzene-d4
Concen: 50.00 ug/l
RT: 13.301 min Scan# 4311
Delta R.T. 0.002 min
Lab File: VN067147.D
Acq: 19 May 2021 13:32


Tgt Ion:152 Resp: 304812
Ion Ratio Lower Upper
152 100
115 54.2 27.0 80.8
150 158.4 0.0 350.2

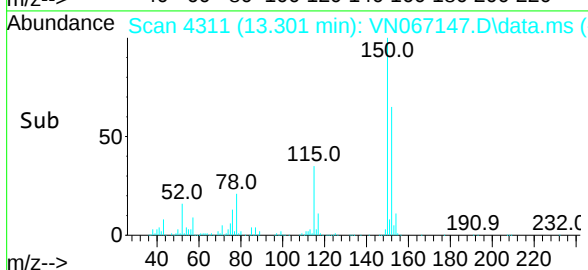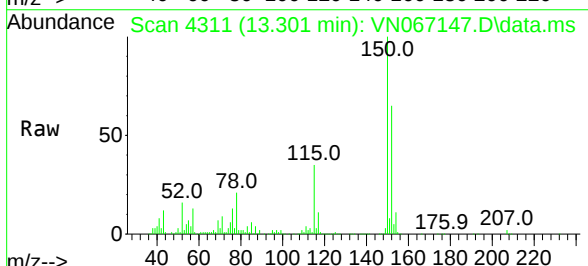



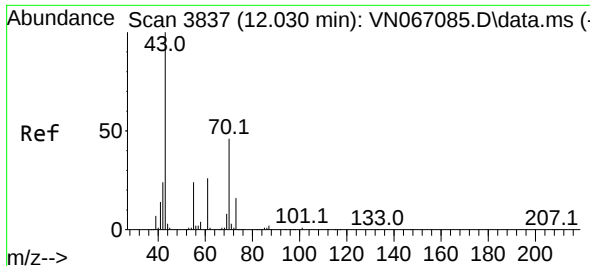


#74
N-amy1 acetate
Concen: 5.67 ug/l
RT: 11.998 min Scan# 3825
Delta R.T. -0.032 min
Lab File: VN067147.D
Acq: 19 May 2021 13:32

Instrument :
MSVOA_N
ClientSampled :



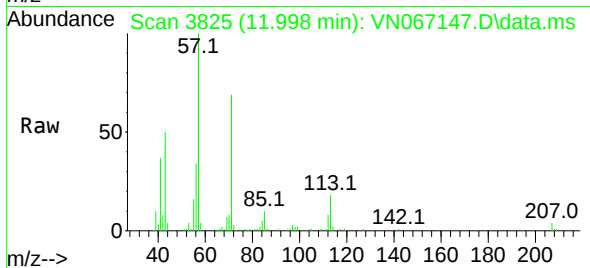



Tgt Ion:	43	Resp:	24027
Ion Ratio	100	Lower	Upper
70	12.7	36.7	55.1#
55	13.8	17.6	26.4#
61	0.0	18.9	28.3#

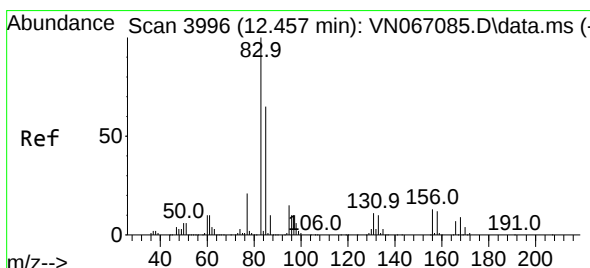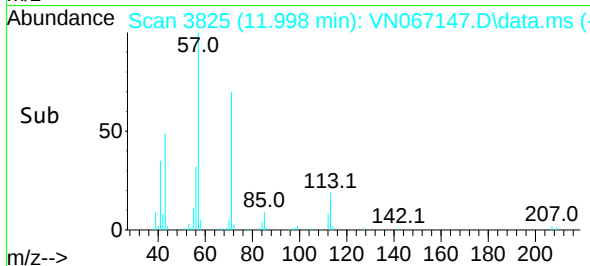

#75
1,1,2,2-Tetrachloroethane
Concen: 1.49 ug/l
RT: 12.510 min Scan# 4016
Delta R.T. 0.053 min
Lab File: VN067147.D
Acq: 19 May 2021 13:32

Tgt Ion:	83	Resp:	11499
Ion Ratio	100	Lower	Upper
131	0.0	5.3	16.1#
85	30.0	32.6	97.8#


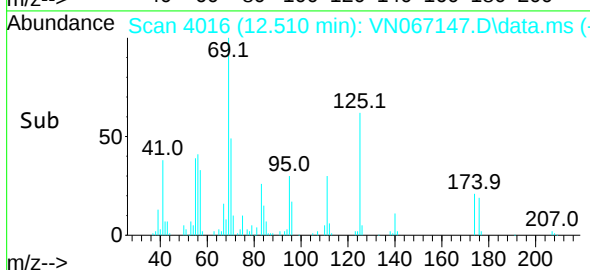

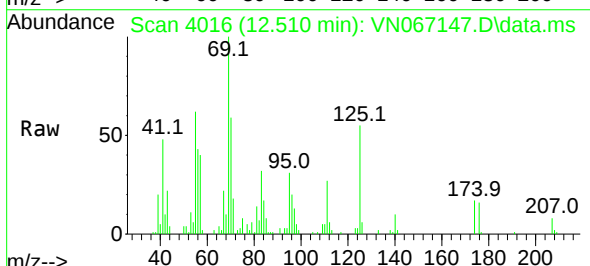


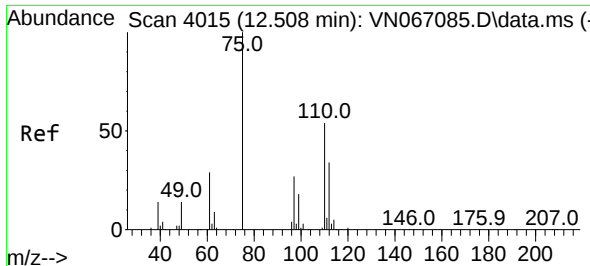

#76
1,2,3-Trichloropropane
Concen: 20.88 ug/l
RT: 12.360 min Scan# 3960
Delta R.T. -0.148 min
Lab File: VN067147.D
Acq: 19 May 2021 13:32




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 75 Resp: 134334
Ion Ratio Lower Upper
75 100
77 1.1 0.0 0.0#

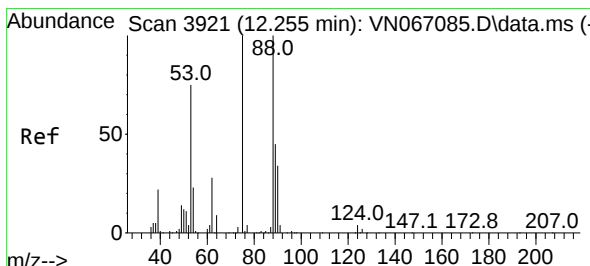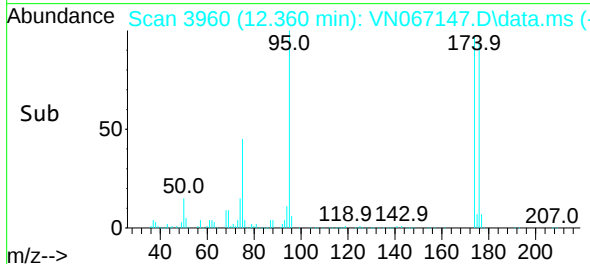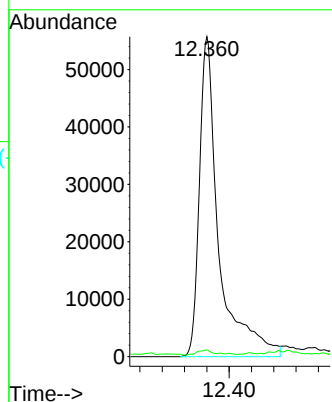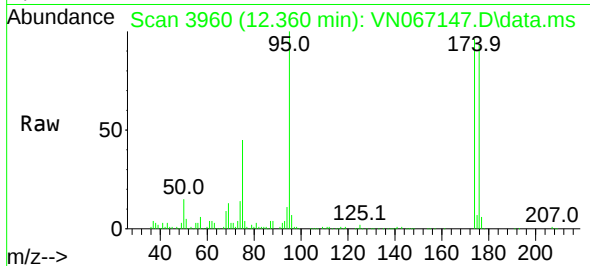

#81
trans-1,4-Dichloro-2-butene
Concen: 62.98 ug/l
RT: 12.360 min Scan# 3960
Delta R.T. 0.105 min
Lab File: VN067147.D
Acq: 19 May 2021 13:32

Tgt Ion: 75 Resp: 134334
Ion Ratio Lower Upper
75 100
53 0.0 66.3 99.5#
89 0.0 39.5 59.3#


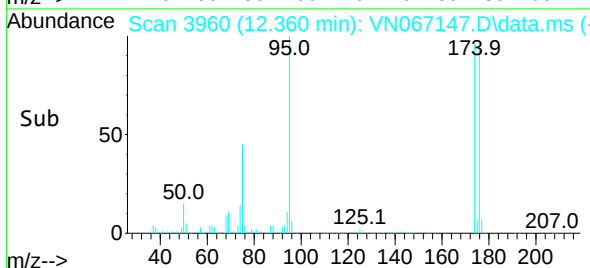

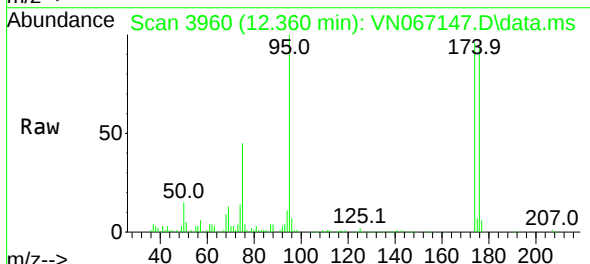




#82
4-Chlorotoluene
Concen: 1.22 ug/l
RT: 12.752 min Scan# 4106
Delta R.T. 0.025 min
Lab File: VN067147.D
Acq: 19 May 2021 13:32




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion: 91 Resp: 613
Ion Ratio Lower Upper
91 100
126 98.5 17.7 53.1#

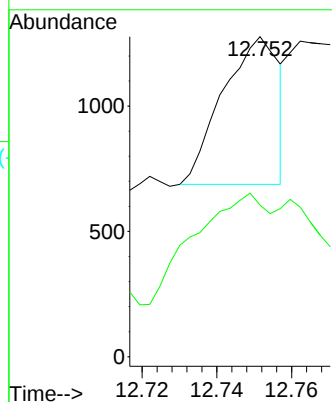

#85
sec-Butylbenzene
Concen: 0.29 ug/l
RT: 13.127 min Scan# 4246
Delta R.T. 0.003 min
Lab File: VN067147.D
Acq: 19 May 2021 13:32

Tgt Ion:105 Resp: 7008
Ion Ratio Lower Upper
105 100
134 22.8 10.5 31.5


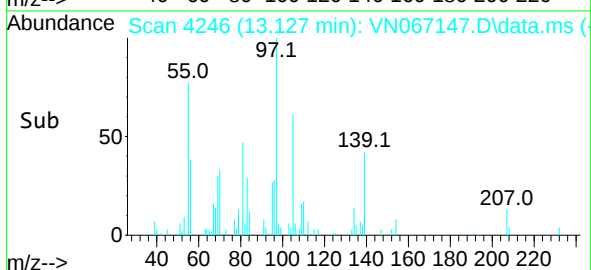

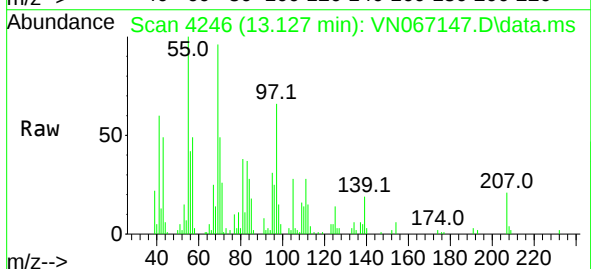


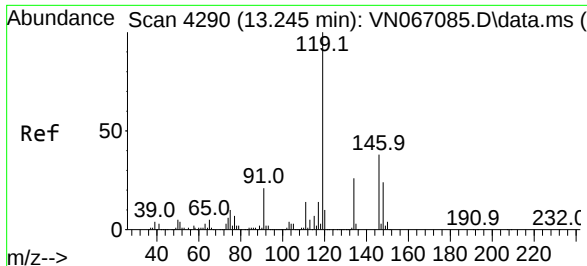

#86
p-Isopropyltoluene
Concen: 0.35 ug/l
RT: 13.248 min Scan# 4291
Delta R.T. 0.003 min
Lab File: VN067147.D
Acq: 19 May 2021 13:32




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion:119 Resp: 7254
Ion Ratio Lower Upper
119 100
134 34.1 13.3 39.9
91 25.5 10.7 32.1

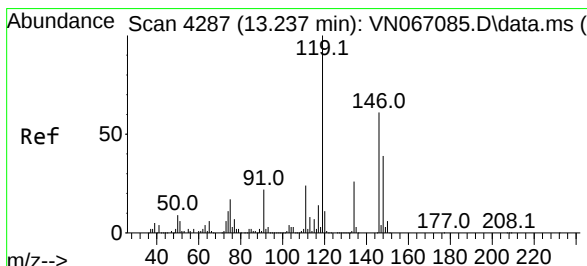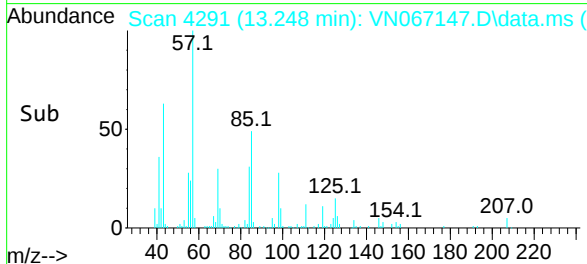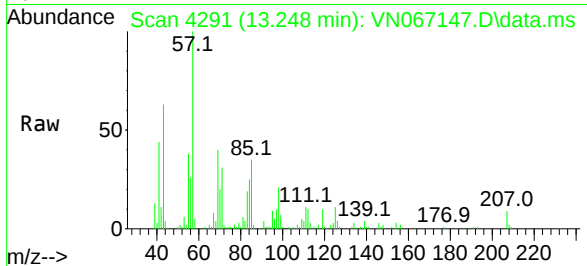

#87
1,3-Dichlorobenzene
Concen: 0.24 ug/l
RT: 13.248 min Scan# 4291
Delta R.T. 0.011 min
Lab File: VN067147.D
Acq: 19 May 2021 13:32

Tgt Ion:146 Resp: 2434
Ion Ratio Lower Upper
146 100
111 0.0 19.3 57.8#
148 66.4 32.0 96.2


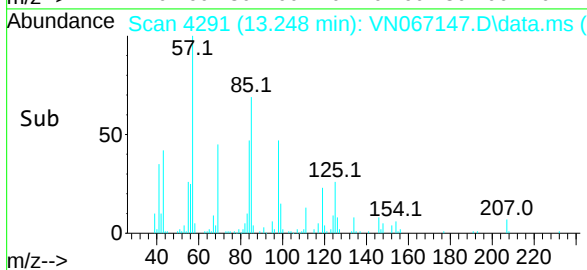

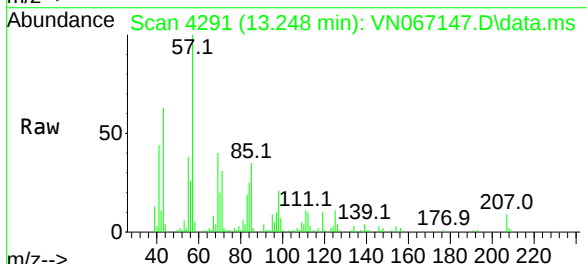




#88
1,4-Dichlorobenzene
Concen: 0.39 ug/l
RT: 13.320 min Scan# 4318
Delta R.T. 0.002 min
Lab File: VN067147.D
Acq: 19 May 2021 13:32




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion:146 Resp: 4179
Ion Ratio Lower Upper
146 100
111 429.5 18.5 55.5#
148 73.4 31.4 94.3

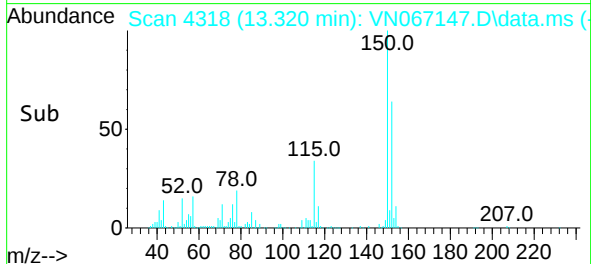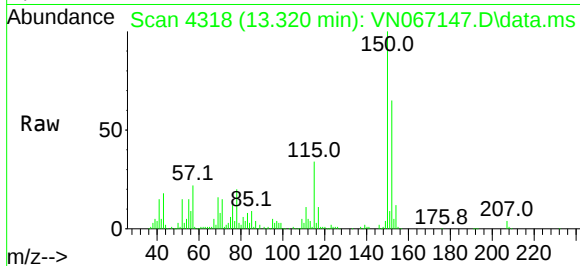

#89
n-Butylbenzene
Concen: 0.37 ug/l
RT: 13.580 min Scan# 4415
Delta R.T. 0.008 min
Lab File: VN067147.D
Acq: 19 May 2021 13:32

Tgt Ion: 91 Resp: 5866
Ion Ratio Lower Upper
91 100
92 81.6 26.5 79.5#
134 21.0 14.3 42.9


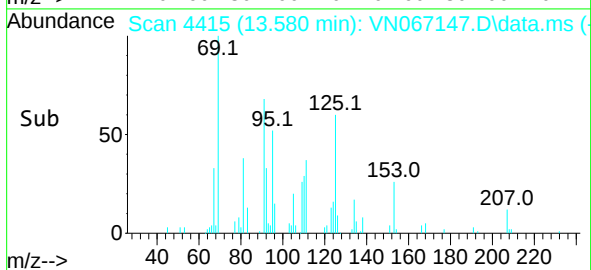

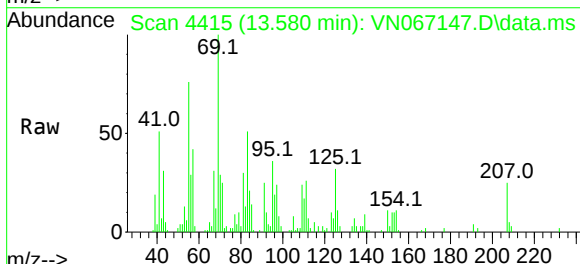




#90
Hexachloroethane
Concen: 0.62 ug/l
RT: 13.854 min Scan# 4517
Delta R.T. 0.027 min
Lab File: VN067147.D
Acq: 19 May 2021 13:32




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion:117 Resp: 2362
Ion Ratio Lower Upper
117 100
201 0.0 45.5 136.5#

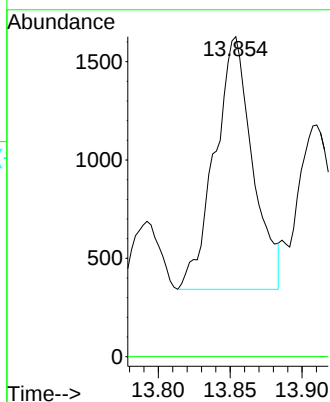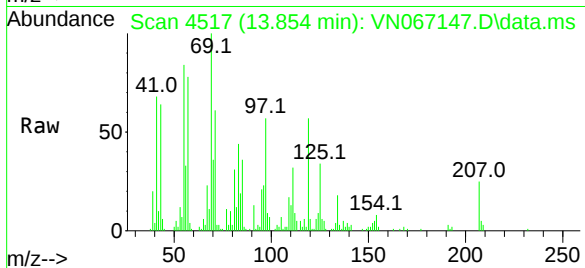

#92
1,2-Dibromo-3-Chloropropane
Concen: 0.59 ug/l
RT: 14.251 min Scan# 4665
Delta R.T. 0.022 min
Lab File: VN067147.D
Acq: 19 May 2021 13:32

Tgt Ion: 75 Resp: 675
Ion Ratio Lower Upper
75 100
155 52.0 49.9 149.7
157 16.4 63.8 191.4#


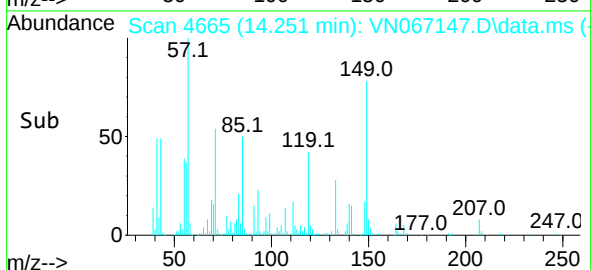

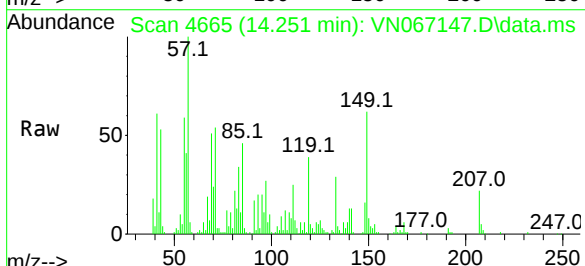


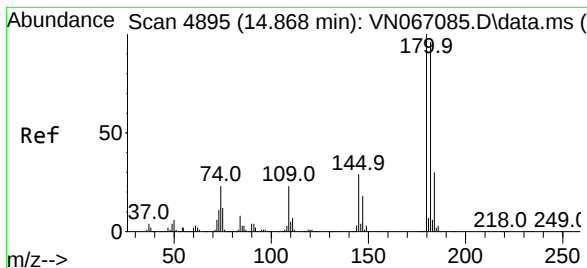

#93
1,2,4-Trichlorobenzene
Concen: 1.28 ug/l
RT: 14.873 min Scan# 4897
Delta R.T. 0.005 min
Lab File: VN067147.D
Acq: 19 May 2021 13:32




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion:180 Resp: 6921
Ion Ratio Lower Upper
180 100
182 90.7 47.3 141.8
145 461.9 14.0 42.0#

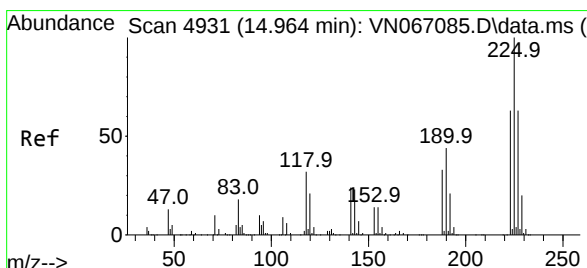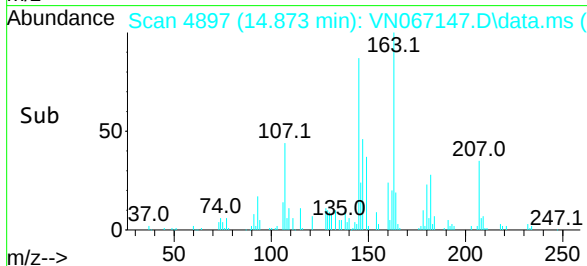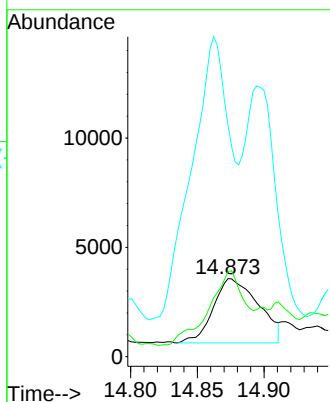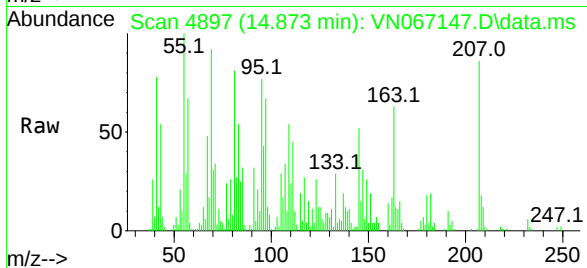

#94
Hexachlorobutadiene
Concen: 0.56 ug/l
RT: 14.967 min Scan# 4932
Delta R.T. 0.003 min
Lab File: VN067147.D
Acq: 19 May 2021 13:32

Tgt Ion:225 Resp: 2088
Ion Ratio Lower Upper
225 100
223 67.2 31.7 95.1
227 69.5 31.7 95.1


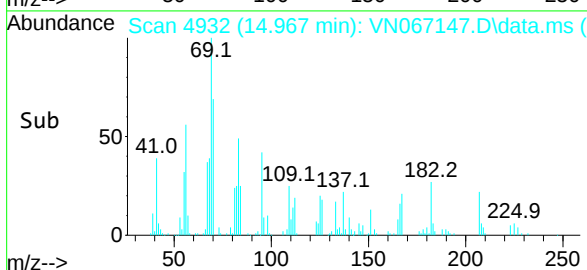

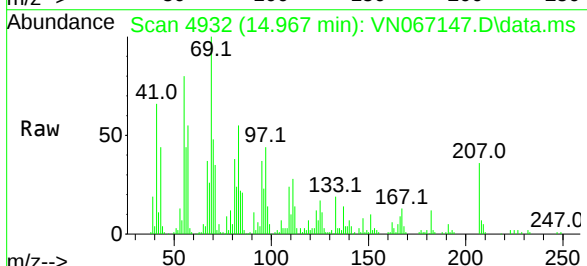


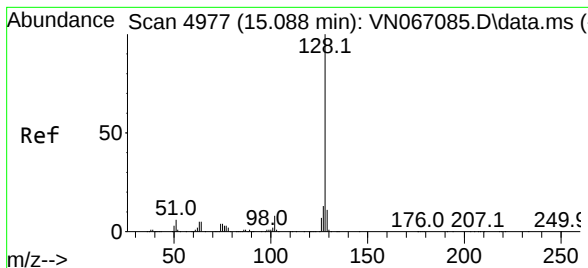

#95
Naphthalene
Concen: 5.67 ug/l
RT: 15.090 min Scan# 4978
Delta R.T. 0.002 min
Lab File: VN067147.D
Acq: 19 May 2021 13:32

Instrument :
MSVOA_N
ClientSampled :

Tgt Ion:128 Resp: 33513
Ion Ratio Lower Upper
128 100
127 0.0 10.2 15.2#
129 2.4 8.6 13.0#

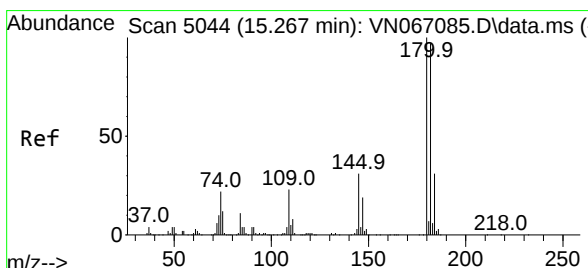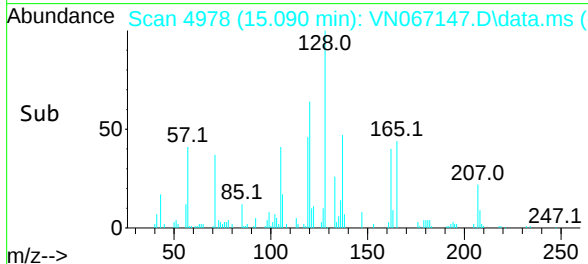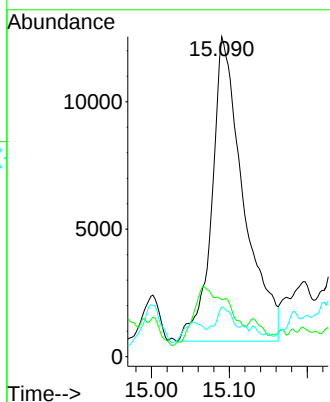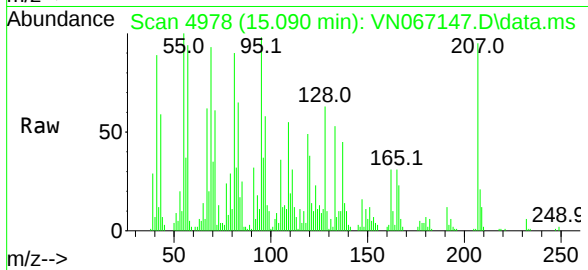

#96
1,2,3-Trichlorobenzene
Concen: 0.74 ug/l
RT: 15.267 min Scan# 5044
Delta R.T. 0.000 min
Lab File: VN067147.D
Acq: 19 May 2021 13:32

Tgt Ion:180 Resp: 3710
Ion Ratio Lower Upper
180 100
182 244.2 48.5 145.6#
145 0.0 15.4 46.2#

