


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN051921\
 Data File : VN067141.D
 Acq On : 19 May 2021 10:33
 Operator : JC/MD
 Sample : BFB
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N051421W.M
 Title : SW846 8260
 Last Update : Tue May 18 04:00:15 2021

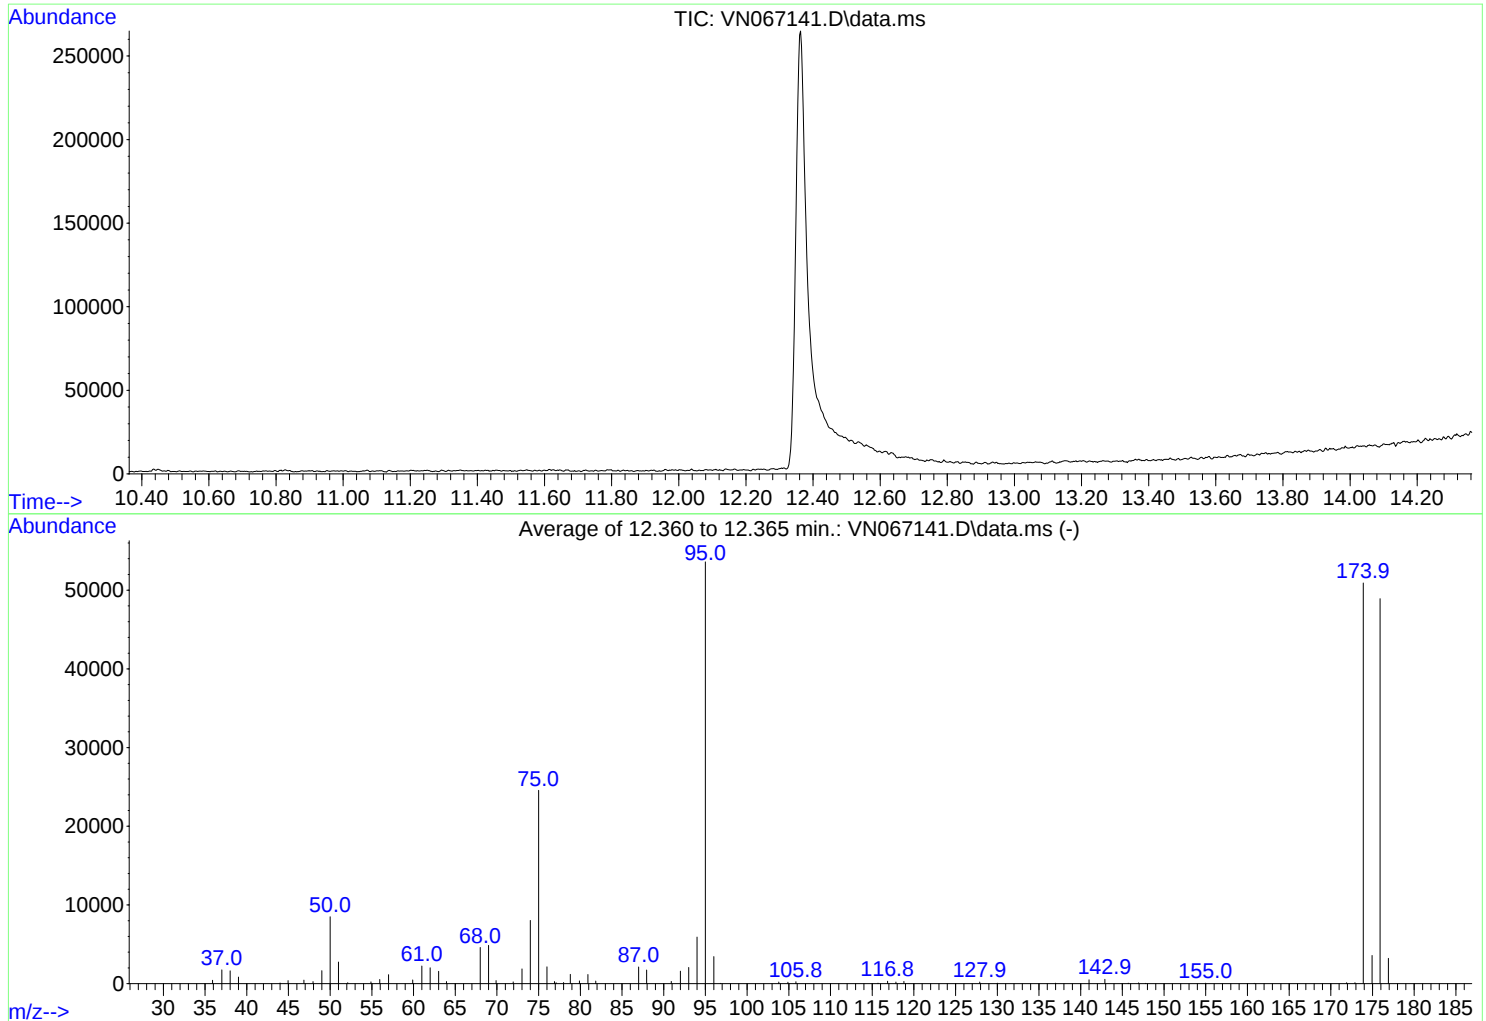

AutoFind: Scans 3960, 3961, 3962; Background Corrected with Scan 3943

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.9	8506	PASS
75	95	30	60	45.8	24560	PASS
95	95	100	100	100.0	53605	PASS
96	95	5	9	6.4	3433	PASS
173	174	0.00	2	0.3	131	PASS
174	95	50	100	95.0	50920	PASS
175	174	5	9	7.0	3577	PASS
176	174	95	101	96.1	48925	PASS
177	176	5	9	6.5	3204	PASS