
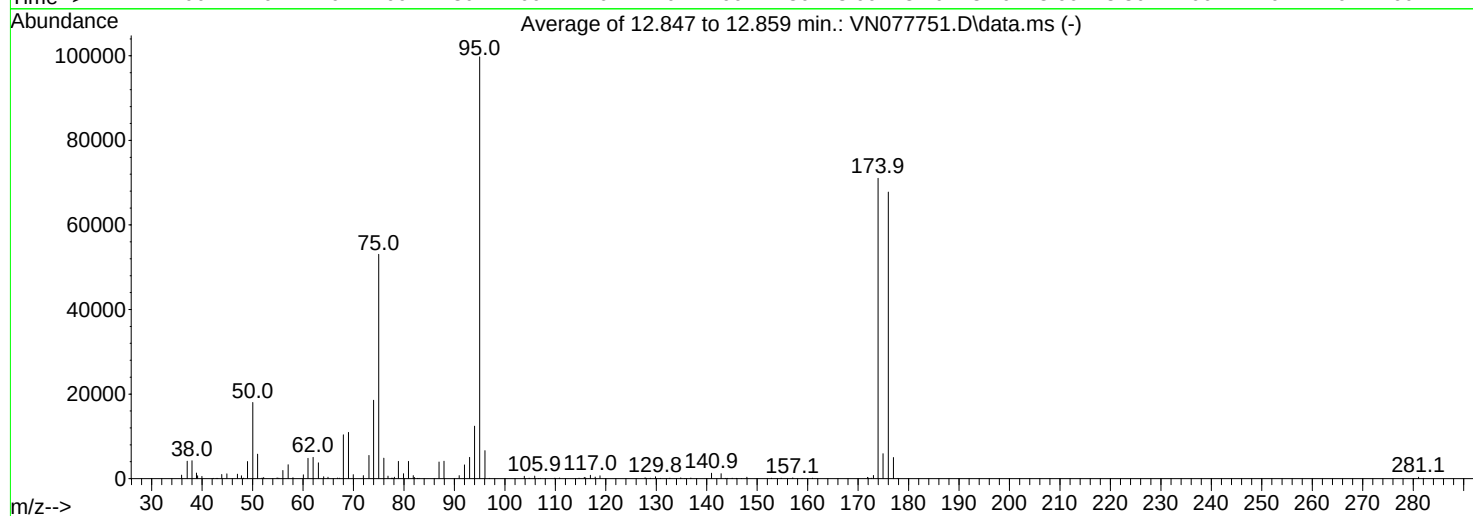


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN051923\
Data File : VN077751.D
Acq On : 19 May 2023 08:41
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N051523W.M
Title : SW846 8260
Last Update : Tue May 16 04:07:42 2023

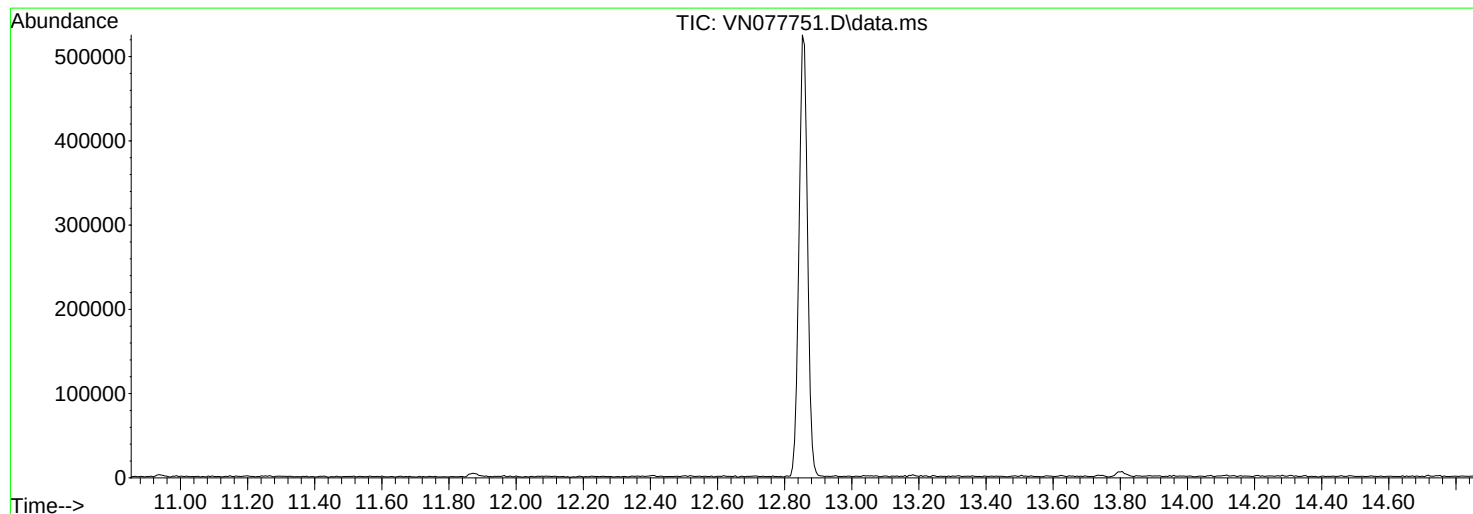

AutoFind: Scans 1852, 1853, 1854; Background Corrected with Scan 1843

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	18.1	18023	PASS
75	95	30	60	53.2	53043	PASS
95	95	100	100	100.0	99757	PASS
96	95	5	9	6.6	6631	PASS
173	174	0.00	2	1.1	755	PASS
174	95	50	100	71.2	71043	PASS
175	174	5	9	8.3	5900	PASS
176	174	95	101	95.4	67768	PASS
177	176	5	9	7.4	5014	PASS

Average of 12.847 to 12.859 min.: VN077751.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.95	833	47.00	1078	57.05	3277	69.00	1093
37.05	4121	47.80	695	58.00	221	69.95	94
38.00	4244	48.20	128	60.05	908	71.95	73
38.90	1340	49.00	4064	61.00	4824	73.05	548
39.10	665	50.05	18023	62.00	5050	74.00	18532
39.95	541	51.00	5810	63.05	3761	75.00	53043
42.20	73	51.90	159	64.10	453	76.00	4853
42.80	68	52.20	268	64.95	336	76.85	614
43.10	72	54.85	191	66.85	150	77.50	131
43.90	996	55.20	121	67.20	117	77.70	100
44.90	1141	56.00	1951	68.00	10369	78.10	361

Average of 12.847 to 12.859 min.: VN077751.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
78.90	4095	93.00	5021	110.85	170	130.80	84
79.90	1168	94.00	12425	114.70	116	132.70	103
80.90	4094	95.00	99757	115.75	290	134.85	198
81.85	739	96.05	6631	116.00	200	135.70	50
82.10	270	96.90	72	116.95	784	136.85	161
82.70	61	103.85	568	117.90	386	140.95	1281
83.00	76	104.80	134	118.85	675	142.85	1163
86.95	3922	105.90	590	127.80	227	143.70	84
87.95	4136	106.70	54	128.00	77	144.10	64
90.95	708	107.00	77	128.80	111	145.05	121
92.00	3265	109.90	131	129.85	474	145.90	69

Average of 12.847 to 12.859 min.: VN077751.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
146.90	55	173.95	71043				
147.95	337	174.95	5900				
152.80	117	176.00	67768				
154.75	125	177.00	5014				
157.05	179	177.90	74				
158.90	87	281.05	325				
160.95	131	282.00	63				
171.85	320						
172.10	170						
172.60	116						
173.05	755						

Instrument :

MSVOA_N

ClientSampleId :

BFB