
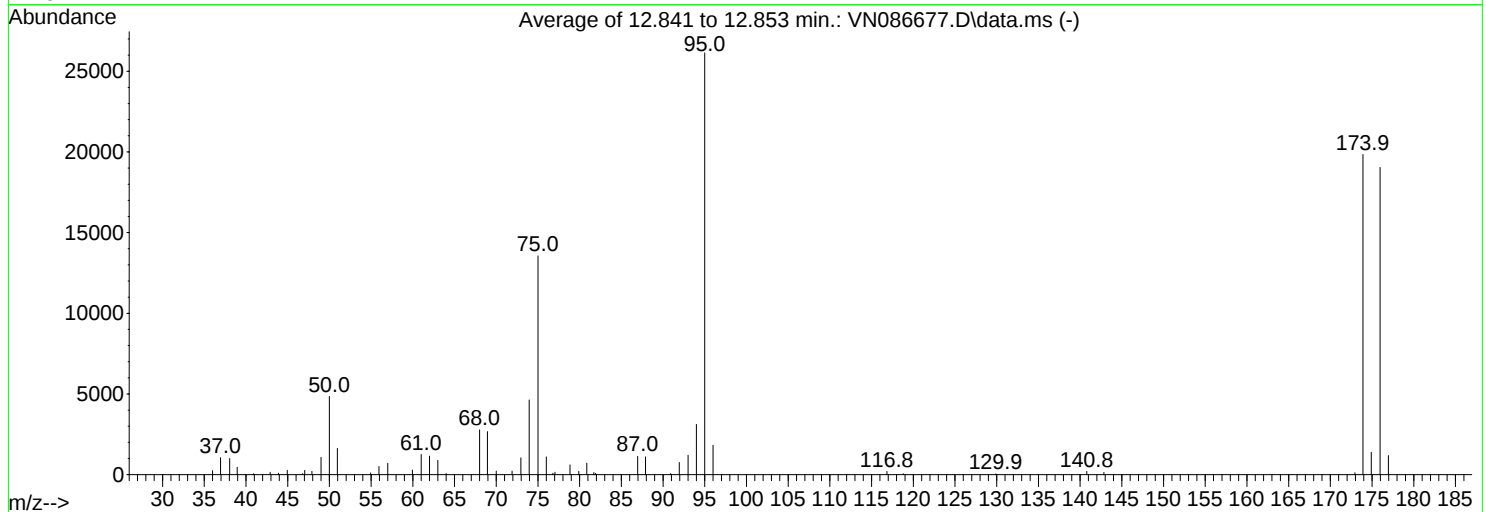


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN051925\
Data File : VN086677.D
Acq On : 19 May 2025 09:39
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N051625W.M
Title : SW846 8260
Last Update : Sat May 17 00:46:13 2025

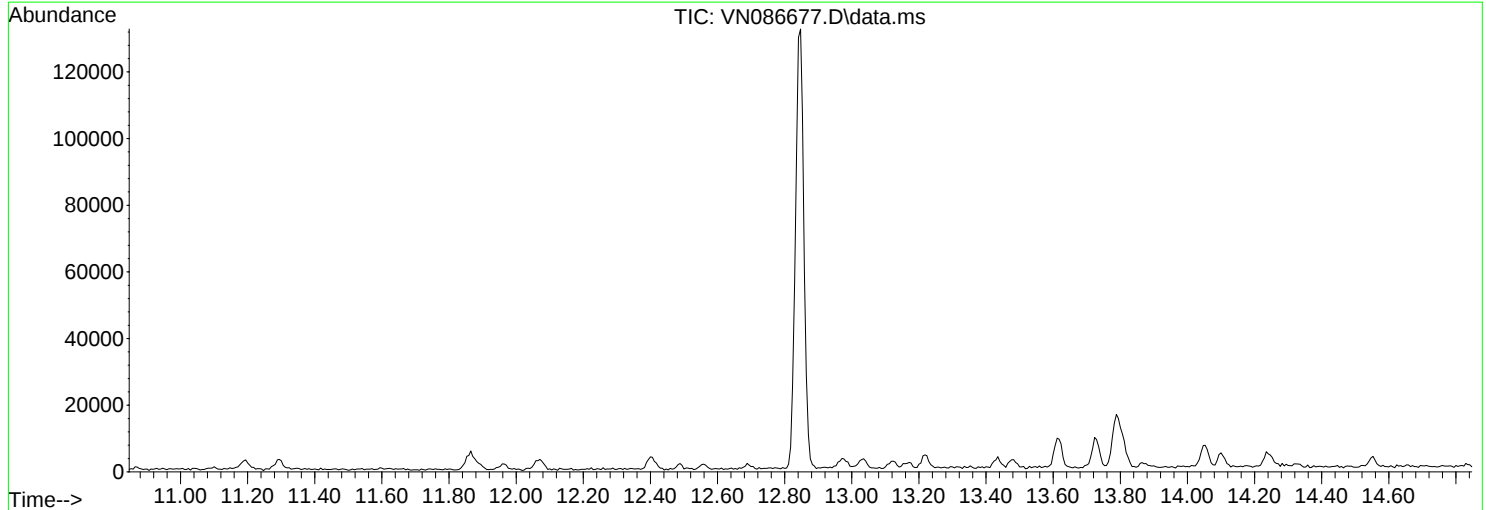

AutoFind: Scans 1851, 1852, 1853; Background Corrected with Scan 1843

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	18.5	4849	PASS
75	95	30	60	51.8	13552	PASS
95	95	100	100	100.0	26141	PASS
96	95	5	9	7.0	1827	PASS
173	174	0.00	2	0.6	115	PASS
174	95	50	100	75.9	19845	PASS
175	174	5	9	7.0	1389	PASS
176	174	95	101	95.9	19040	PASS
177	176	5	9	6.2	1177	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.00	245	47.90	211	64.00	68	78.85	60
36.95	1052	49.00	1071	68.00	2777	79.90	20
38.05	998	50.00	4849	68.95	2671	80.85	71
38.95	461	50.95	1624	70.00	215	81.70	12
39.90	21	54.95	107	71.90	223	81.90	80
40.90	57	55.95	509	72.95	1046	86.95	1134
42.90	147	57.00	703	73.95	4632	87.90	1097
43.90	87	59.95	284	75.00	13552	90.90	66
44.95	268	61.00	1247	76.00	1098	91.95	751
46.80	64	62.00	1155	76.80	91	93.00	1196
47.05	265	63.00	887	77.05	147	94.00	3113

Average of 12.841 to 12.853 min.: VN086677.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
95.00	26141	176.95	1177				
96.00	1827						
116.85	195						
118.80	58						
129.90	53						
140.80	195						
142.85	143						
172.95	115						
173.90	19845						
174.90	1389						
175.95	19040						

Instrument :

MSVOA_N

ClientSampleId :

BFB