Quantitation Report   (Not Reviewed)

Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN052019\
Data File : VN055665.D
Acq On   : 20 May 2019 11:37
Operator : JC/SP
Sample   : PB119556TB
Misc   : 5.00mL/MSVOA N/WATER
ALS Vial : 8   Sample Multiplier: 1

Quant Time: May 21 04:33:21 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N051719W.M
Quant Title : SW846 8260
QLast Update : Fri May 17 23:54:12 2019
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc Units	Dev(Min)
1) Pentafluorobenzene	7.67	168	441428	50.00 ug/l	0.00
34) 1,4-Difluorobenzene	8.59	114	624854	50.00 ug/l	0.00
63) Chlorobenzene-d5	11.41	117	540094	50.00 ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.34	152	217418	50.00 ug/l	0.00
System Monitoring Compounds					
33) 1,2-Dichloroethane-d4	8.03	65	200668	41.47 ug/l	0.00
Spiked Amount 50.000			Recovery =	82.94%	
35) Dibromofluoromethane	7.59	113	189364	47.71 ug/l	0.00
Spiked Amount 50.000			Recovery =	95.42%	
50) Toluene-d8	10.09	98	724668	48.28 ug/l	0.00
Spiked Amount 50.000			Recovery =	96.56%	
62) 4-Bromofluorobenzene	12.40	95	238529	46.02 ug/l	0.00
Spiked Amount 50.000			Recovery =	92.04%	

Target Compounds	R.T.	QIon	Response	Conc Units	Qvalue
13) Acrolein	3.61	56	69	1.511 ug/l #	1
16) Acetone	3.83	43	10503	5.319 ug/l	94
18) Methyl Acetate	4.33	43	3310	0.782 ug/l #	62
20) Methylene Chloride	4.56	84	3271	0.726 ug/l #	81
25) 2-Butanone	6.85	43	2905	1.052 ug/l	97
29) Tetrahydrofuran	7.22	42	986	0.539 ug/l #	39
31) Cyclohexane	7.67	56	6385	0.890 ug/l #	1
36) 1,1-Dichloropropene	7.67	75	25558	4.588 ug/l #	49
38) Carbon Tetrachloride	7.67	117	35561	5.974 ug/l #	15
41) Methacrylonitrile	7.21	41	535	0.249 ug/l #	100
43) Isopropyl Acetate	8.17	43	15372	1.758 ug/l #	91
45) 1,2-Dichloropropane	9.26	63	1739	0.403 ug/l #	43
48) Methyl methacrylate	9.18	41	8645	2.212 ug/l #	11
49) 1,4-Dioxane	9.26	88	91	1.172 ug/l #	1
51) 4-Methyl-2-Pentanone	9.99	43	4337	0.846 ug/l	91
54) cis-1,3-Dichloropropene	9.90	75	64725	9.271 ug/l #	56
57) 1,3-Dichloropropane	10.76	76	12735	1.900 ug/l #	42
59) 2-Hexanone	10.76	43	162632	45.033 ug/l #	51
65) Chlorobenzene	11.44	112	3012	0.276 ug/l	94
68) m/p-Xylenes	11.62	106	1742	0.237 ug/l #	36
73) Isopropylbenzene	12.25	105	1126	Below Cal	94
74) N-amyl acetate	11.88	43	18785	3.077 ug/l #	51
75) 1,1,2,2-Tetrachloroethane	12.52	83	197	Below Cal #	26
76) 1,2,3-Trichloropropane	12.40	75	106982	24.114 ug/l #	100
77) Bromobenzene	12.53	156	108126	24.215 ug/l #	1
79) 2-Chlorotoluene	12.68	91	986	Below Cal #	60
80) 1,3,5-Trimethylbenzene	12.73	105	14045	Below Cal	99
81) trans-1,4-Dichloro-2-buten	12.40	75	106982	61.988 ug/l #	17
83) tert-Butylbenzene	12.99	119	879	Below Cal #	67
84) 1,2,4-Trimethylbenzene	13.04	105	2405	Below Cal	73
85) sec-Butylbenzene	13.17	105	1516	Below Cal	98
86) p-Isopropyltoluene	13.29	119	1617	Below Cal	87
90) Hexachloroethane	13.88	117	168	Below Cal	59
91) 1,2-Dichlorobenzene	13.66	146	1587	0.216 ug/l	81

Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN052019\
Data File : VN055665.D
Acq On : 20 May 2019 11:37
Operator : JC/SP
Sample : PB119556TB
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 8 Sample Multiplier: 1

Quant Time: May 21 04:33:21 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N051719W.M
Quant Title : SW846 8260
QLast Update : Fri May 17 23:54:12 2019
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc Units	Dev(Min)
92) 1,2-Dibromo-3-Chloropropan	14.26	75	411	0.417 ug/l #	47
93) 1,2,4-Trichlorobenzene	14.91	180	1989	0.531 ug/l #	82
94) Hexachlorobutadiene	15.02	225	537	Below Cal	78
95) Naphthalene	15.14	128	11648	2.758 ug/l #	86
96) 1,2,3-Trichlorobenzene	15.32	180	2117	0.540 ug/l #	89

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Quantitation Report (Not Reviewed)

Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN052019\
Data File : VN055665.D
Acq On : 20 May 2019 11:37
Operator : JC/SP
Sample : PB119556TB
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 8 Sample Multiplier: 1

Quant Time: May 21 04:33:21 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N051719W.M
Quant Title : SW846 8260
QLast Update : Fri May 17 23:54:12 2019
Response via : Initial Calibration

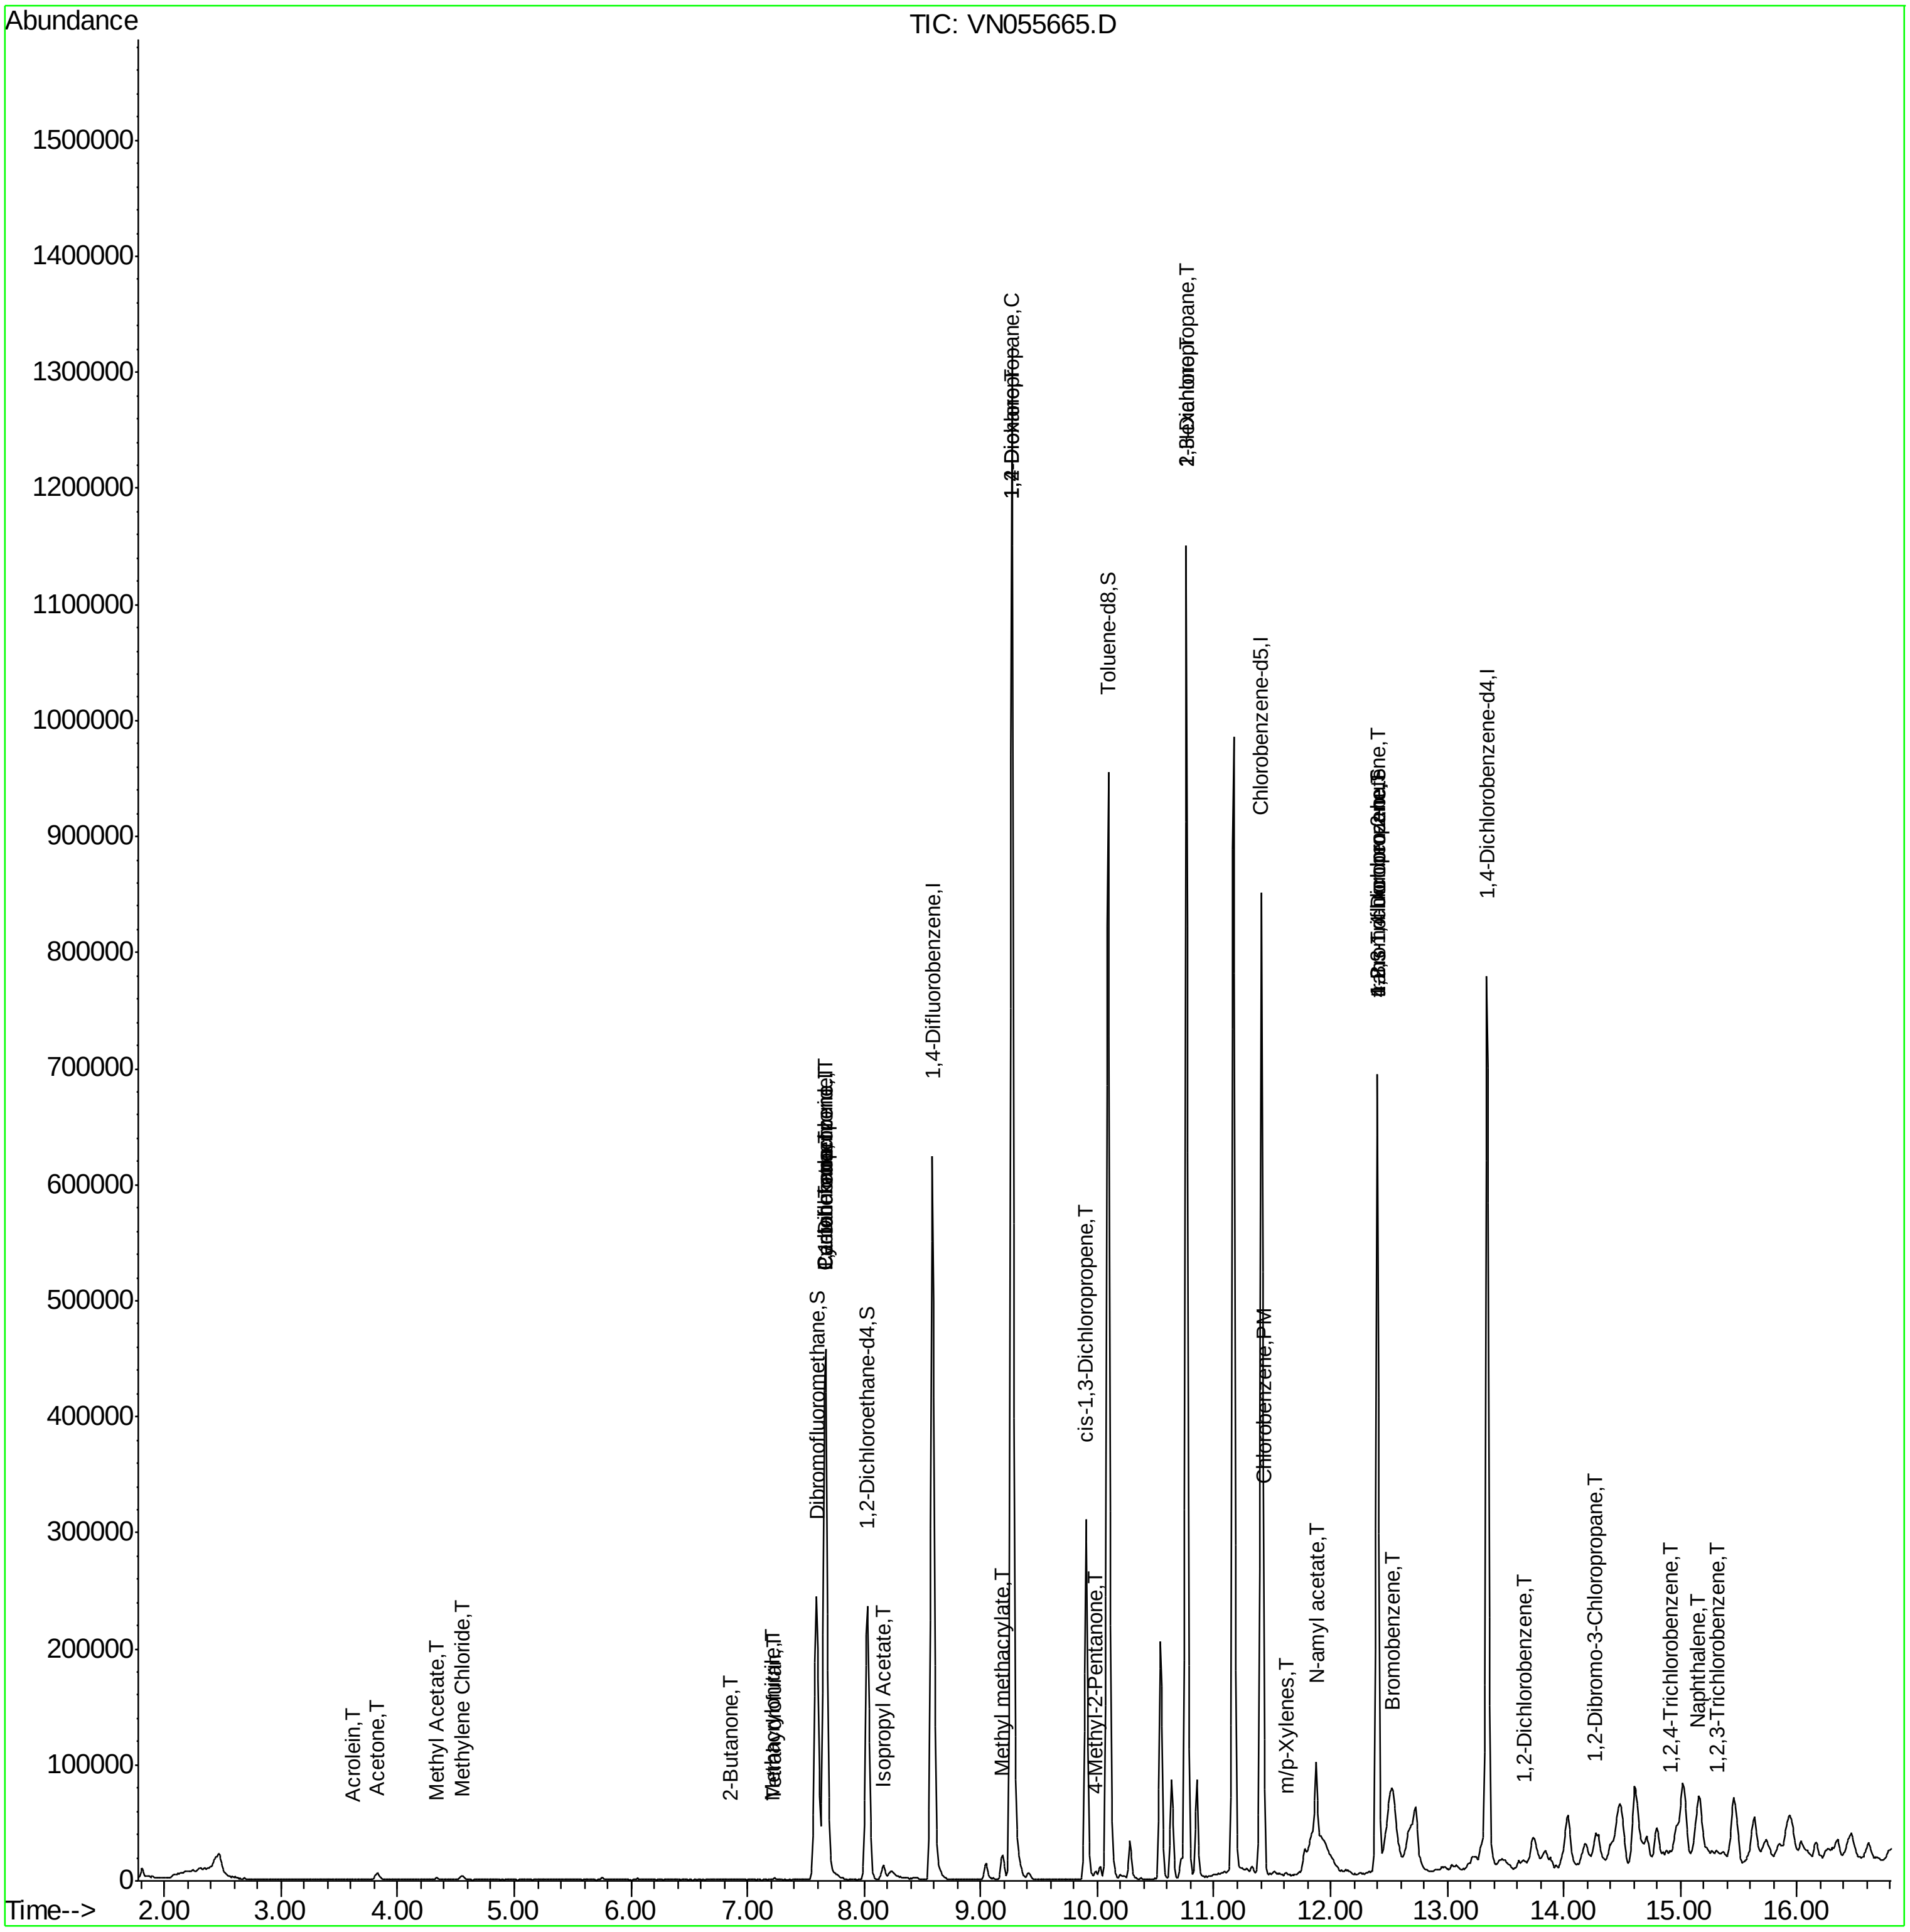

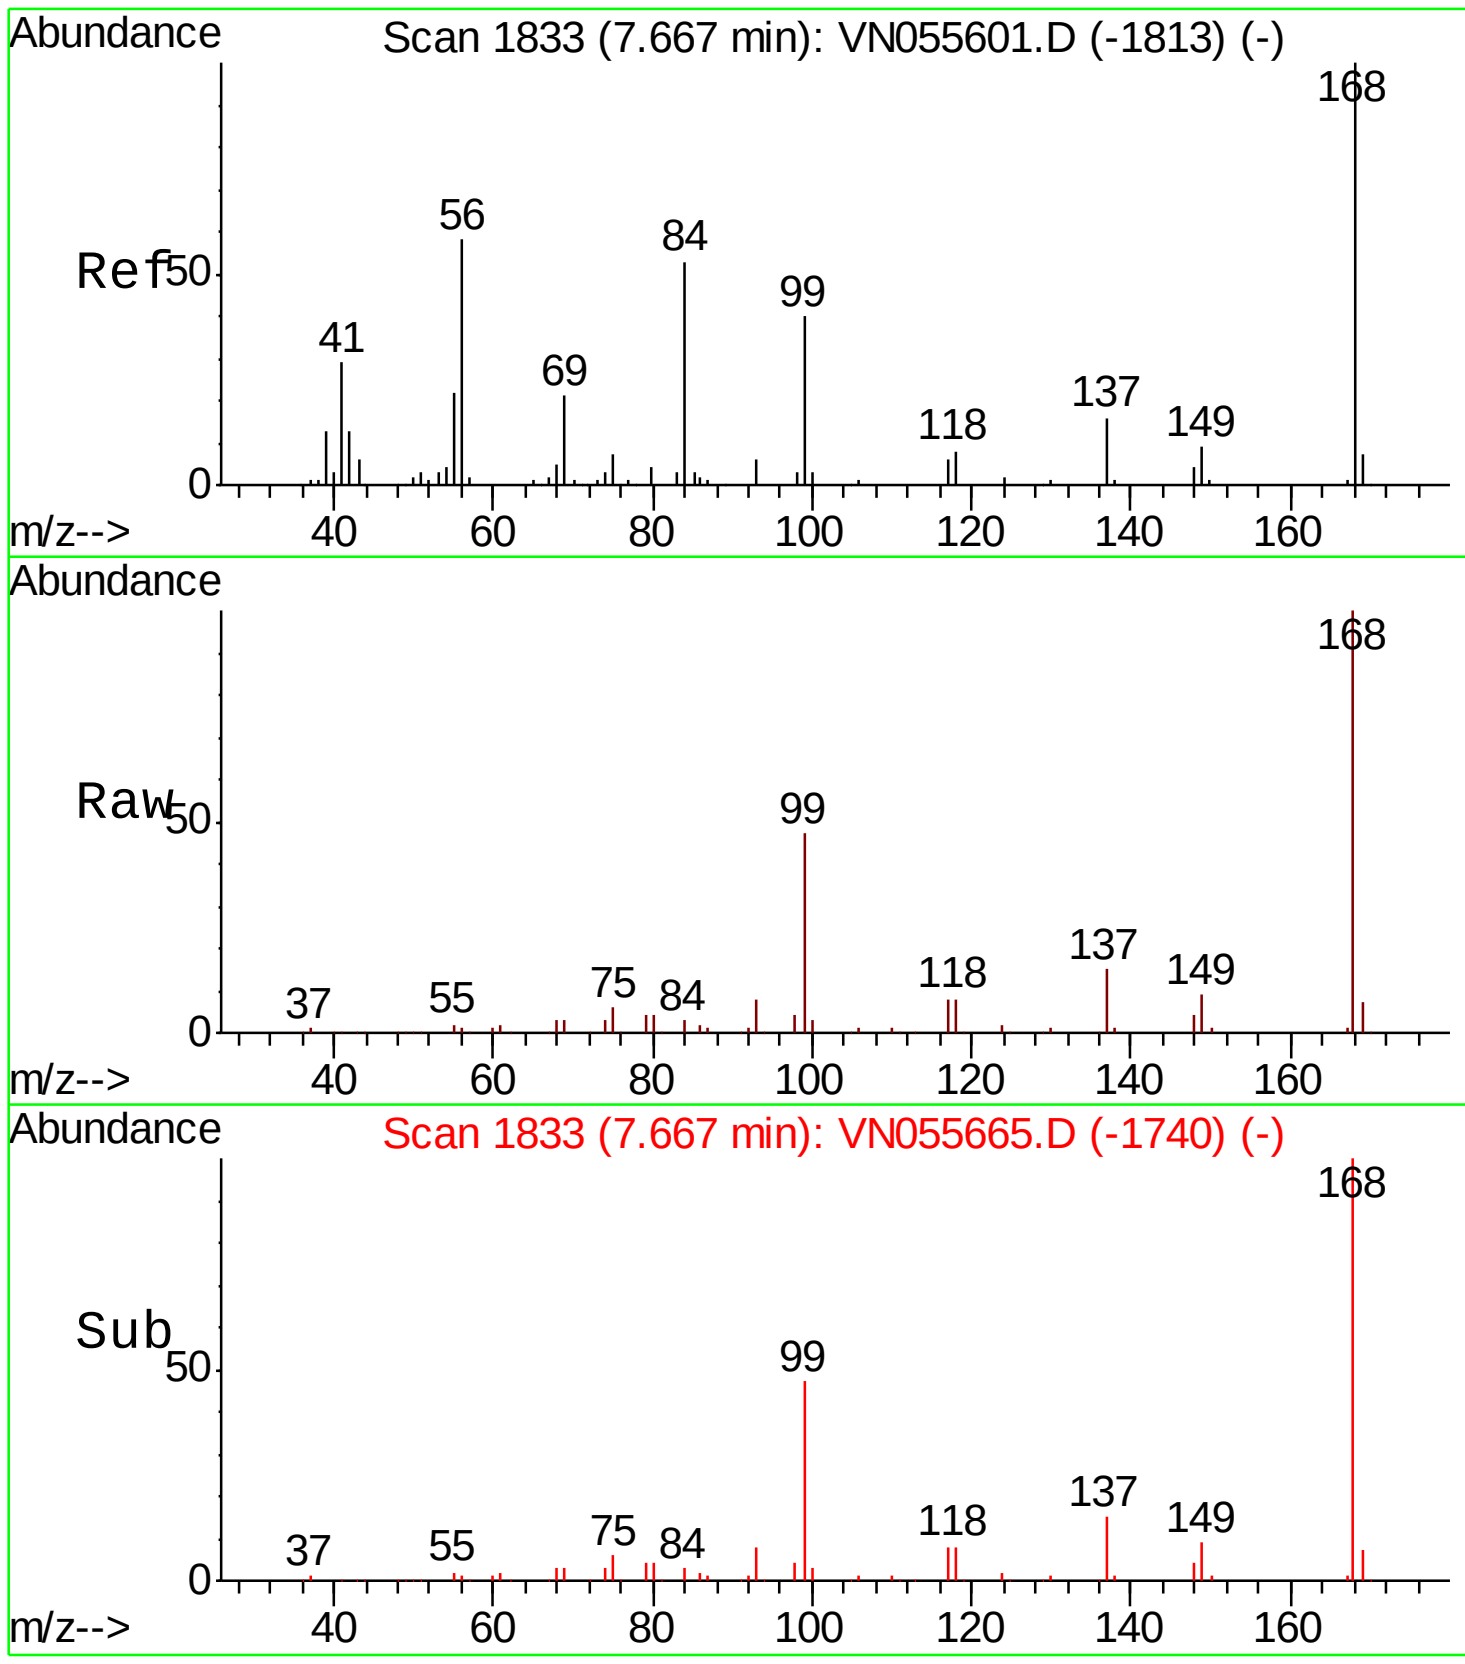

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.67 min Scan# 1833
Delta R.T.   -0.00 min
Lab File: VN055665.D
Acq: 20 May 2019 11:37

Tgt Ion:168 Resp: 441428

Ion	Ratio	Lower	Upper
168	100		
99	47.5	40.2	60.2



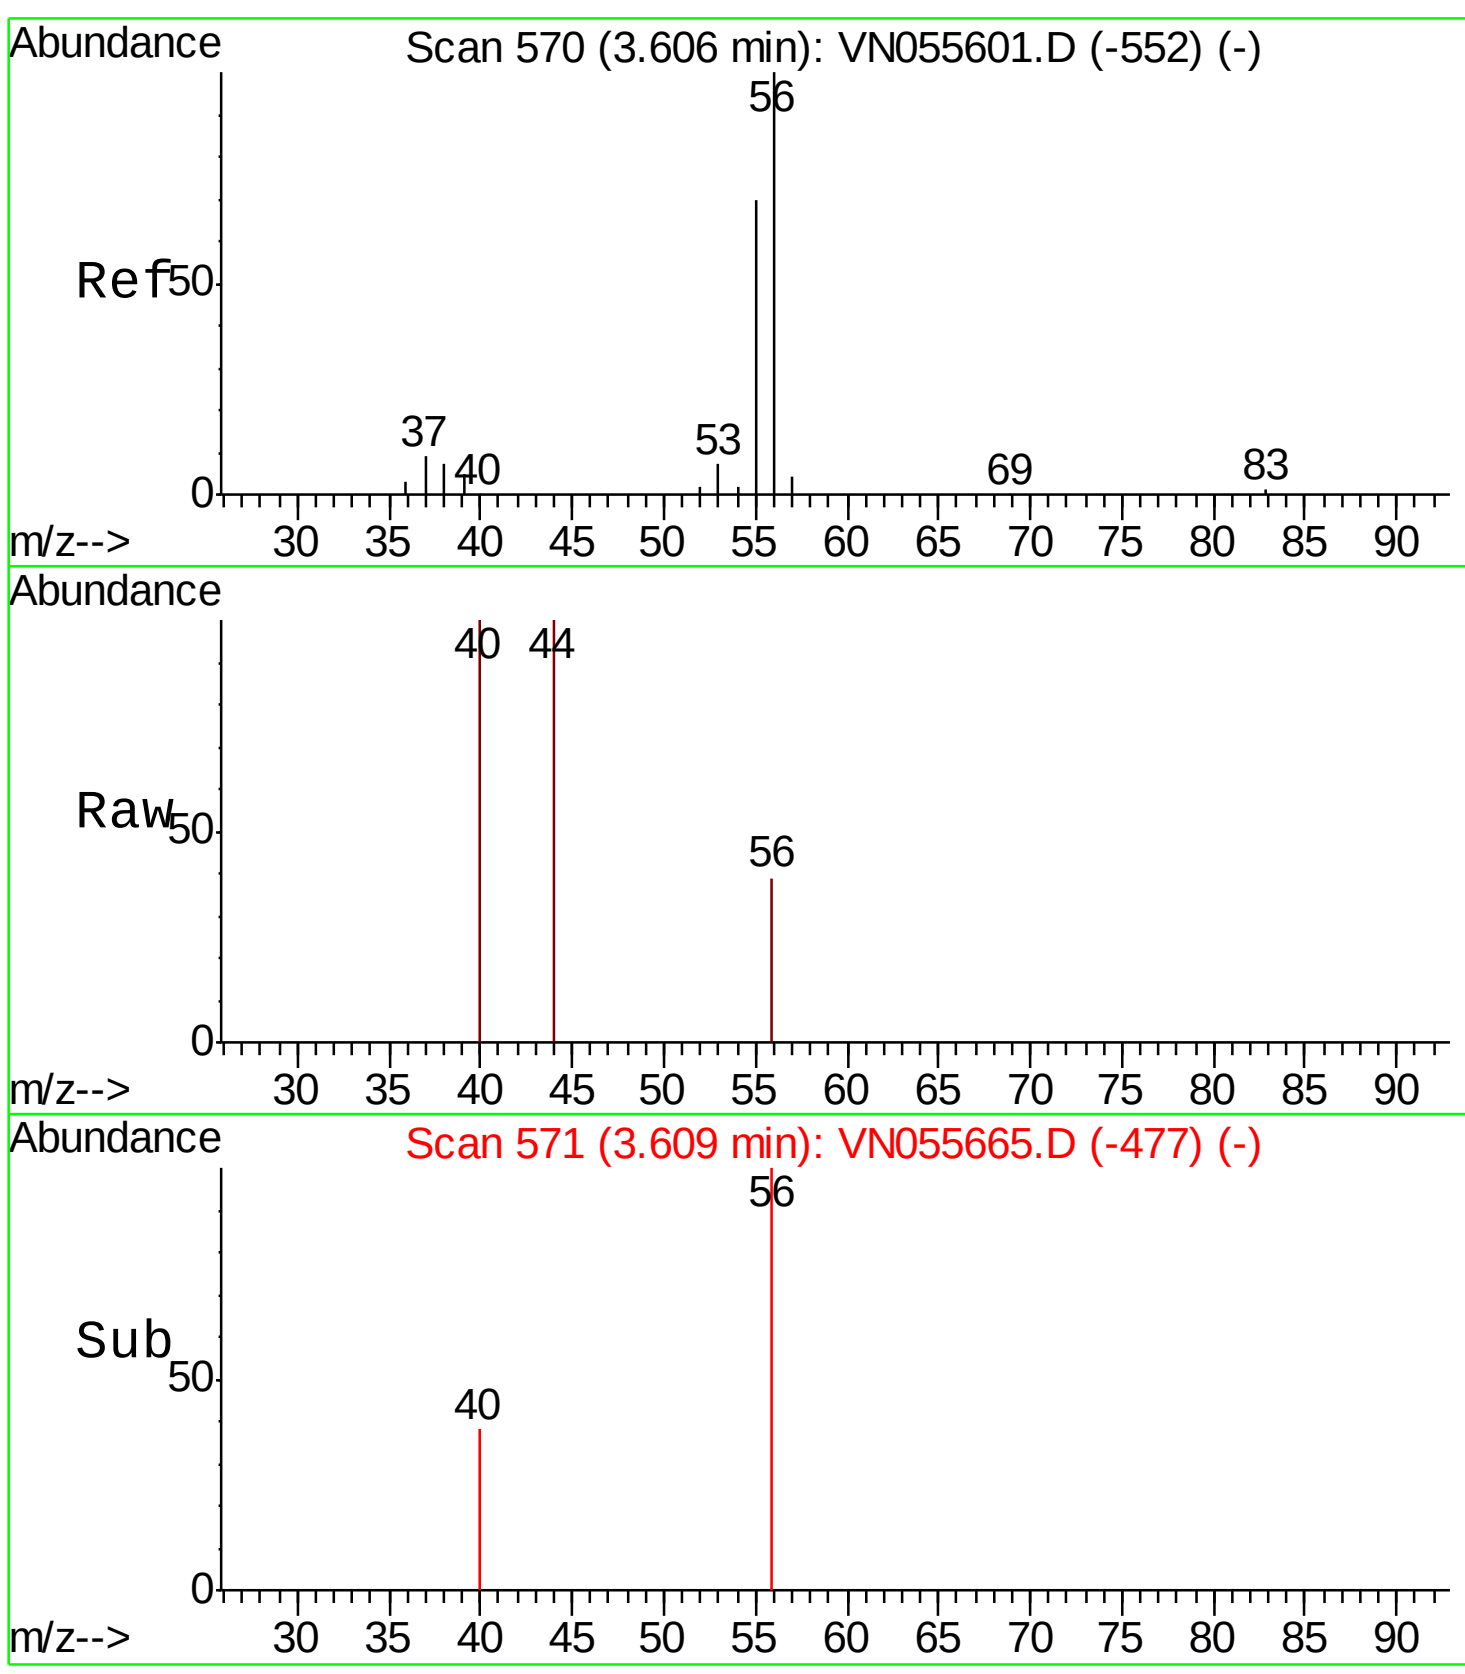

#13
Acrolein
Concen: 1.511 ug/l
RT: 3.61 min Scan# 571
Delta R.T.   0.00 min
Lab File: VN055665.D
Acq: 20 May 2019 11:37

Tgt Ion: 56 Resp: 69

Ion	Ratio	Lower	Upper
56	100		
55	231.9	56.5	84.7#



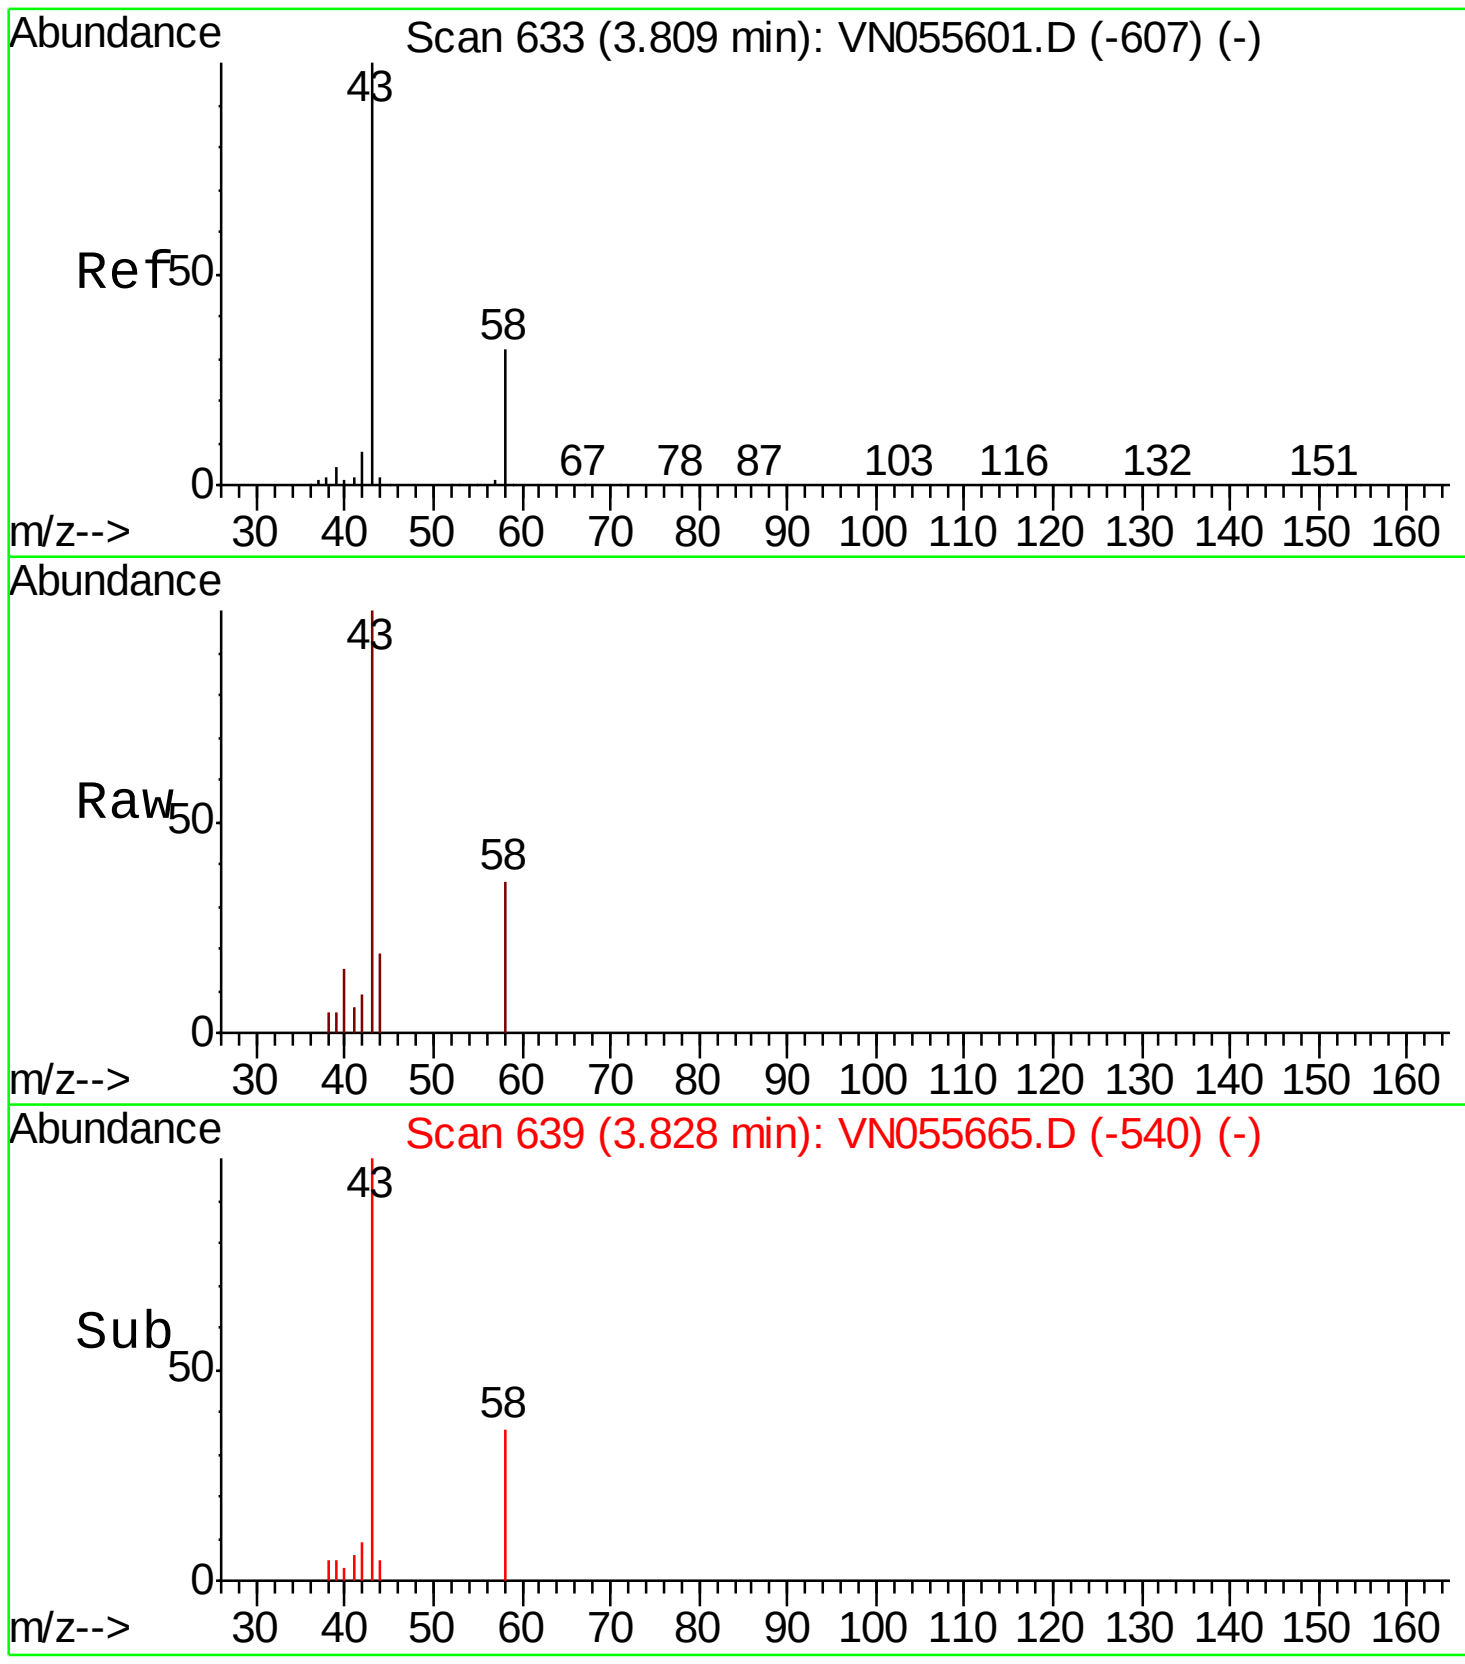

#16
Acetone
Concen: 5.319 ug/l
RT: 3.83 min Scan# 639
Delta R.T.   0.02 min
Lab File: VN055665.D
Acq: 20 May 2019 11:37

Tgt Ion: 43 Resp: 10503

Ion	Ratio	Lower	Upper
43	100		
58	35.6	26.0	39.0



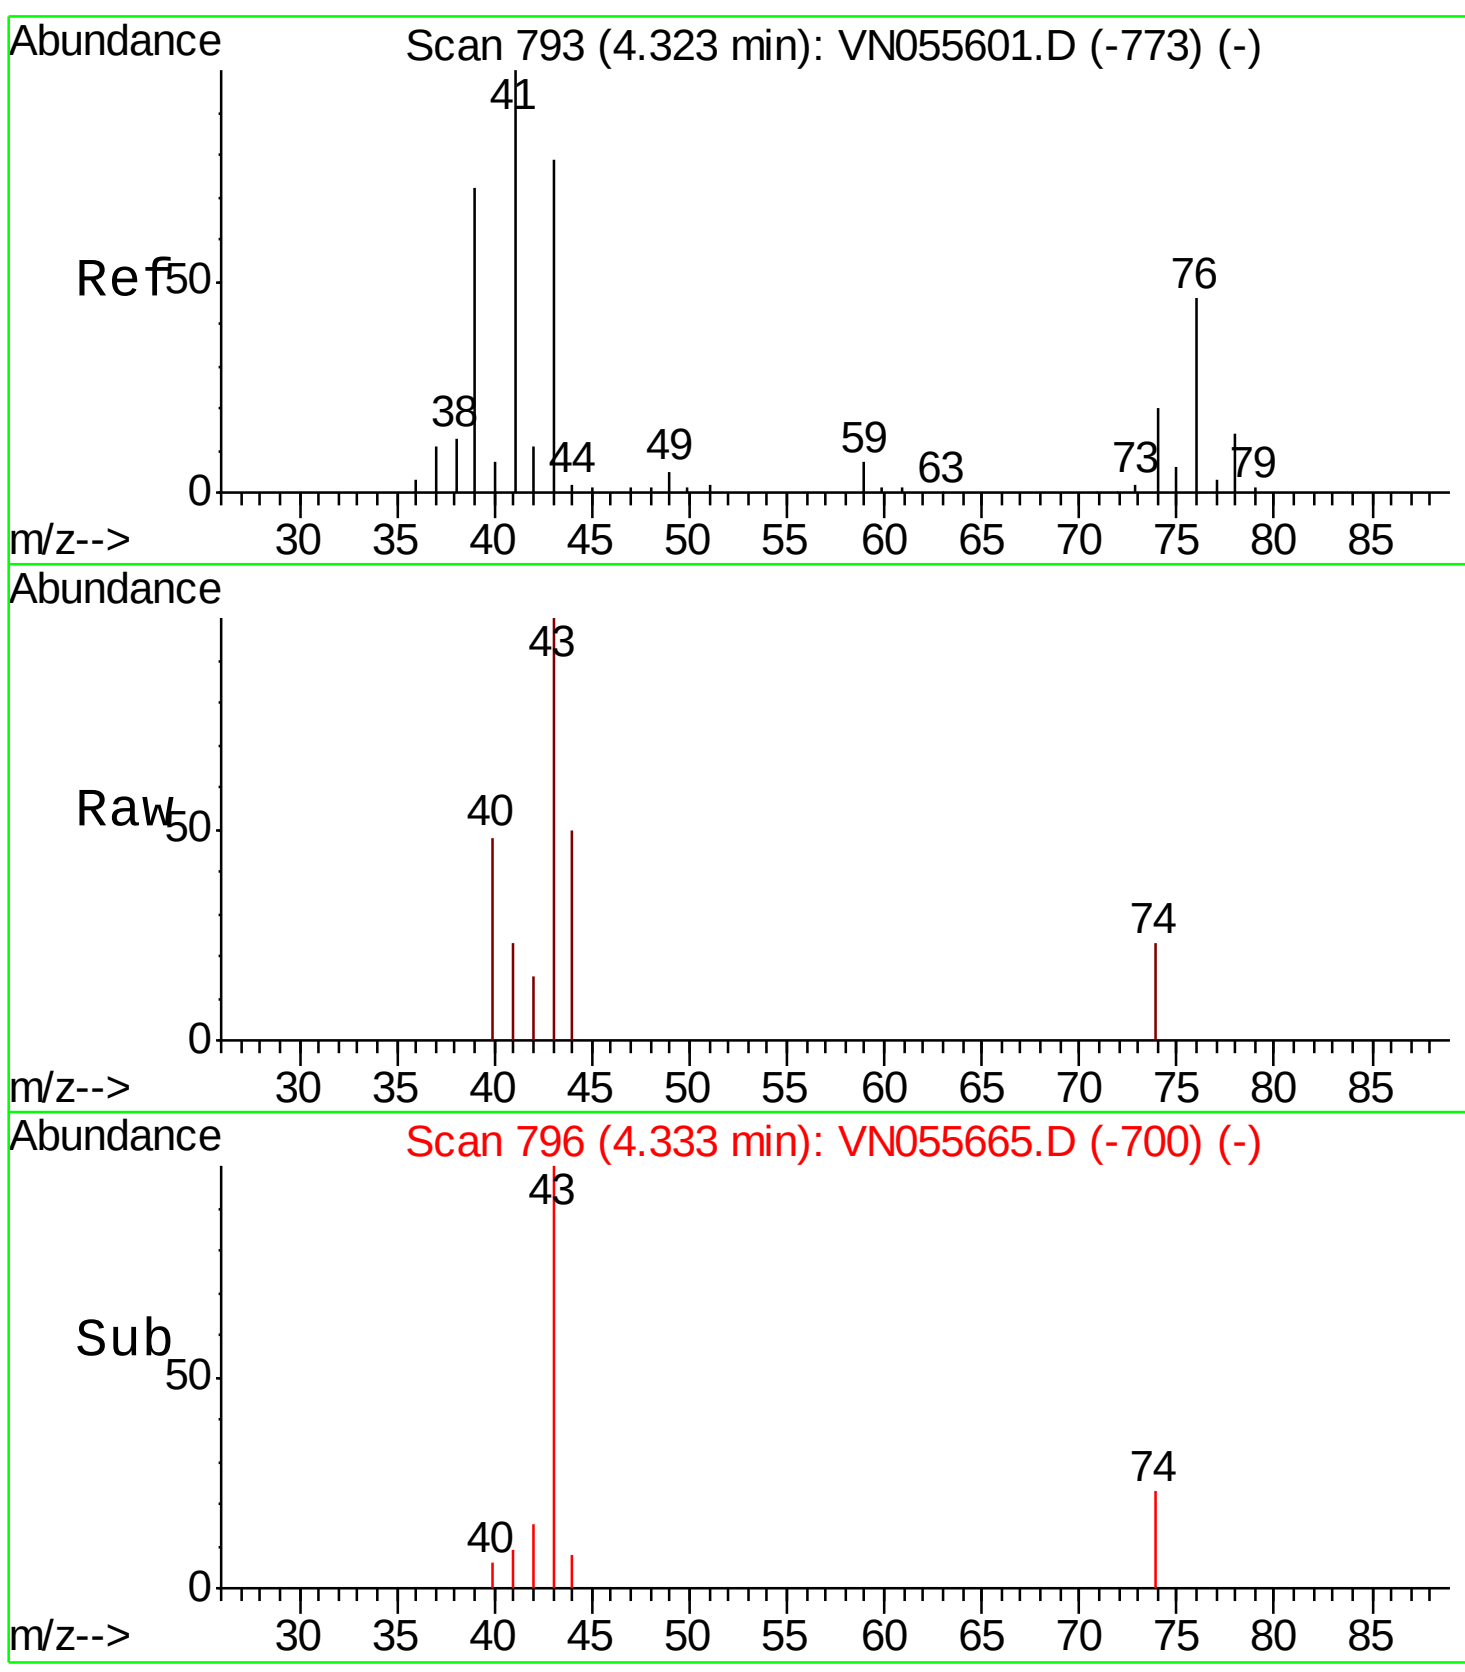

#18
Methyl Acetate
Concen: 0.782 ug/l
RT: 4.33 min Scan# 796
Delta R.T.   0.01 min
Lab File: VN055665.D
Acq: 20 May 2019 11:37

Tgt Ion: 43 Resp: 3310

Ion	Ratio	Lower	Upper
43	100		
74	6.1	19.9	29.9#



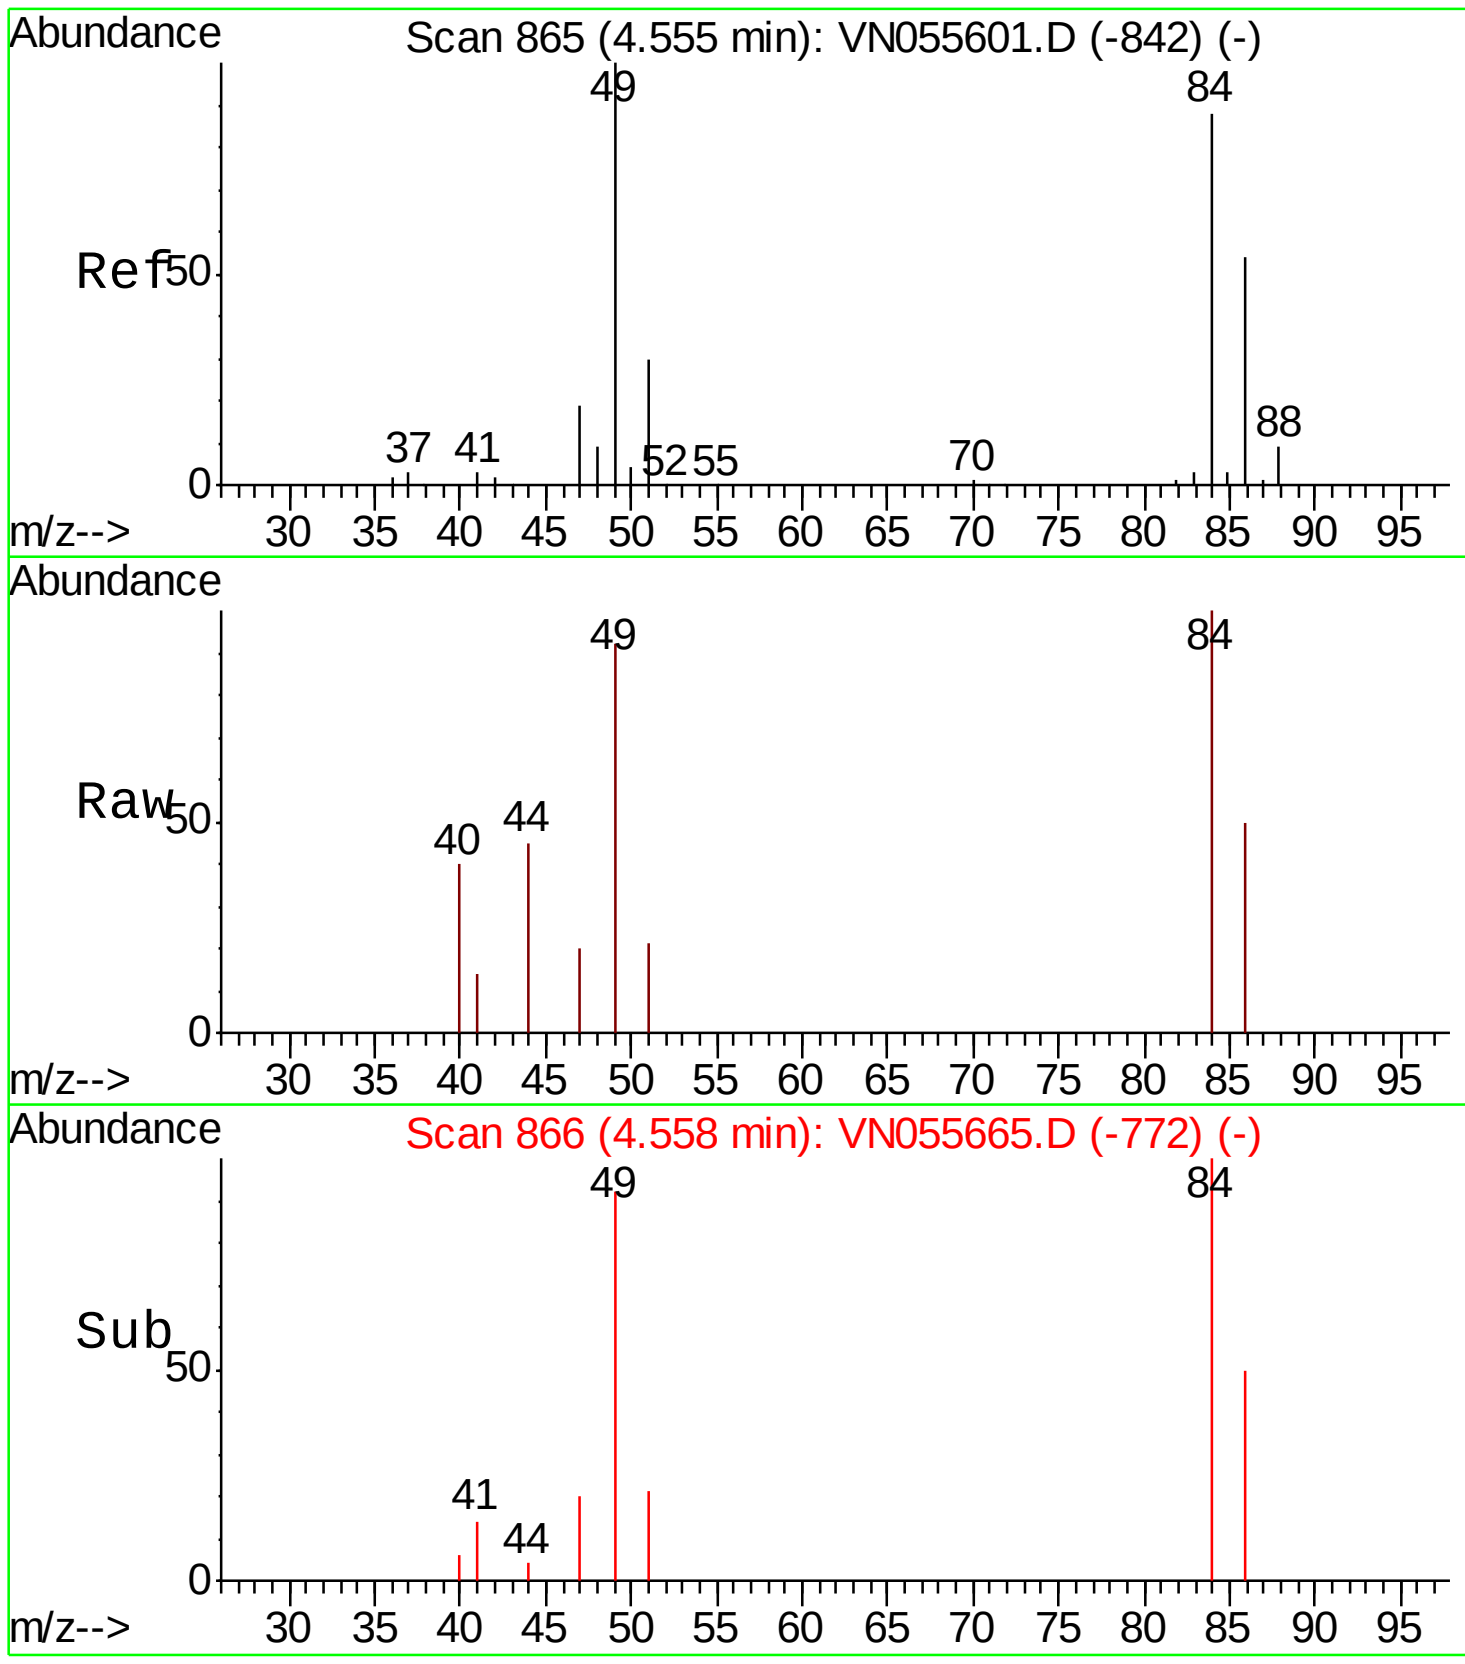

#20
Methylene Chloride
Concen: 0.726 ug/l
RT: 4.56 min Scan# 866
Delta R.T. 0.00 min
Lab File: VN055665.D
Acq: 20 May 2019 11:37

Tgt Ion: 84 Resp: 3271

Ion	Ratio	Lower	Upper
84	100		
49	92.2	91.0	136.4
51	21.0	27.5	41.3#
86	50.3	49.4	74.0



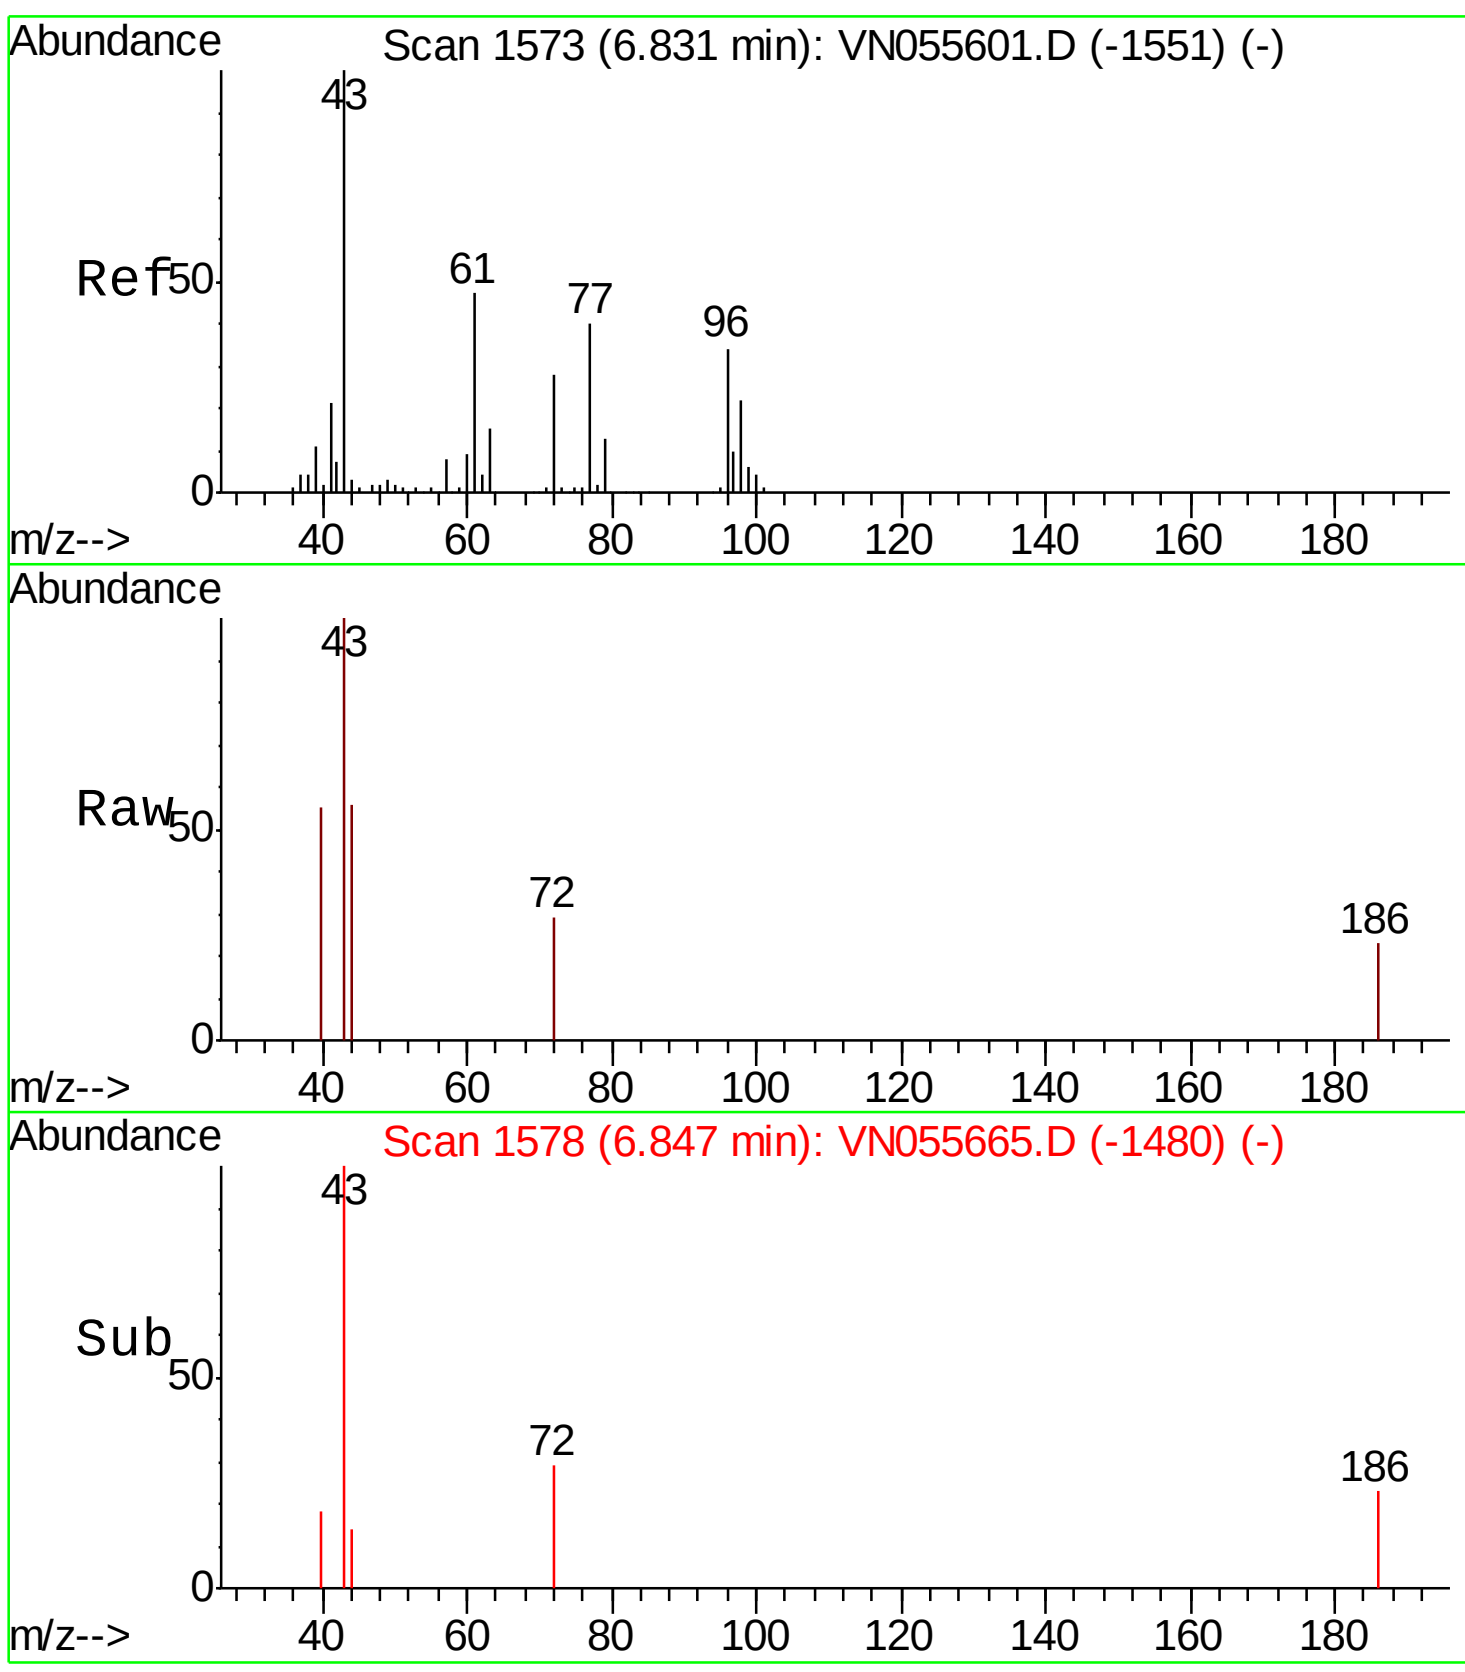

#25
2-Butanone
Concen: 1.052 ug/l
RT: 6.85 min Scan# 1578
Delta R.T. 0.02 min
Lab File: VN055665.D
Acq: 20 May 2019 11:37

Tgt Ion: 43 Resp: 2905

Ion	Ratio	Lower	Upper
43	100		
72	29.4	22.3	33.5



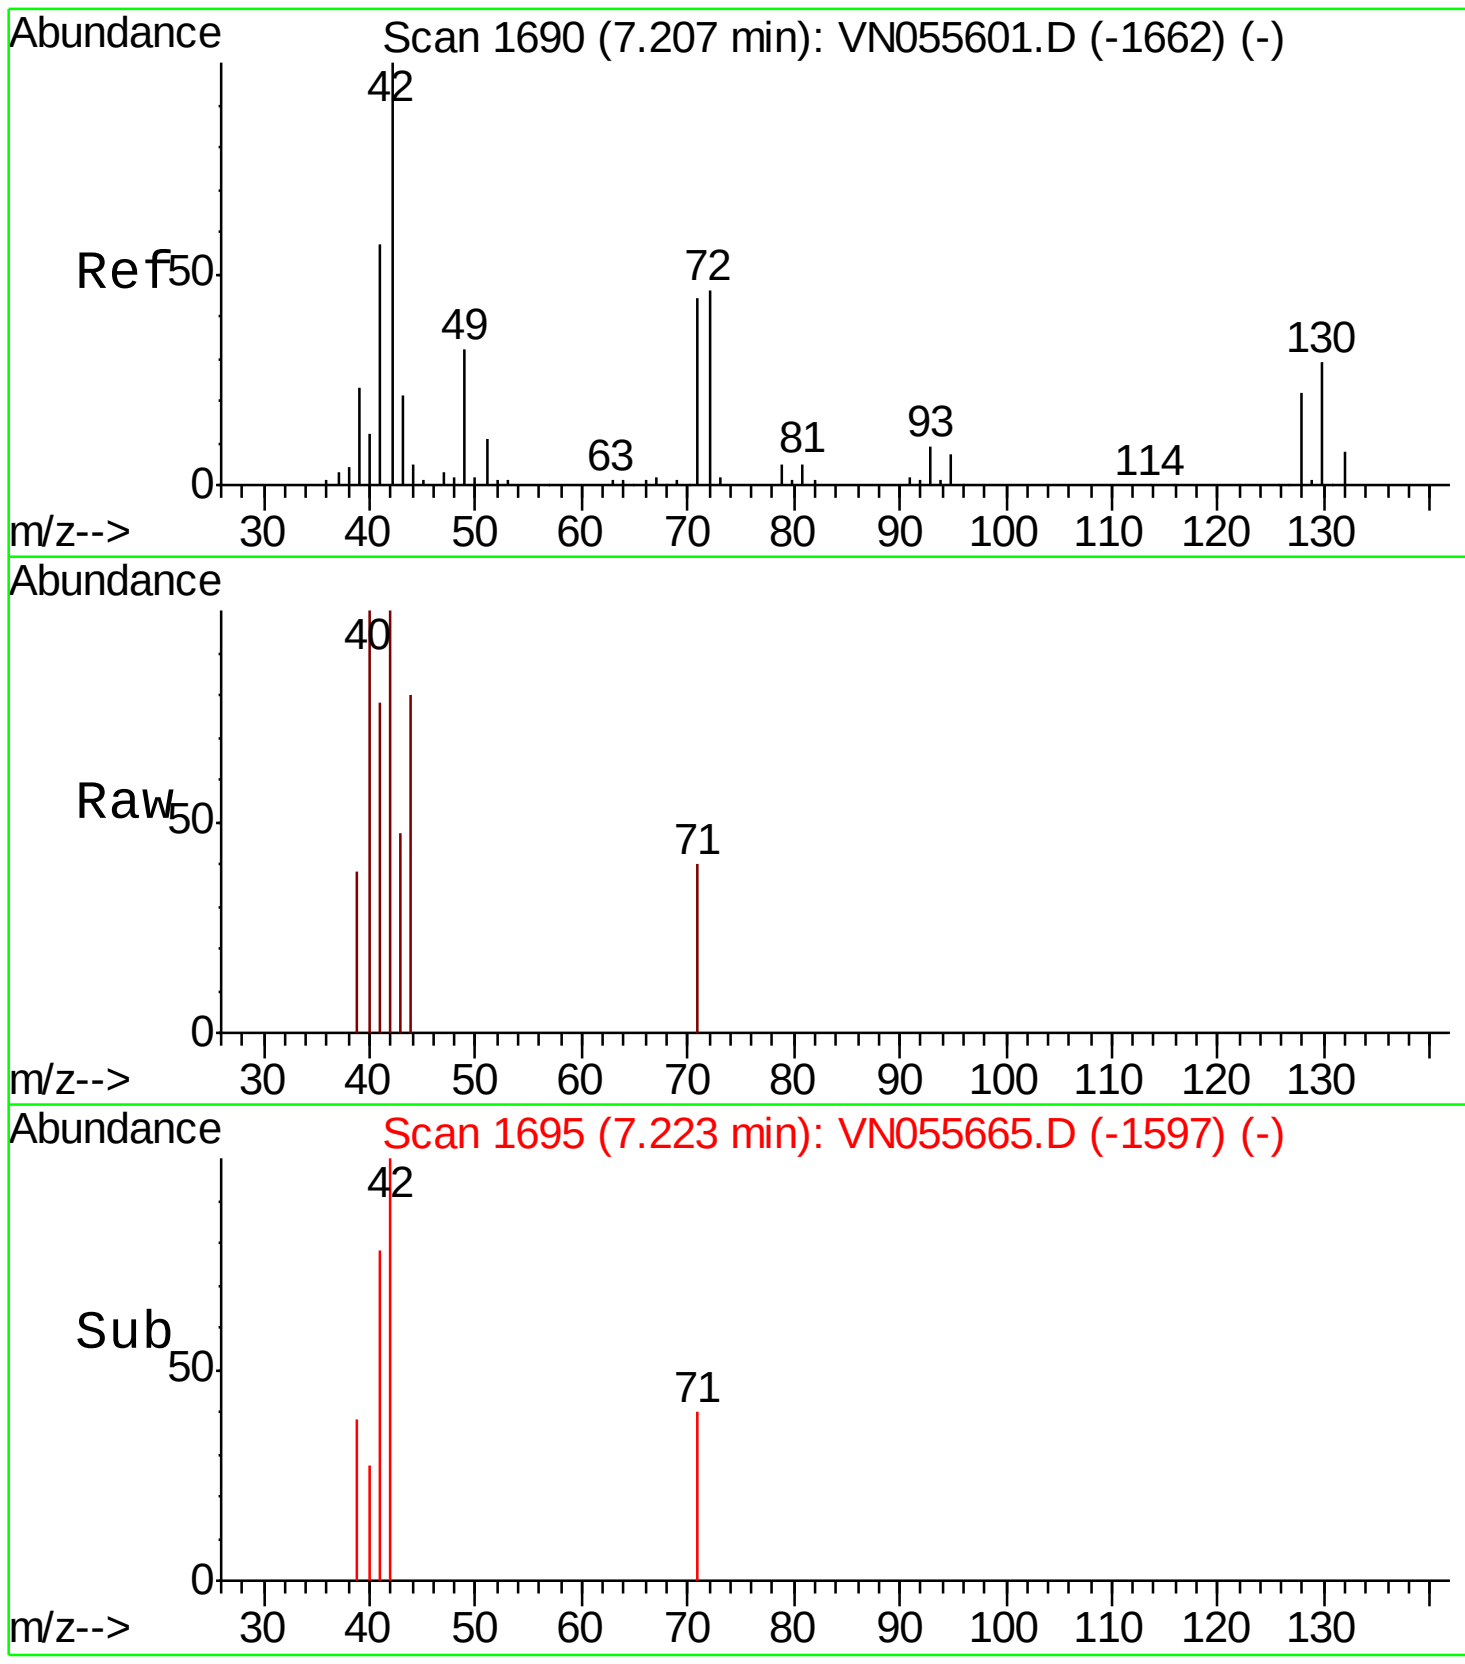

#29
Tetrahydrofuran
Concen: 0.539 ug/l
RT: 7.22 min   Scan# 1695
Delta R.T.   0.02 min
Lab File: VN055665.D
Acq: 20 May 2019   11:37

Tgt Ion: 42 Resp: 986

Ion	Ratio	Lower	Upper
42	100		
72	9.5	36.5	54.7#
71	0.0	34.9	52.3#



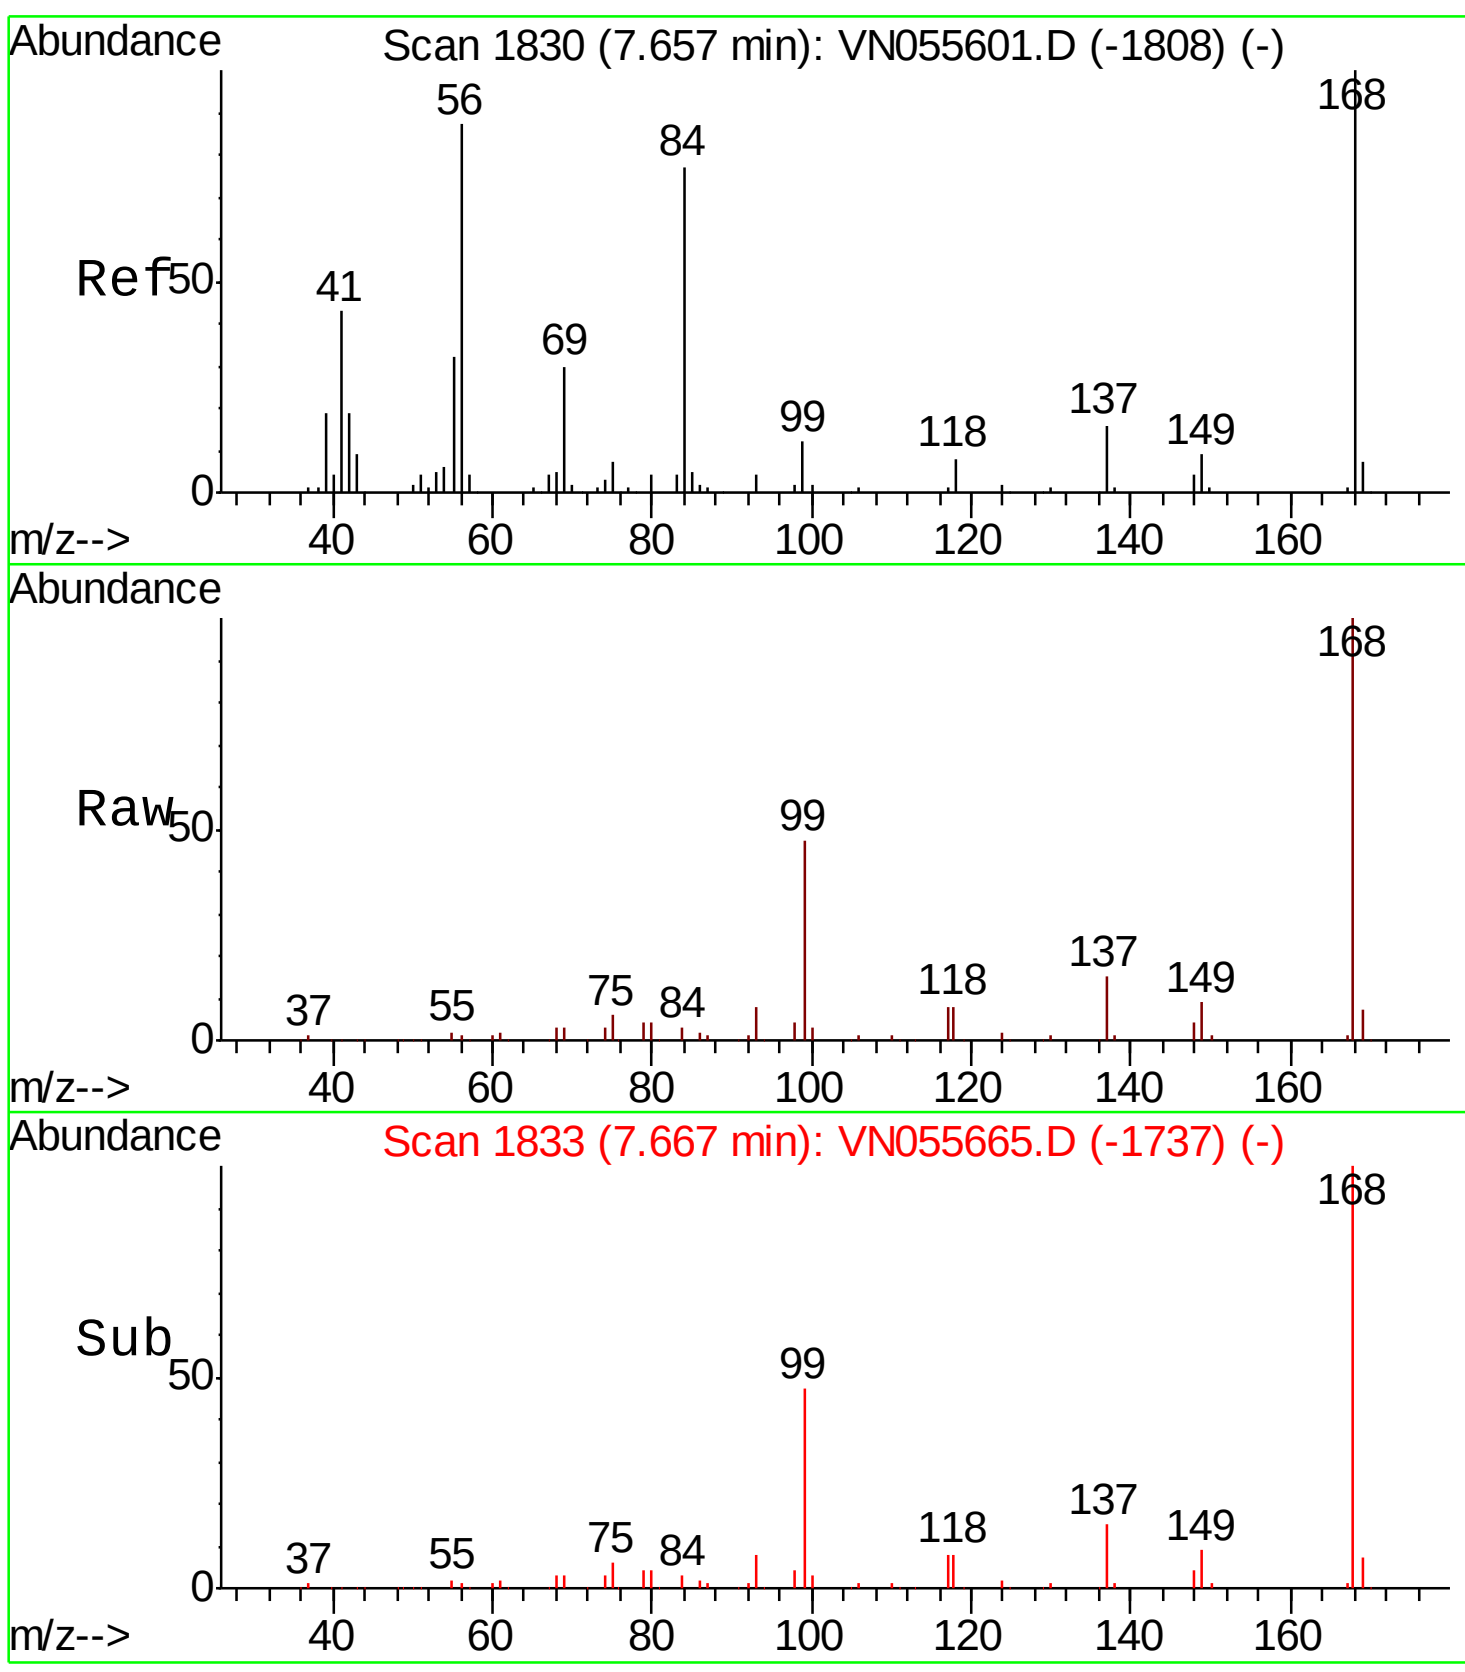

#31
Cyclohexane
Concen: 0.890 ug/l
RT: 7.67 min   Scan# 1833
Delta R.T.   0.01 min
Lab File: VN055665.D
Acq: 20 May 2019   11:37

Tgt Ion: 56 Resp: 6385

Ion	Ratio	Lower	Upper
56	100		
69	198.8	27.2	40.8#
84	178.6	71.3	106.9#



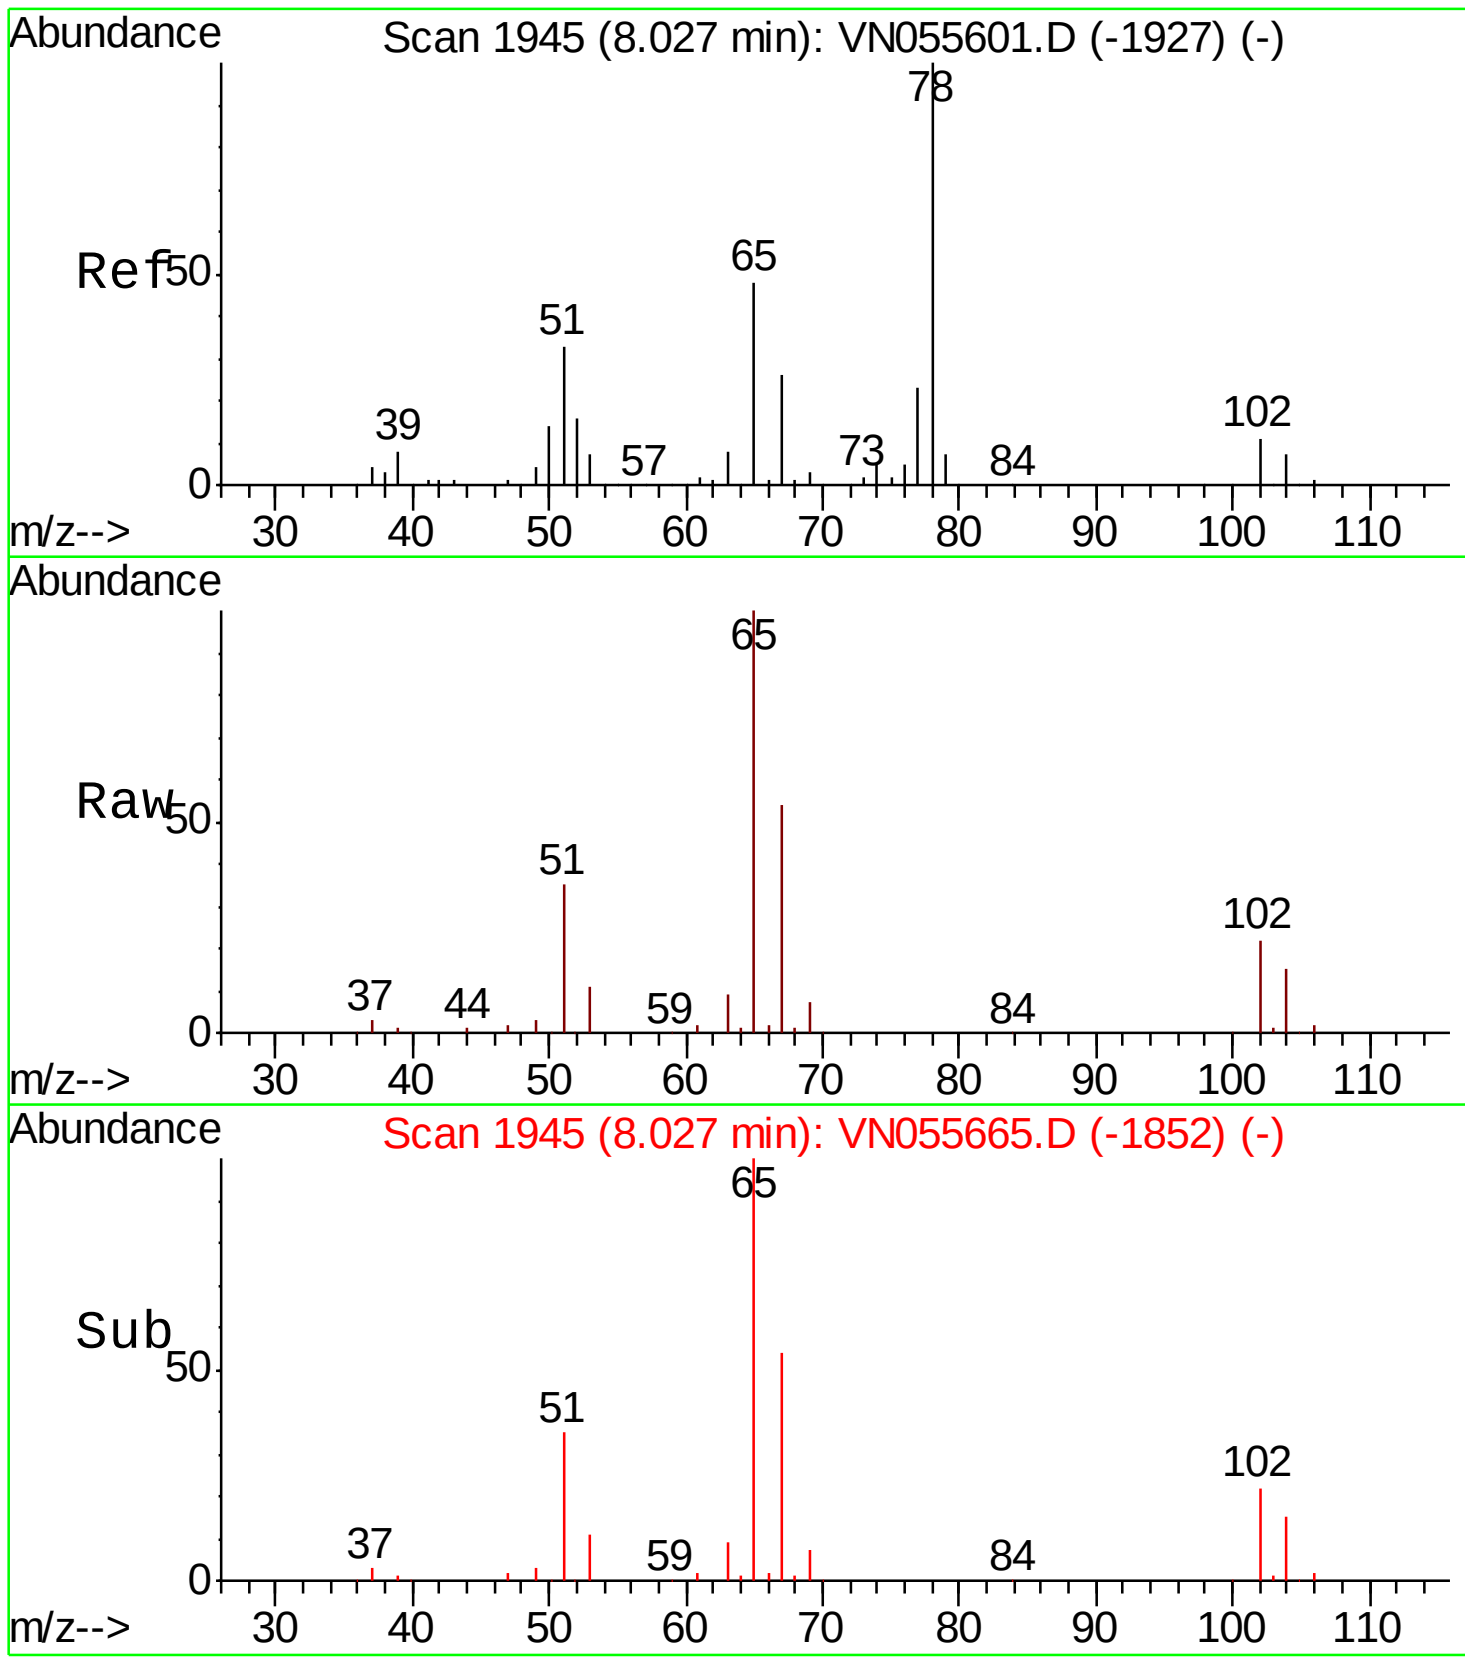

#33
1,2-Dichloroethane-d4
Concen: 41.469 ug/l
RT: 8.03 min   Scan# 1945
Delta R.T.   -0.00 min
Lab File: VN055665.D
Acq: 20 May 2019   11:37

Tgt Ion: 65 Resp: 200668

Ion	Ratio	Lower	Upper
65	100		
67	54.5	0.0	108.6



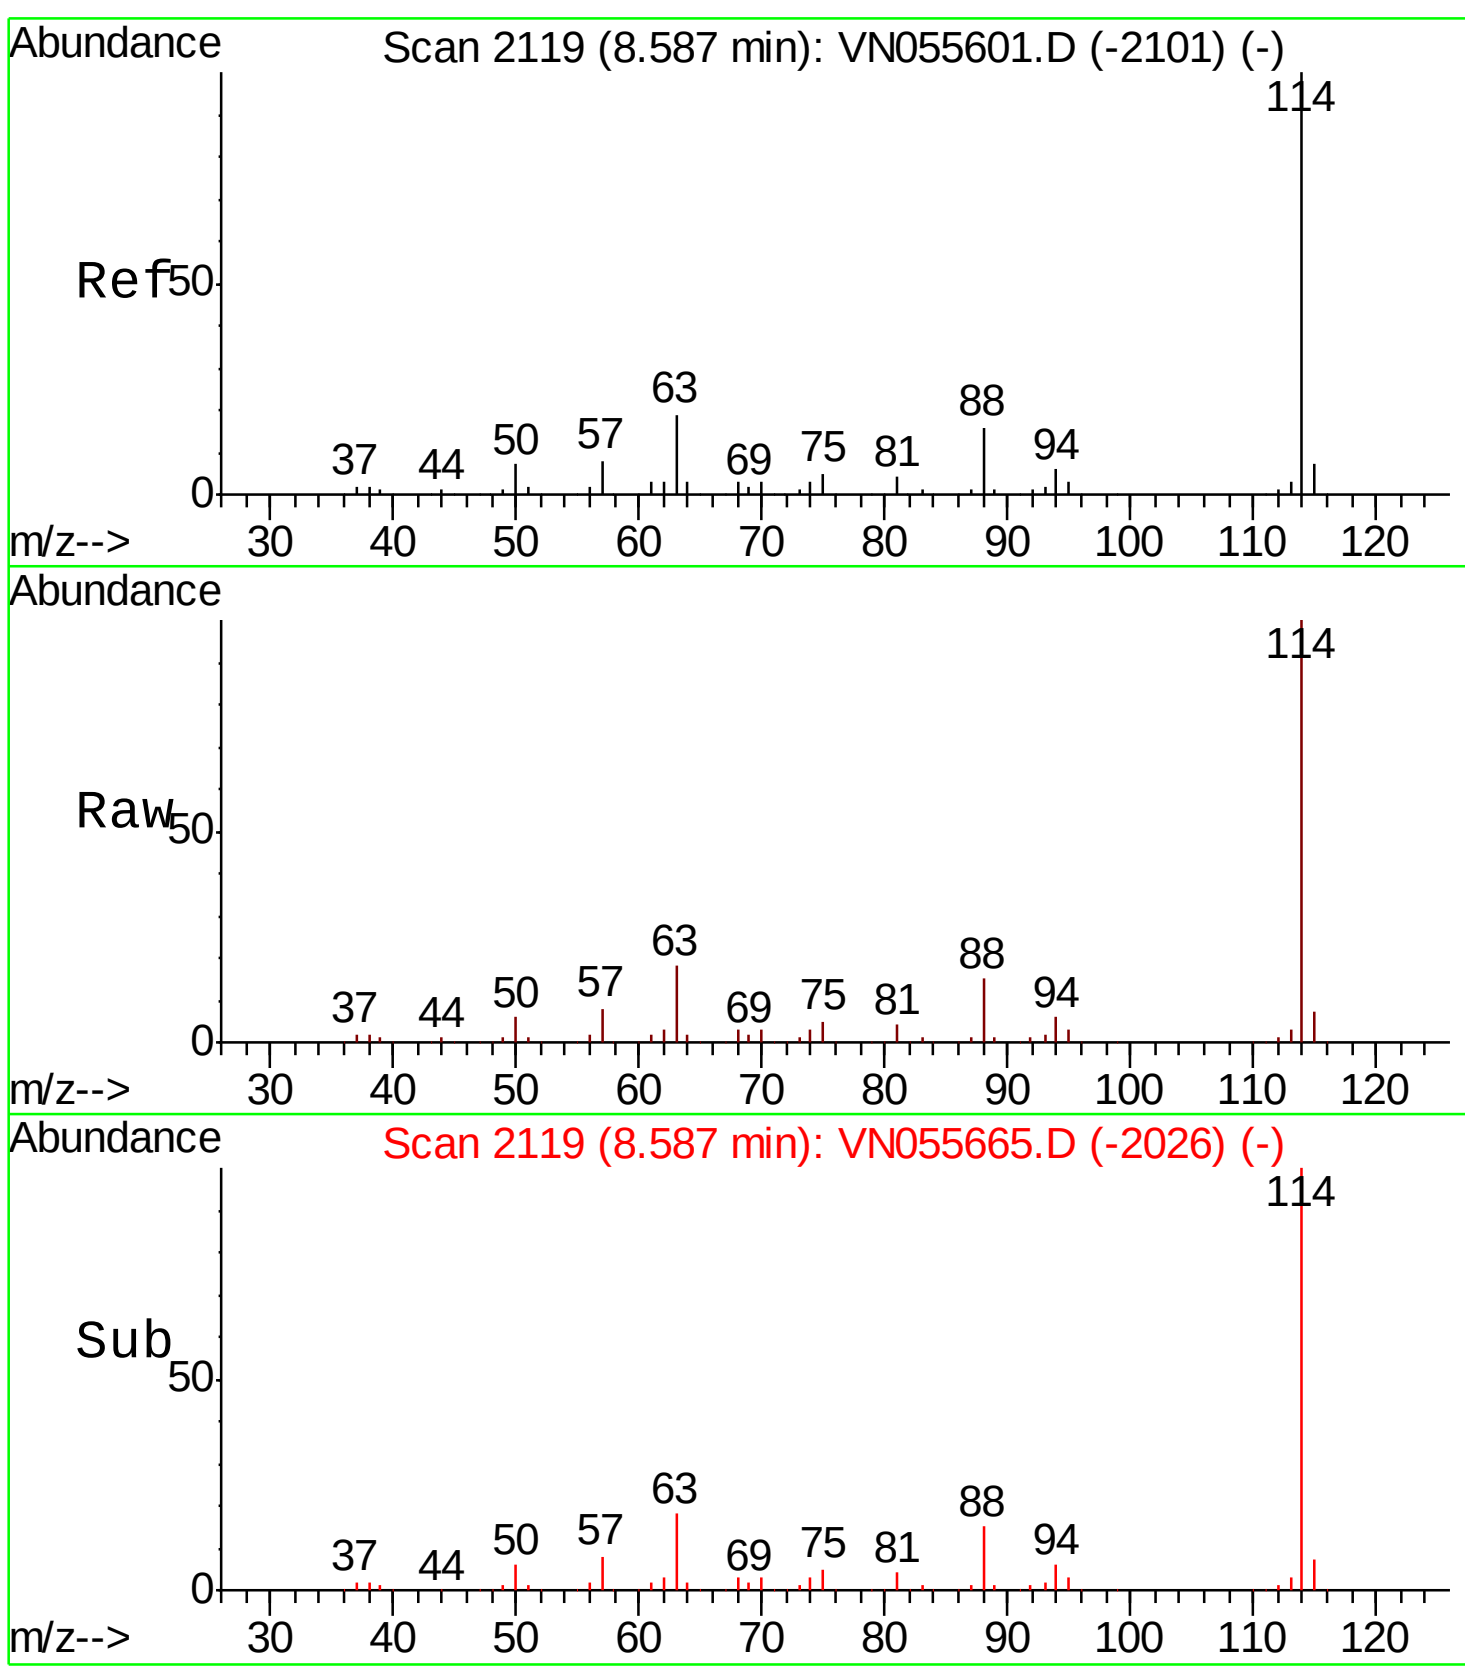

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 8.59 min   Scan# 2119
Delta R.T.   -0.00 min
Lab File: VN055665.D
Acq: 20 May 2019   11:37

Tgt Ion:114 Resp: 624854

Ion	Ratio	Lower	Upper
114	100		
63	18.4	0.0	38.2
88	15.4	0.0	31.0

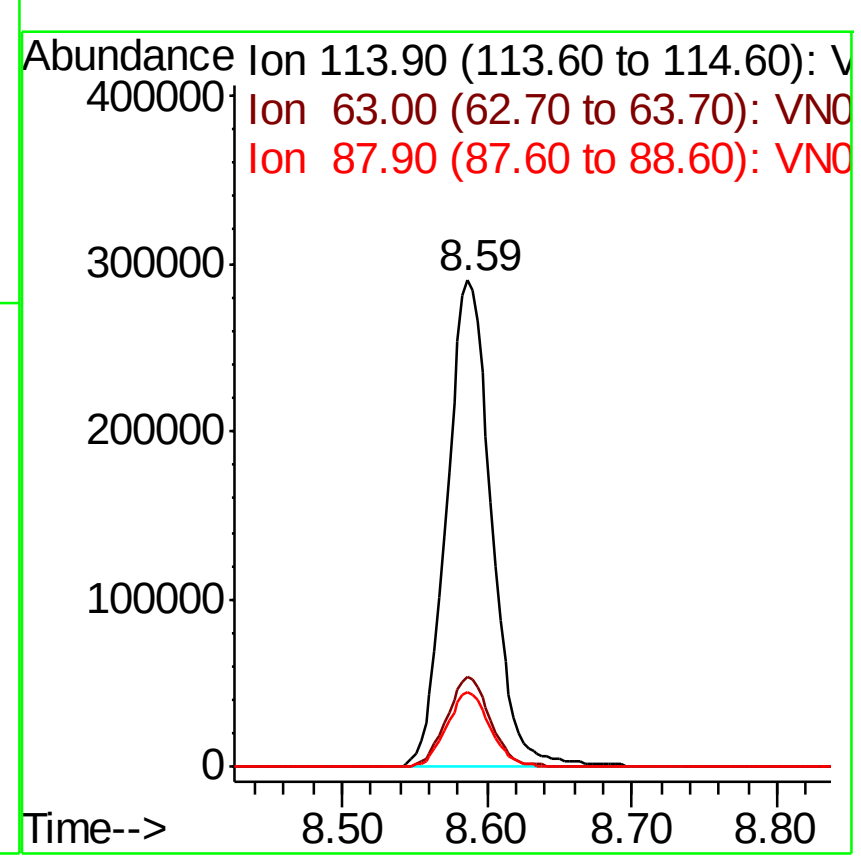

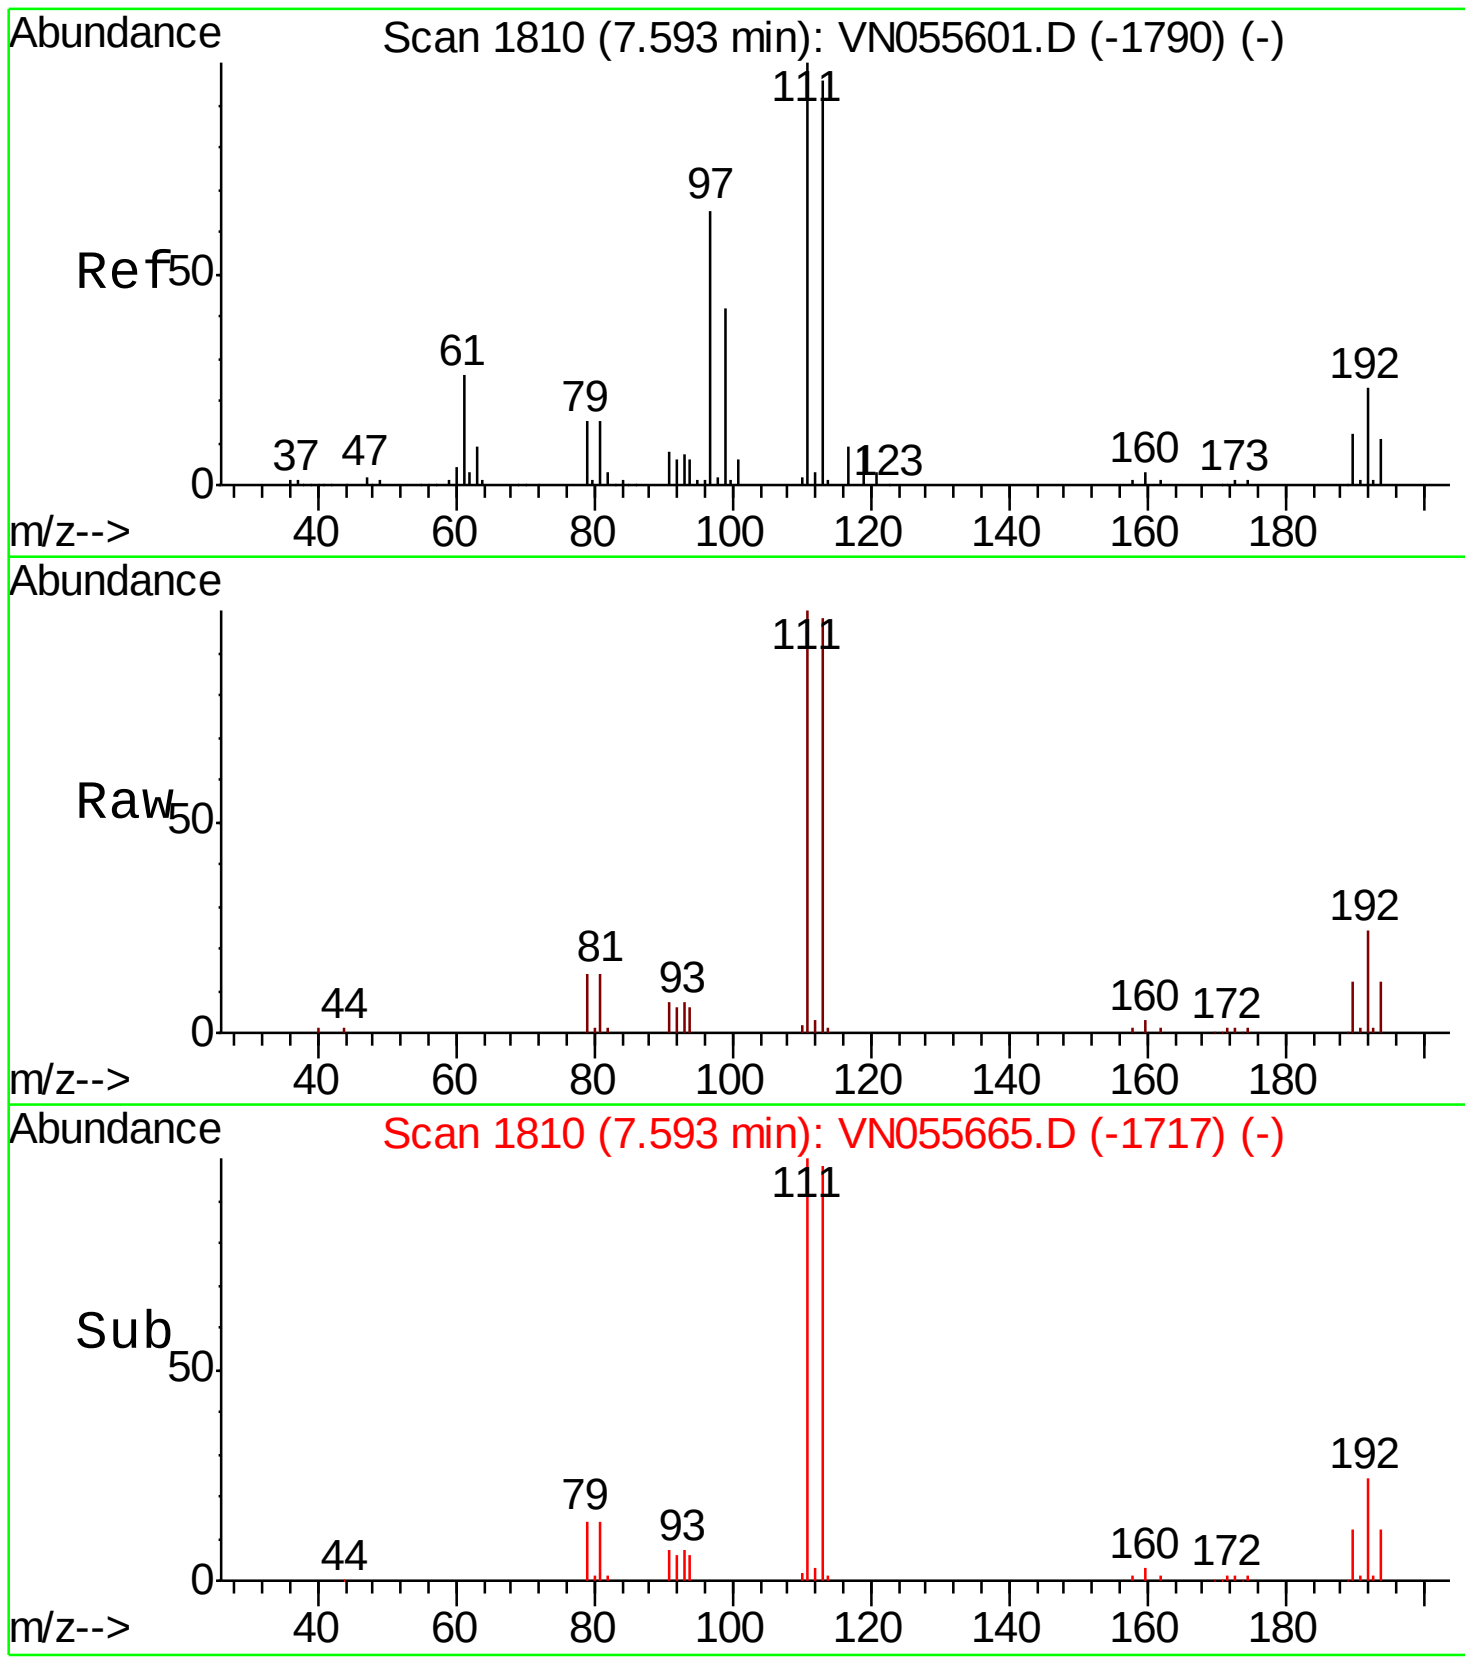

#35
Dibromofluoromethane
Concen: 47.707 ug/l
RT: 7.59 min Scan# 1810
Delta R.T. -0.00 min
Lab File: VN055665.D
Acq: 20 May 2019 11:37

Tgt Ion:113 Resp: 189364

Ion	Ratio	Lower	Upper
113	100		
111	102.5	82.5	123.7
192	24.0	18.7	28.1



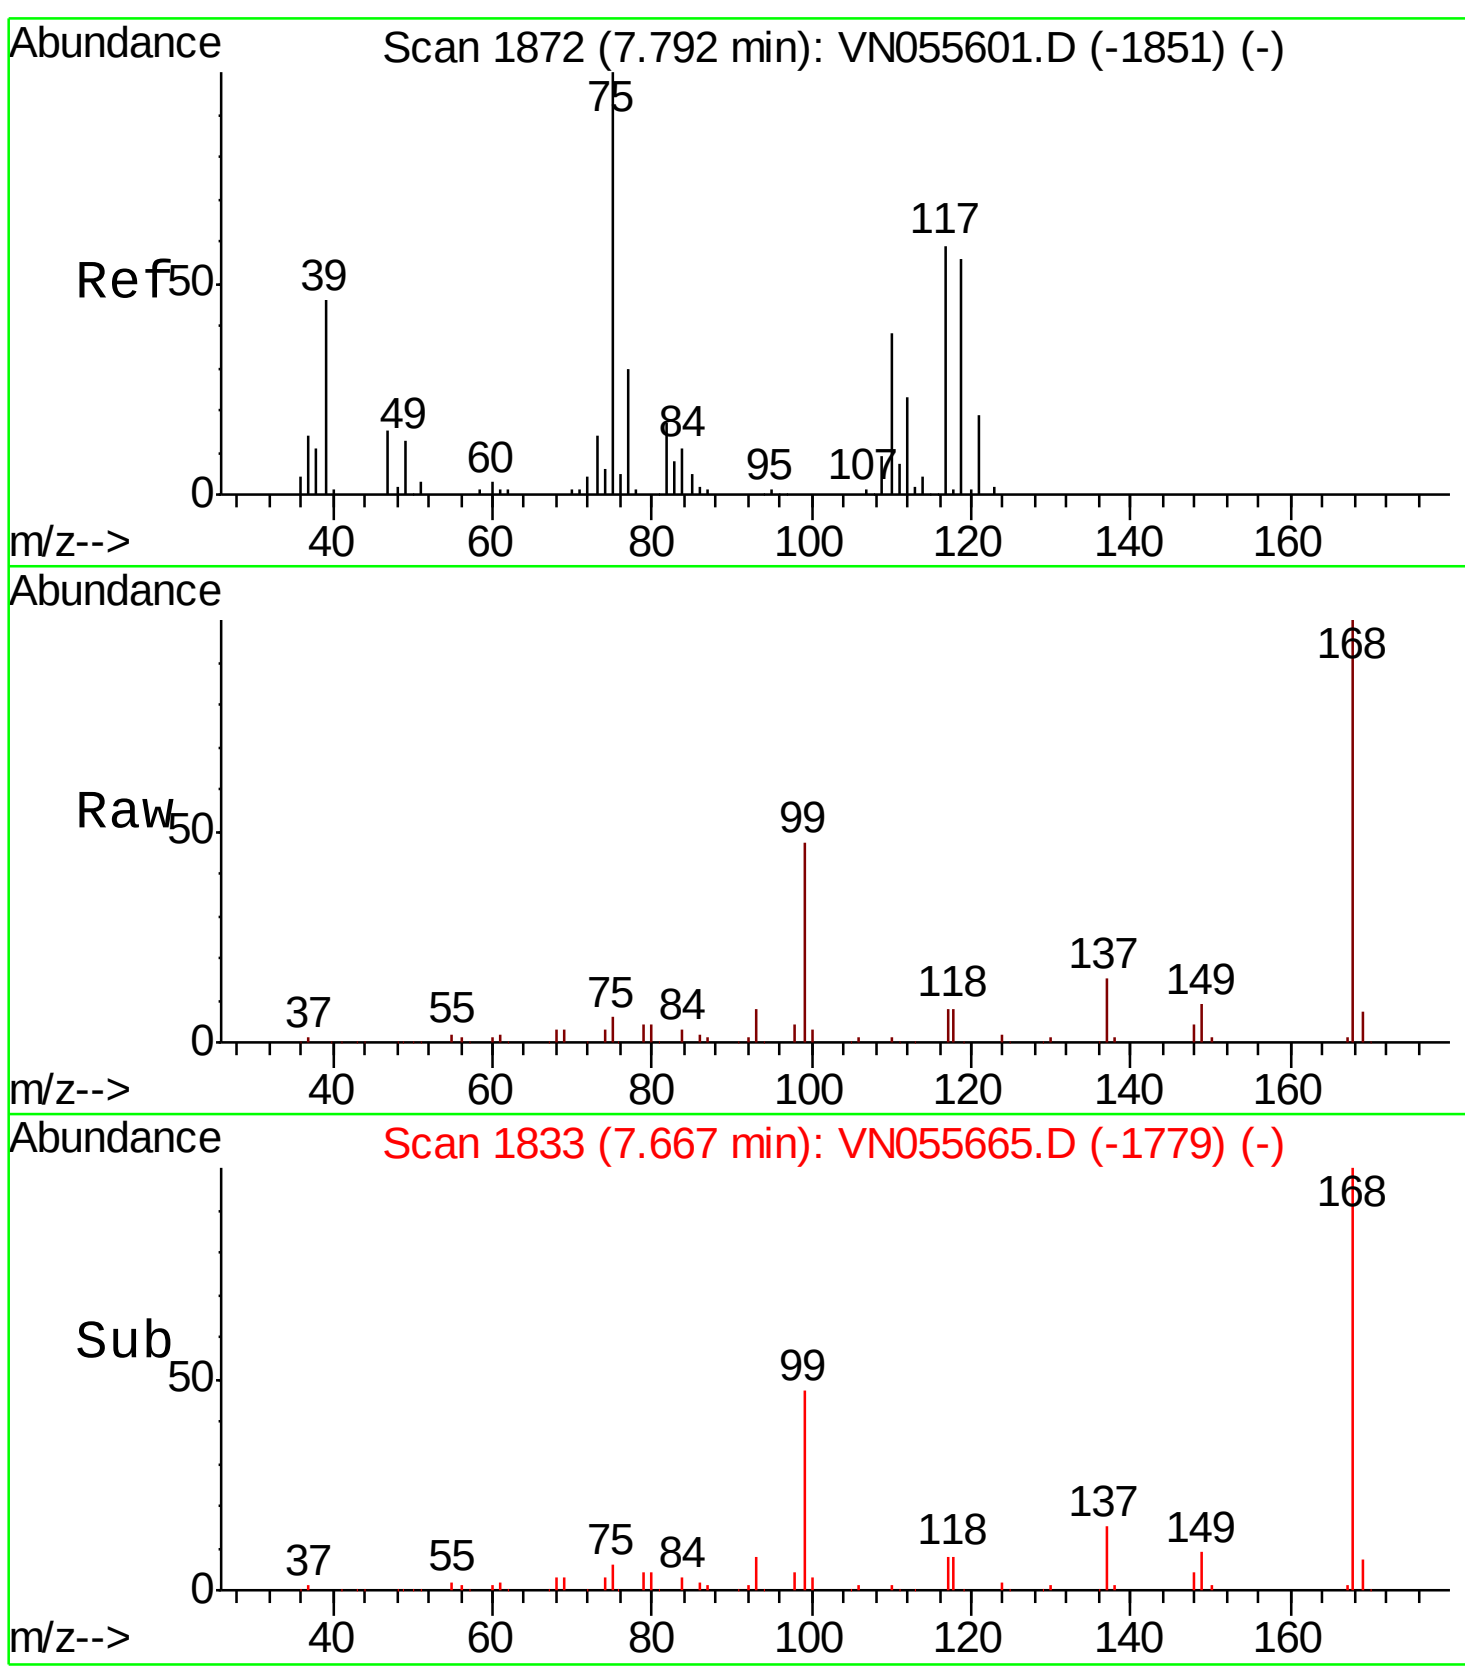

#36
1,1-Dichloropropene
Concen: 4.588 ug/l
RT: 7.67 min Scan# 1833
Delta R.T. -0.13 min
Lab File: VN055665.D
Acq: 20 May 2019 11:37

Tgt Ion: 75 Resp: 25558

Ion	Ratio	Lower	Upper
75	100		
110	9.4	18.6	55.6#
77	0.0	24.9	37.3#



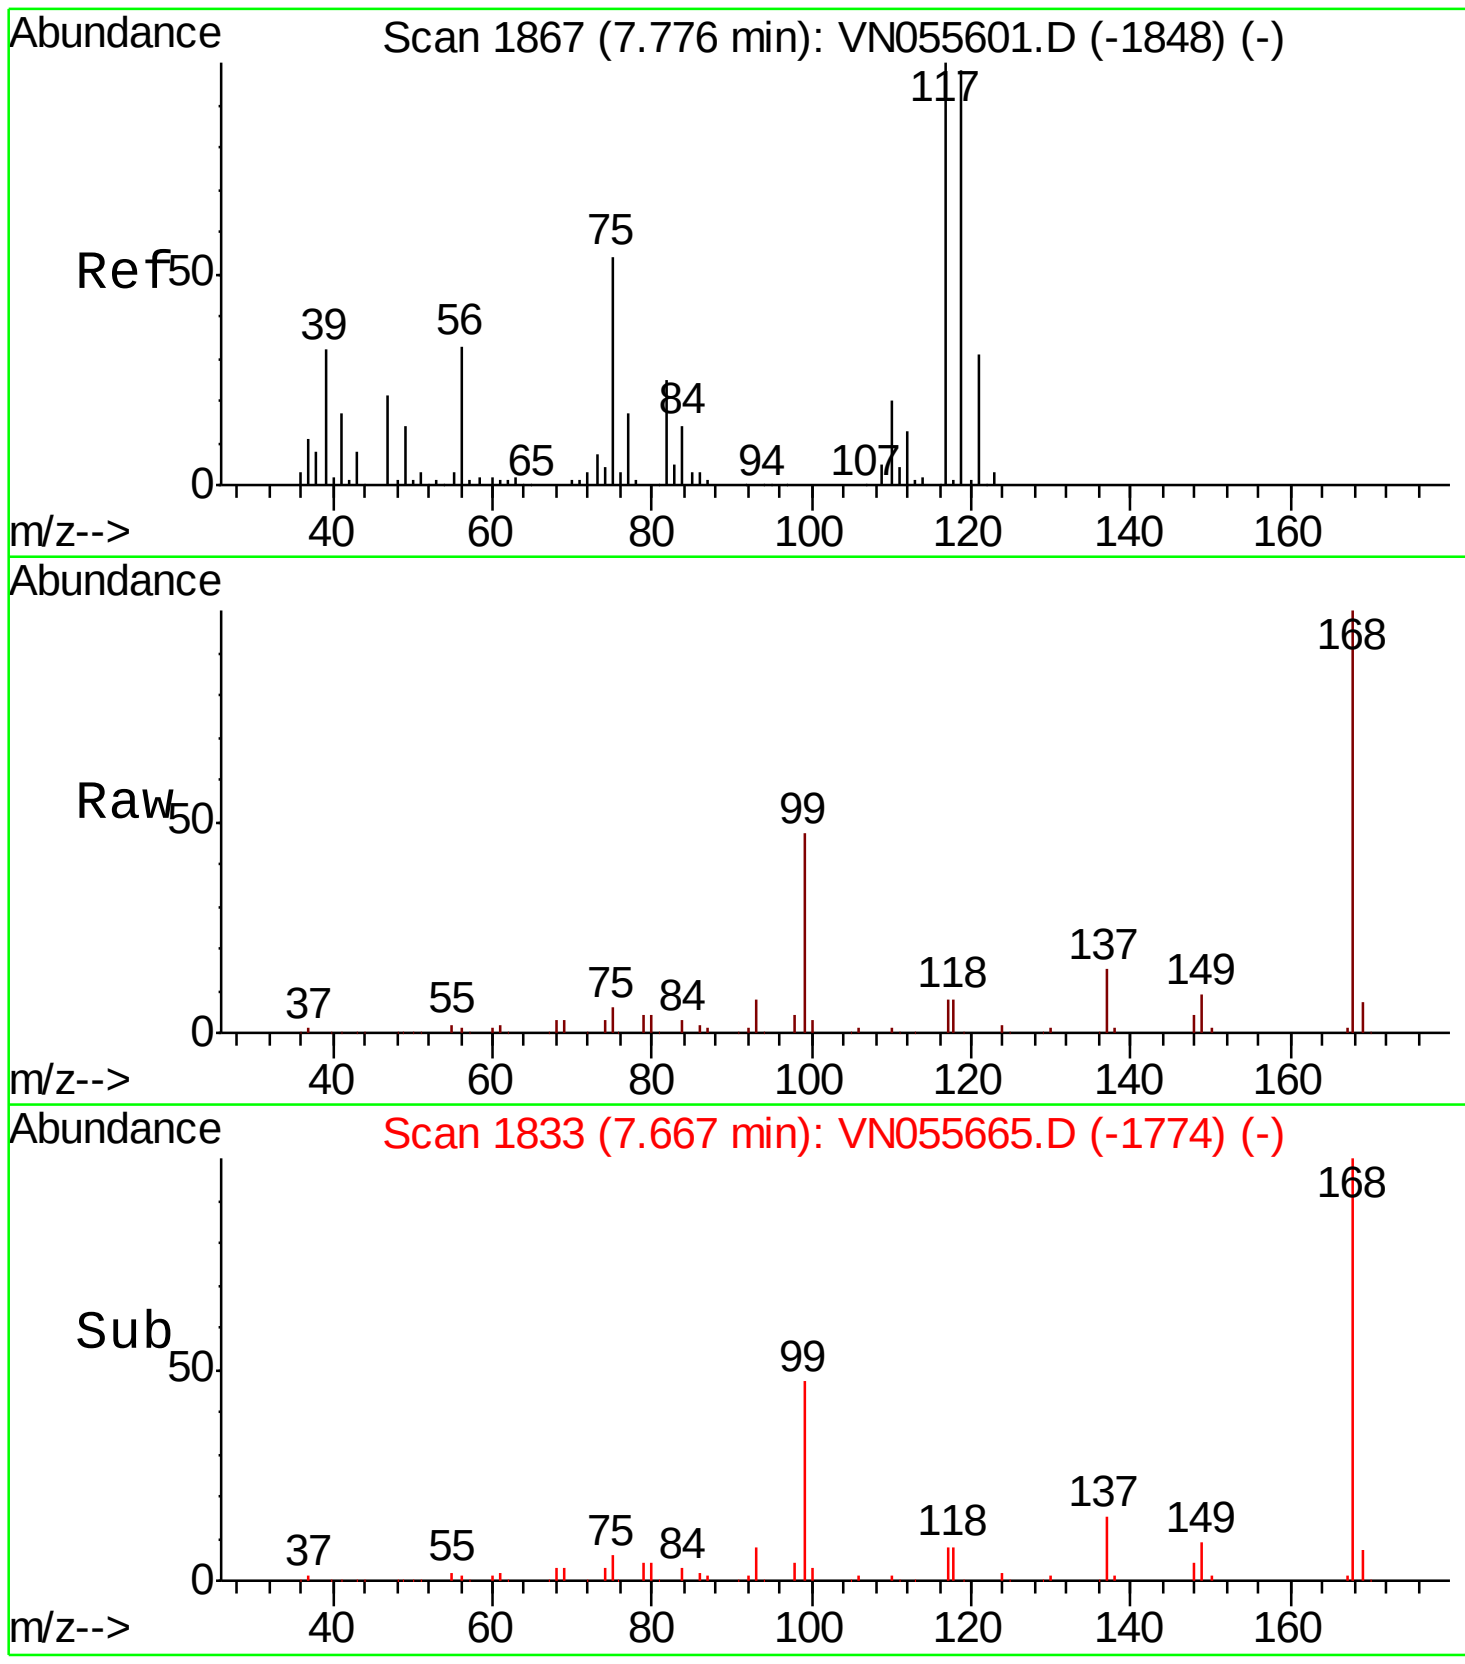

#38
Carbon Tetrachloride
Concen: 5.974 ug/l
RT: 7.67 min Scan# 1833
Delta R.T. -0.11 min
Lab File: VN055665.D
Acq: 20 May 2019 11:37

Tgt Ion:117 Resp: 35561

Ion	Ratio	Lower	Upper
117	100		
119	4.6	77.8	116.8#
121	0.0	24.6	37.0#



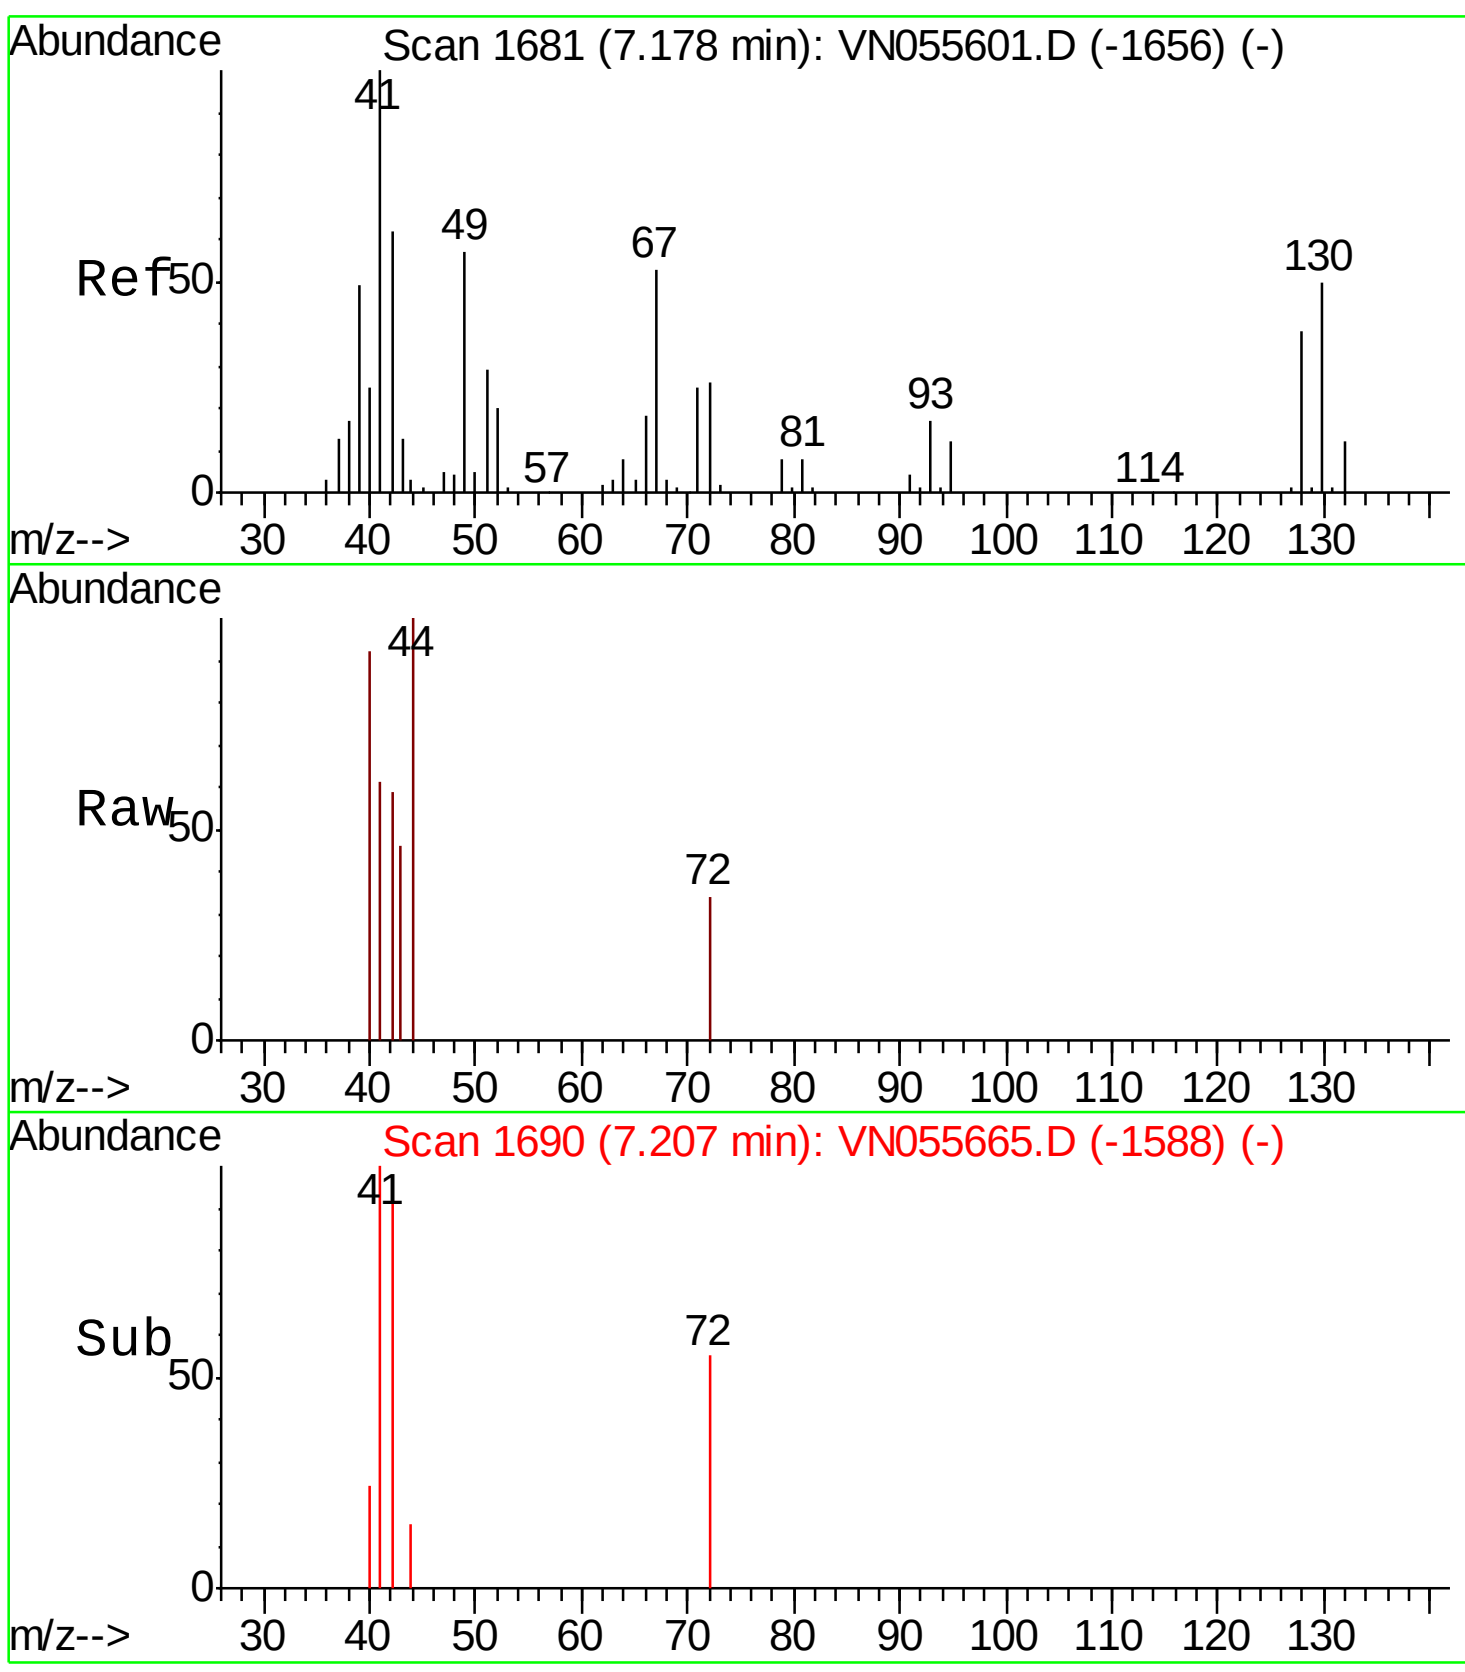

#41
Methacrylonitrile
Concen: 0.249 ug/l
RT: 7.21 min Scan# 1690
Delta R.T. 0.03 min
Lab File: VN055665.D
Acq: 20 May 2019 11:37

Tgt Ion: 41 Resp: 535

Ion	Ratio	Lower	Upper
41	100		
39	0.0	0.0	0.0
67	0.0	0.0	0.0
52	0.0	0.0	0.0



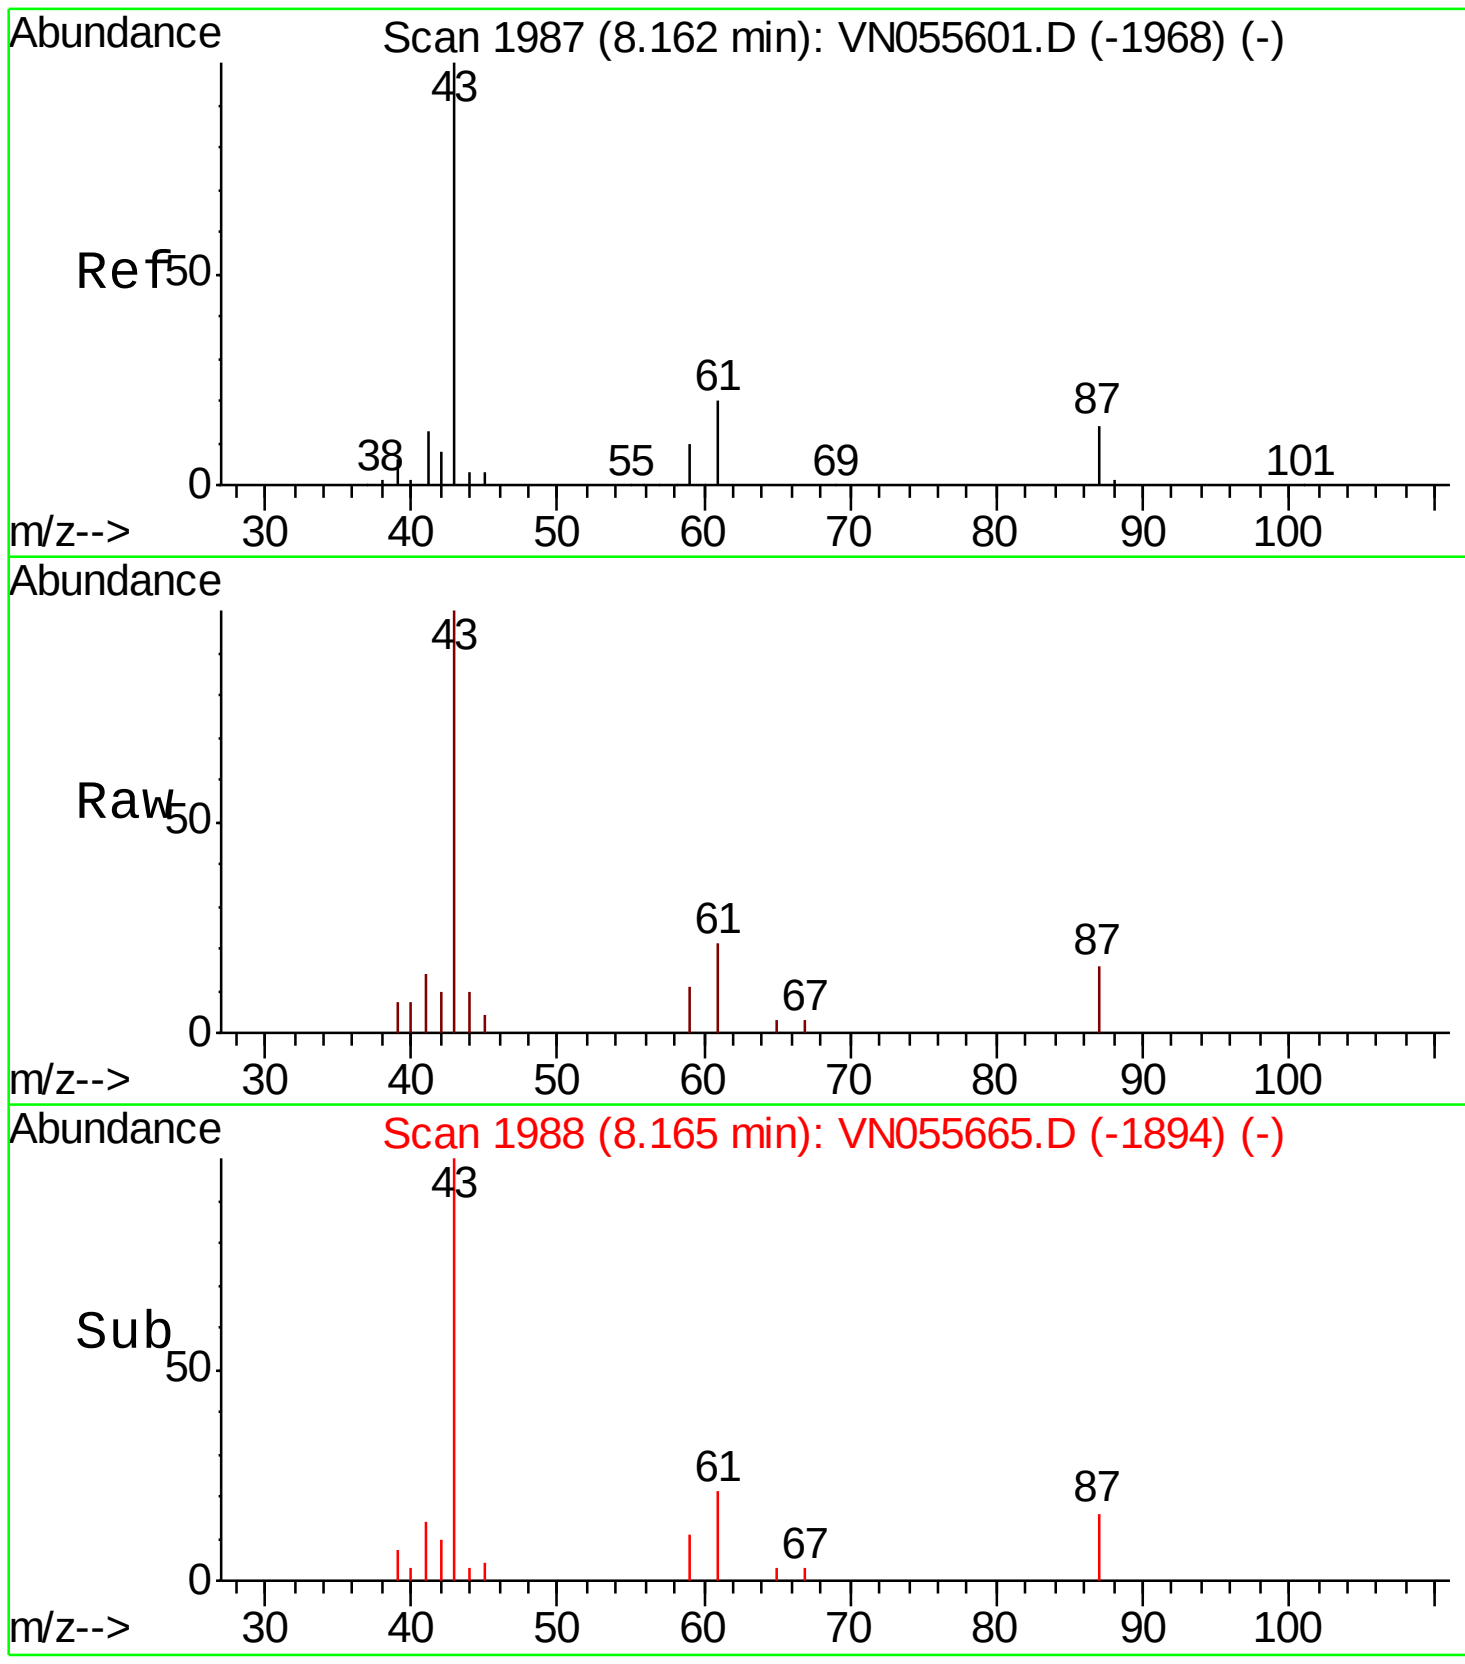

#43
Isopropyl Acetate
Concen: 1.758 ug/l
RT: 8.17 min Scan# 1988
Delta R.T. 0.00 min
Lab File: VN055665.D
Acq: 20 May 2019 11:37

Tgt Ion: 43 Resp: 15372

Ion	Ratio	Lower	Upper
43	100		
61	20.9	22.1	33.1#
87	14.9	11.8	17.6



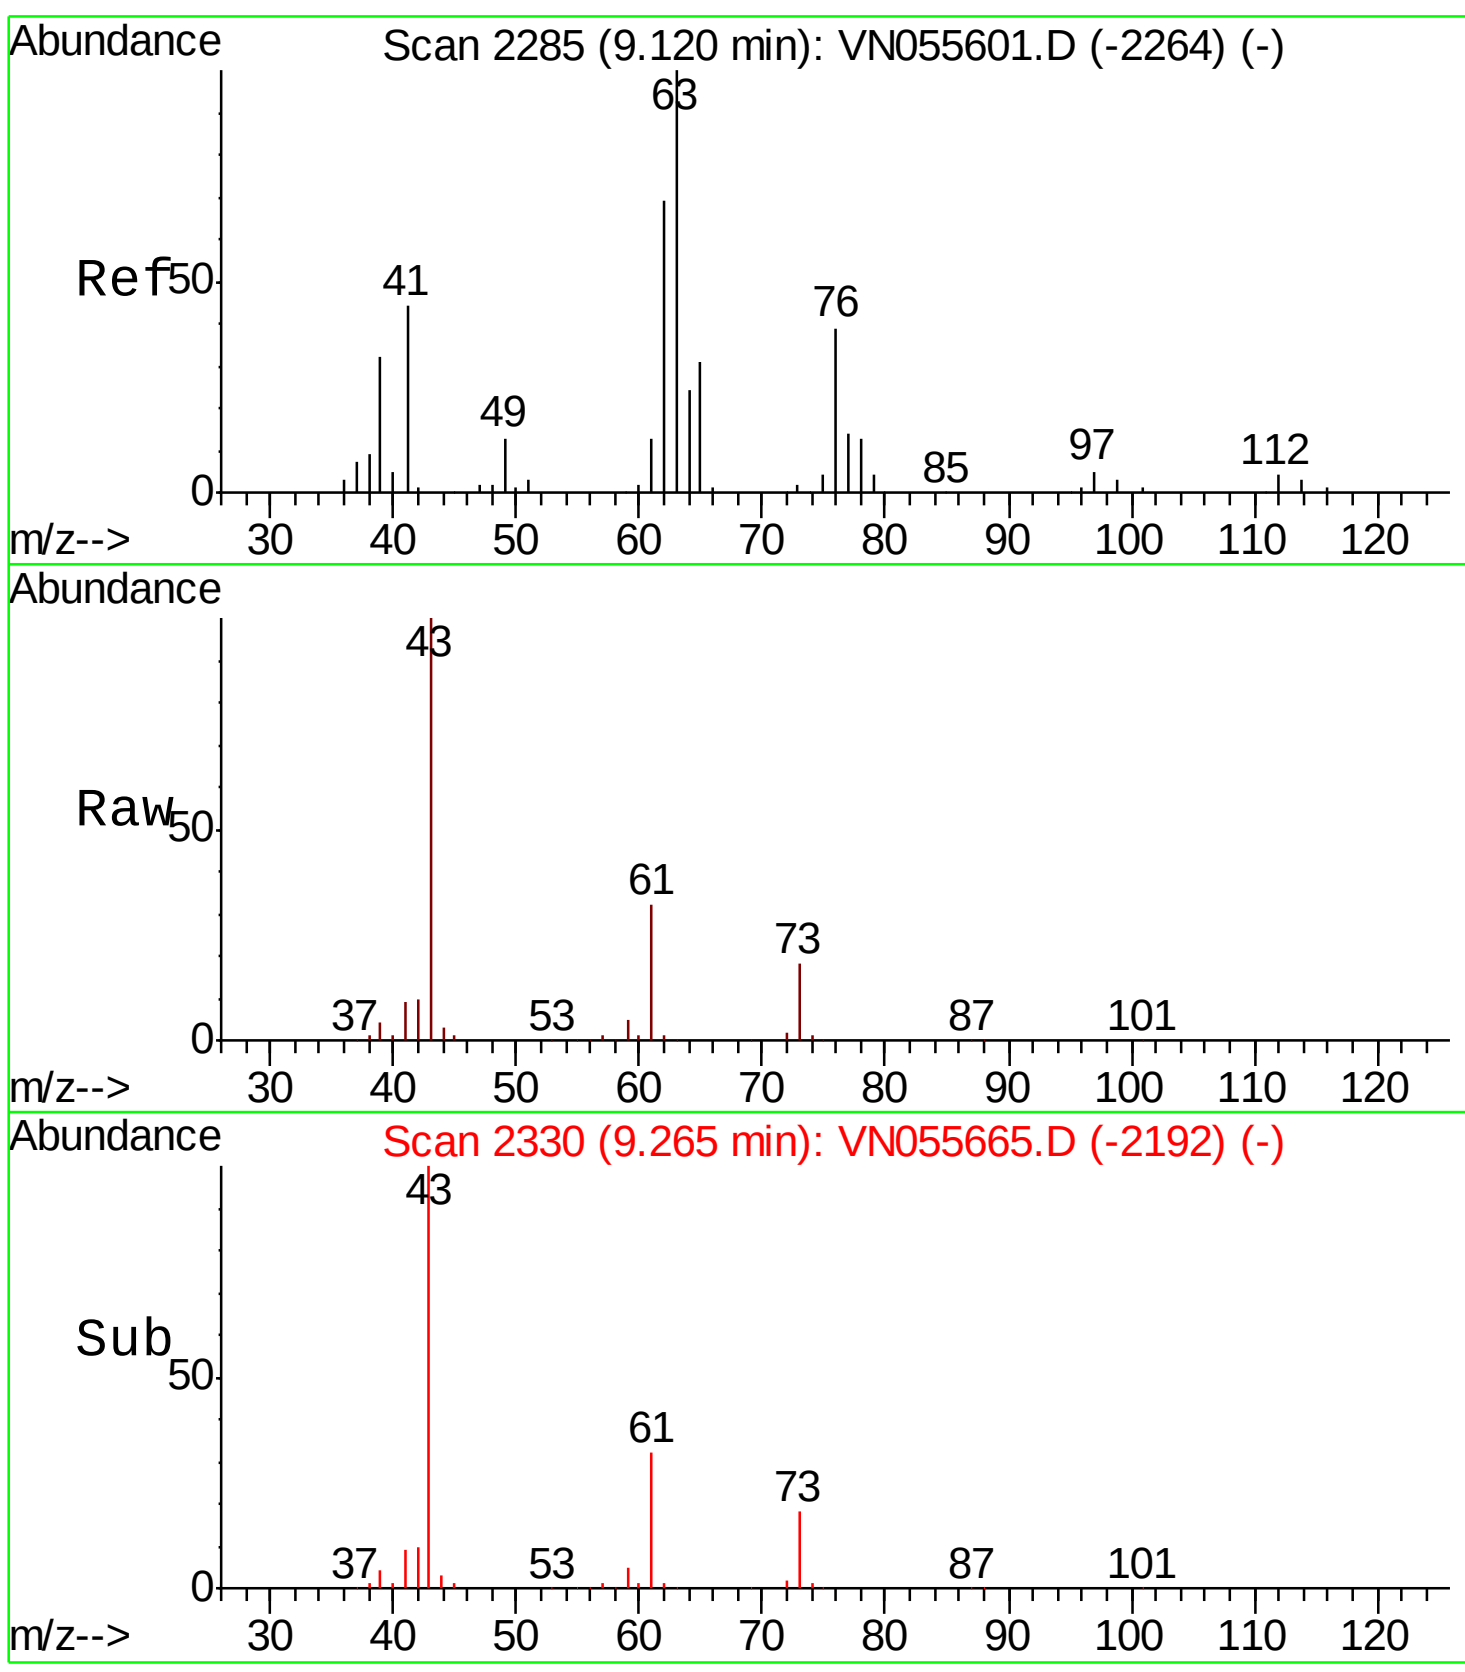

#45
1,2-Dichloropropane
Concen: 0.403 ug/l
RT: 9.26 min Scan# 2330
Delta R.T. 0.14 min
Lab File: VN055665.D
Acq: 20 May 2019 11:37

Tgt Ion: 63 Resp: 1739

Ion	Ratio	Lower	Upper
63	100		
65	0.0	25.2	37.8#



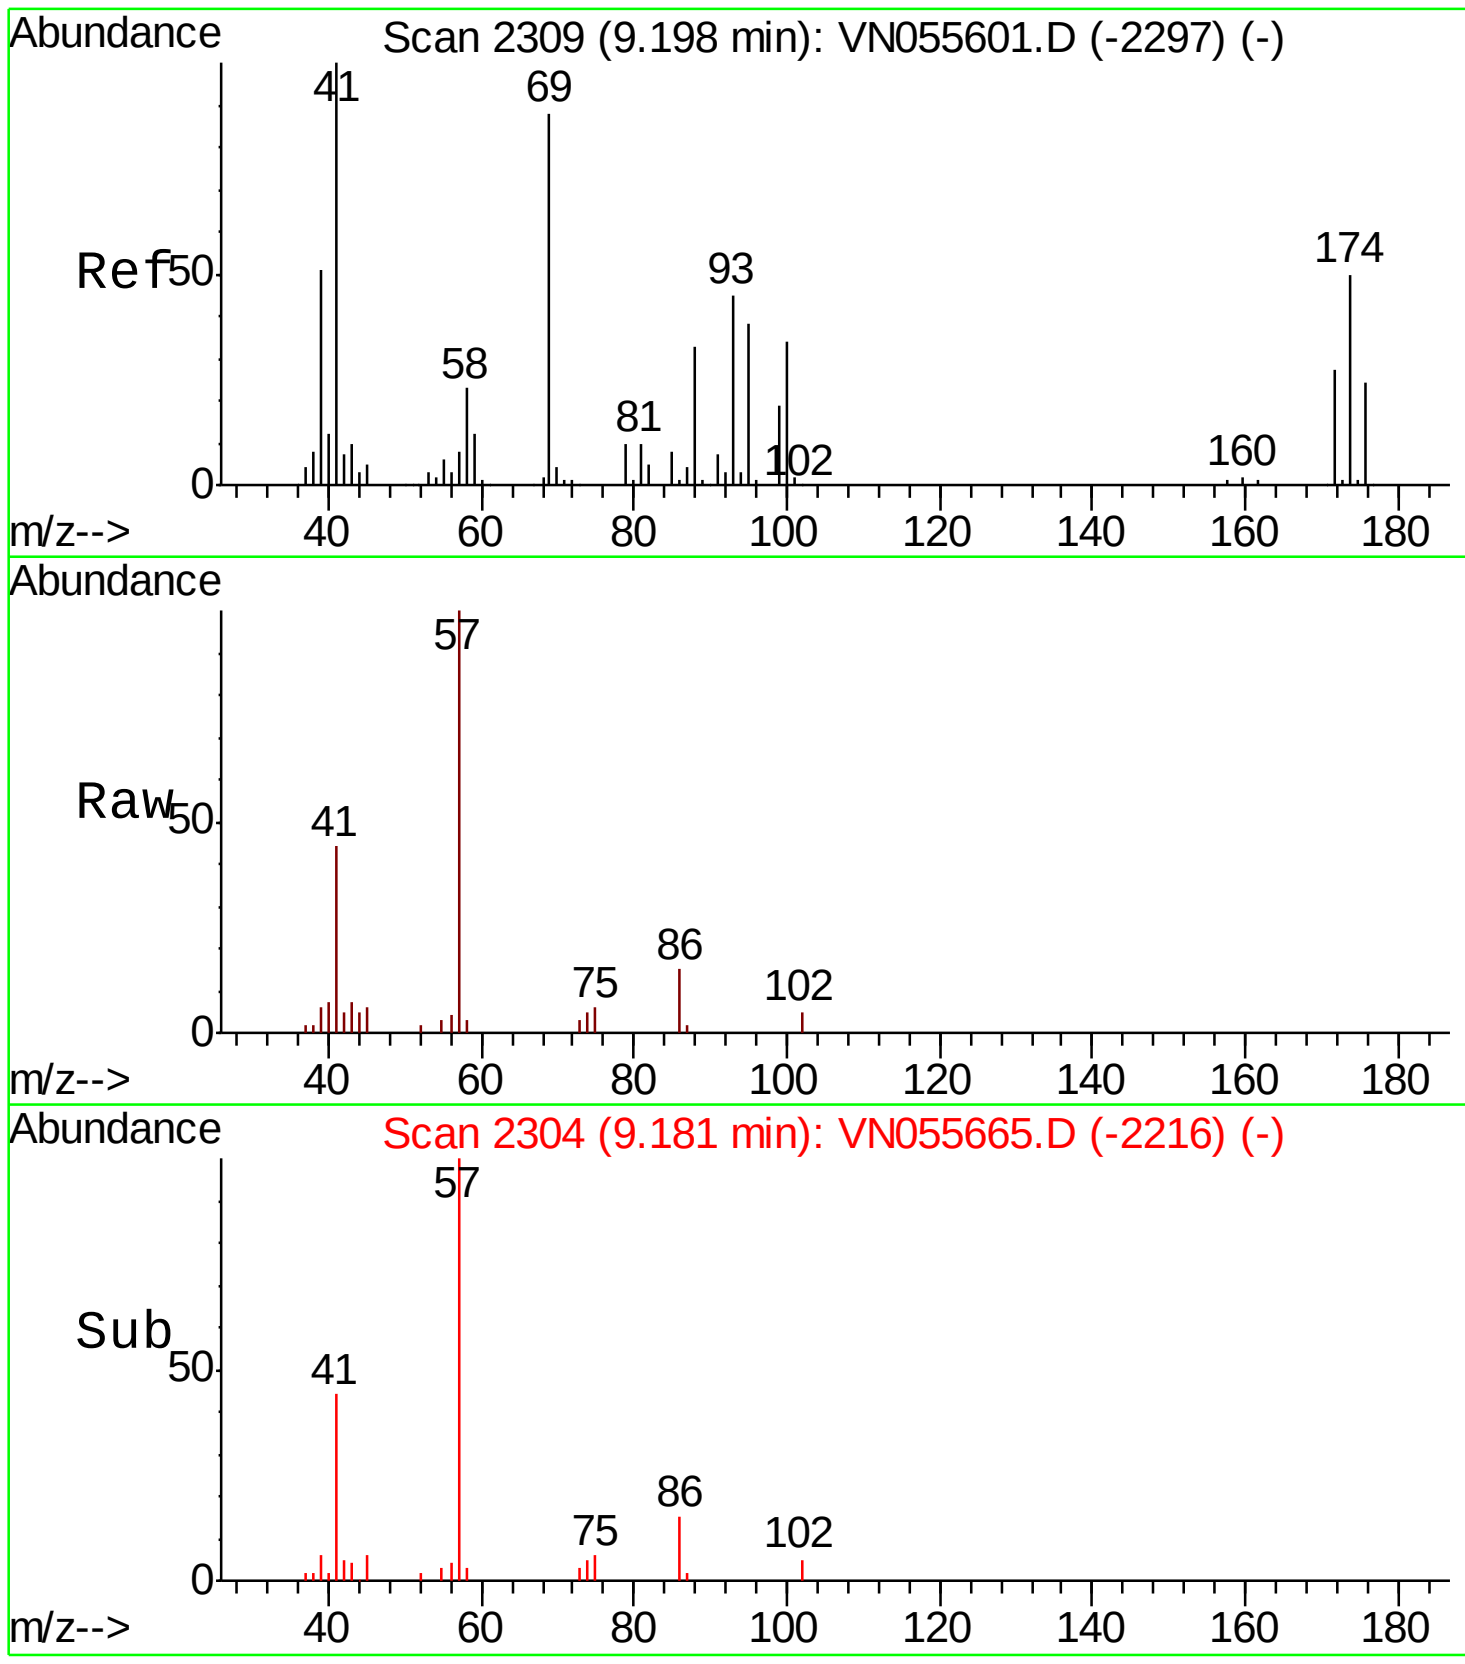

#48
Methyl methacrylate
Concen: 2.212 ug/l
RT: 9.18 min Scan# 2304
Delta R.T. -0.02 min
Lab File: VN055665.D
Acq: 20 May 2019 11:37

Tgt Ion: 41 Resp: 8645

Ion	Ratio	Lower	Upper
41	100		
69	0.0	74.2	111.2#
39	0.0	43.8	65.8#



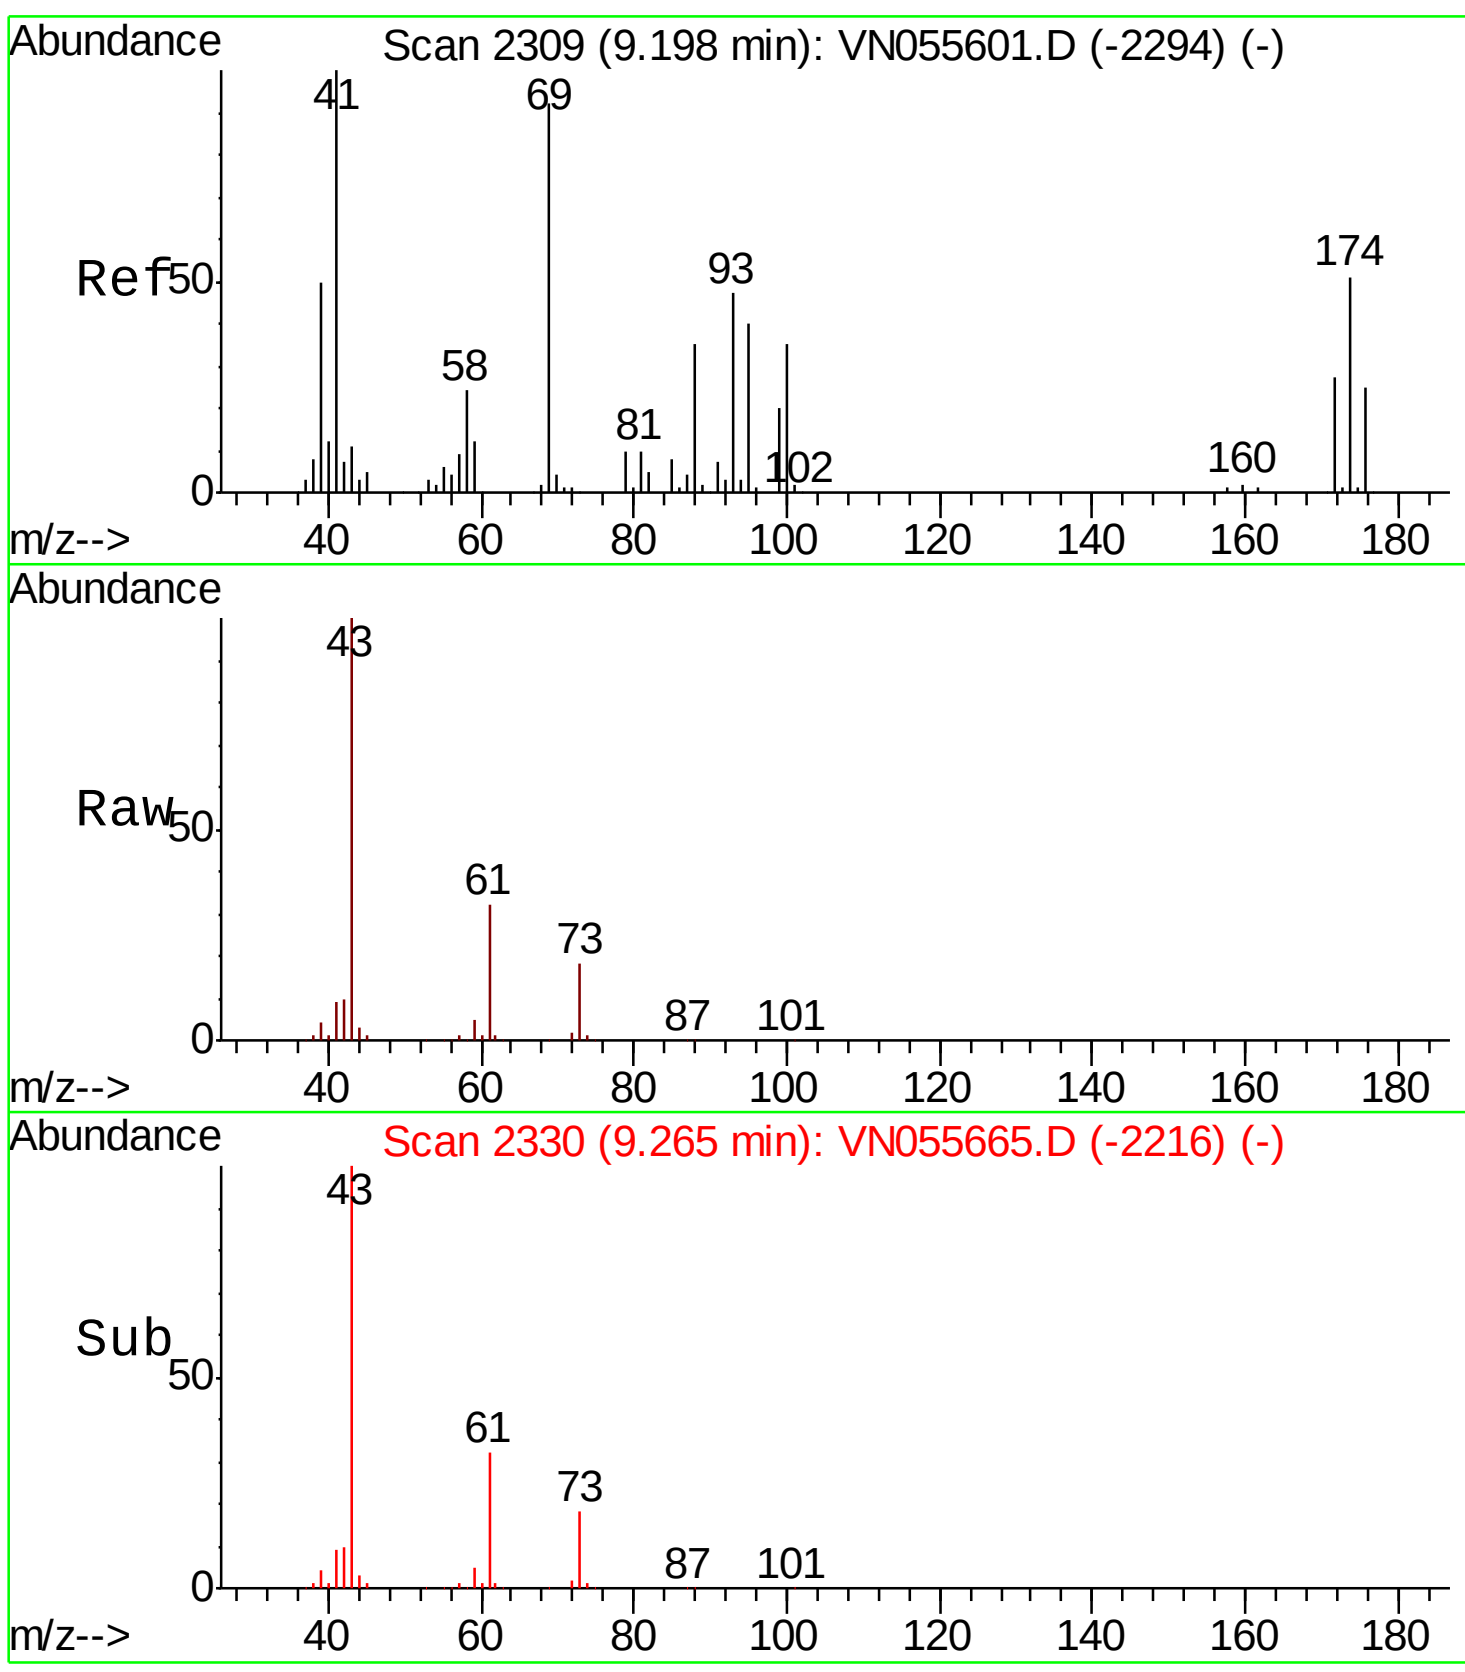

#49
1,4-Dioxane
Concen: 1.172 ug/l
RT: 9.26 min Scan# 2330
Delta R.T. 0.07 min
Lab File: VN055665.D
Acq: 20 May 2019 11:37

Tgt Ion: 88 Resp: 91

Ion	Ratio	Lower	Upper
88	100		
43	1464712.1	22.4	33.6#
58	5637.4	53.4	80.2#



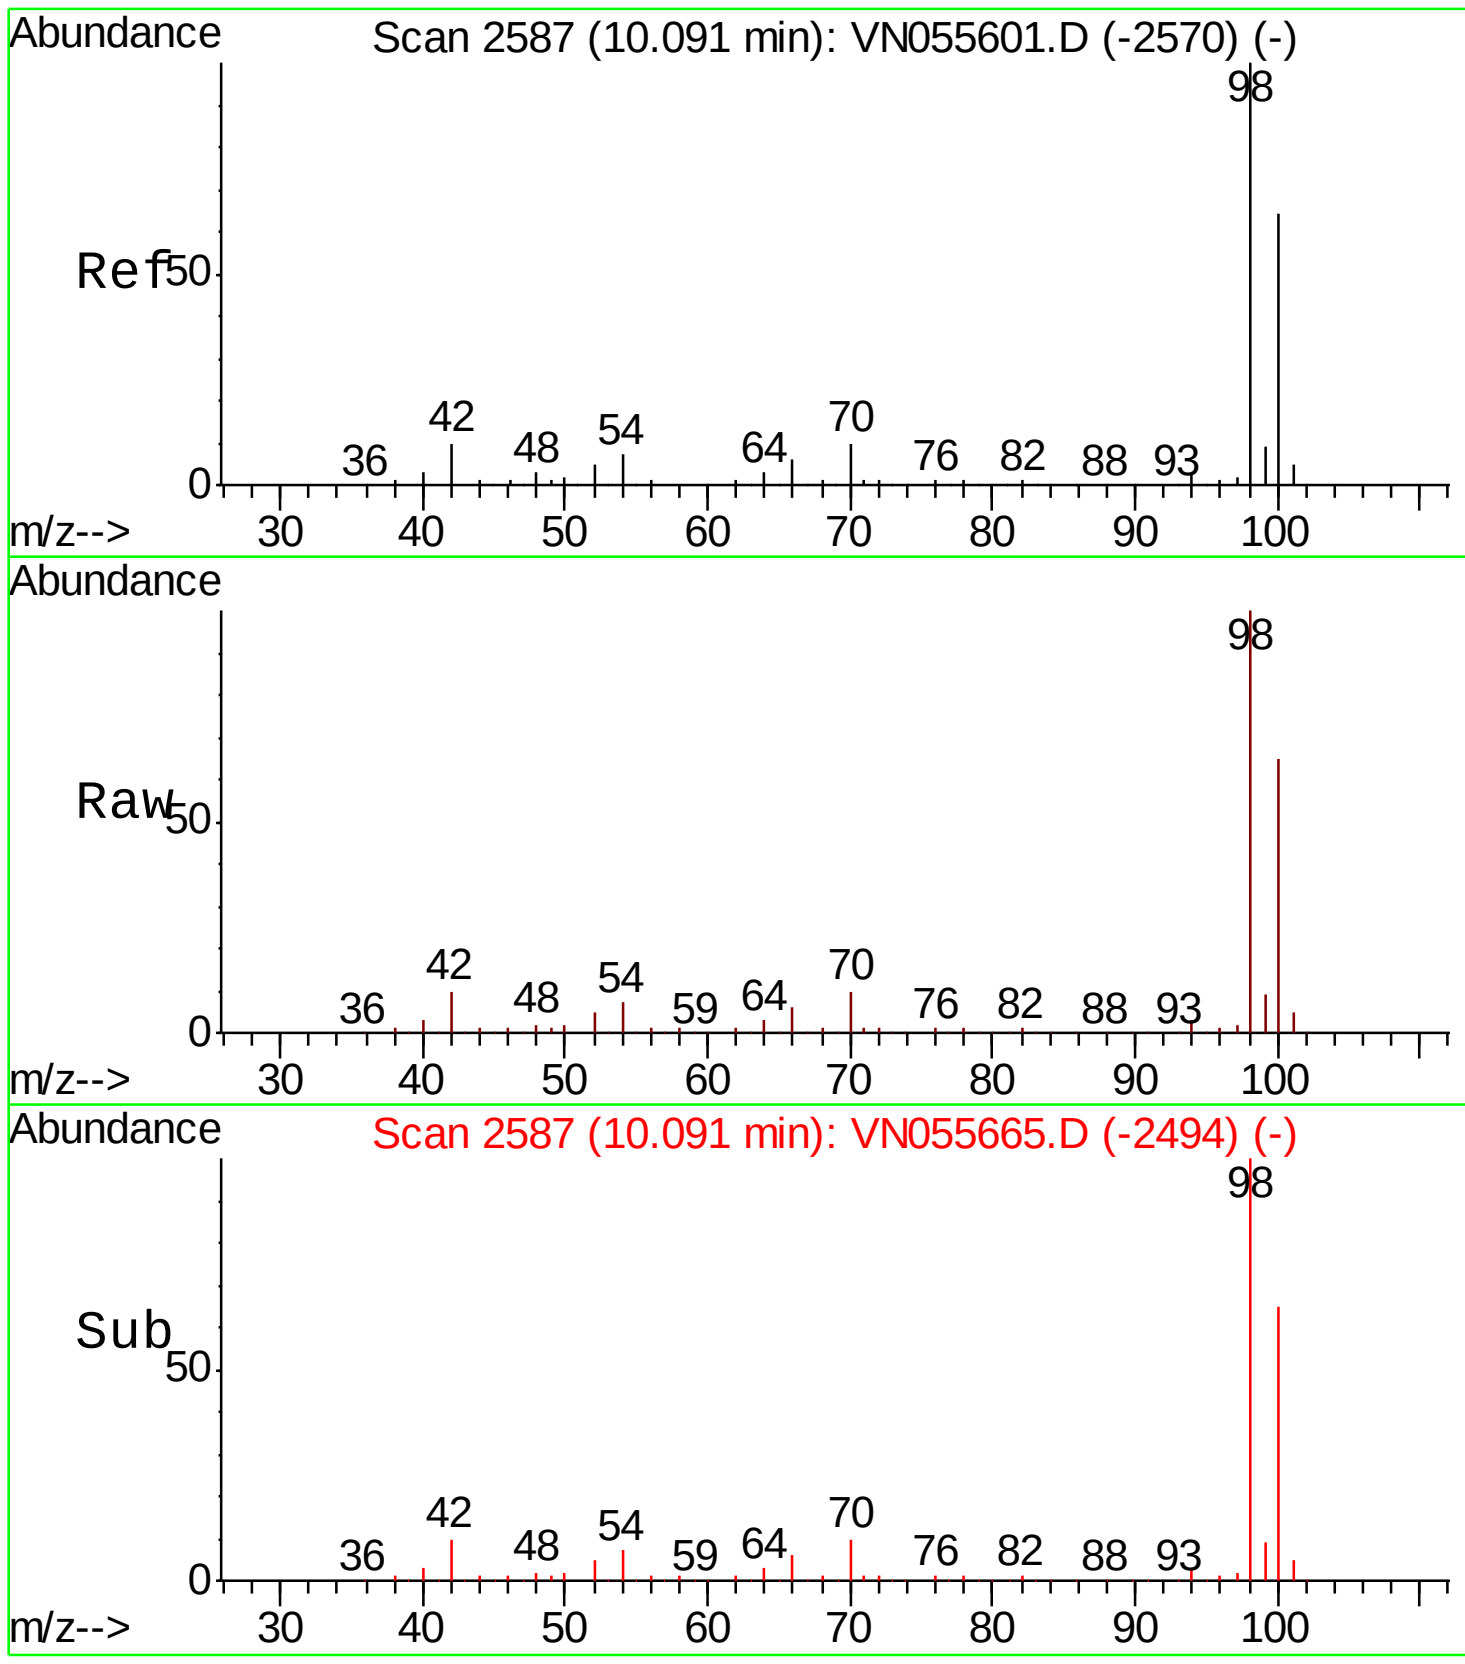

#50
Toluene-d8
Concen: 48.283 ug/l
RT: 10.09 min Scan# 2587
Delta R.T. -0.00 min
Lab File: VN055665.D
Acq: 20 May 2019 11:37

Tgt Ion: 98	Resp:	724668	
Ion	Ratio	Lower	Upper
98	100		
100	64.7	51.9	77.9



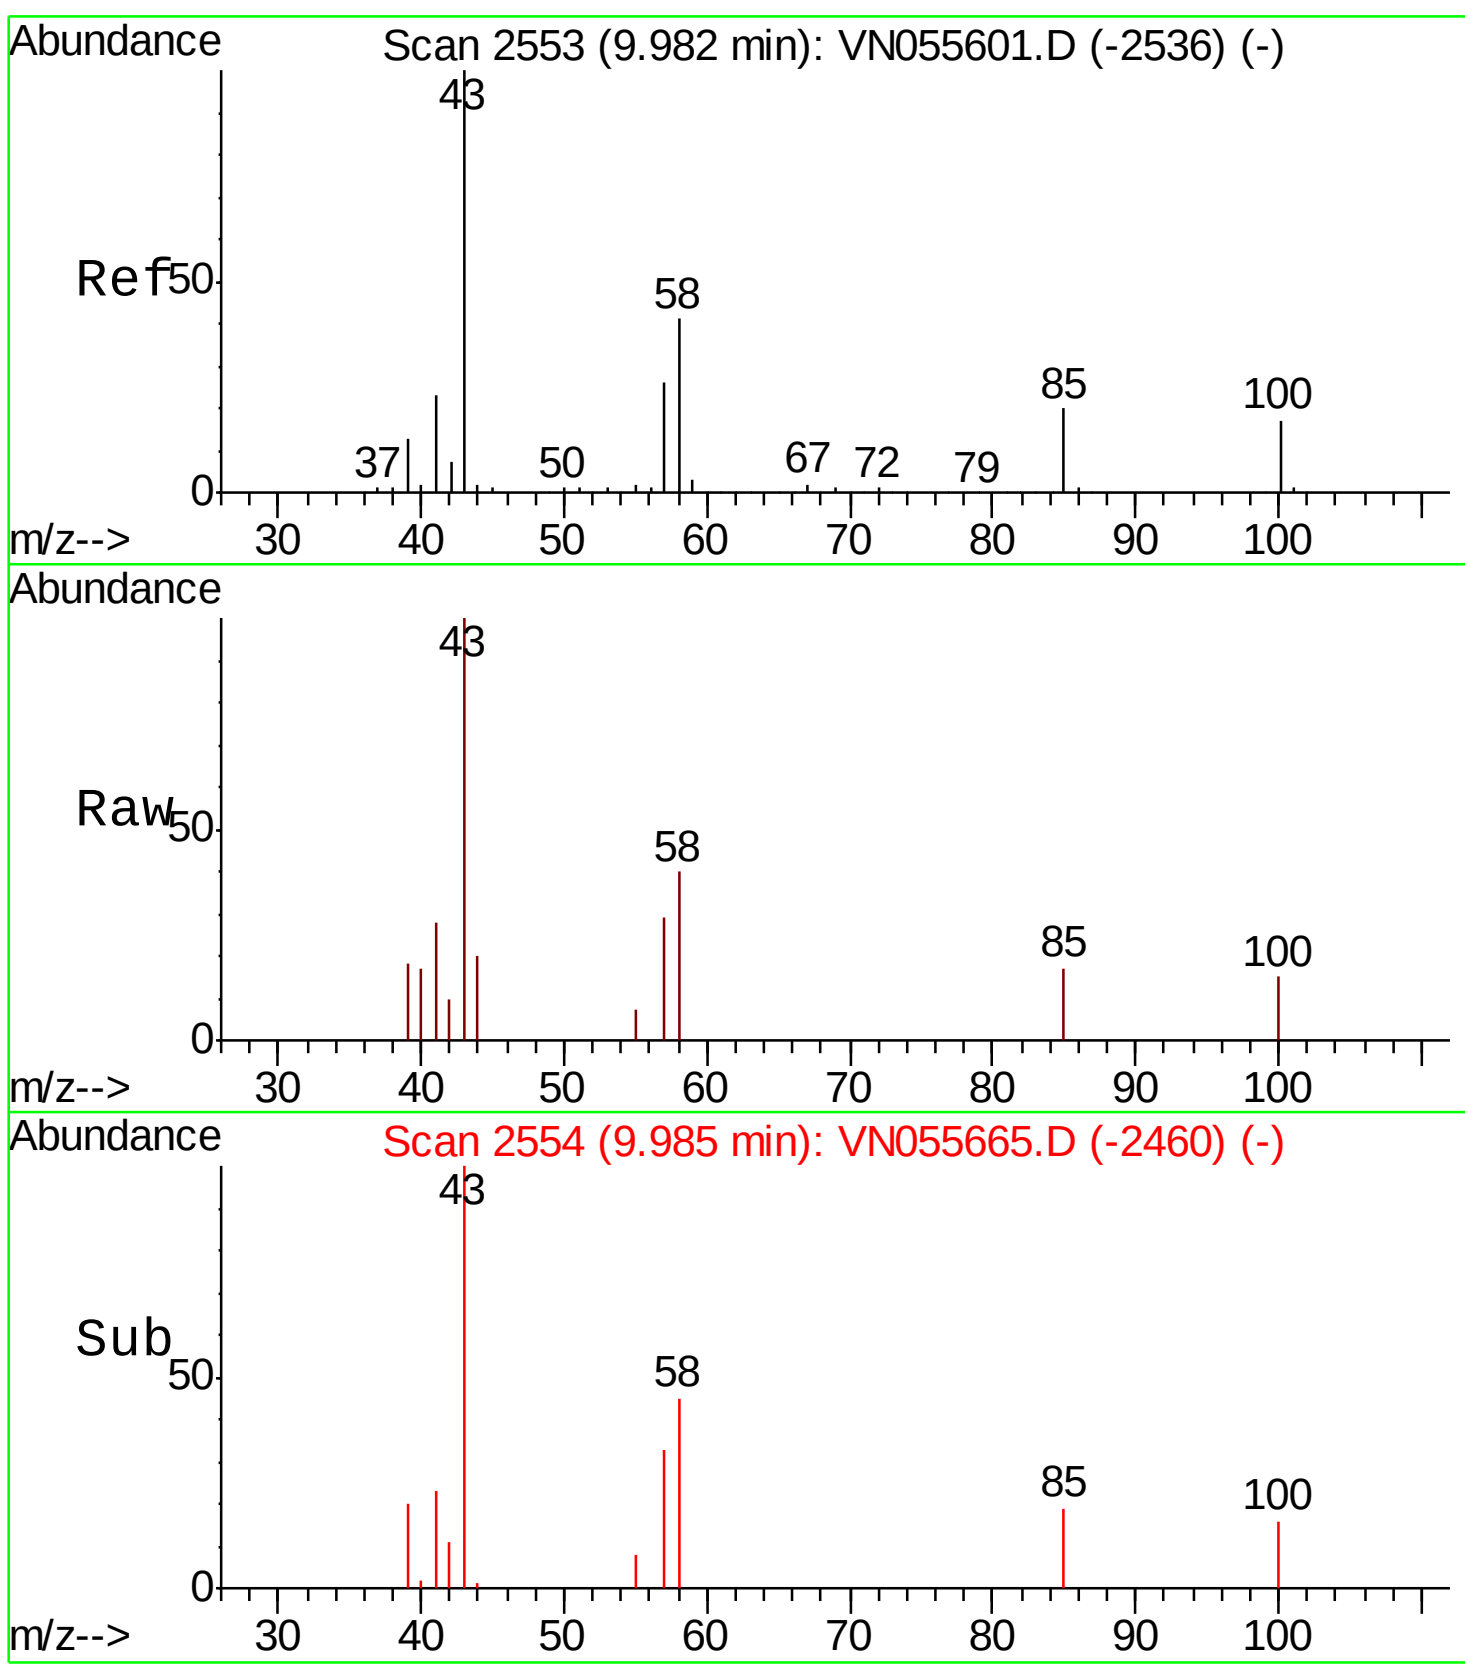

#51
4-Methyl-2-Pentanone
Concen: 0.846 ug/l
RT: 9.99 min Scan# 2554
Delta R.T. 0.00 min
Lab File: VN055665.D
Acq: 20 May 2019 11:37

Tgt Ion: 43	Resp:	4337	
Ion	Ratio	Lower	Upper
43	100		
58	46.6	32.7	49.1



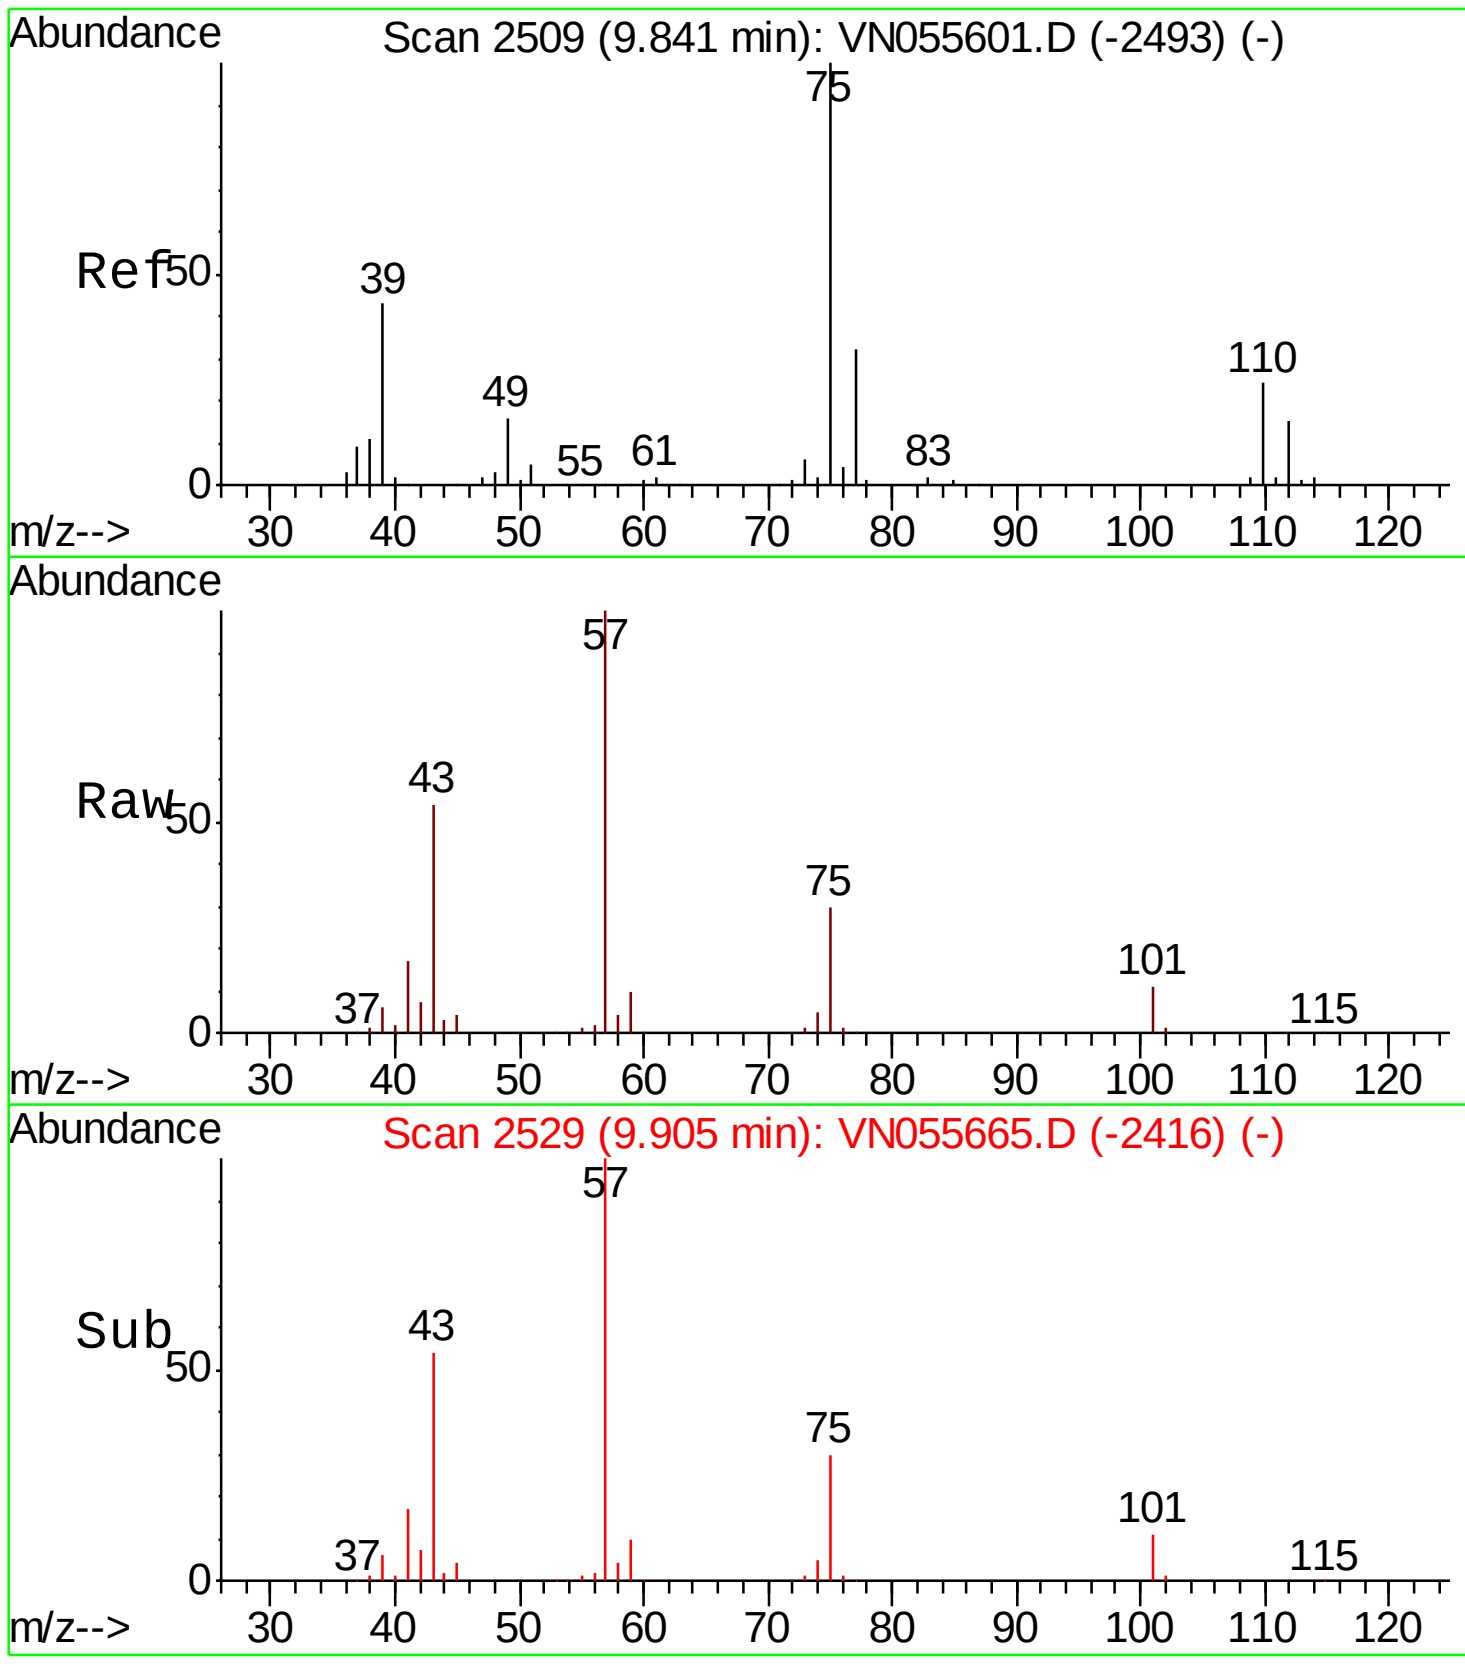

#54
cis-1,3-Dichloropropene
Concen: 9.271 ug/l
RT: 9.90 min Scan# 2529
Delta R.T. 0.06 min
Lab File: VN055665.D
Acq: 20 May 2019 11:37

Tgt Ion: 75 Resp: 64725

Ion	Ratio	Lower	Upper
75	100		
77	0.5	25.7	38.5#
39	21.2	34.7	52.1#



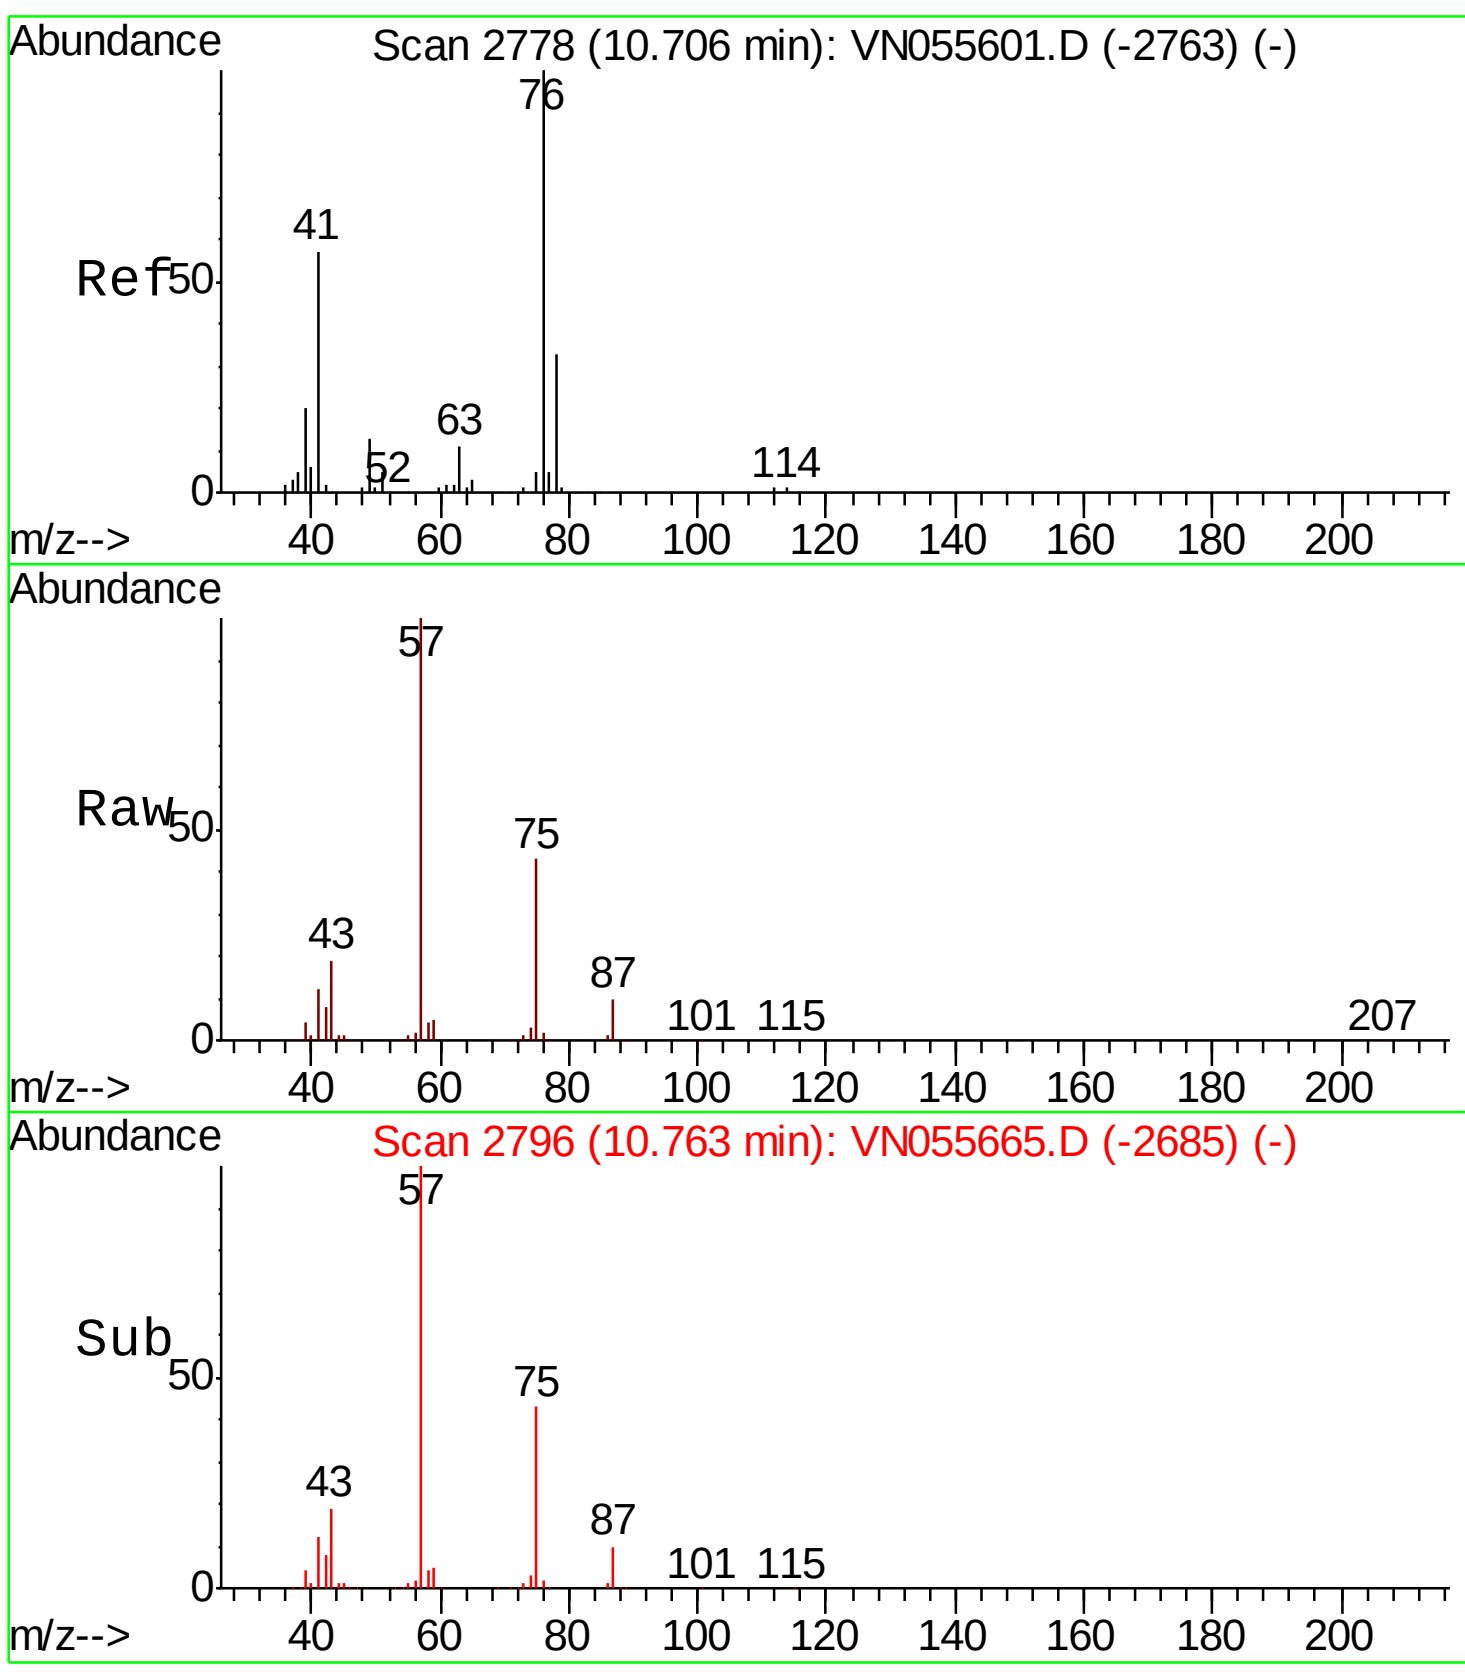

#57
1,3-Dichloropropane
Concen: 1.900 ug/l
RT: 10.76 min Scan# 2796
Delta R.T. 0.06 min
Lab File: VN055665.D
Acq: 20 May 2019 11:37

Tgt Ion: 76 Resp: 12735

Ion	Ratio	Lower	Upper
76	100		
78	0.0	26.5	39.7#



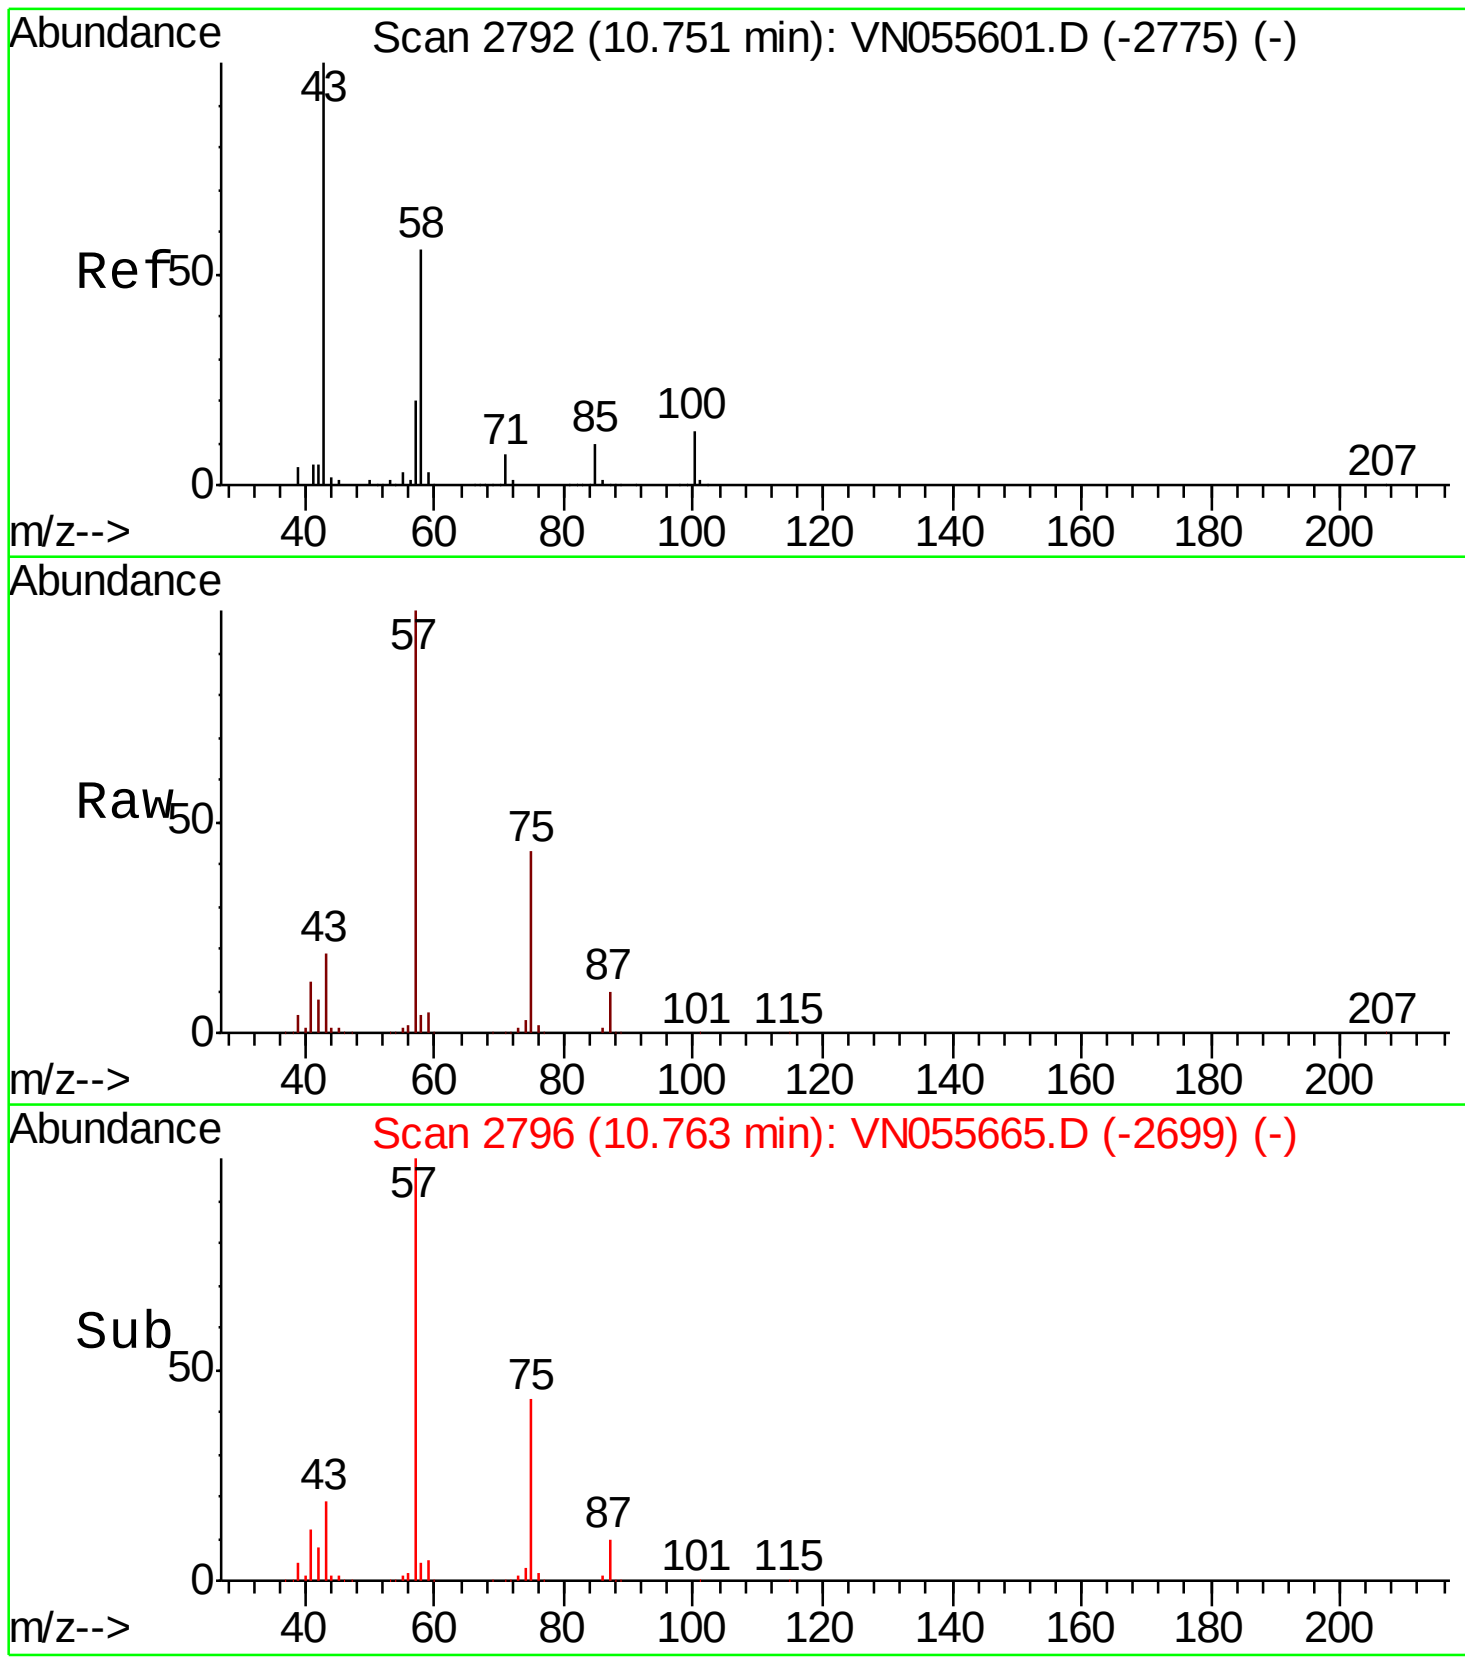

#59
2-Hexanone
Concen: 45.033 ug/l
RT: 10.76 min Scan# 2796
Delta R.T. 0.01 min
Lab File: VN055665.D
Acq: 20 May 2019 11:37

Tgt Ion: 43 Resp: 162632

Ion	Ratio	Lower	Upper
43	100		
58	20.1	28.1	84.4#



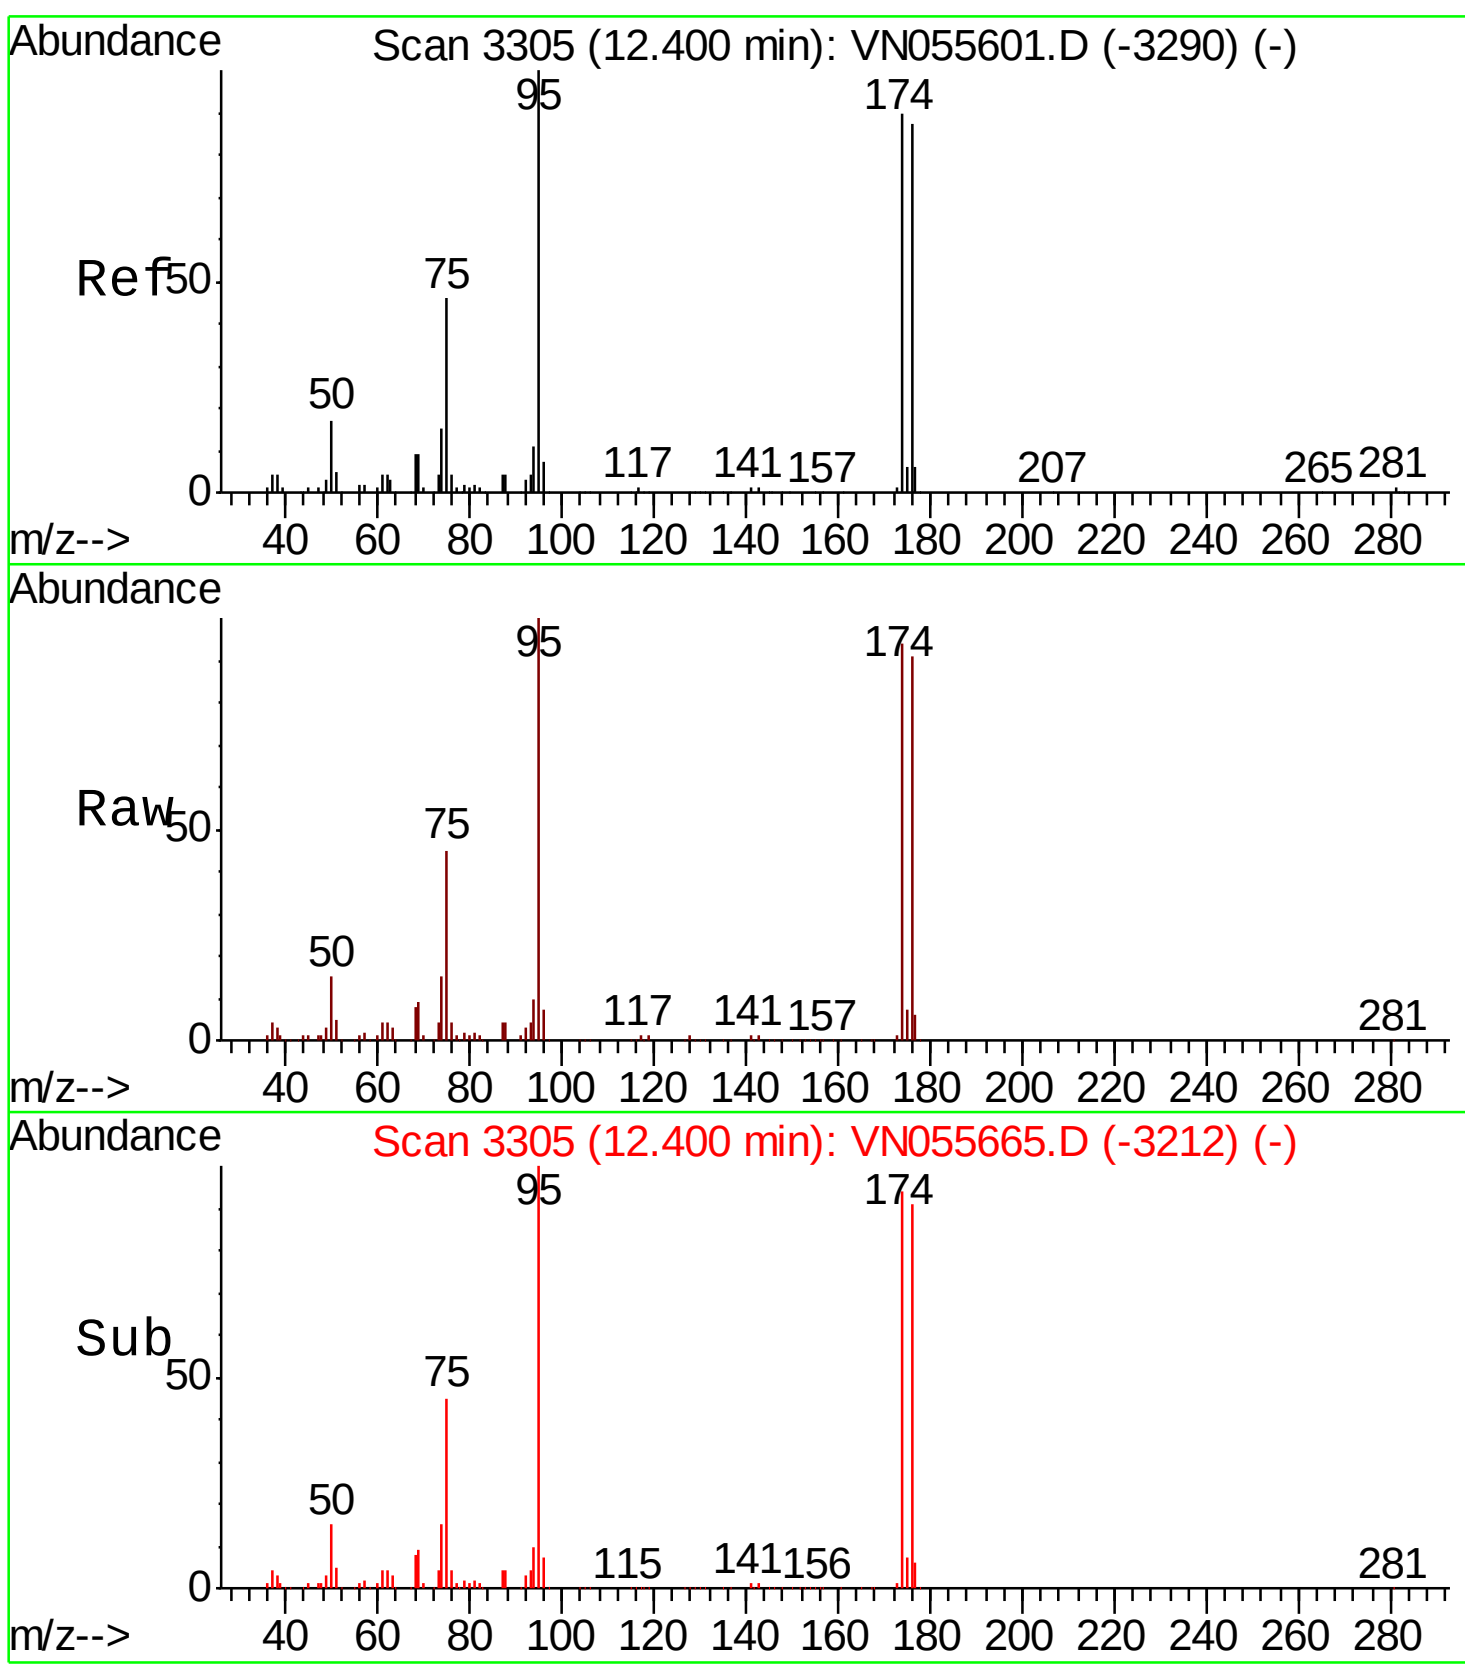

#62
4-Bromofluorobenzene
Concen: 46.024 ug/l
RT: 12.40 min Scan# 3305
Delta R.T. -0.00 min
Lab File: VN055665.D
Acq: 20 May 2019 11:37

Tgt Ion: 95 Resp: 238529

Ion	Ratio	Lower	Upper
95	100		
174	94.9	0.0	180.6
176	92.1	0.0	177.4



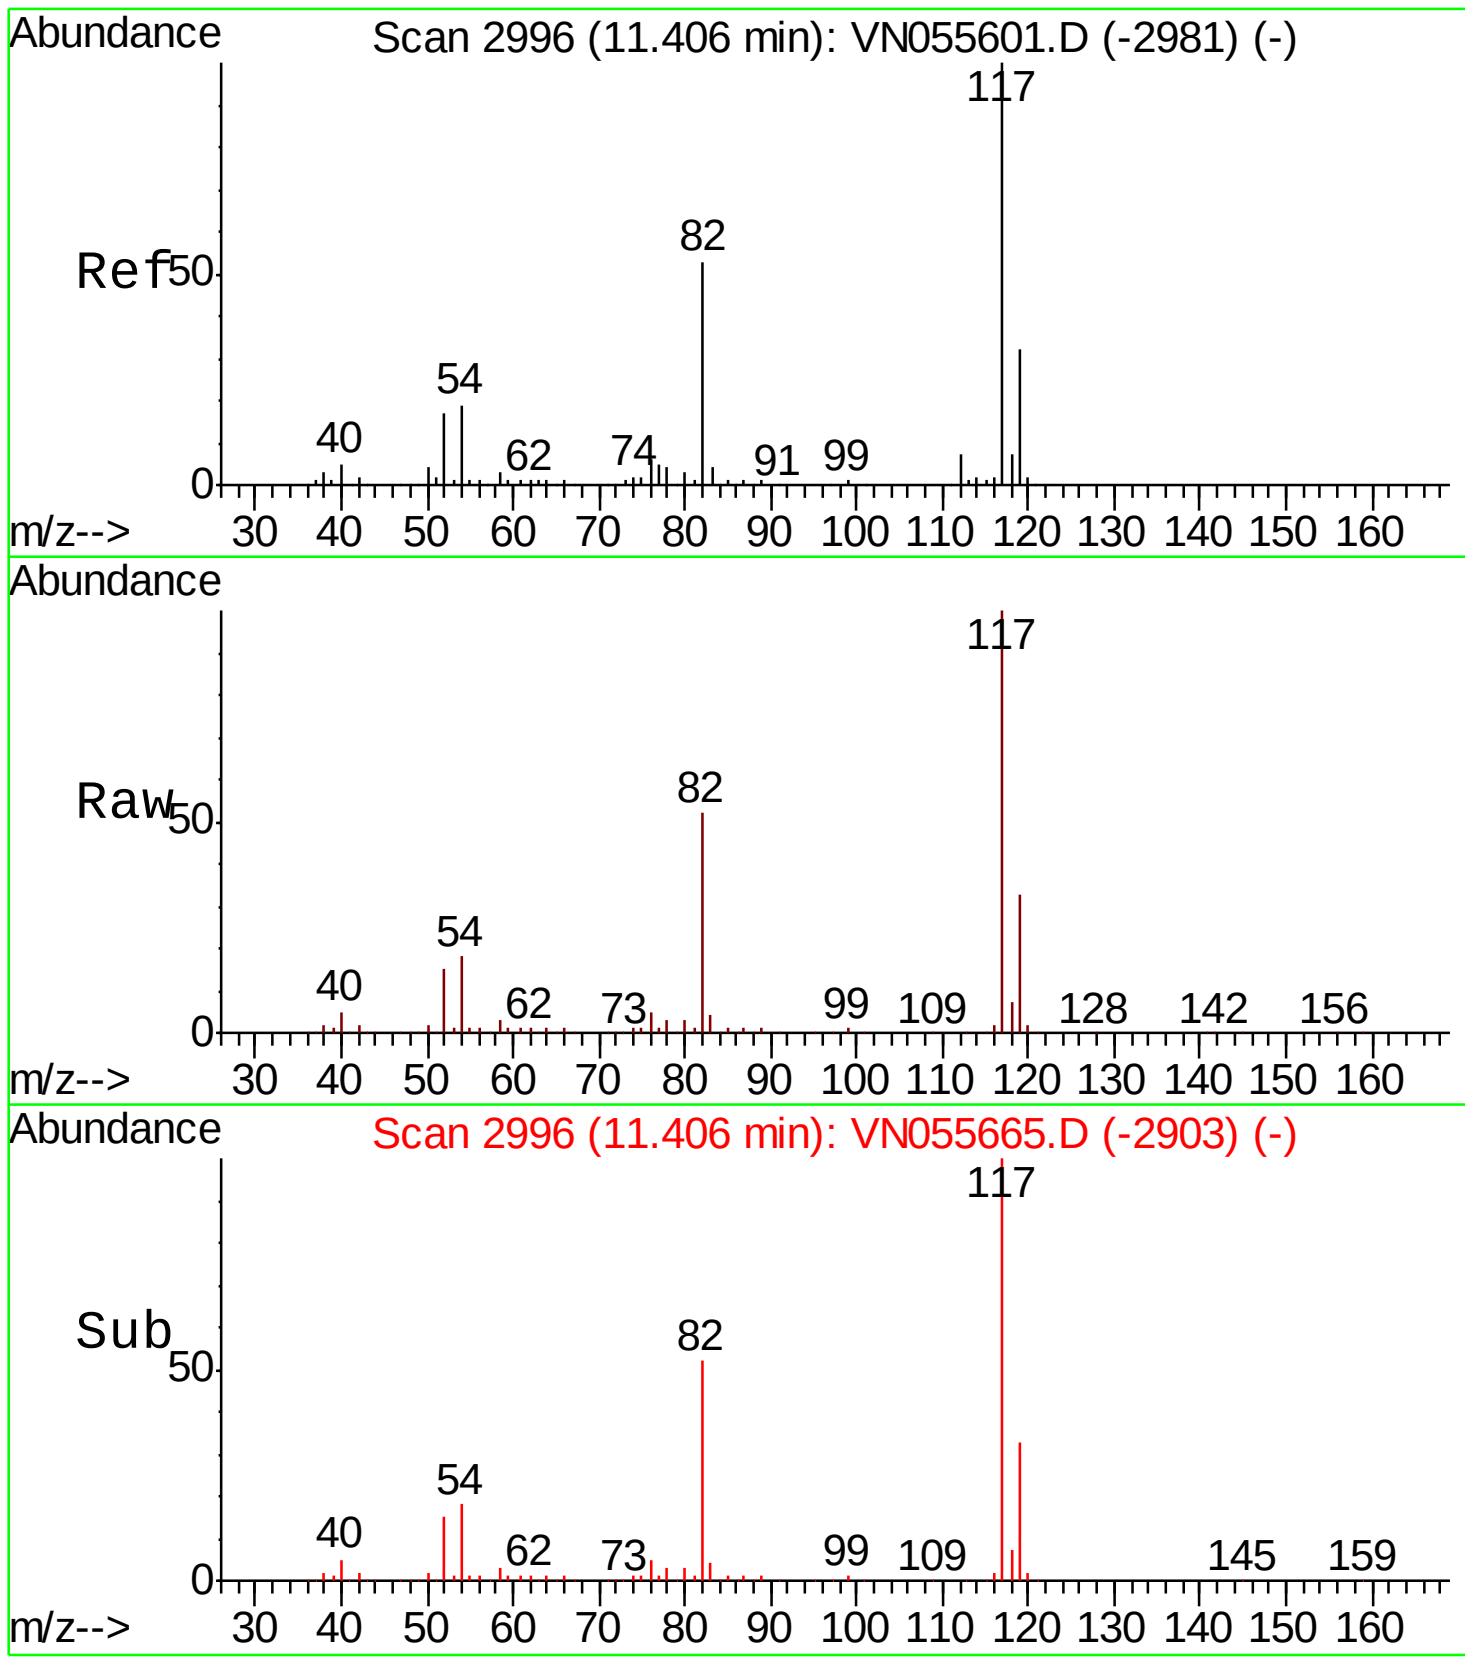

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.41 min   Scan# 2996
Delta R.T.   -0.00 min
Lab File: VN055665.D
Acq: 20 May 2019   11:37

Tgt Ion:117 Resp: 540094

Ion	Ratio	Lower	Upper
117	100		
82	51.7	42.3	63.5
119	32.7	25.4	38.2



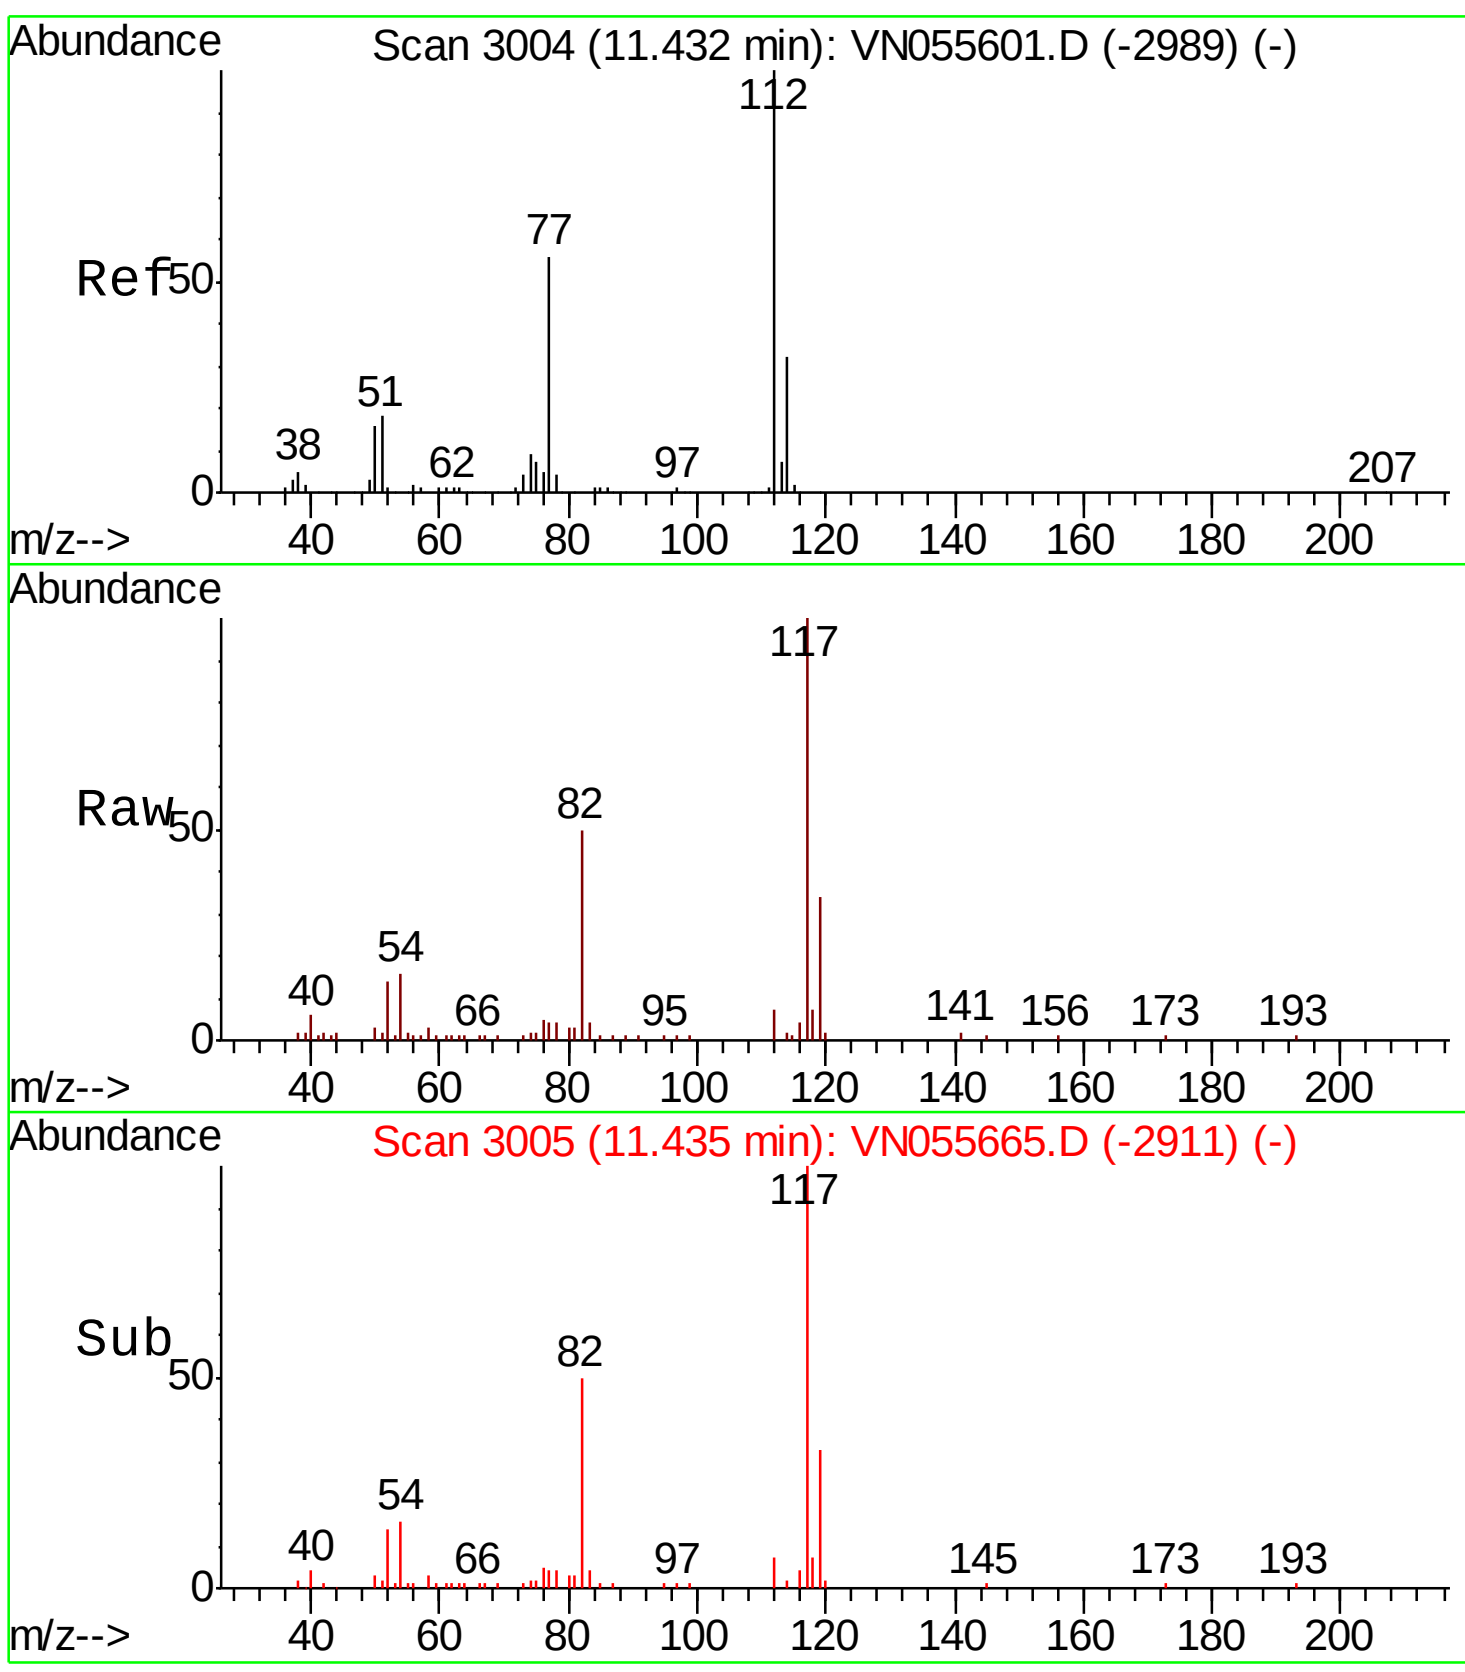

#65
Chlorobenzene
Concen: 0.276 ug/l
RT: 11.44 min   Scan# 3005
Delta R.T.   0.00 min
Lab File: VN055665.D
Acq: 20 May 2019   11:37

Tgt Ion:112 Resp: 3012

Ion	Ratio	Lower	Upper
112	100		
114	28.4	25.6	38.4



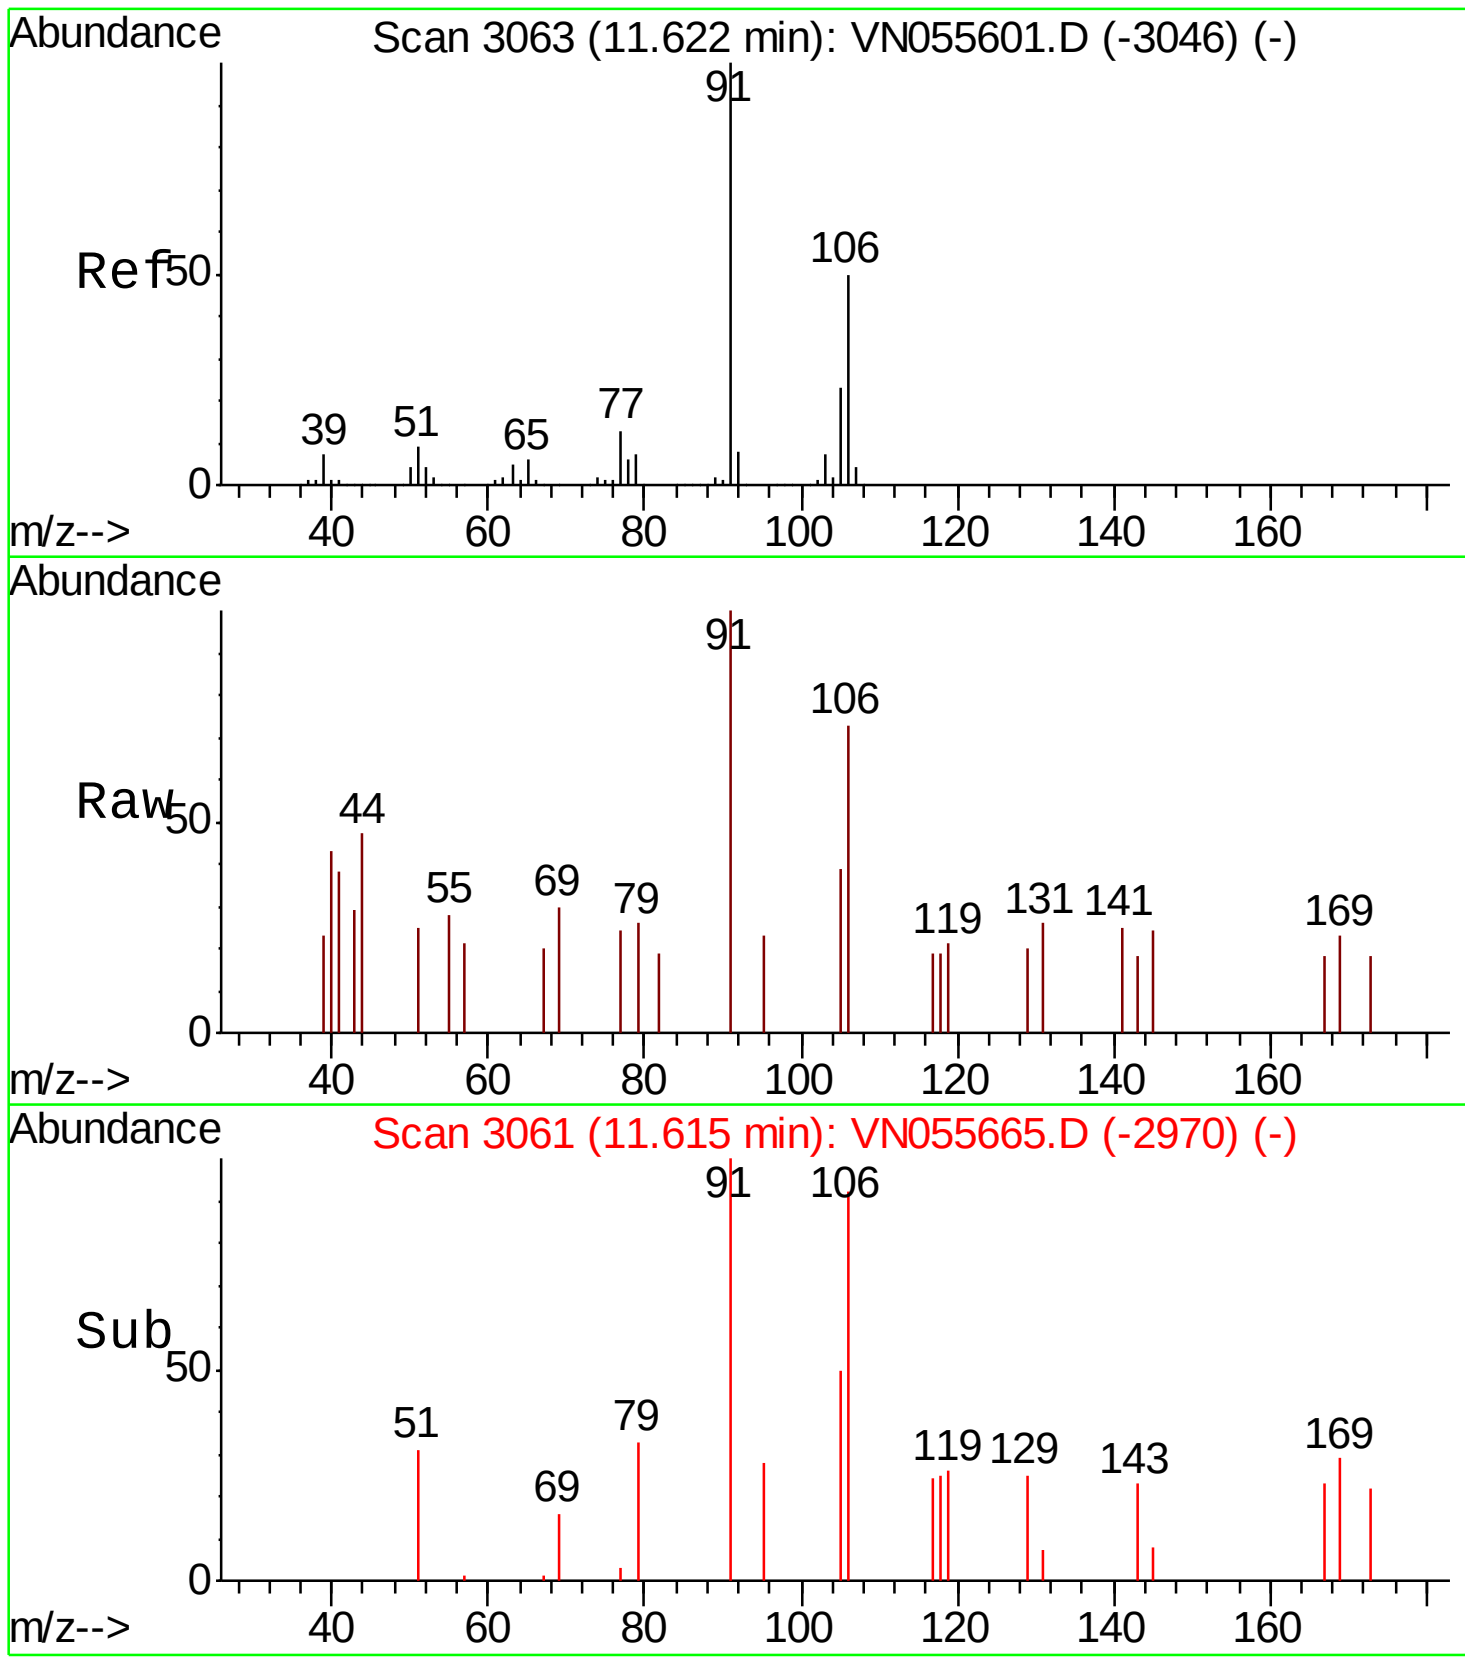

#68
m/p-Xylenes
Concen: 0.237 ug/l
RT: 11.62 min Scan# 3061
Delta R.T. -0.01 min
Lab File: VN055665.D
Acq: 20 May 2019 11:37

Tgt Ion:106 Resp: 1742

Ion	Ratio	Lower	Upper
106	100		
91	103.3	160.5	240.7#



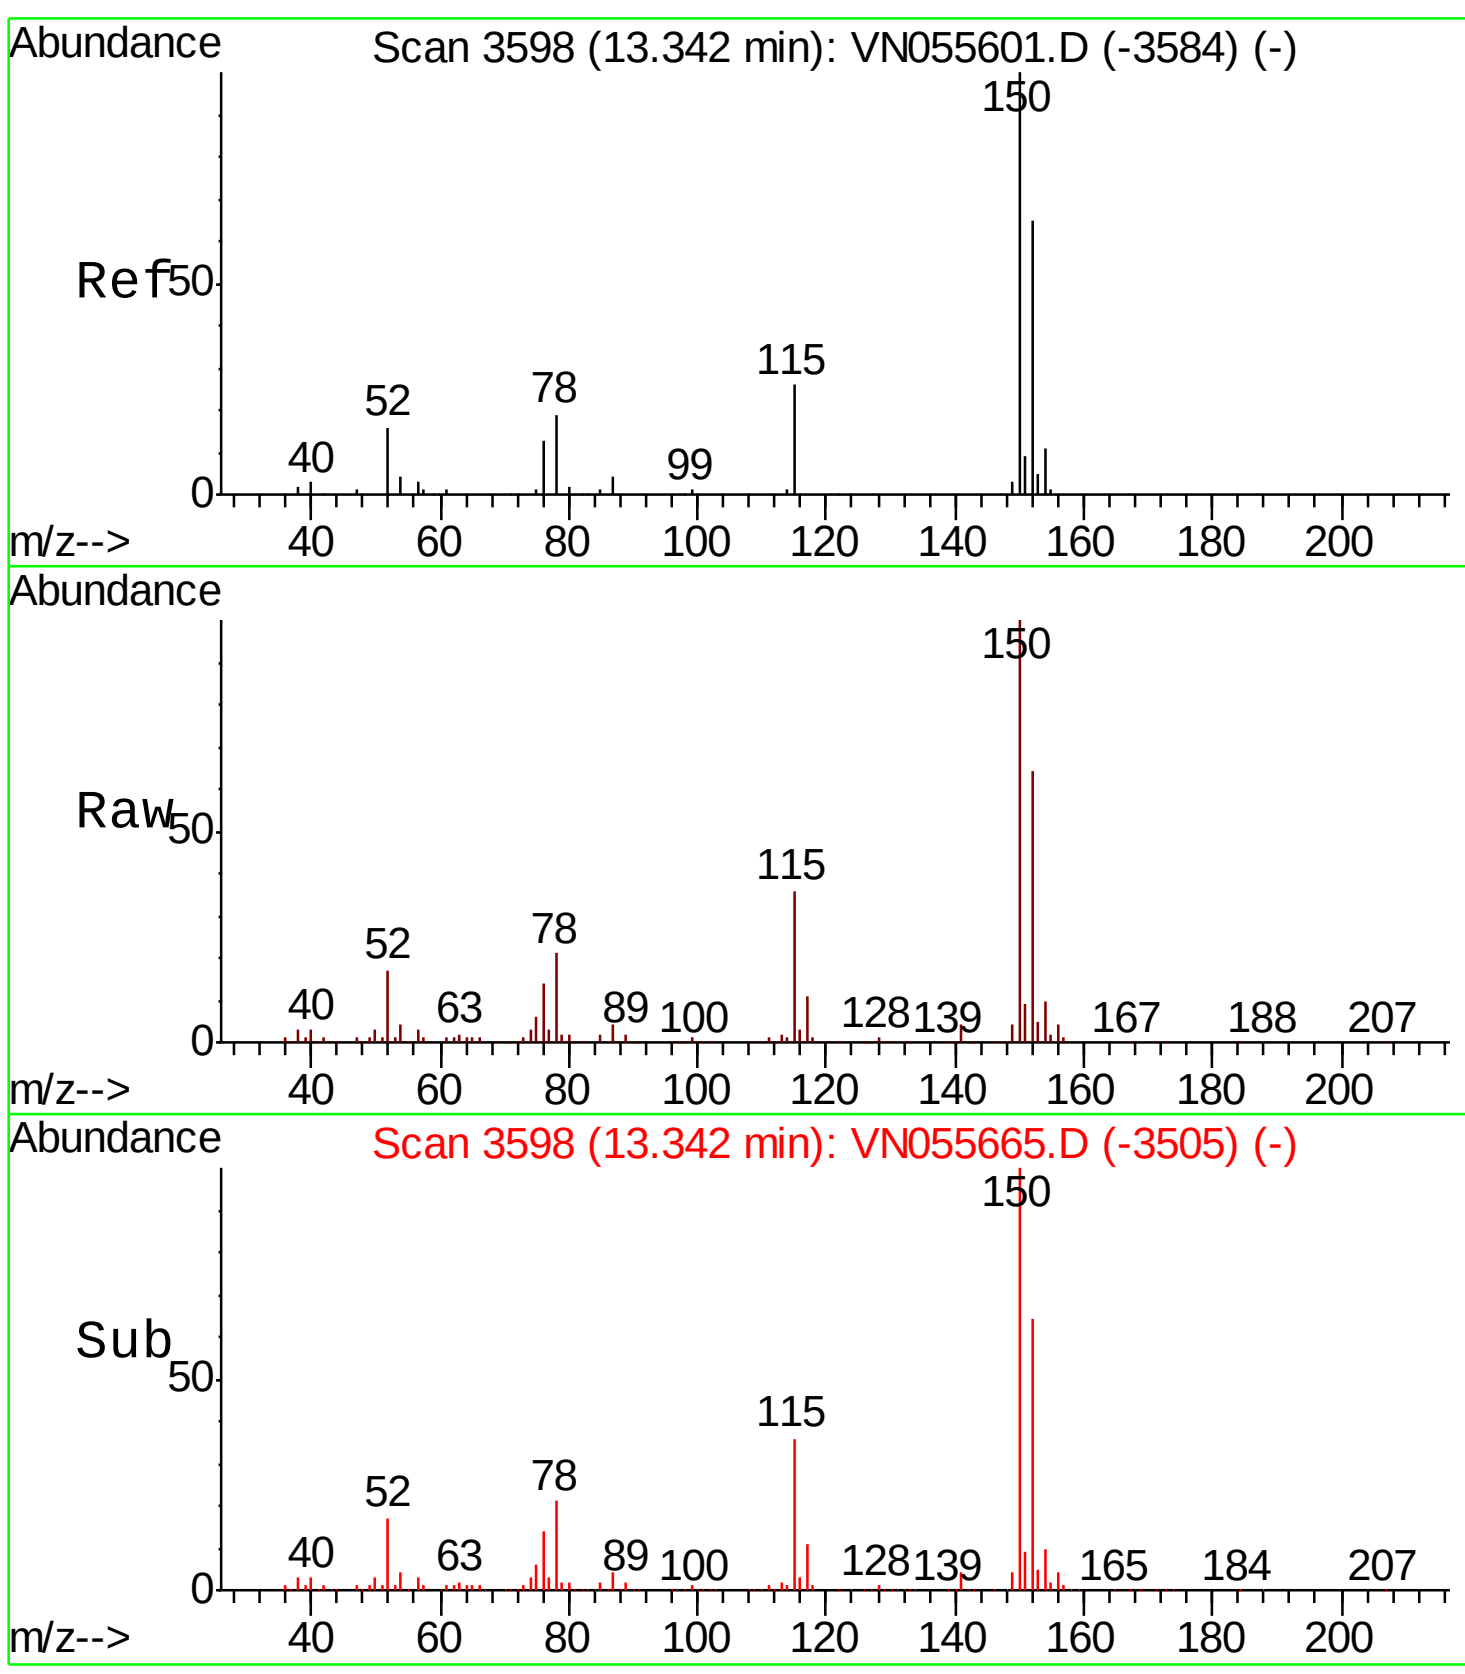

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.34 min Scan# 3598
Delta R.T. -0.00 min
Lab File: VN055665.D
Acq: 20 May 2019 11:37

Tgt Ion:152 Resp: 217418

Ion	Ratio	Lower	Upper
152	100		
115	57.3	28.1	84.2
150	155.8	0.0	348.0

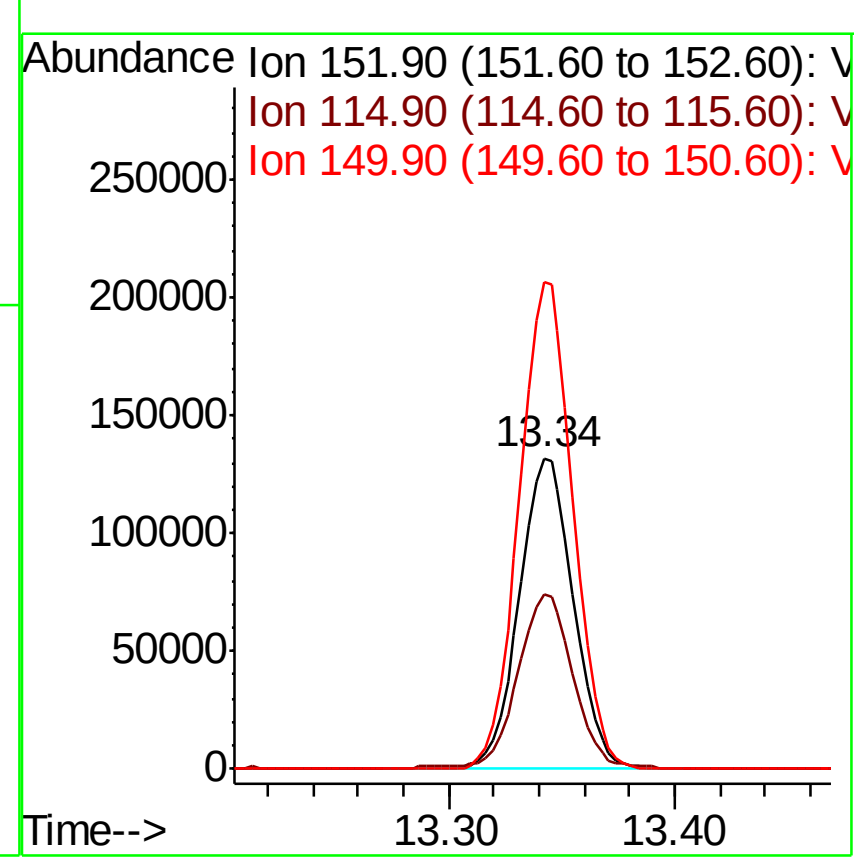

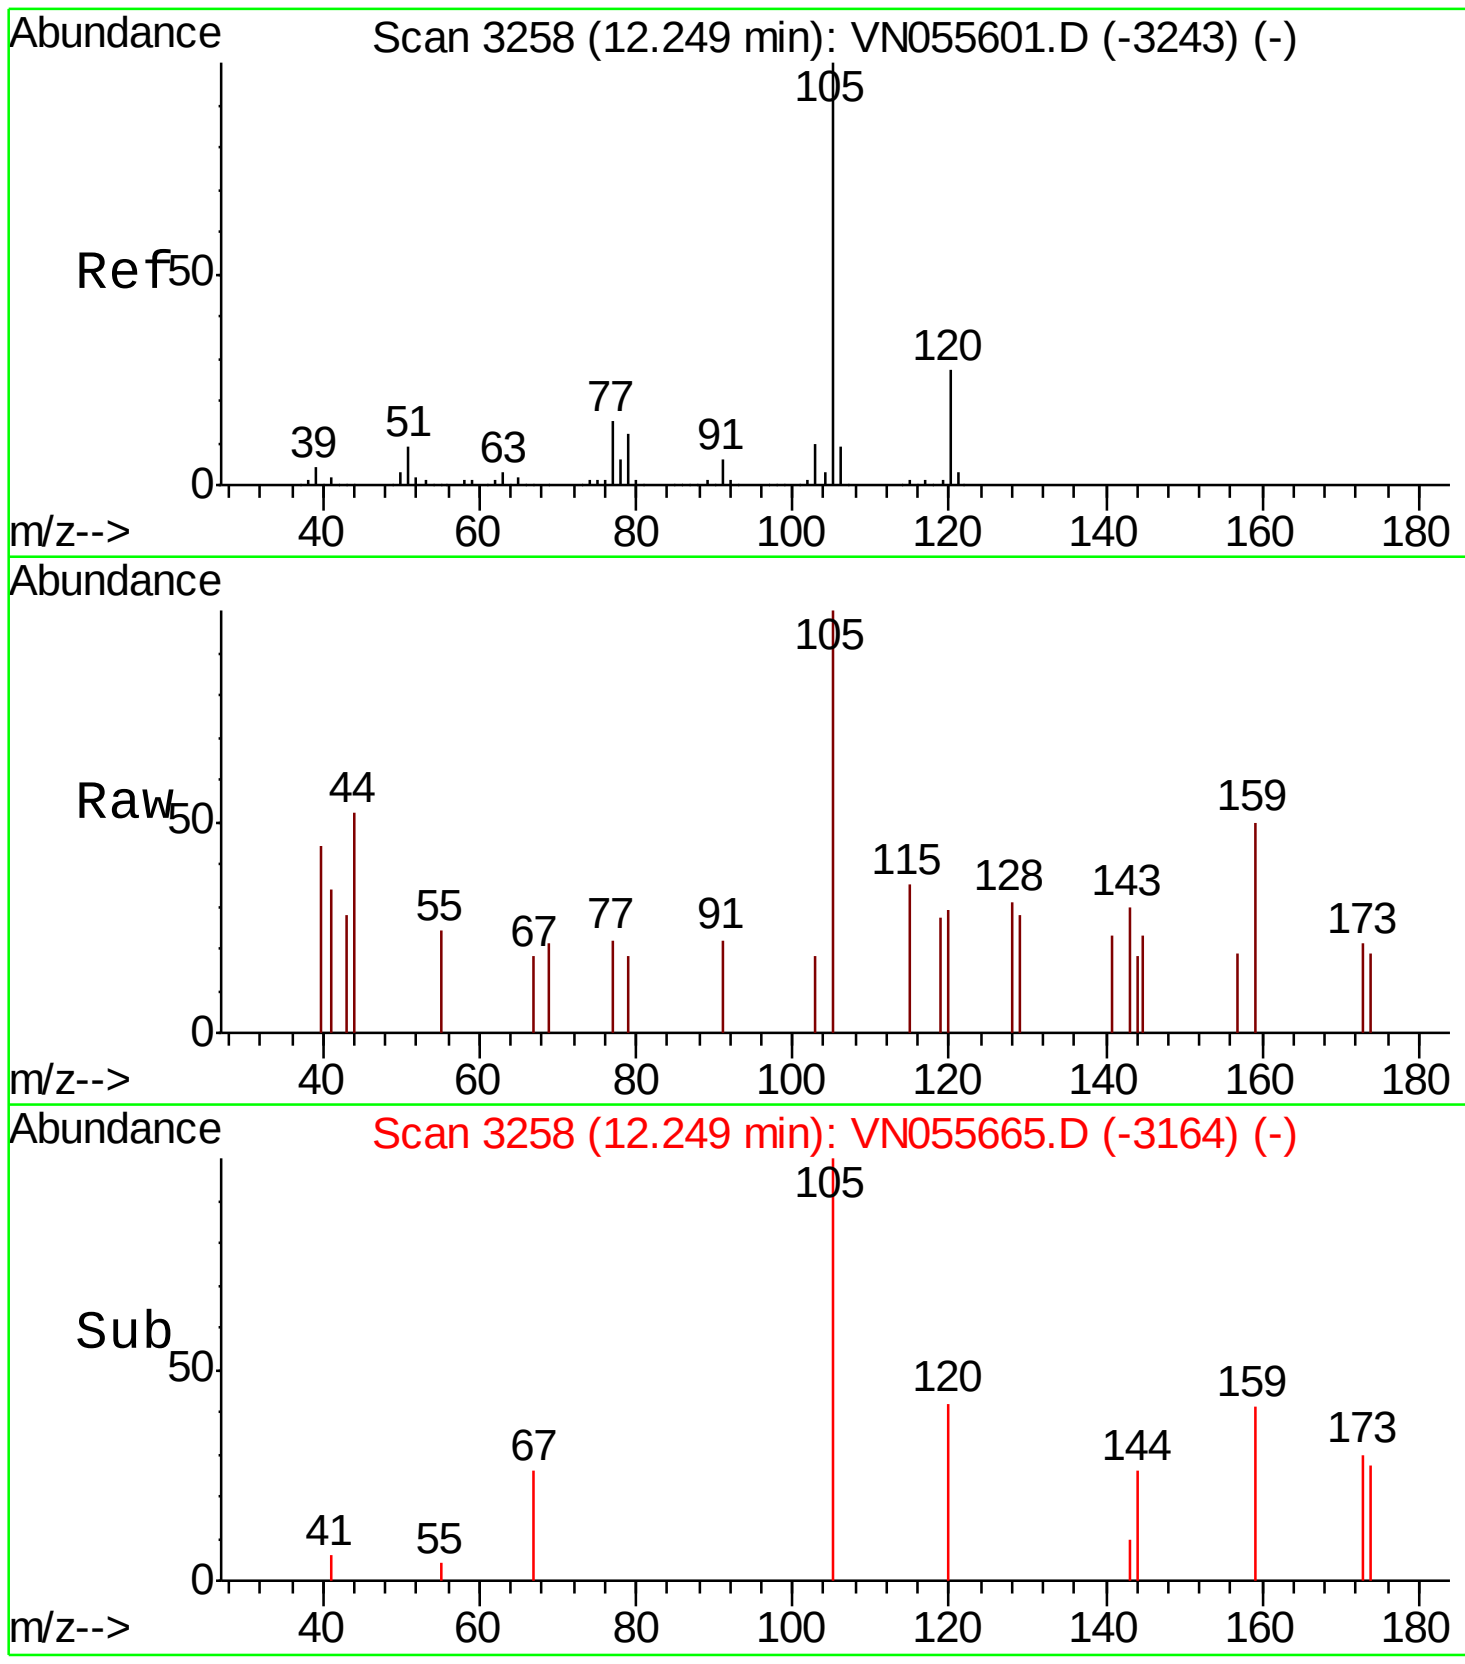

#73
Isopropylbenzene
Concen: Below Cal
RT: 12.25 min Scan# 3258
Delta R.T. 0.00 min
Lab File: VN055665.D
Acq: 20 May 2019 11:37

Tgt Ion:105 Resp: 1126

Ion	Ratio	Lower	Upper
105	100		
120	23.7	13.4	40.2



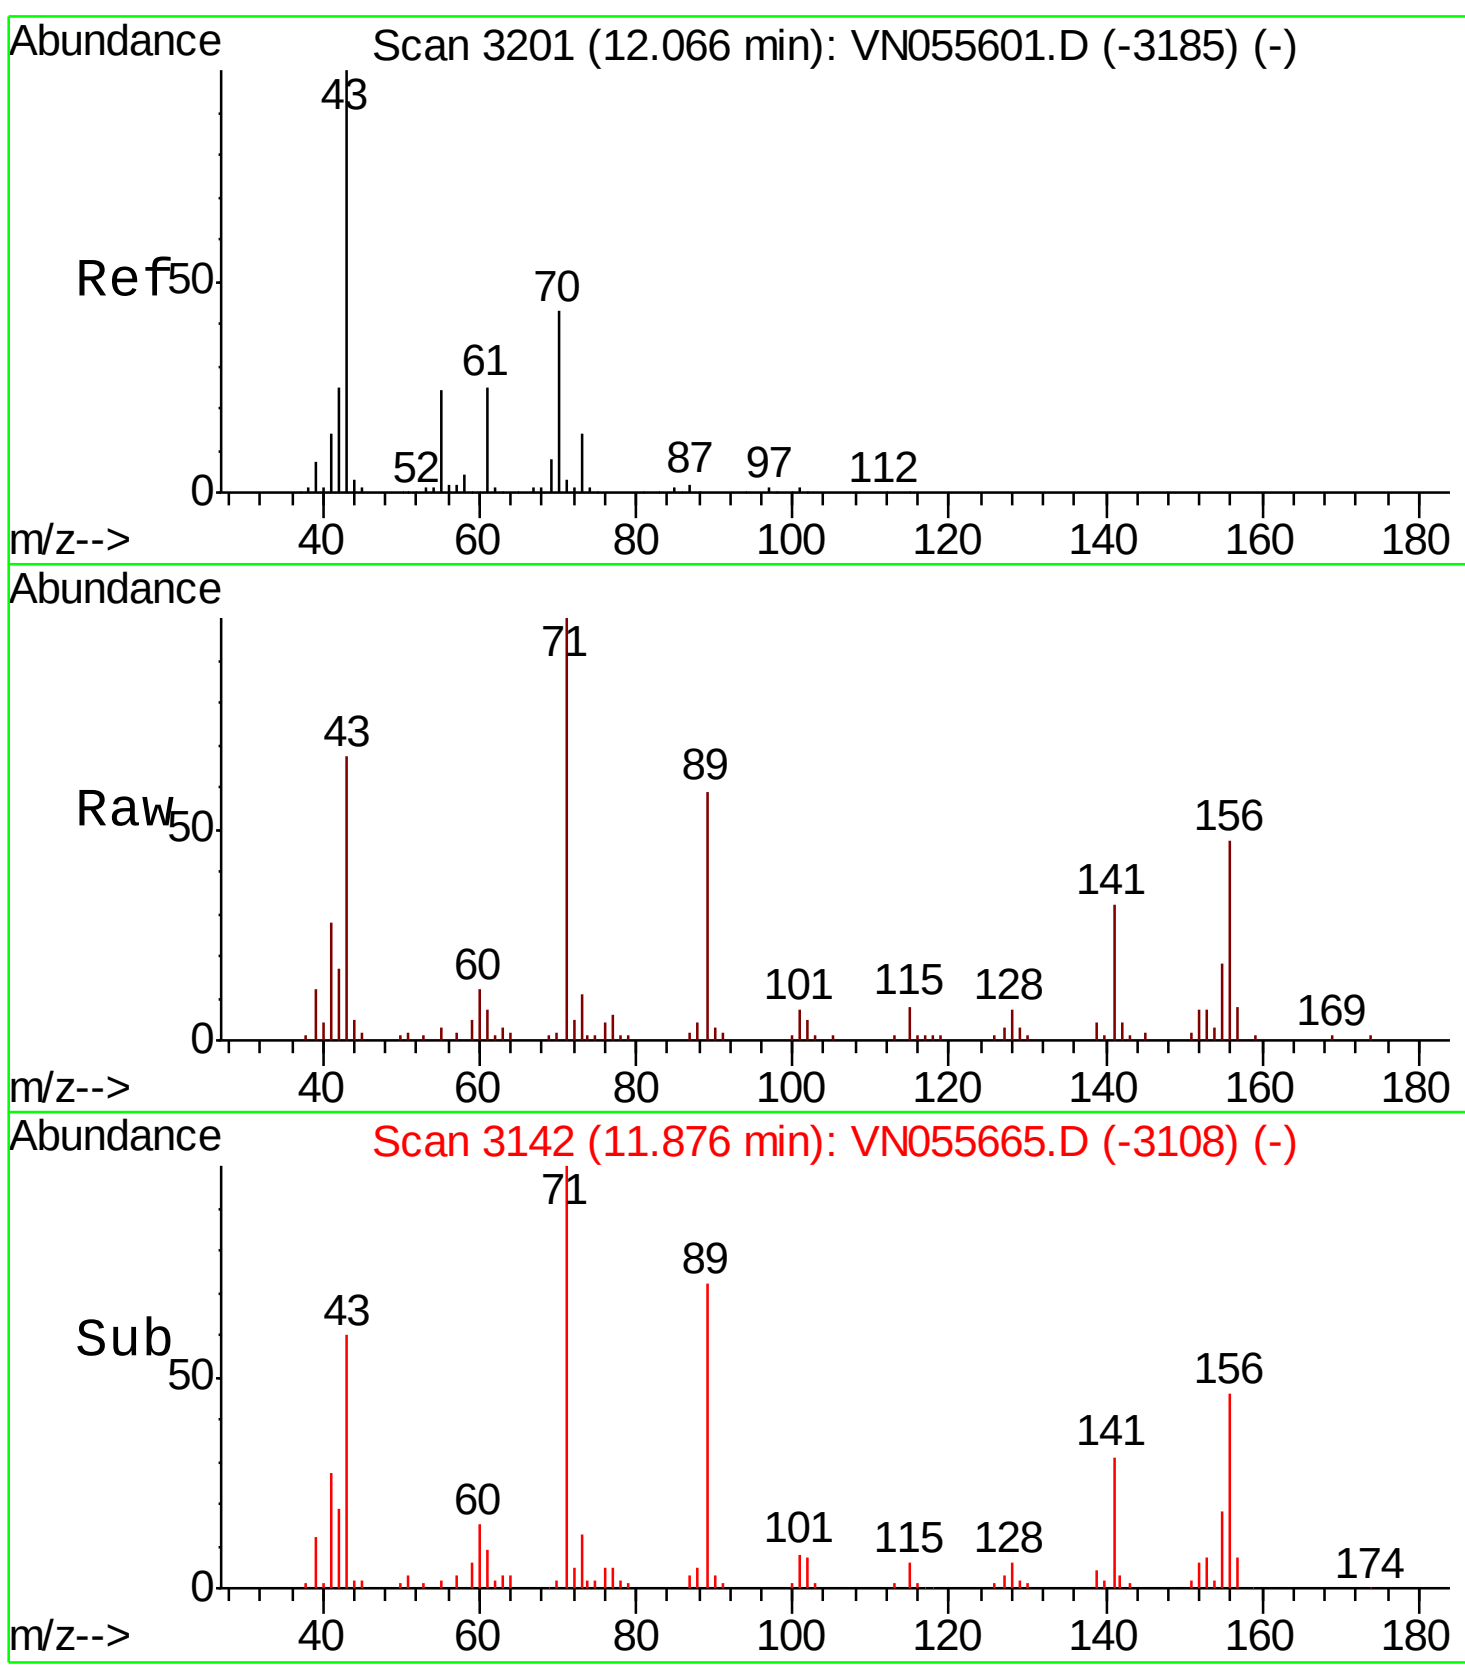

#74
N-amyl acetate
Concen: 3.077 ug/l
RT: 11.88 min Scan# 3142
Delta R.T. -0.19 min
Lab File: VN055665.D
Acq: 20 May 2019 11:37

Tgt Ion: 43 Resp: 18785

Ion	Ratio	Lower	Upper
43	100		
70	1.8	35.0	52.6#
55	3.3	18.9	28.3#
61	11.4	20.1	30.1#



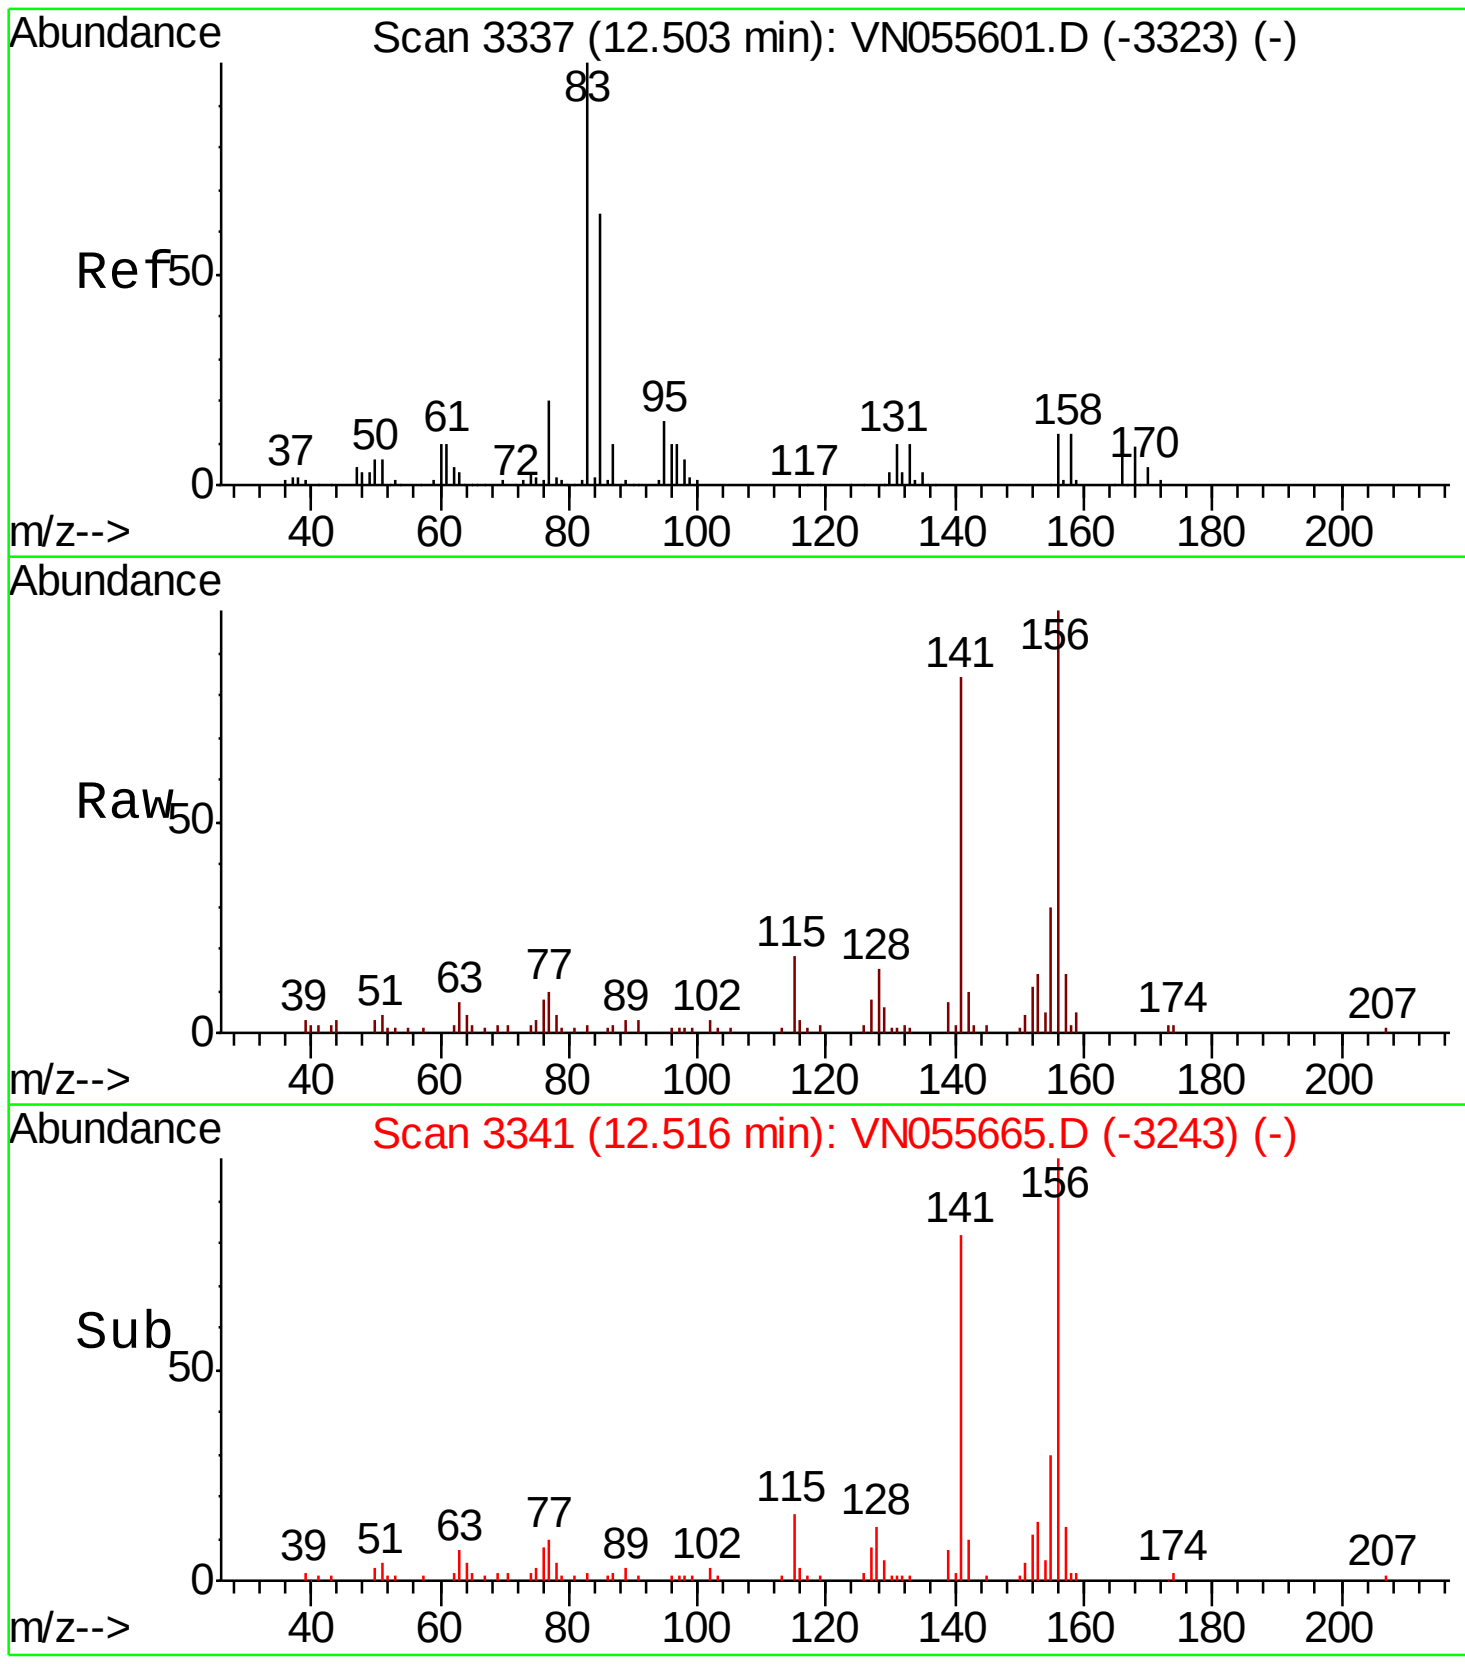

#75
1,1,2,2-Tetrachloroethane
Concen: Below Cal
RT: 12.52 min   Scan# 3341
Delta R.T.   0.01 min
Lab File: VN055665.D
Acq: 20 May 2019   11:37

Tgt Ion: 83 Resp: 197

Ion	Ratio	Lower	Upper
83	100		
131	0.0	5.3	16.1#
85	0.0	32.0	96.2#



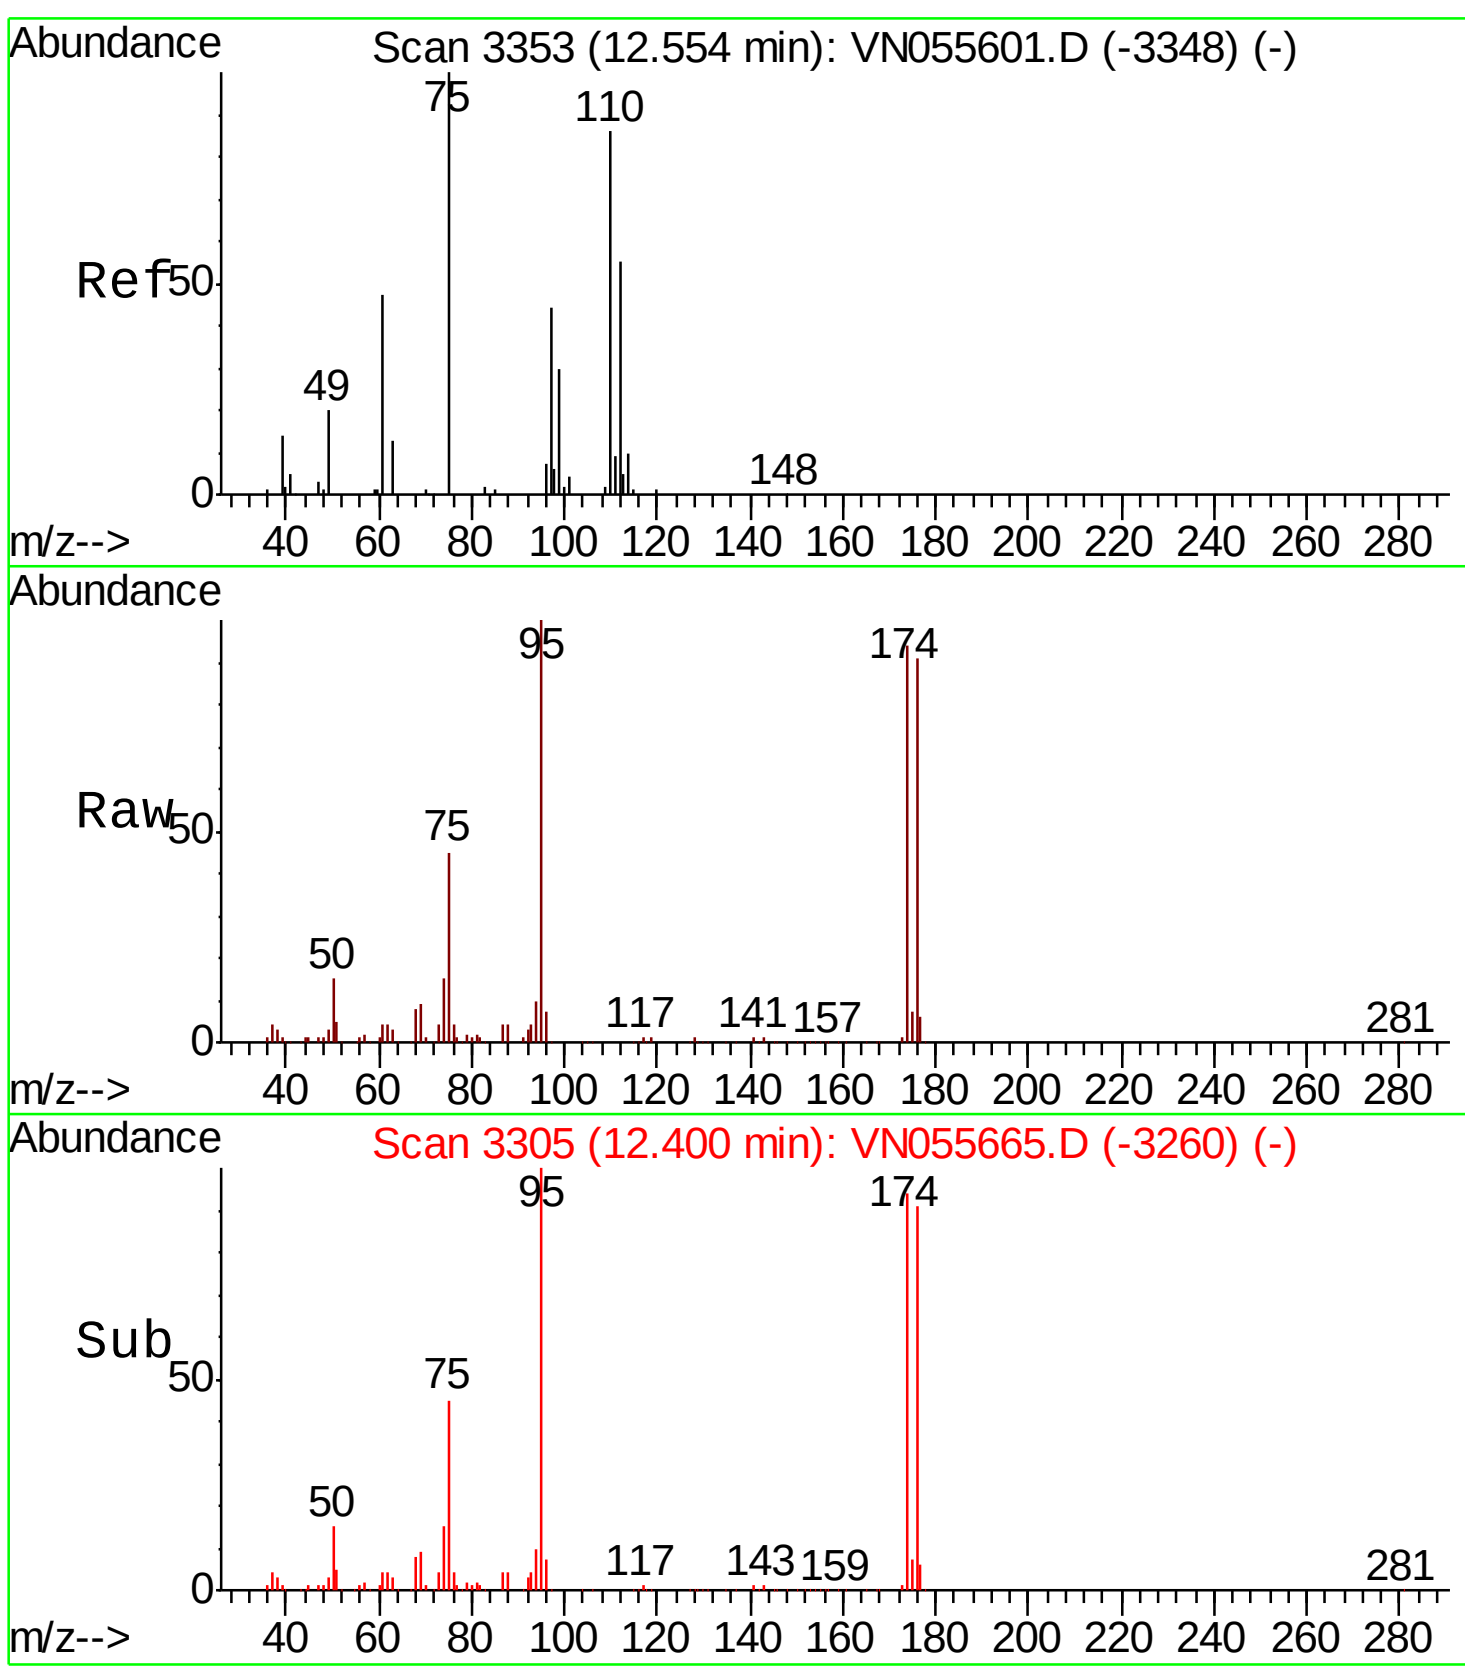

#76
1,2,3-Trichloropropane
Concen: 24.114 ug/l
RT: 12.40 min   Scan# 3305
Delta R.T.   -0.15 min
Lab File: VN055665.D
Acq: 20 May 2019   11:37

Tgt Ion: 75 Resp: 106982

Ion	Ratio	Lower	Upper
75	100		
77	1.4	0.0	0.0#

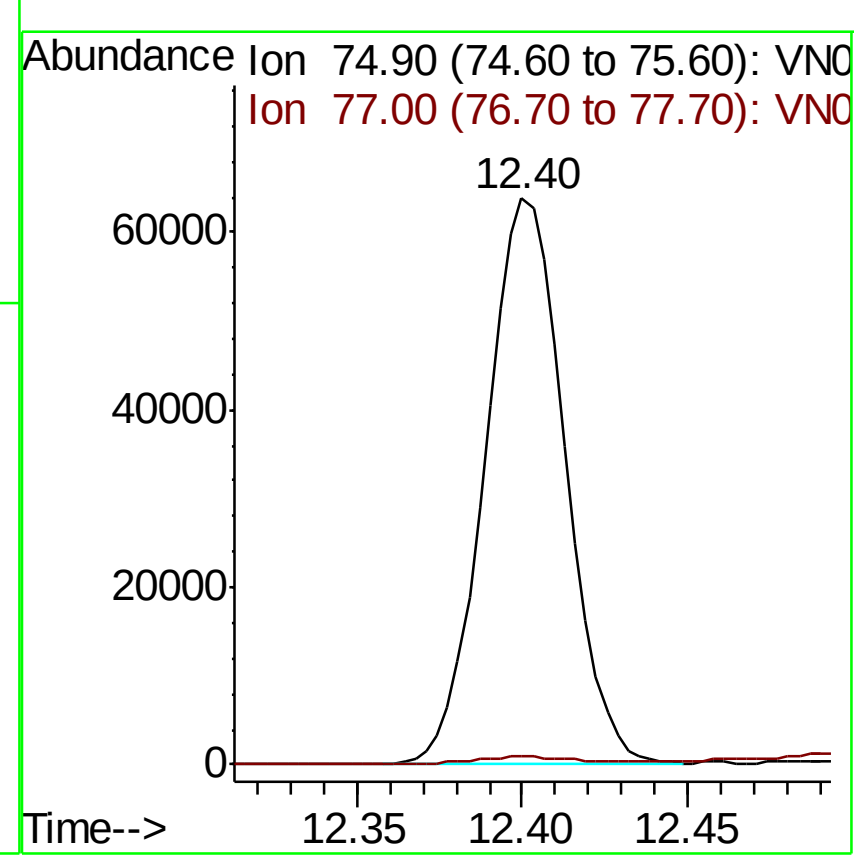

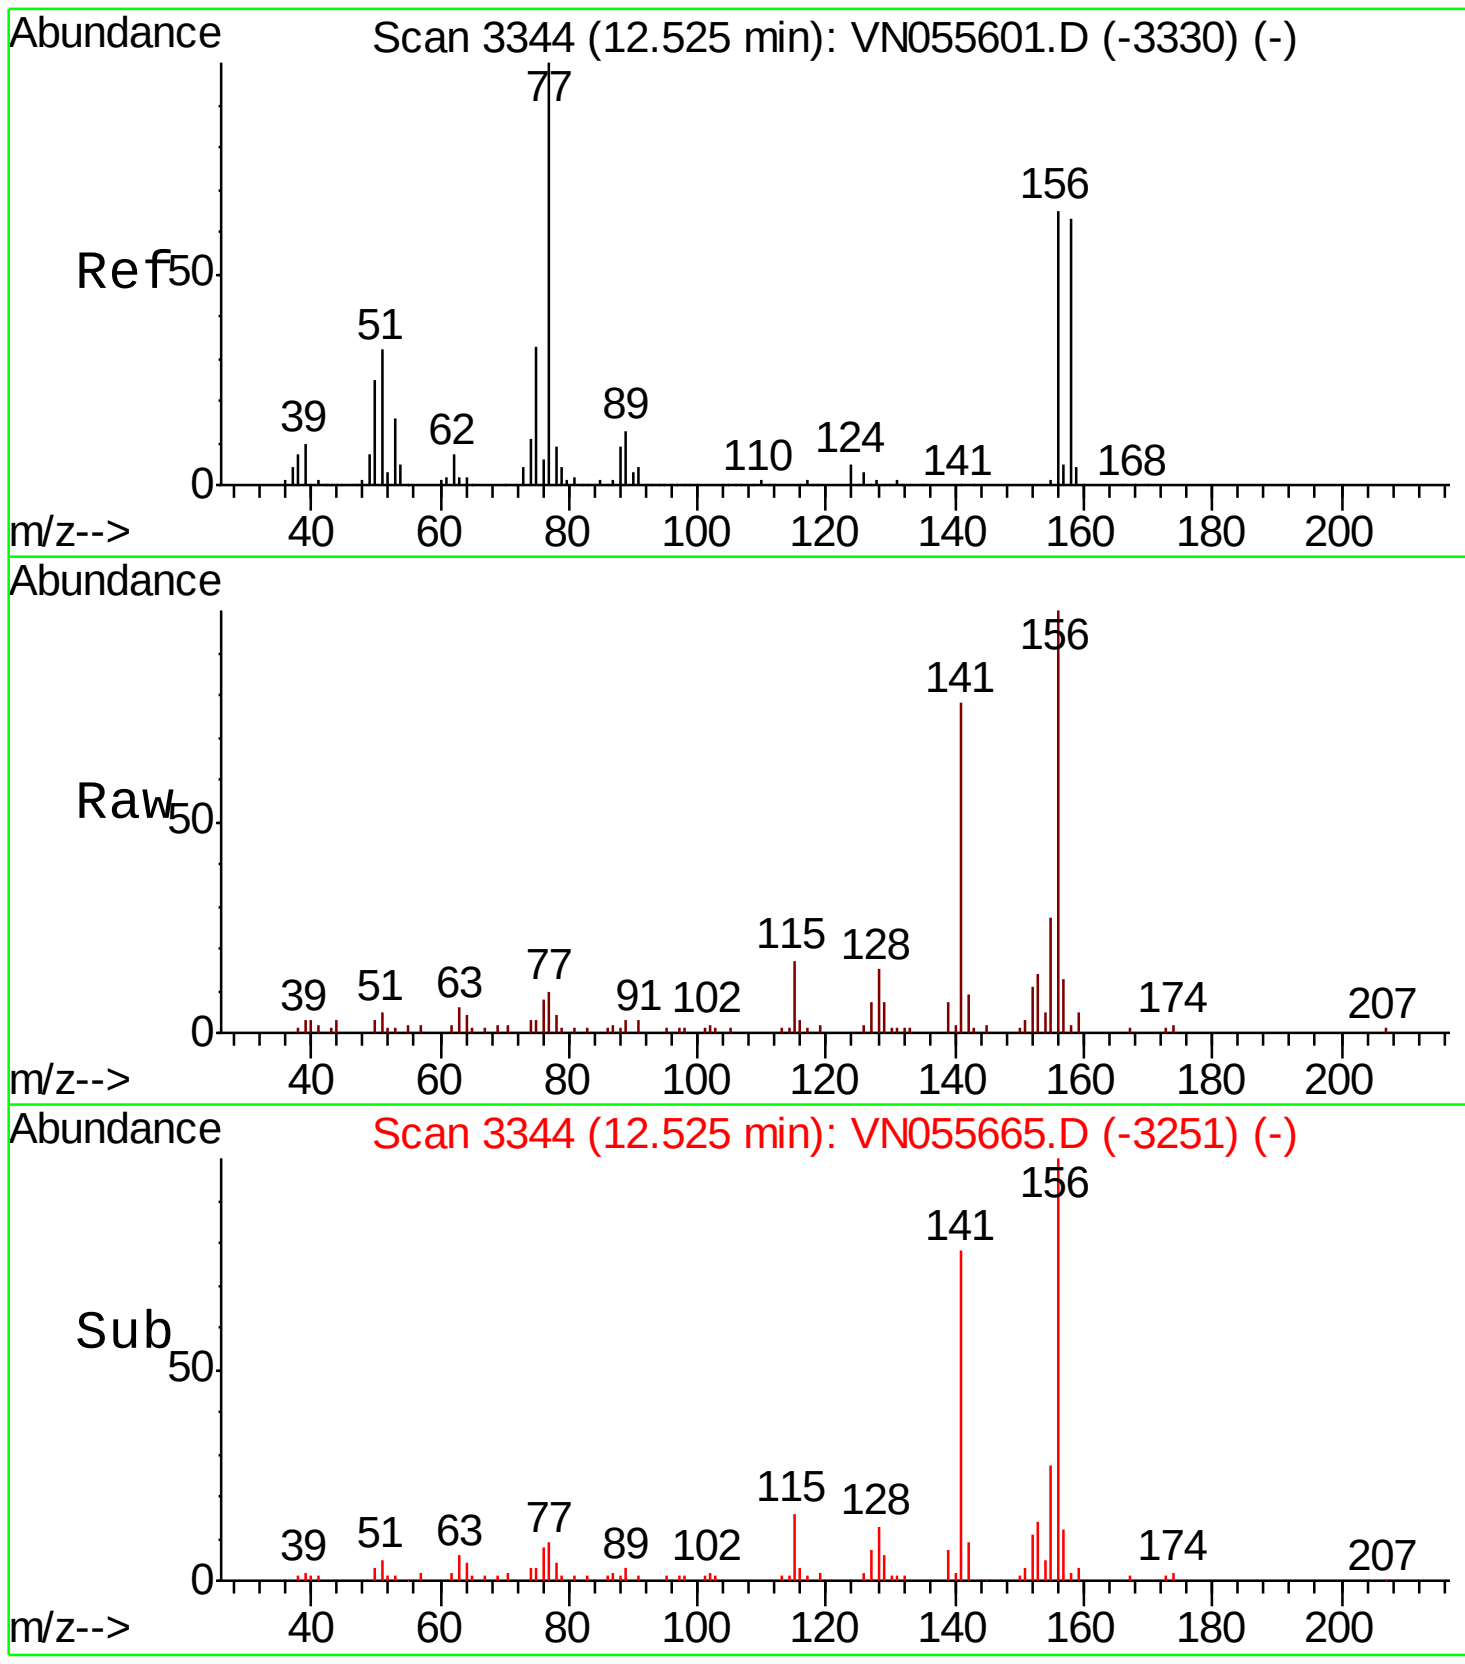

#77
Bromobenzene
Concen: 24.215 ug/l
RT: 12.53 min Scan# 3344
Delta R.T. -0.00 min
Lab File: VN055665.D
Acq: 20 May 2019 11:37

Tgt Ion:156	Resp:		108126
Ion	Ratio	Lower	Upper
156	100		
77	1.9	94.5	283.5#
158	0.9	49.0	147.2#



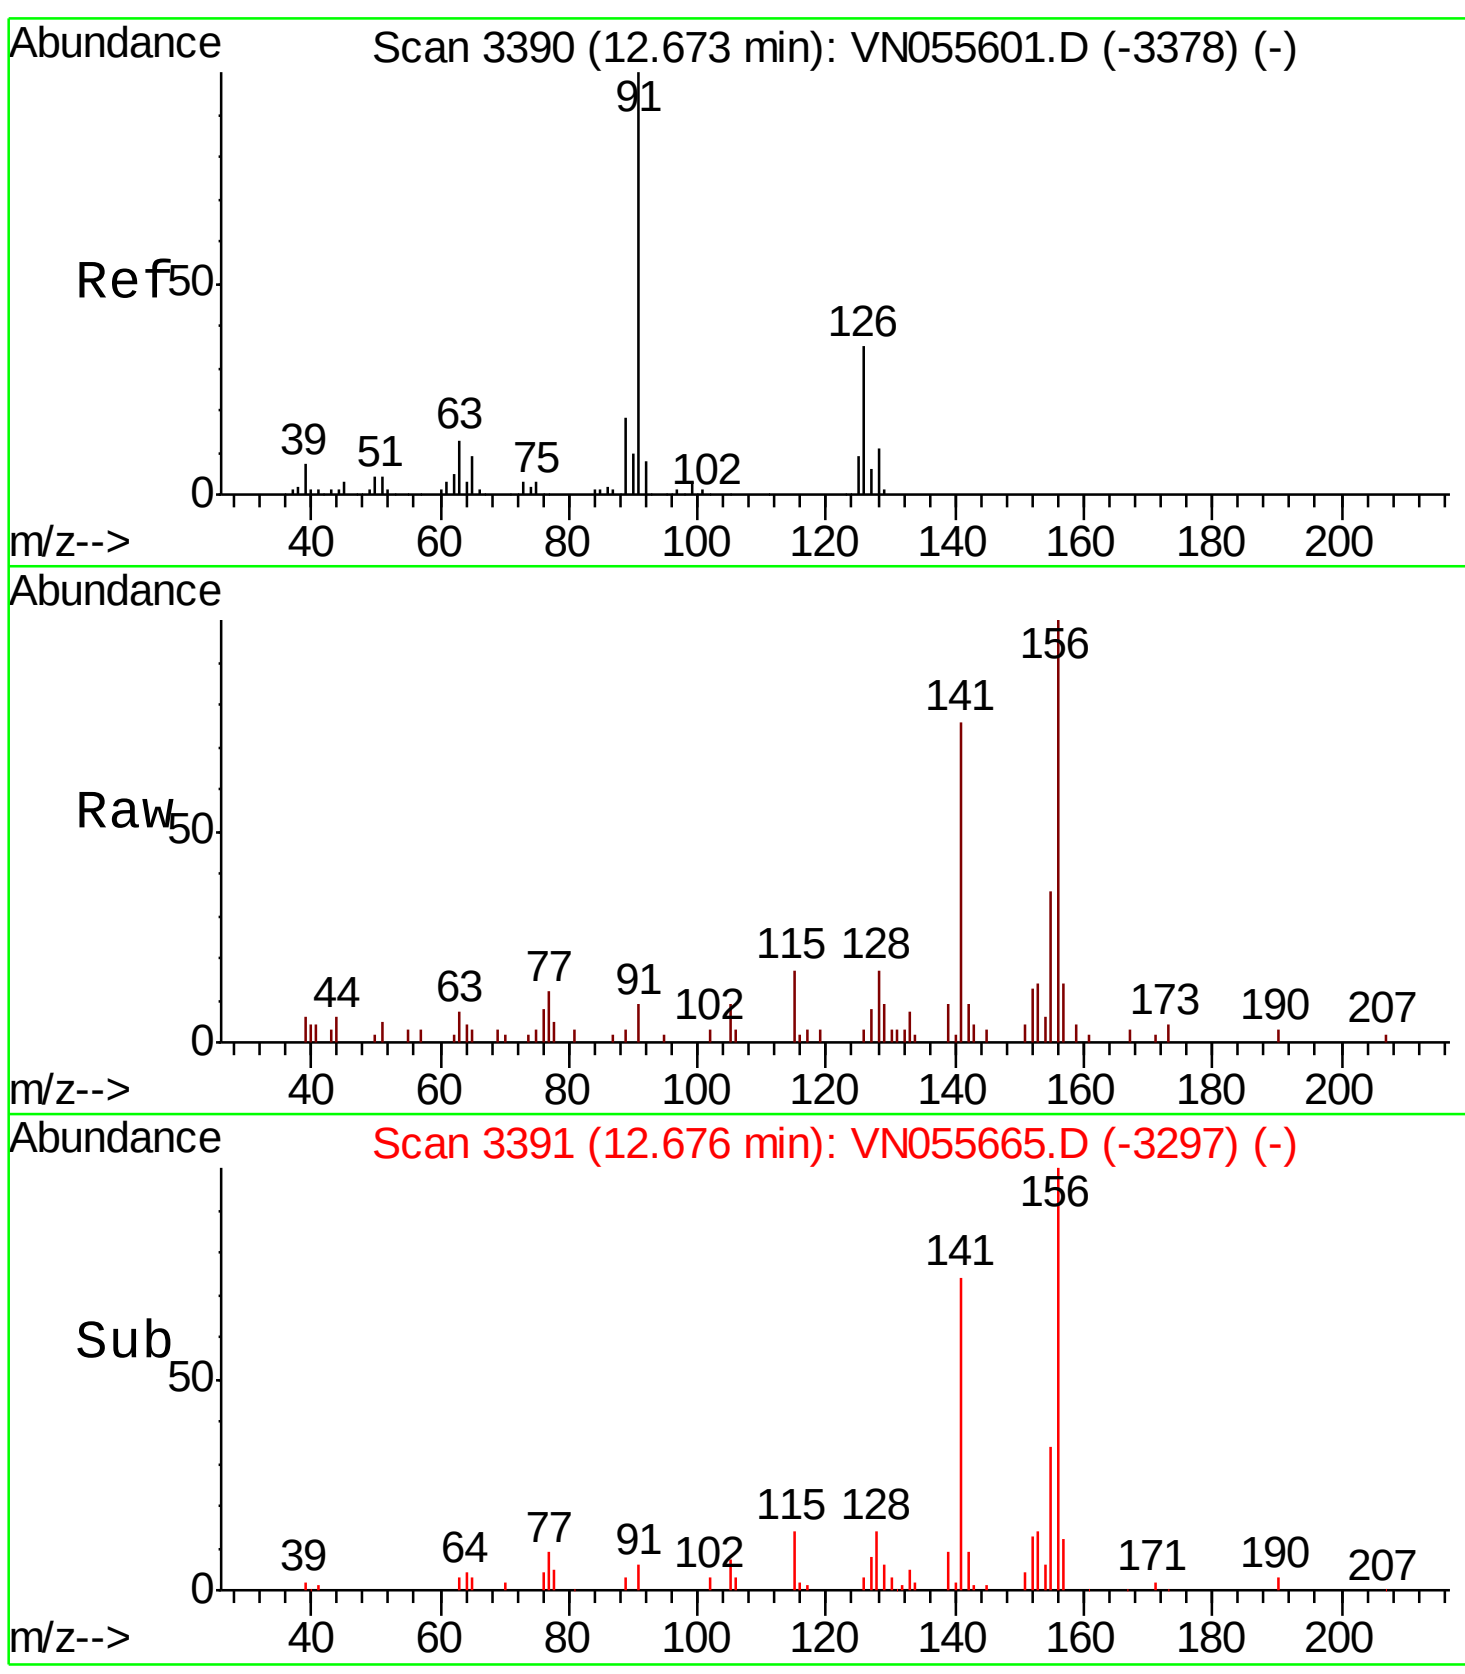

#79
2-Chlorotoluene
Concen: Below Cal
RT: 12.68 min Scan# 3391
Delta R.T. 0.00 min
Lab File: VN055665.D
Acq: 20 May 2019 11:37

Tgt Ion: 91	Resp:		986
Ion	Ratio	Lower	Upper
91	100		
126	59.2	17.8	53.4#



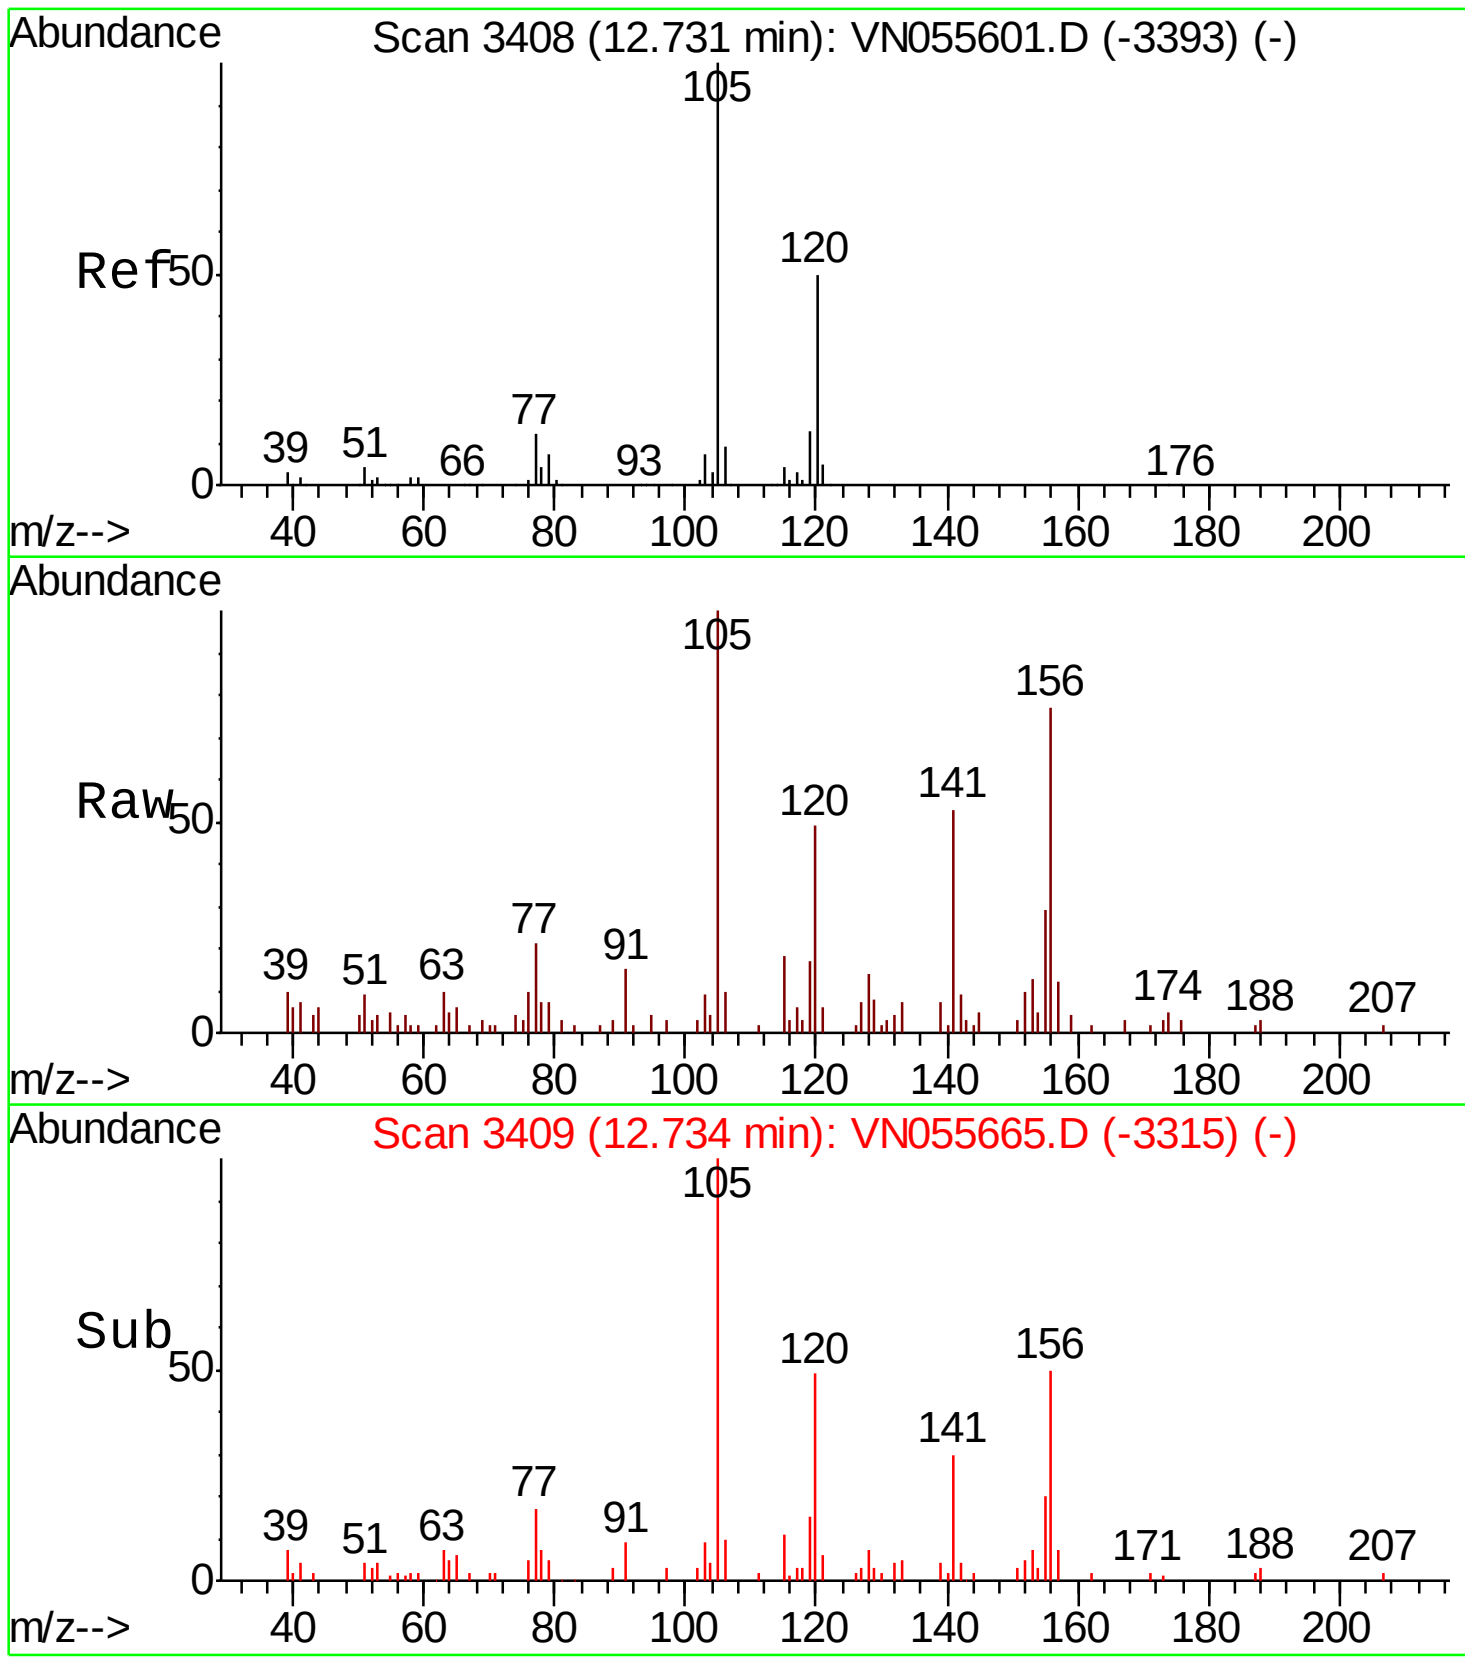

#80
1,3,5-Trimethylbenzene
Concen: Below Cal
RT: 12.73 min   Scan# 3409
Delta R.T.   0.00 min
Lab File: VN055665.D
Acq: 20 May 2019   11:37

Tgt Ion:105	Resp:		14045
Ion	Ratio	Lower	Upper
105	100		
120	48.9	24.6	74.0



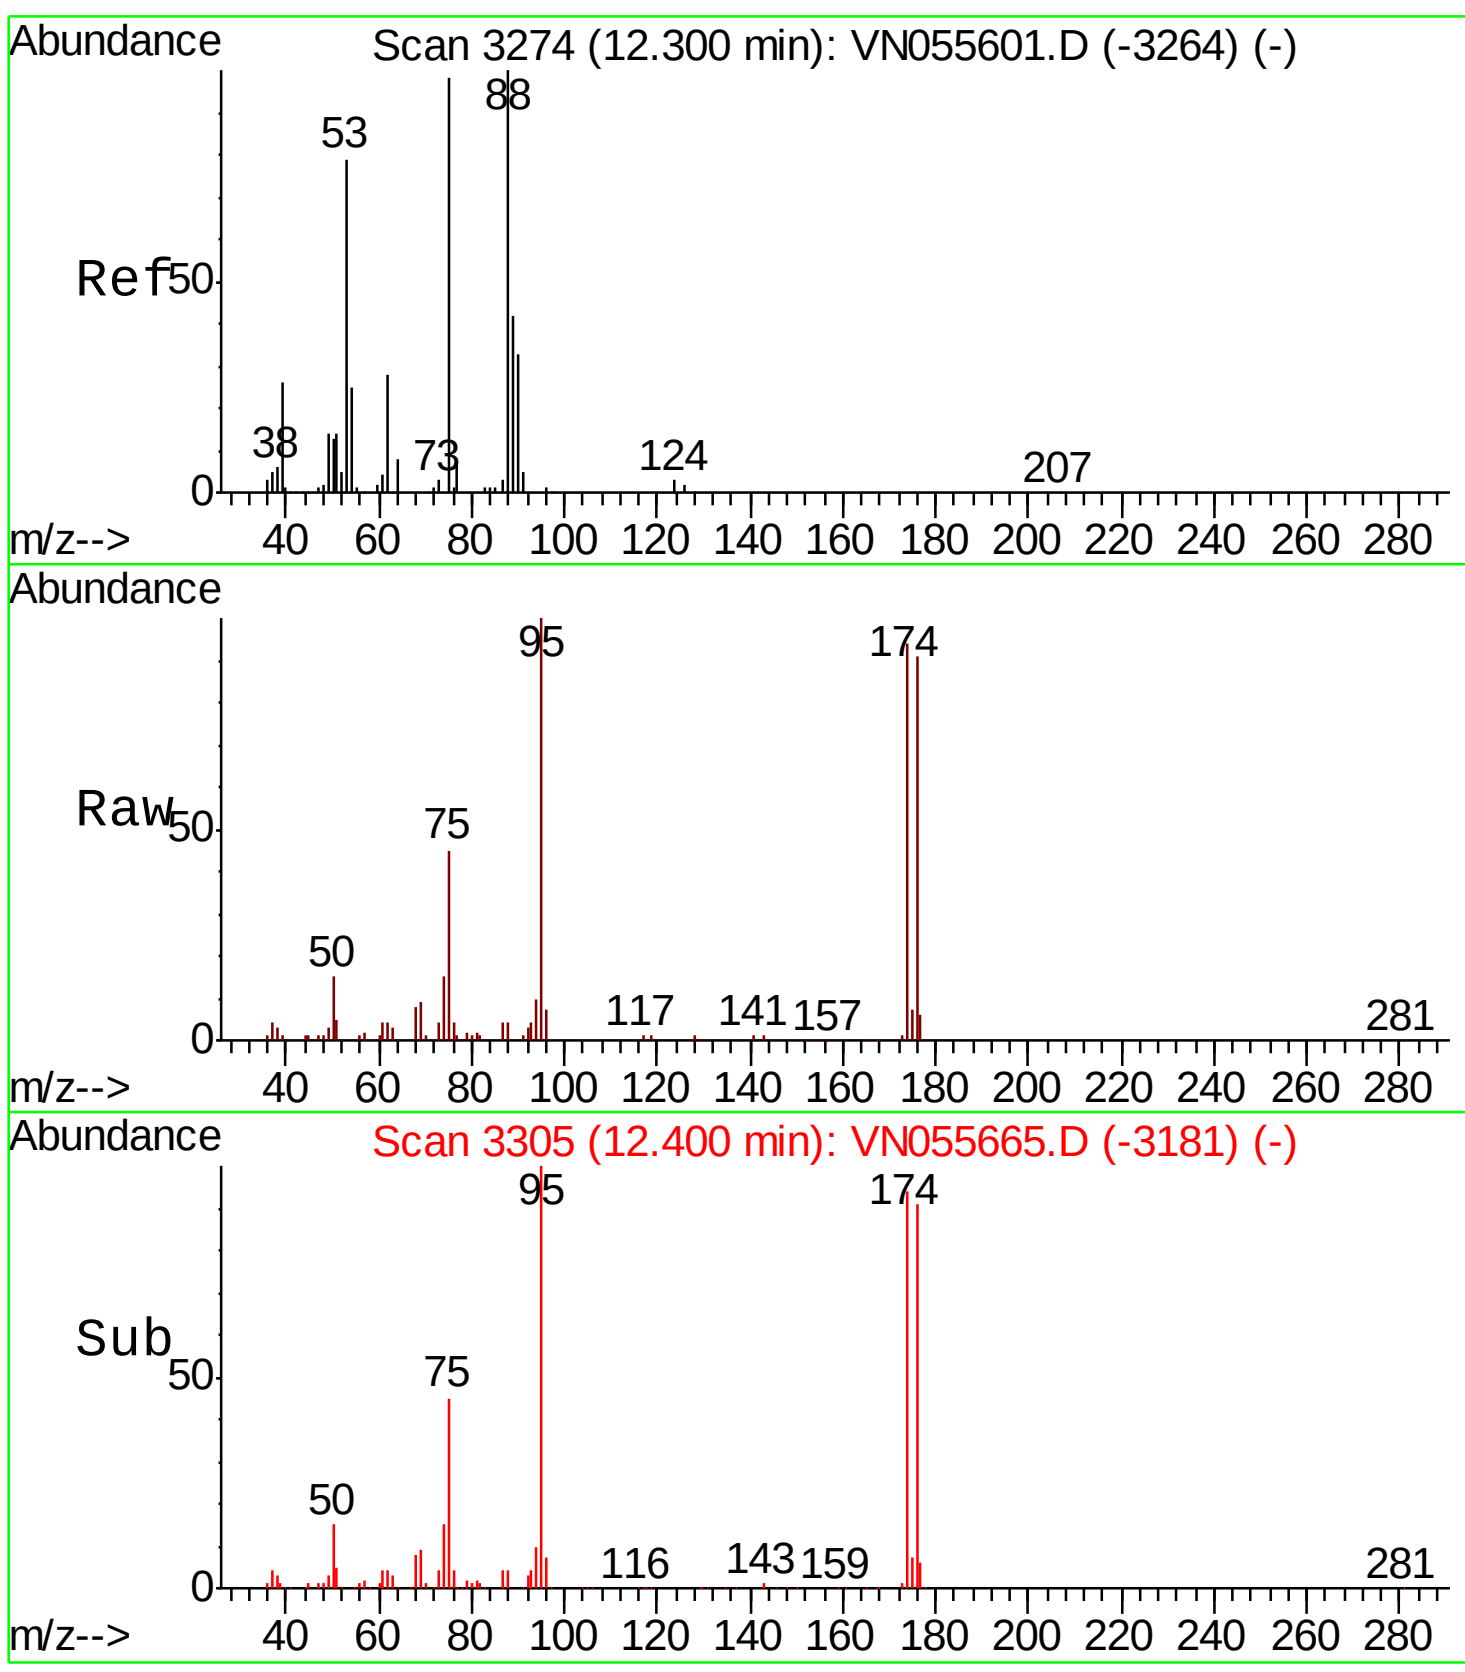

#81
trans-1,4-Dichloro-2-butene
Concen: 61.988 ug/l
RT: 12.40 min   Scan# 3305
Delta R.T.   0.10 min
Lab File: VN055665.D
Acq: 20 May 2019   11:37

Tgt Ion: 75	Resp:		106982
Ion	Ratio	Lower	Upper
75	100		
53	0.0	65.1	97.7#
89	0.0	36.4	54.6#

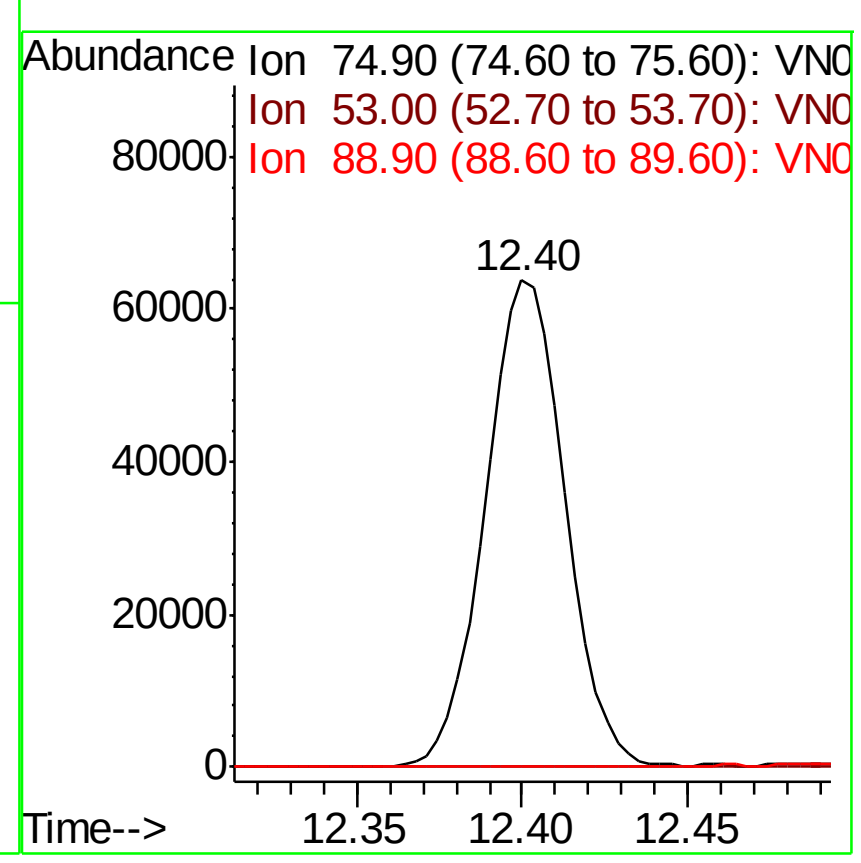

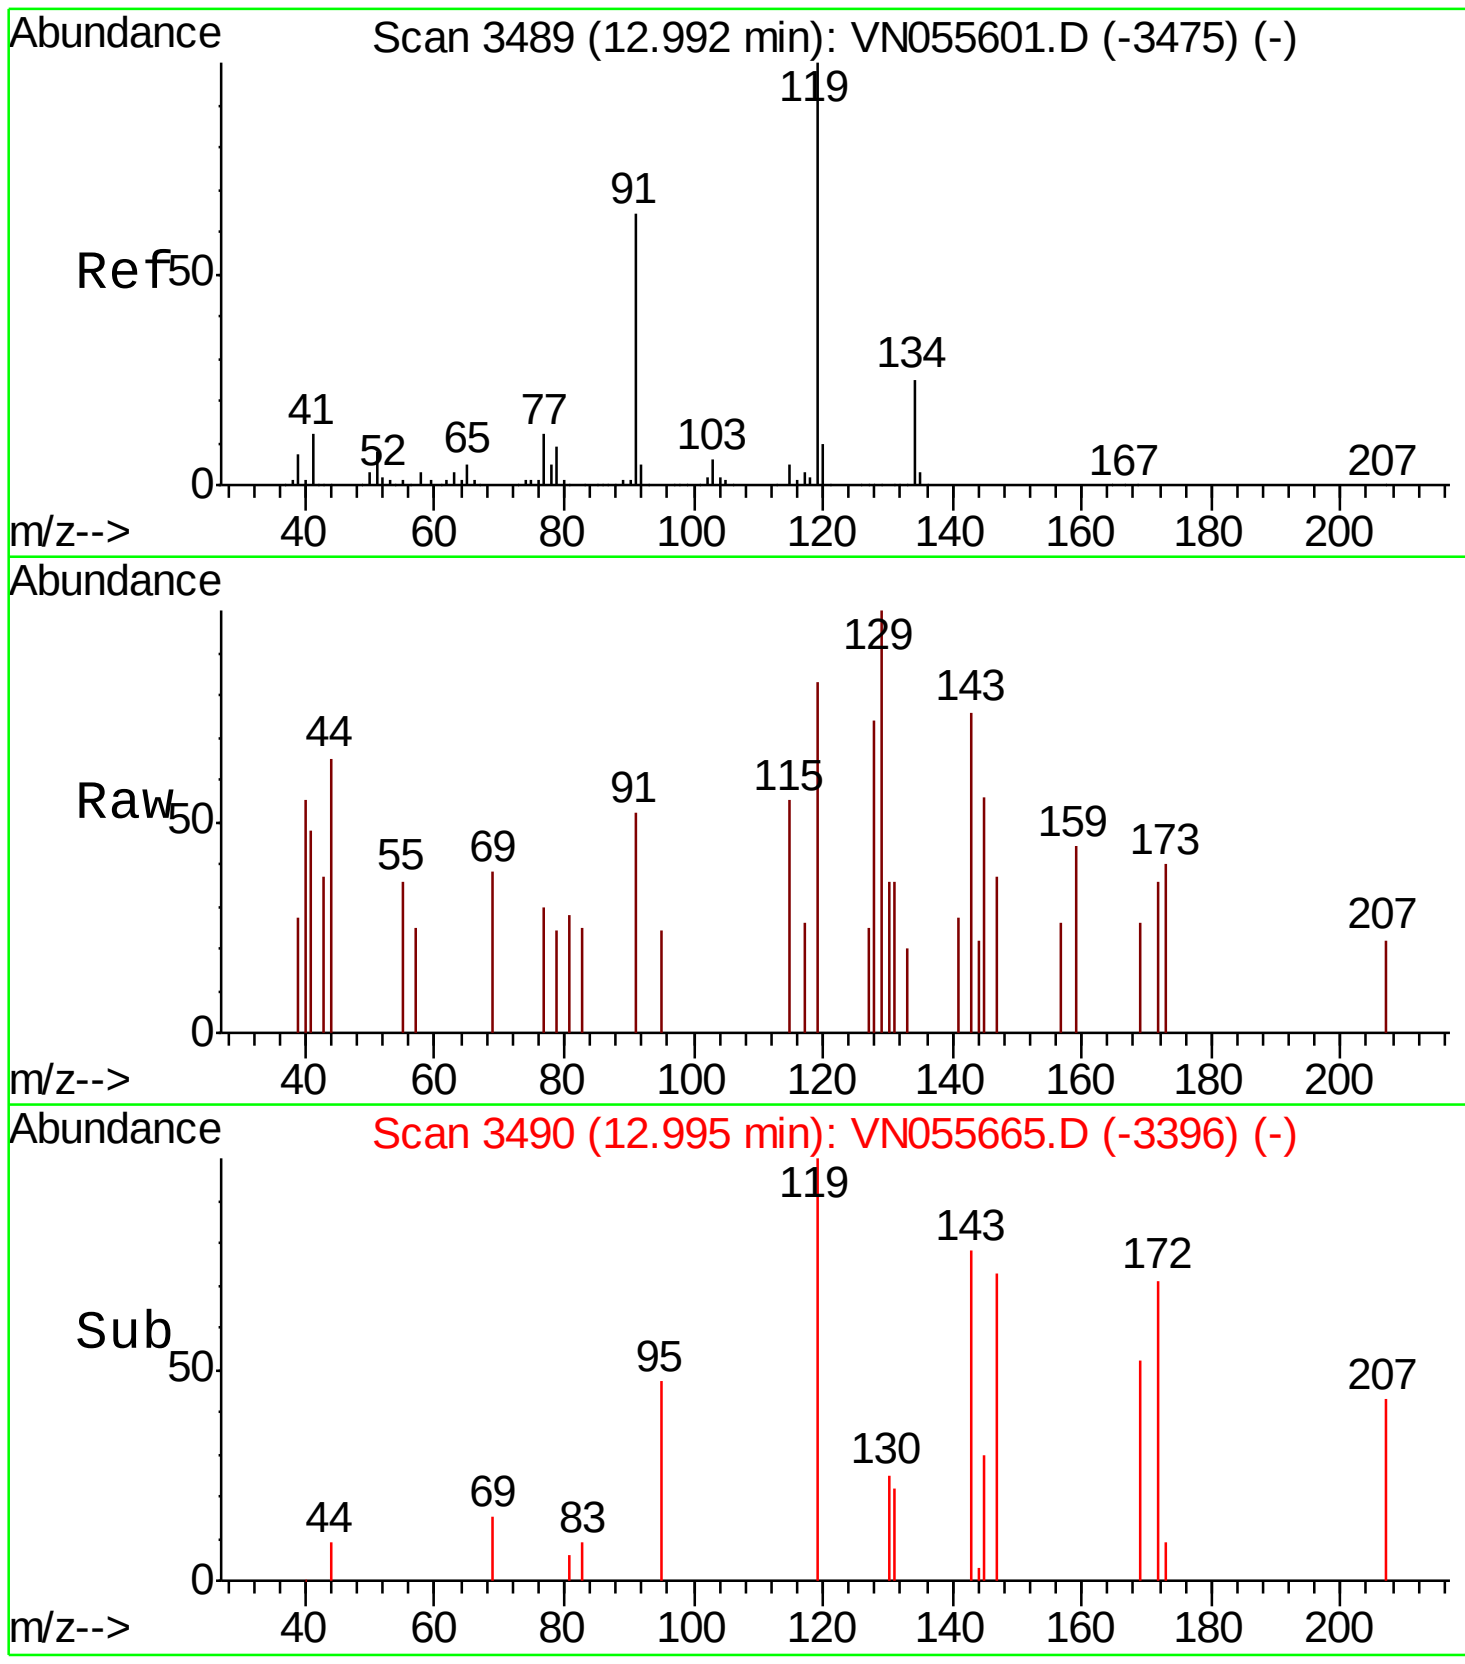

#83
tert-Butylbenzene
Concen: Below Cal
RT: 12.99 min Scan# 3490
Delta R.T. 0.00 min
Lab File: VN055665.D
Acq: 20 May 2019 11:37

Tgt Ion:119 Resp: 879

Ion	Ratio	Lower	Upper
119	100		
91	38.2	31.3	93.8
134	7.3	13.2	39.6#



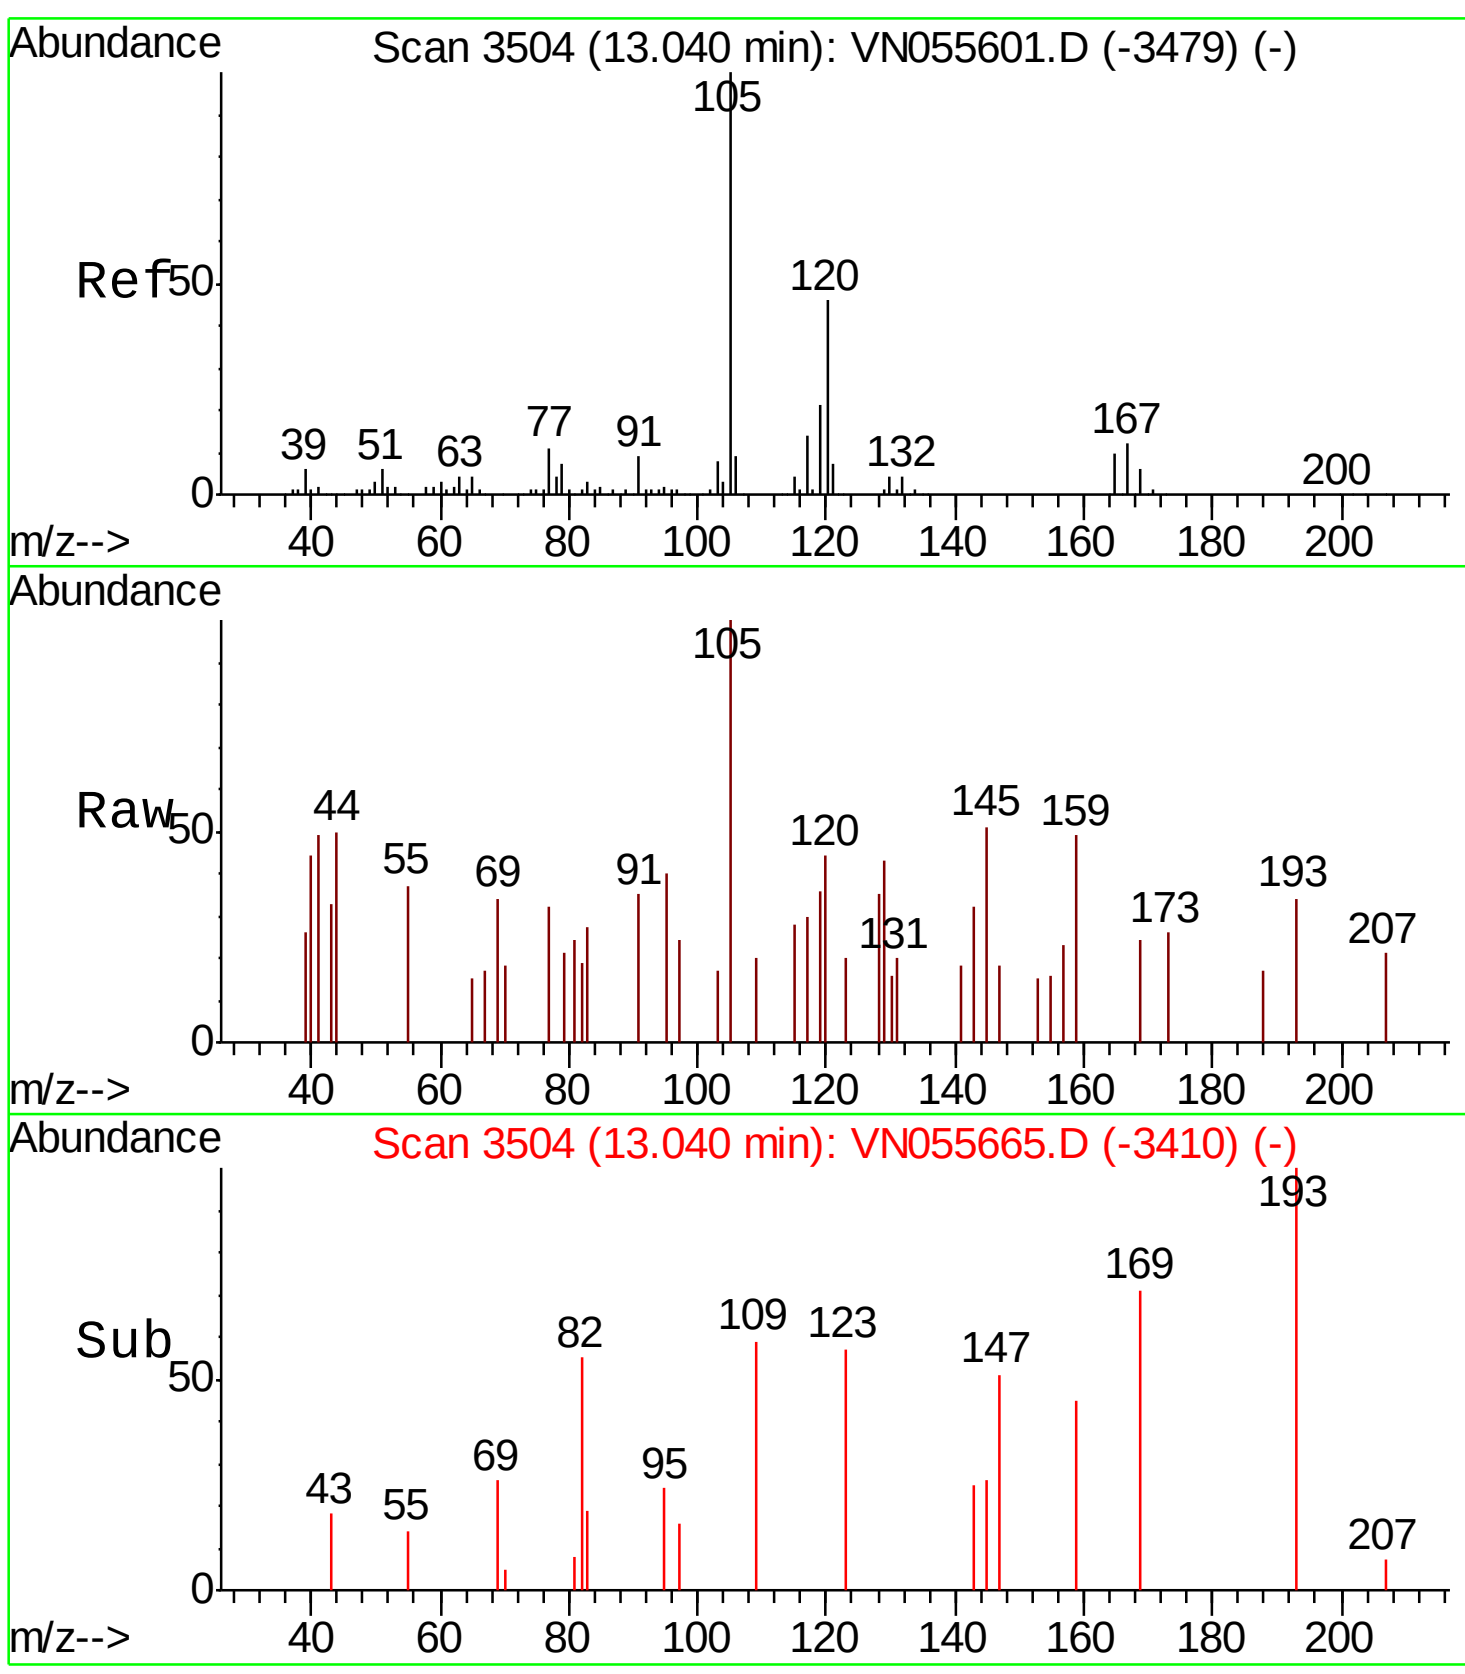

#84
1,2,4-Trimethylbenzene
Concen: Below Cal
RT: 13.04 min Scan# 3504
Delta R.T. 0.00 min
Lab File: VN055665.D
Acq: 20 May 2019 11:37

Tgt Ion:105 Resp: 2405

Ion	Ratio	Lower	Upper
105	100		
120	28.1	23.1	69.2



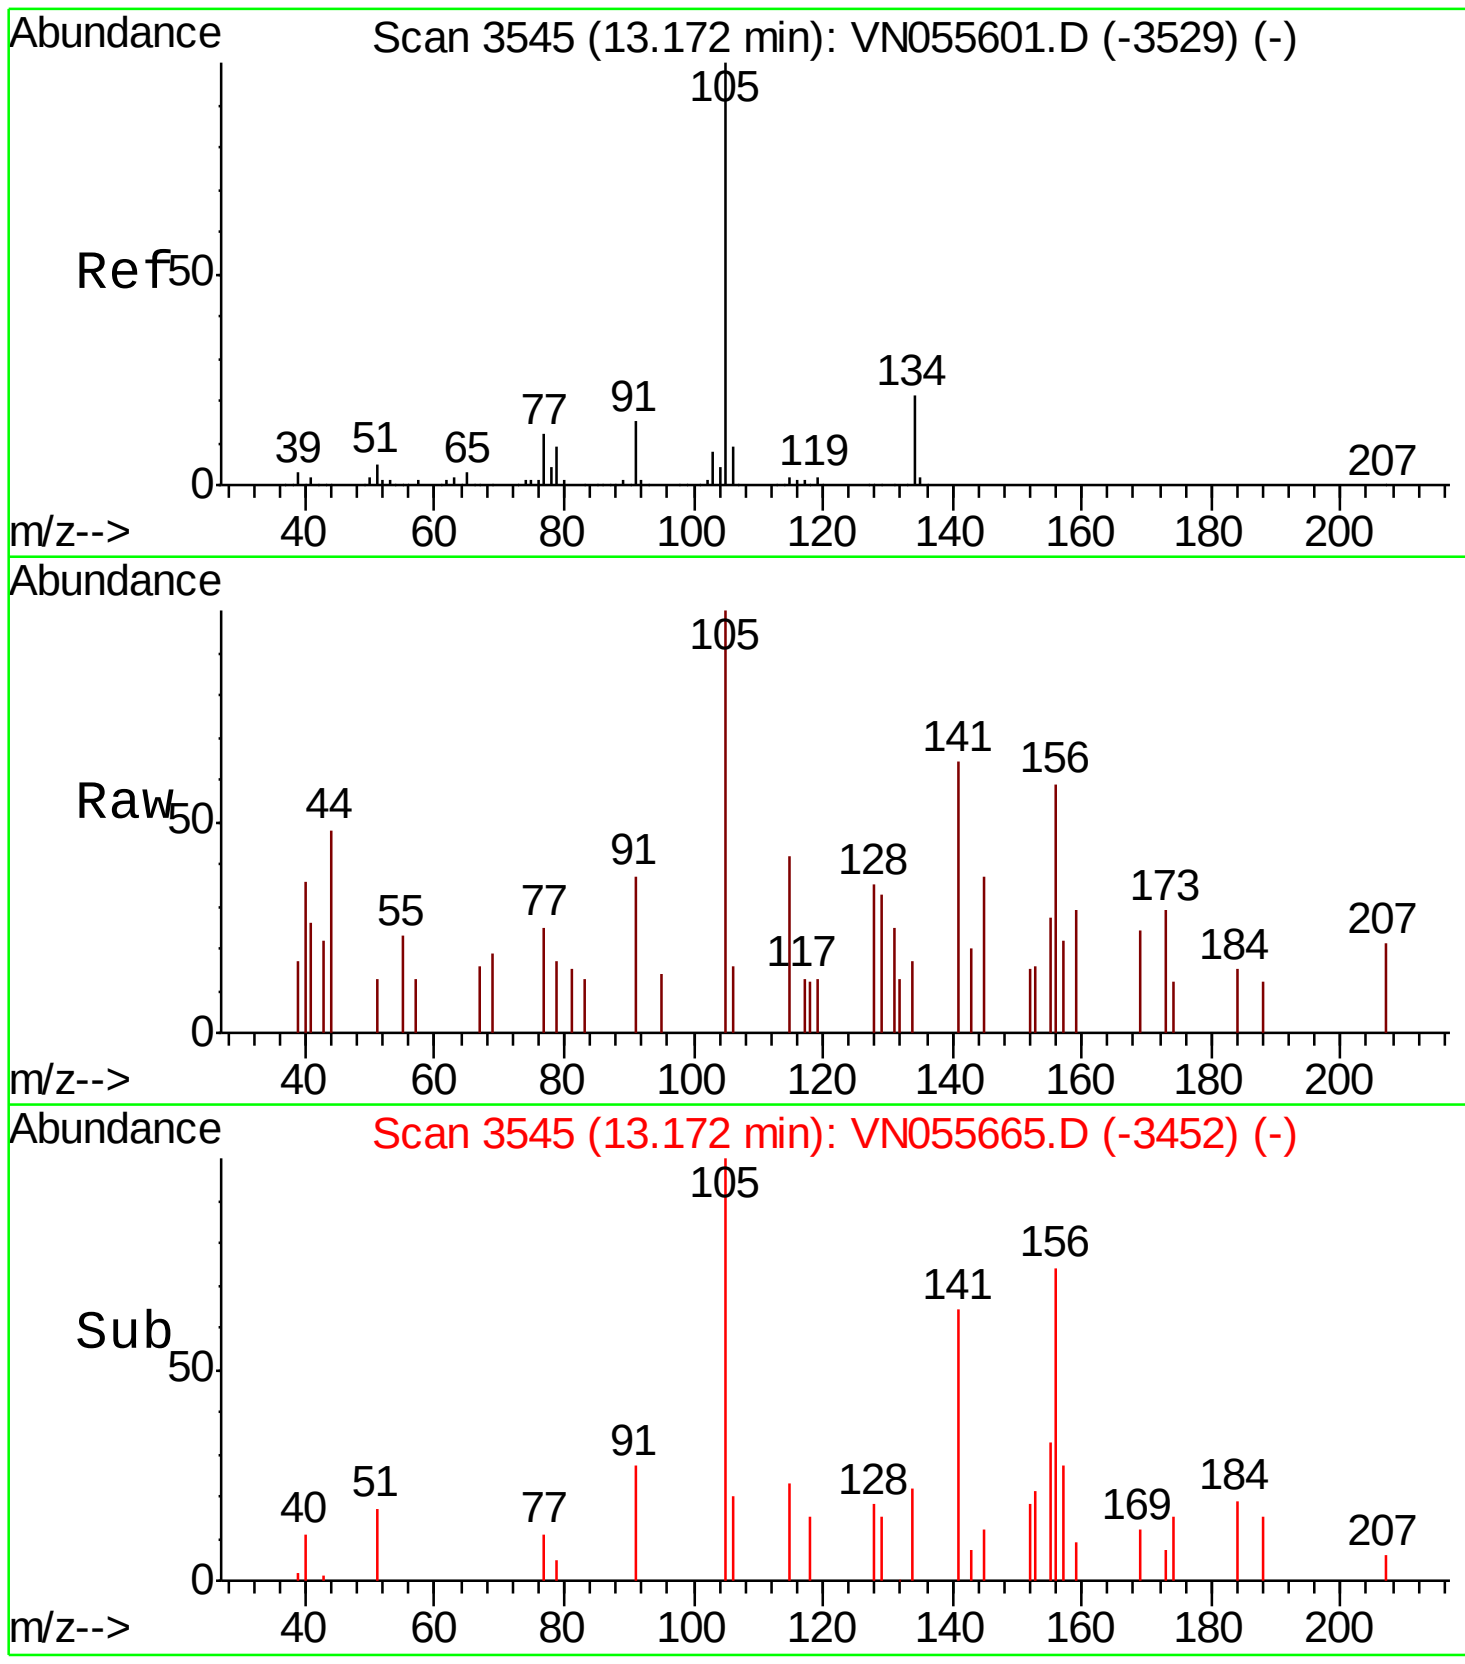

#85
sec-Butylbenzene
Concen: Below Cal
RT: 13.17 min Scan# 3545
Delta R.T. 0.00 min
Lab File: VN055665.D
Acq: 20 May 2019 11:37

Tgt Ion:105 Resp: 1516

Ion	Ratio	Lower	Upper
105	100		
134	21.6	10.3	30.9



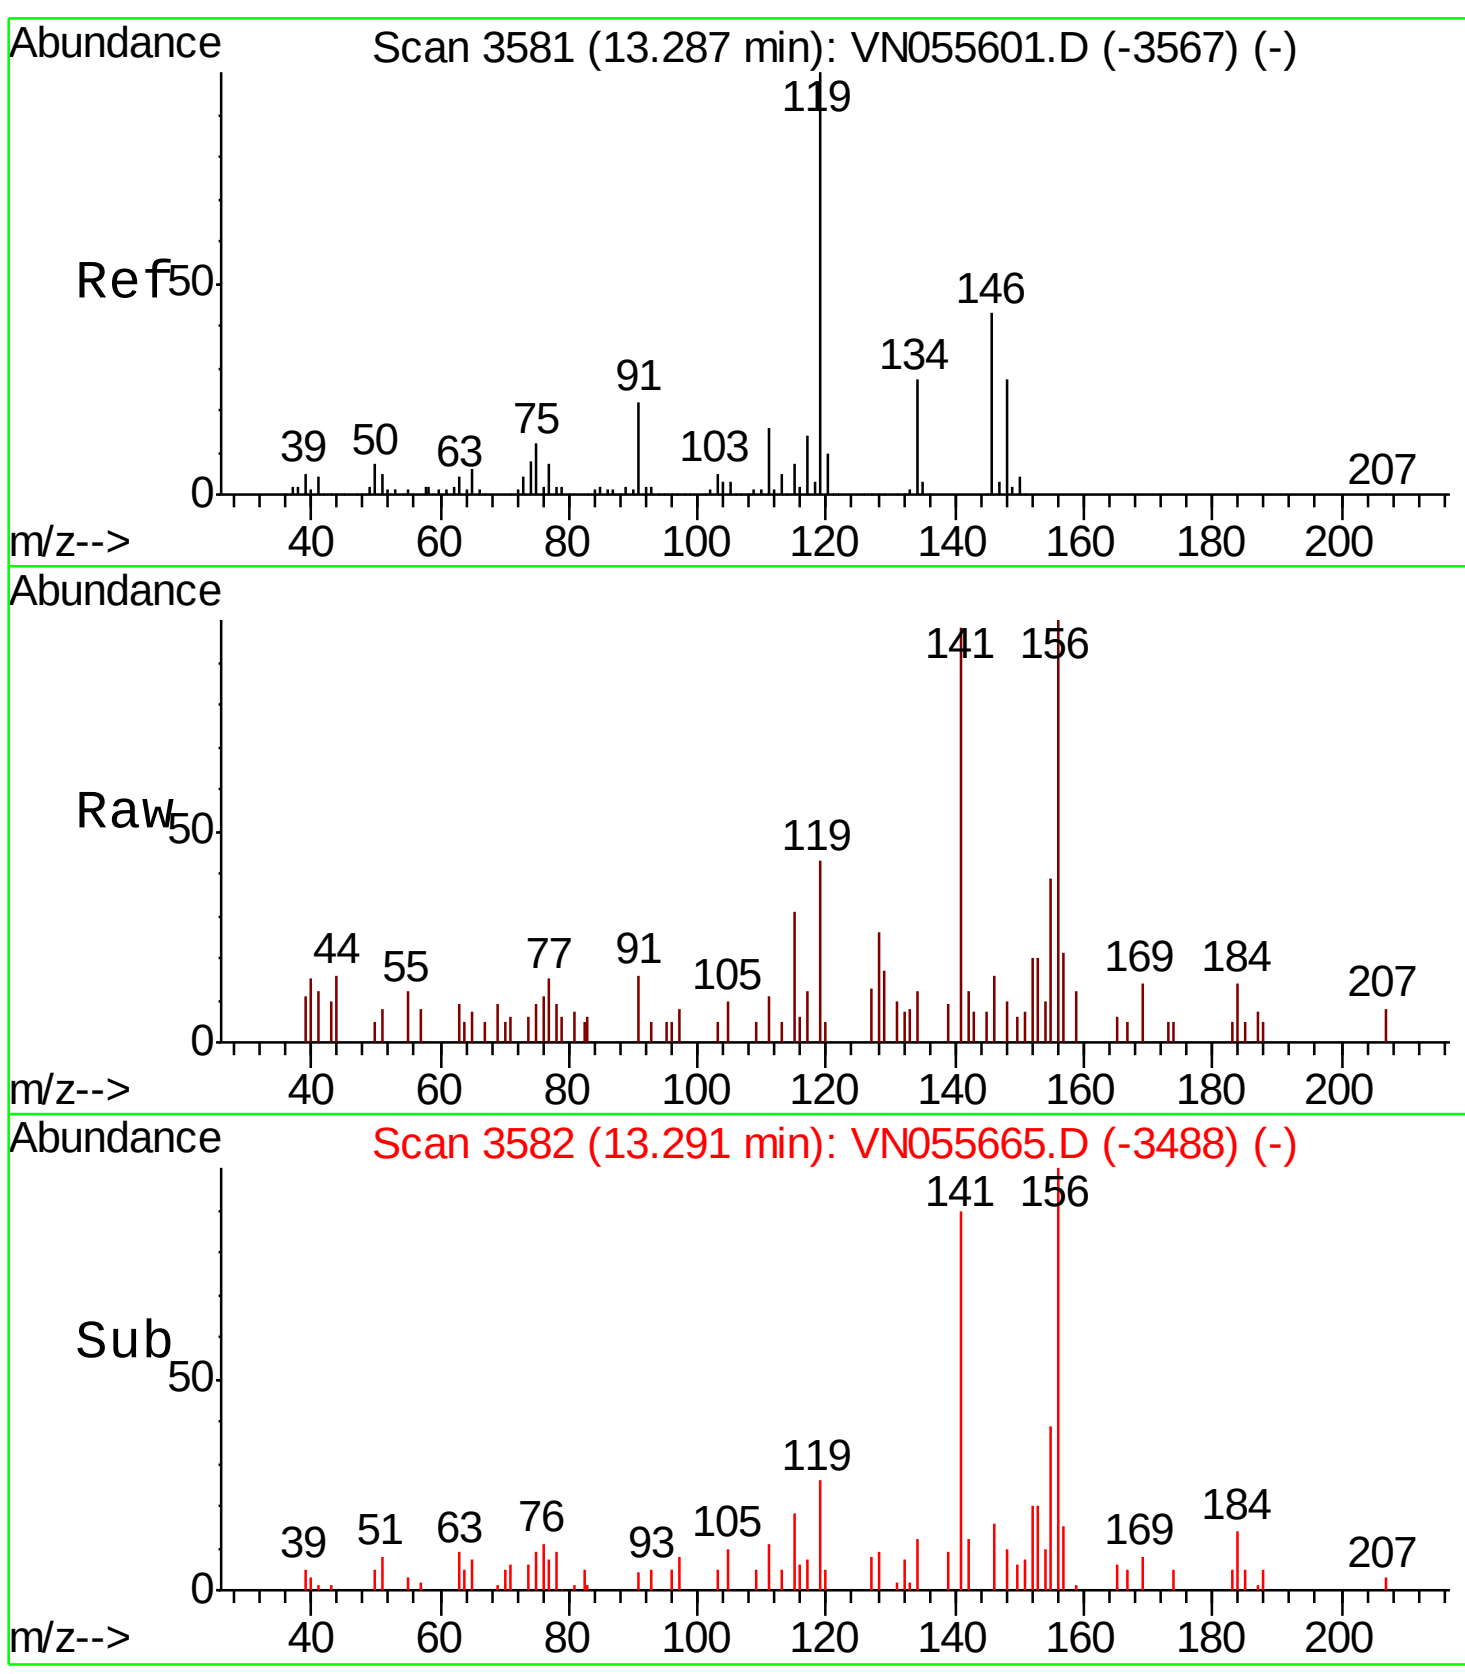

#86
p-Isopropyltoluene
Concen: Below Cal
RT: 13.29 min Scan# 3582
Delta R.T. 0.00 min
Lab File: VN055665.D
Acq: 20 May 2019 11:37

Tgt Ion:119 Resp: 1617

Ion	Ratio	Lower	Upper
119	100		
134	33.2	13.4	40.2
91	28.8	11.0	33.0



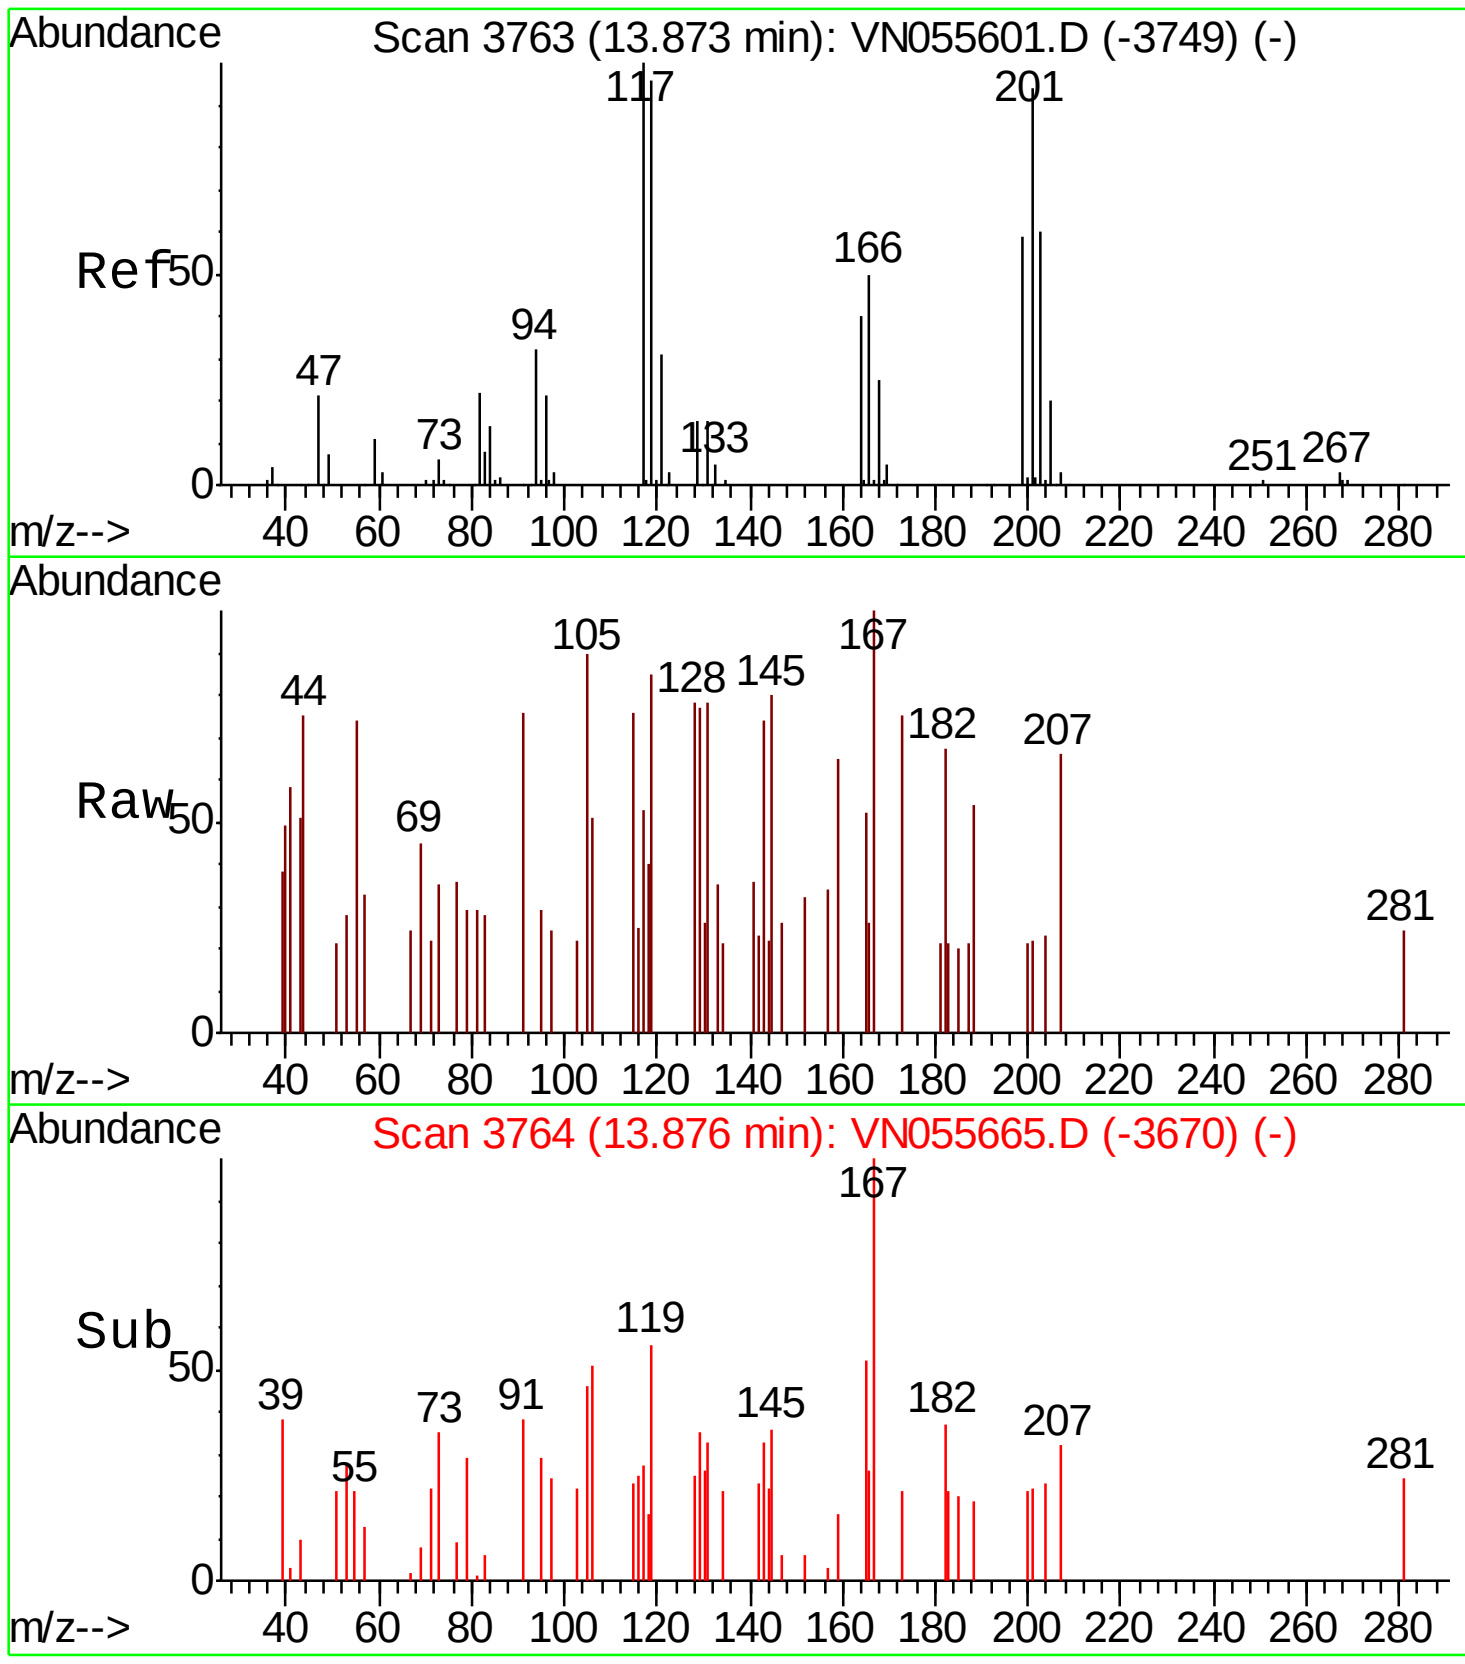

#90
Hexachloroethane
Concen: Below Cal
RT: 13.88 min Scan# 3764
Delta R.T. 0.00 min
Lab File: VN055665.D
Acq: 20 May 2019 11:37

Tgt Ion:117 Resp: 168

Ion	Ratio	Lower	Upper
117	100		
201	54.2	47.1	141.3



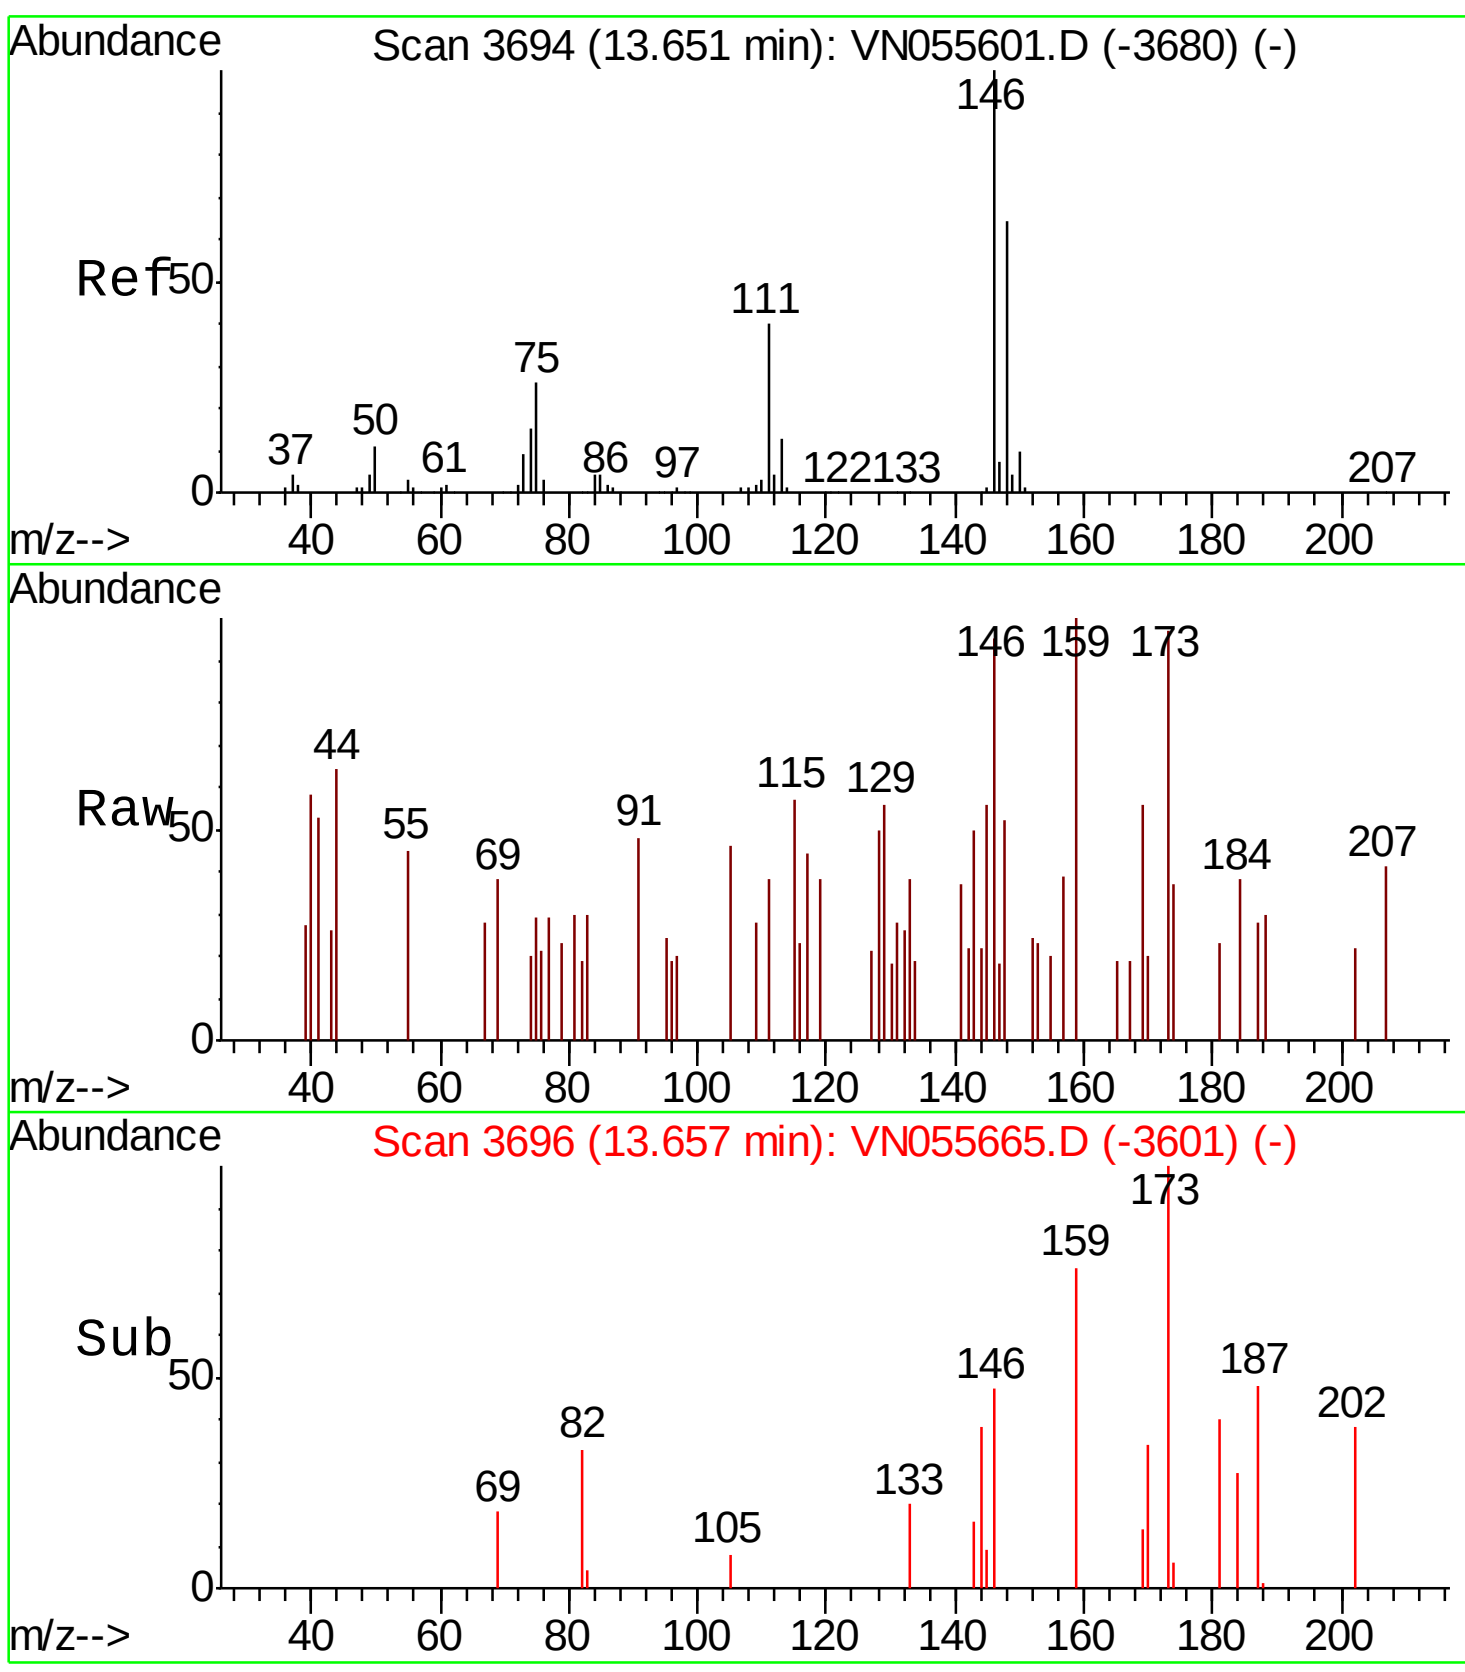

#91
1,2-Dichlorobenzene
Concen: 0.216 ug/l
RT: 13.66 min Scan# 3696
Delta R.T. 0.01 min
Lab File: VN055665.D
Acq: 20 May 2019 11:37

Tgt Ion:146 Resp: 1587

Ion	Ratio	Lower	Upper
146	100		
111	33.5	19.7	59.0
148	44.4	32.1	96.3



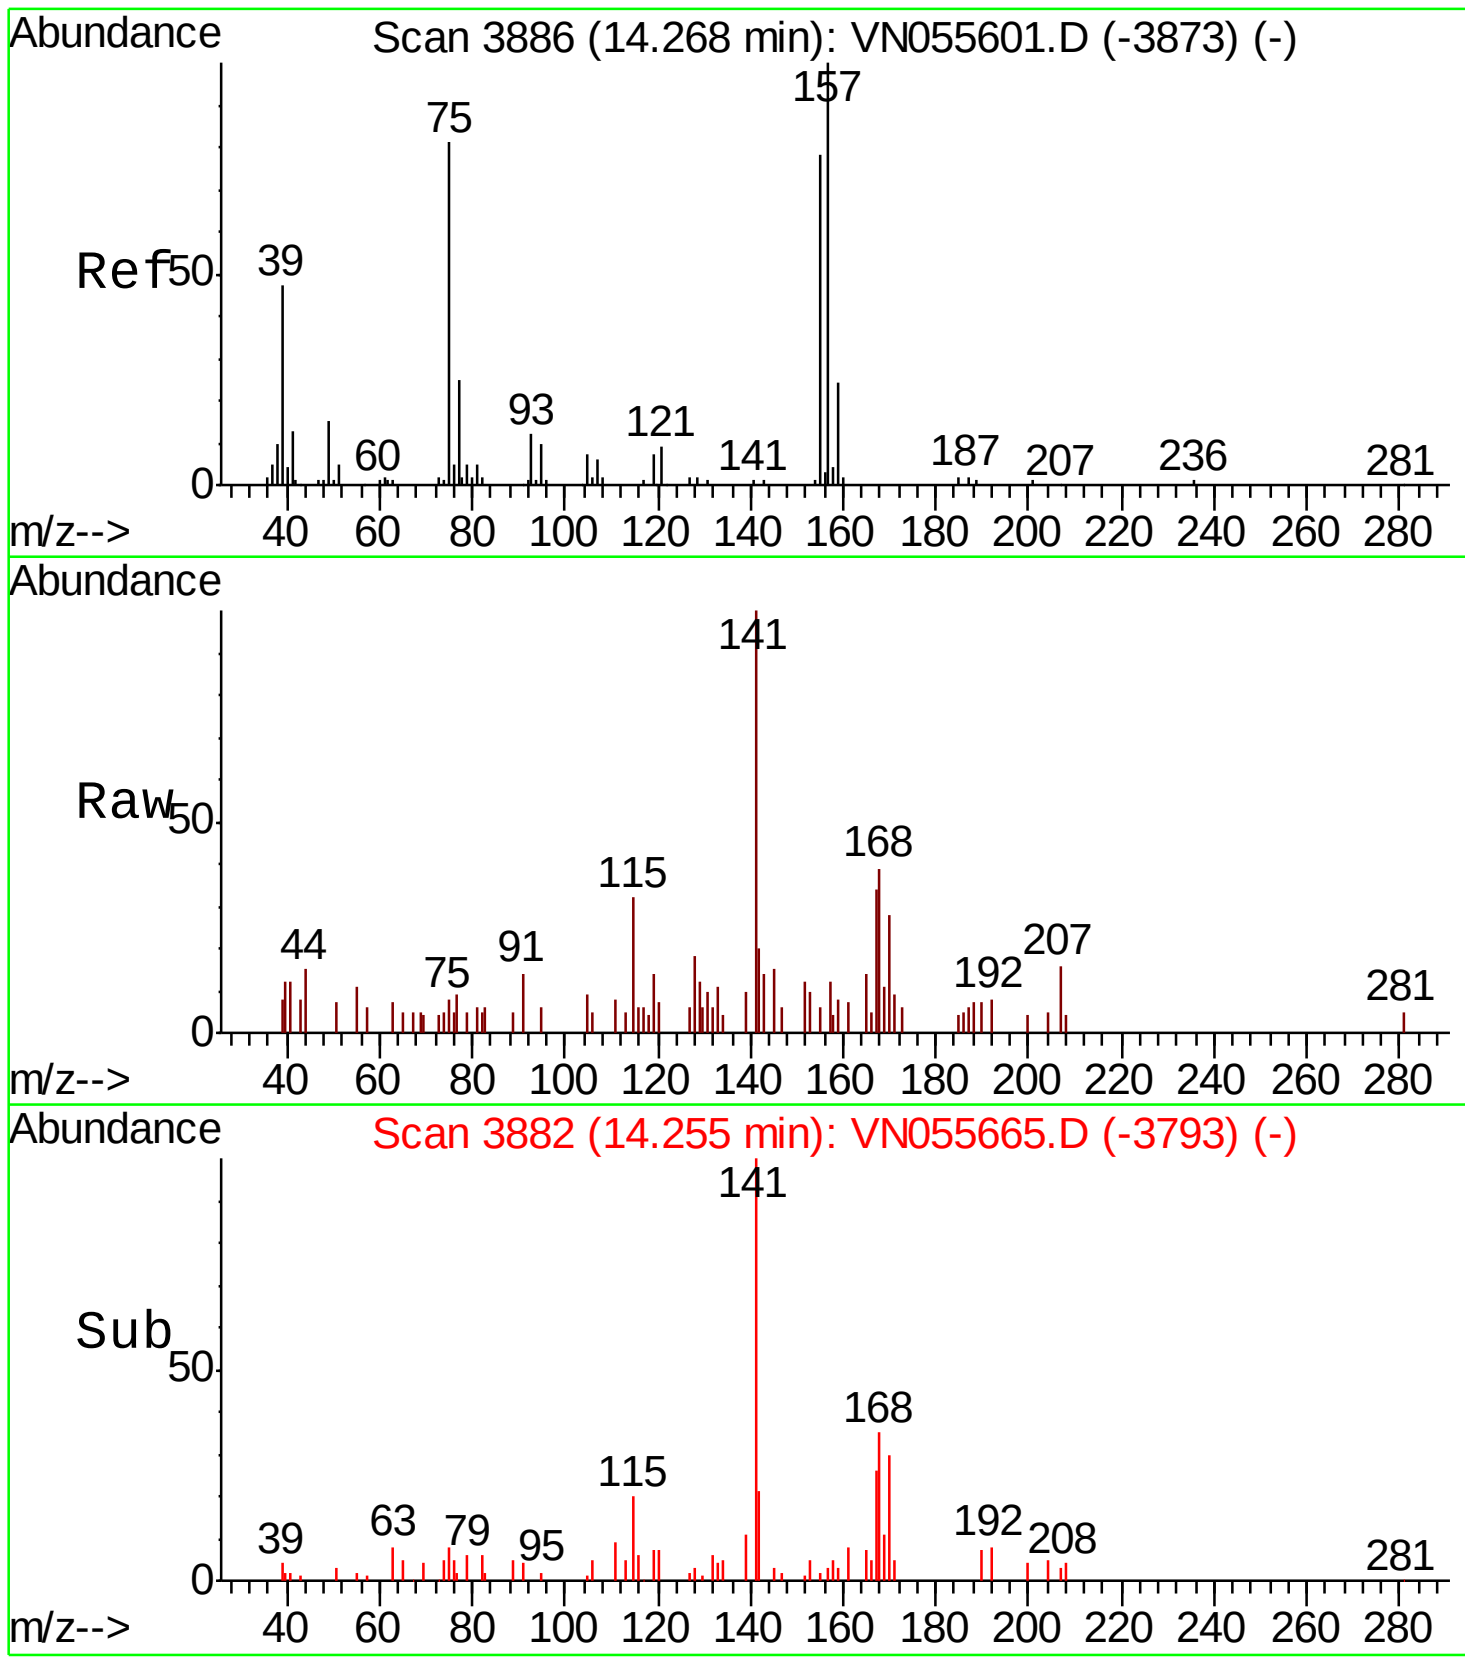

#92
1,2-Dibromo-3-Chloropropane
Concen: 0.417 ug/l
RT: 14.26 min   Scan# 3882
Delta R.T.   -0.01 min
Lab File: VN055665.D
Acq: 20 May 2019   11:37

Tgt Ion: 75 Resp: 411

Ion	Ratio	Lower	Upper
75	100		
155	0.0	48.4	145.0#
157	104.6	62.3	186.8



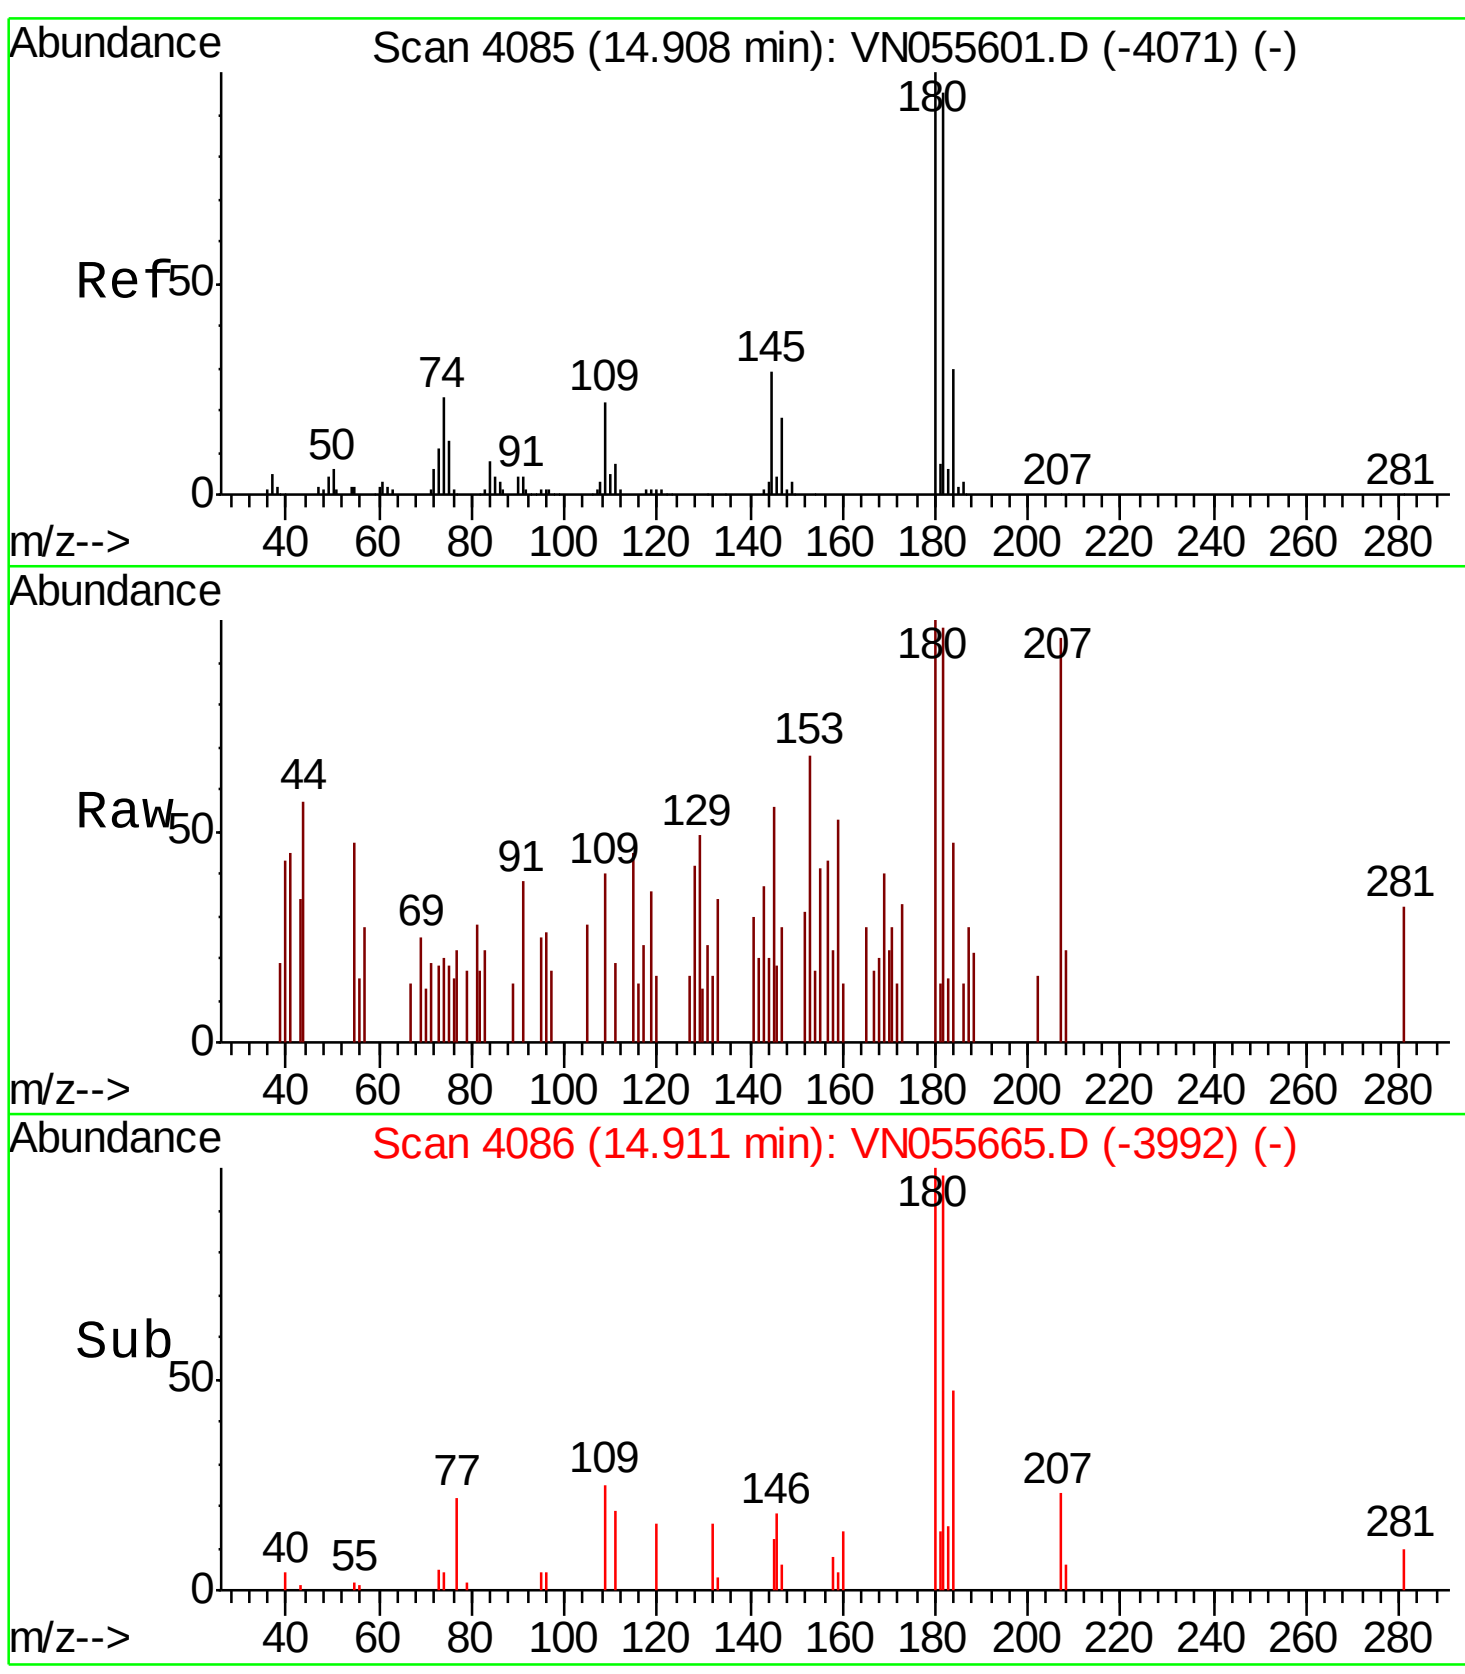

#93
1,2,4-Trichlorobenzene
Concen: 0.531 ug/l
RT: 14.91 min   Scan# 4086
Delta R.T.   0.00 min
Lab File: VN055665.D
Acq: 20 May 2019   11:37

Tgt Ion:180 Resp: 1989

Ion	Ratio	Lower	Upper
180	100		
182	103.3	47.9	143.6
145	0.0	14.3	42.9#



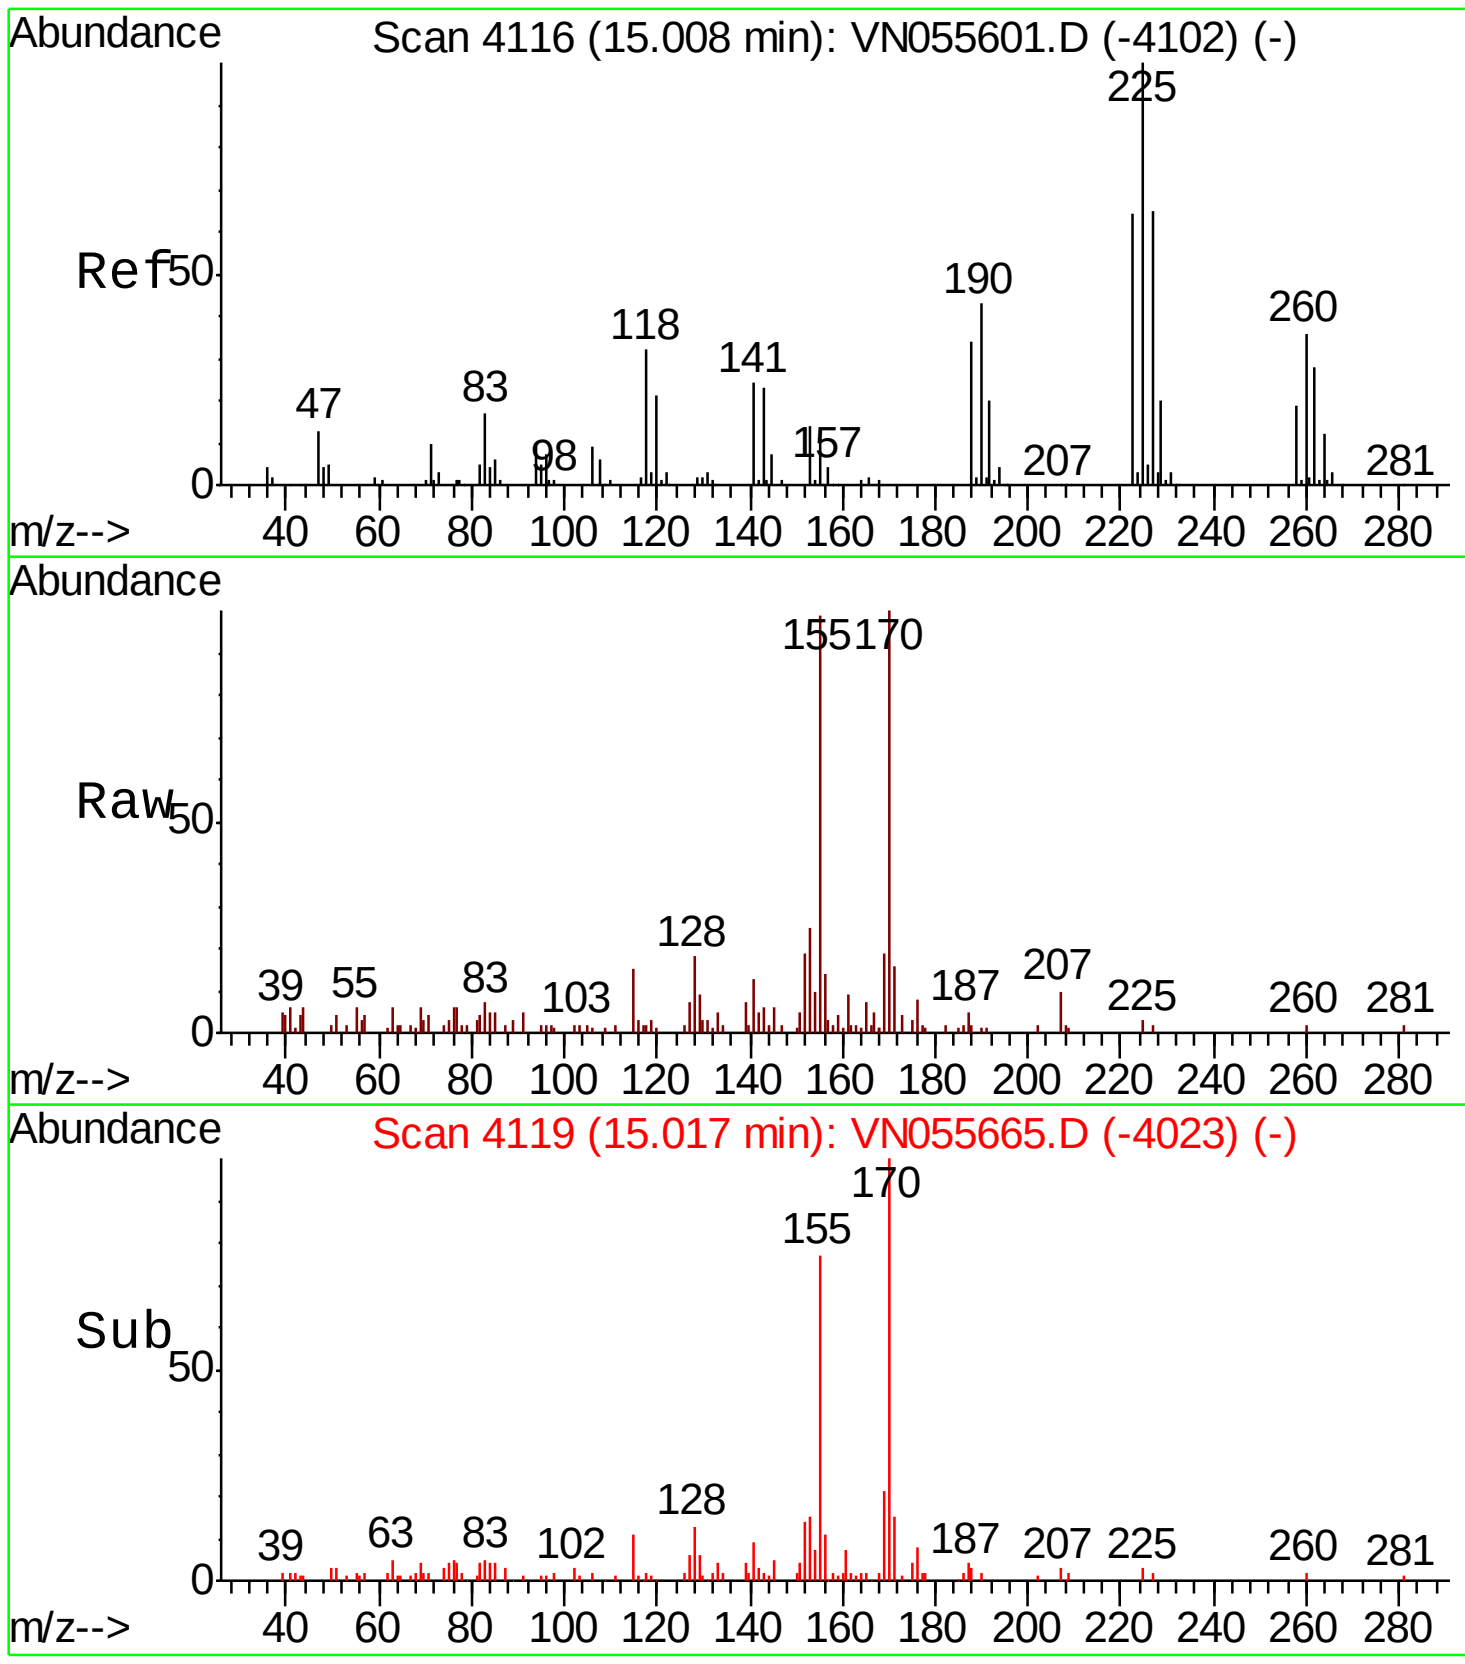

#94
Hexachlorobutadiene
Concen: Below Cal
RT: 15.02 min Scan# 4119
Delta R.T. 0.01 min
Lab File: VN055665.D
Acq: 20 May 2019 11:37

Tgt Ion:225	Resp:		537
Ion	Ratio	Lower	Upper
225	100		
223	38.7	31.6	94.7
227	55.1	32.4	97.0



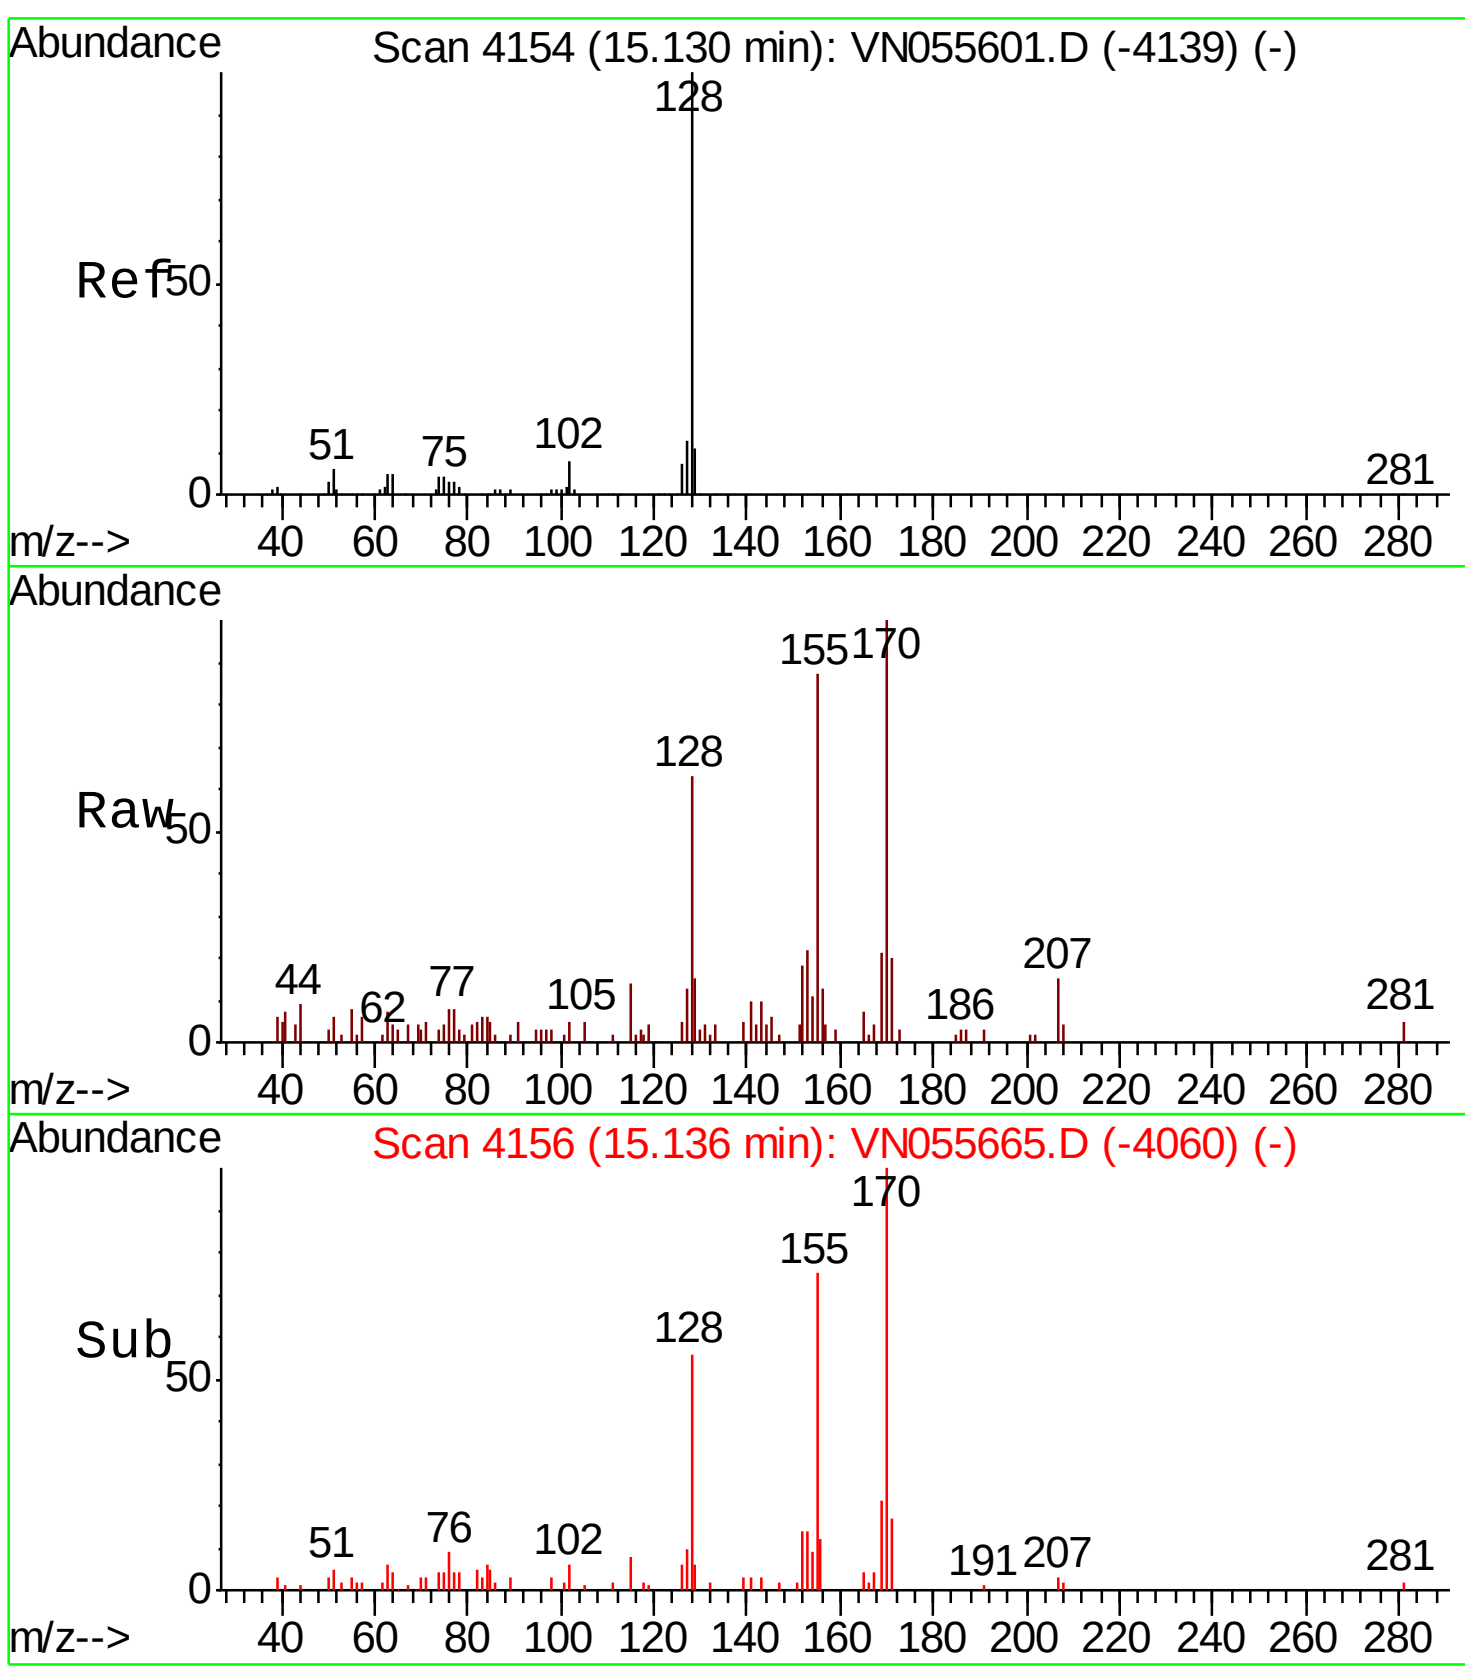

#95
Naphthalene
Concen: 2.758 ug/l
RT: 15.14 min Scan# 4156
Delta R.T. 0.01 min
Lab File: VN055665.D
Acq: 20 May 2019 11:37

Tgt Ion:128	Resp:		11648
Ion	Ratio	Lower	Upper
128	100		
127	12.1	10.2	15.4
129	21.4	8.6	12.8#



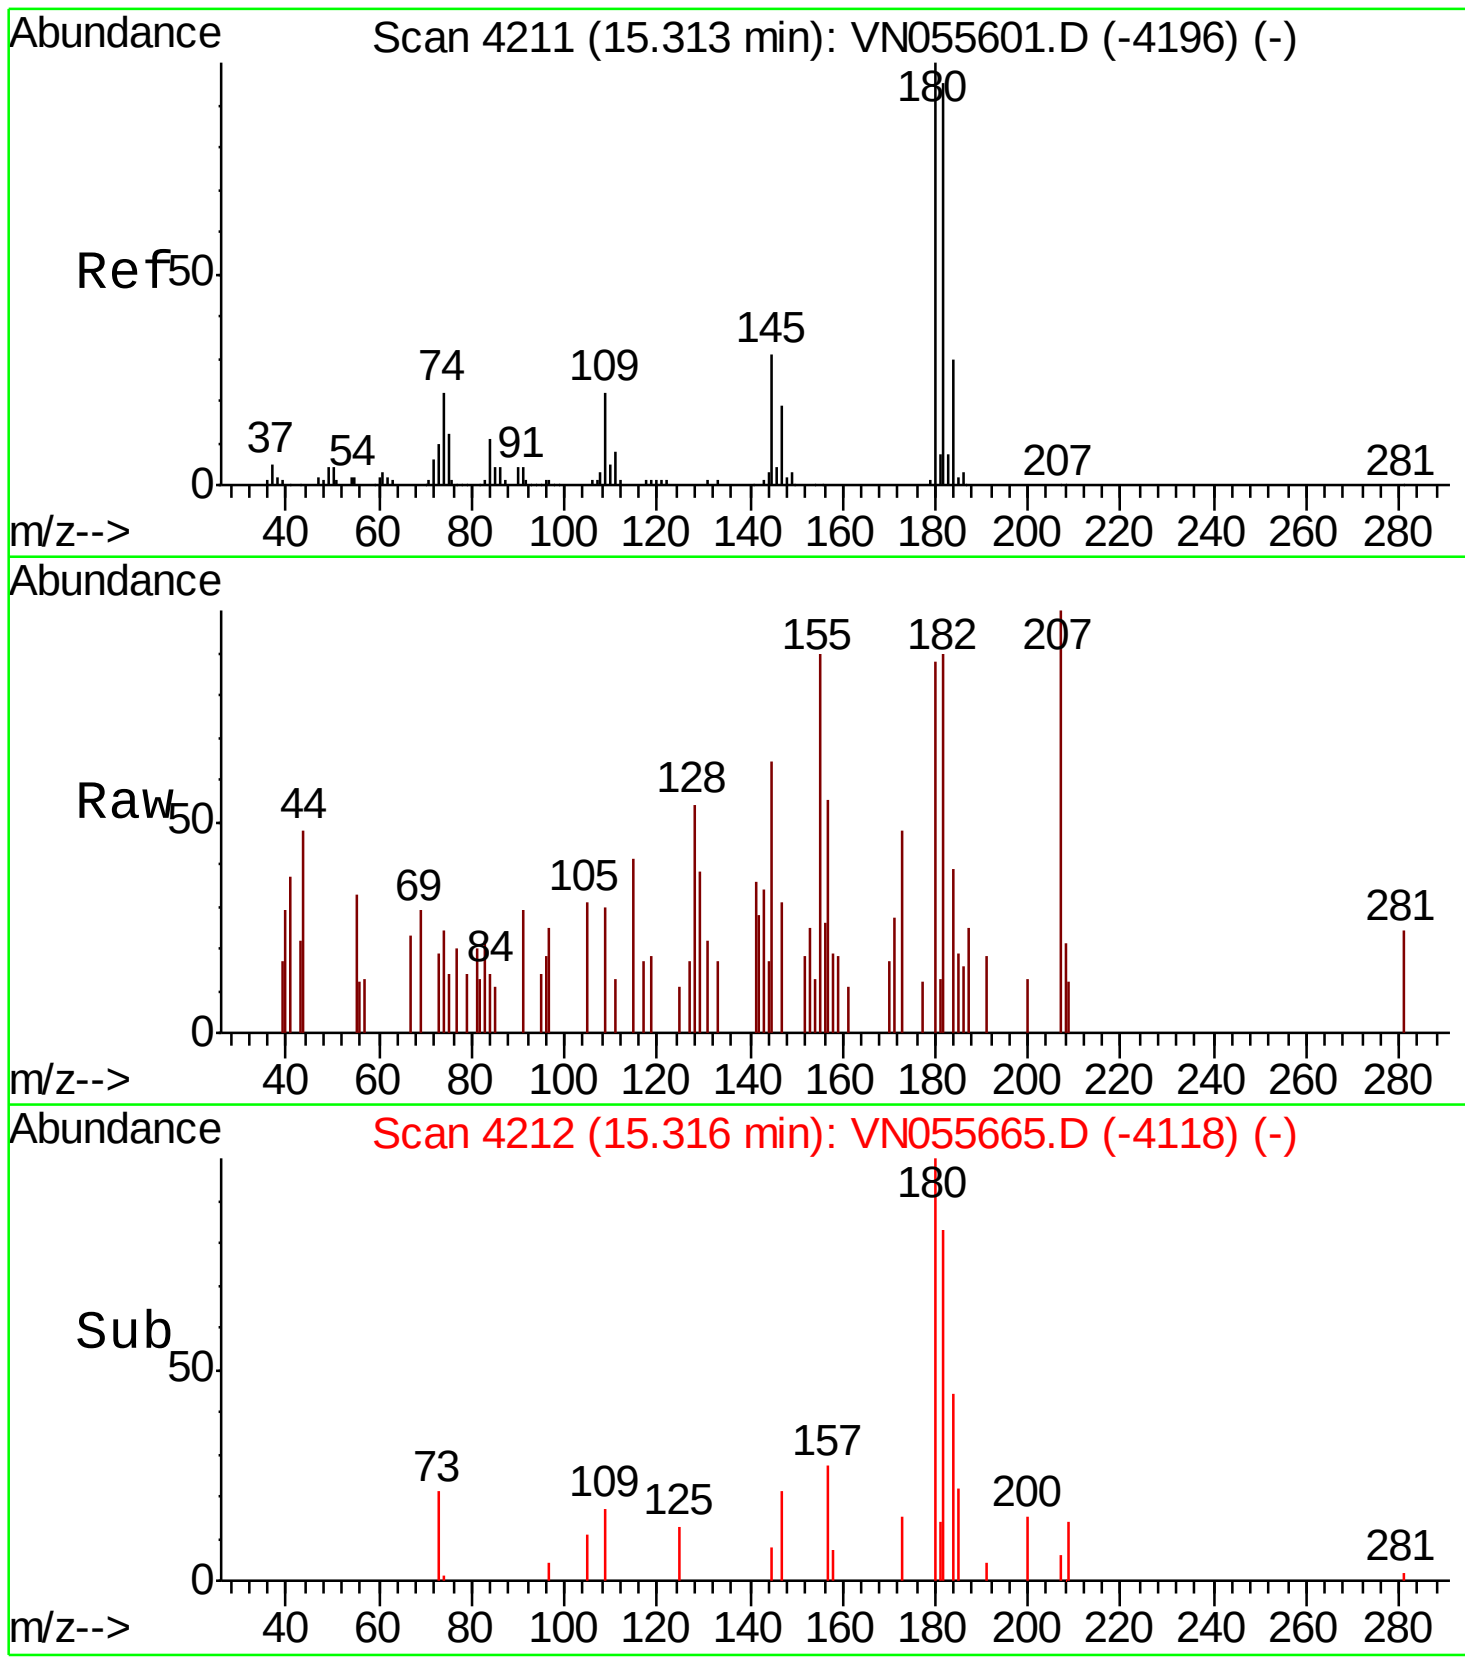

#96
1,2,3-Trichlorobenzene
Concen: 0.540 ug/l
RT: 15.32 min Scan# 4212
Delta R.T. 0.00 min
Lab File: VN055665.D
Acq: 20 May 2019 11:37

Tgt Ion:180 Resp: 2117

Ion	Ratio	Lower	Upper
180	100		
182	95.2	47.9	143.6
145	55.4	15.4	46.1#