


Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN052019\
Data File : VN055687.D
Acq On : 20 May 2019 22:13
Operator : JC/SP
Sample : BFB
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 31 Sample Multiplier: 1

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N051719W.M
Title : SW846 8260
Last Update : Fri May 17 23:54:12 2019

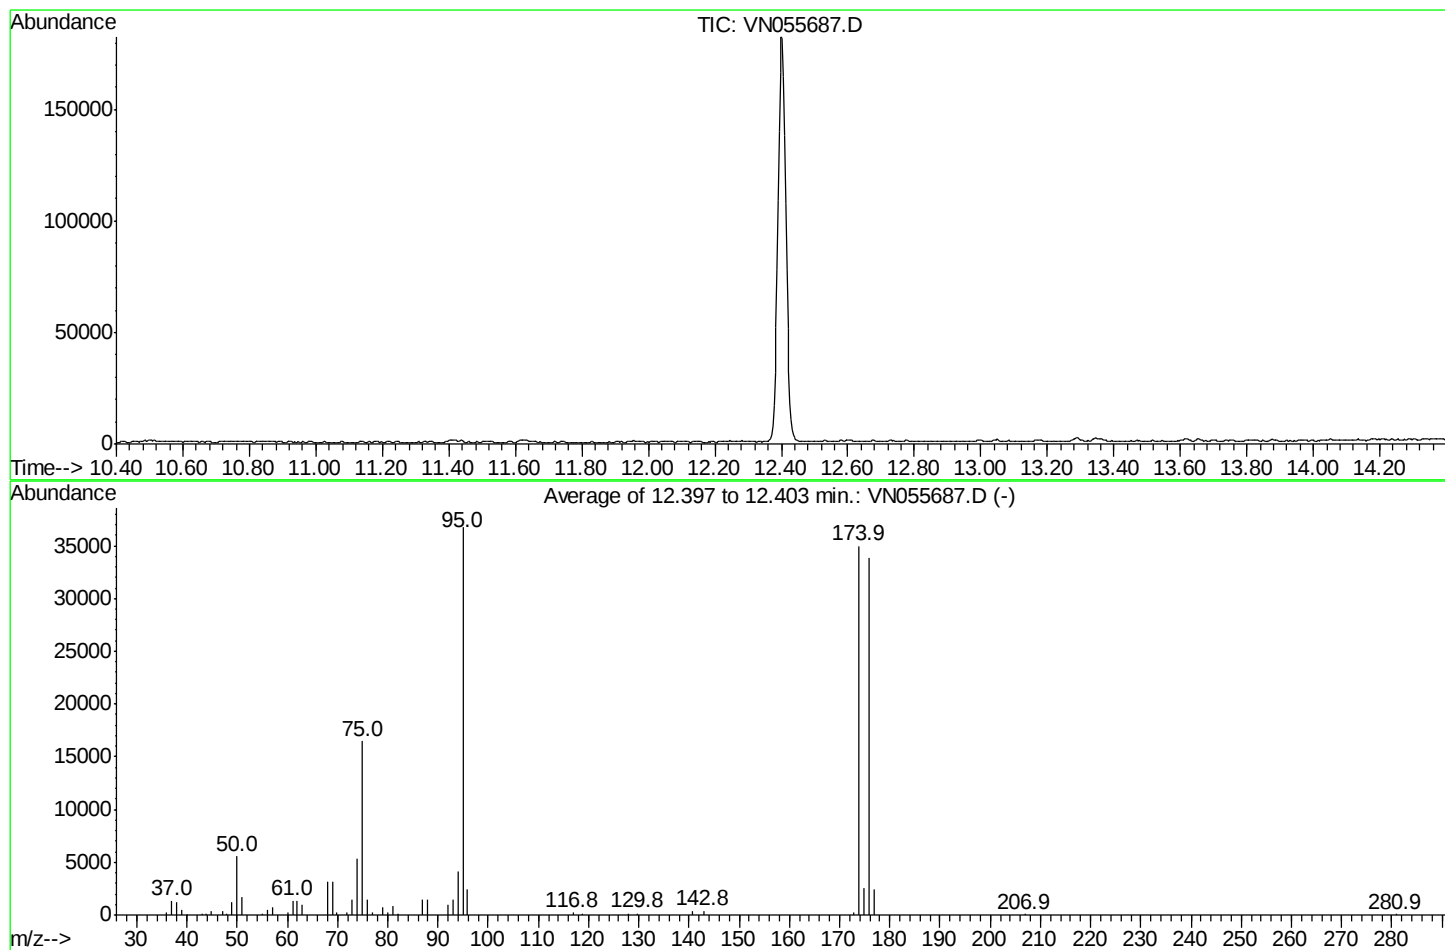

AutoFind: Scans 3304, 3305, 3306; Background Corrected with Scan 3291

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.2	5577	PASS
75	95	30	60	44.8	16453	PASS
95	95	100	100	100.0	36746	PASS
96	95	5	9	6.8	2491	PASS
173	174	0.00	2	0.7	231	PASS
174	95	50	100	95.2	34981	PASS
175	174	5	9	7.4	2603	PASS
176	174	95	101	96.7	33834	PASS
177	176	5	9	7.0	2373	PASS