
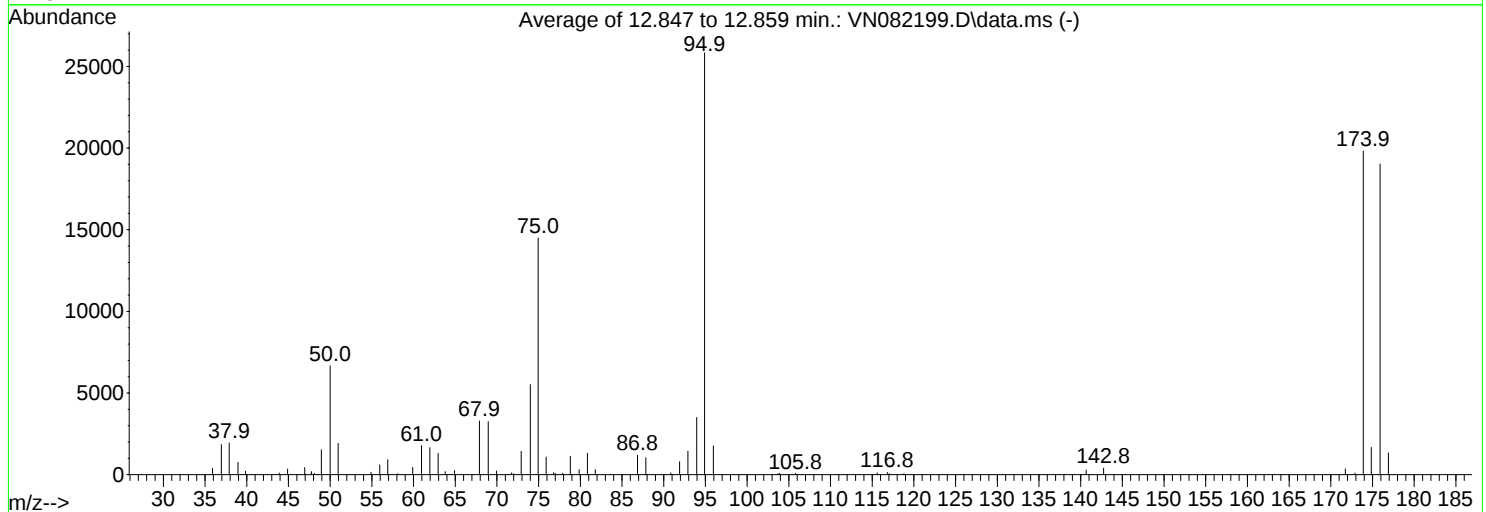


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN052024\
Data File : VN082199.D
Acq On : 20 May 2024 10:27
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N051524W.M
Title : SW846 8260
Last Update : Thu May 16 05:21:06 2024

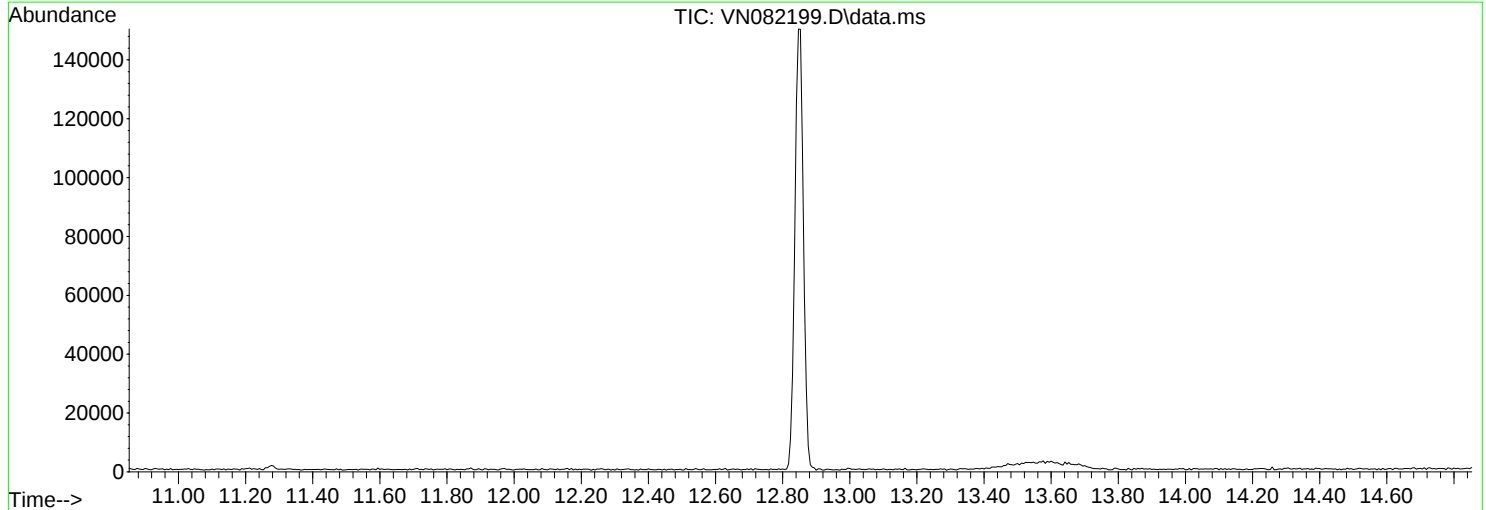

AutoFind: Scans 1852, 1853, 1854; Background Corrected with Scan 1844

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	25.7	6651	PASS
75	95	30	60	56.1	14497	PASS
95	95	100	100	100.0	25835	PASS
96	95	5	9	6.8	1759	PASS
173	174	0.00	2	0.5	96	PASS
174	95	50	100	76.7	19816	PASS
175	174	5	9	8.4	1669	PASS
176	174	95	101	96.0	19029	PASS
177	176	5	9	7.0	1334	PASS

Average of 12.847 to 12.859 min.: VN082199.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.90	387	50.00	6651	64.90	245	77.00	61
36.95	1842	50.95	1913	67.90	3280	77.90	81
37.90	1936	54.90	145	68.95	3254	78.80	112
38.95	752	55.95	598	69.95	226	79.85	30
39.85	210	56.90	908	71.75	113	80.85	1306
43.90	95	58.10	55	72.00	56	81.80	316
44.90	345	59.90	437	72.90	1433	86.85	1185
46.95	427	60.95	1775	74.00	5520	87.85	1042
47.75	191	61.95	1658	74.95	14497	90.85	113
48.10	77	62.95	1307	75.90	1079	91.90	798
48.95	1534	63.80	186	76.80	125	92.90	1438

Average of 12.847 to 12.859 min.: VN082199.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
93.95	3495	142.75	400				
94.90	25835	171.75	357				
95.95	1759	172.90	96				
103.70	69	173.90	19816				
103.90	66	174.85	1669				
105.80	76	175.90	19029				
115.60	108	176.90	1334				
116.80	140						
117.10	61						
118.80	55						
140.65	288						

Instrument :
MSVOA_N
ClientSampleId :
BFB