


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN052025\
Data File : VN086705.D
Acq On : 20 May 2025 09:32
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N051625W.M
Title : SW846 8260
Last Update : Sat May 17 00:46:13 2025

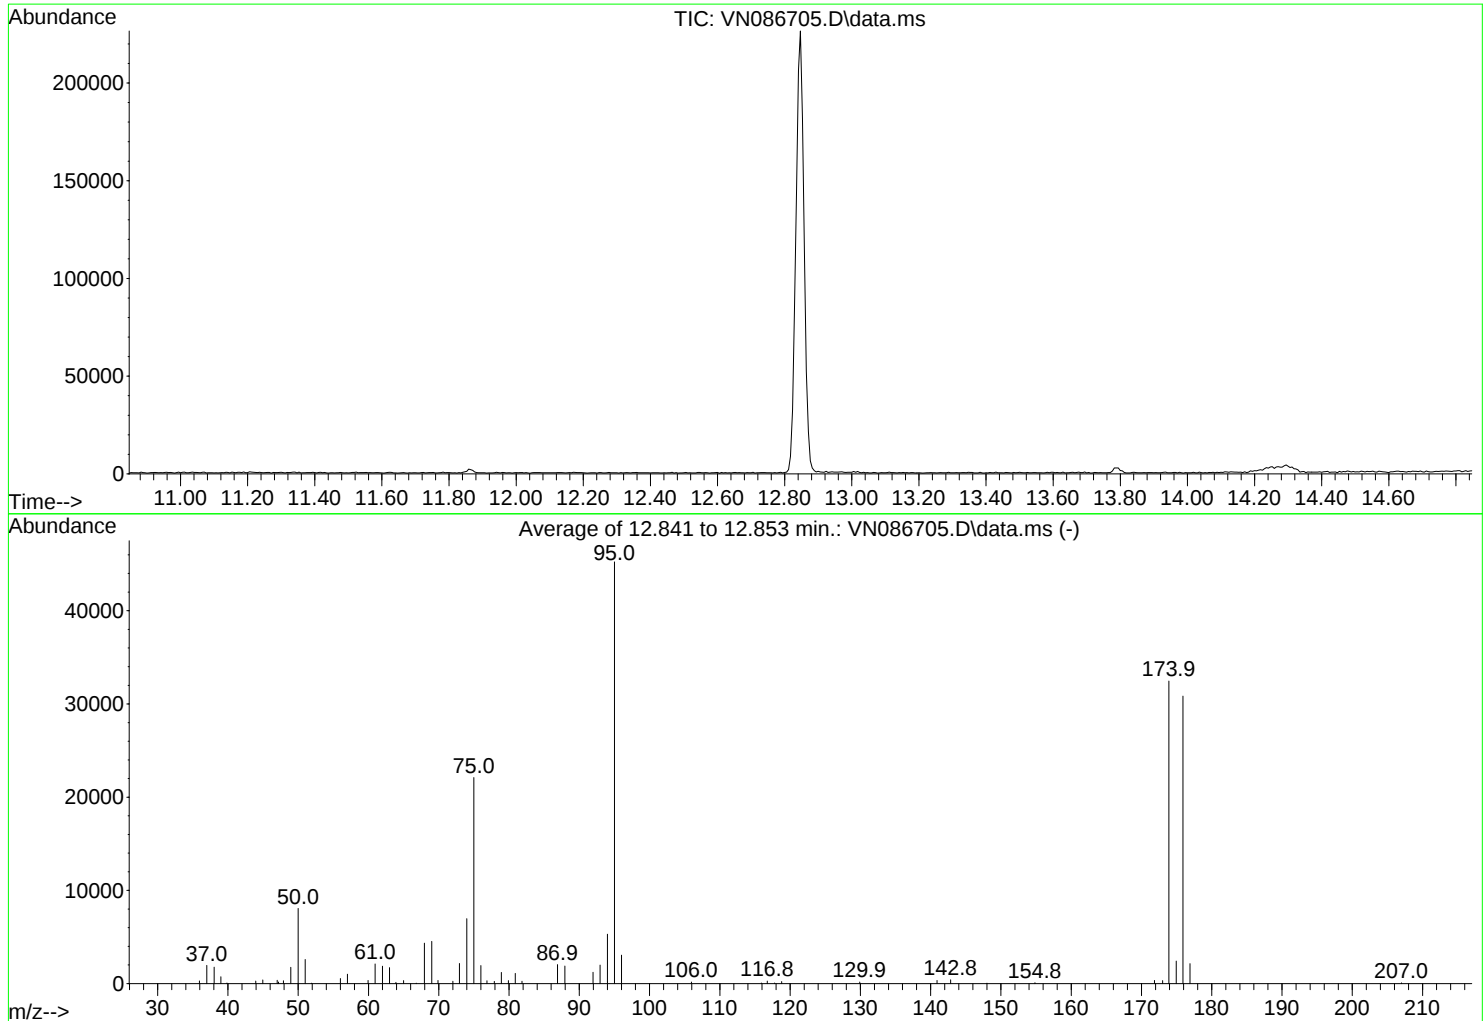

AutoFind: Scans 1851, 1852, 1853; Background Corrected with Scan 1843

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	17.8	8067	PASS
75	95	30	60	48.9	22107	PASS
95	95	100	100	100.0	45245	PASS
96	95	5	9	6.8	3064	PASS
173	174	0.00	2	1.0	327	PASS
174	95	50	100	71.7	32461	PASS
175	174	5	9	7.4	2416	PASS
176	174	95	101	95.0	30840	PASS
177	176	5	9	7.0	2155	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.95	284	50.00	8067	66.80	51	78.90	1201
37.00	1957	51.00	2595	67.95	4345	79.90	321
38.05	1777	51.90	59	69.00	4533	80.90	110
39.00	732	56.00	555	69.90	346	81.85	26
39.85	72	57.00	1007	72.00	262	86.90	2044
43.95	271	59.95	352	72.95	2168	87.95	1880
44.95	391	60.95	2121	74.00	6966	91.95	1218
47.00	358	62.00	1874	75.00	22107	92.95	1990
47.20	173	63.00	1715	76.00	1948	94.00	5311
47.90	304	63.90	137	76.85	316	95.00	45245
48.95	1757	65.00	329	77.90	234	96.00	3064

Average of 12.841 to 12.853 min.: VN086705.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
105.95	178	173.00	327				
115.90	63	173.90	32461				
116.75	274	174.95	2416				
117.80	66	175.90	30840				
118.80	226	176.90	2155				
129.90	166	207.00	83				
140.90	342						
142.85	410						
148.00	57						
154.85	111						
171.85	345						

Instrument :

MSVOA_N

ClientSampleId :

BFB