



1,4-Dioxane

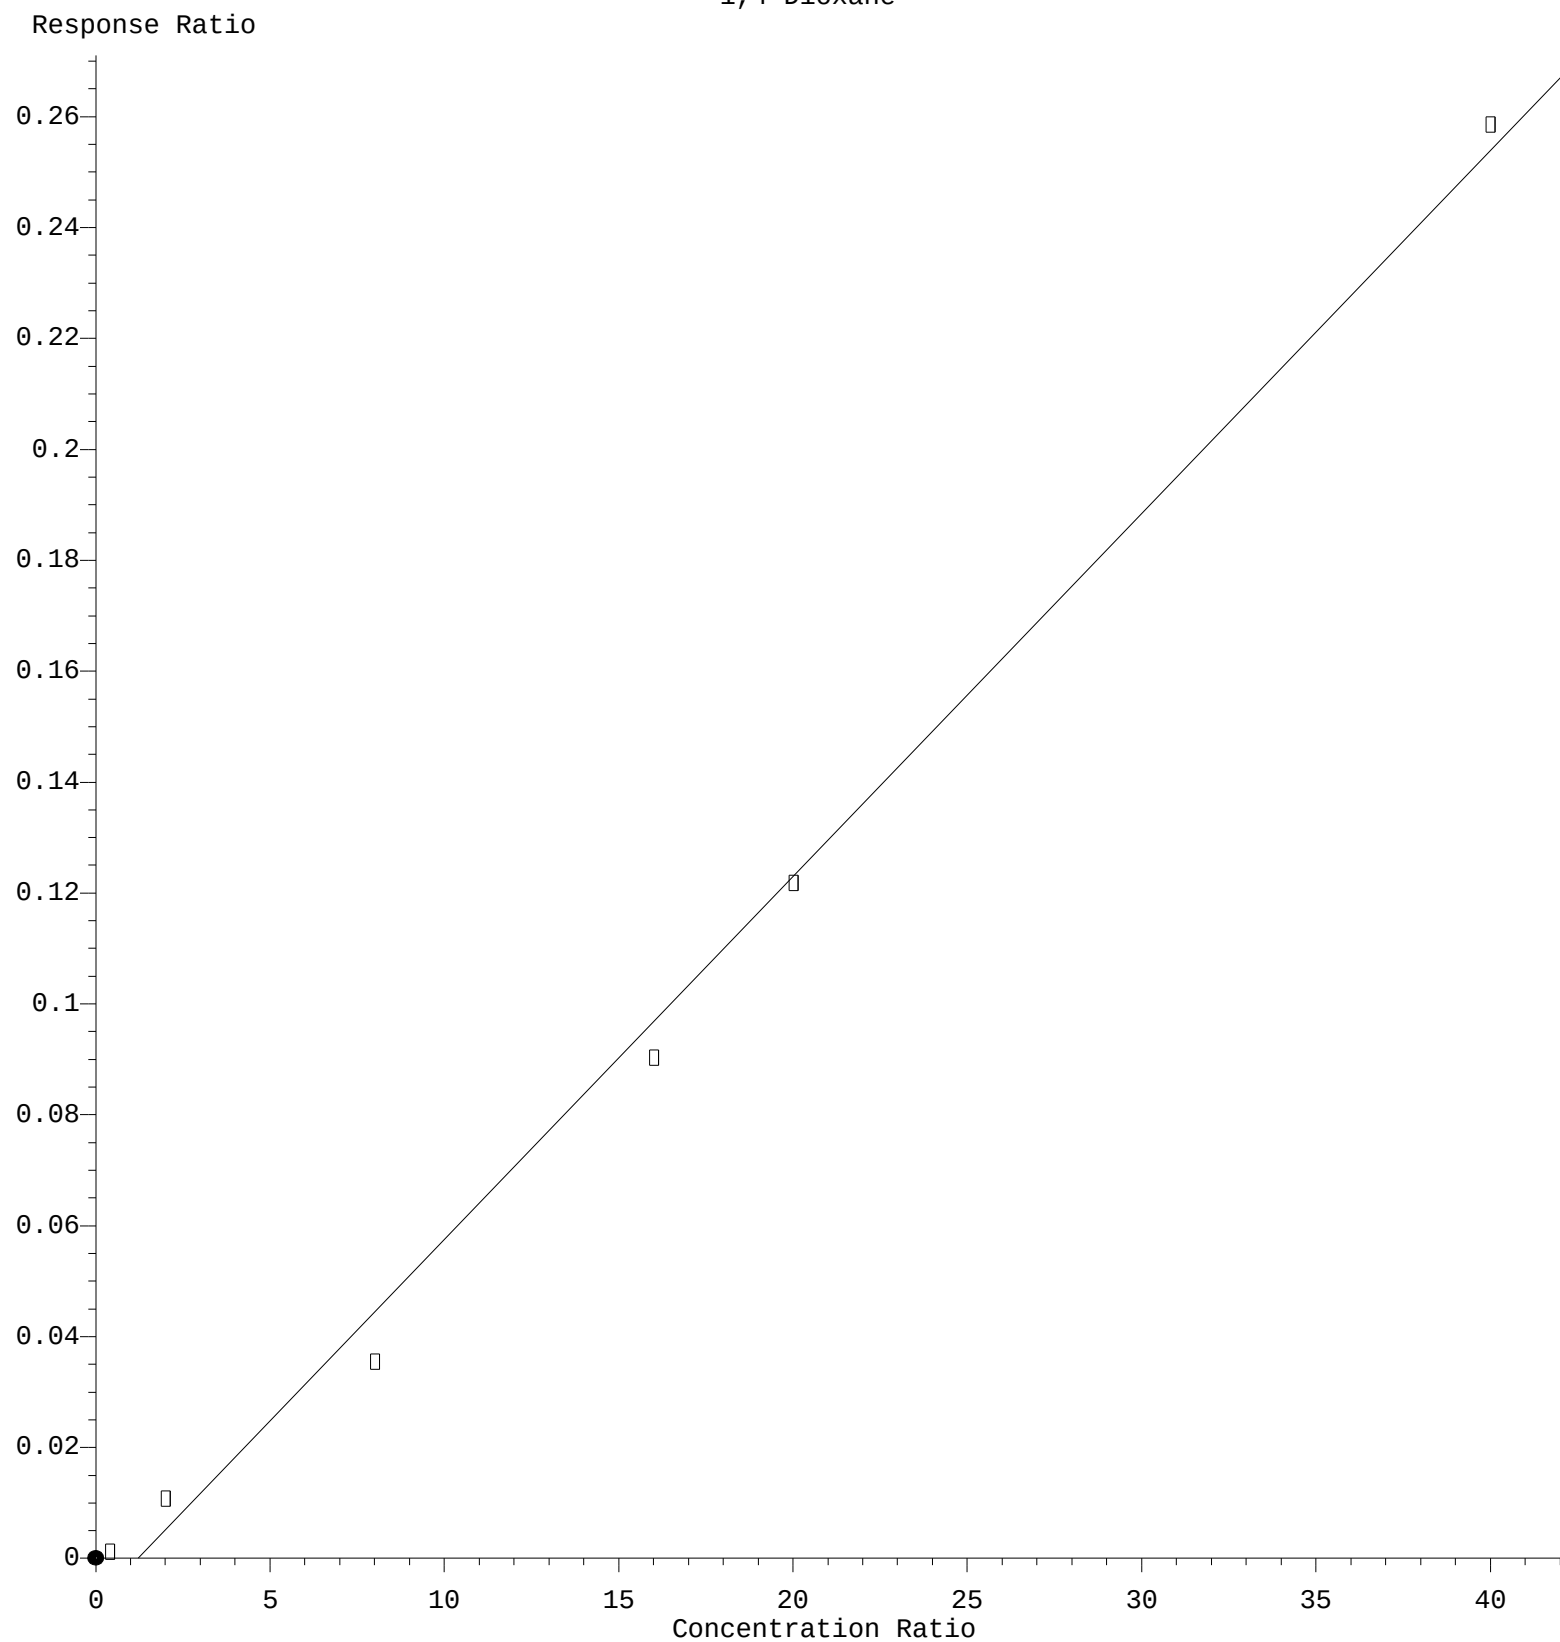

Response = $6.545 \times 10^{-3} \times \text{Amt} - 7.929 \times 10^{-3}$
 Coef of Det (r^2) = 0.995277 Curve Fit: Linear
 Method Name: Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N052121W.M
 Calibration Table Last Updated: Fri May 21 17:24:08 2021

Ethyl methacrylate

Response Ratio

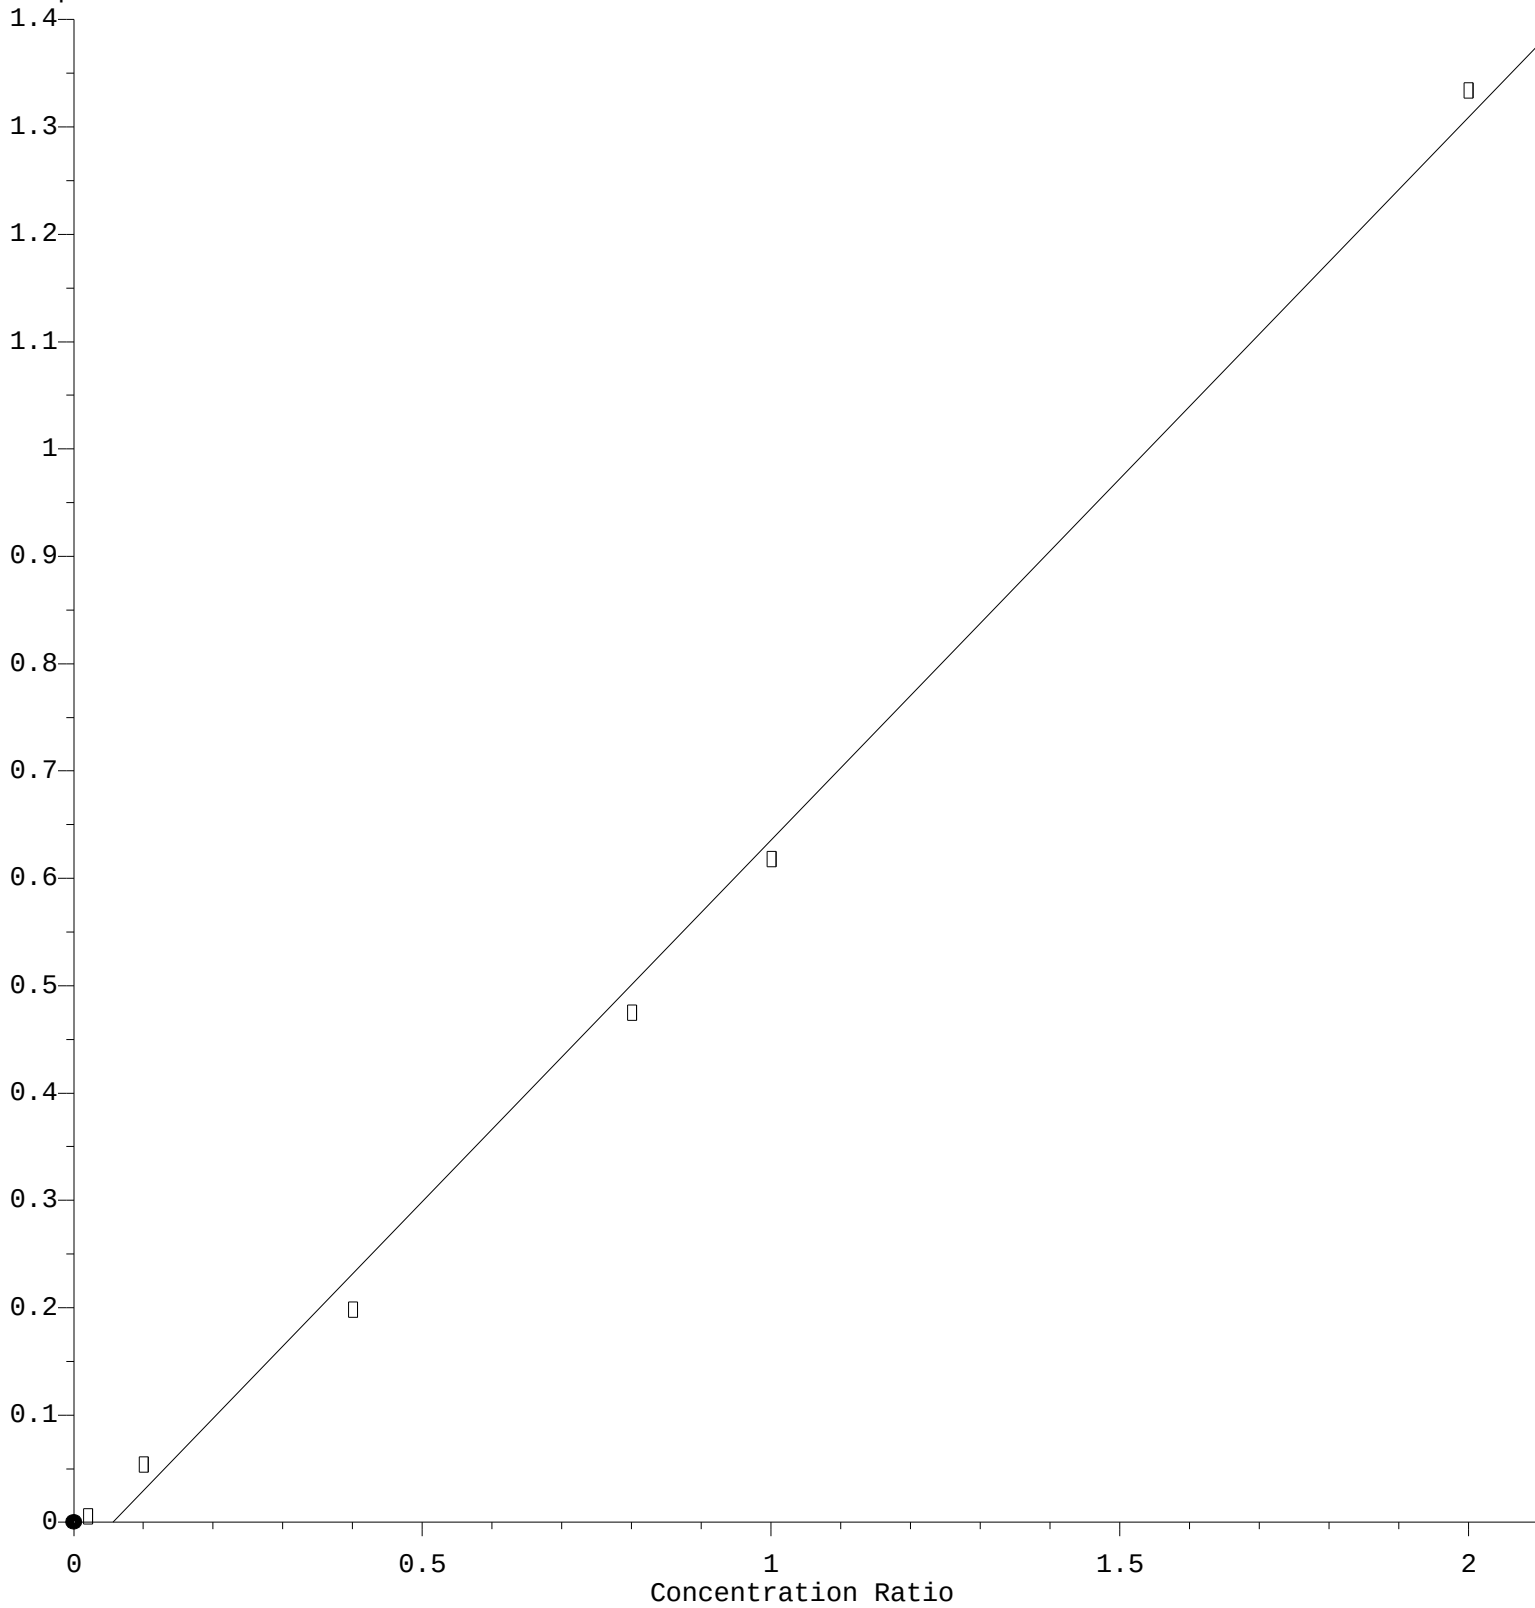

$$\text{Response} = 6.733\text{e-}001 * \text{Amt} - 3.757\text{e-}002$$


Coef of Det (r^2) = 0.996542 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N052121W.M

Calibration Table Last Updated: Fri May 21 17:24:08 2021

2-Chloroethyl Vinyl ether


Response Ratio

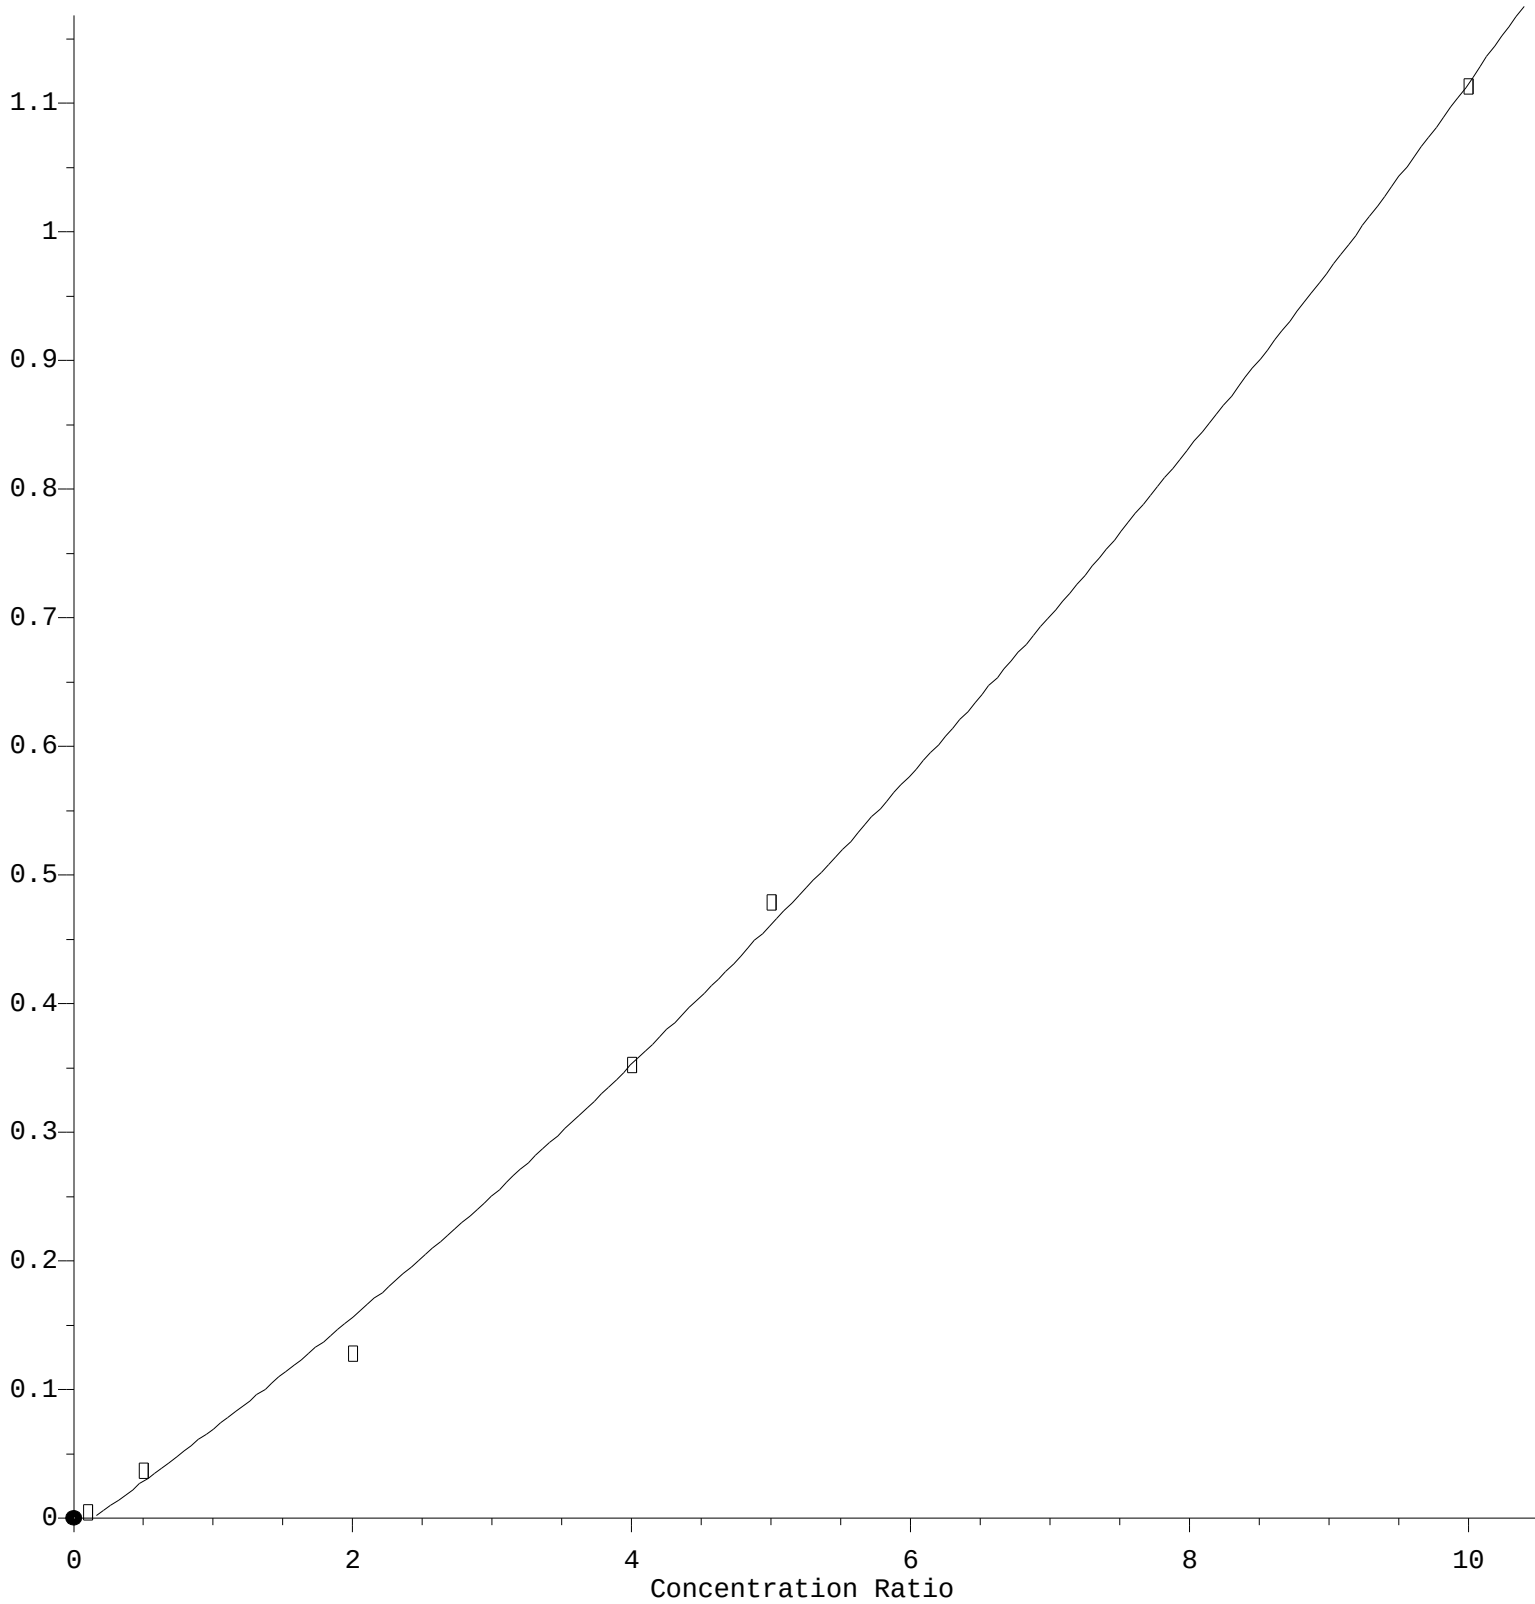

$R = 3.645e-003 A^2 + 7.617e-002 A - 1.027e-002$
 Coef of Det (r^2) = 0.998582 Curve Fit: Quadratic
 Method Name: Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N052121W.M
 Calibration Table Last Updated: Fri May 21 17:24:08 2021

2-Hexanone

Response Ratio

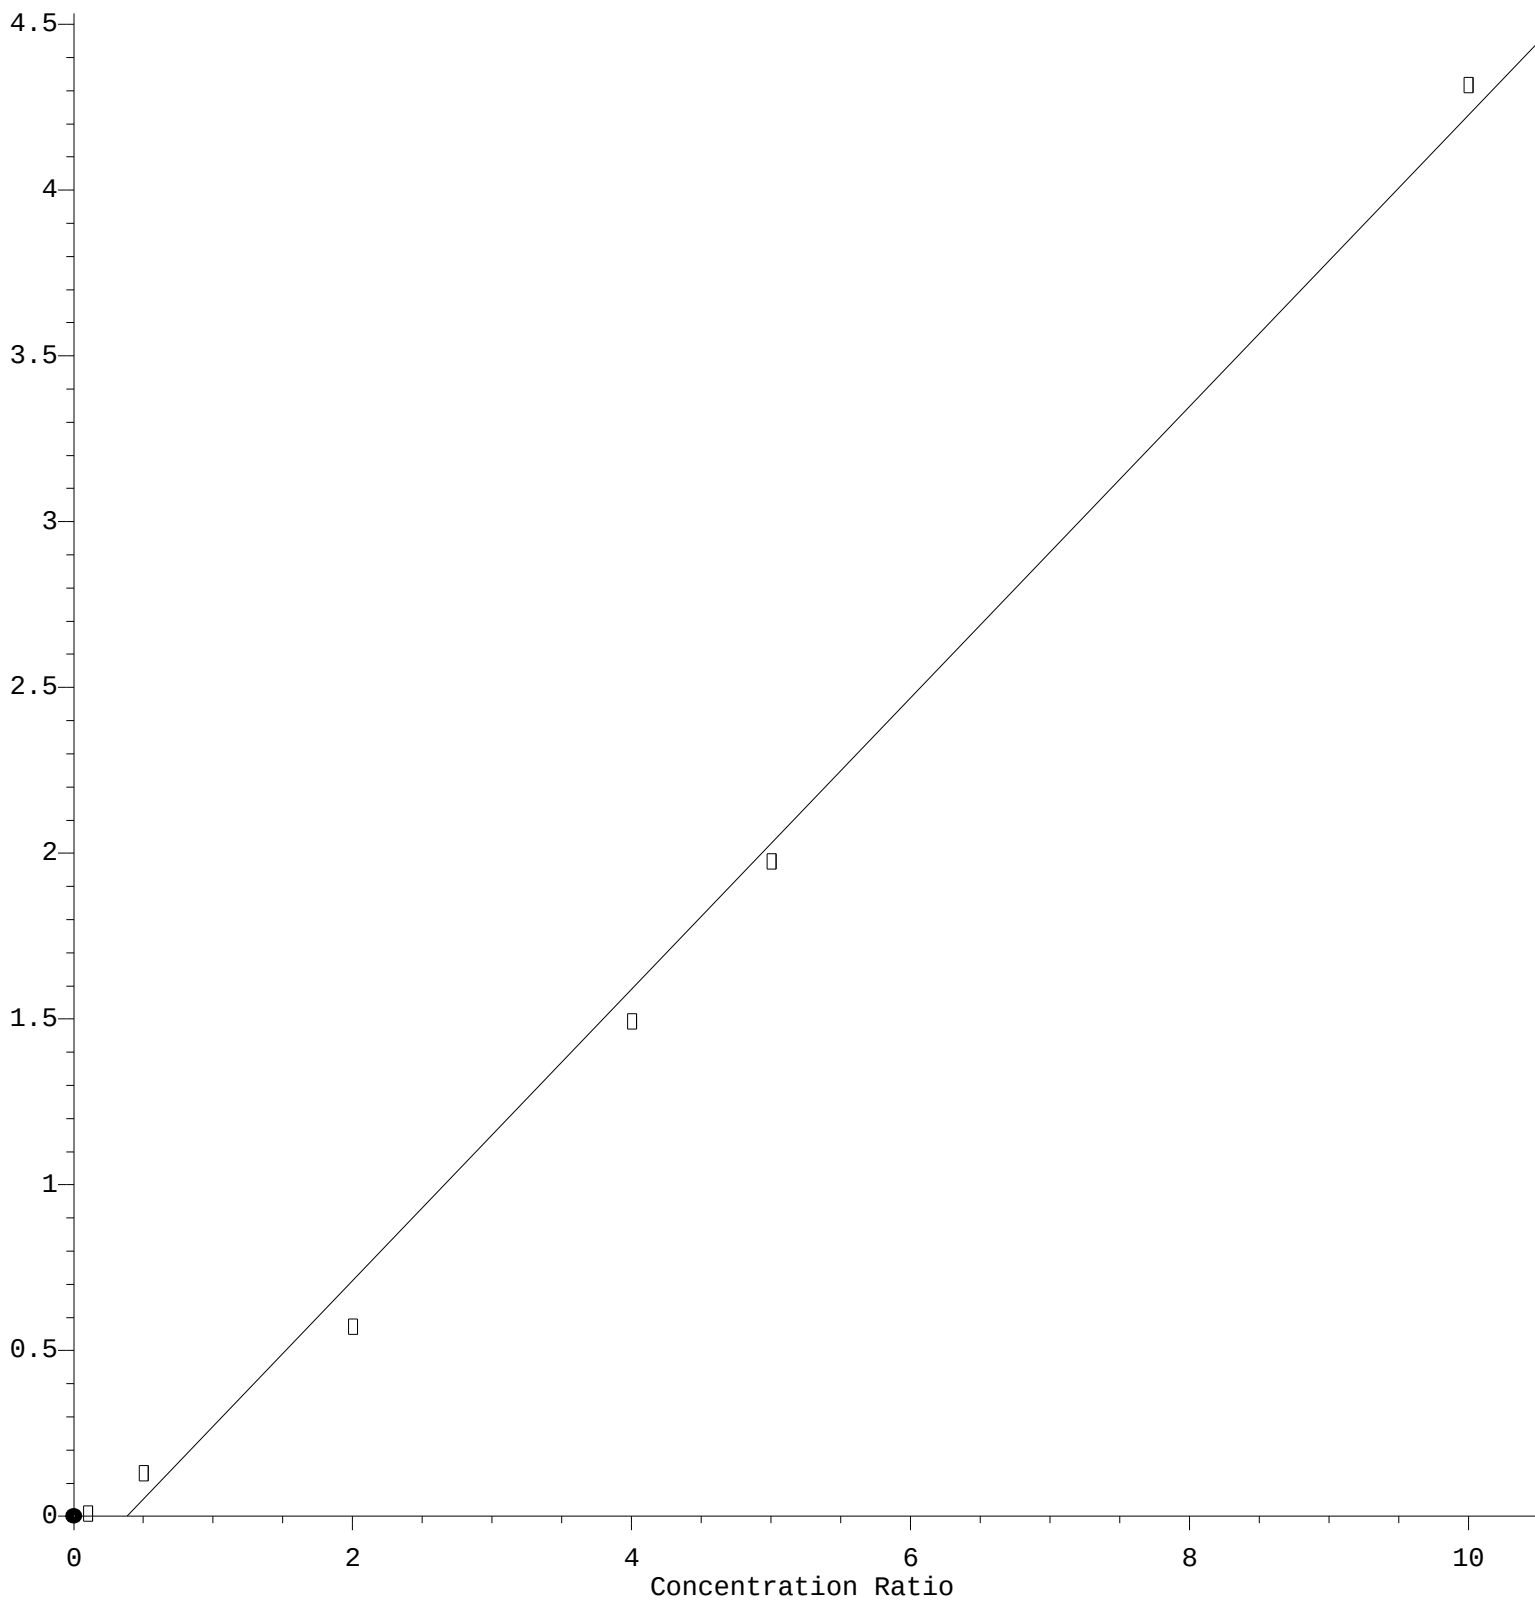

$$\text{Response} = 4.391\text{e-}001 * \text{Amt} - 1.657\text{e-}001$$


Coef of Det (r^2) = 0.995129 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N052121W.M

Calibration Table Last Updated: Fri May 21 17:24:08 2021

Styrene

Response Ratio

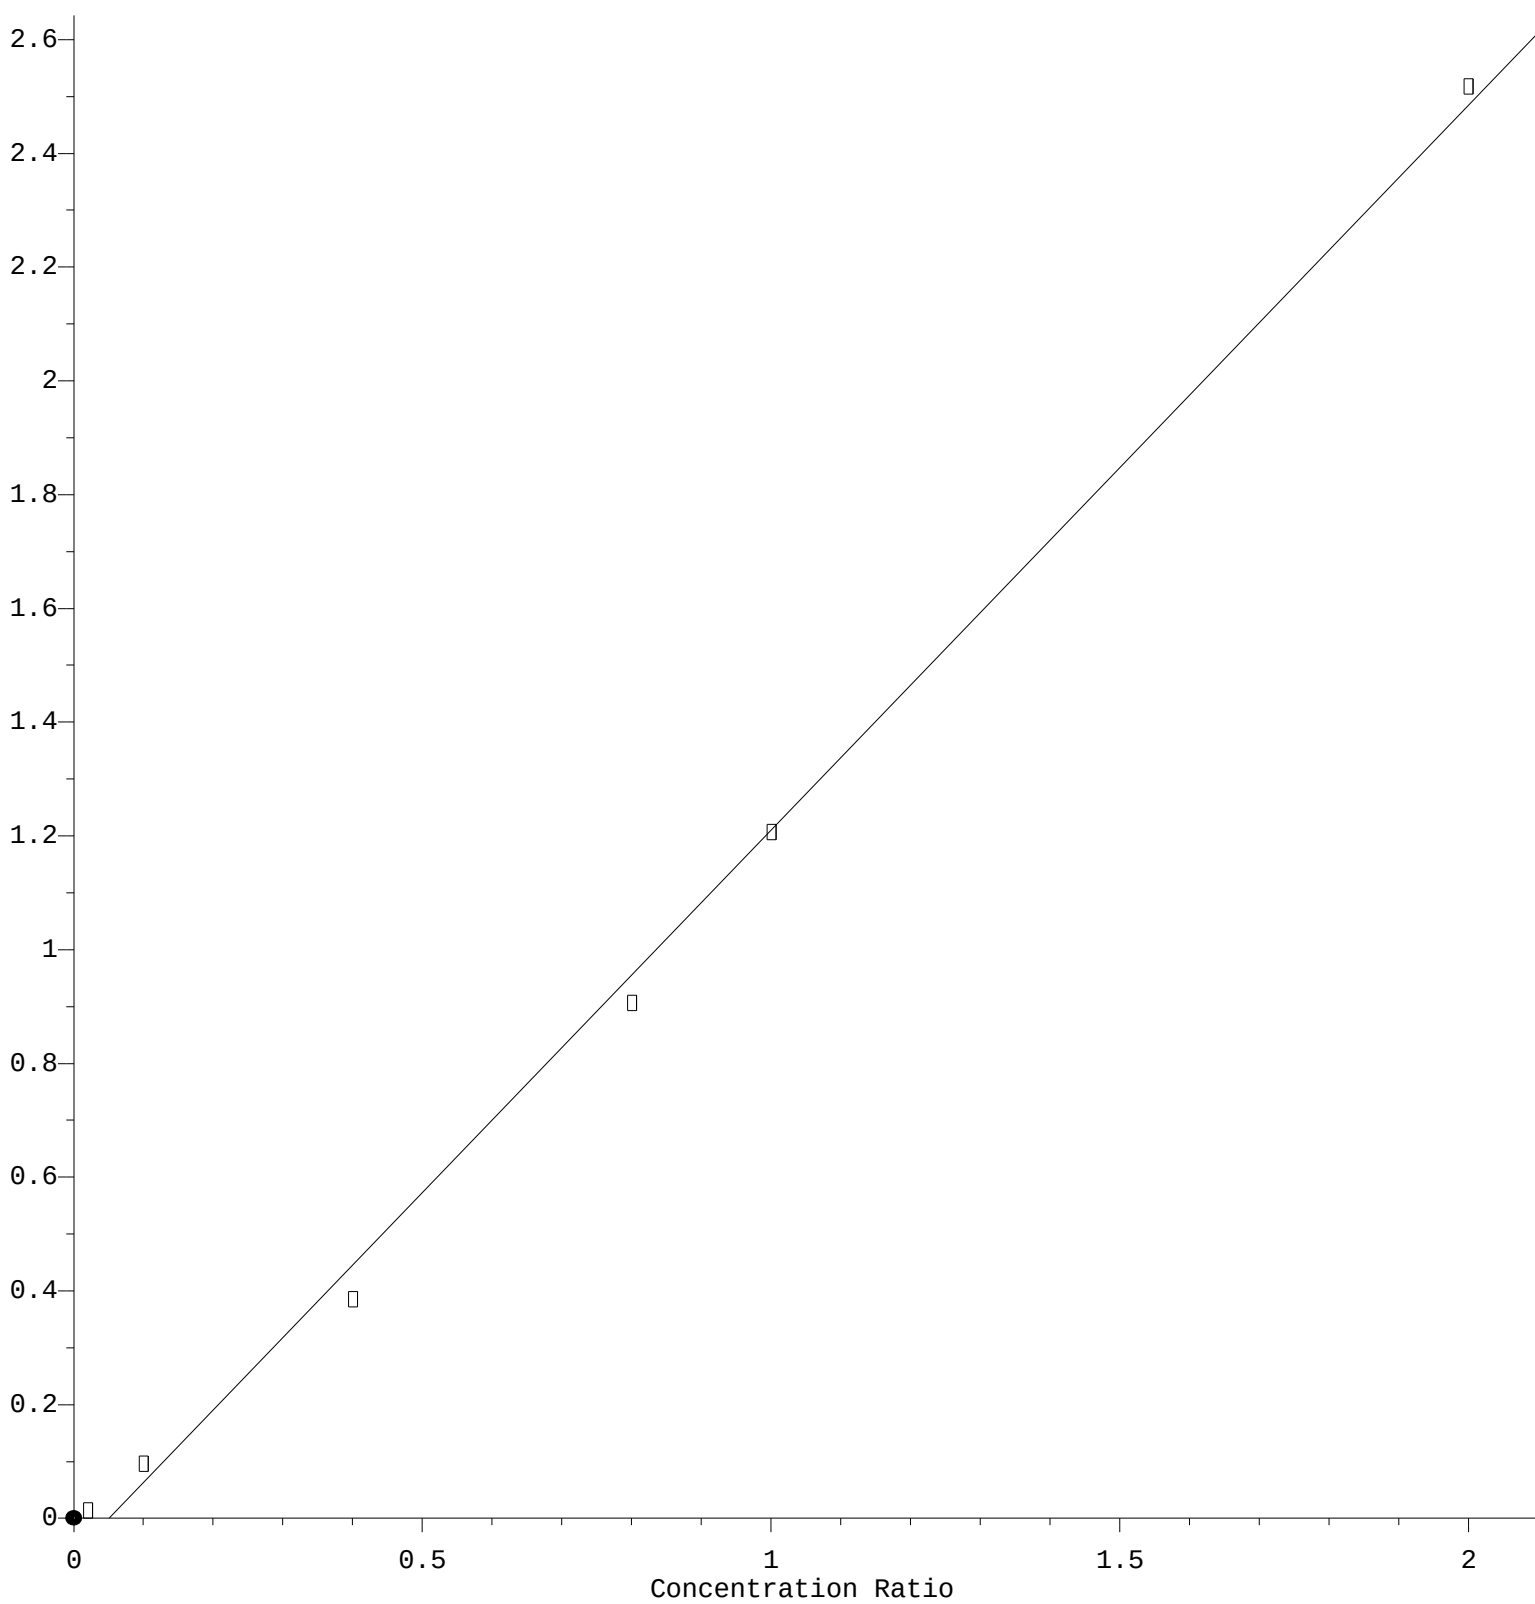

$$\text{Response} = 1.274\text{e}+000 * \text{Amt} - 6.377\text{e}-002$$


Coef of Det (r^2) = 0.997529 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N052121W.M

Calibration Table Last Updated: Fri May 21 17:24:08 2021

trans-1,4-Dichloro-2-butene

Response Ratio

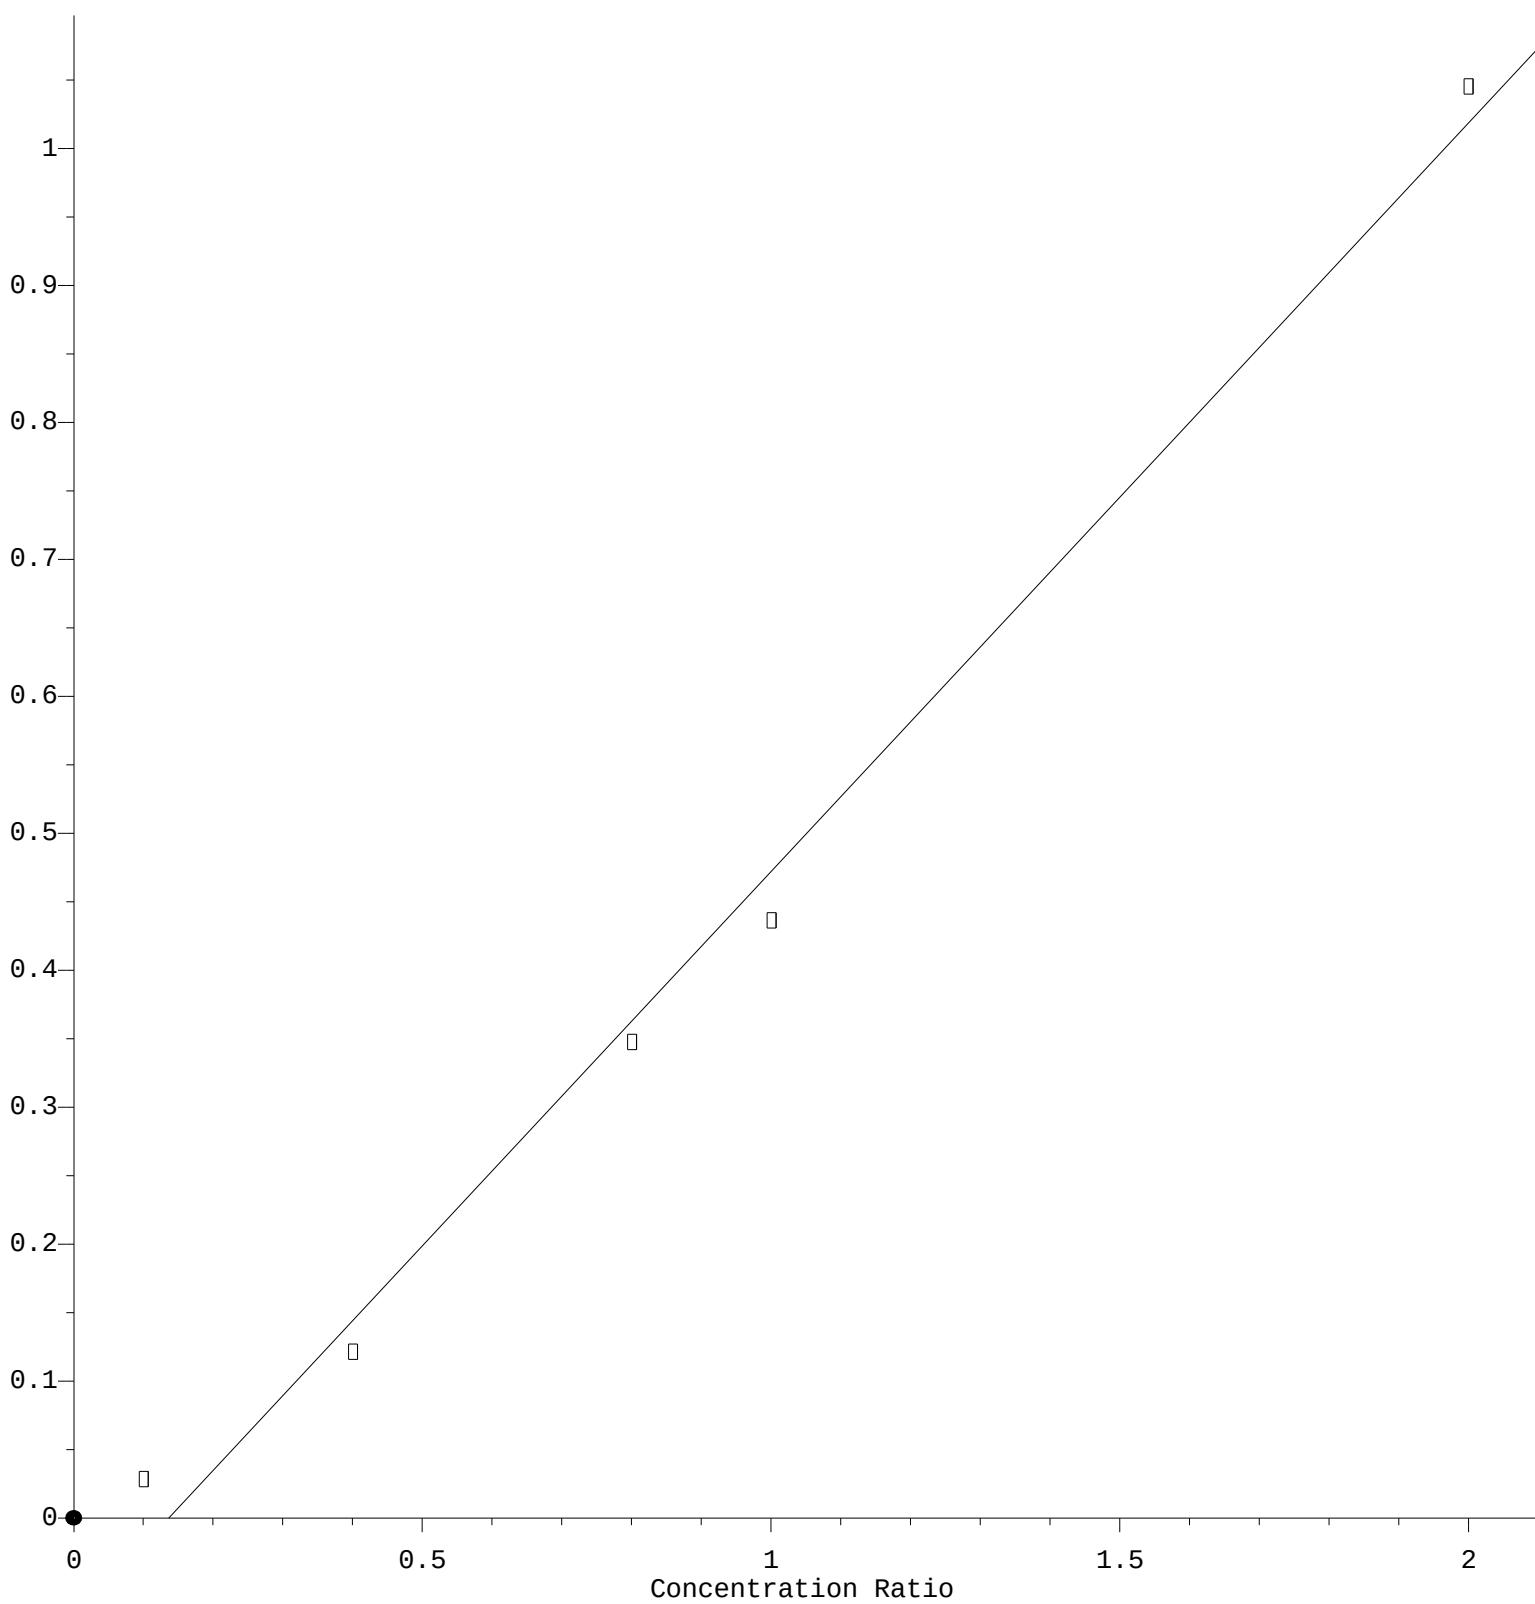

$$\text{Response} = 5.464\text{e-}001 * \text{Amt} - 7.415\text{e-}002$$


Coef of Det (r^2) = 0.992061 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N052121W.M

Calibration Table Last Updated: Fri May 21 17:24:08 2021

1,2,4-Trichlorobenzene

Response Ratio

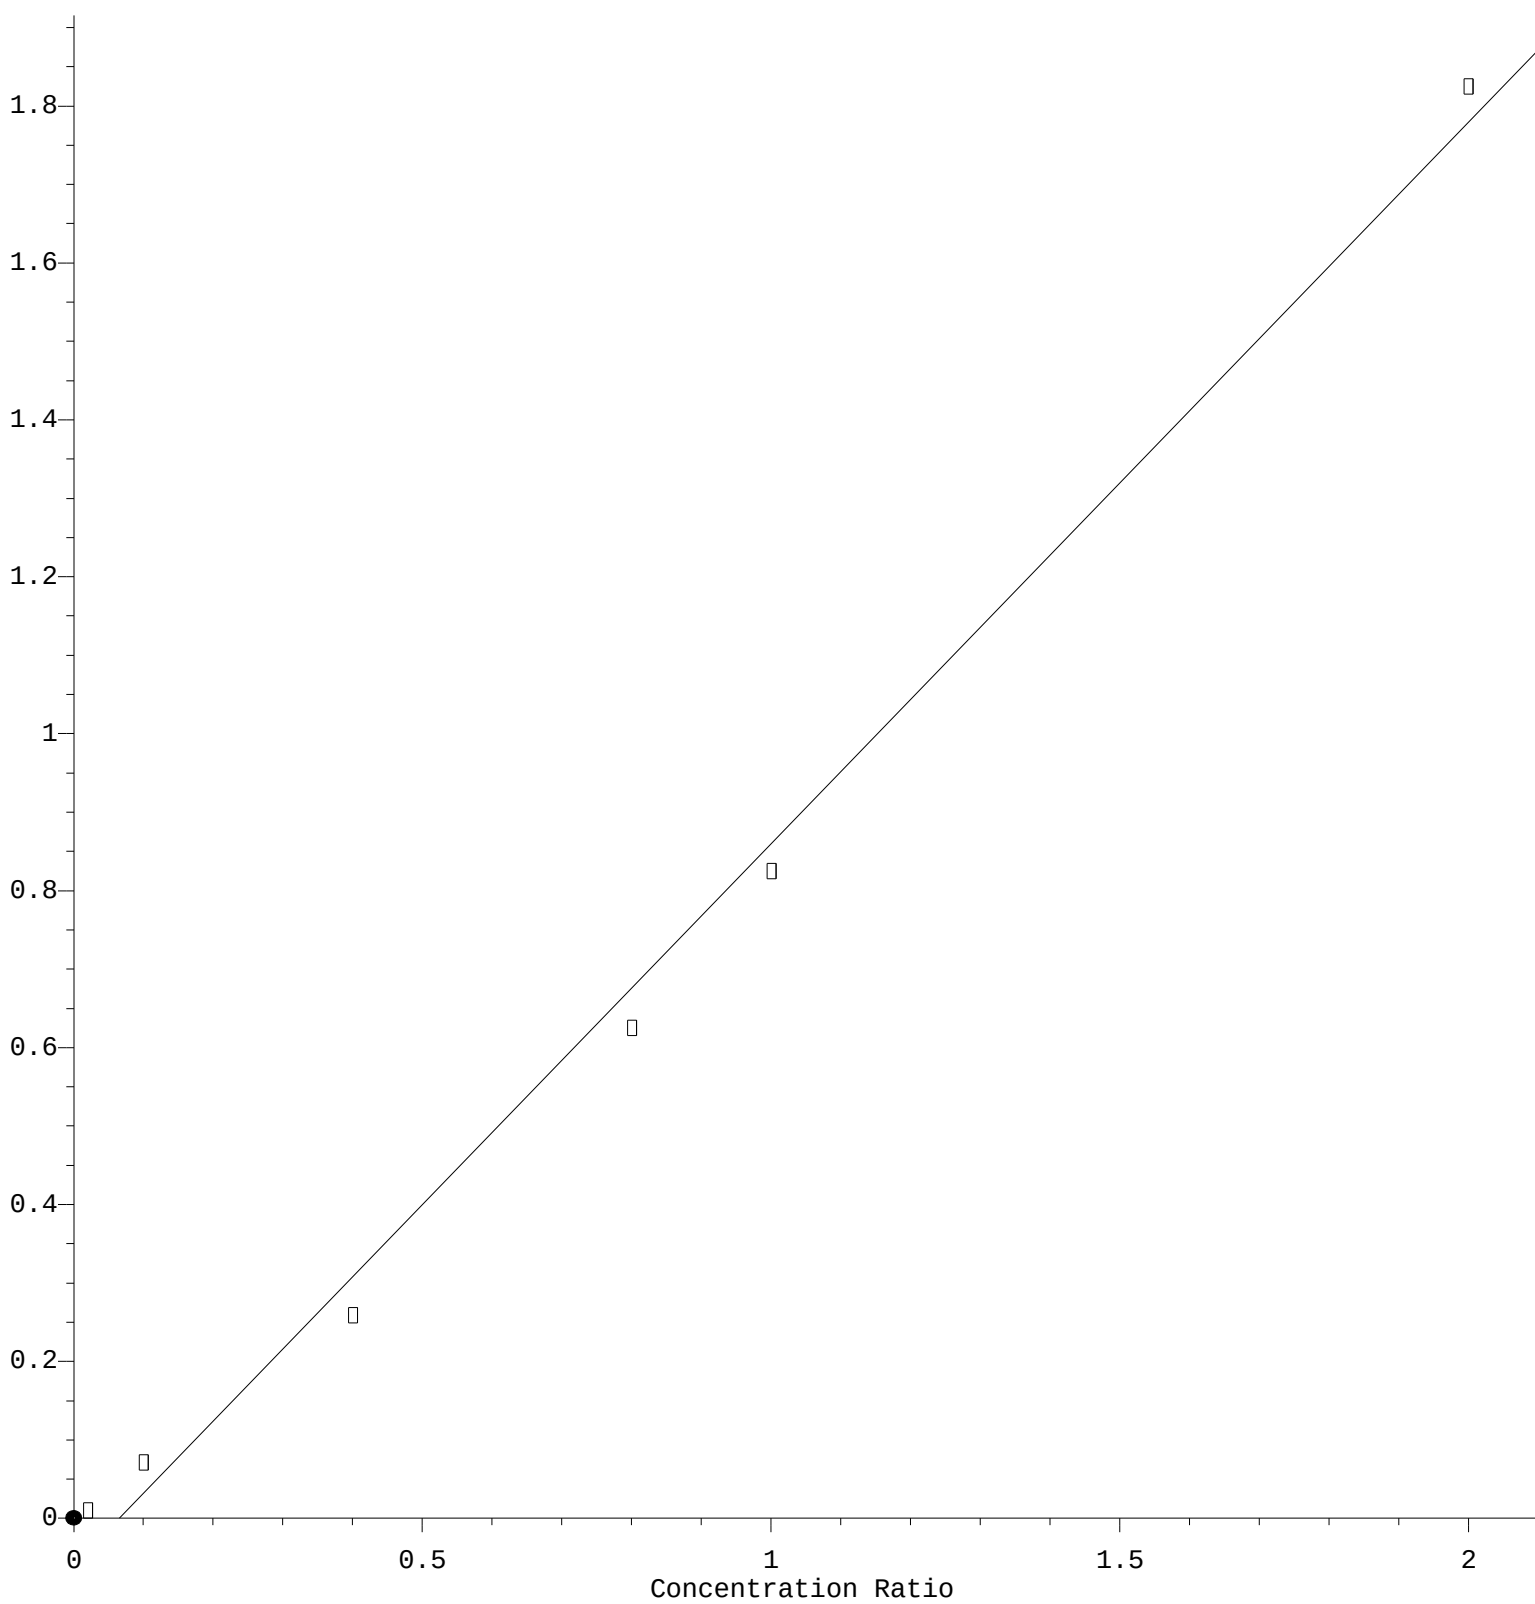

$$\text{Response} = 9.195\text{e-}001 * \text{Amt} - 5.998\text{e-}002$$


Coef of Det (r^2) = 0.994559 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N052121W.M

Calibration Table Last Updated: Fri May 21 17:24:08 2021

Naphthalene

Response Ratio

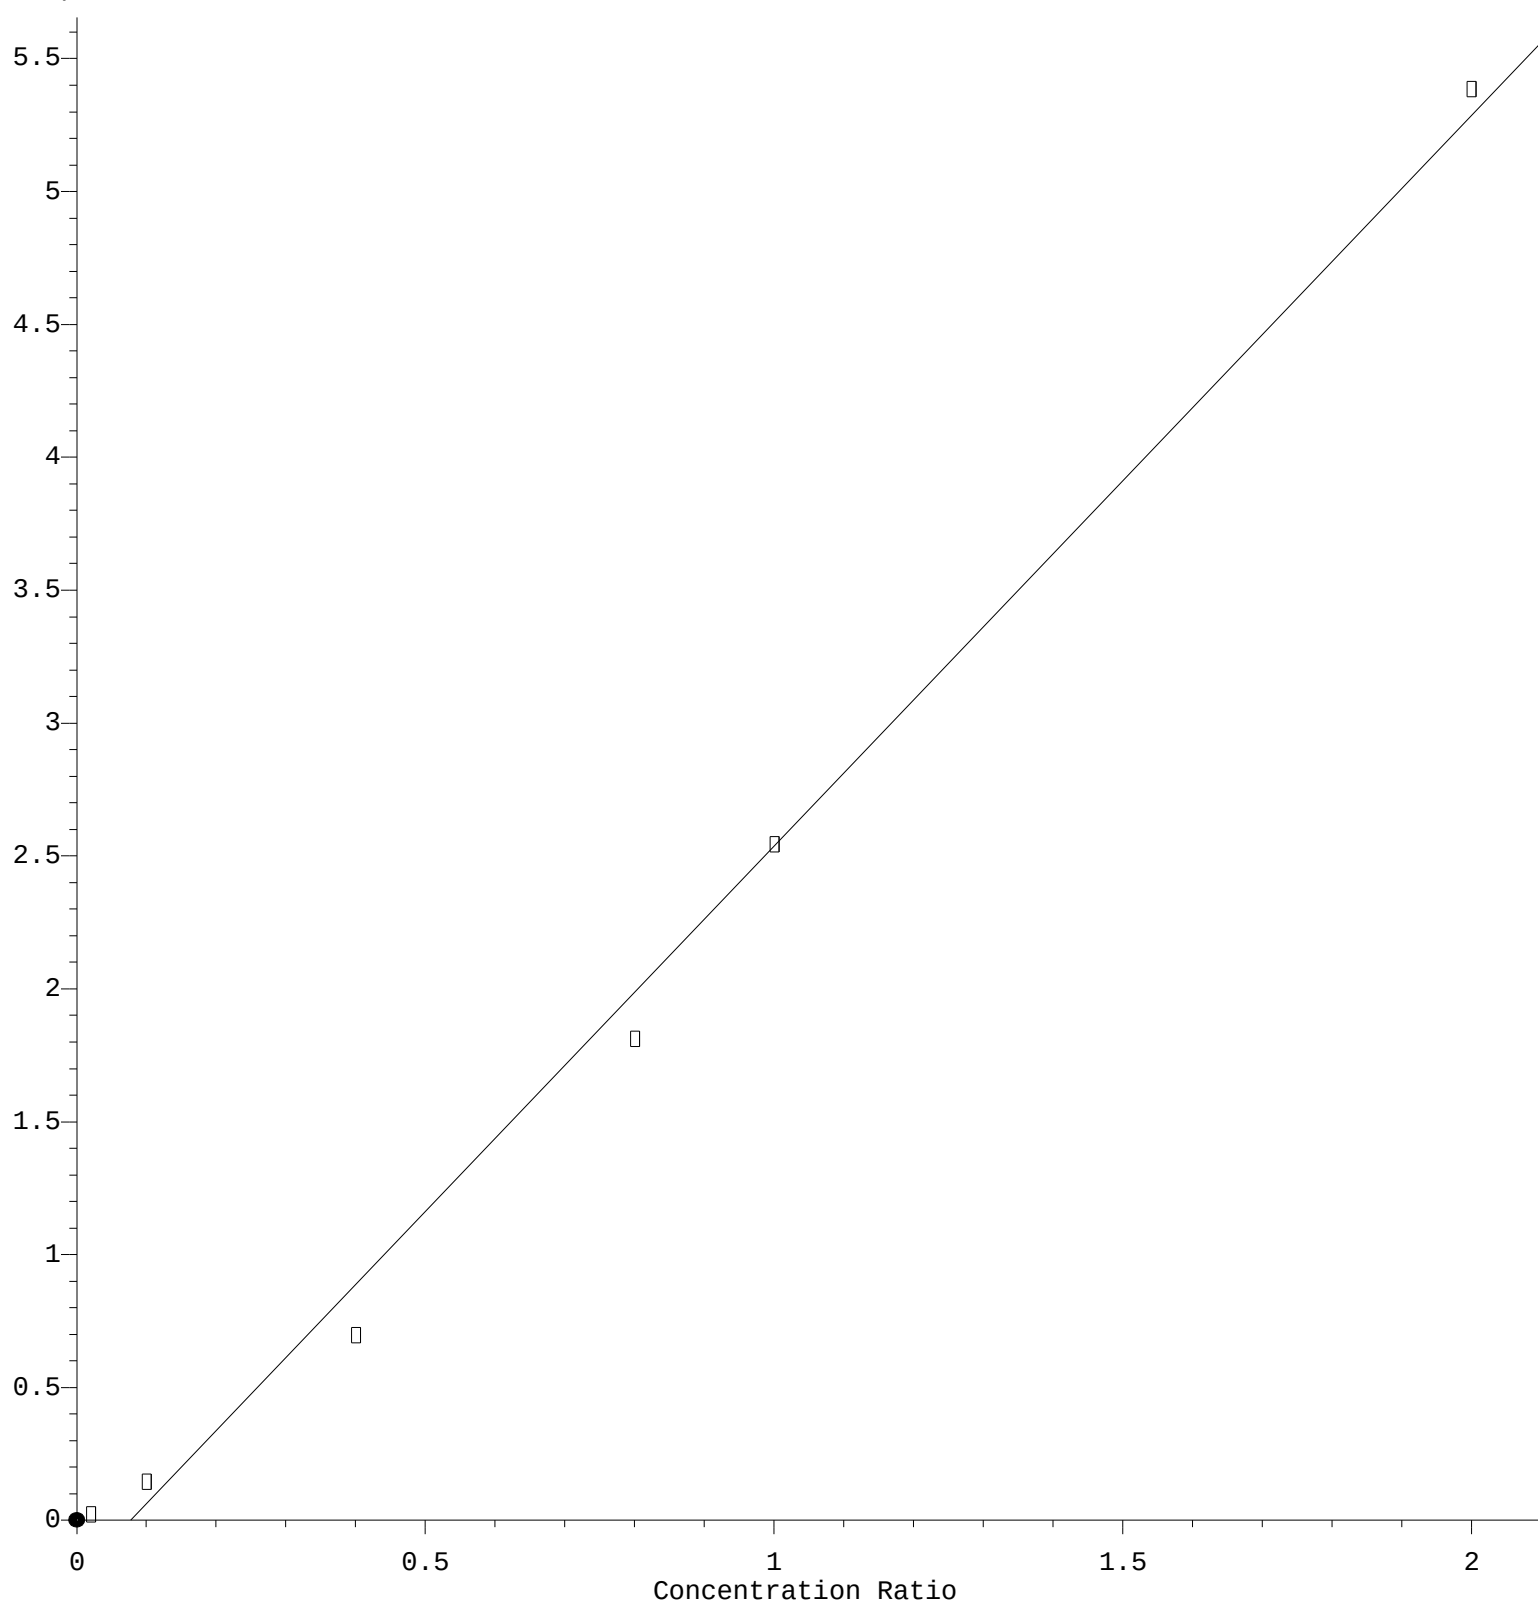

Response = 2.749e+000 * Amt - 2.124e-001
Coef of Det (r^2) = 0.994364 Curve Fit: Linear
Method Name: Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N052121W.M
Calibration Table Last Updated: Fri May 21 17:24:08 2021