

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN052124\
 Data File : VN082264.D
 Acq On : 22 May 2024 01:33
 Operator : JC\MD
 Sample : P2494-04 40X
 Misc : 5.07g/10mL/100uL/5.00mL/MSVOA_N/MEOH
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 4

Quant Time: May 22 04:36:39 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N051524W.M
 Quant Title : SW846 8260
 QLast Update : Thu May 16 05:21:06 2024
 Response via : Initial Calibration

Compound	R.T. QIon		Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	8.229	168	175328	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	9.100	114	307285	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.870	117	294114	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.794	152	139650	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.576	65	138621	50.071	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	= 100.140%	
35) Dibromofluoromethane	8.171	113	97201	51.422	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	= 102.840%	
50) Toluene-d8	10.570	98	387830	53.515	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	= 107.020%	
62) 4-Bromofluorobenzene	12.853	95	141248	54.606	ug/l	0.00
Spiked Amount	50.000	Range	64 - 133	Recovery	= 109.220%	
Target Compounds						
					Qvalue	
5) Bromomethane	2.965	94	489	0.316	ug/l #	66
16) Acetone	4.441	43	535	0.471	ug/l #	43
20) Methylene Chloride	5.271	84	1339	0.584	ug/l #	84
31) Cyclohexane	8.229	56	8967	2.028	ug/l #	52
36) 1,1-Dichloropropene	8.229	75	15591	4.918	ug/l #	47
38) Carbon Tetrachloride	8.224	117	19561	6.087	ug/l #	17
39) Methylcyclohexane	9.606	83	8764	2.522	ug/l	96
40) Benzene	8.612	78	25734	2.722	ug/l	100
43) Isopropyl Acetate	8.682	43	5447	0.866	ug/l #	52
52) Toluene	10.635	92	45939	8.097	ug/l	98
55) 1,1,2-Trichloroethane	11.006	97	1015	0.492	ug/l #	14
59) 2-Hexanone	11.170	43	1631	0.624	ug/l #	23
67) Ethyl Benzene	11.964	91	30890	2.658	ug/l	99
68) m/p-Xylenes	12.064	106	67440	15.831	ug/l	93
69) o-Xylene	12.400	106	59989	14.538	ug/l	92
70) Styrene	12.406	104	15346	2.239	ug/l #	37
73) Isopropylbenzene	12.694	105	7617	0.687	ug/l	99
74) N-amyl acetate	12.482	43	2083	0.341	ug/l #	59
76) 1,2,3-Trichloropropane	12.853	75	84004	28.580	ug/l #	1
78) n-propylbenzene	13.035	91	14376	1.094	ug/l	99
79) 2-Chlorotoluene	13.129	91	2171	0.263	ug/l #	49
80) 1,3,5-Trimethylbenzene	13.176	105	102839	11.464	ug/l	97
81) trans-1,4-Dichloro-2-b...	12.853	75	84004	66.847	ug/l #	13
82) 4-Chlorotoluene	13.176	91	11665	1.446	ug/l #	41
83) tert-Butylbenzene	13.482	119	26017	3.315	ug/l #	60
84) 1,2,4-Trimethylbenzene	13.482	105	200248	21.818	ug/l	97
85) sec-Butylbenzene	13.611	105	6147	0.565	ug/l #	66
86) p-Isopropyltoluene	13.729	119	7249	0.820	ug/l	90
89) n-Butylbenzene	14.058	91	4019	0.506	ug/l #	31
90) Hexachloroethane	14.335	117	3547	2.165	ug/l #	17
92) 1,2-Dibromo-3-Chloropr...	14.735	75	379	0.577	ug/l #	2
95) Naphthalene	15.641	128	2841646	356.778	ug/l	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN052124\
Data File : VN082264.D
Acq On : 22 May 2024 01:33
Operator : JC\MD
Sample : P2494-04 40X
Misc : 5.07g/10mL/100uL/5.00mL/MSVOA_N/MEOH
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
4

Quant Time: May 22 04:36:39 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N051524W.M
Quant Title : SW846 8260
QLast Update : Thu May 16 05:21:06 2024
Response via : Initial Calibration




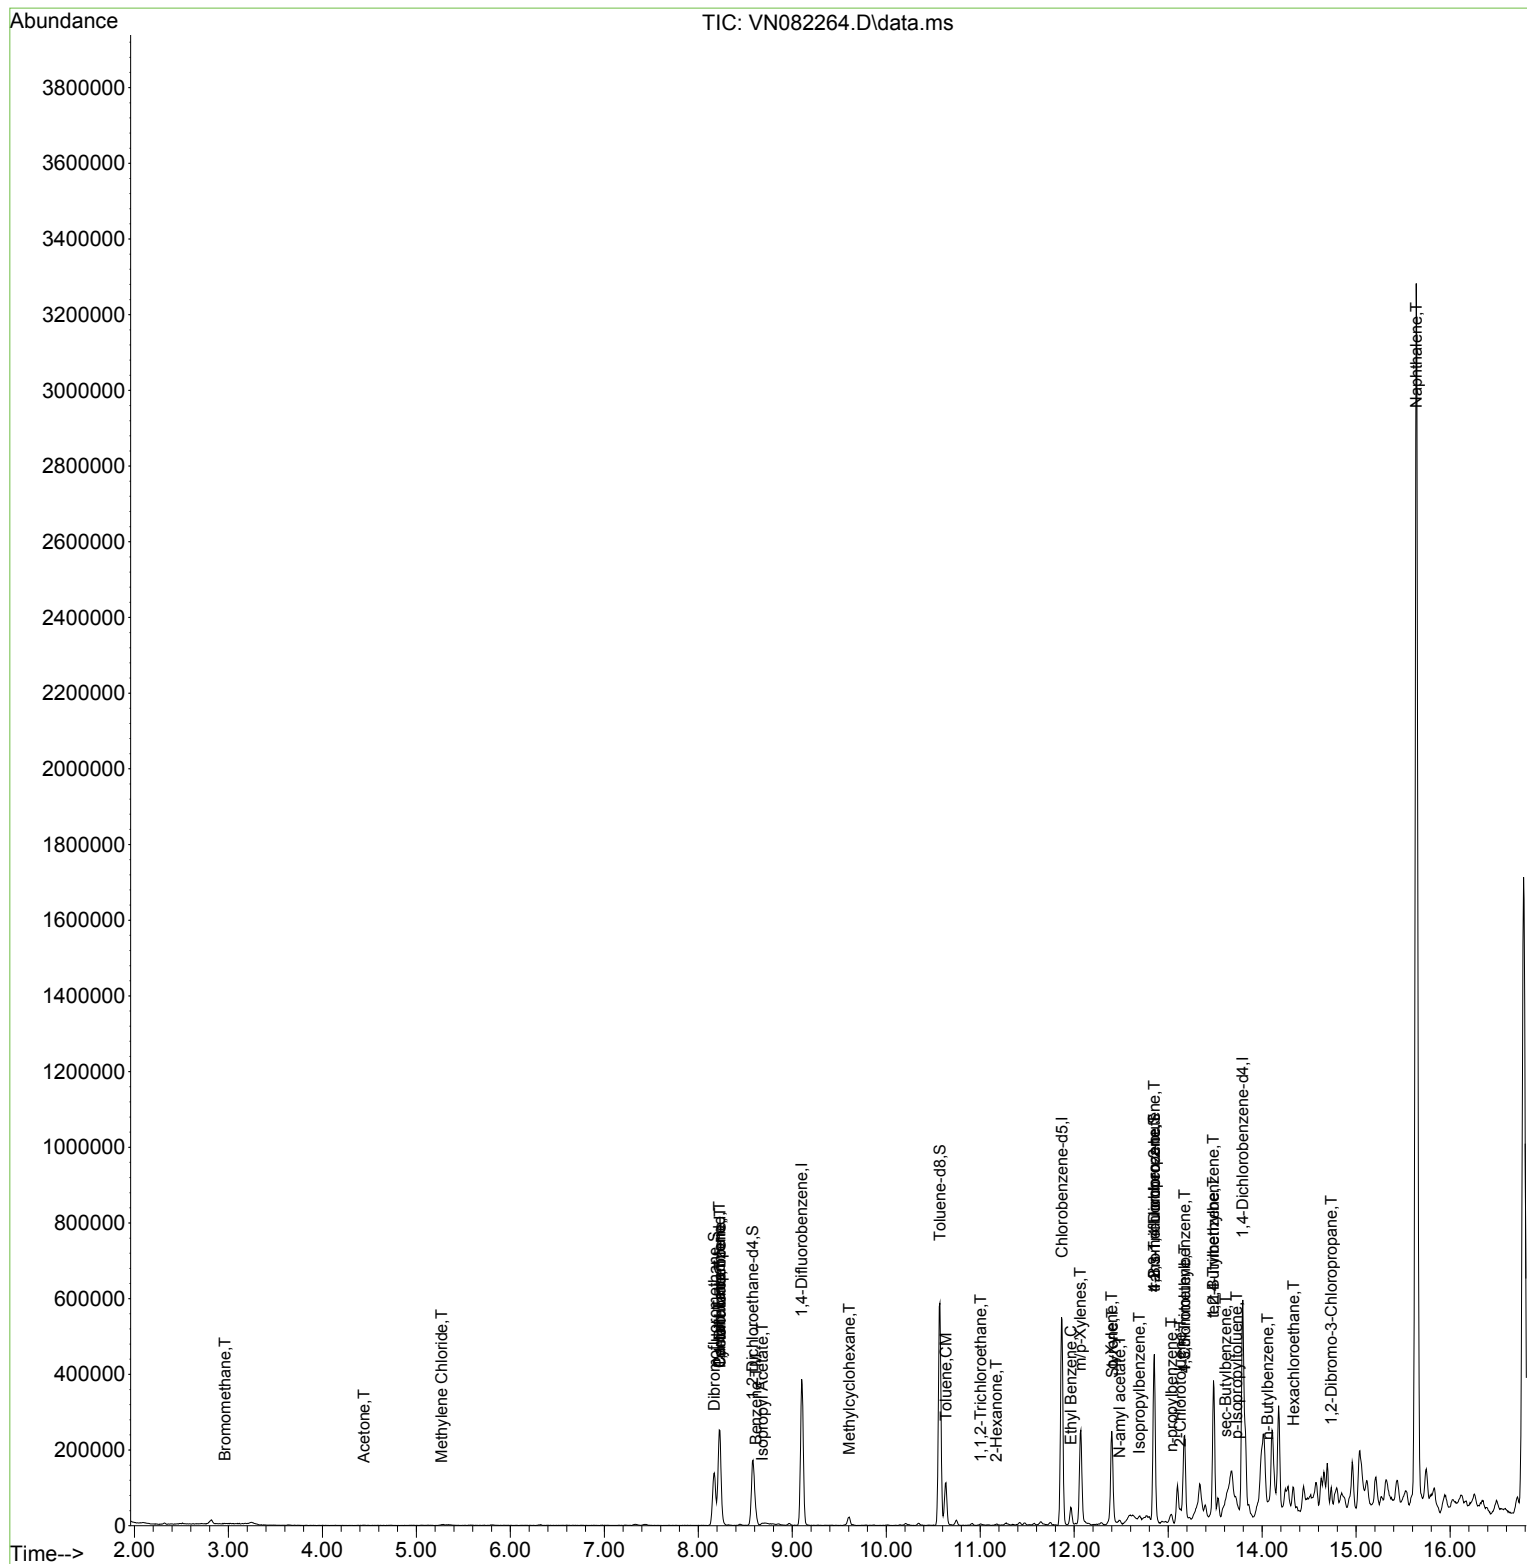


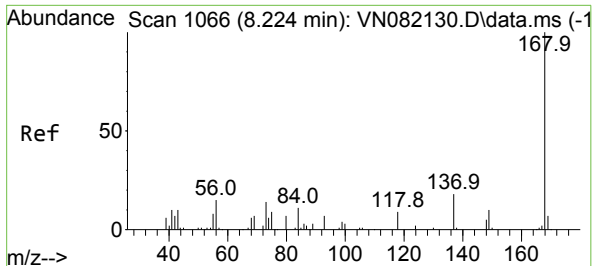

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.229 min Scan# 1066
Delta R.T. 0.005 min
Lab File: VN082264.D
Acq: 22 May 2024 01:33




Instrument :
MSVOA_N
ClientSampleId :
4


Tgt Ion:168 Resp: 175328
Ion Ratio Lower Upper
168 100
99 63.5 48.2 72.4

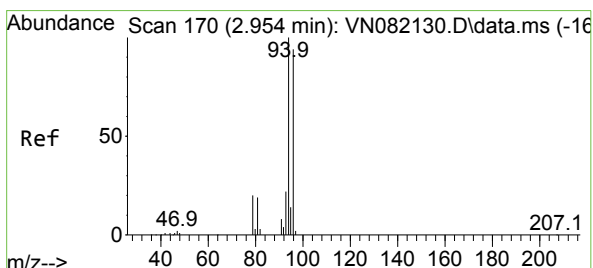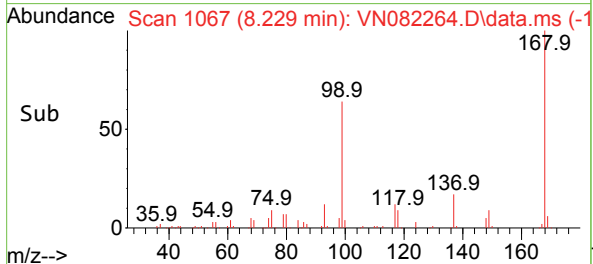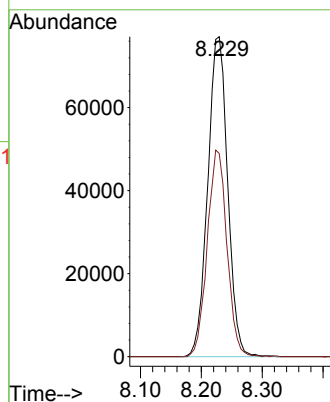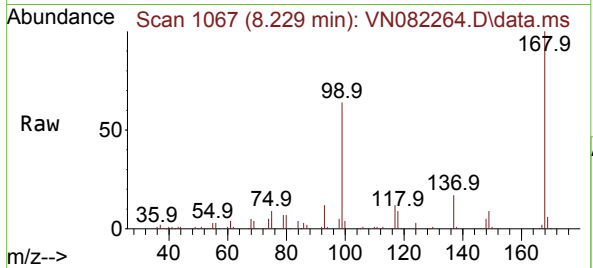

#5
Bromomethane
Concen: 0.316 ug/l
RT: 2.965 min Scan# 172
Delta R.T. 0.012 min
Lab File: VN082264.D
Acq: 22 May 2024 01:33

Tgt Ion: 94 Resp: 489
Ion Ratio Lower Upper
94 100
96 60.8 74.8 112.2#

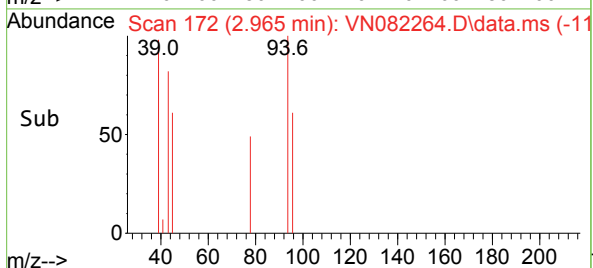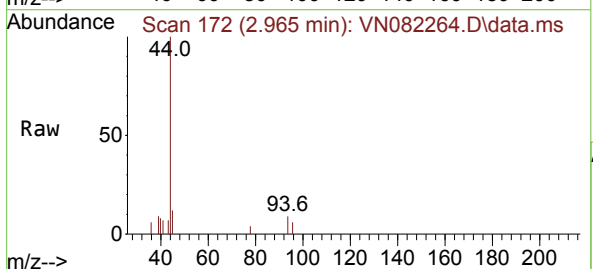



#16

Acetone

Concen: 0.471 ug/l

RT: 4.441 min Scan# 41

Delta R.T. 0.017 min

Lab File: VN082264.D

Acq: 22 May 2024 01:33

Instrument :

MSVOA_N

ClientSampleId :





4

Tgt Ion: 43 Resp: 535

Ion Ratio Lower Upper

43 100

58 0.0 25.2 37.8#

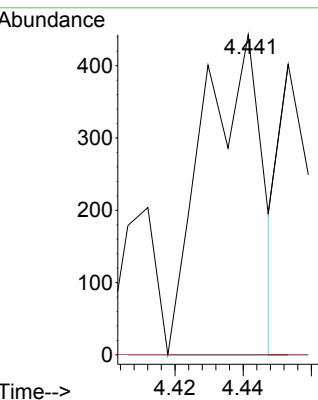

#20

Methylene Chloride

Concen: 0.584 ug/l

RT: 5.271 min Scan# 564

Delta R.T. -0.006 min

Lab File: VN082264.D

Acq: 22 May 2024 01:33

Tgt Ion: 84 Resp: 1339




Ion Ratio Lower Upper


84 100

49 98.7 84.9 127.3

51 28.7 27.0 40.6


86 37.9 52.3 78.5#

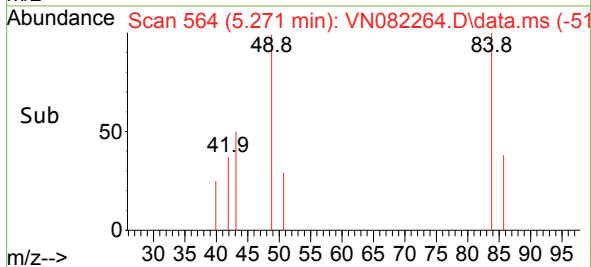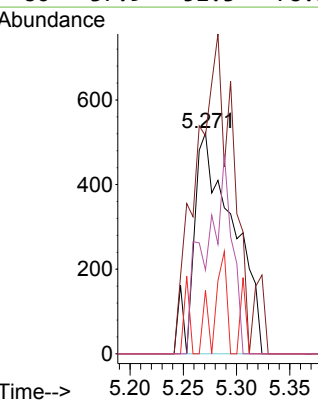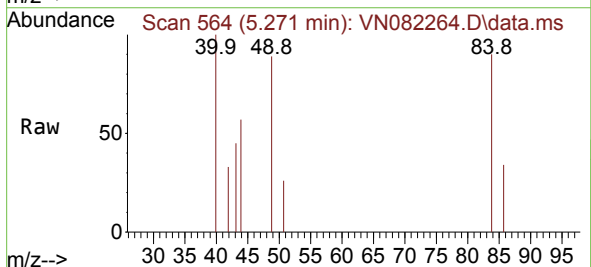






#31
Cyclohexane
Concen: 2.028 ug/l
RT: 8.229 min Scan# 1067
Delta R.T. -0.030 min
Lab File: VN082264.D
Acq: 22 May 2024 01:33

Instrument :
MSVOA_N
ClientSampleId :
4







Tgt Ion: 56 Resp: 8967
Ion Ratio Lower Upper
56 100
69 103.2 24.4 36.6#
84 116.7 77.0 115.4#

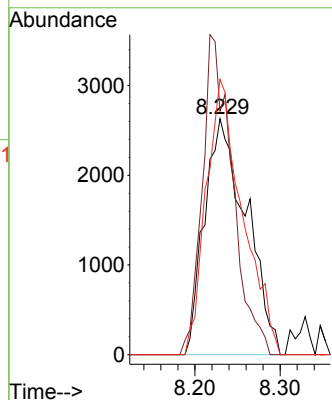

#33
1,2-Dichloroethane-d4
Concen: 50.071 ug/l
RT: 8.576 min Scan# 1126
Delta R.T. -0.000 min
Lab File: VN082264.D
Acq: 22 May 2024 01:33

Tgt Ion: 65 Resp: 138621
Ion Ratio Lower Upper
65 100
67 50.3 0.0 103.0

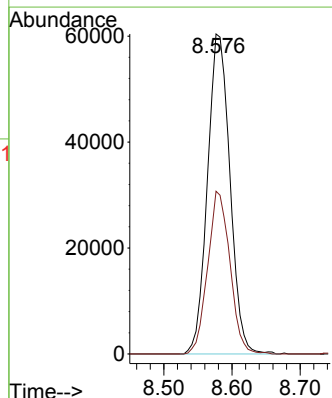



#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 9.100 min Scan# 1

Delta R.T. -0.000 min

Lab File: VN082264.D

Acq: 22 May 2024 01:33

Instrument :

MSVOA_N

ClientSampleId :

4





Tgt Ion:114 Resp: 307285

Ion Ratio Lower Upper

114 100

63 24.3 0.0 41.0

88 15.1 0.0 31.4

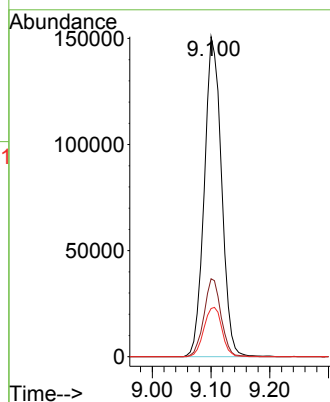

#35

Dibromofluoromethane

Concen: 51.422 ug/l

RT: 8.171 min Scan# 1057

Delta R.T. 0.006 min

Lab File: VN082264.D

Acq: 22 May 2024 01:33




Tgt Ion:113 Resp: 97201


Ion Ratio Lower Upper

113 100

111 104.3 83.4 125.2

192 18.1 14.0 21.0





#36

1,1-Dichloropropene

Concen: 4.918 ug/l

RT: 8.229 min Scan# 1067

Delta R.T. -0.141 min

Lab File: VN082264.D


Acq: 22 May 2024 01:33

Instrument :

MSVOA_N

ClientSampleId :

4






Tgt Ion: 75 Resp: 15591

Ion Ratio Lower Upper

75 100

110 6.9 17.8 53.5#

77 0.0 25.0 37.4#

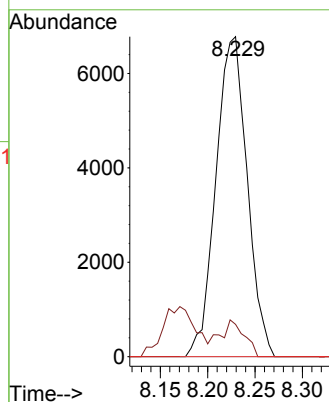

#38

Carbon Tetrachloride

Concen: 6.087 ug/l

RT: 8.224 min Scan# 1066

Delta R.T. -0.141 min

Lab File: VN082264.D

Acq: 22 May 2024 01:33




Tgt Ion: 117 Resp: 19561


Ion Ratio Lower Upper

117 100

119 6.3 76.5 114.7#

121 0.0 23.9 35.9#

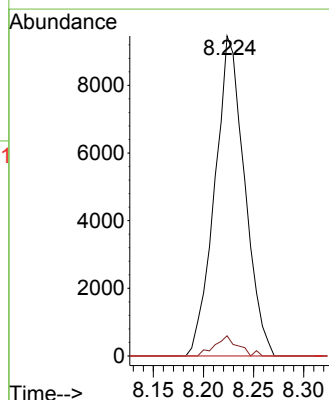



#39

Methylcyclohexane

Concen: 2.522 ug/l

RT: 9.606 min Scan# 1131

Delta R.T. 0.006 min

Lab File: VN082264.D

Acq: 22 May 2024 01:33

Instrument :

MSVOA_N

ClientSampleId :

4





Tgt Ion: 83 Resp: 8764

Ion Ratio Lower Upper

83 100

55 71.9 53.0 79.6

98 46.5 37.1 55.7

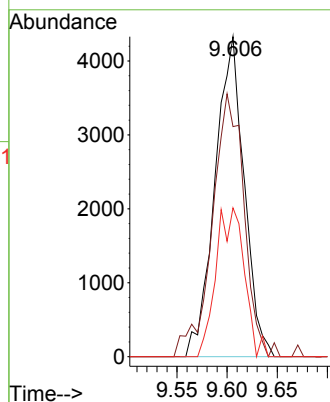

#40

Benzene

Concen: 2.722 ug/l

RT: 8.612 min Scan# 1132

Delta R.T. 0.006 min

Lab File: VN082264.D




Acq: 22 May 2024 01:33


Tgt Ion: 78 Resp: 25734

Ion Ratio Lower Upper

78 100

77 25.0 20.0 30.0









#43
Isopropyl Acetate
Concen: 0.866 ug/l
RT: 8.682 min Scan# 1144
Delta R.T. -0.006 min
Lab File: VN082264.D
Acq: 22 May 2024 01:33




Instrument :
MSVOA_N
ClientSampleId :
4


Tgt Ion: 43 Resp: 5447
Ion Ratio Lower Upper
43 100
61 0.0 22.8 34.2#
87 0.0 12.0 18.0#

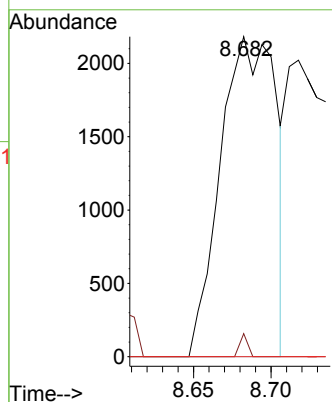

#50
Toluene-d8
Concen: 53.515 ug/l
RT: 10.570 min Scan# 1465
Delta R.T. -0.000 min
Lab File: VN082264.D
Acq: 22 May 2024 01:33

Tgt Ion: 98 Resp: 387830
Ion Ratio Lower Upper
98 100
100 64.4 51.8 77.6

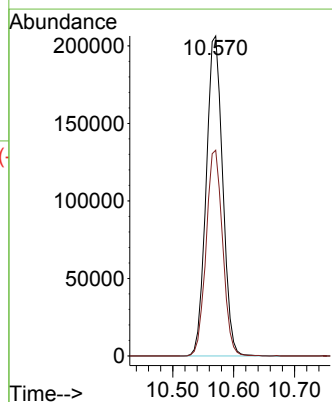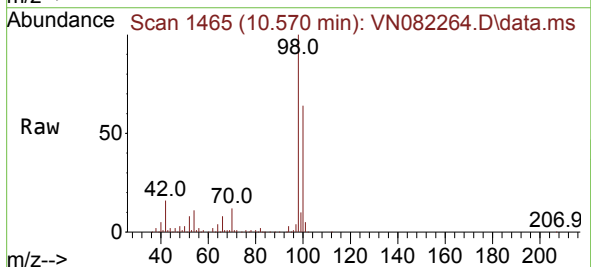



#52

Toluene

Concen: 8.097 ug/l

RT: 10.635 min Scan# 14

Delta R.T. 0.006 min

Lab File: VN082264.D

Acq: 22 May 2024 01:33

Instrument :

MSVOA_N

ClientSampleId :





4

Tgt Ion: 92 Resp: 45939

Ion Ratio Lower Upper

92 100

91 173.7 136.7 205.1

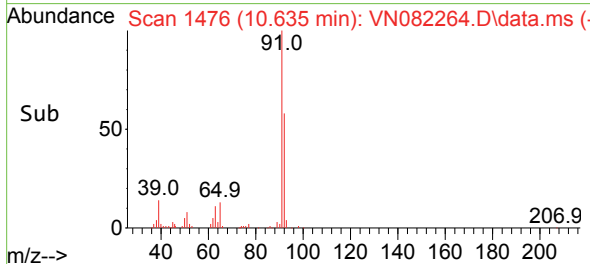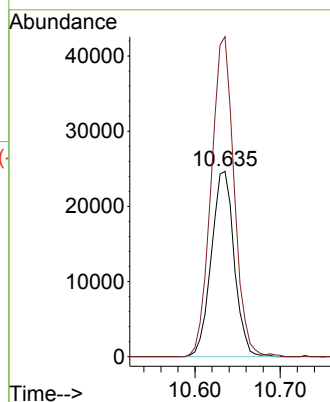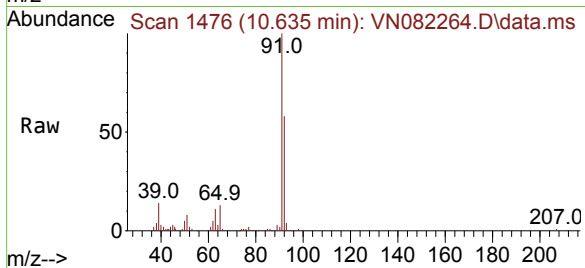

#55

1,1,2-Trichloroethane

Concen: 0.492 ug/l

RT: 11.006 min Scan# 1539

Delta R.T. -0.012 min

Lab File: VN082264.D

Acq: 22 May 2024 01:33

Tgt Ion: 97 Resp: 1015




Ion Ratio Lower Upper


97 100

83 0.0 70.4 105.6#

85 0.0 45.6 68.4#

99 0.0 50.9 76.3#


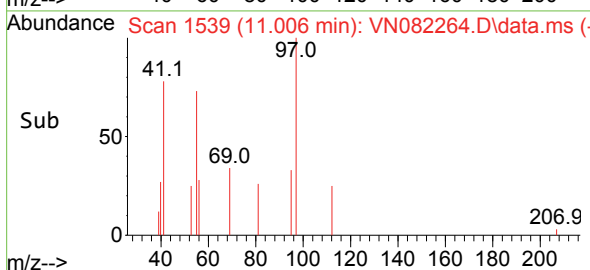

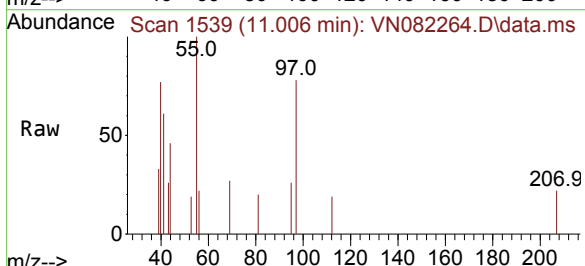




#59
2-Hexanone
Concen: 0.624 ug/l
RT: 11.170 min Scan# 11
Delta R.T. -0.024 min
Lab File: VN082264.D
Acq: 22 May 2024 01:33




Instrument :
MSVOA_N
ClientSampleId :
4


Tgt Ion: 43 Resp: 1631
Ion Ratio Lower Upper
43 100
58 0.0 28.3 84.9#

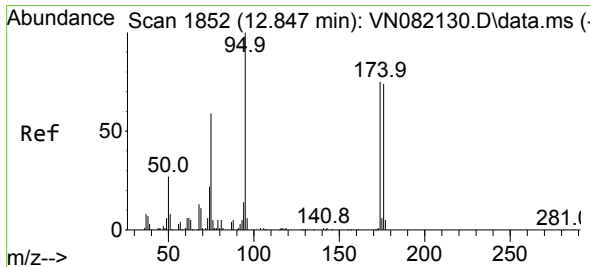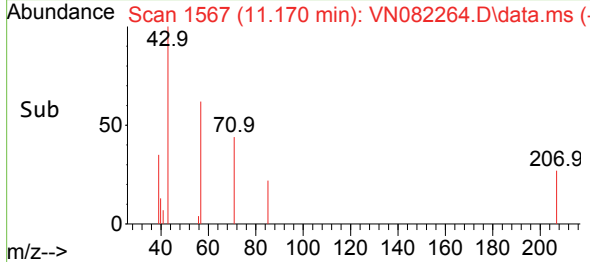

#62
4-Bromofluorobenzene
Concen: 54.606 ug/l
RT: 12.853 min Scan# 1853
Delta R.T. 0.006 min
Lab File: VN082264.D
Acq: 22 May 2024 01:33

Tgt Ion: 95 Resp: 141248
Ion Ratio Lower Upper
95 100
174 75.9 0.0 160.6
176 73.2 0.0 152.8


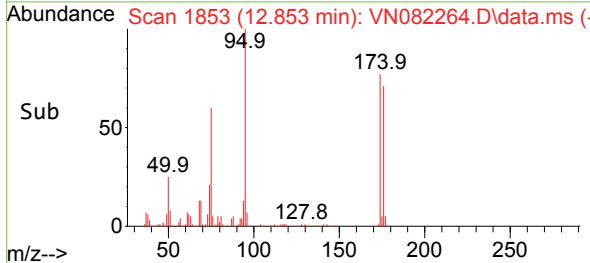
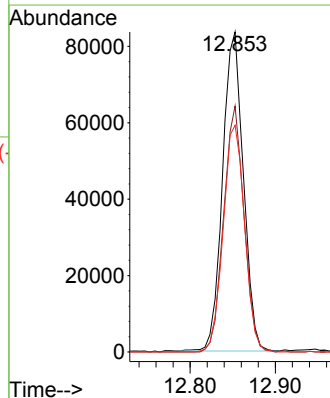
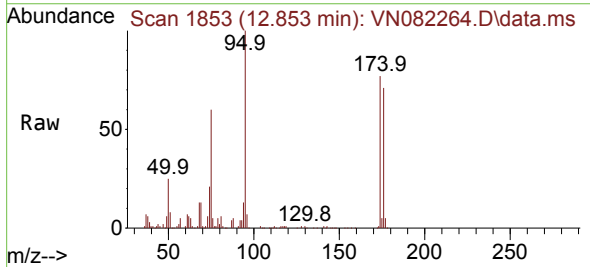




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.870 min Scan# 11
Delta R.T. 0.006 min
Lab File: VN082264.D
Acq: 22 May 2024 01:33




Instrument :
MSVOA_N
ClientSampleId :
4


Tgt Ion:117 Resp: 294114
Ion Ratio Lower Upper
117 100
82 57.6 44.6 66.8
119 30.7 25.9 38.9



#67
Ethyl Benzene
Concen: 2.658 ug/l
RT: 11.964 min Scan# 1702
Delta R.T. -0.000 min
Lab File: VN082264.D
Acq: 22 May 2024 01:33

Tgt Ion: 91 Resp: 30890
Ion Ratio Lower Upper
91 100
106 31.2 25.3 37.9




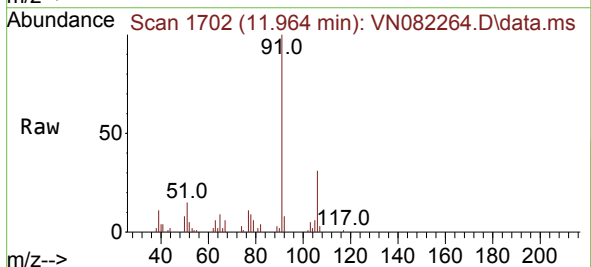




#68
m/p-Xylenes
Concen: 15.831 ug/l
RT: 12.064 min Scan# 1719
Delta R.T. -0.006 min
Lab File: VN082264.D
Acq: 22 May 2024 01:33




Instrument :
MSVOA_N
ClientSampleId :
4


Tgt Ion:106 Resp: 67440
Ion Ratio Lower Upper
106 100
91 209.4 159.4 239.0



#69
o-Xylene
Concen: 14.538 ug/l
RT: 12.400 min Scan# 1776
Delta R.T. -0.000 min
Lab File: VN082264.D
Acq: 22 May 2024 01:33

Tgt Ion:106 Resp: 59989
Ion Ratio Lower Upper
106 100
91 222.1 104.7 314.1









#70
Styrene
Concen: 2.239 ug/l
RT: 12.406 min Scan# 11
Delta R.T. -0.006 min
Lab File: VN082264.D
Acq: 22 May 2024 01:33




Instrument :
MSVOA_N
ClientSampleId :
4


Tgt Ion	Ratio	Lower	Upper
104	100		
78	100.5	38.6	58.0#
103	90.8	43.8	65.6#

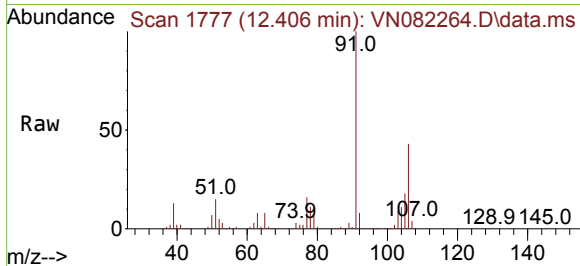

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.794 min Scan# 2013
Delta R.T. -0.000 min
Lab File: VN082264.D
Acq: 22 May 2024 01:33

Tgt Ion	Ratio	Lower	Upper
152	100		
115	62.6	30.4	91.3
150	154.0	0.0	353.2




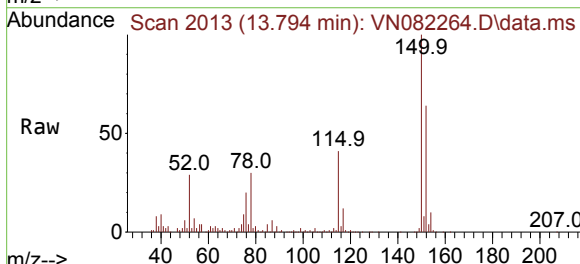




#73
Isopropylbenzene
Concen: 0.687 ug/l
RT: 12.694 min Scan# 11
Delta R.T. -0.000 min
Lab File: VN082264.D
Acq: 22 May 2024 01:33




Instrument :
MSVOA_N
ClientSampleId :
4


Tgt Ion:105 Resp: 7617
Ion Ratio Lower Upper
105 100
120 27.1 13.4 40.1

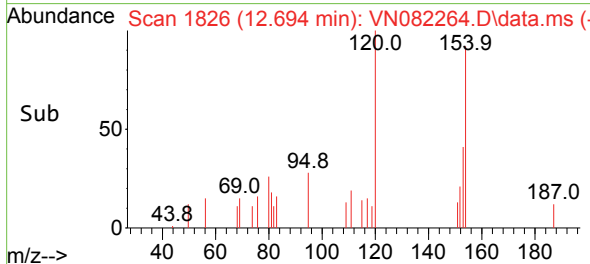

#74
N-ethyl acetate
Concen: 0.341 ug/l
RT: 12.482 min Scan# 1790
Delta R.T. -0.012 min
Lab File: VN082264.D
Acq: 22 May 2024 01:33

Tgt Ion: 43 Resp: 2083
Ion Ratio Lower Upper
43 100
70 28.5 39.0 58.4#
55 53.0 21.3 31.9#
61 0.0 20.5 30.7#

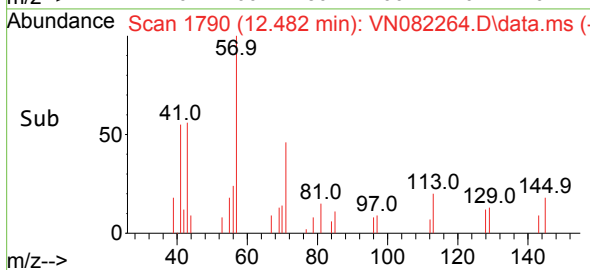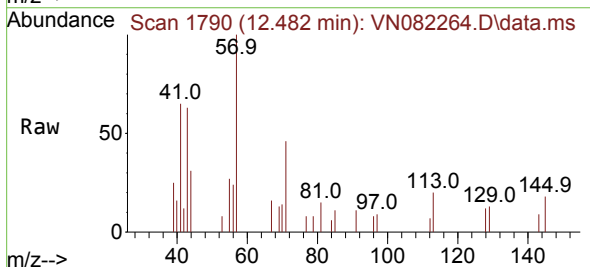



#76

1,2,3-Trichloropropane

Concen: 28.580 ug/l

RT: 12.853 min Scan# 1853

Delta R.T. -0.141 min

Lab File: VN082264.D

Acq: 22 May 2024 01:33

Instrument :

MSVOA_N

ClientSampleId :





4

Tgt Ion: 75 Resp: 84004

Ion Ratio Lower Upper

75 100

77 1.9 90.5 271.3#

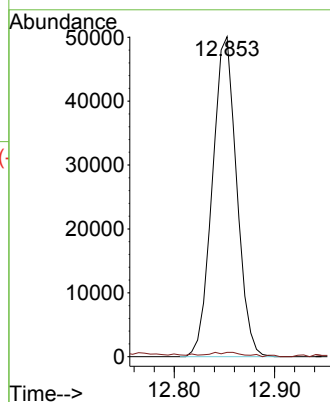

#78

n-propylbenzene

Concen: 1.094 ug/l

RT: 13.035 min Scan# 1884

Delta R.T. -0.000 min

Lab File: VN082264.D




Acq: 22 May 2024 01:33


Tgt Ion: 91 Resp: 14376

Ion Ratio Lower Upper

91 100

120 22.6 11.7 35.0





#79

2-Chlorotoluene

Concen: 0.263 ug/l

RT: 13.129 min Scan# 1900

Delta R.T. -0.000 min

Lab File: VN082264.D

Acq: 22 May 2024 01:33

Instrument :

MSVOA_N

ClientSampleId :





4

Tgt Ion: 91 Resp: 2171

Ion Ratio Lower Upper

91 100

126 5.5 17.5 52.5#

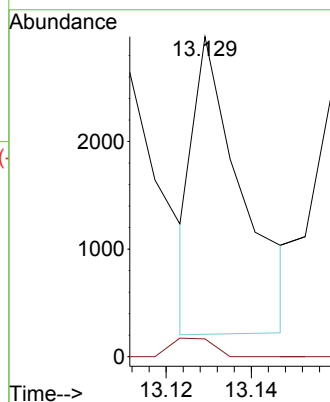

#80

1,3,5-Trimethylbenzene

Concen: 11.464 ug/l

RT: 13.176 min Scan# 1908

Delta R.T. -0.000 min

Lab File: VN082264.D




Acq: 22 May 2024 01:33


Tgt Ion: 105 Resp: 102839

Ion Ratio Lower Upper

105 100

120 47.7 24.8 74.3







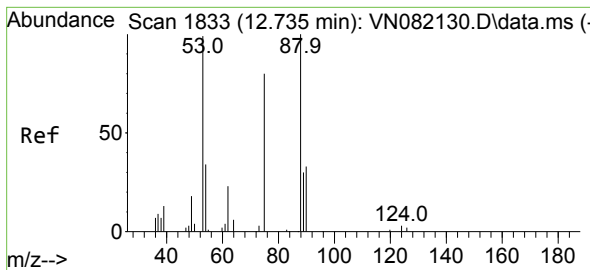

#81
 trans-1,4-Dichloro-2-butene
 Concen: 66.847 ug/l
 RT: 12.853 min Scan# 1853
 Delta R.T. 0.117 min
 Lab File: VN082264.D
 Acq: 22 May 2024 01:33




Instrument :
 MSVOA_N
 ClientSampleId :
 4


Tgt Ion: 75 Resp: 84004
 Ion Ratio Lower Upper
 75 100
 53 0.3 72.9 109.3#
 89 0.1 39.1 58.7#

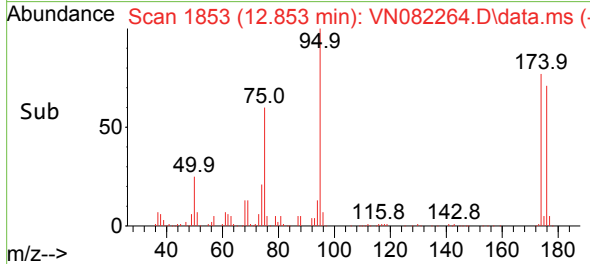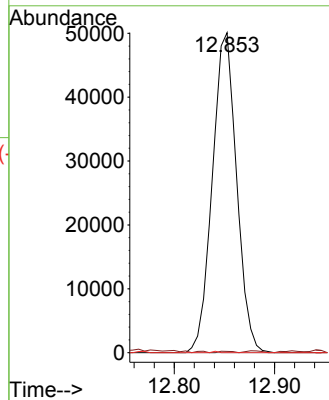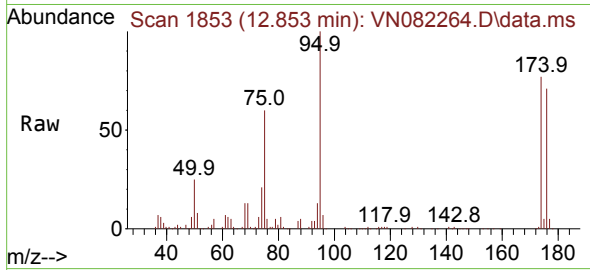

#82
 4-Chlorotoluene
 Concen: 1.446 ug/l
 RT: 13.176 min Scan# 1908
 Delta R.T. -0.047 min
 Lab File: VN082264.D
 Acq: 22 May 2024 01:33

Tgt Ion: 91 Resp: 11665
 Ion Ratio Lower Upper
 91 100
 126 0.5 17.4 52.3#

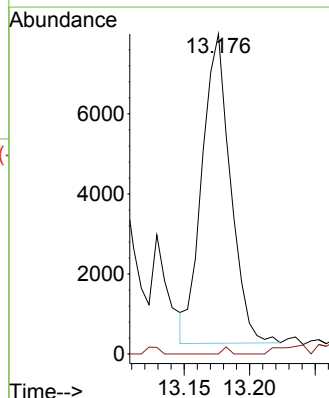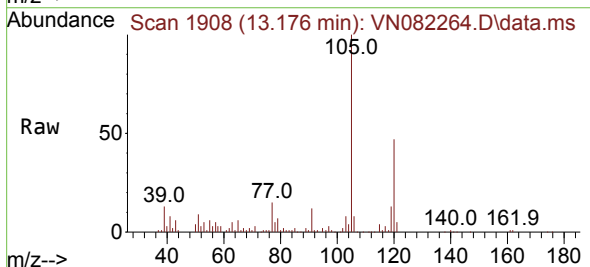



#83

tert-Butylbenzene

Concen: 3.315 ug/l

RT: 13.482 min Scan# 1960

Delta R.T. 0.041 min

Lab File: VN082264.D

Acq: 22 May 2024 01:33

Instrument :

MSVOA_N

ClientSampleId :

4





Tgt Ion:119 Resp: 26017

Ion Ratio Lower Upper

119 100

91 94.1 32.6 97.8

134 0.0 12.4 37.0#

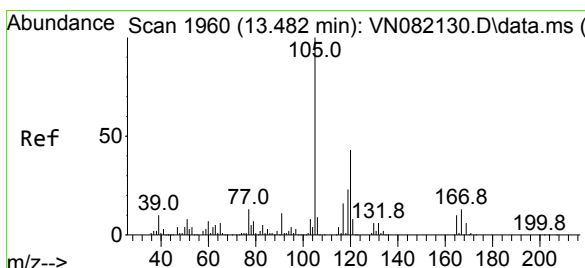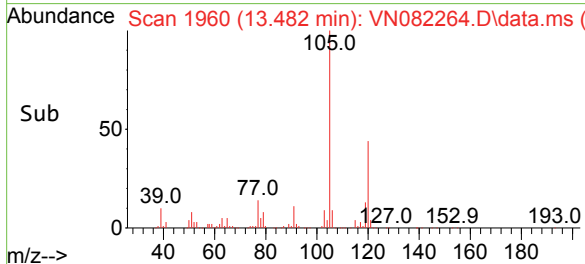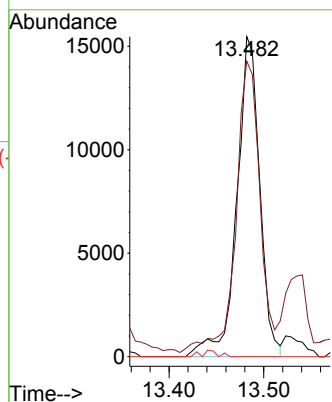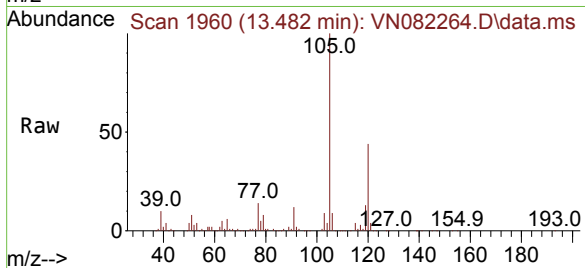

#84

1,2,4-Trimethylbenzene

Concen: 21.818 ug/l

RT: 13.482 min Scan# 1960

Delta R.T. -0.000 min

Lab File: VN082264.D




Acq: 22 May 2024 01:33


Tgt Ion:105 Resp: 200248

Ion Ratio Lower Upper

105 100

120 43.9 22.9 68.7


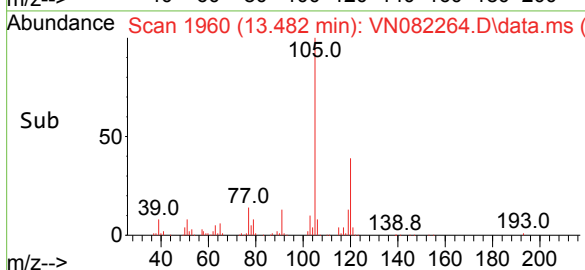
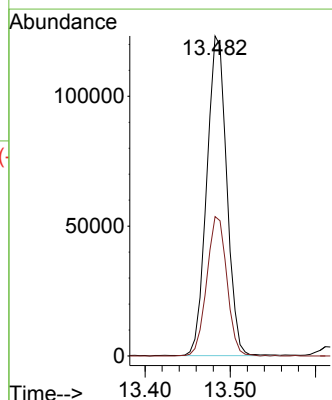
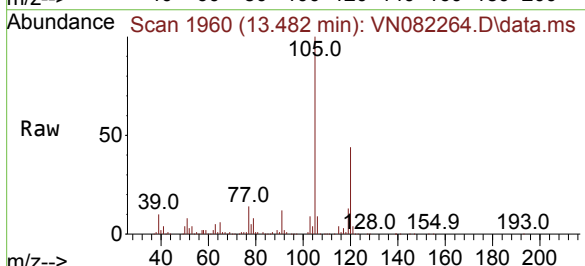




#85
 sec-Butylbenzene
 Concen: 0.565 ug/l
 RT: 13.611 min Scan# 1983
 Delta R.T. -0.006 min
 Lab File: VN082264.D
 Acq: 22 May 2024 01:33




Instrument :
 MSVOA_N
 ClientSampleId :
 4


Tgt Ion:105 Resp: 6147
 Ion Ratio Lower Upper
 105 100
 134 36.2 10.2 30.4#

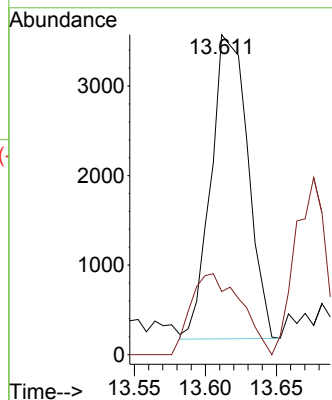

#86
 p-Isopropyltoluene
 Concen: 0.820 ug/l
 RT: 13.729 min Scan# 2002
 Delta R.T. -0.000 min
 Lab File: VN082264.D
 Acq: 22 May 2024 01:33

Tgt Ion:119 Resp: 7249
 Ion Ratio Lower Upper
 119 100
 134 27.0 13.2 39.5
 91 33.4 11.8 35.3

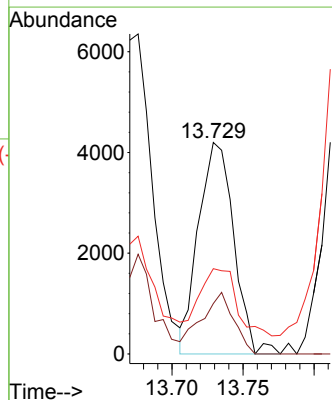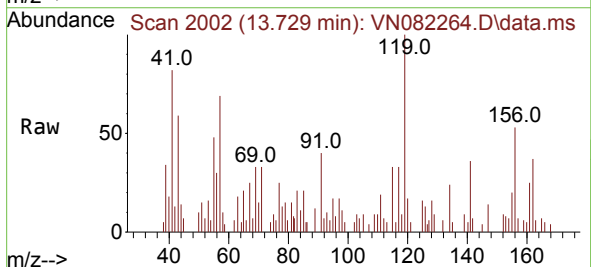



#89

n-Butylbenzene

Concen: 0.506 ug/l

RT: 14.058 min Scan# 2058

Delta R.T. -0.000 min

Lab File: VN082264.D

Acq: 22 May 2024 01:33

Instrument :

MSVOA_N

ClientSampleId :

4





Tgt Ion: 91 Resp: 4019

Ion Ratio Lower Upper

91 100

92 107.2 26.2 78.5#

134 0.0 13.2 39.5#

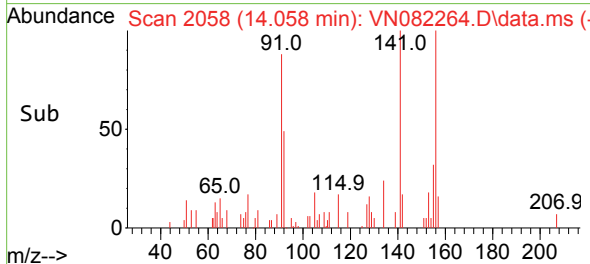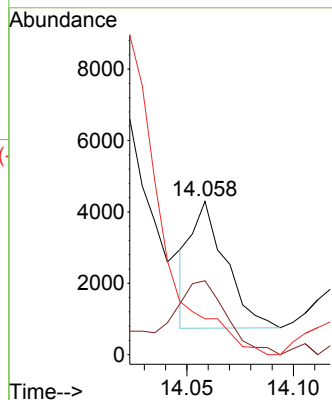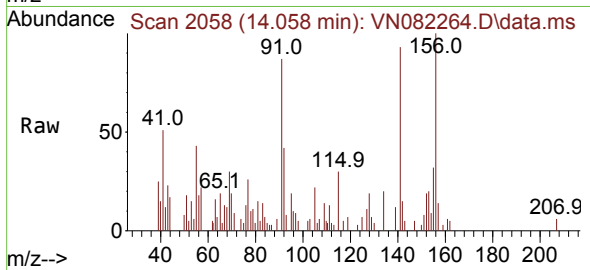

#90

Hexachloroethane

Concen: 2.165 ug/l

RT: 14.335 min Scan# 2105

Delta R.T. -0.000 min

Lab File: VN082264.D




Acq: 22 May 2024 01:33


Tgt Ion: 117 Resp: 3547

Ion Ratio Lower Upper

117 100

201 0.0 33.3 99.8#


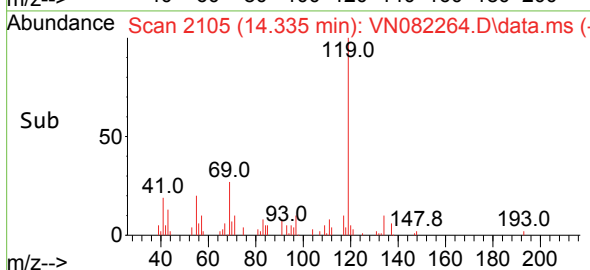
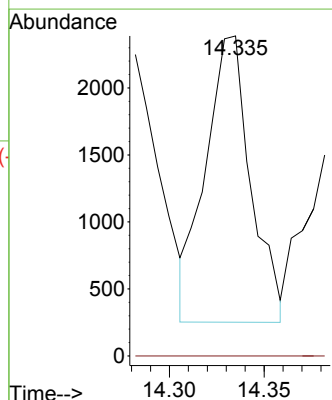
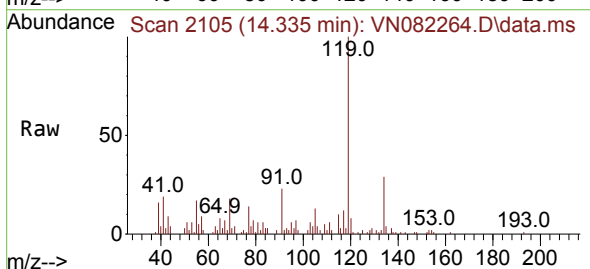


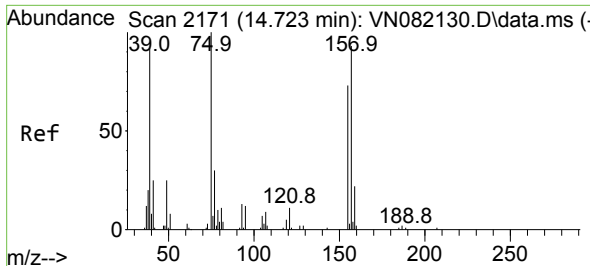

#92
1,2-Dibromo-3-Chloropropane
Concen: 0.577 ug/l
RT: 14.735 min Scan# 2173
Delta R.T. 0.012 min
Lab File: VN082264.D
Acq: 22 May 2024 01:33

Instrument :
MSVOA_N
ClientSampleId :
4

Tgt Ion: 75 Resp: 379
Ion Ratio Lower Upper
75 100
155 0.0 42.6 128.0#
157 0.0 53.0 159.0#

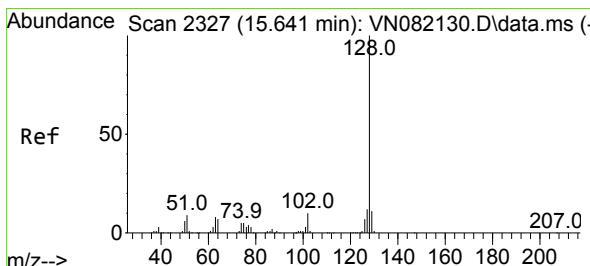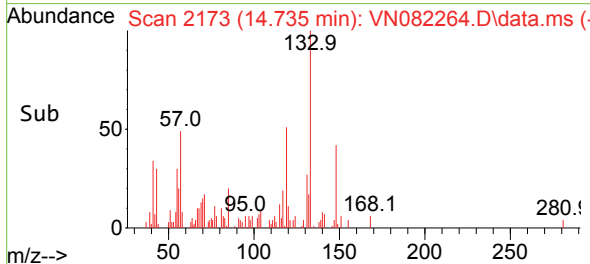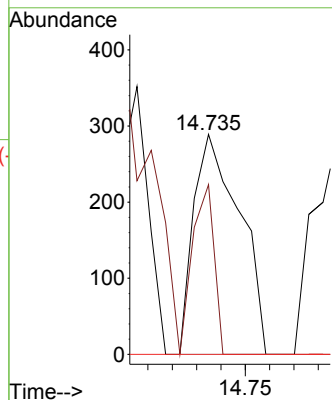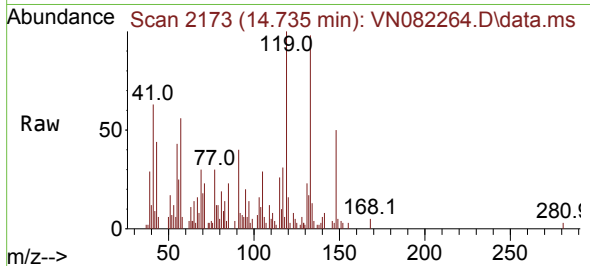

#95
Naphthalene
Concen: 356.778 ug/l
RT: 15.641 min Scan# 2327
Delta R.T. -0.000 min
Lab File: VN082264.D
Acq: 22 May 2024 01:33

Tgt Ion: 128 Resp: 2841646
Ion Ratio Lower Upper
128 100
127 13.3 10.1 15.1
129 10.8 8.9 13.3

