

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN052124\
 Data File : VN082272.D
 Acq On : 22 May 2024 04:45
 Operator : JC\MD
 Sample : P2494-12 40X
 Misc : 5.03g/10mL/100uL/5.00mL/MSVOA_N/MEOH
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 12

Quant Time: May 22 07:40:35 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N051524W.M
 Quant Title : SW846 8260
 QLast Update : Thu May 16 05:21:06 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	8.224	168	200939	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	9.100	114	344733	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.865	117	329881	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.794	152	154717	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.577	65	156139	49.211	ug/l	0.00
Spiked Amount 50.000	Range 74 - 125		Recovery =	98.420%		
35) Dibromofluoromethane	8.165	113	107795	50.831	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery =	101.660%		
50) Toluene-d8	10.571	98	438440	53.926	ug/l	0.00
Spiked Amount 50.000	Range 86 - 113		Recovery =	107.860%		
62) 4-Bromofluorobenzene	12.847	95	167180	57.610	ug/l	0.00
Spiked Amount 50.000	Range 64 - 133		Recovery =	115.220%		
Target Compounds						Qvalue
16) Acetone	4.441	43	681	0.523	ug/l #	43
20) Methylene Chloride	5.289	84	1250	0.476	ug/l #	86
31) Cyclohexane	8.229	56	8652	1.707	ug/l #	56
36) 1,1-Dichloropropene	8.224	75	18026	5.068	ug/l #	50
38) Carbon Tetrachloride	8.224	117	22399	6.213	ug/l #	14
39) Methylcyclohexane	9.600	83	4718	1.210	ug/l	93
40) Benzene	8.606	78	20433	1.927	ug/l	91
43) Isopropyl Acetate	8.712	43	6101	0.865	ug/l #	52
52) Toluene	10.629	92	36532	5.740	ug/l	99
55) 1,1,2-Trichloroethane	11.012	97	518	0.224	ug/l #	43
67) Ethyl Benzene	11.965	91	22830	1.751	ug/l	99
68) m/p-Xylenes	12.070	106	51726	10.826	ug/l	87
69) o-Xylene	12.400	106	44475	9.610	ug/l	90
70) Styrene	12.406	104	9346	1.216	ug/l #	18
71) Bromoform	12.688	173	57	0.730	ug/l #	28
73) Isopropylbenzene	12.700	105	6176	0.502	ug/l	87
74) N-amyl acetate	12.488	43	1413	0.209	ug/l #	47
76) 1,2,3-Trichloropropane	12.847	75	97692	30.000	ug/l #	1
78) n-propylbenzene	13.041	91	10761	0.739	ug/l	95
79) 2-Chlorotoluene	13.100	91	7243	0.792	ug/l #	40
80) 1,3,5-Trimethylbenzene	13.176	105	70591	7.103	ug/l	96
81) trans-1,4-Dichloro-2-b...	12.847	75	97692	70.168	ug/l #	13
82) 4-Chlorotoluene	13.176	91	8270	0.925	ug/l #	40
83) tert-Butylbenzene	13.670	119	6847	0.787	ug/l	73
84) 1,2,4-Trimethylbenzene	13.482	105	144853	14.246	ug/l	96
85) sec-Butylbenzene	13.482	105	144853	12.019	ug/l #	56
86) p-Isopropyltoluene	13.729	119	4799	0.490	ug/l	93
89) n-Butylbenzene	14.059	91	2980	0.339	ug/l #	64
90) Hexachloroethane	14.329	117	2700	1.488	ug/l #	17
92) 1,2-Dibromo-3-Chloropr...	14.735	75	181	0.249	ug/l #	2
95) Naphthalene	15.641	128	1834890	207.941	ug/l	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN052124\
Data File : VN082272.D
Acq On : 22 May 2024 04:45
Operator : JC\MD
Sample : P2494-12 40X
Misc : 5.03g/10mL/100uL/5.00mL/MSVOA_N/MEOH
ALS Vial : 47 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
12

Quant Time: May 22 07:40:35 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N051524W.M
Quant Title : SW846 8260
QLast Update : Thu May 16 05:21:06 2024
Response via : Initial Calibration

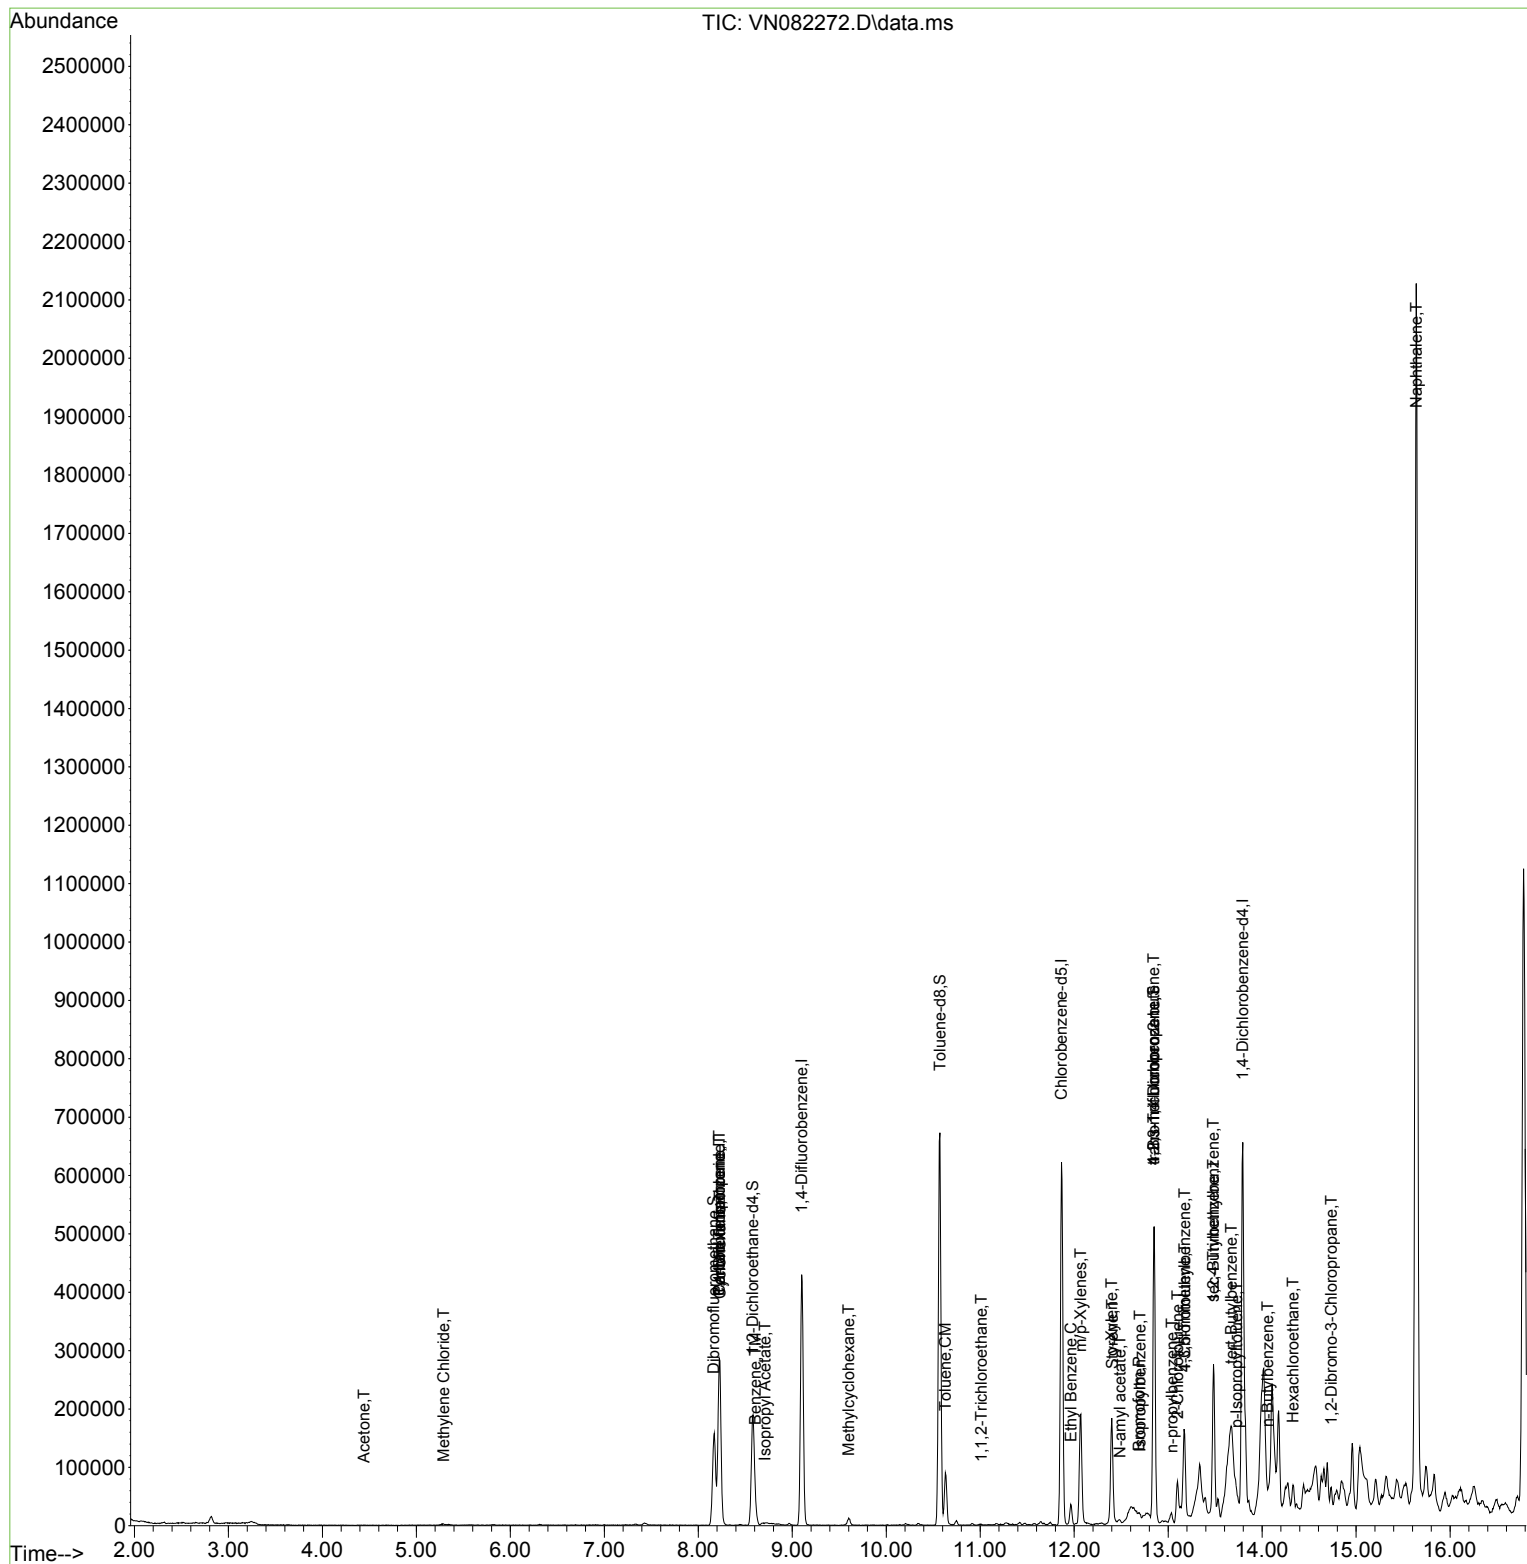



#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 8.224 min Scan# 1

Delta R.T. -0.000 min

Lab File: VN082272.D

Acq: 22 May 2024 04:45

Instrument :

MSVOA_N

ClientSampleId :





12

Tgt Ion:168 Resp: 200939

Ion Ratio Lower Upper

168 100

99 62.8 48.2 72.4

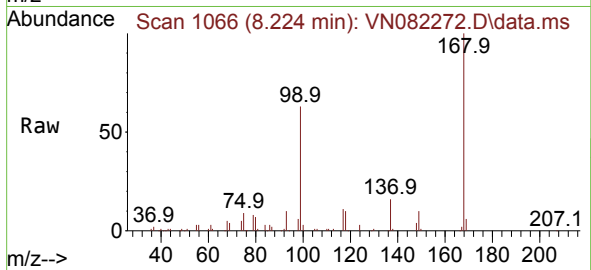

#16

Acetone

Concen: 0.523 ug/l

RT: 4.441 min Scan# 423

Delta R.T. 0.018 min

Lab File: VN082272.D




Acq: 22 May 2024 04:45


Tgt Ion: 43 Resp: 681

Ion Ratio Lower Upper

43 100


58 0.0 25.2 37.8#

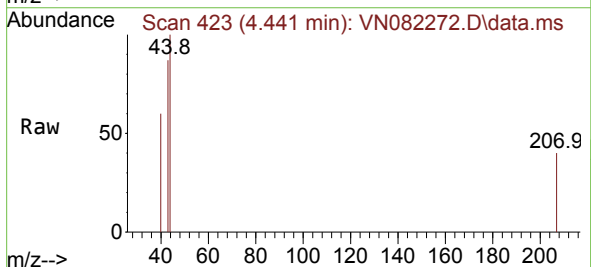



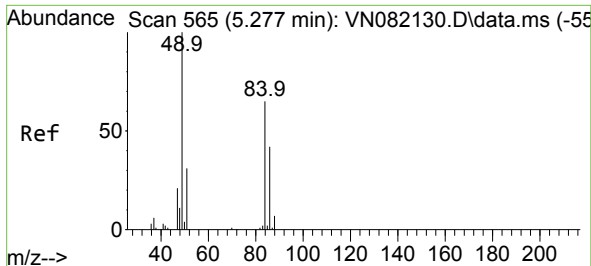


#20
Methylene Chloride
Concen: 0.476 ug/l
RT: 5.289 min Scan# 51
Delta R.T. 0.012 min
Lab File: VN082272.D
Acq: 22 May 2024 04:45

Instrument :
MSVOA_N
ClientSampleId :
12







Tgt Ion:	84	Resp:	1250
Ion	Ratio	Lower	Upper
84	100		
49	110.2	84.9	127.3
51	51.2	27.0	40.6#
86	48.4	52.3	78.5#

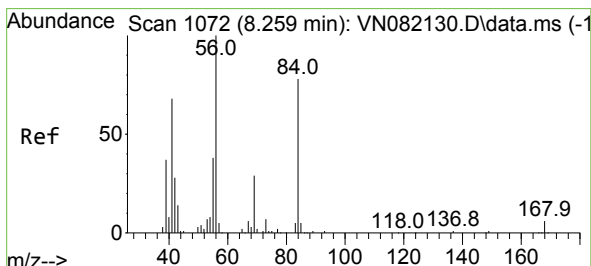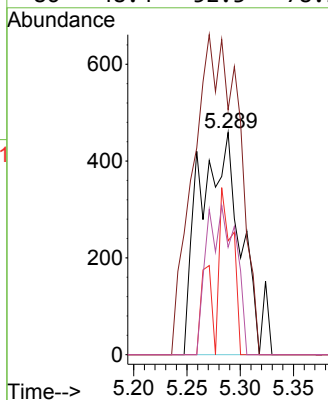

#31
Cyclohexane
Concen: 1.707 ug/l
RT: 8.229 min Scan# 1067
Delta R.T. -0.030 min
Lab File: VN082272.D
Acq: 22 May 2024 04:45

Tgt Ion:	56	Resp:	8652
Ion	Ratio	Lower	Upper
56	100		
69	126.8	24.4	36.6#
84	94.3	77.0	115.4

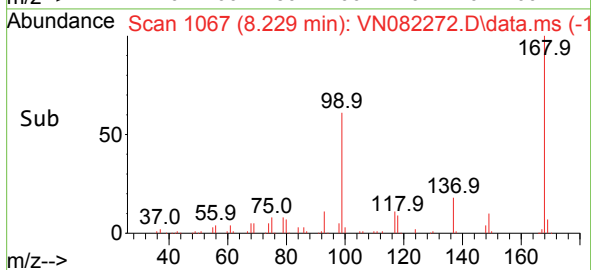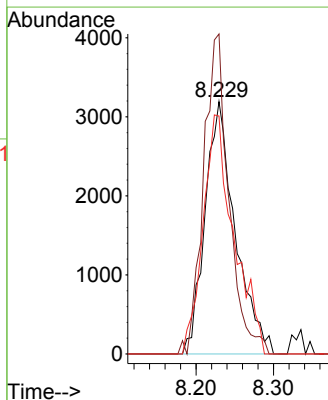

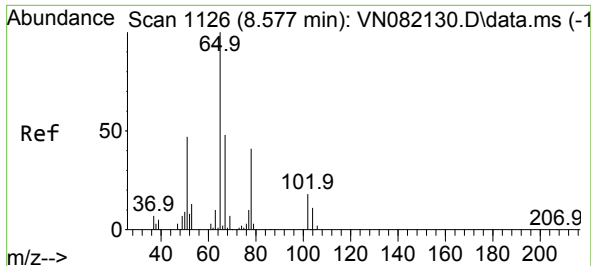

#33

1,2-Dichloroethane-d4

Concen: 49.211 ug/l

RT: 8.577 min Scan# 1126

Delta R.T. -0.000 min

Lab File: VN082272.D

Acq: 22 May 2024 04:45

Instrument :

MSVOA_N

ClientSampleId :





12

Tgt Ion: 65 Resp: 156139

Ion Ratio Lower Upper

65 100

67 50.0 0.0 103.0



#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 9.100 min Scan# 1215

Delta R.T. -0.000 min

Lab File: VN082272.D

Acq: 22 May 2024 04:45




Tgt Ion: 114 Resp: 344733


Ion Ratio Lower Upper

114 100

63 23.6 0.0 41.0

88 16.2 0.0 31.4


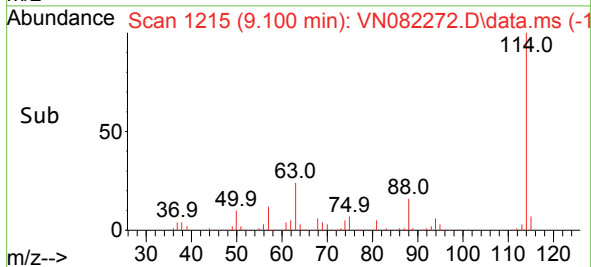

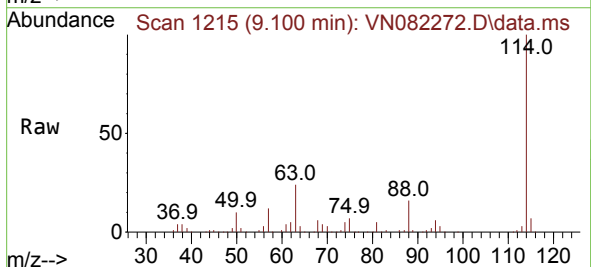


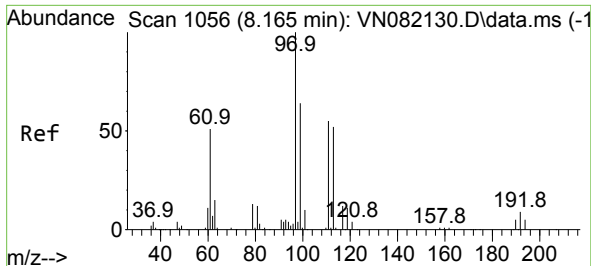

#35
Dibromofluoromethane
Concen: 50.831 ug/l
RT: 8.165 min Scan# 1056
Delta R.T. -0.000 min
Lab File: VN082272.D
Acq: 22 May 2024 04:45




Instrument :
MSVOA_N
ClientSampleId :
12


Tgt Ion:113 Resp: 107795
Ion Ratio Lower Upper
113 100
111 104.4 83.4 125.2
192 19.2 14.0 21.0

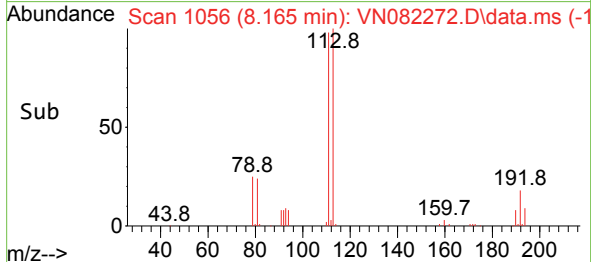

#36
1,1-Dichloropropene
Concen: 5.068 ug/l
RT: 8.224 min Scan# 1066
Delta R.T. -0.147 min
Lab File: VN082272.D
Acq: 22 May 2024 04:45

Tgt Ion: 75 Resp: 18026
Ion Ratio Lower Upper
75 100
110 9.7 17.8 53.5#
77 0.0 25.0 37.4#


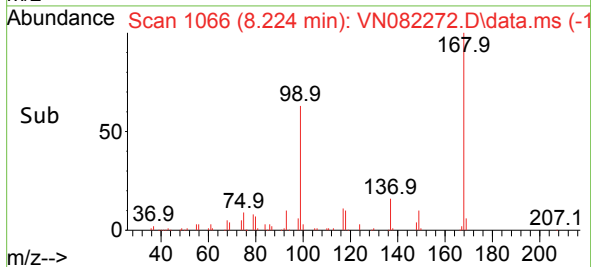

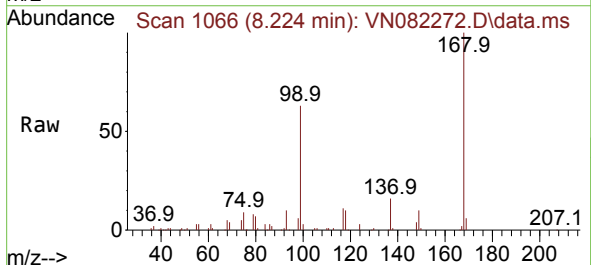




#38
Carbon Tetrachloride
Concen: 6.213 ug/l
RT: 8.224 min Scan# 11
Delta R.T. -0.141 min
Lab File: VN082272.D
Acq: 22 May 2024 04:45




Instrument :
MSVOA_N
ClientSampleId :
12


Tgt Ion:117 Resp: 22399
Ion Ratio Lower Upper
117 100
119 3.0 76.5 114.7#
121 0.0 23.9 35.9#

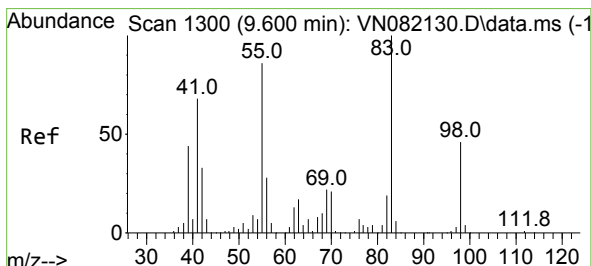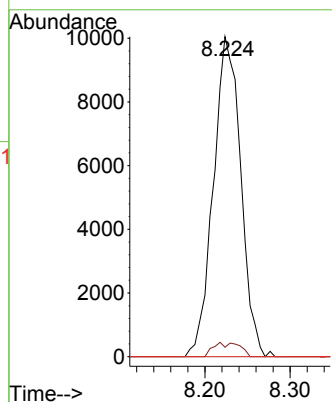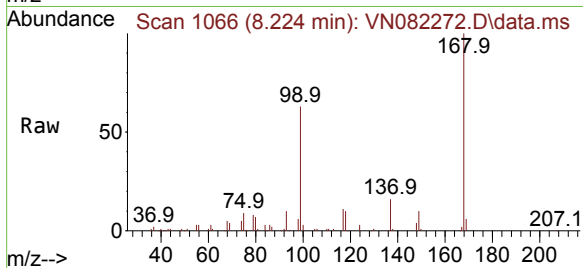

#39
Methylcyclohexane
Concen: 1.210 ug/l
RT: 9.600 min Scan# 1300
Delta R.T. -0.000 min
Lab File: VN082272.D
Acq: 22 May 2024 04:45

Tgt Ion: 83 Resp: 4718
Ion Ratio Lower Upper
83 100
55 73.5 53.0 79.6
98 43.7 37.1 55.7


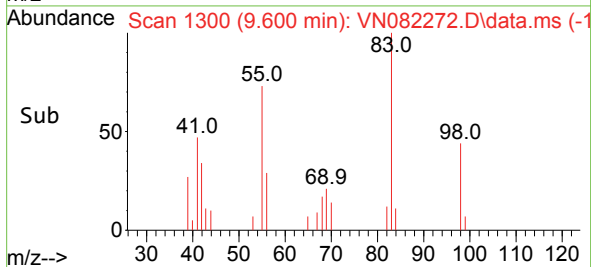
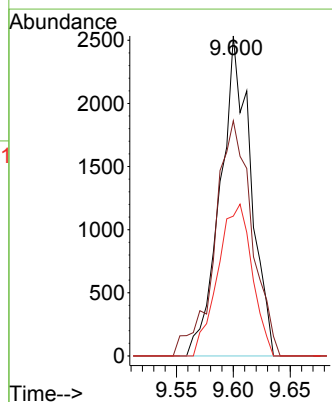
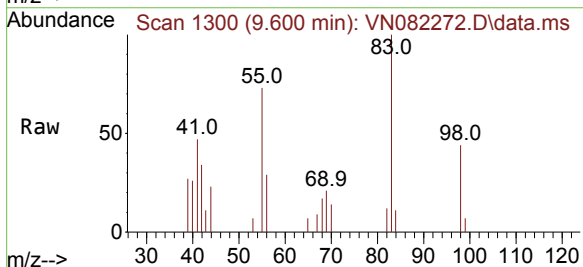




#40
Benzene
Concen: 1.927 ug/l
RT: 8.606 min Scan# 1131
Delta R.T. -0.000 min
Lab File: VN082272.D
Acq: 22 May 2024 04:45




Instrument :
MSVOA_N
ClientSampleId :
12


Tgt Ion: 78 Resp: 20433
Ion Ratio Lower Upper
78 100
77 20.6 20.0 30.0

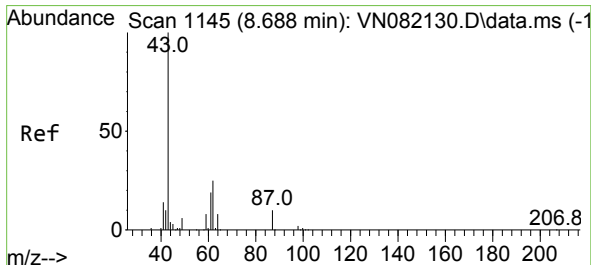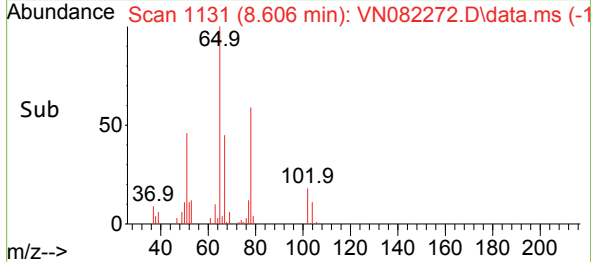

#43
Isopropyl Acetate
Concen: 0.865 ug/l
RT: 8.712 min Scan# 1149
Delta R.T. 0.023 min
Lab File: VN082272.D
Acq: 22 May 2024 04:45

Tgt Ion: 43 Resp: 6101
Ion Ratio Lower Upper
43 100
61 0.0 22.8 34.2#
87 0.0 12.0 18.0#


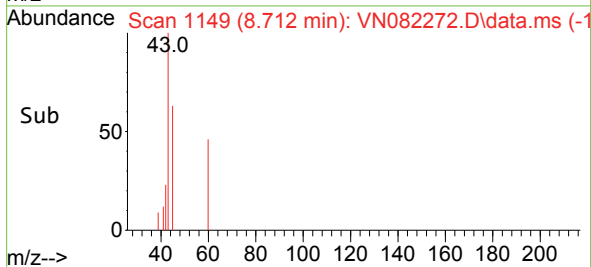
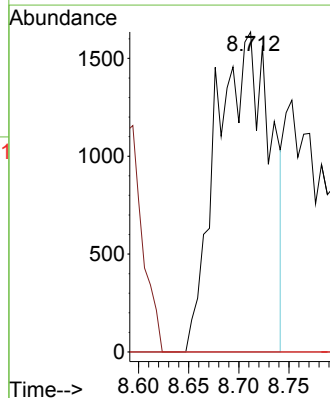
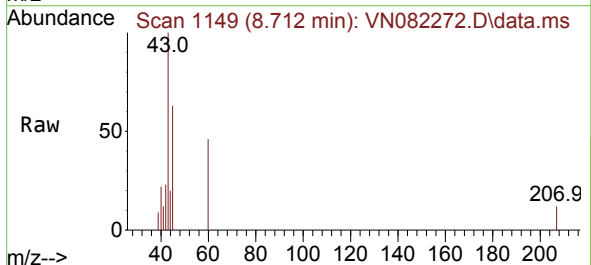




#50
Toluene-d8
Concen: 53.926 ug/l
RT: 10.571 min Scan# 1465
Delta R.T. -0.000 min
Lab File: VN082272.D
Acq: 22 May 2024 04:45




Instrument :
MSVOA_N
ClientSampleId :
12


Tgt Ion: 98 Resp: 438440
Ion Ratio Lower Upper
98 100
100 64.7 51.8 77.6

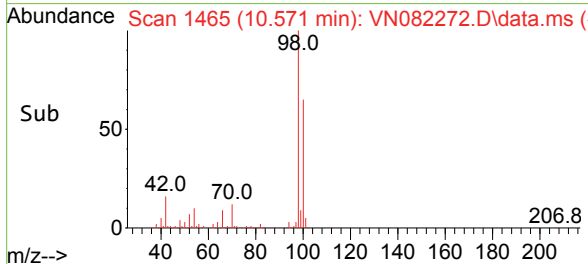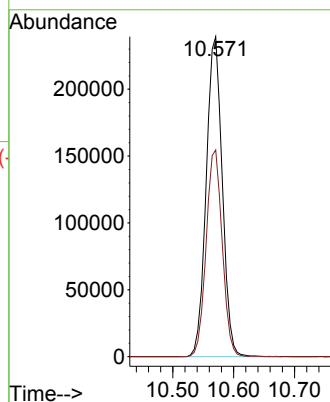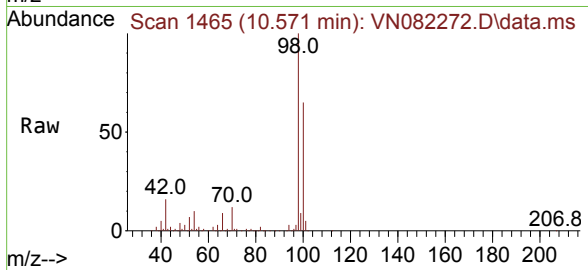

#52
Toluene
Concen: 5.740 ug/l
RT: 10.629 min Scan# 1475
Delta R.T. -0.000 min
Lab File: VN082272.D
Acq: 22 May 2024 04:45

Tgt Ion: 92 Resp: 36532
Ion Ratio Lower Upper
92 100
91 172.2 136.7 205.1




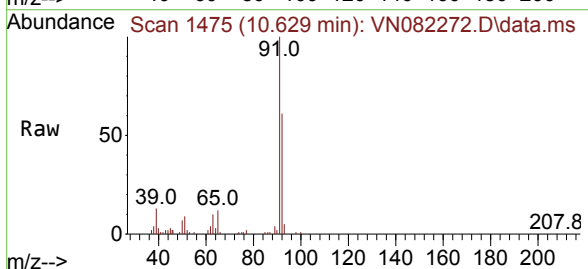


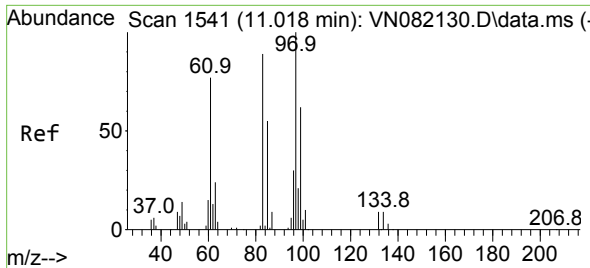

#55
 1,1,2-Trichloroethane
 Concen: 0.224 ug/l
 RT: 11.012 min Scan# 11
 Delta R.T. -0.006 min
 Lab File: VN082272.D
 Acq: 22 May 2024 04:45




Instrument :
 MSVOA_N
 ClientSampleId :
 12


Tgt Ion: 97 Resp: 518
 Ion Ratio Lower Upper
 97 100
 83 64.7 70.4 105.6#
 85 0.0 45.6 68.4#
 99 0.0 50.9 76.3#

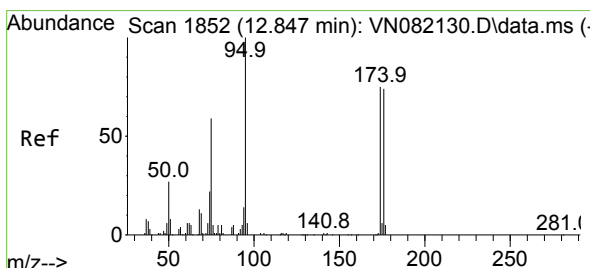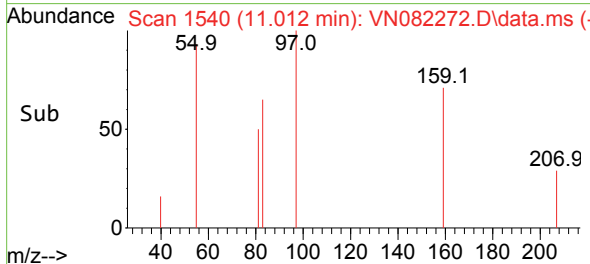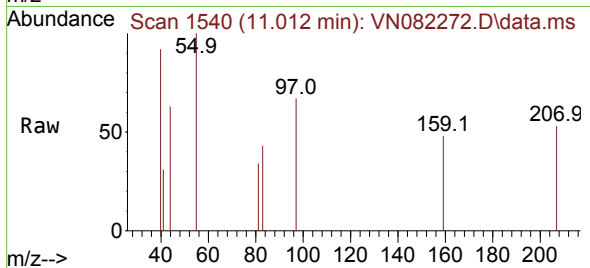

#62
 4-Bromofluorobenzene
 Concen: 57.610 ug/l
 RT: 12.847 min Scan# 1852
 Delta R.T. -0.000 min
 Lab File: VN082272.D
 Acq: 22 May 2024 04:45

Tgt Ion: 95 Resp: 167180
 Ion Ratio Lower Upper
 95 100
 174 74.8 0.0 160.6
 176 72.4 0.0 152.8

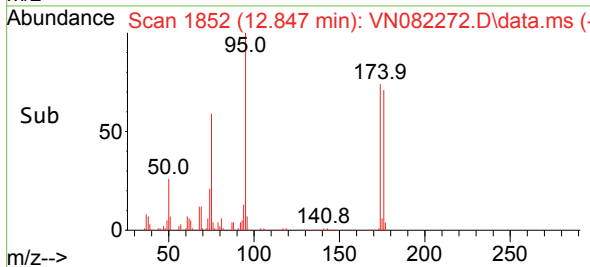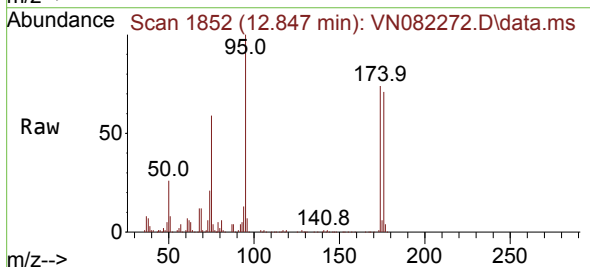



#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 11.865 min Scan# 117

Delta R.T. -0.000 min

Lab File: VN082272.D

Acq: 22 May 2024 04:45

Instrument :

MSVOA_N

ClientSampleId :

12





Tgt Ion:117 Resp: 329881

Ion Ratio Lower Upper

117 100

82 61.5 44.6 66.8

119 31.5 25.9 38.9

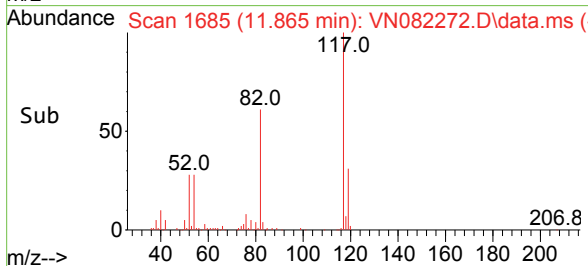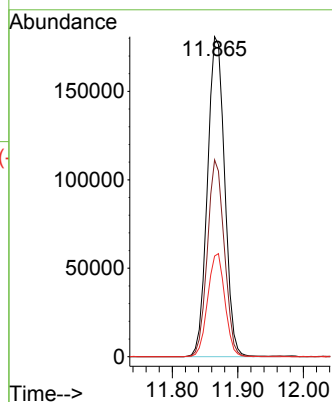

#67

Ethyl Benzene

Concen: 1.751 ug/l

RT: 11.965 min Scan# 1702

Delta R.T. -0.000 min

Lab File: VN082272.D




Acq: 22 May 2024 04:45


Tgt Ion: 91 Resp: 22830

Ion Ratio Lower Upper

91 100

106 32.0 25.3 37.9


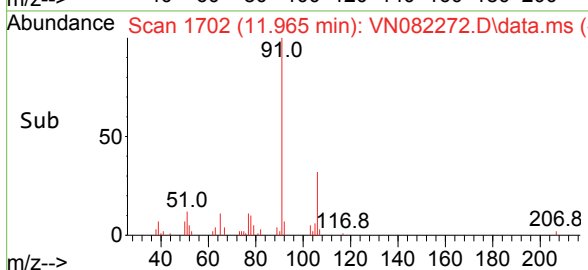

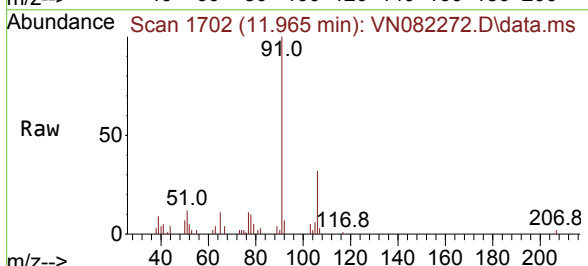




#68
m/p-Xylenes
Concen: 10.826 ug/l
RT: 12.070 min Scan# 1720
Delta R.T. -0.000 min
Lab File: VN082272.D
Acq: 22 May 2024 04:45




Instrument :
MSVOA_N
ClientSampleId :
12


Tgt Ion:106 Resp: 51726
Ion Ratio Lower Upper
106 100
91 218.5 159.4 239.0



#69
o-Xylene
Concen: 9.610 ug/l
RT: 12.400 min Scan# 1776
Delta R.T. -0.000 min
Lab File: VN082272.D
Acq: 22 May 2024 04:45

Tgt Ion:106 Resp: 44475
Ion Ratio Lower Upper
106 100
91 224.3 104.7 314.1

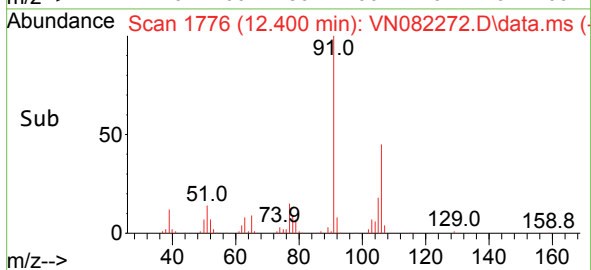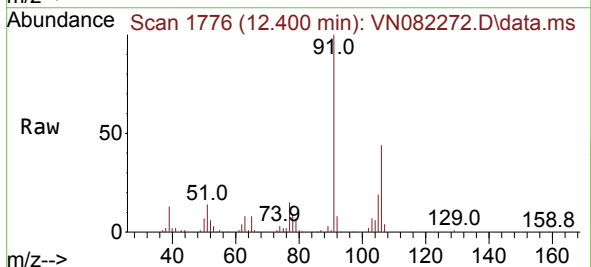



#70

Styrene

Concen: 1.216 ug/l

RT: 12.406 min Scan# 11

Delta R.T. -0.006 min

Lab File: VN082272.D

Acq: 22 May 2024 04:45

Instrument :

MSVOA_N

ClientSampleId :

12





Tgt Ion:104 Resp: 9346

Ion Ratio Lower Upper

104 100

78 115.0 38.6 58.0#

103 103.3 43.8 65.6#

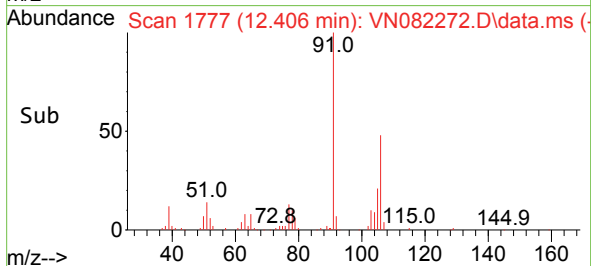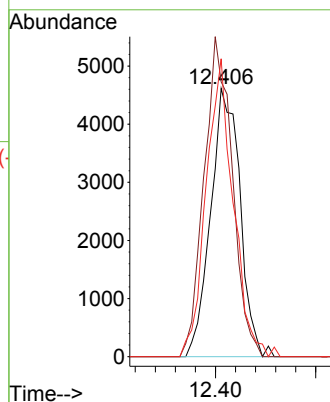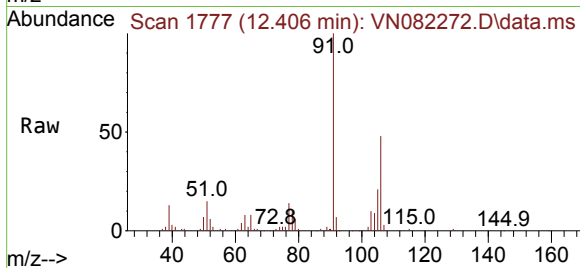

#71

Bromoform

Concen: 0.730 ug/l

RT: 12.688 min Scan# 1825

Delta R.T. 0.112 min

Lab File: VN082272.D

Acq: 22 May 2024 04:45




Tgt Ion:173 Resp: 57


Ion Ratio Lower Upper

173 100

175 0.0 24.6 74.0#

254 0.0 0.0 0.0

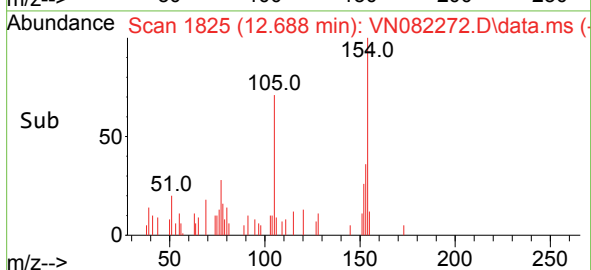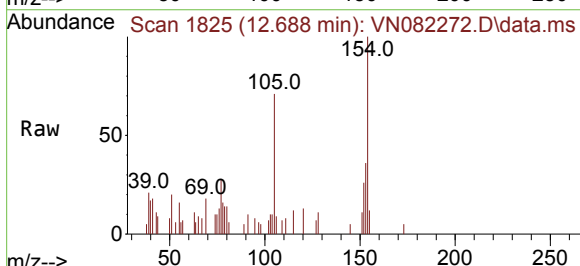



#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.794 min Scan# 2013

Delta R.T. -0.000 min

Lab File: VN082272.D

Acq: 22 May 2024 04:45

Instrument :

MSVOA_N

ClientSampleId :

12





Tgt Ion:152 Resp: 154717

Ion Ratio Lower Upper

152 100

115 62.8 30.4 91.3

150 159.5 0.0 353.2

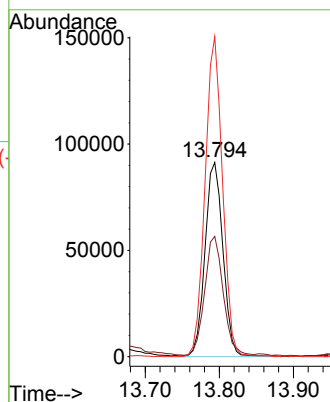

#73

Isopropylbenzene

Concen: 0.502 ug/l

RT: 12.700 min Scan# 1827

Delta R.T. 0.006 min

Lab File: VN082272.D




Acq: 22 May 2024 04:45


Tgt Ion:105 Resp: 6176

Ion Ratio Lower Upper

105 100

120 19.9 13.4 40.1

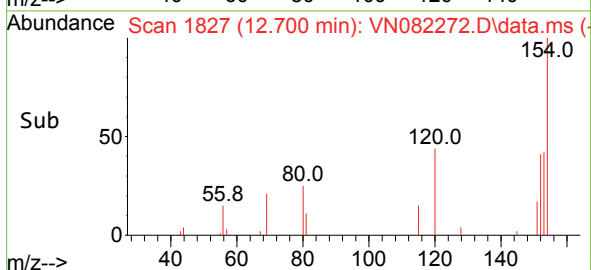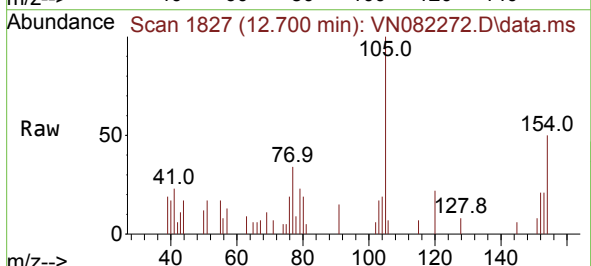



#74

N-amy1 acetate

Concen: 0.209 ug/l

RT: 12.488 min Scan# 1

Delta R.T. -0.006 min

Lab File: VN082272.D


Acq: 22 May 2024 04:45

Instrument :

MSVOA_N

ClientSampleId :

12

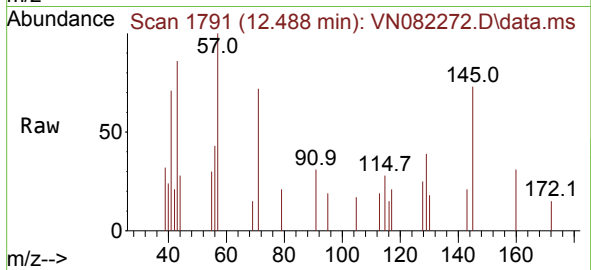

Tgt Ion: 43 Resp: 1413




Ion	Ratio	Lower	Upper
-----	-------	-------	-------

43	100		
----	-----	--	--

70	8.5	39.0	58.4#
----	-----	------	-------

55	49.0	21.3	31.9#
----	------	------	-------

61	0.0	20.5	30.7#
----	-----	------	-------



#76

1,2,3-Trichloropropane

Concen: 30.000 ug/l

RT: 12.847 min Scan# 1852

Delta R.T. -0.147 min

Lab File: VN082272.D




Acq: 22 May 2024 04:45


Tgt Ion: 75 Resp: 97692

Ion	Ratio	Lower	Upper
-----	-------	-------	-------

75	100		
----	-----	--	--

77	2.2	90.5	271.3#
----	-----	------	--------


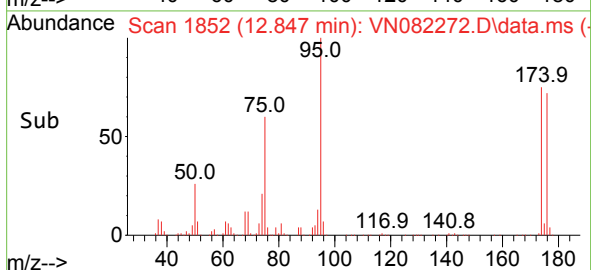
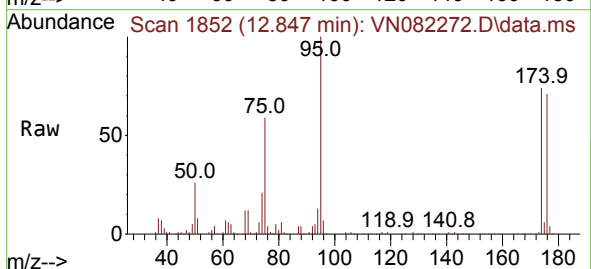



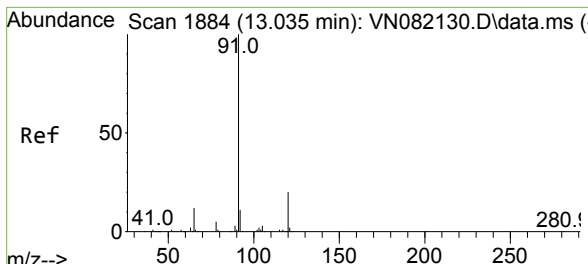

#78
n-propylbenzene
Concen: 0.739 ug/l
RT: 13.041 min Scan# 1885
Delta R.T. 0.006 min
Lab File: VN082272.D
Acq: 22 May 2024 04:45




Instrument :
MSVOA_N
ClientSampleId :
12


Tgt Ion: 91 Resp: 10761
Ion Ratio Lower Upper
91 100
120 25.8 11.7 35.0

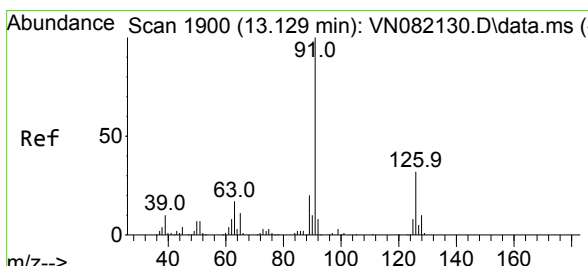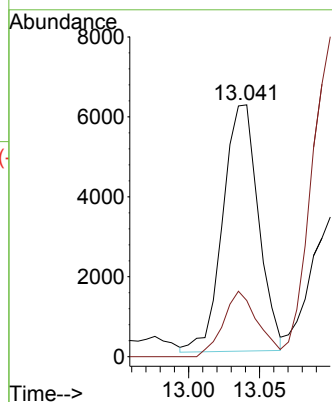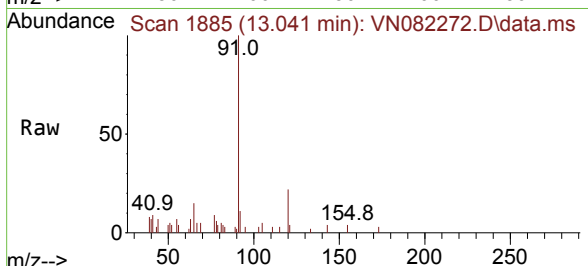

#79
2-Chlorotoluene
Concen: 0.792 ug/l
RT: 13.100 min Scan# 1895
Delta R.T. -0.030 min
Lab File: VN082272.D
Acq: 22 May 2024 04:45

Tgt Ion: 91 Resp: 7243
Ion Ratio Lower Upper
91 100
126 0.0 17.5 52.5#

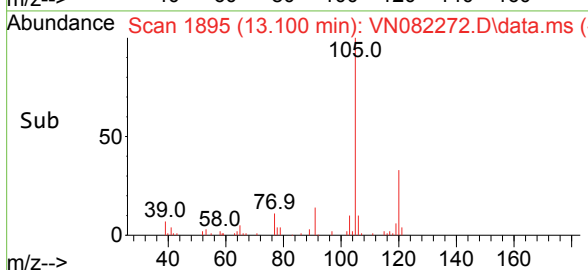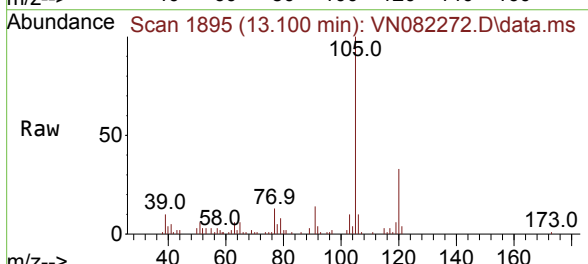



#80

1,3,5-Trimethylbenzene

Concen: 7.103 ug/l

RT: 13.176 min Scan# 1908

Delta R.T. -0.000 min

Lab File: VN082272.D

Acq: 22 May 2024 04:45

Instrument :

MSVOA_N

ClientSampleId :





12

Tgt Ion:105 Resp: 70591

Ion Ratio Lower Upper

105 100

120 47.0 24.8 74.3

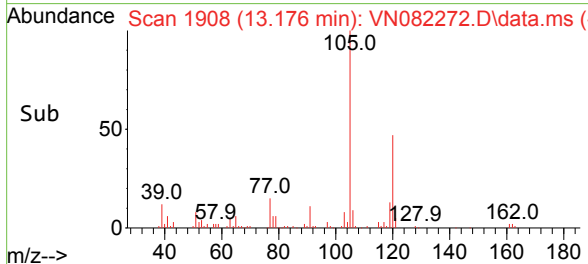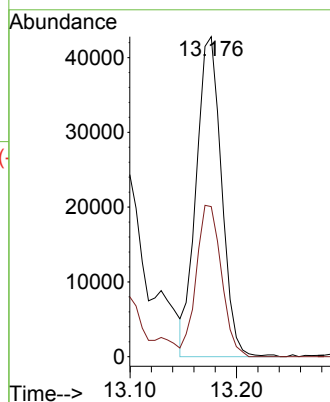

#81

trans-1,4-Dichloro-2-butene

Concen: 70.168 ug/l

RT: 12.847 min Scan# 1852

Delta R.T. 0.112 min

Lab File: VN082272.D

Acq: 22 May 2024 04:45




Tgt Ion: 75 Resp: 97692


Ion Ratio Lower Upper

75 100

53 0.2 72.9 109.3#

89 0.1 39.1 58.7#

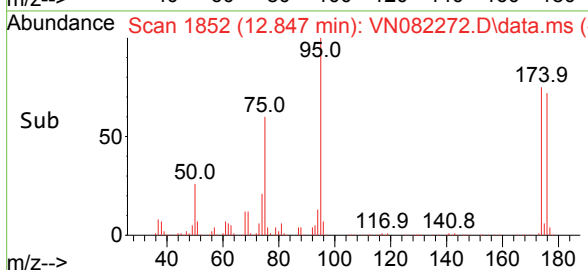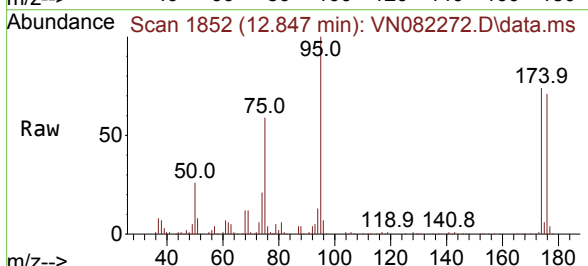



#82

4-Chlorotoluene

Concen: 0.925 ug/l

RT: 13.176 min Scan# 1916

Delta R.T. -0.047 min

Lab File: VN082272.D

Acq: 22 May 2024 04:45

Instrument :

MSVOA_N

ClientSampleId :





12

Tgt Ion: 91 Resp: 8270

Ion Ratio Lower Upper

91 100

126 0.0 17.4 52.3#



#83

tert-Butylbenzene

Concen: 0.787 ug/l

RT: 13.670 min Scan# 1992

Delta R.T. 0.229 min

Lab File: VN082272.D

Acq: 22 May 2024 04:45




Tgt Ion: 119 Resp: 6847


Ion Ratio Lower Upper

119 100

91 40.9 32.6 97.8

134 33.2 12.4 37.0

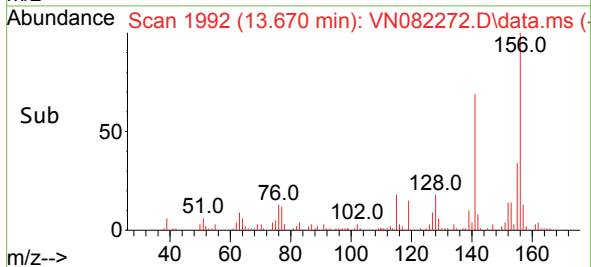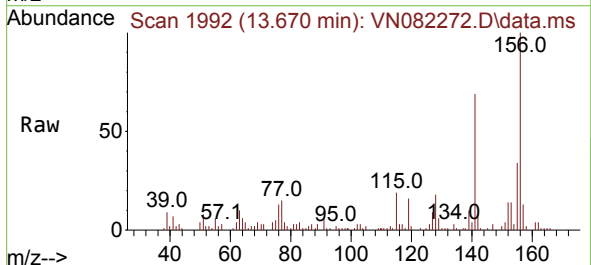



#84

1,2,4-Trimethylbenzene

Concen: 14.246 ug/l

RT: 13.482 min Scan# 1960

Delta R.T. -0.000 min

Lab File: VN082272.D

Acq: 22 May 2024 04:45

Instrument :

MSVOA_N

ClientSampleId :





12

Tgt Ion:105 Resp: 144853

Ion Ratio Lower Upper

105 100

120 42.9 22.9 68.7

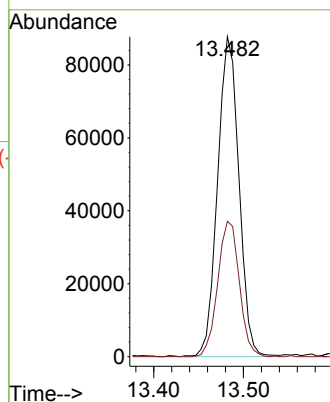

#85

sec-Butylbenzene

Concen: 12.019 ug/l

RT: 13.482 min Scan# 1960

Delta R.T. -0.135 min

Lab File: VN082272.D




Acq: 22 May 2024 04:45


Tgt Ion:105 Resp: 144853

Ion Ratio Lower Upper

105 100

134 0.0 10.2 30.4#

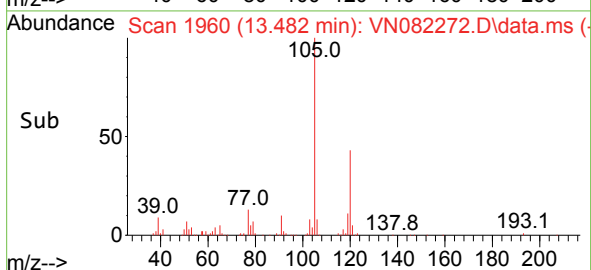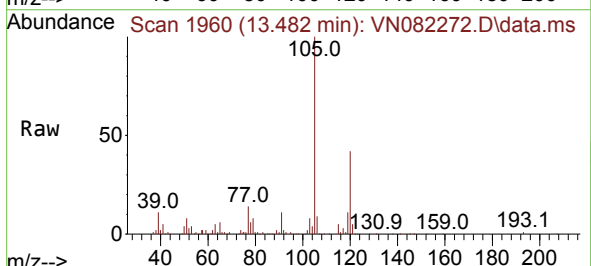

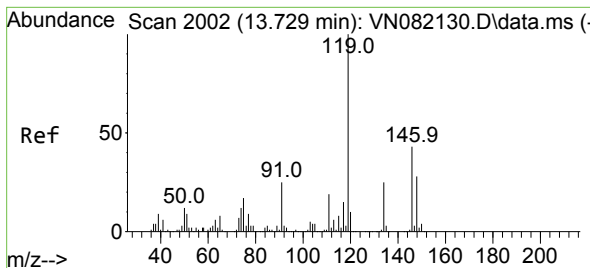

#86

p-Isopropyltoluene

Concen: 0.490 ug/l

RT: 13.729 min Scan# 2002

Delta R.T. -0.000 min

Lab File: VN082272.D

Acq: 22 May 2024 04:45

Instrument :

MSVOA_N

ClientSampleId :

12





Tgt Ion:119 Resp: 4799

Ion Ratio Lower Upper

119 100

134 31.8 13.2 39.5

91 25.0 11.8 35.3

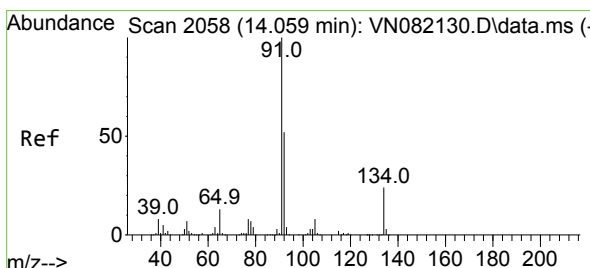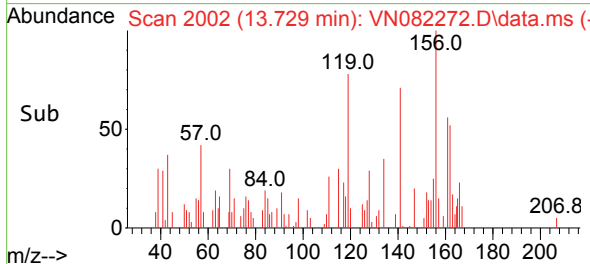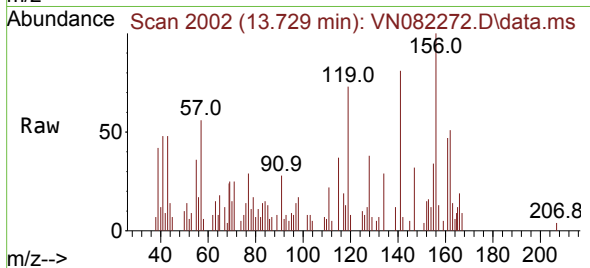

#89

n-Butylbenzene

Concen: 0.339 ug/l

RT: 14.059 min Scan# 2058

Delta R.T. -0.000 min

Lab File: VN082272.D

Acq: 22 May 2024 04:45




Tgt Ion: 91 Resp: 2980


Ion Ratio Lower Upper

91 100

92 72.6 26.2 78.5

134 0.0 13.2 39.5#

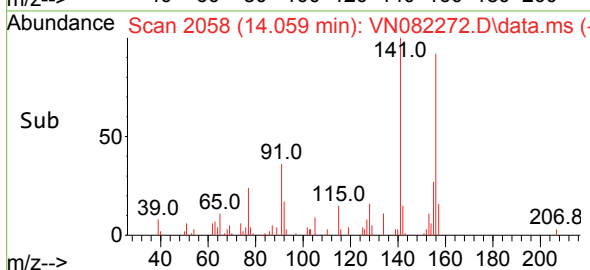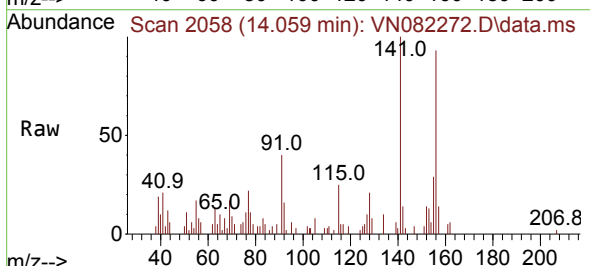



#90

Hexachloroethane

Concen: 1.488 ug/l

RT: 14.329 min Scan# 2104

Delta R.T. -0.006 min

Lab File: VN082272.D

Acq: 22 May 2024 04:45

Instrument :

MSVOA_N

ClientSampleId :





12

Tgt Ion:117 Resp: 2700

Ion Ratio Lower Upper

117 100

201 0.0 33.3 99.8#

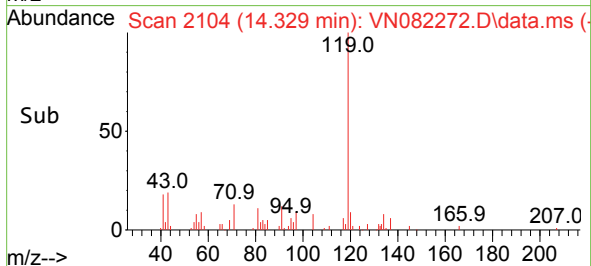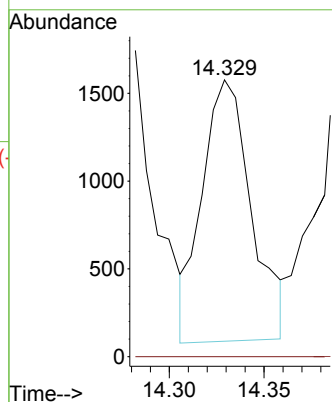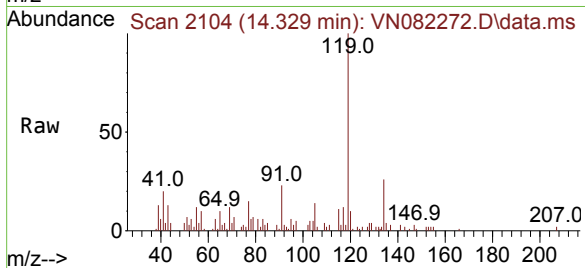

#92

1,2-Dibromo-3-Chloropropane

Concen: 0.249 ug/l

RT: 14.735 min Scan# 2173

Delta R.T. 0.012 min

Lab File: VN082272.D

Acq: 22 May 2024 04:45




Tgt Ion: 75 Resp: 181


Ion Ratio Lower Upper

75 100

155 0.0 42.6 128.0#


157 0.0 53.0 159.0#

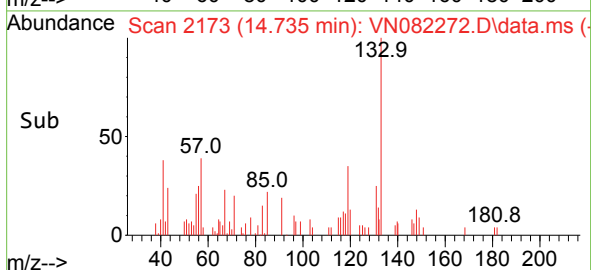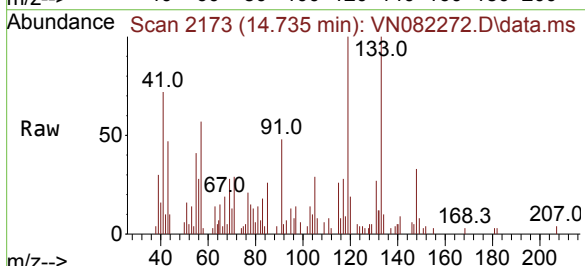

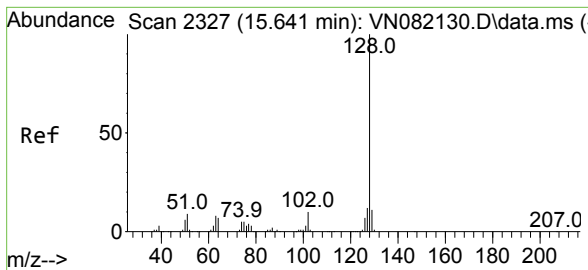

#95
Naphthalene
Concen: 207.941 ug/l
RT: 15.641 min Scan# 21
Delta R.T. -0.000 min
Lab File: VN082272.D
Acq: 22 May 2024 04:45

Instrument :
MSVOA_N
ClientSampleId :
12

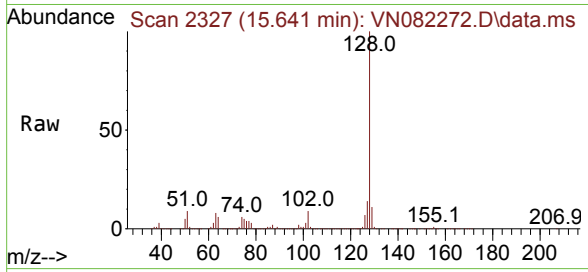

Tgt Ion:128 Resp: 1834890
Ion Ratio Lower Upper
128 100
127 13.2 10.1 15.1
129 10.9 8.9 13.3

