

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN052124\
 Data File : VN082241.D
 Acq On : 21 May 2024 15:29
 Operator : JC\MD
 Sample : P2532-03
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 STORAGE-BLANK-WATER-REF-4

Quant Time: May 22 01:27:48 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N051524W.M
 Quant Title : SW846 8260
 QLast Update : Thu May 16 05:21:06 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	8.229	168	157334	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	9.100	114	282460	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.865	117	266636	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.794	152	109735	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.582	65	133733	53.830	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	=	107.660%
35) Dibromofluoromethane	8.171	113	92771	53.391	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	106.780%
50) Toluene-d8	10.570	98	365042	54.797	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	=	109.600%
62) 4-Bromofluorobenzene	12.847	95	121521	51.108	ug/l	0.00
Spiked Amount	50.000	Range	64 - 133	Recovery	=	102.220%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN052124\
Data File : VN082241.D
Acq On : 21 May 2024 15:29
Operator : JC\MD
Sample : P2532-03
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
STORAGE-BLANK-WATER-REF-4

Quant Time: May 22 01:27:48 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N051524W.M
Quant Title : SW846 8260
QLast Update : Thu May 16 05:21:06 2024
Response via : Initial Calibration




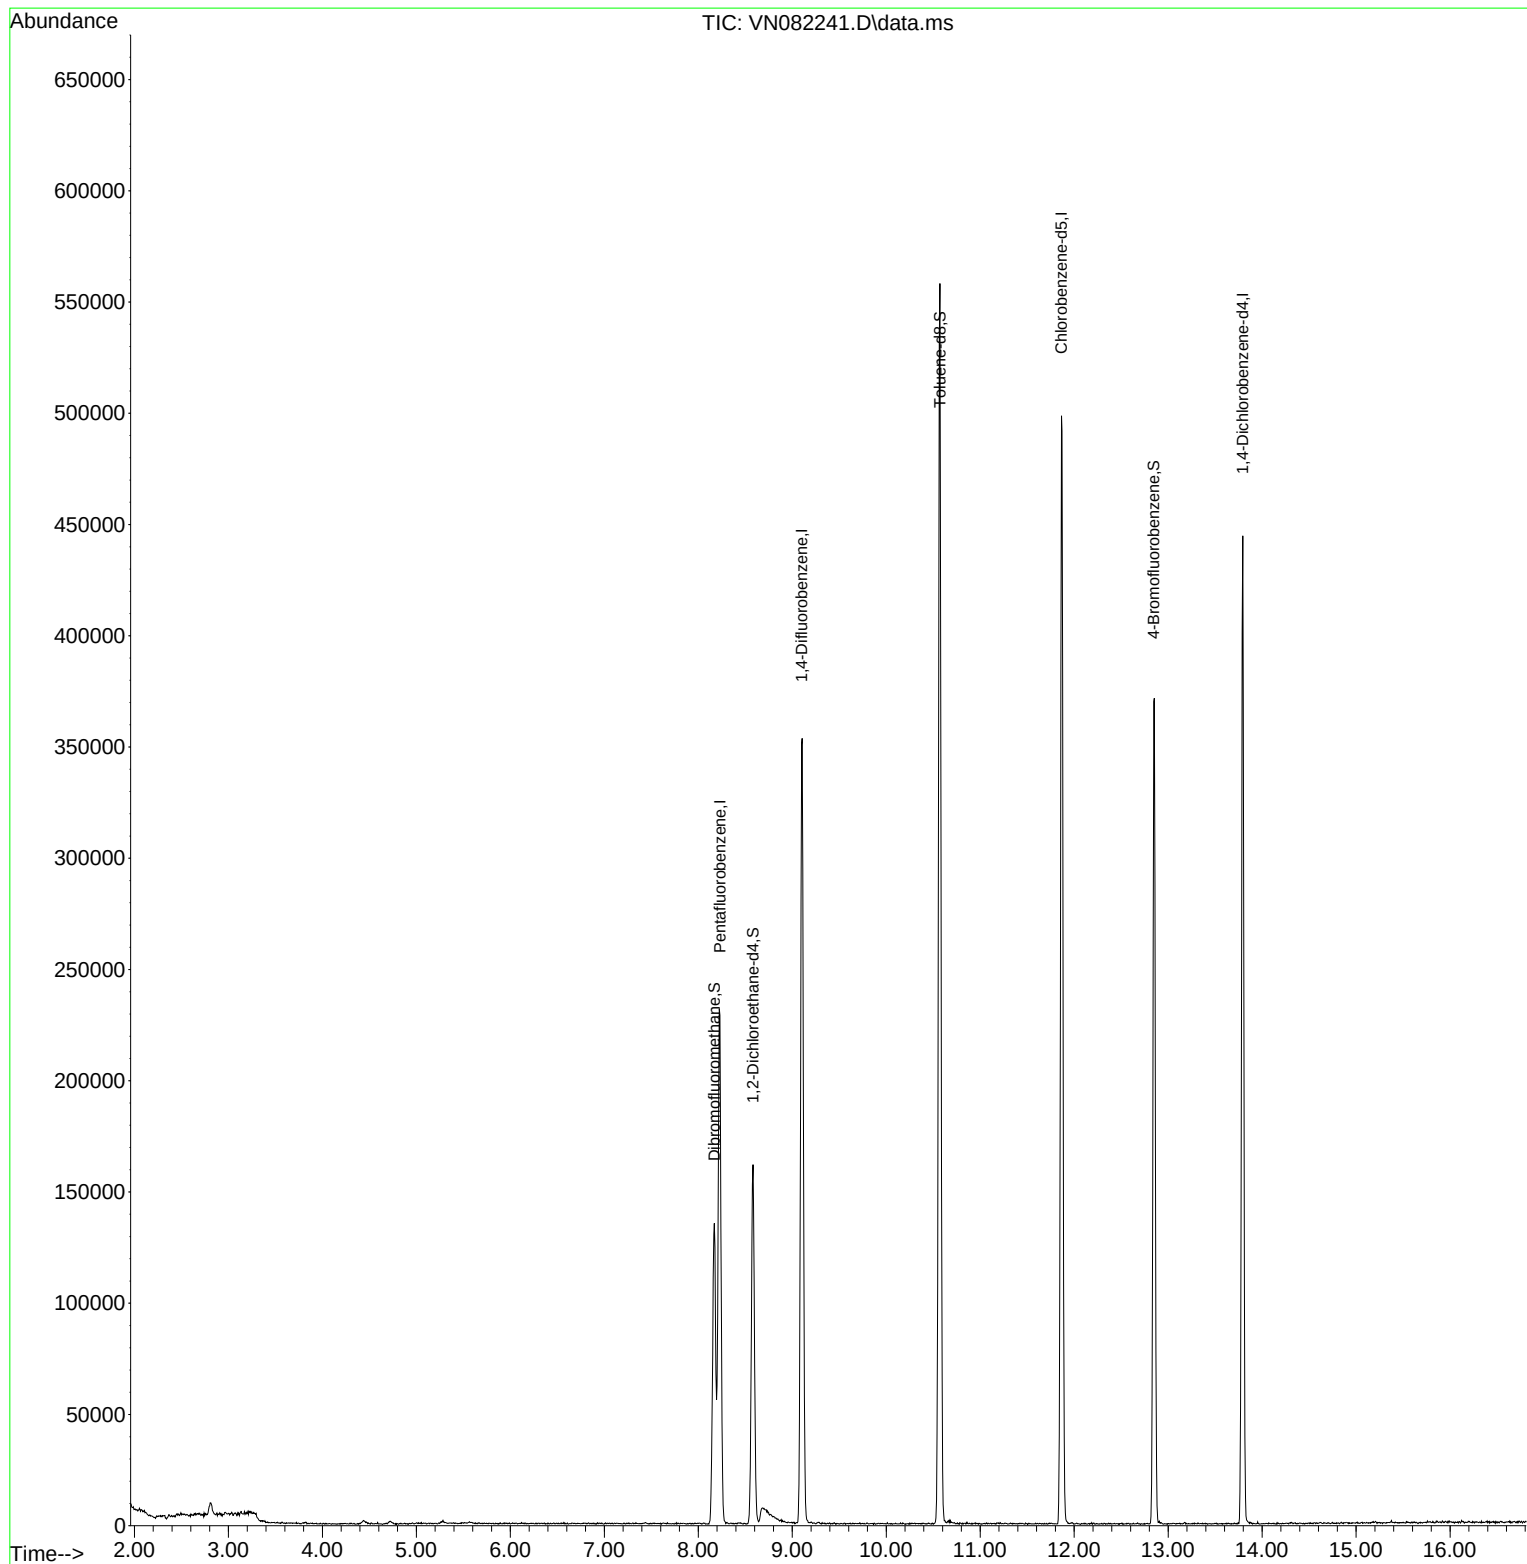


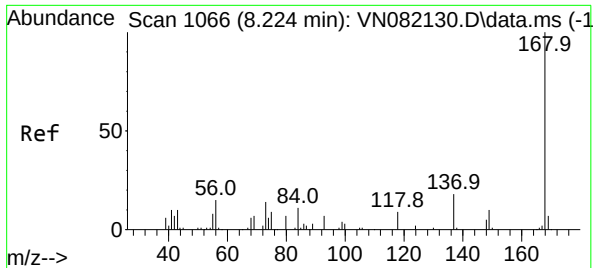

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.229 min Scan# 1066
Delta R.T. 0.005 min
Lab File: VN082241.D
Acq: 21 May 2024 15:29




Instrument :
MSVOA_N
ClientSampleId :
STORAGE-BLANK-WATER-REF-4


Tgt Ion:168 Resp: 157334
Ion Ratio Lower Upper
168 100
99 61.5 48.2 72.4

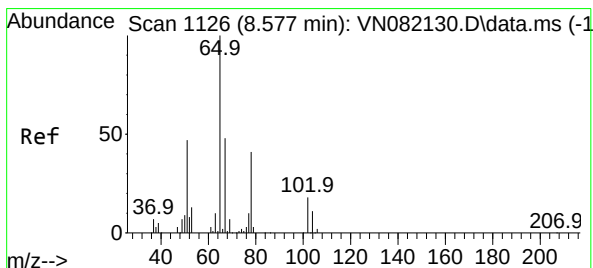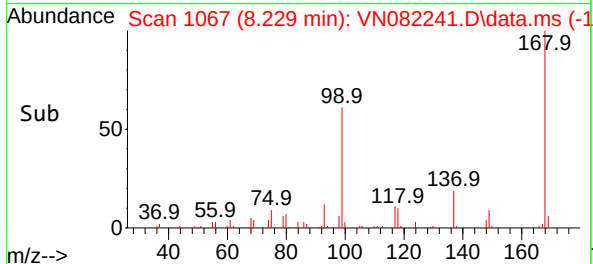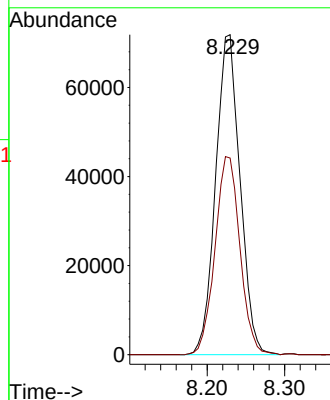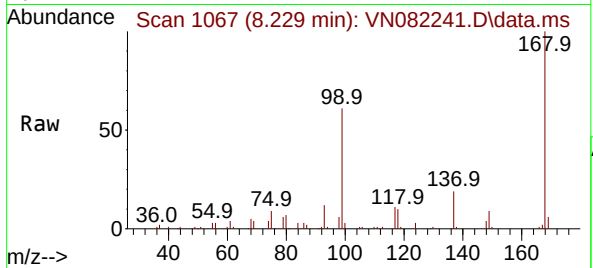

#33
1,2-Dichloroethane-d4
Concen: 53.830 ug/l
RT: 8.582 min Scan# 1127
Delta R.T. 0.006 min
Lab File: VN082241.D
Acq: 21 May 2024 15:29

Tgt Ion: 65 Resp: 133733
Ion Ratio Lower Upper
65 100
67 50.8 0.0 103.0

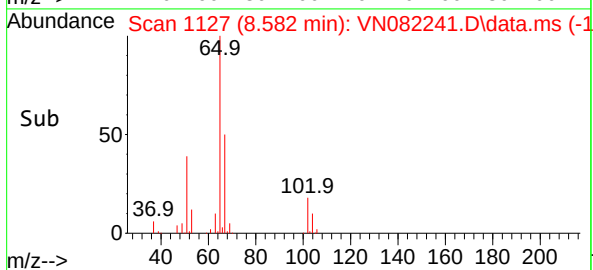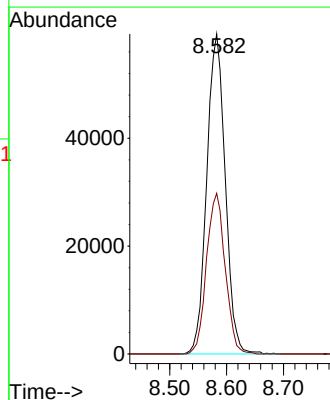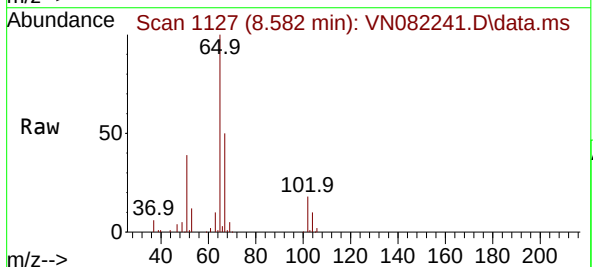

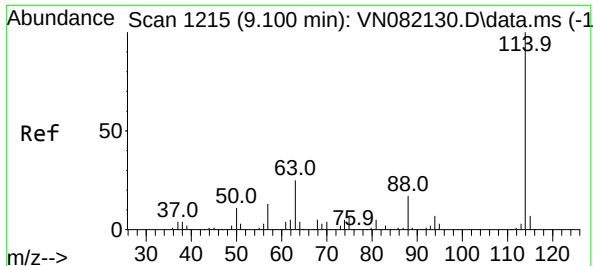

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 9.100 min Scan# 11

Delta R.T. -0.000 min

Lab File: VN082241.D

Acq: 21 May 2024 15:29

Instrument :

MSVOA_N

ClientSampleId :

STORAGE-BLANK-WATER-REF-4





Tgt Ion:114 Resp: 282460

Ion Ratio Lower Upper

114 100

63 23.8 0.0 41.0

88 15.9 0.0 31.4

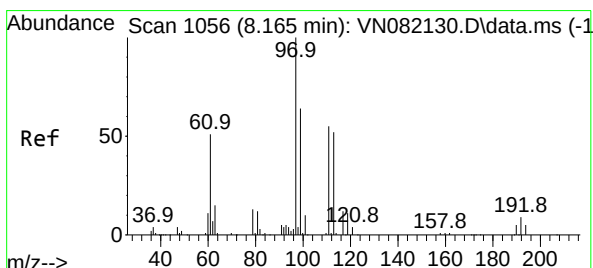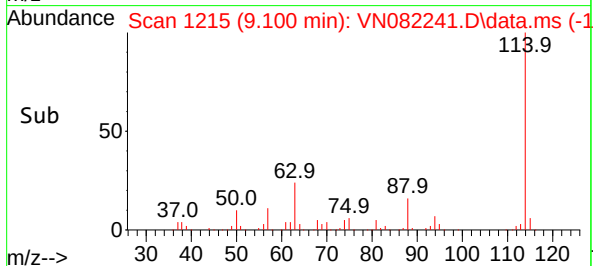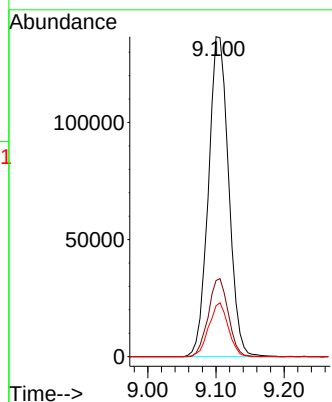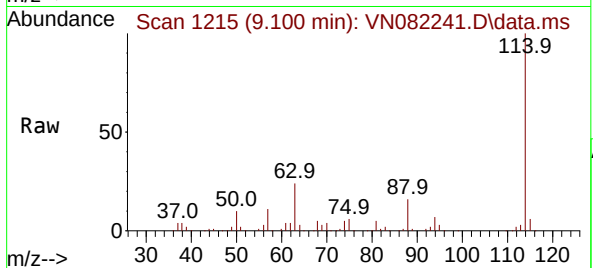

#35

Dibromofluoromethane

Concen: 53.391 ug/l

RT: 8.171 min Scan# 1057

Delta R.T. 0.006 min

Lab File: VN082241.D

Acq: 21 May 2024 15:29




Tgt Ion:113 Resp: 92771


Ion Ratio Lower Upper

113 100

111 104.6 83.4 125.2

192 18.9 14.0 21.0


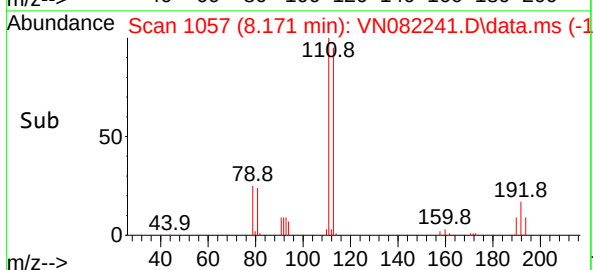
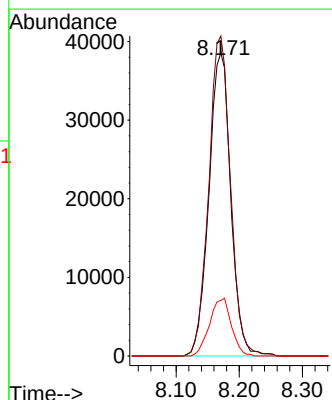
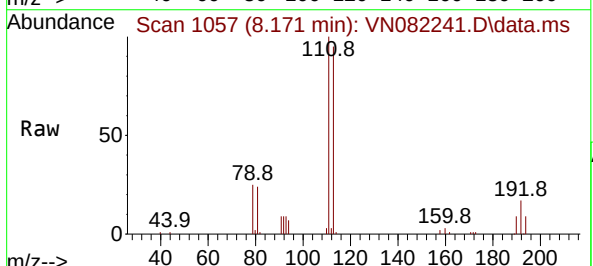


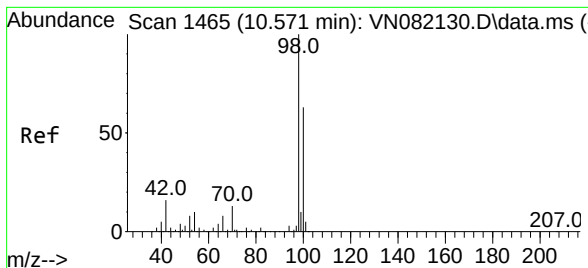

#50
Toluene-d8
Concen: 54.797 ug/l
RT: 10.570 min Scan# 1465
Delta R.T. -0.000 min
Lab File: VN082241.D
Acq: 21 May 2024 15:29




Instrument :
MSVOA_N
ClientSampleId :
STORAGE-BLANK-WATER-REF-4


Tgt Ion: 98 Resp: 365042
Ion Ratio Lower Upper
98 100
100 63.7 51.8 77.6

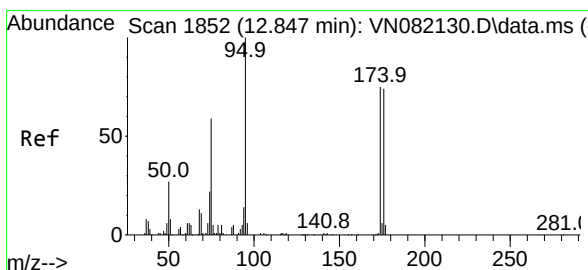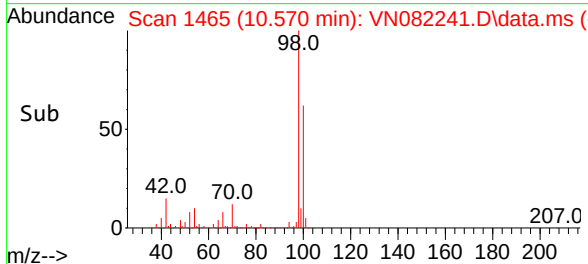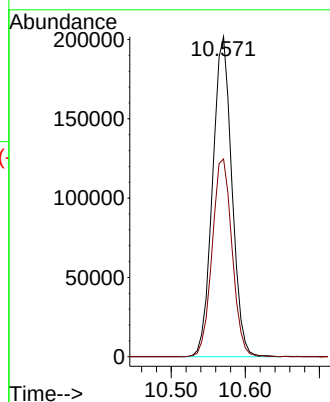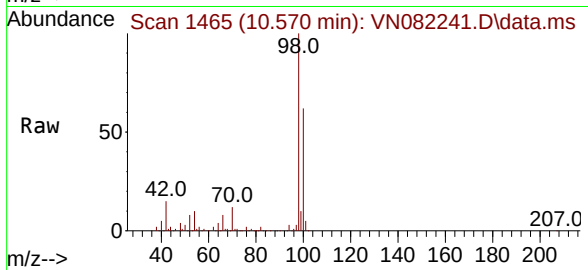

#62
4-Bromofluorobenzene
Concen: 51.108 ug/l
RT: 12.847 min Scan# 1852
Delta R.T. -0.000 min
Lab File: VN082241.D
Acq: 21 May 2024 15:29

Tgt Ion: 95 Resp: 121521
Ion Ratio Lower Upper
95 100
174 74.4 0.0 160.6
176 71.2 0.0 152.8


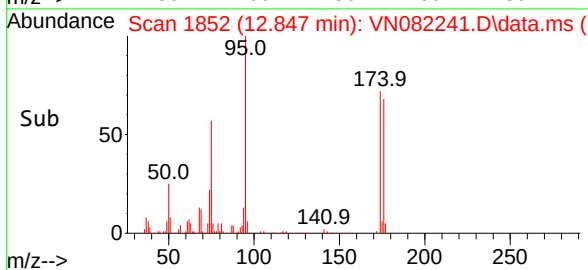
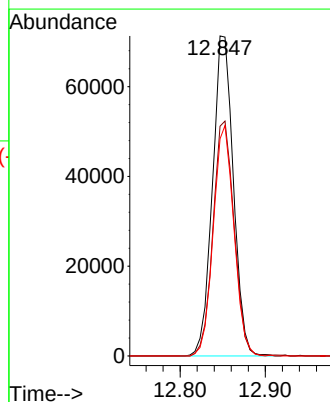
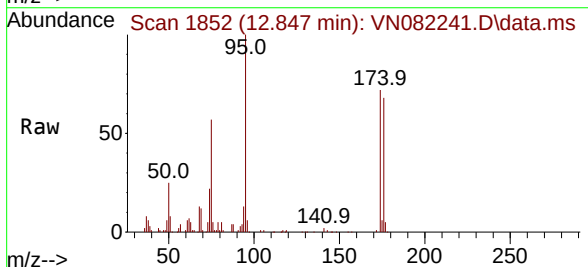


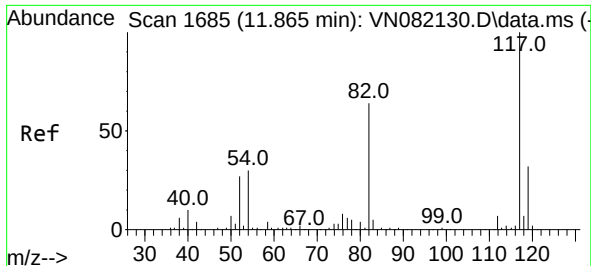

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.865 min Scan# 11
Delta R.T. -0.000 min
Lab File: VN082241.D
Acq: 21 May 2024 15:29

Instrument :
MSVOA_N
ClientSampleId :
STORAGE-BLANK-WATER-REF-4

Tgt Ion:117 Resp: 266636
Ion Ratio Lower Upper
117 100
82 60.5 44.6 66.8
119 30.6 25.9 38.9

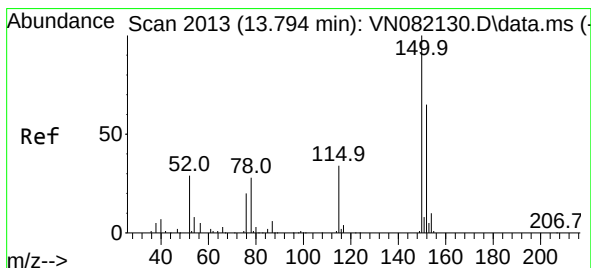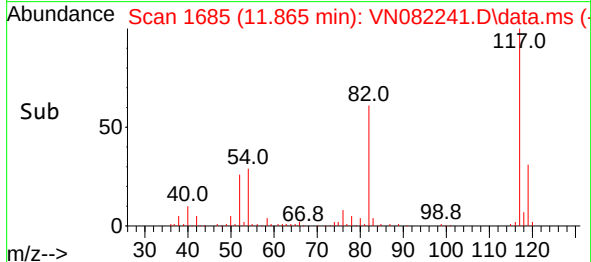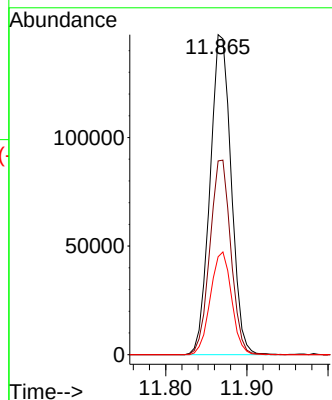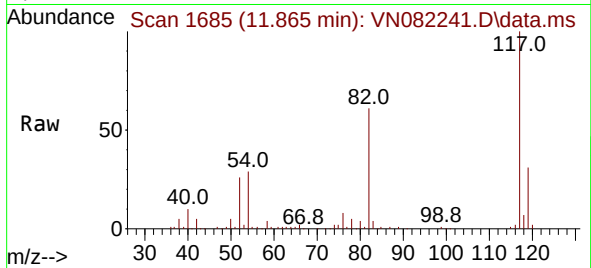

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.794 min Scan# 2013
Delta R.T. -0.000 min
Lab File: VN082241.D
Acq: 21 May 2024 15:29

Tgt Ion:152 Resp: 109735
Ion Ratio Lower Upper
152 100
115 60.1 30.4 91.3
150 157.1 0.0 353.2

