
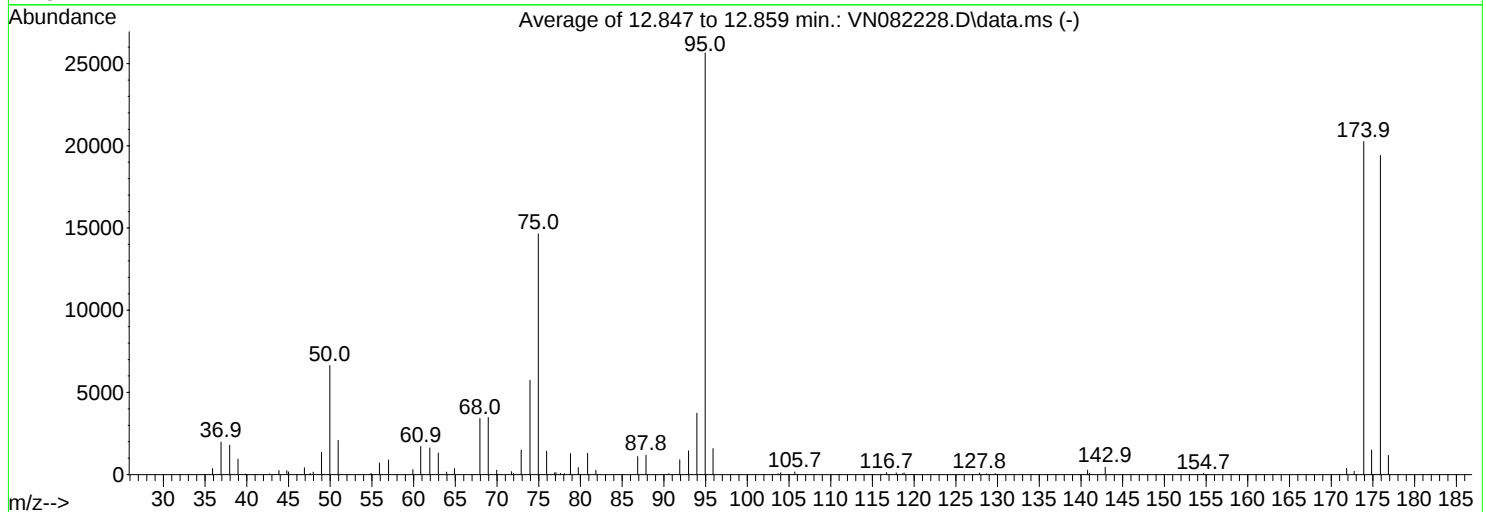


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN052124\
Data File : VN082228.D
Acq On : 21 May 2024 08:44
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N051524W.M
Title : SW846 8260
Last Update : Thu May 16 05:21:06 2024

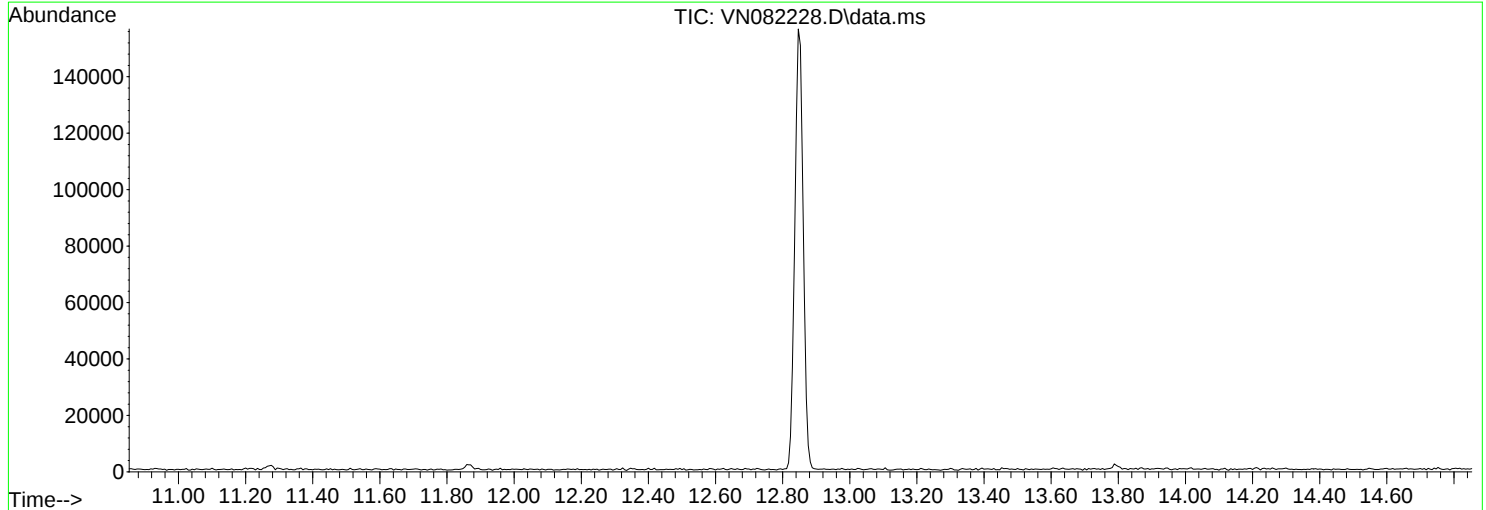

AutoFind: Scans 1852, 1853, 1854; Background Corrected with Scan 1844

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	25.9	6640	PASS
75	95	30	60	57.1	14646	PASS
95	95	100	100	100.0	25651	PASS
96	95	5	9	6.2	1588	PASS
173	174	0.00	2	1.0	202	PASS
174	95	50	100	79.0	20264	PASS
175	174	5	9	7.4	1500	PASS
176	174	95	101	95.8	19410	PASS
177	176	5	9	6.0	1170	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.90	372	47.95	154	63.95	153	76.90	101
36.90	1975	48.95	1360	64.90	368	77.05	128
37.95	1790	49.95	6640	67.95	3417	77.60	7
38.95	943	50.95	2081	68.95	3478	78.10	5
39.85	41	54.90	78	69.95	273	78.80	1286
42.70	52	55.90	715	71.75	184	79.75	425
43.85	258	57.00	899	72.00	71	80.85	1299
44.80	240	59.90	313	72.90	1503	81.85	267
45.00	165	60.85	1714	73.95	5738	86.85	1103
46.90	416	61.95	1623	74.95	14646	87.85	1184
47.60	67	62.95	1311	75.95	1427	90.60	55

Average of 12.847 to 12.859 min.: VN082228.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
91.90	910	118.80	110	174.85	1500		
92.95	1446	127.85	101	175.90	19410		
93.95	3738	128.70	55	176.85	1170		
94.95	25651	129.70	72				
95.90	1588	140.80	268				
103.70	55	141.00	83				
104.00	116	142.90	452				
105.70	162	154.70	70				
116.70	127	171.85	384				
117.85	106	172.75	202				
118.60	55	173.90	20264				

Instrument :

MSVOA_N

ClientSampleId :

BFB